

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
 Data File : BN016934.D
 Acq On : 13 Oct 2021 18:03
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Oct 14 02:10:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 13 02:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	19238	0.40	ng	0.00
7) Naphthalene-d8	10.444	136	82755	0.40	ng	#-0.01
13) Acenaphthene-d10	14.294	164	42410	0.40	ng	0.00
19) Phenanthrene-d10	17.029	188	78238	0.40	ng	#-0.01
29) Chrysene-d12	21.227	240	80886	0.40	ng	# 0.00
35) Perylene-d12	23.477	264	80760	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	17534	0.40	ng	0.00
5) Phenol-d6	6.868	99	18984	0.39	ng	0.00
8) Nitrobenzene-d5	8.822	82	19554	0.37	ng	0.00
11) 2-Methylnaphthalene-d10	12.038	152	44685	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.791	330	6444	0.34	ng	0.00
15) 2-Fluorobiphenyl	12.924	172	64360	0.40	ng	0.00
27) Fluoranthene-d10	19.073	212	77965	0.40	ng	0.00
31) Terphenyl-d14	19.683	244	69661	0.39	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.281	88	5160	0.40	ng	96
3) n-Nitrosodimethylamine	3.603	42	5995	0.41	ng	99
6) bis(2-Chloroethyl)ether	7.126	93	20774	0.40	ng	100
9) Naphthalene	10.495	128	84799	0.39	ng	100
10) Hexachlorobutadiene	10.787	225	16816	0.40	ng	# 100
12) 2-Methylnaphthalene	12.114	142	54280	0.40	ng	100
16) Acenaphthylene	14.015	152	65503	0.38	ng	100
17) Acenaphthene	14.357	154	46134	0.39	ng	99
18) Fluorene	15.347	166	54651	0.39	ng	100
20) 4,6-Dinitro-2-methylph...	15.436	198	1809	0.30	ng	95
21) 4-Bromophenyl-phenylether	16.238	248	17792	0.39	ng	99
22) Hexachlorobenzene	16.348	284	21089	0.40	ng	99
23) Atrazine	16.518	200	11114	0.37	ng	99
24) Pentachlorophenol	16.689	266	5558	0.41	ng	100
25) Phenanthrene	17.078	178	89038	0.40	ng	100
26) Anthracene	17.163	178	74334	0.39	ng	100
28) Fluoranthene	19.102	202	101768	0.42	ng	100
30) Pyrene	19.465	202	101455	0.39	ng	100
32) Benzo(a)anthracene	21.216	228	94341	0.39	ng	99
33) Chrysene	21.270	228	108689	0.41	ng	99
34) Bis(2-ethylhexyl)phtha...	21.163	149	31956	0.40	ng	99
36) Indeno(1,2,3-cd)pyrene	25.747	276	109338	0.36	ng	100
37) Benzo(b)fluoranthene	22.800	252	106956	0.41	ng	99
38) Benzo(k)fluoranthene	22.844	252	107369	0.42	ng	99
39) Benzo(a)pyrene	23.378	252	93348	0.39	ng	100
40) Dibenzo(a,h)anthracene	25.767	278	90499	0.36	ng	99
41) Benzo(g,h,i)perylene	26.438	276	88569	0.33	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
Data File : BN016934.D
Acq On : 13 Oct 2021 18:03
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Oct 14 02:10:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 02:19:57 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.688 min Scan# 500
 Delta R.T. -0.001 min
 Lab File: BN016934.D
 Acq: 13 Oct 2021 18:03

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:152 Resp: 19238




Ion	Ratio	Lower	Upper
152	100		
150	153.6	122.6	183.8
115	57.6	46.1	69.1




#2
 1,4-Dioxane
 Concen: 0.40 ng
 RT: 3.281 min Scan# 22
 Delta R.T. -0.000 min
 Lab File: BN016934.D
 Acq: 13 Oct 2021 18:03

Tgt Ion: 88 Resp: 5160

Ion	Ratio	Lower	Upper
88	100		
43	28.7	24.3	36.5
58	77.4	65.2	97.8









#3
n-Nitrosodimethylamine
Concen: 0.41 ng
RT: 3.603 min Scan# 57
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 42 Resp: 5995




Ion	Ratio	Lower	Upper
42	100		
74	142.2	114.4	171.6
44	7.1	5.7	8.5




#4
2-Fluorophenol
Concen: 0.40 ng
RT: 5.291 min Scan# 240
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion: 112 Resp: 17534

Ion	Ratio	Lower	Upper
112	100		
64	56.0	45.0	67.4
63	28.5	22.6	33.8









#5
Phenol-d6
Concen: 0.39 ng
RT: 6.868 min Scan# 411
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 99 Resp: 18984
Ion Ratio Lower Upper
99 100
42 17.7 14.2 21.4
71 30.8 24.5 36.7



#6
bis(2-Chloroethyl)ether
Concen: 0.40 ng
RT: 7.126 min Scan# 439
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion: 93 Resp: 20774
Ion Ratio Lower Upper
93 100
63 75.3 60.3 90.5
95 32.9 26.2 39.4









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.444 min Scan# 736
Delta R.T. -0.013 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	82755
Ion Ratio	Lower	Upper	
136	100		
137	10.9	8.7	13.1
54	8.7	3.7	5.5#
68	7.2	3.2	4.8#



#8
Nitrobenzene-d5
Concen: 0.37 ng
RT: 8.822 min Scan# 608
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:	82	Resp:	19554
Ion Ratio	Lower	Upper	
82	100		
128	36.5	28.3	42.5
54	52.5	43.0	64.4









#9
Naphthalene
Concen: 0.39 ng
RT: 10.495 min Scan# 740
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	128	Resp:	84799
Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.7	13.1
127	13.1	10.6	16.0



#10
Hexachlorobutadiene
Concen: 0.40 ng
RT: 10.787 min Scan# 763
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:	225	Resp:	16816
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.2	51.1	76.7









#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 12.038 min Scan# 939
Delta R.T. -0.005 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 44685
Ion Ratio Lower Upper
152 100
151 20.5 16.2 24.4

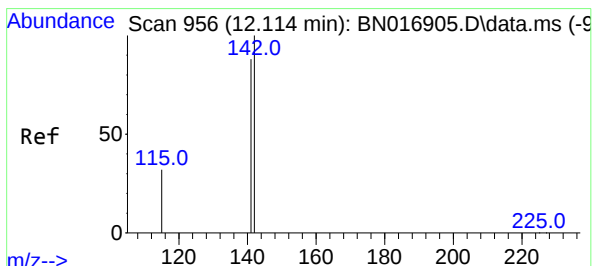

#12
2-Methylnaphthalene
Concen: 0.40 ng
RT: 12.114 min Scan# 956
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:142 Resp: 54280
Ion Ratio Lower Upper
142 100
141 87.6 70.5 105.7
115 32.6 26.0 39.0









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.294 min Scan# 1185
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 42410
Ion Ratio Lower Upper
164 100
162 100.8 81.4 122.0
160 45.4 37.0 55.4



#14
2,4,6-Tribromophenol
Concen: 0.34 ng
RT: 15.791 min Scan# 1303
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:330 Resp: 6444
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 29.8 24.4 36.6







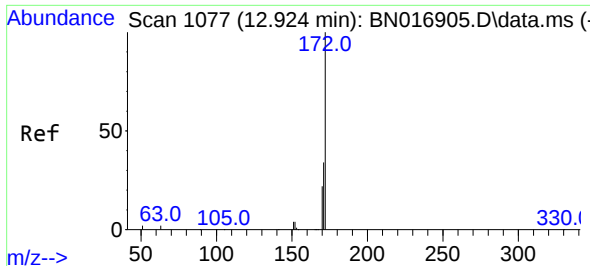

#15
2-Fluorobiphenyl
Concen: 0.40 ng
RT: 12.924 min Scan# 1077
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172 Resp: 64360
Ion Ratio Lower Upper
172 100
171 34.2 27.4 41.0
170 22.3 18.1 27.1

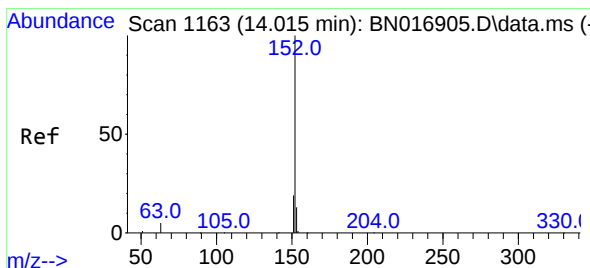

#16
Acenaphthylene
Concen: 0.38 ng
RT: 14.015 min Scan# 1163
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:152 Resp: 65503
Ion Ratio Lower Upper
152 100
151 19.4 15.5 23.3
153 13.0 10.3 15.5









#17
Acenaphthene
Concen: 0.39 ng
RT: 14.357 min Scan# 1190
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 46134
Ion Ratio Lower Upper
154 100
153 112.4 91.2 136.8
152 54.5 44.4 66.6



#18
Fluorene
Concen: 0.39 ng
RT: 15.347 min Scan# 1268
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:166 Resp: 54651
Ion Ratio Lower Upper
166 100
165 98.0 78.1 117.1
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.029 min Scan# 1404
Delta R.T. -0.013 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 78238
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.5 4.9 7.3#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.30 ng
RT: 15.436 min Scan# 1275
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:198 Resp: 1809
Ion Ratio Lower Upper
198 100
182 15.6 11.0 16.6
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.39 ng
RT: 16.238 min Scan# 1339
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 17792
Ion Ratio Lower Upper
248 100
250 96.5 78.2 117.2
141 52.5 43.1 64.7



#22
Hexachlorobenzene
Concen: 0.40 ng
RT: 16.348 min Scan# 1348
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:284 Resp: 21089
Ion Ratio Lower Upper
284 100
142 31.9 25.1 37.7
249 29.2 23.2 34.8









#23
Atrazine
Concen: 0.37 ng
RT: 16.518 min Scan# 1362
Delta R.T. -0.001 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 11114
Ion Ratio Lower Upper
200 100
173 23.1 18.0 27.0
215 49.5 40.0 60.0



#24
Pentachlorophenol
Concen: 0.41 ng
RT: 16.689 min Scan# 1376
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:266 Resp: 5558
Ion Ratio Lower Upper
266 100
264 62.6 50.5 75.7
268 64.1 51.2 76.8









#25
Phenanthrene
Concen: 0.40 ng
RT: 17.078 min Scan# 1408
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 89038
Ion Ratio Lower Upper
178 100
176 19.0 15.0 22.4
179 15.5 12.3 18.5



#26
Anthracene
Concen: 0.39 ng
RT: 17.163 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:178 Resp: 74334
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.3 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.40 ng
RT: 19.073 min Scan# 1698
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 77965
Ion Ratio Lower Upper
212 100
106 13.5 10.7 16.1
104 7.5 5.8 8.8



#28
Fluoranthene
Concen: 0.42 ng
RT: 19.102 min Scan# 1704
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:202 Resp: 101768
Ion Ratio Lower Upper
202 100
101 11.5 9.0 13.4
203 17.4 13.8 20.8









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.227 min Scan# 2001
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 80886
Ion Ratio Lower Upper
240 100
120 13.2 8.6 12.8#
236 26.5 21.0 31.4



#30
Pyrene
Concen: 0.39 ng
RT: 19.465 min Scan# 1777
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:202 Resp: 101455
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.4 14.0 21.0









#31
Terphenyl-d14
Concen: 0.39 ng
RT: 19.683 min Scan# 1821
Delta R.T. 0.005 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 69661
Ion Ratio Lower Upper
244 100
212 7.0 5.7 8.5
122 10.5 9.8 14.6



#32
Benzo(a)anthracene
Concen: 0.39 ng
RT: 21.216 min Scan# 2000
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:228 Resp: 94341
Ion Ratio Lower Upper
228 100
226 26.3 20.6 31.0
229 19.7 15.8 23.8









#33
Chrysene
Concen: 0.41 ng
RT: 21.270 min Scan# 2005
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:228 Resp: 108689
Ion Ratio Lower Upper
228 100
226 29.0 22.6 34.0
229 19.8 16.0 24.0



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.40 ng
RT: 21.163 min Scan# 1995
Delta R.T. -0.001 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03


Tgt Ion:149 Resp: 31956
Ion Ratio Lower Upper
149 100
167 27.9 22.1 33.1
279 4.4 3.4 5.0








#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.477 min Scan# 2425
 Delta R.T. 0.003 min
 Lab File: BN016934.D
 Acq: 13 Oct 2021 18:03

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4







Tgt Ion:264 Resp: 80760
 Ion Ratio Lower Upper
 264 100
 260 24.5 19.4 29.2
 265 23.1 18.6 27.8



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.36 ng
 RT: 25.747 min Scan# 3088
 Delta R.T. 0.003 min
 Lab File: BN016934.D
 Acq: 13 Oct 2021 18:03

Tgt Ion:276 Resp: 109338
 Ion Ratio Lower Upper
 276 100
 138 24.9 20.2 30.4
 277 25.3 20.2 30.4









#37
Benzo(b)fluoranthene
Concen: 0.41 ng
RT: 22.800 min Scan# 2227
Delta R.T. -0.000 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 106956
Ion Ratio Lower Upper
252 100
253 22.3 17.7 26.5
125 10.1 7.8 11.8



#38
Benzo(k)fluoranthene
Concen: 0.42 ng
RT: 22.844 min Scan# 2240
Delta R.T. 0.003 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03


Tgt Ion:252 Resp: 107369
Ion Ratio Lower Upper
252 100
253 22.4 18.1 27.1
125 11.0 9.8 14.8








#39
Benzo(a)pyrene
Concen: 0.39 ng
RT: 23.378 min Scan# 2396
Delta R.T. 0.003 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:252 Resp: 93348
Ion Ratio Lower Upper
252 100
253 22.5 18.1 27.1
125 11.1 9.0 13.4



#40
Dibenzo(a,h)anthracene
Concen: 0.36 ng
RT: 25.767 min Scan# 3094
Delta R.T. 0.003 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Tgt Ion:278 Resp: 90499
Ion Ratio Lower Upper
278 100
139 16.5 13.8 20.6
279 24.1 19.0 28.6





#41
Benzo(g,h,i)perylene
Concen: 0.33 ng
RT: 26.438 min Scan# 3290
Delta R.T. 0.003 min
Lab File: BN016934.D
Acq: 13 Oct 2021 18:03

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 88569
Ion Ratio Lower Upper
276 100
277 23.8 19.1 28.7
138 21.0 16.6 24.8

