
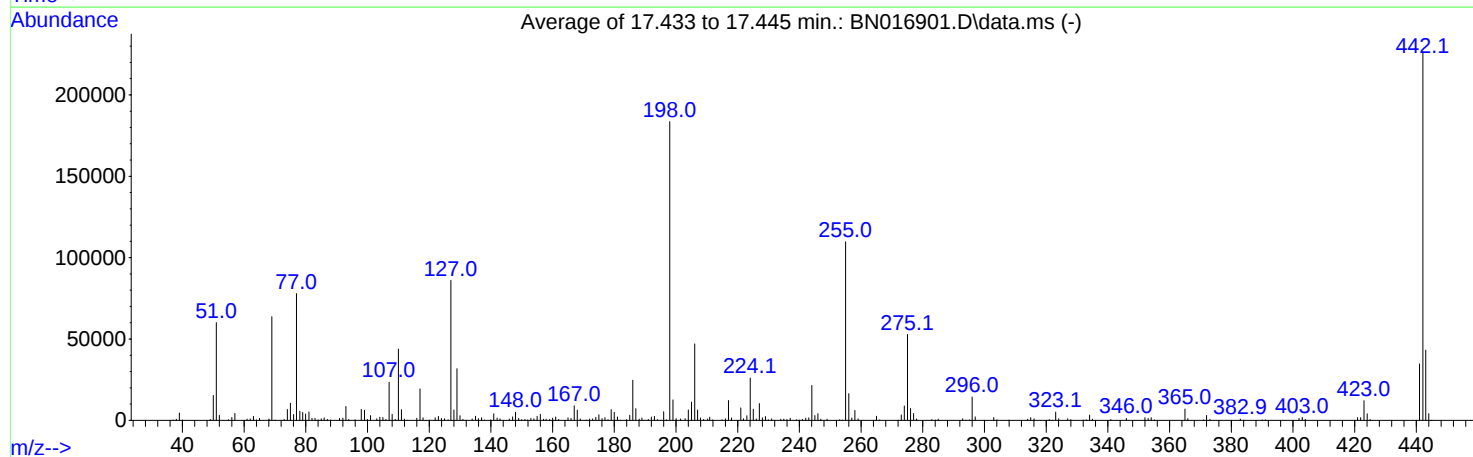


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN101321\  
 Data File : BN016901.D  
 Acq On : 12 Oct 2021 16:56  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN101321.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Oct 13 02:19:57 2021

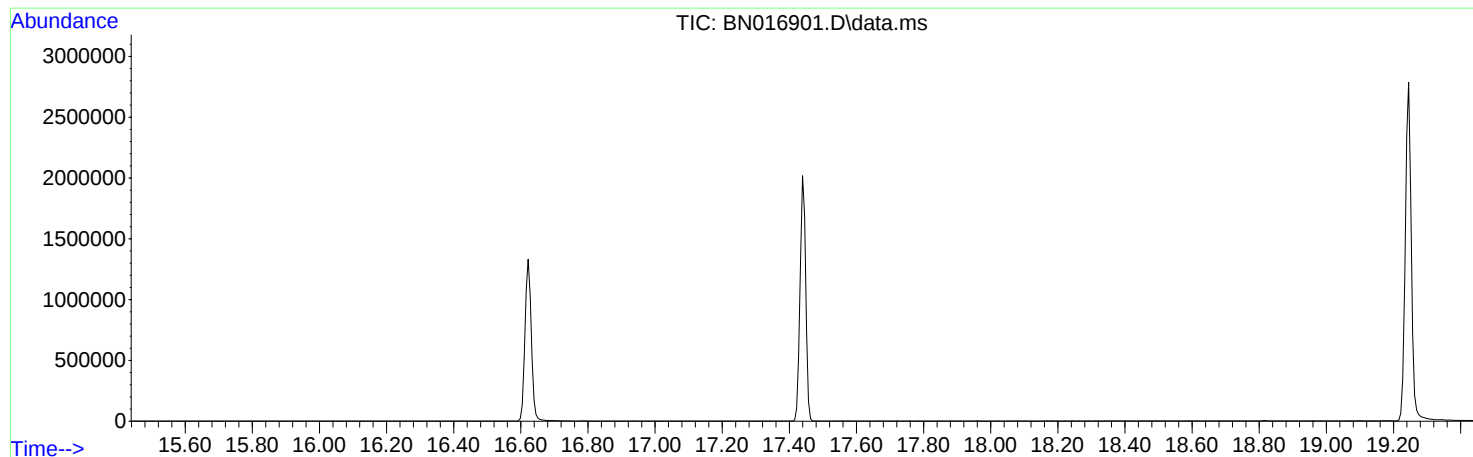




AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2433

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 32.7         | 60109      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.2          | 763        | PASS                |
| 69             | 198             | 0.00            | 100             | 34.7         | 63731      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 233        | PASS                |
| 127            | 198             | 10              | 80              | 46.8         | 86000      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 353        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 183616     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 12601      | PASS                |
| 275            | 198             | 10              | 60              | 28.7         | 52773      | PASS                |
| 365            | 198             | 1               | 100             | 3.8          | 7035       | PASS                |
| 441            | 198             | 0.01            | 100             | 18.9         | 34704      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 226069     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 43187      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN101321\  
Data File : BN016901.D  
Acq On : 12 Oct 2021 16:56  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Oct 13 05:53:38 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 13 05:53:33 2021  
Response via : Initial Calibration

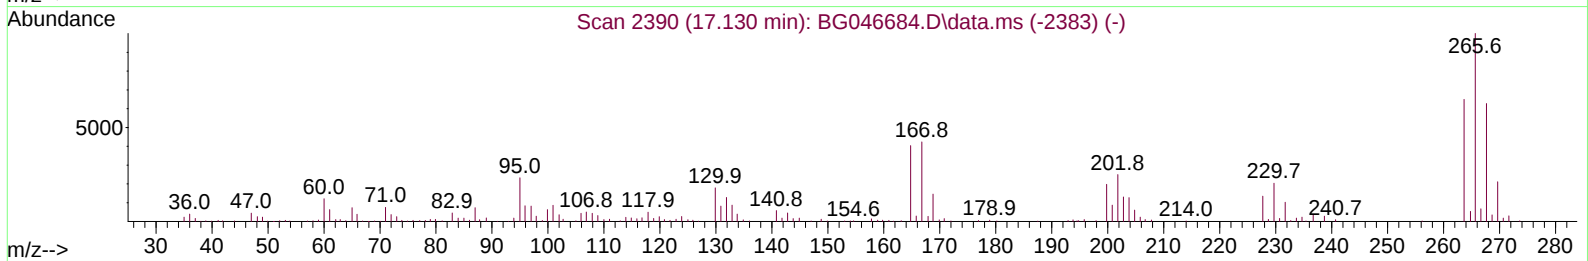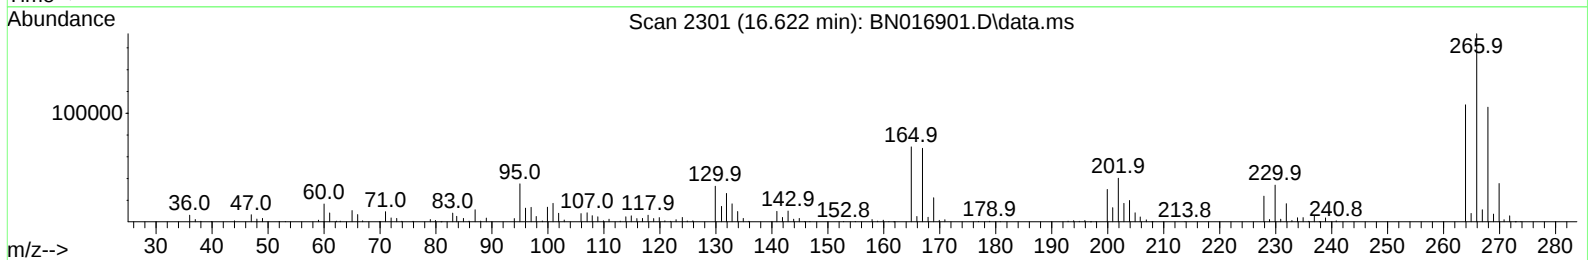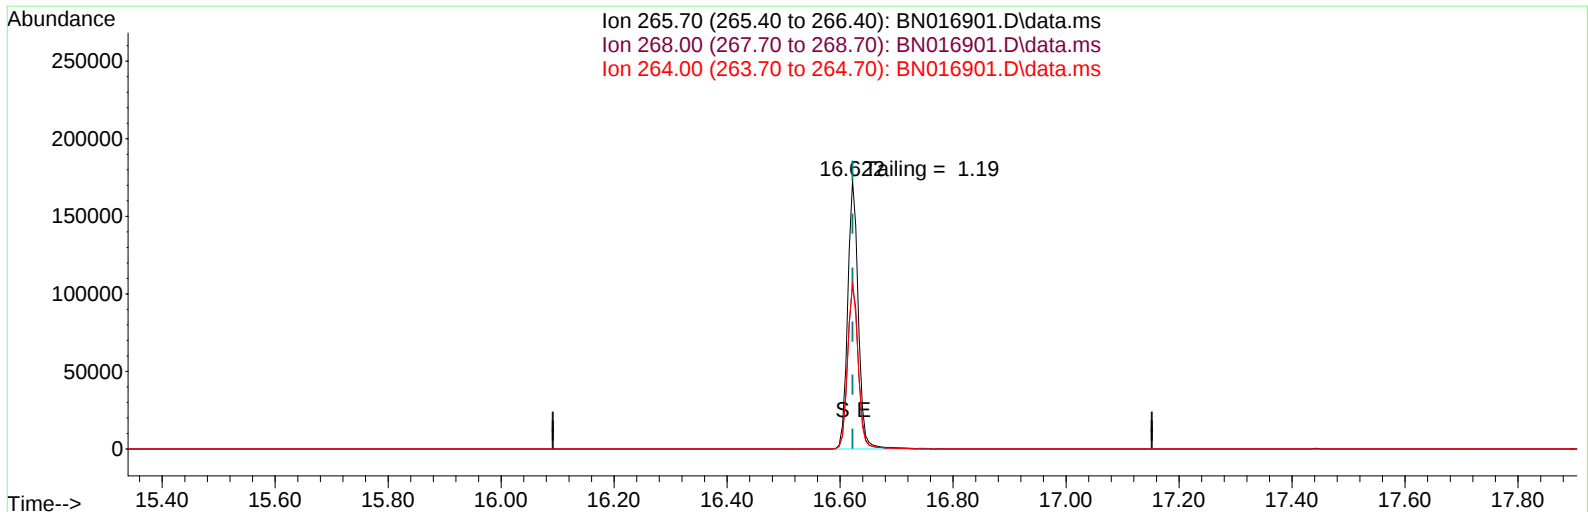

TIC: BN016901.D\data.ms

**(70) Pentachlorophenol (C)**

16.622min ( 0.000) 26834.75 ng

response 226808

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 61.02  |
| 264.00 | 61.60  | 62.26  |
| 0.00   | 0.00   | 0.00   |



# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/13/2021    | BNA_N            | <u>BN016901.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 734615           | 20.486             |
| DDD           | 3226             | 20.092             |
| DDE           | 0                | 19.58              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3226          | 737841           | 0.44               |
|               |                  |                    |