
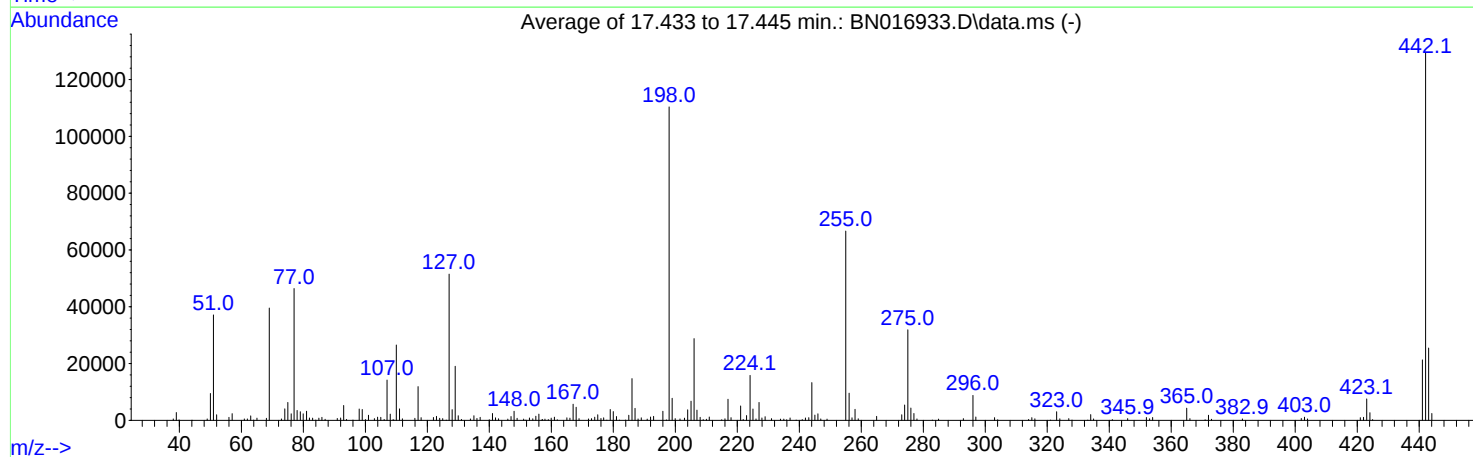


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
 Data File : BN016933.D
 Acq On : 13 Oct 2021 17:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 13 02:19:57 2021

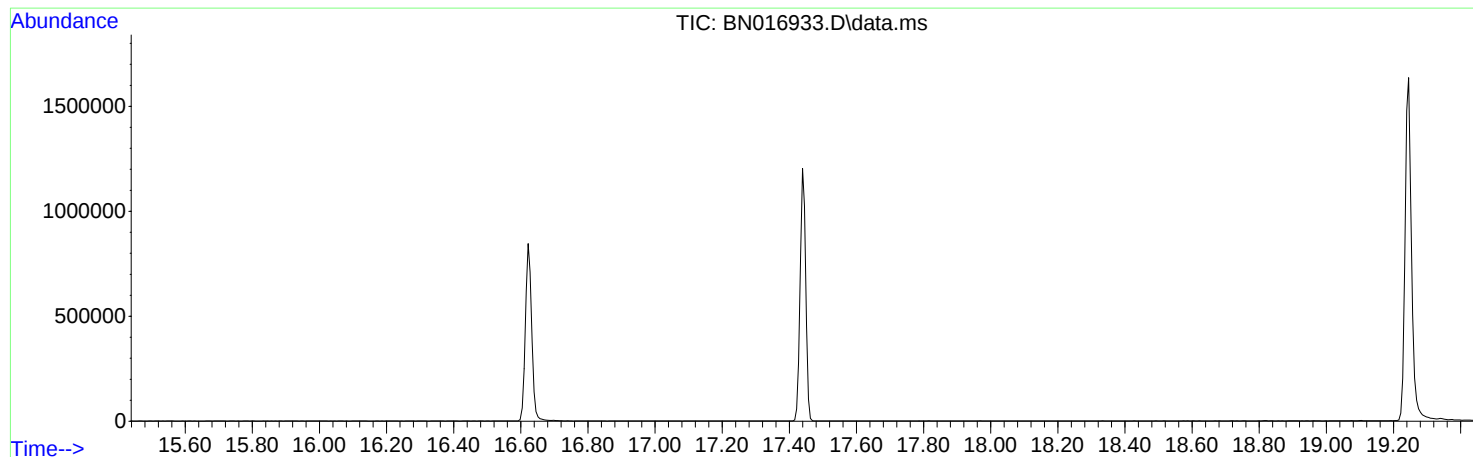




AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	37147	PASS
68	69	0.00	2	1.9	747	PASS
69	198	0.00	100	35.8	39552	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	51496	PASS
197	198	0.00	2	0.2	182	PASS
198	198	100	100	100.0	110368	PASS
199	198	5	9	7.0	7763	PASS
275	198	10	60	28.9	31875	PASS
365	198	1	100	3.9	4319	PASS
441	198	0.01	100	19.3	21327	PASS
442	442	50	100	100.0	129539	PASS
443	442	15	24	19.7	25469	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
Data File : BN016933.D
Acq On : 13 Oct 2021 17:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:07:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

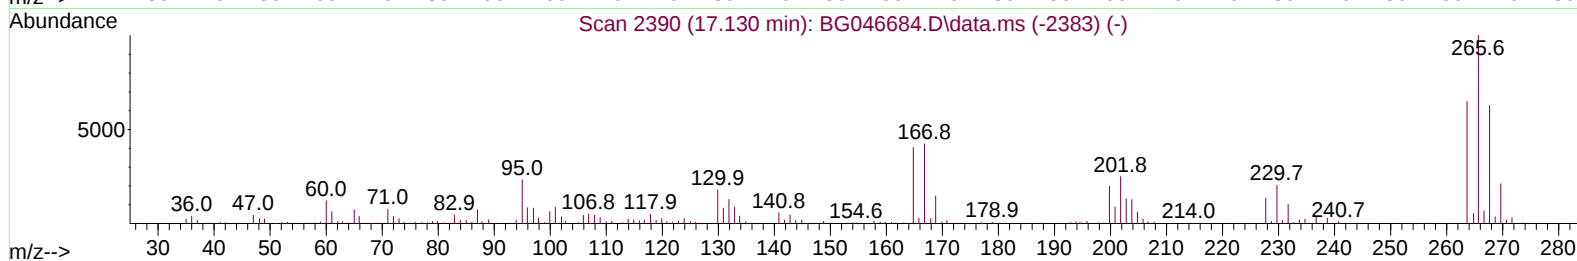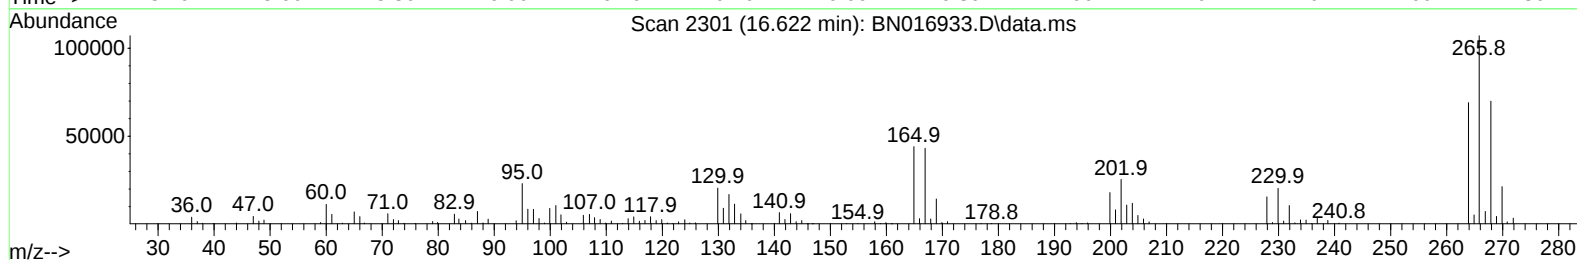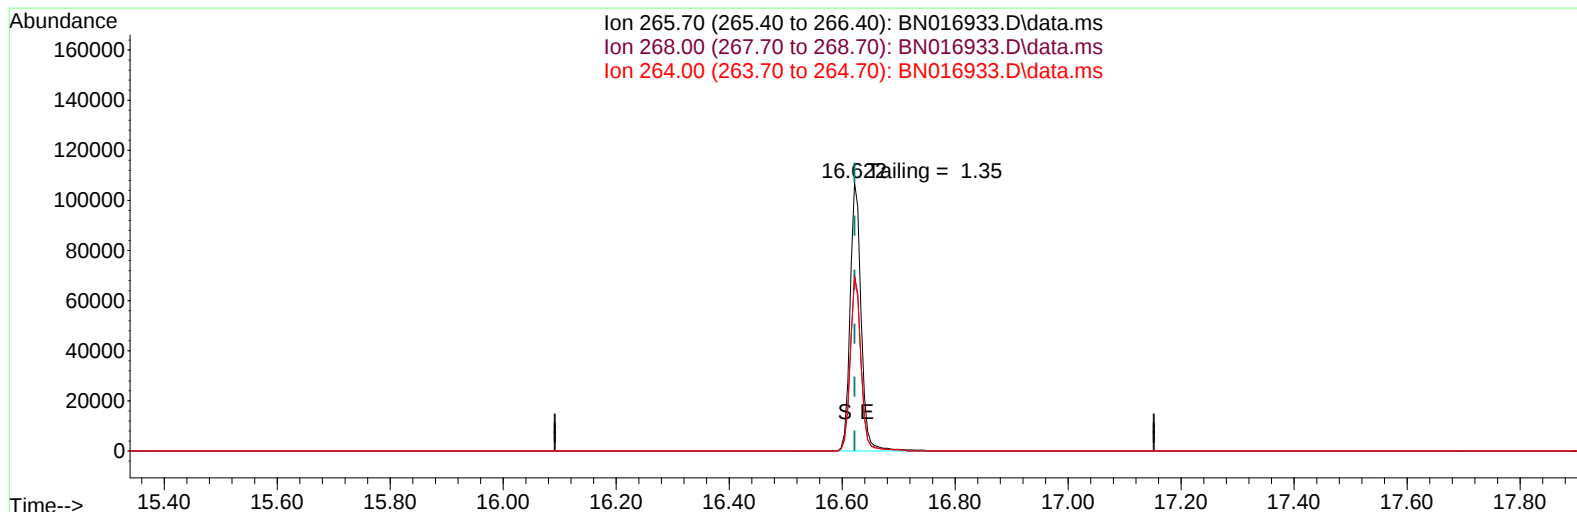

TIC: BN016933.D\data.ms

(70) Pentachlorophenol (C)

16.622min (+ 0.000) 33193.44 ng




response 146137

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.33
264.00	61.60	64.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101321\
Data File : BN016933.D
Acq On : 13 Oct 2021 17:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 04:07:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

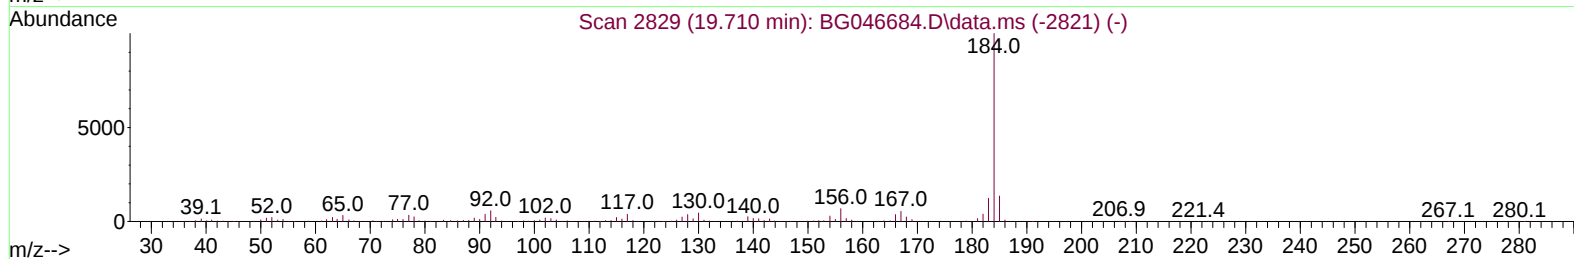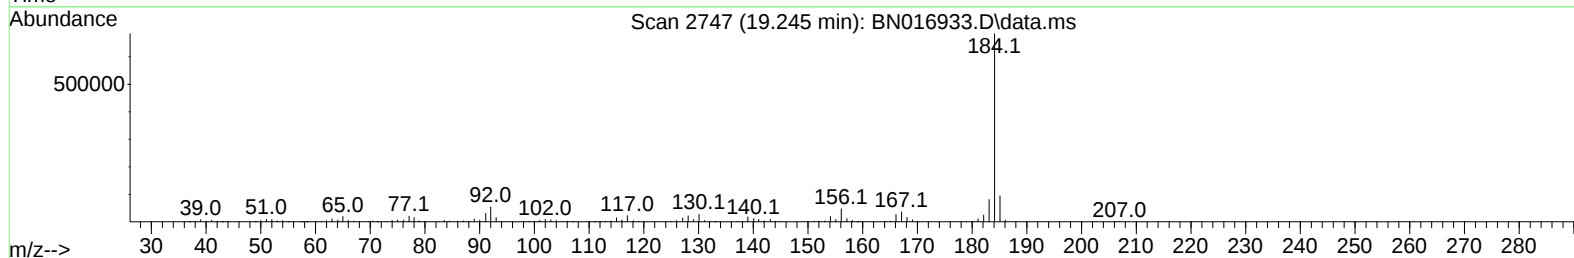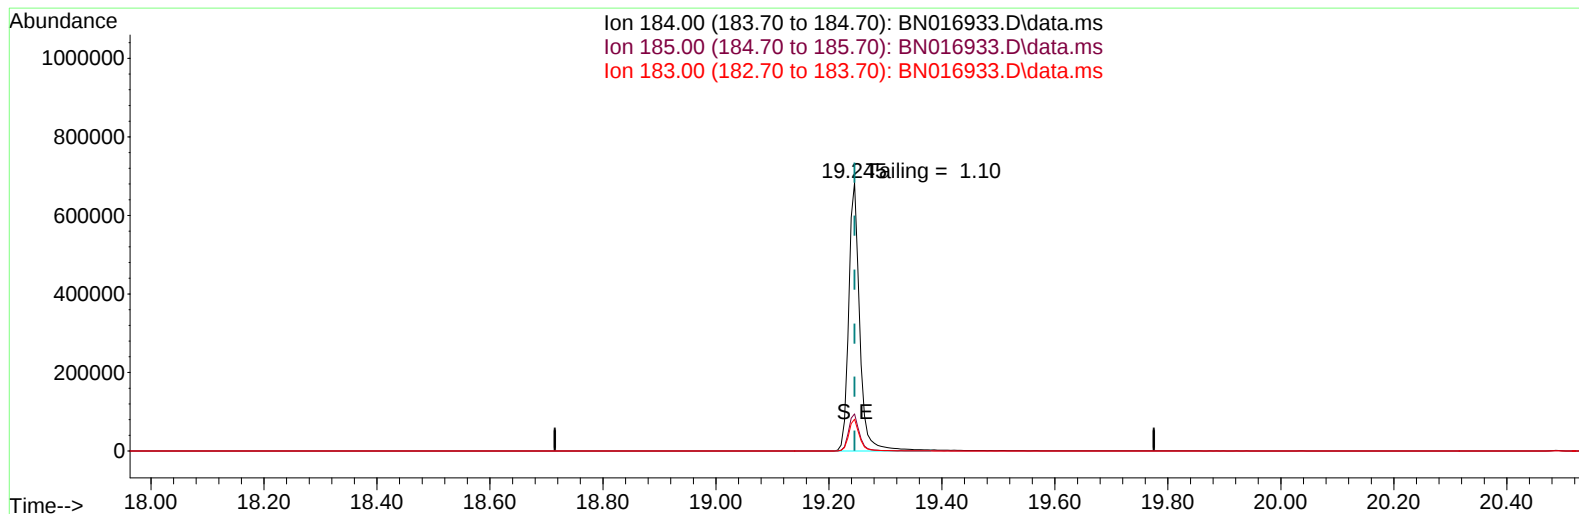

TIC: BN016933.D\data.ms

(77) Benzidine

19.245min (0.000) 0.00 ng

response 936274

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.85
183.00	13.20	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2021	BNA_N	<u>BN016933.D</u>
Compound Name	Response	Retention Time
DDT	396002	20.486
DDD	48639	20.045
DDE	502	19.533
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49141	445143	11.04

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP