
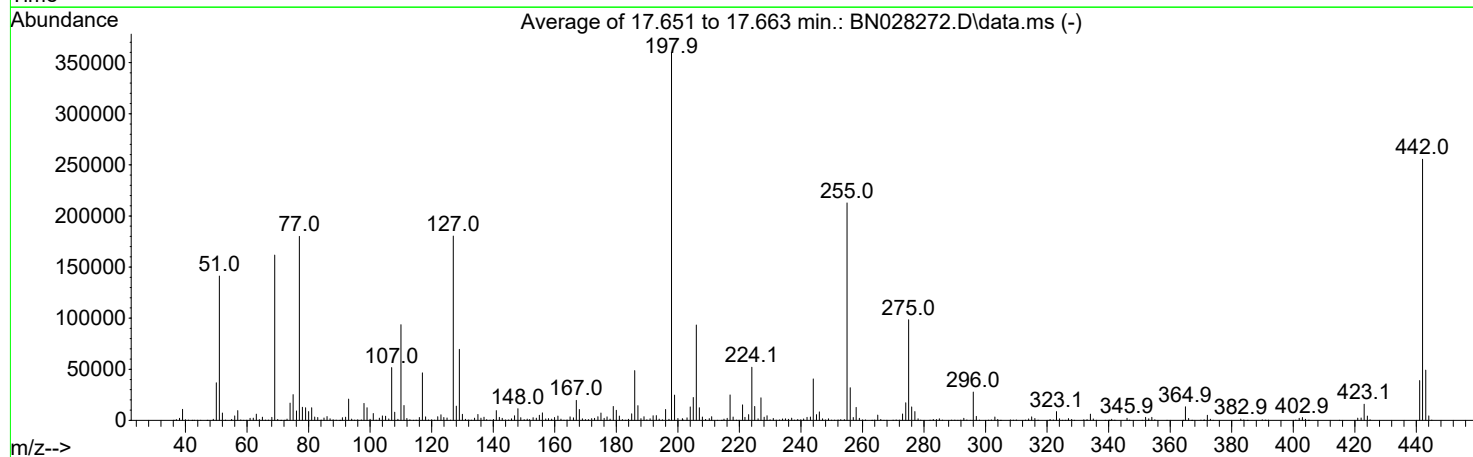


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101323\
Data File : BN028272.D
Acq On : 13 Oct 2023 08:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 13 02:17:11 2023

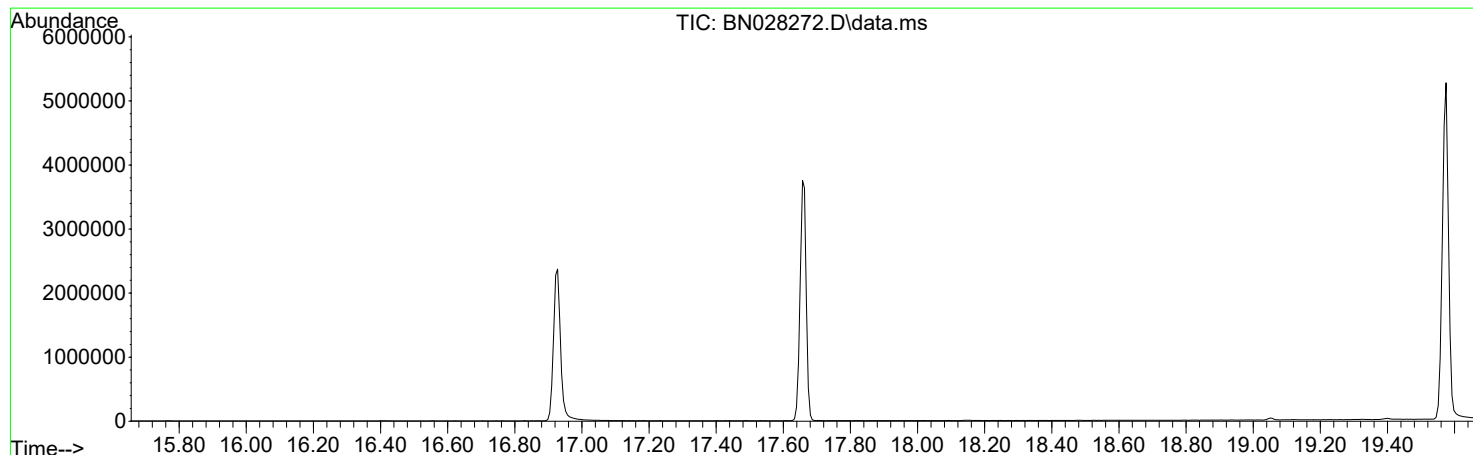

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	141184	PASS
68	69	0.00	2	1.9	3051	PASS
69	198	0.00	100	44.9	161749	PASS
70	69	0.00	2	0.6	893	PASS
127	198	10	80	50.1	180352	PASS
197	198	0.00	2	0.3	1149	PASS
198	198	100	100	100.0	359936	PASS
199	198	5	9	6.9	24723	PASS
275	198	10	60	27.3	98432	PASS
365	198	1	100	3.7	13309	PASS
441	198	0.01	100	10.8	38968	PASS
442	442	50	100	100.0	255509	PASS
443	442	15	24	19.2	49171	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/13/2023	BNA_N	<u>BN028272.D</u>
Compound Name	Response	Retention Time
DDT	1259900	20.763
DDD	49807	20.327
DDE	1257	19.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
51064	1310964	3.90

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101323\
Data File : BN028272.D
Acq On : 13 Oct 2023 08:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 02:49:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:49:17 2023
Response via : Initial Calibration

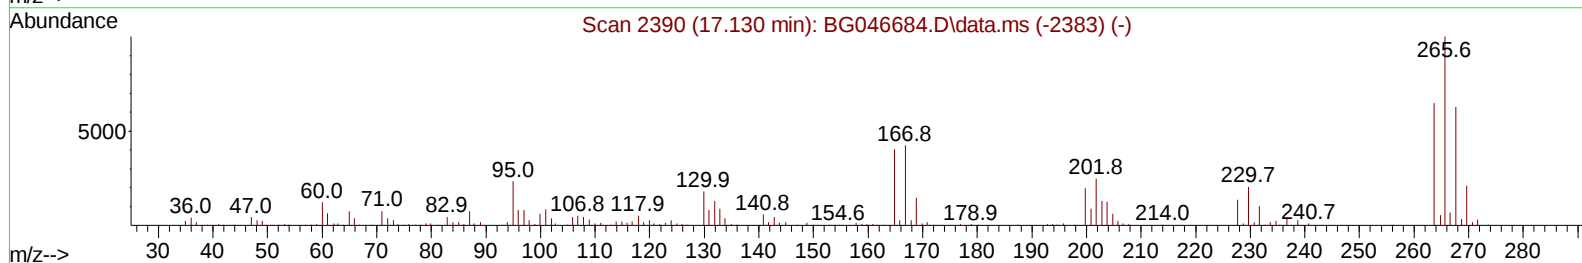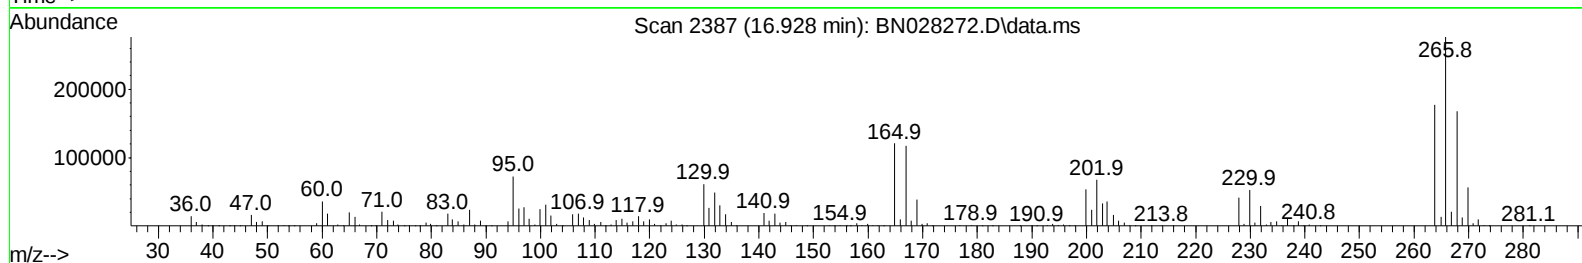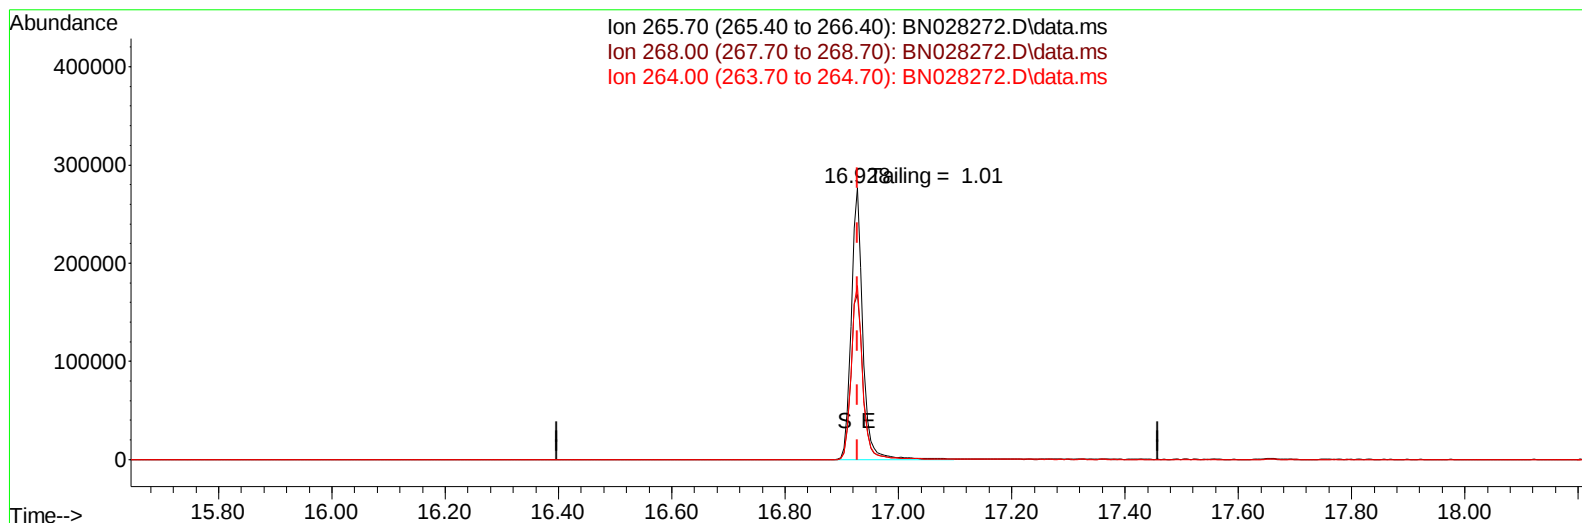

TIC: BN028272.D\data.ms

(70) Pentachlorophenol (C)

16.928min (0.000) 20123.21 ng




response 394331

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.83
264.00	61.60	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101323\
 Data File : BN028272.D
 Acq On : 13 Oct 2023 08:36
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 14 02:49:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 02:49:17 2023
 Response via : Initial Calibration

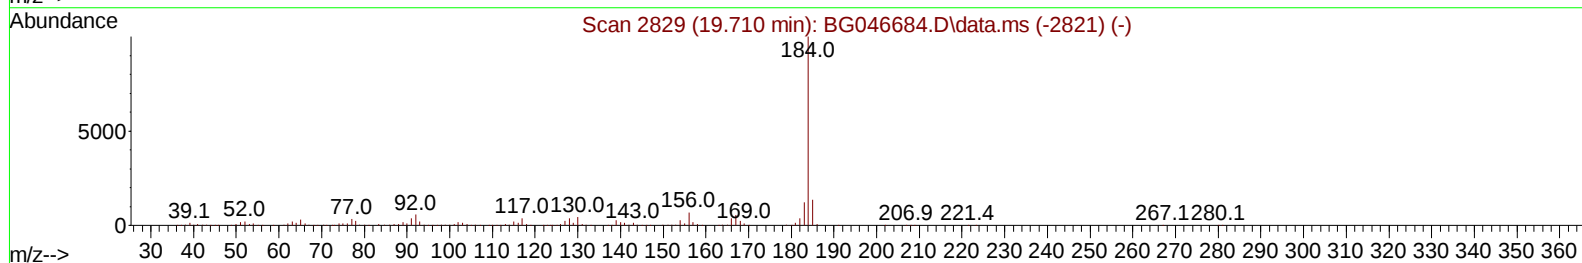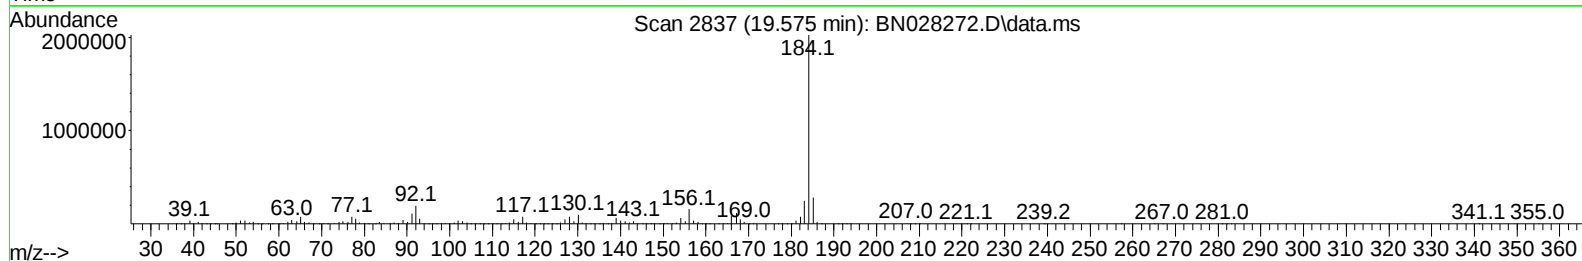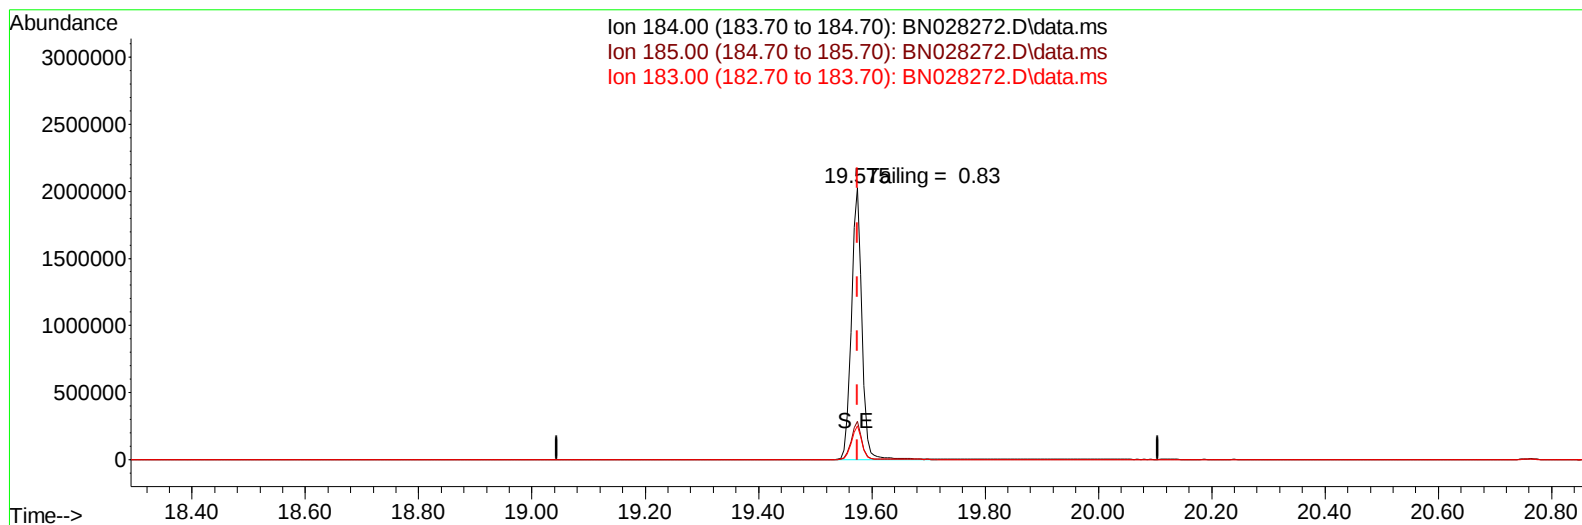

TIC: BN028272.D\data.ms

(77) Benzidine

19.575min (0.000) 1552070.94 ng

response 2631374

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	12.34
0.00	0.00	0.00