
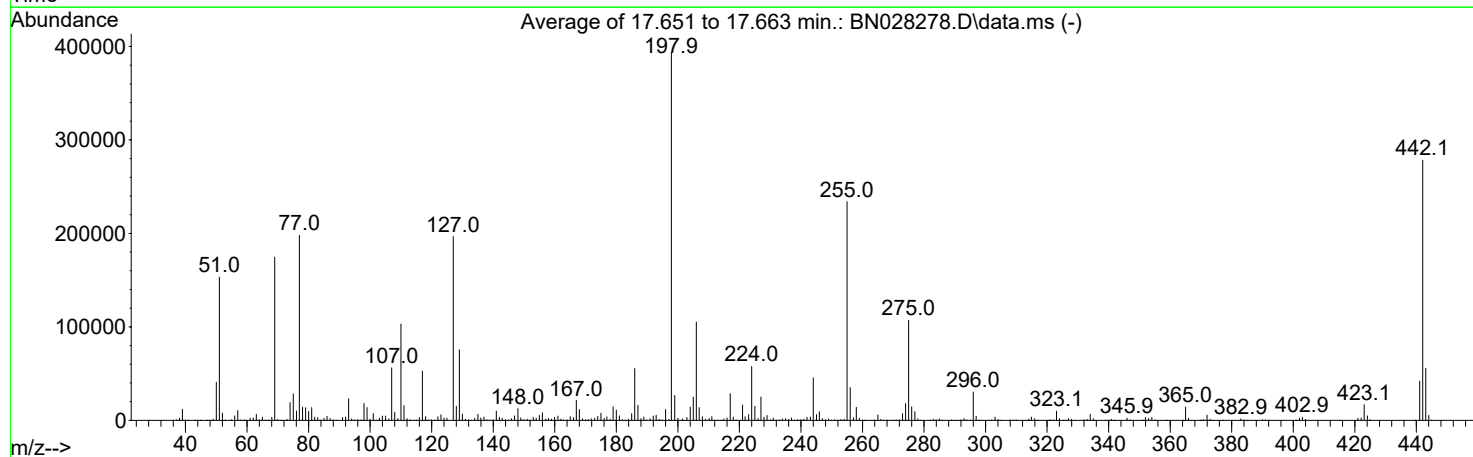


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101323\
 Data File : BN028278.D
 Acq On : 13 Oct 2023 15:16
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 13 02:17:11 2023

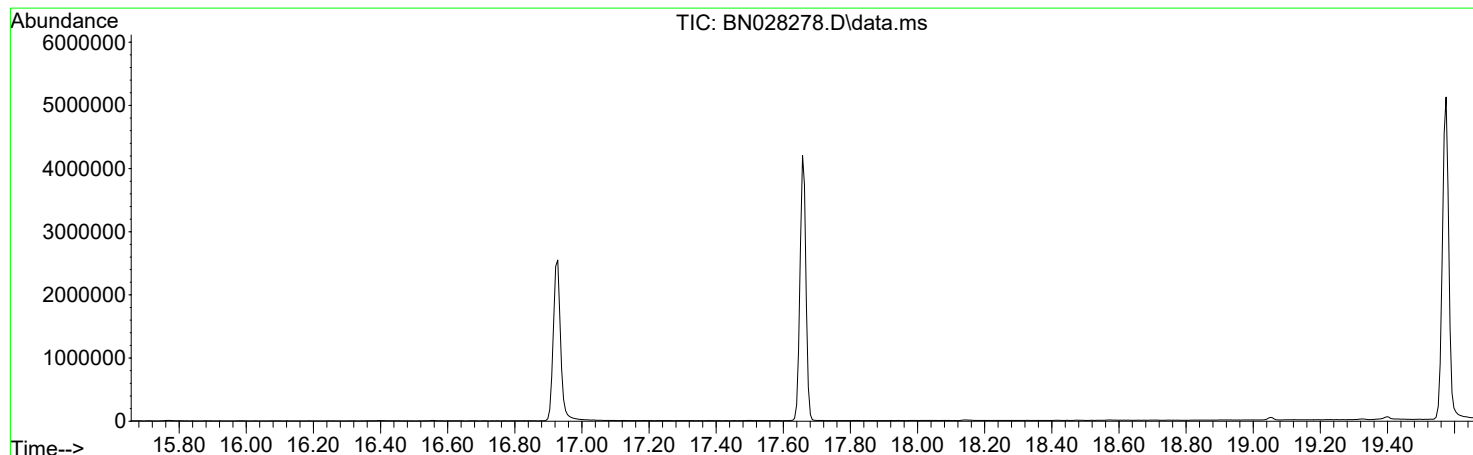

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	153216	PASS
68	69	0.00	2	1.9	3298	PASS
69	198	0.00	100	44.4	174549	PASS
70	69	0.00	2	0.5	928	PASS
127	198	10	80	50.0	196651	PASS
197	198	0.00	2	0.3	994	PASS
198	198	100	100	100.0	393515	PASS
199	198	5	9	6.8	26795	PASS
275	198	10	60	27.2	107043	PASS
365	198	1	100	3.6	14187	PASS
441	198	0.01	100	10.7	41981	PASS
442	442	50	100	100.0	278379	PASS
443	442	15	24	20.1	55829	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/13/2023	BNA_N	<u>BN028278.D</u>
Compound Name	Response	Retention Time
DDT	1367772	20.763
DDD	42947	20.327
DDE	1280	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44227	1411999	3.13

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101323\
Data File : BN028278.D
Acq On : 13 Oct 2023 15:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 02:50:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:49:17 2023
Response via : Initial Calibration

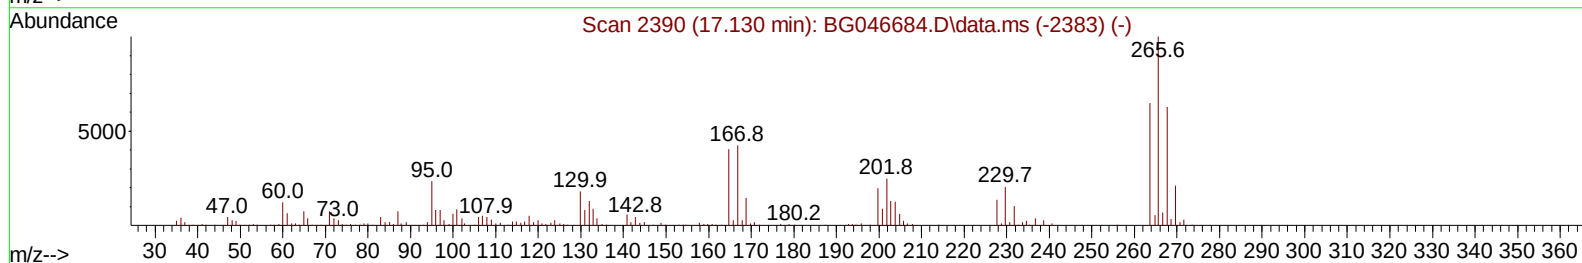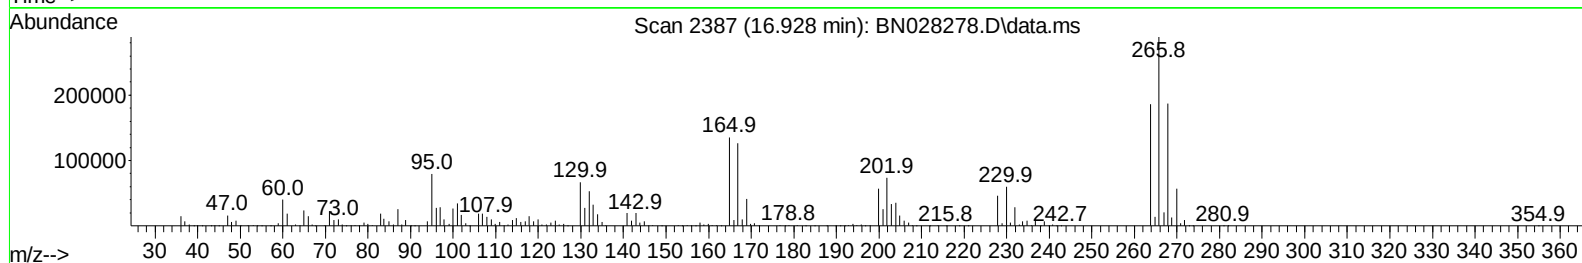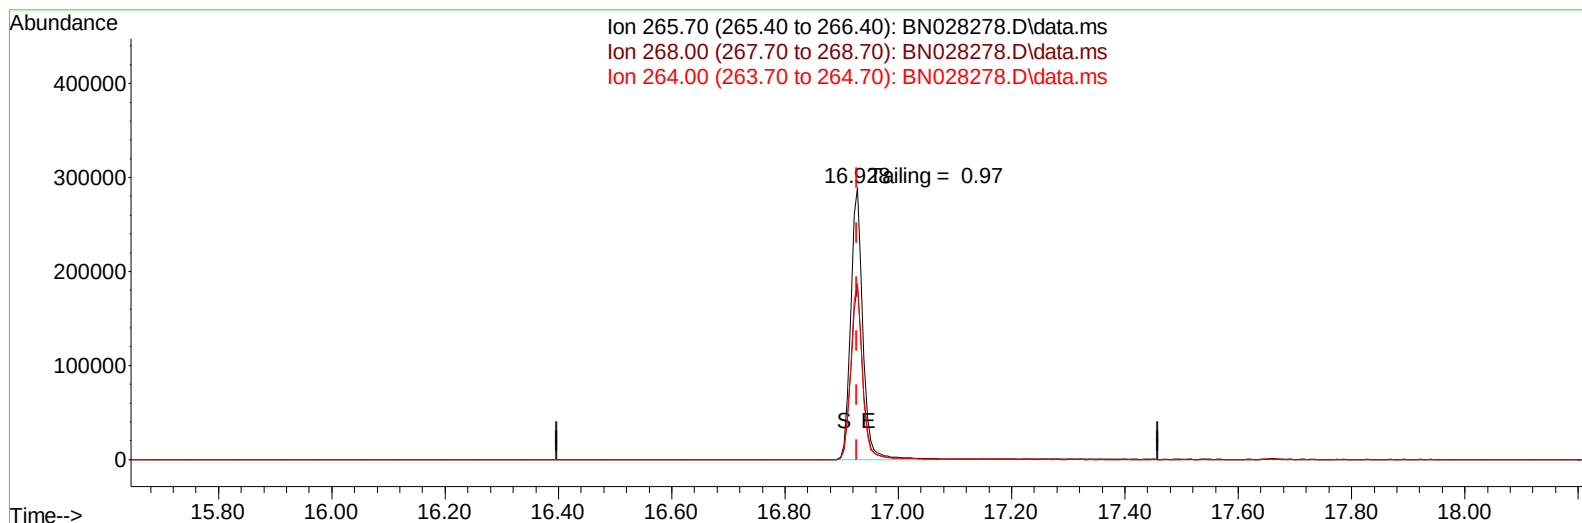

TIC: BN028278.D\data.ms

(70) Pentachlorophenol (C)

16.928min (+ 0.000) 20393.69 ng




response 431160

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.67
264.00	61.60	64.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101323\
Data File : BN028278.D
Acq On : 13 Oct 2023 15:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 02:50:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:49:17 2023
Response via : Initial Calibration

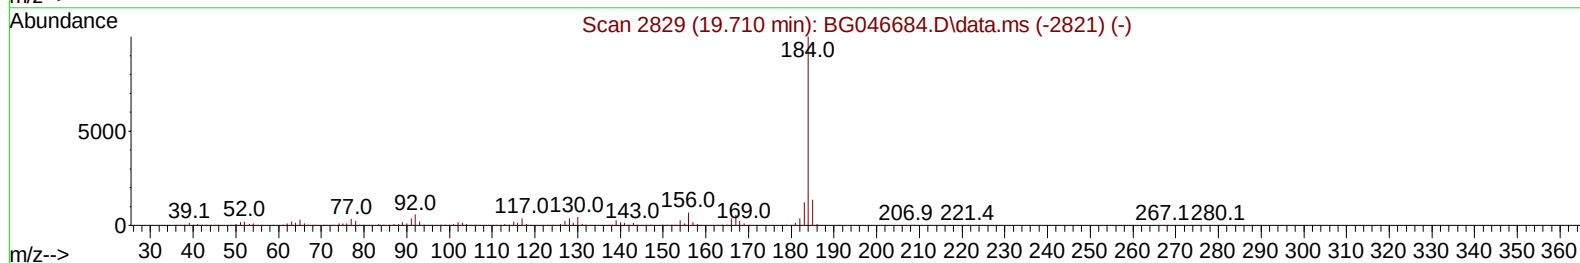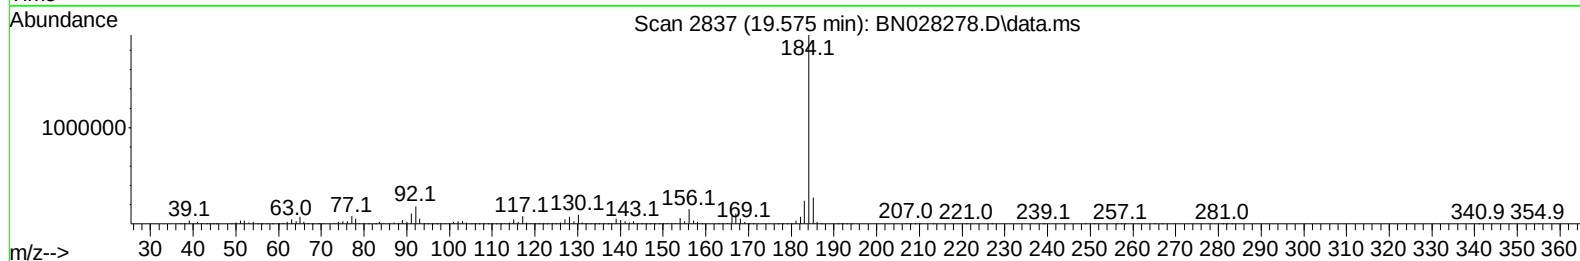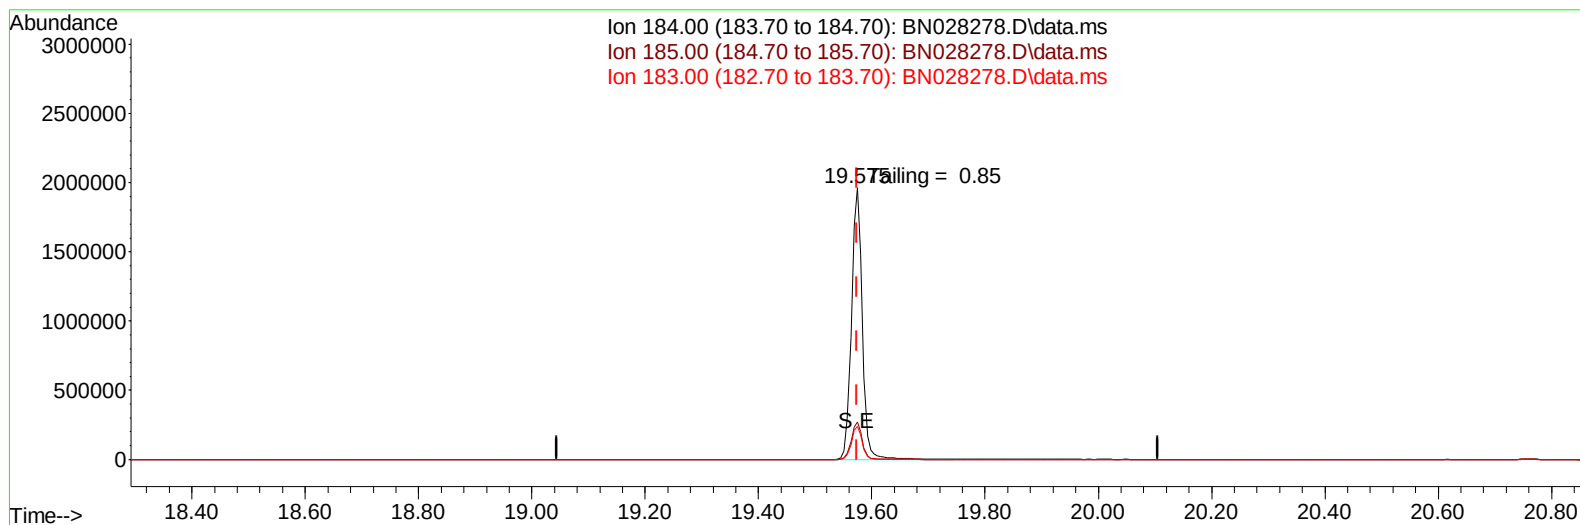

TIC: BN028278.D\data.ms

(77) Benzidine

19.575min (+ 0.000) 0.00 ng

response 2627213

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	12.10
0.00	0.00	0.00