
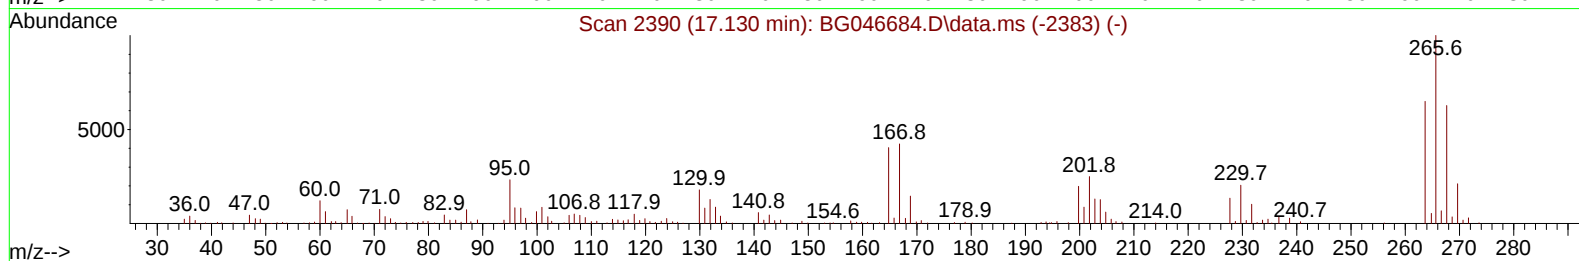
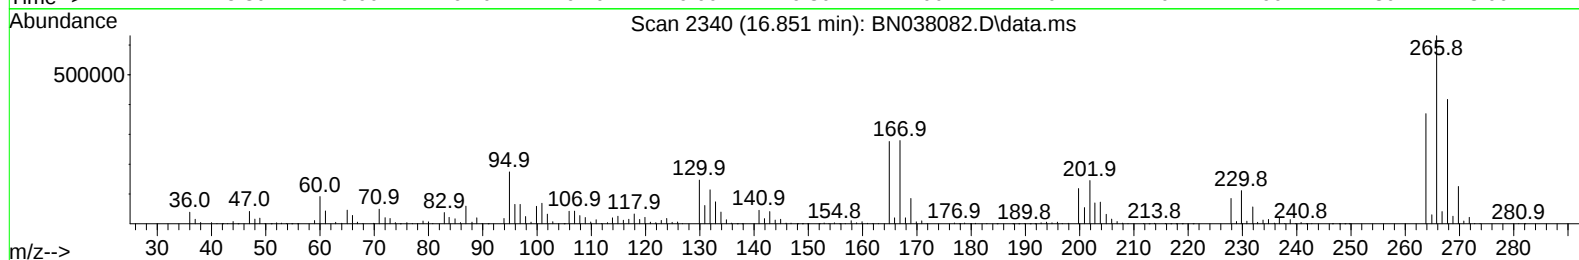


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101325\
Data File : BN038082.D
Acq On : 14 Oct 2025 00:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 04:05:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 13 13:56:00 2025
Response via : Initial Calibration

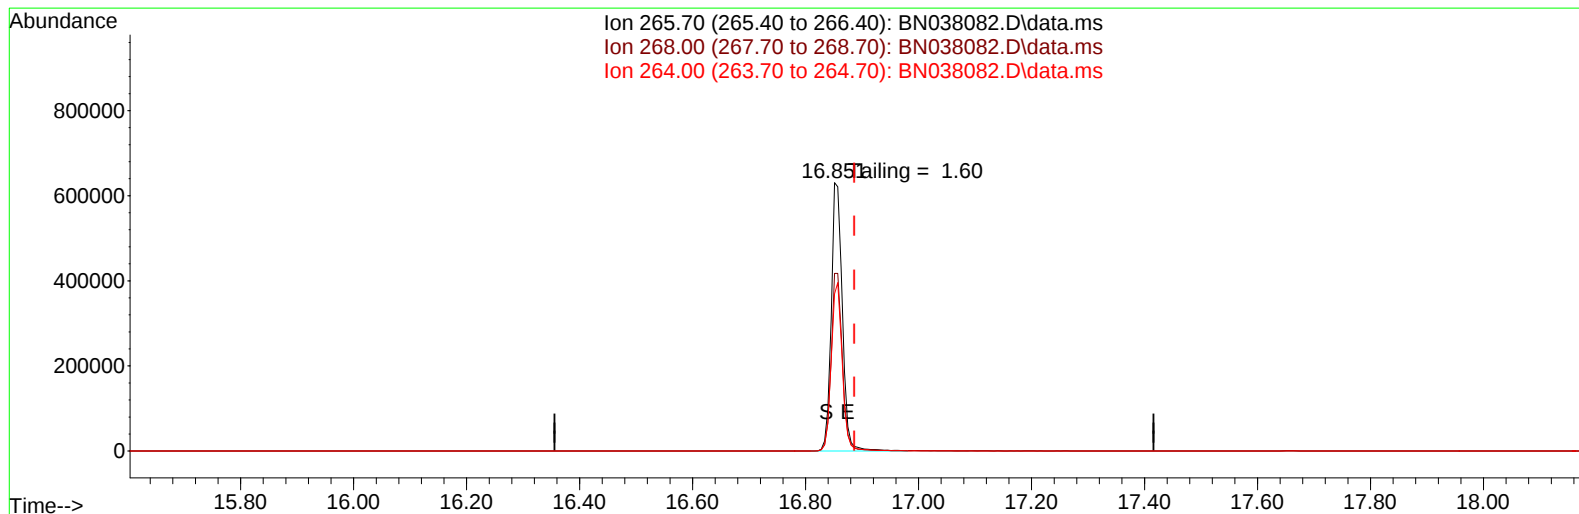

TIC: BN038082.D\data.ms

(70) Pentachlorophenol (C)




16.851min (-0.035) 0.00 ng

response 862228

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.16
264.00	61.60	58.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101325\
Data File : BN038082.D
Acq On : 14 Oct 2025 00:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 04:05:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 13 13:56:00 2025
Response via : Initial Calibration

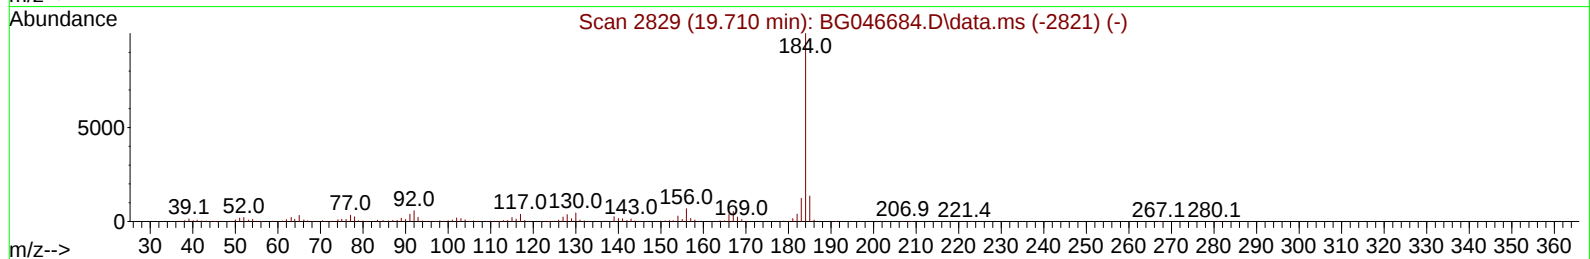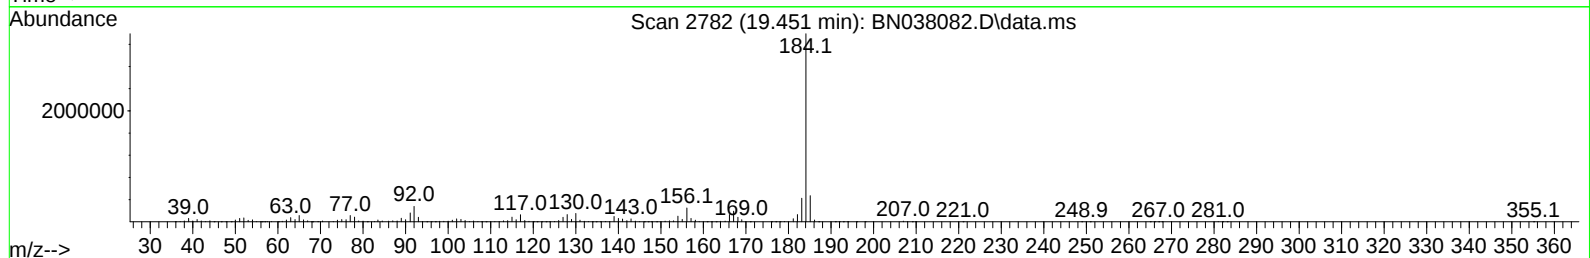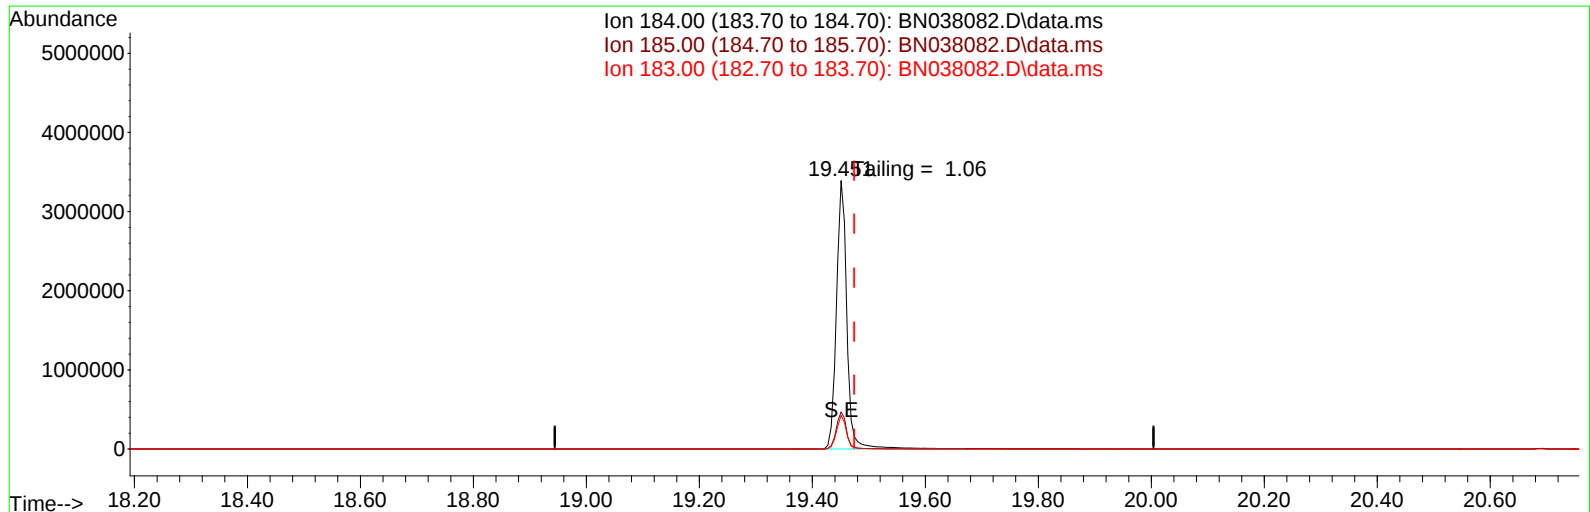

TIC: BN038082.D\data.ms

(77) Benzdine

19.451min (-0.023) 0.00 ng

response 4359890

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.86
183.00	13.20	12.55
0.00	0.00	0.00