


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101325\
Data File : BN038065.D
Acq On : 13 Oct 2025 13:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 24 11:00:01 2025

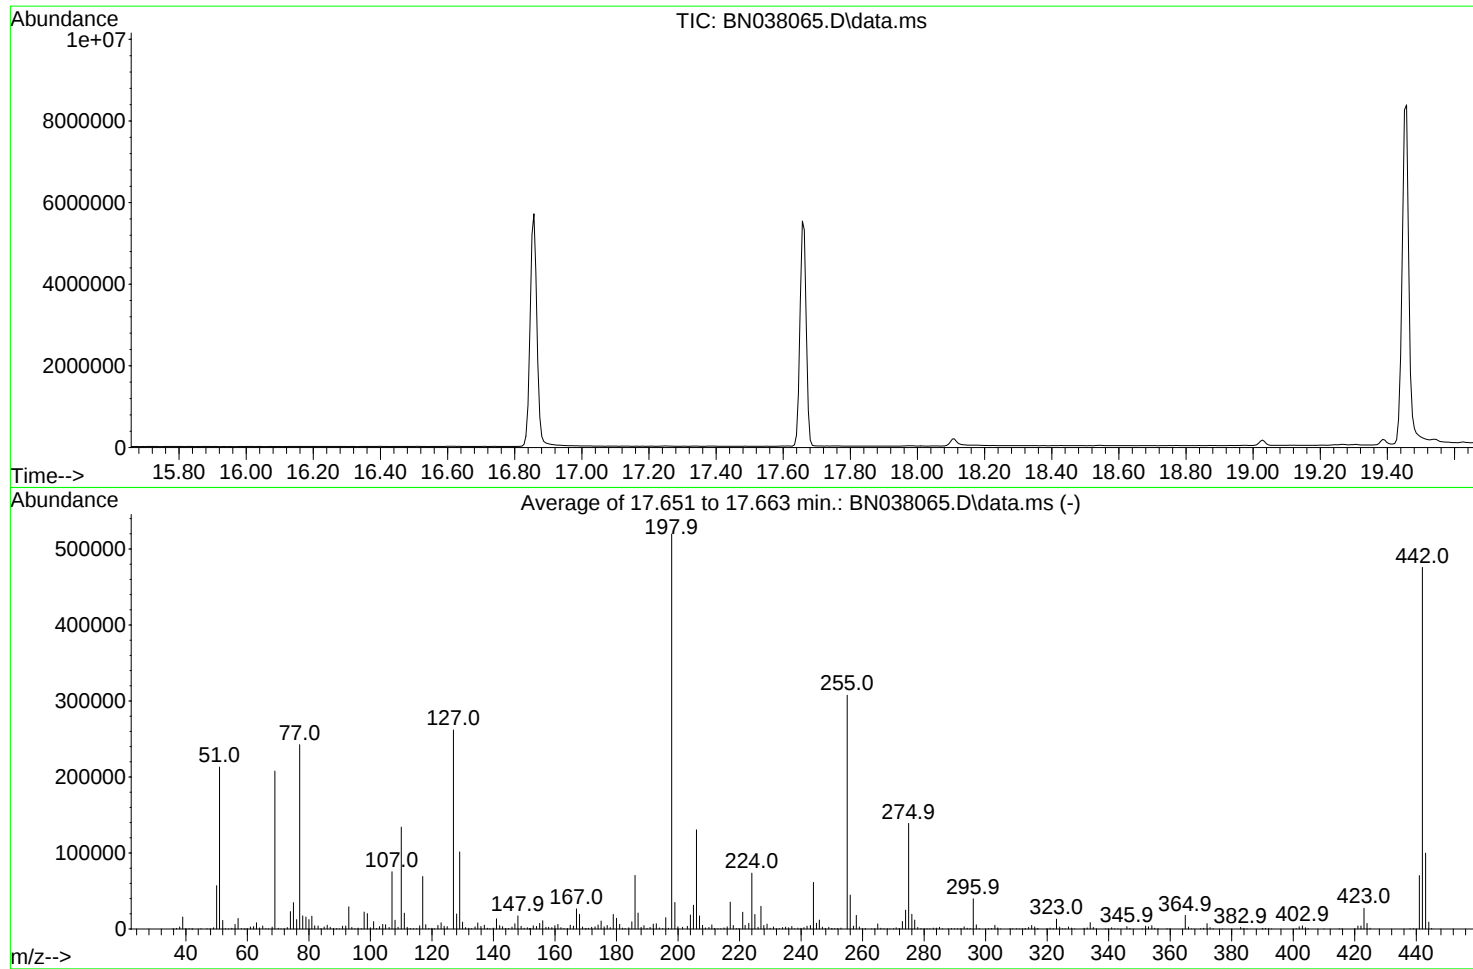




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.2	2414	PASS
69	69	100	100	100.0	207810	PASS
70	69	0.00	2	0.5	1031	PASS
197	198	0.00	2	0.2	1009	PASS
198	198	100	100	100.0	519680	PASS
199	198	5	9	6.7	34837	PASS
365	198	1	100	3.4	17780	PASS
441	443	0.01	150	70.3	70149	PASS
442	442	100	100	100.0	475904	PASS
443	442	15	24	21.0	99800	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101325\
Data File : BN038065.D
Acq On : 13 Oct 2025 13:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 13 13:56:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 13 13:56:00 2025
Response via : Initial Calibration

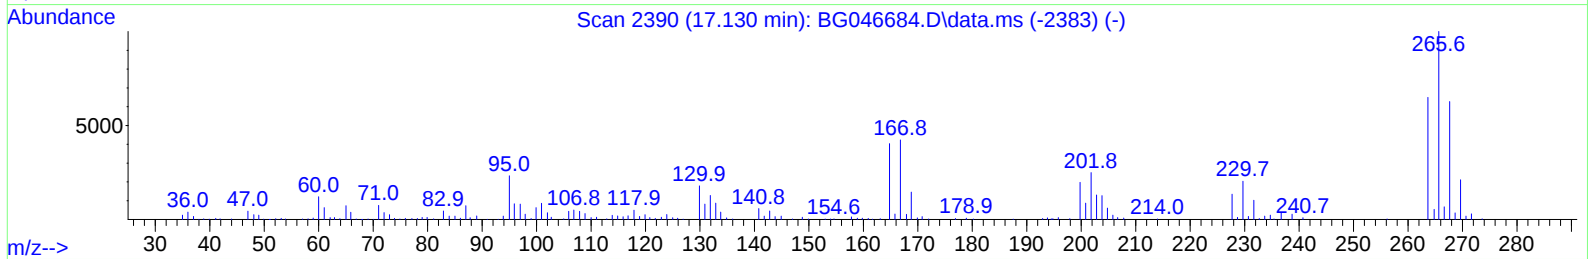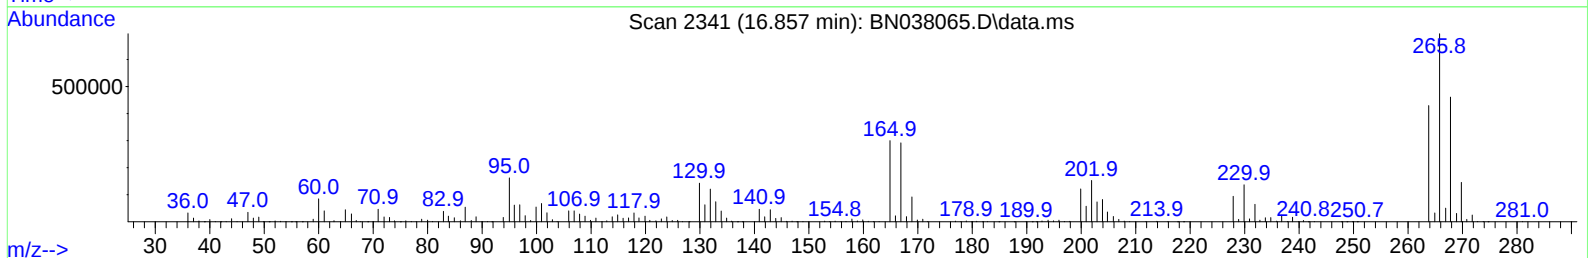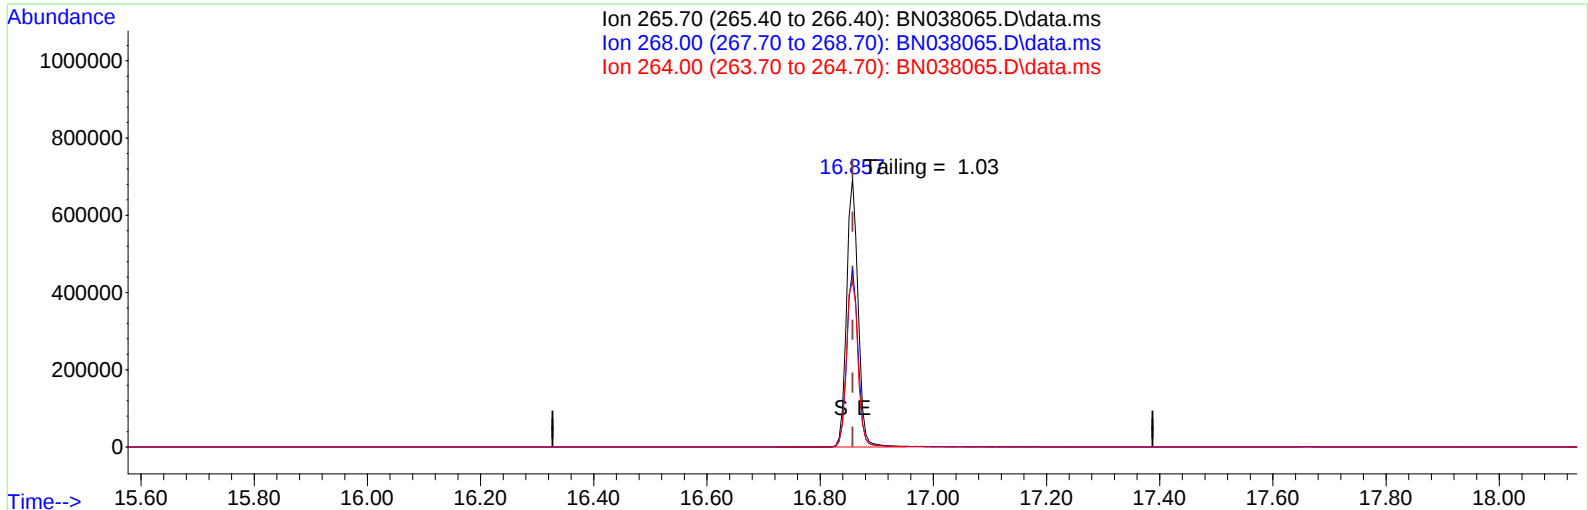

TIC: BN038065.D\data.ms

(70) Pentachlorophenol (C)

16.857min (0.000) 0.00 ng




response 981737

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.35
264.00	61.60	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101325\
Data File : BN038065.D
Acq On : 13 Oct 2025 13:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 13 13:56:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 13 13:56:00 2025
Response via : Initial Calibration

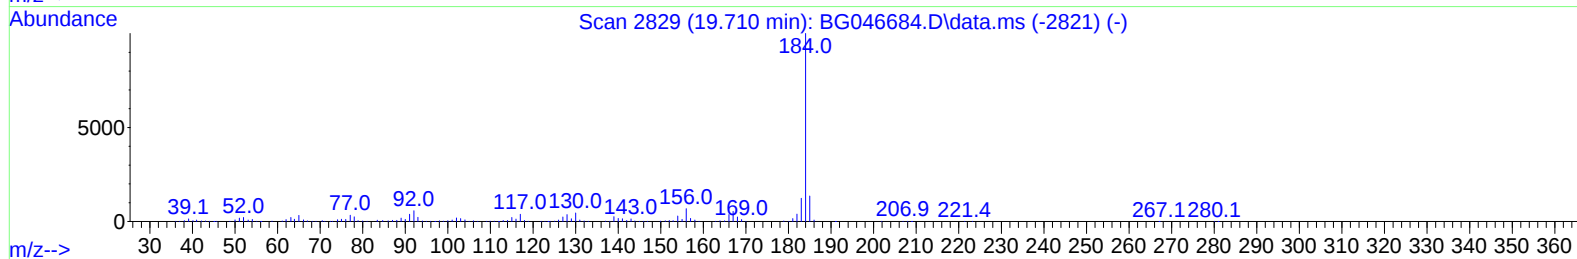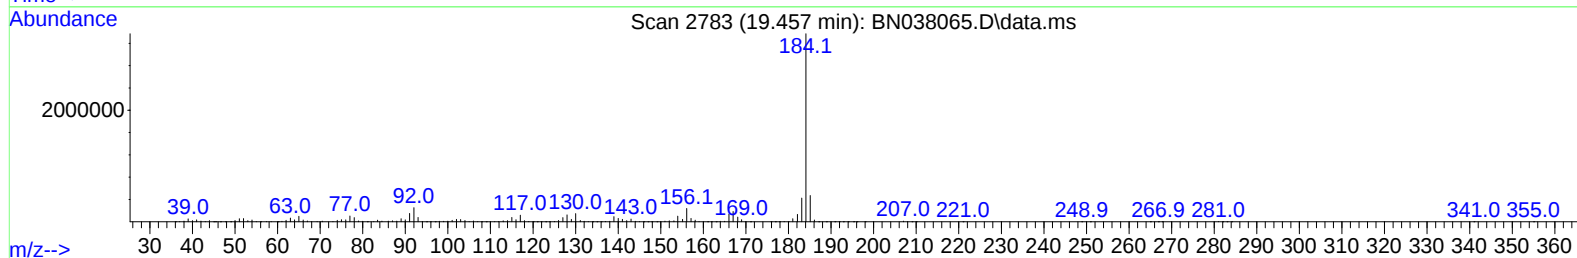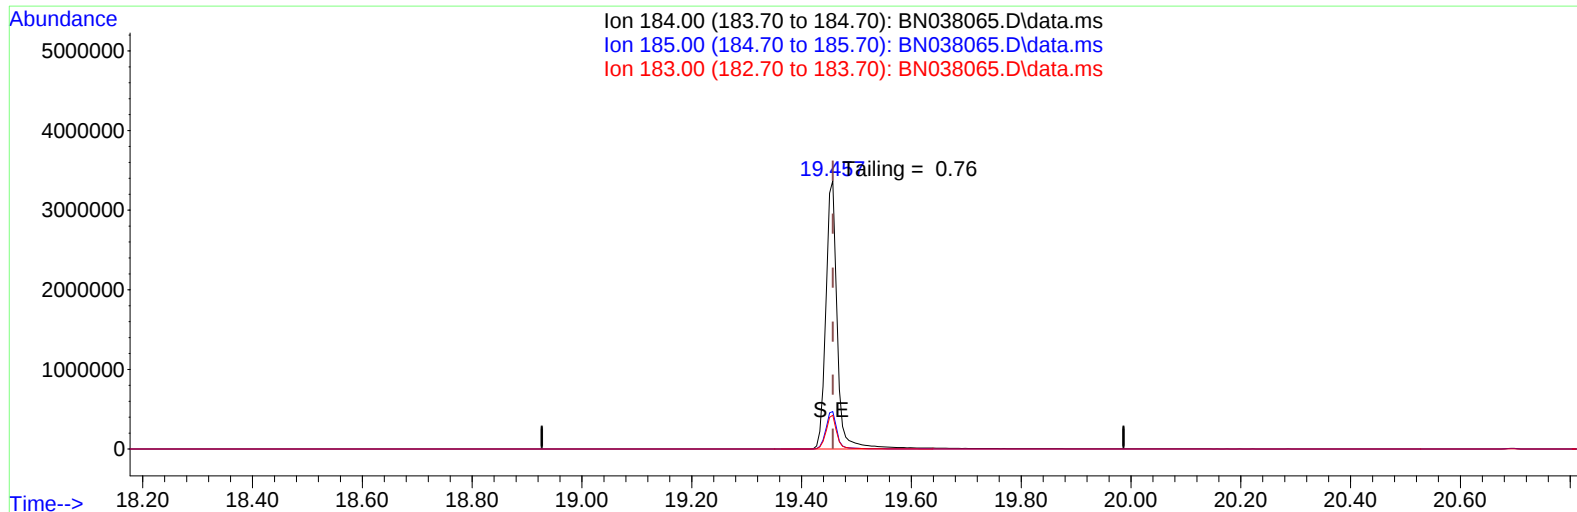

TIC: BN038065.D\data.ms

(77) Benzidine

19.457min (0.000) 0.00 ng

response 4930116

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.95
183.00	13.20	12.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2025	BNA_N	<u>BN038065.D</u>
Compound Name	Response	Retention Time
DDT	1986801	20.692
DDD	17211	20.251
DDE	771	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17982	2004783	0.90

Instrument :
BNA_N
ClientSampleId :
DFTPP