

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
 Data File : BN008144.D
 Acq On : 14 Oct 2019 21:01
 Operator : JU
 Sample : K5096-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 15 03:02:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:19:29 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	2347	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	11646	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	7795	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	1123437	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.21
20) Perylene-d12	23.39	264	18810	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	4408	0.22	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.25	252	3701	0.057	ng/ul#	Ovalue 57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008144.D
Acq On : 14 Oct 2019 21:01
Operator : JU
Sample : K5096-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 15 03:02:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

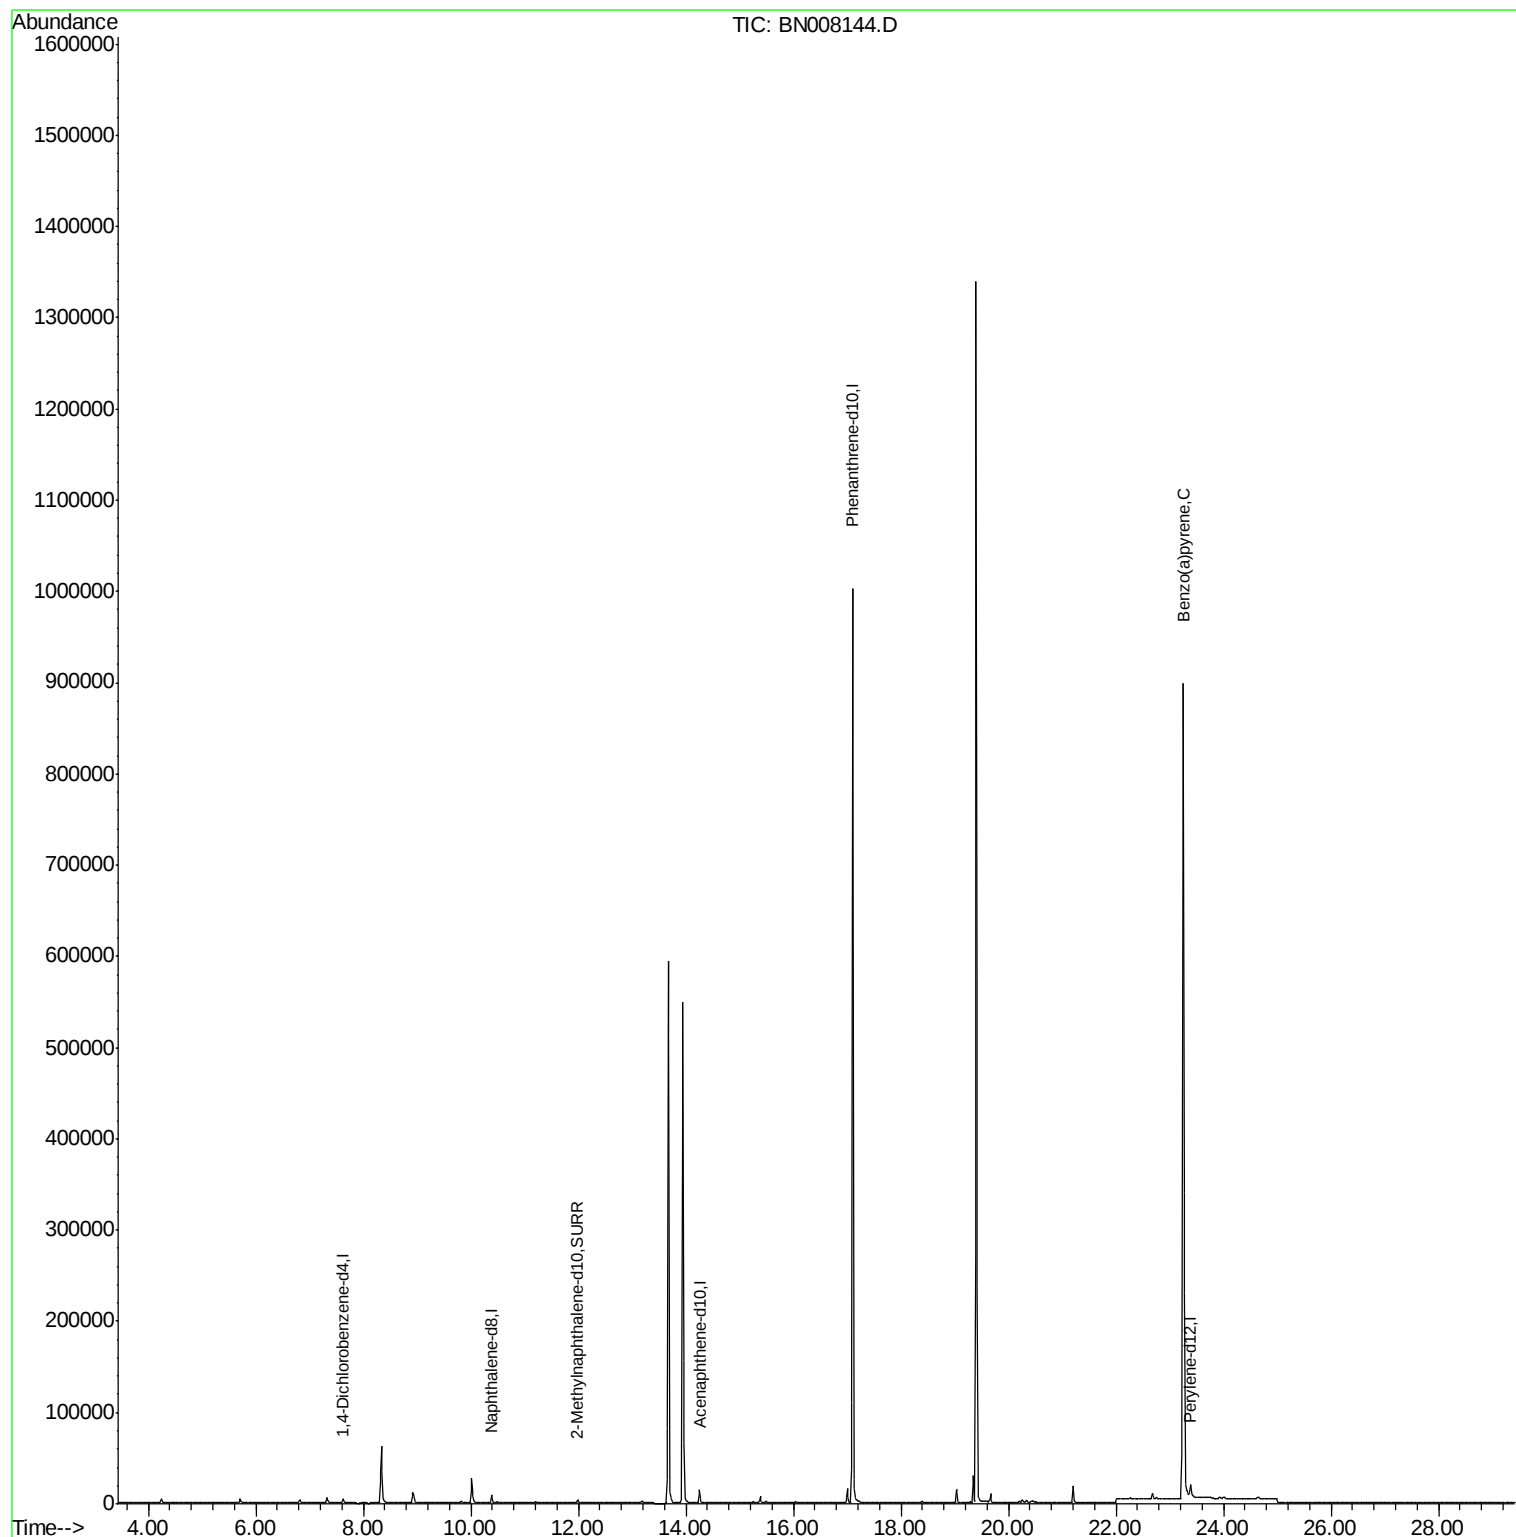

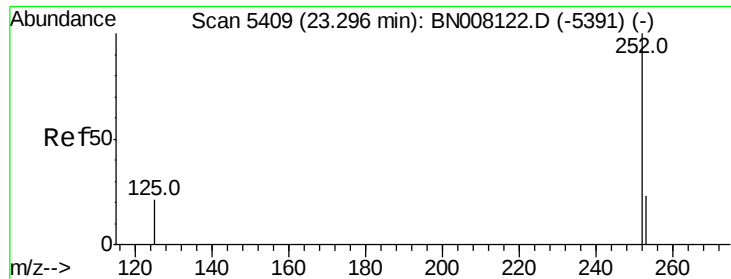

#23

Benzo(a)pyrene

Concen: 0.057 ng/ul

RT: 23.25 min Scan# 5394

Delta R.T. -0.05 min


Lab File: BN008144.D

Acq: 14 Oct 2019 21:01

Instrument :

BNA_N

ClientSampleId :

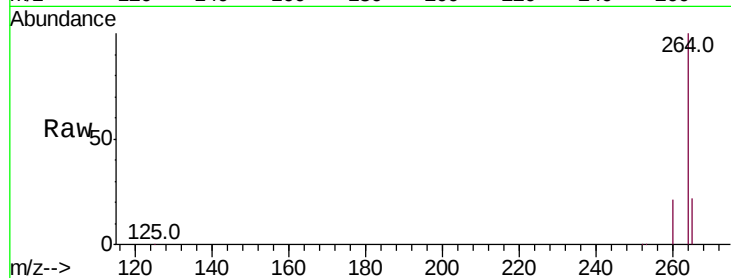

Tot Ion: 252 Resp: 3701

Ion Ratio Lower Upper

252 100

253 47.7 22.8 34.2#

125 48.3 18.4 27.6#

