

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
 Data File : BN008146.D
 Acq On : 14 Oct 2019 22:13
 Operator : JU
 Sample : K5096-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 15 03:02:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:19:29 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	2699	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	13245	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	8654	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	1496084	0.40	ng/ul	0.10
16) Chrysene-d12	21.38	240	57	0.40	ng/ul	0.17
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.40
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	5223	0.23	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
18) Benzo(a)anthracene	21.38	228	5	0.024	ng/ul#	Ovalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008146.D
Acq On : 14 Oct 2019 22:13
Operator : JU
Sample : K5096-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 15 03:02:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

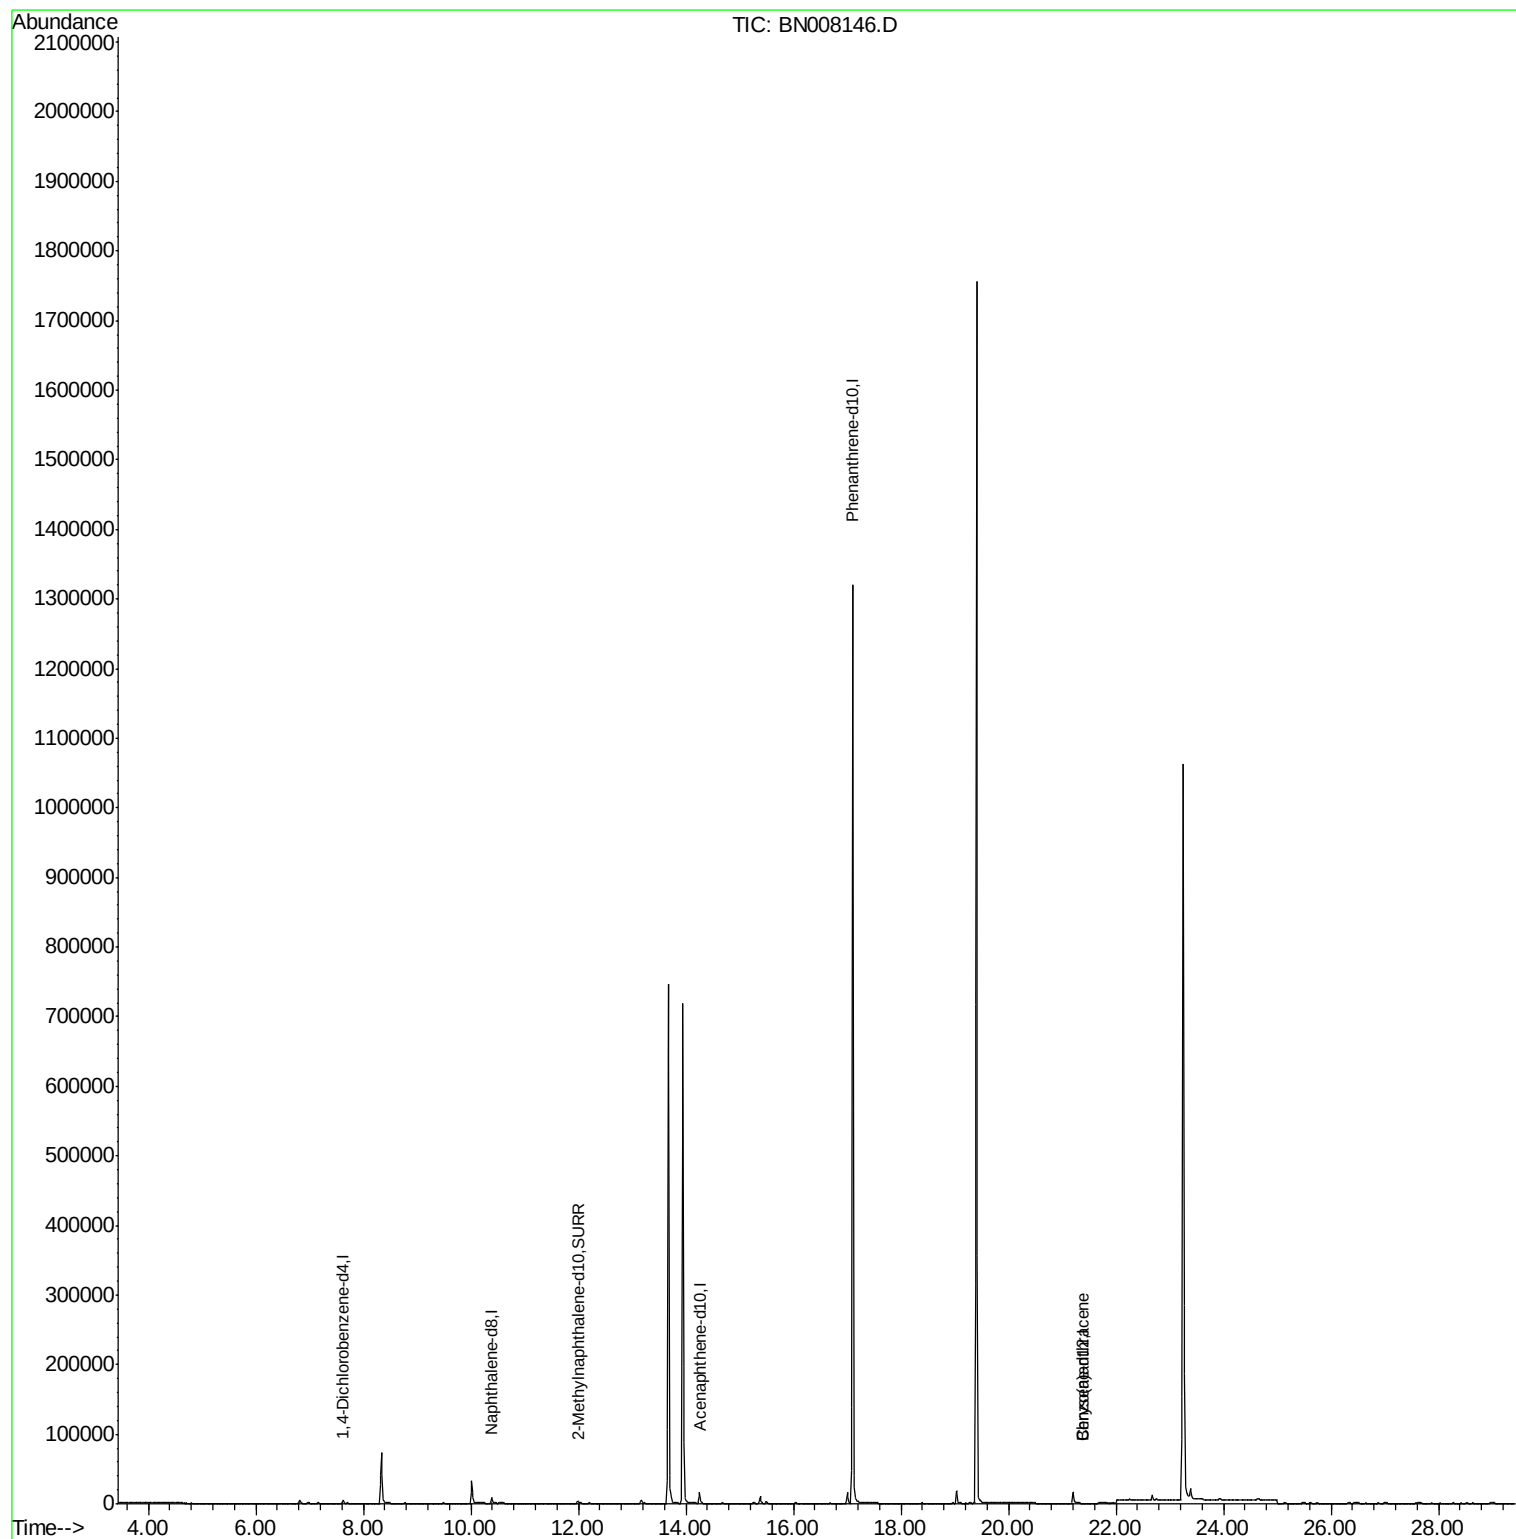

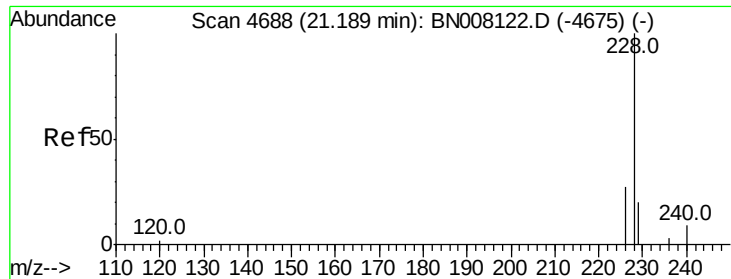

#18

Benzo(a)anthracene

Concen: 0.024 ng/ul

RT: 21.38 min Scan# 4753

Delta R.T. 0.19 min

Lab File: BN008146.D

Acq: 14 Oct 2019 22:13

Instrument :

BNA_N

ClientSampleId :

Tot Ion:228	Resp:	5
Ion	Ratio	Lower Upper
228	100	
229	122.7	16.2 24.2#
226	125.0	21.4 32.0#

