

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
 Data File : BN008151.D
 Acq On : 15 Oct 2019 01:47
 Operator : JU
 Sample : K5097-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 15 03:03:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:19:29 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	2094	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	10516	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	7005	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	15814	0.40	ng/ul	0.00
16) Chrysene-d12	21.20	240	15321	0.40	ng/ul	0.00
20) Perylene-d12	23.38	264	14654	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	1797	0.10	ng/ul	0.00
14) Fluoranthene-d10	19.04	212	5619	0.10	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.24	252	1423	0.028	ng/ul#	Ovalue 13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008151.D
Acq On : 15 Oct 2019 01:47
Operator : JU
Sample : K5097-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 15 03:03:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

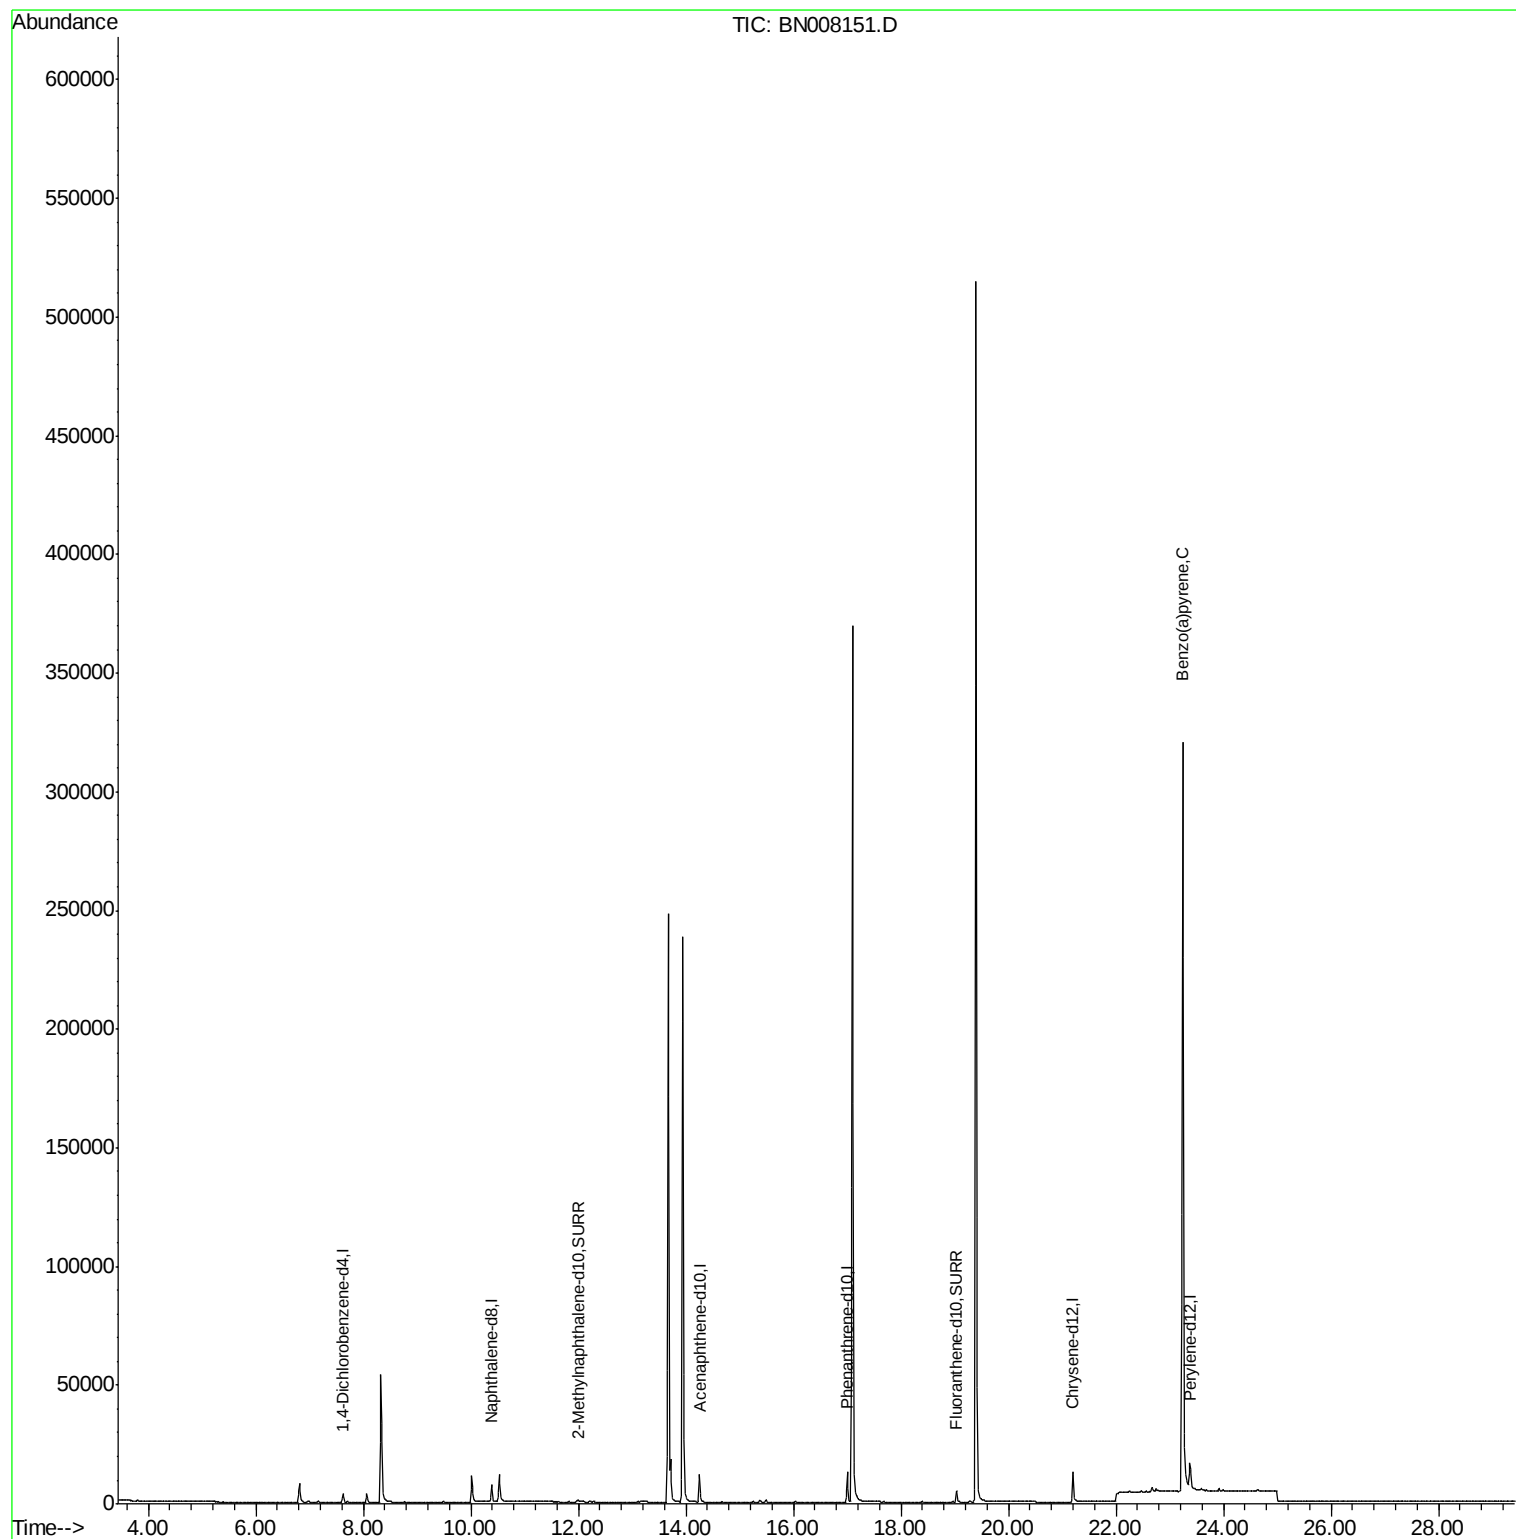

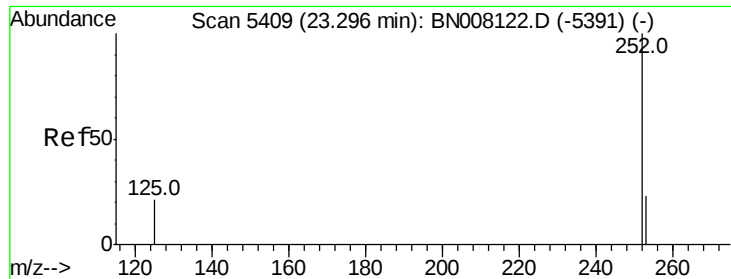

#23

Benzo(a)pyrene

Concen: 0.028 ng/ul

RT: 23.24 min Scan# 5391

Delta R.T. -0.06 min


Lab File: BN008151.D

Acq: 15 Oct 2019 01:47

Instrument :

BNA_N

ClientSampleId :

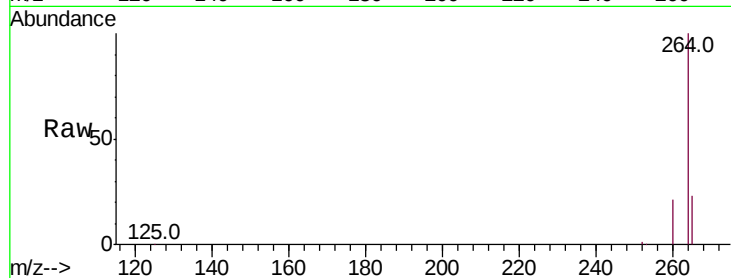

Tot Ion:252 Resp: 1423

Ion Ratio Lower Upper

252 100

253 68.3 22.8 34.2#

125 72.2 18.4 27.6#

