


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101419\
Data File : BN008137.D
Acq On : 14 Oct 2019 16:50
Operator : JU
Sample : K5096-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMG9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:29:53 PM

Quant Time: Oct 14 17:42:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

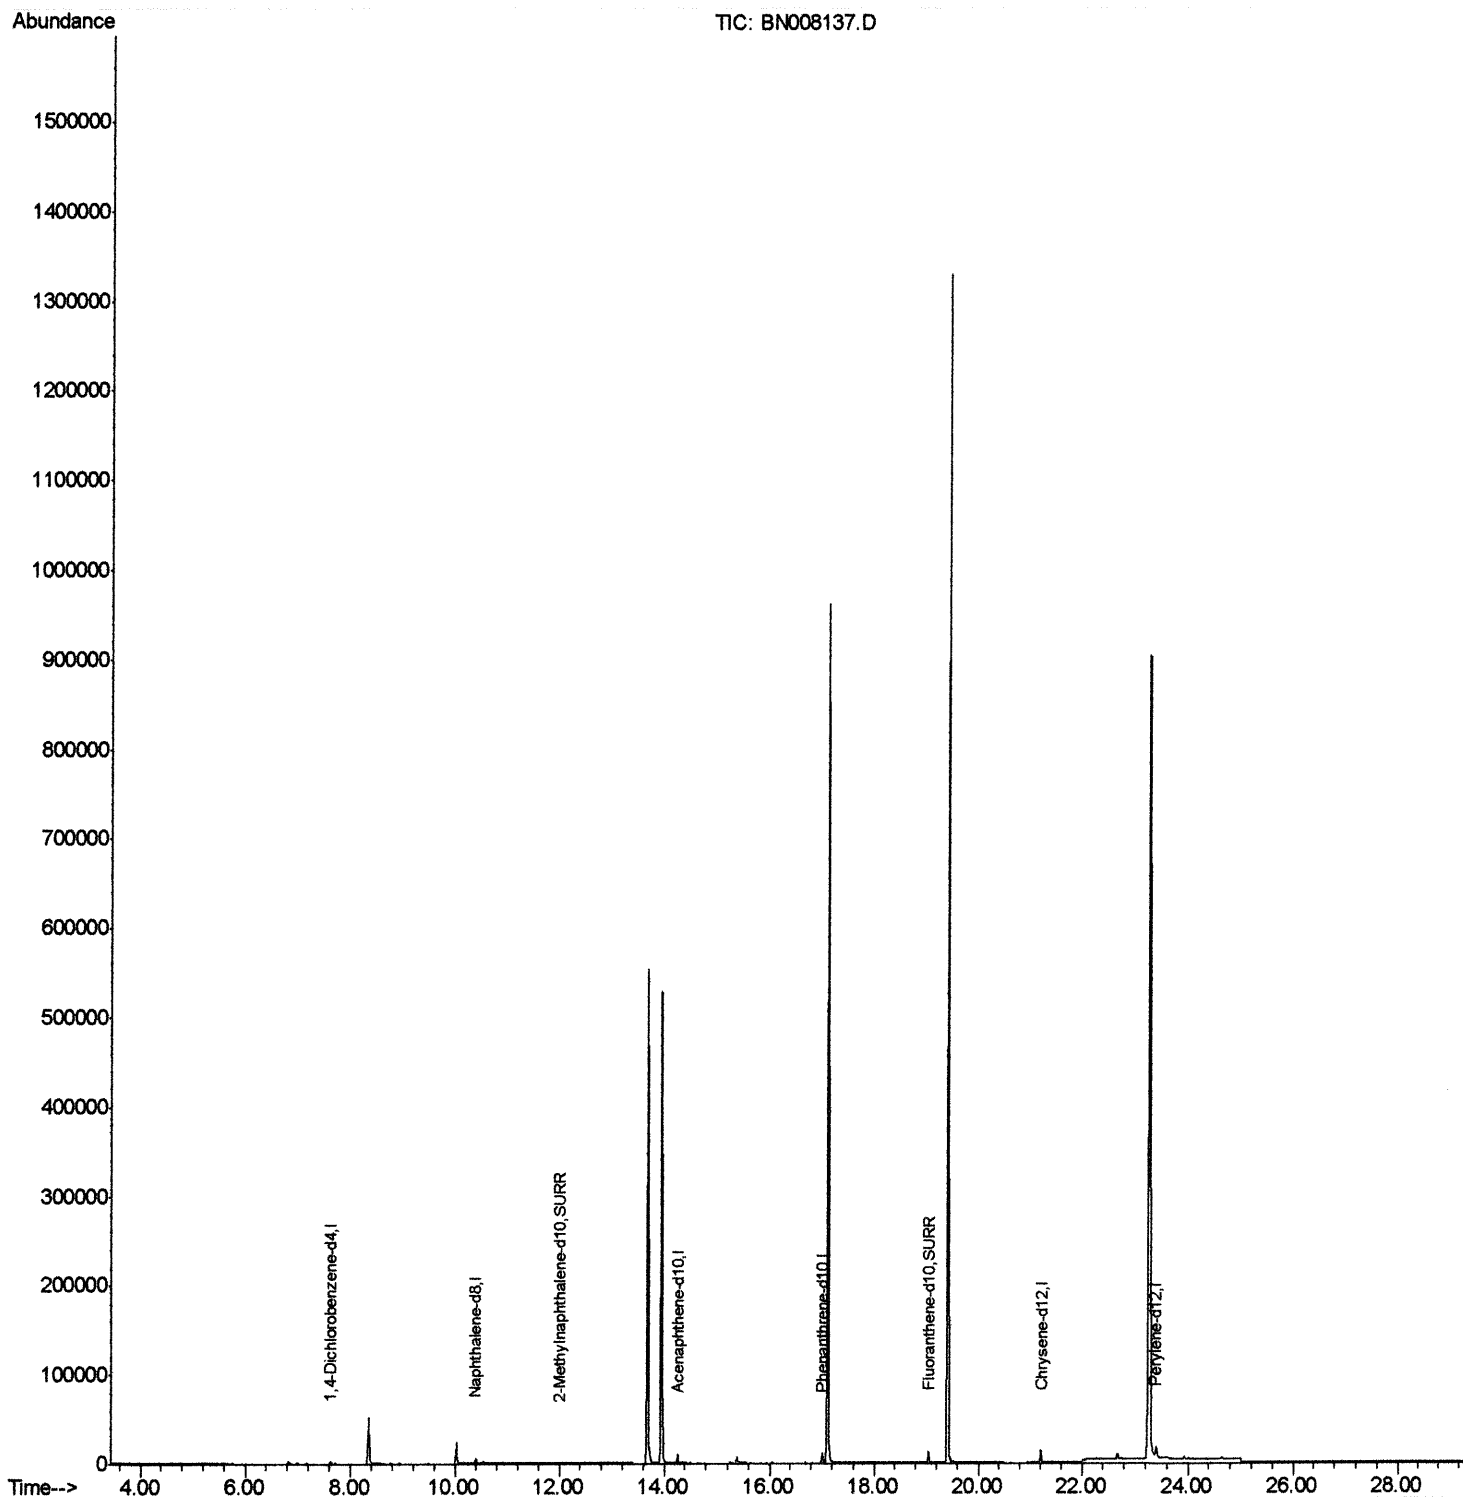




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101419\
Data File : BN008137.D
Acq On : 14 Oct 2019 16:50
Operator : JU
Sample : K5096-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMG9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:29:53 PM

Quant Time: Oct 14 17:40:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

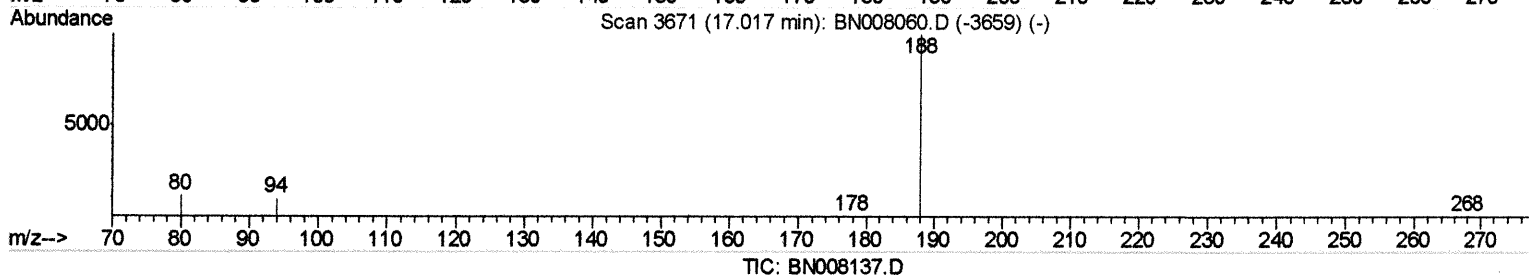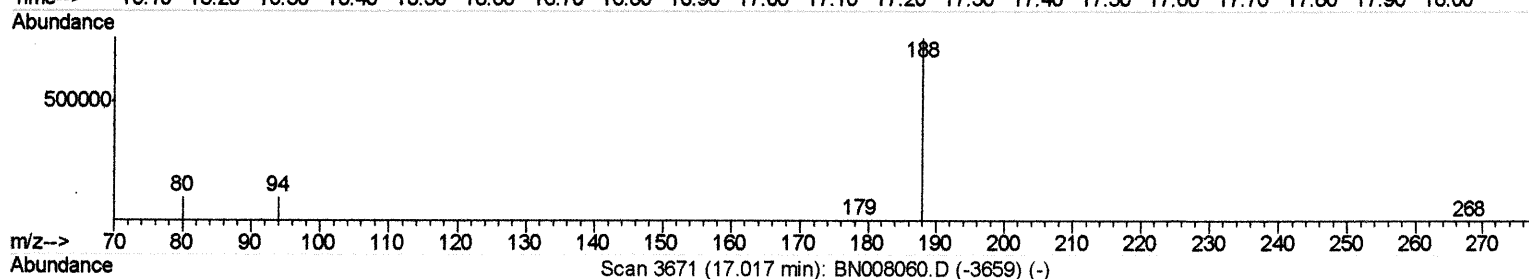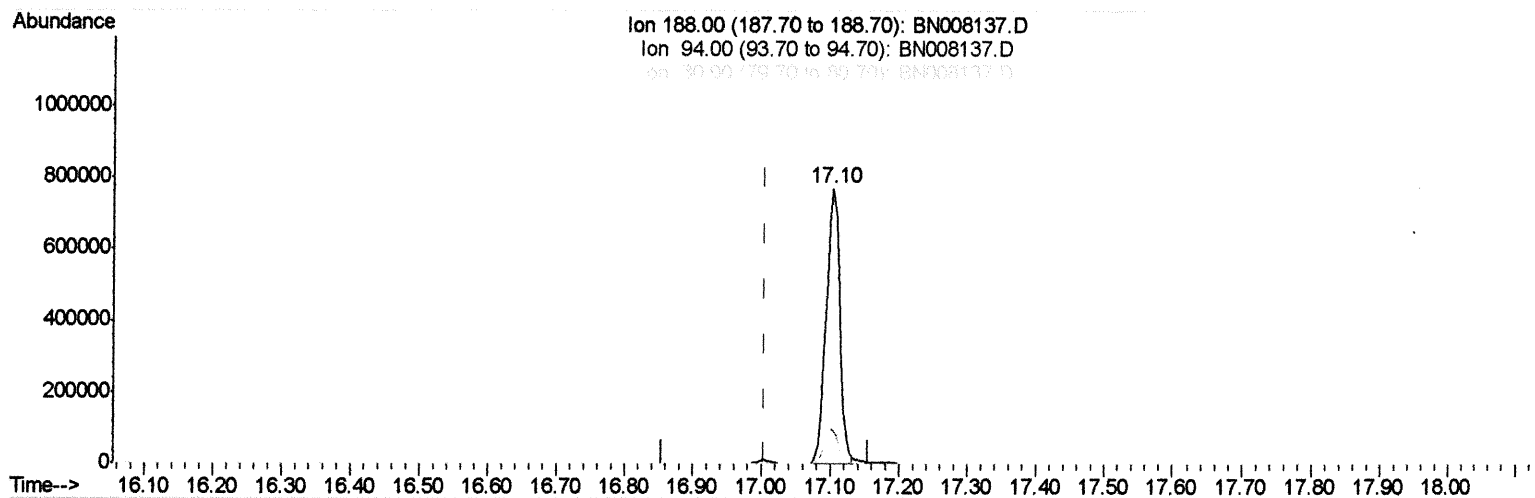

(10) Phenanthrene-d10 (I)

17.102min (+0.097) 0.40ng/ul

response 1073801

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	12.64
80.00	12.60	12.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101419\
Data File : BN008137.D
Acq On : 14 Oct 2019 16:50
Operator : JU
Sample : K5096-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
JLMG9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:29:53 PM

Quant Time: Oct 14 17:40:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

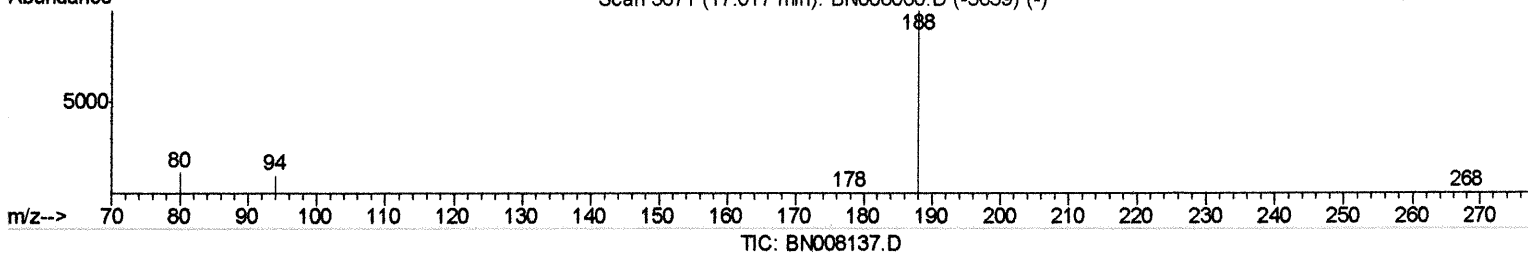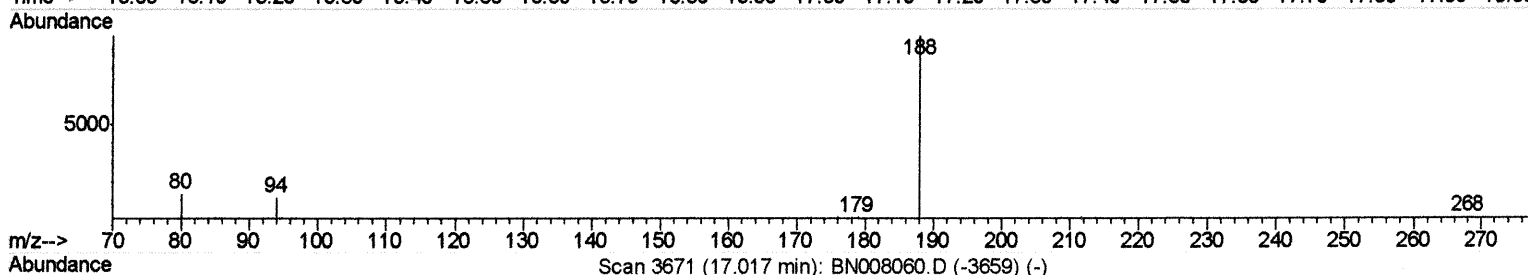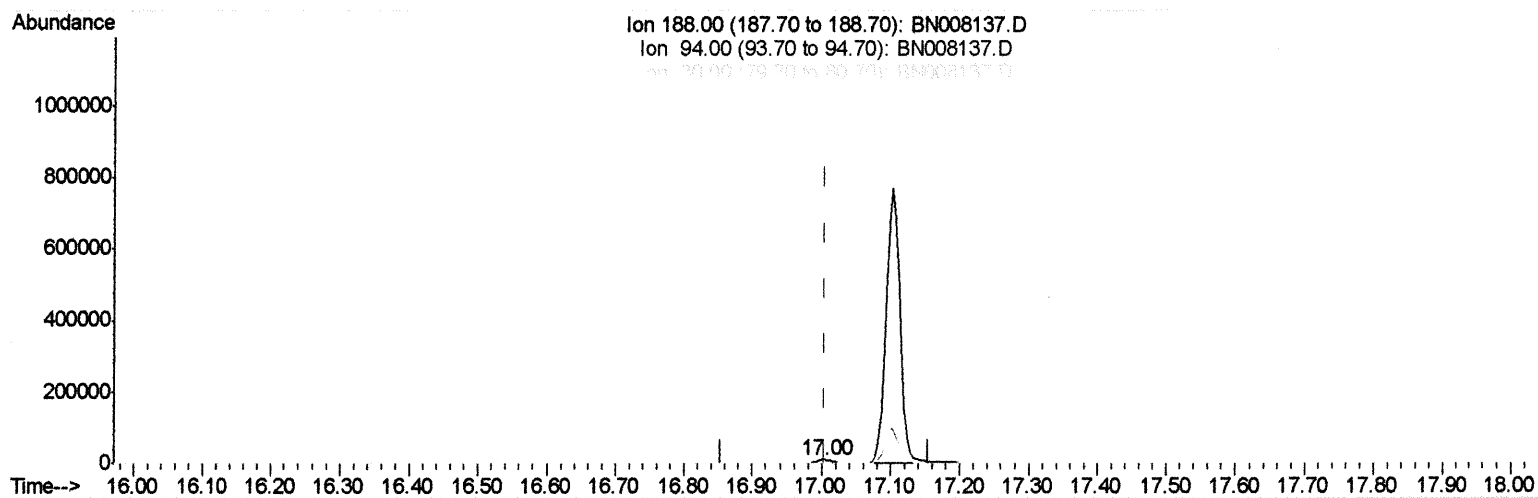

(10) Phenanthrene-d10 (I)

17.004min (-0.000) 0.40ng/ul m *ju 10/16/19*

response 14434

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	11.52
80.00	12.60	13.75
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101419\
Data File : BN008137.D
Acq On : 14 Oct 2019 16:50
Operator : JU
Sample : K5096-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMG9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:29:53 PM

Quant Time: Oct 14 17:40:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

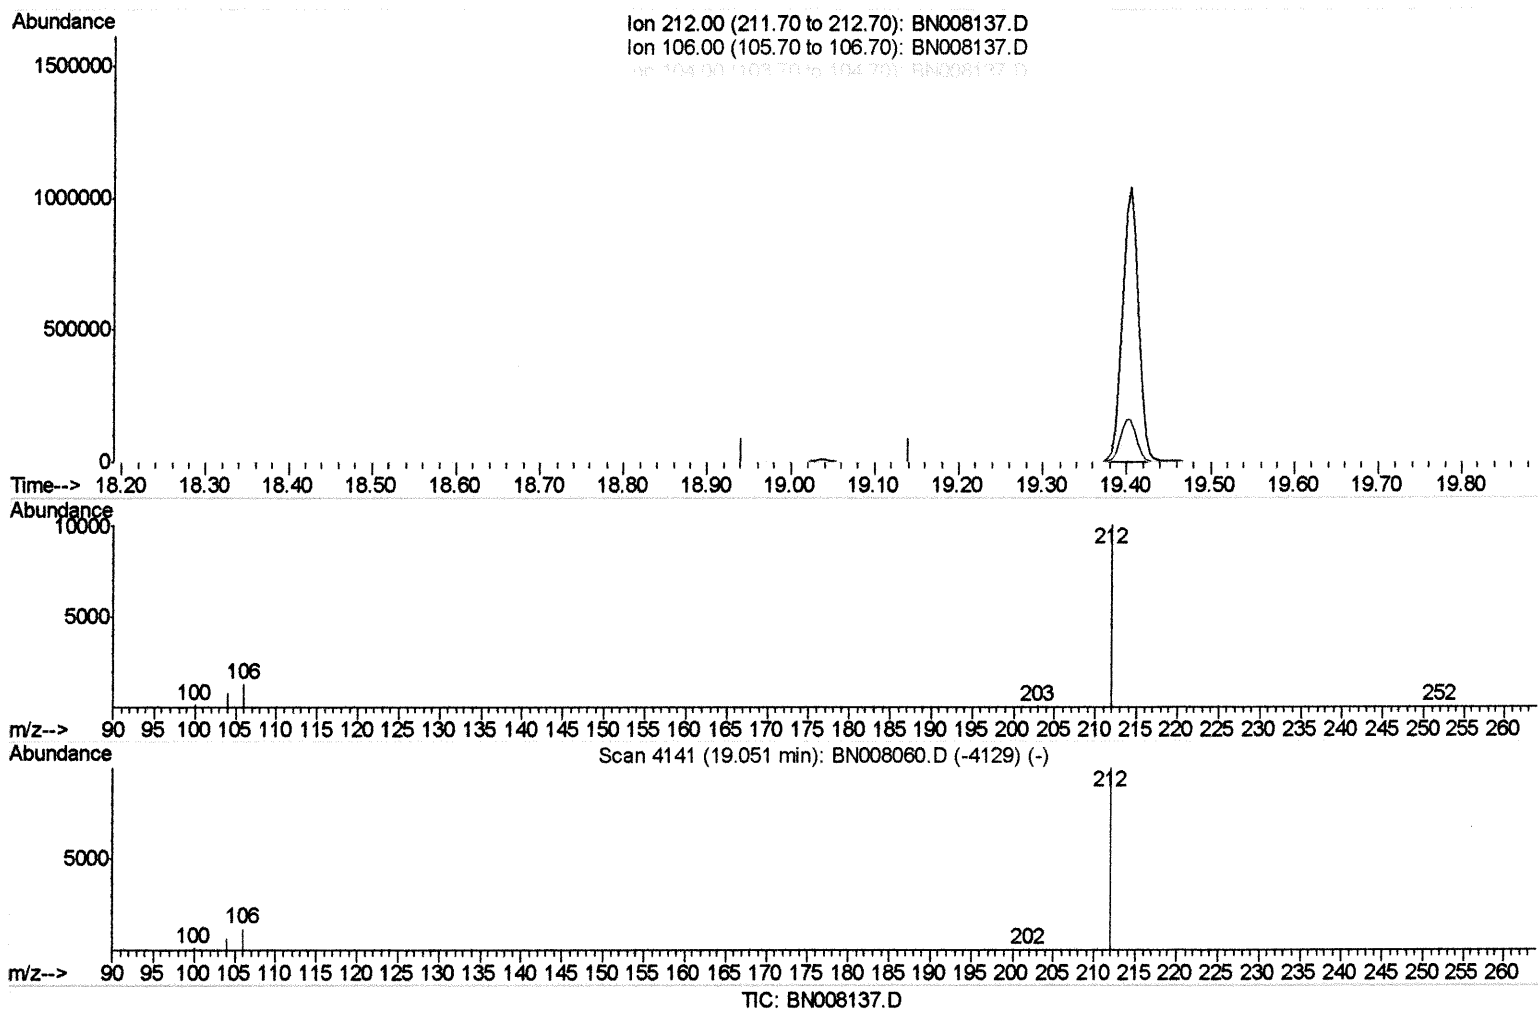

(14) Fluoranthene-d10 (SURR)

19.042min (-19.042) 0.00ng/ui

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	12.70	0.00#
104.00	7.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101419\
Data File : BN008137.D
Acq On : 14 Oct 2019 16:50
Operator : JU
Sample : K5096-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMG9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:29:53 PM

Quant Time: Oct 14 17:40:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

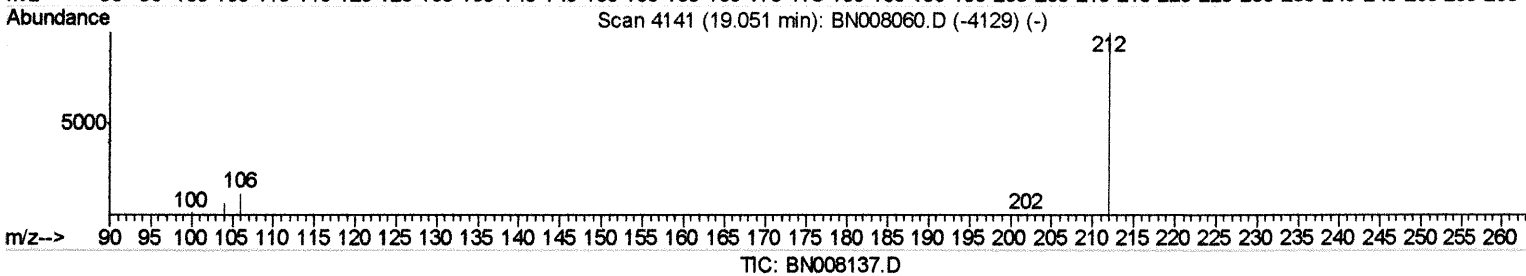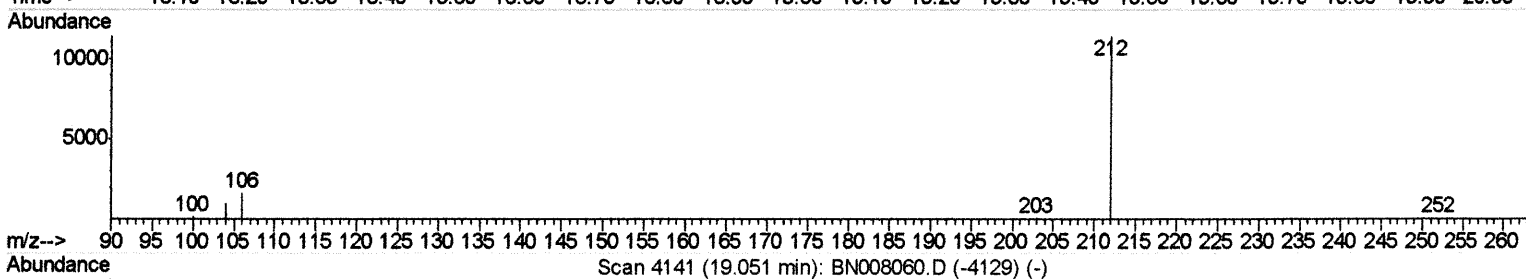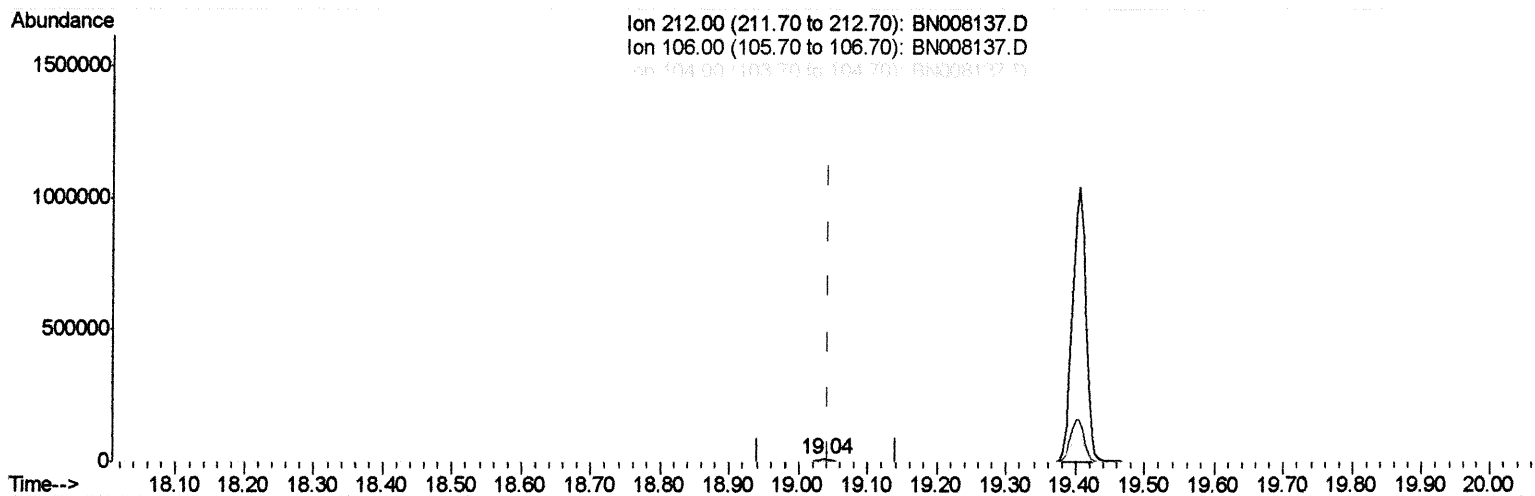

(14) Fluoranthene-d10 (SURR)

19.037min (-0.005) 0.31ng/ul m *JU 10/16/19*

response 15290

Ion	Exp%	Act%
212.00	100	100
106.00	12.70	0.00#
104.00	7.20	0.00#
0.00	0.00	0.00



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101419\
Data File : BN008137.D
Acq On : 14 Oct 2019 16:50
Operator : JU
Sample : K5096-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMG9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:29:53 PM

Quant Time: Oct 14 17:40:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

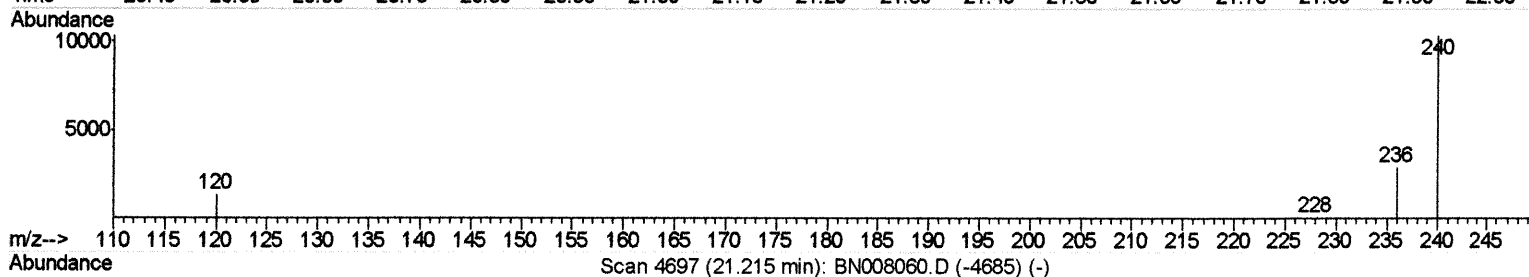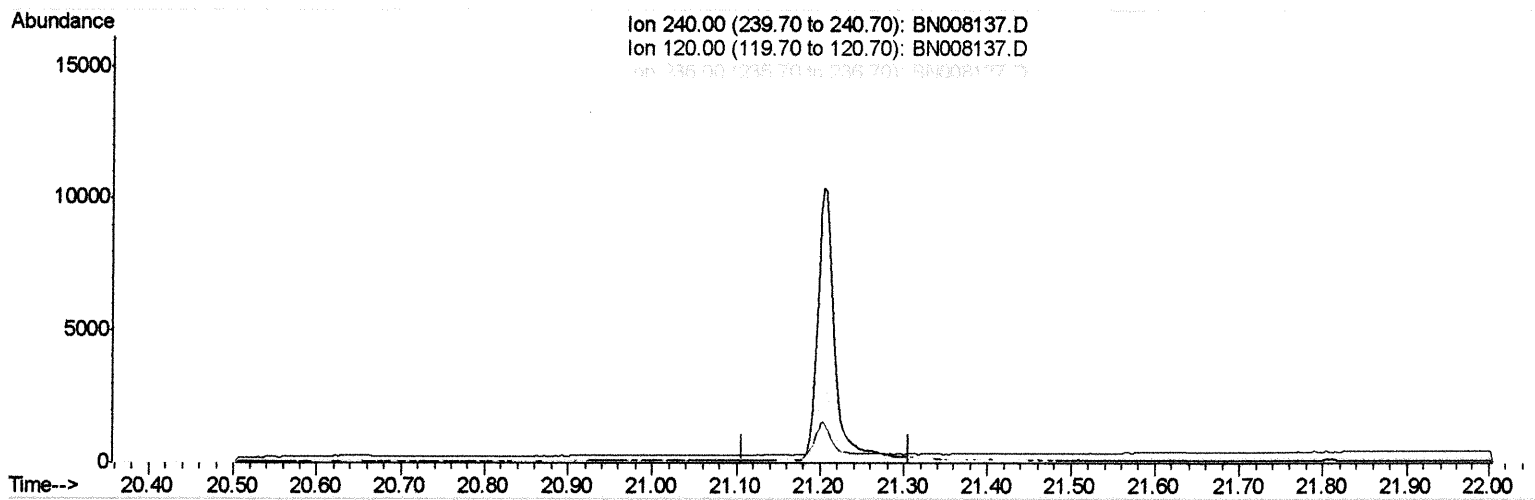

TIC: BN008137.D

(16) Chrysene-d12 (I)

21.207min (-21.207) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.70	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101419\
 Data File : BN008137.D
 Acq On : 14 Oct 2019 16:50
 Operator : JU
 Sample : K5096-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLMG9

Manual Integrations
 APPROVED

mohammad
 10/15/2019 1:29:53 PM

Quant Time: Oct 14 17:40:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:19:29 2019
 Response via : Initial Calibration

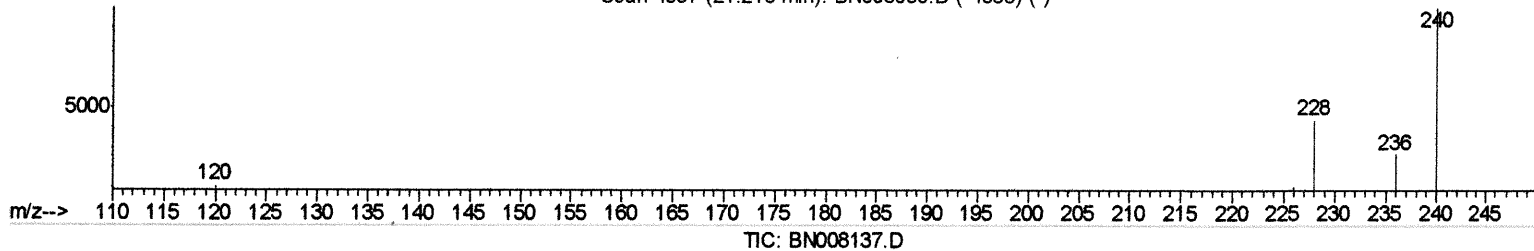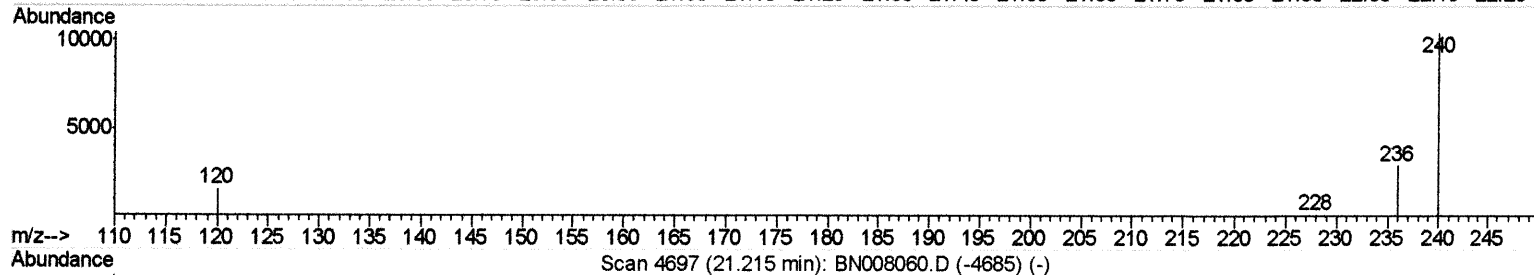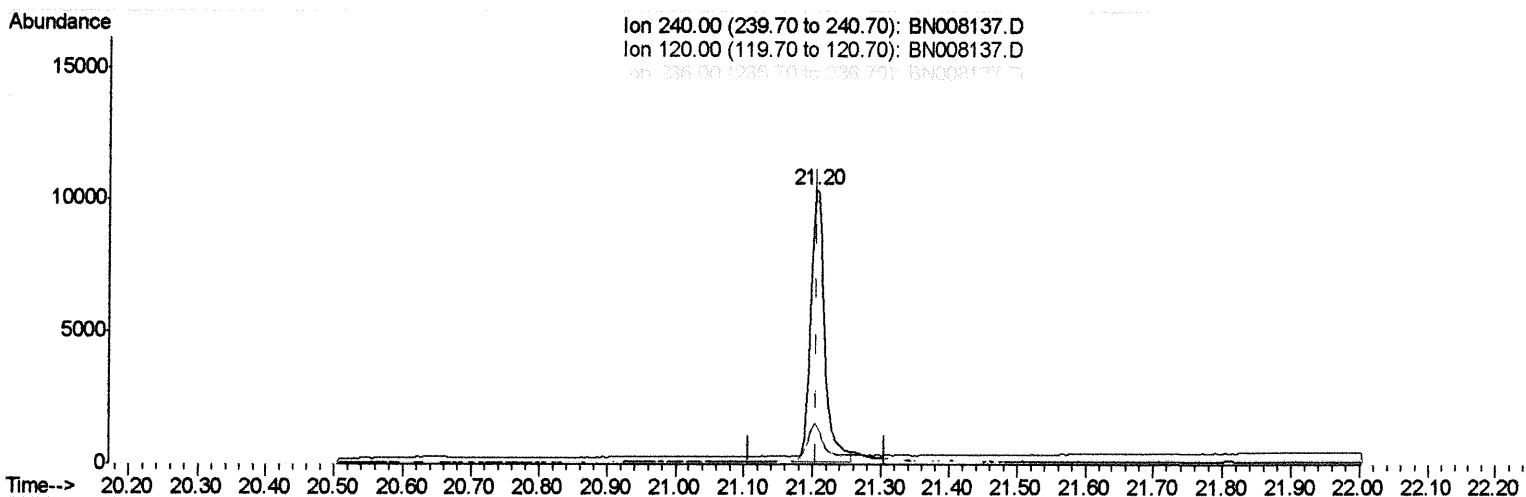

(16) Chrysene-d12 (I)

21.204min (-0.003) 0.40ng/ul m *JU 10/16/19*

response 14563

Ion	Exp%	Act%
240.00	100	100
120.00	14.70	14.99
236.00	28.40	28.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101419\
 Data File : BN008137.D
 Acq On : 14 Oct 2019 16:50
 Operator : JU
 Sample : K5096-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLMG9

Manual Integrations
 APPROVED

mohammad
 10/15/2019 1:29:53 PM

Quant Time: Oct 14 17:42:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:19:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	1899	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	9424	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	6193	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	14434m	0.40	ng/ul	0.00
16) Chrysene-d12	21.20	240	14563m	0.40	ng/ul	0.00
20) Perylene-d12	23.39	264	15790	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.99	152	3822	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.04	212	15290m	0.31	ng/ul	0.00

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed