


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:38:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

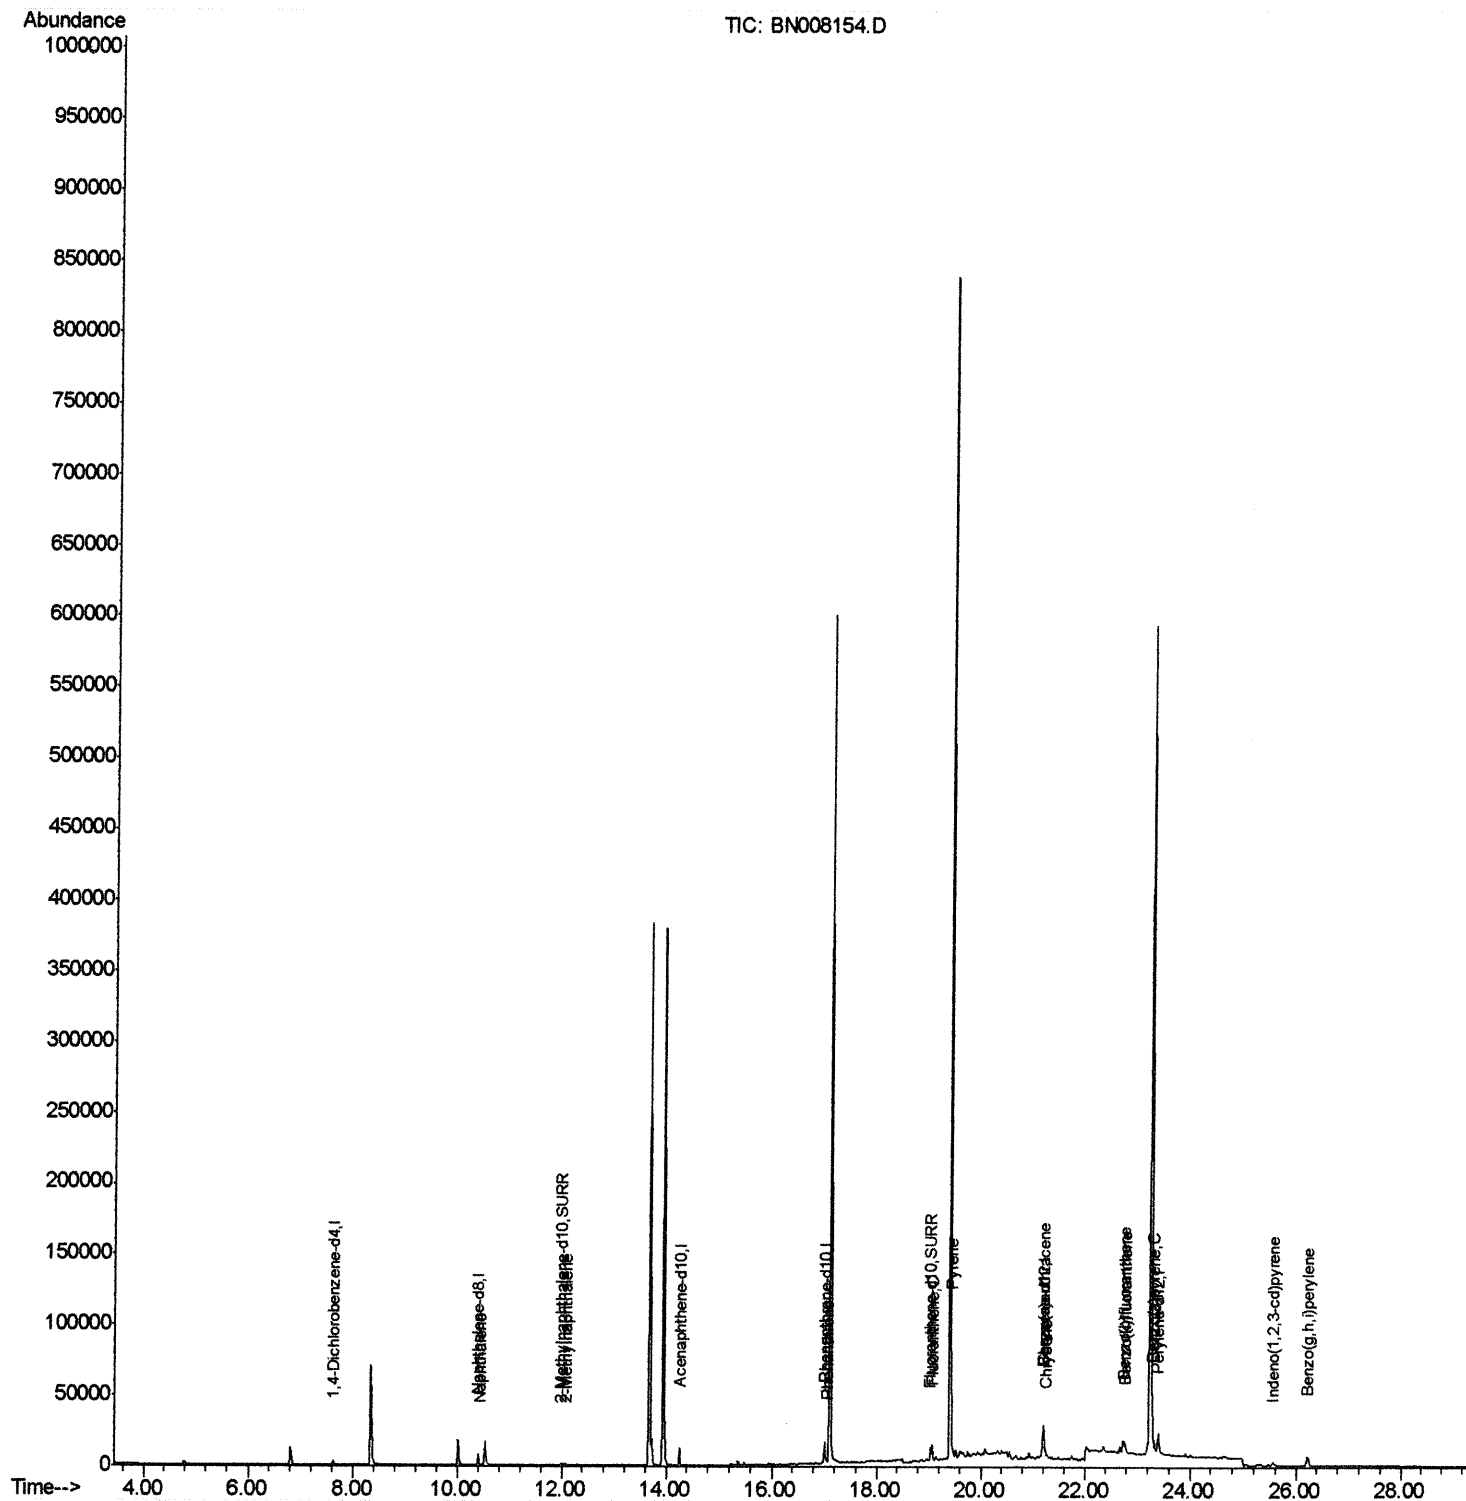




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:28:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

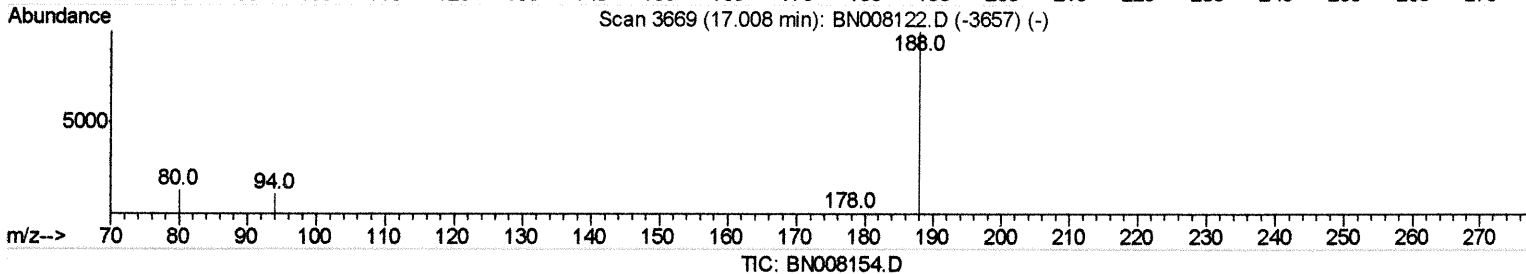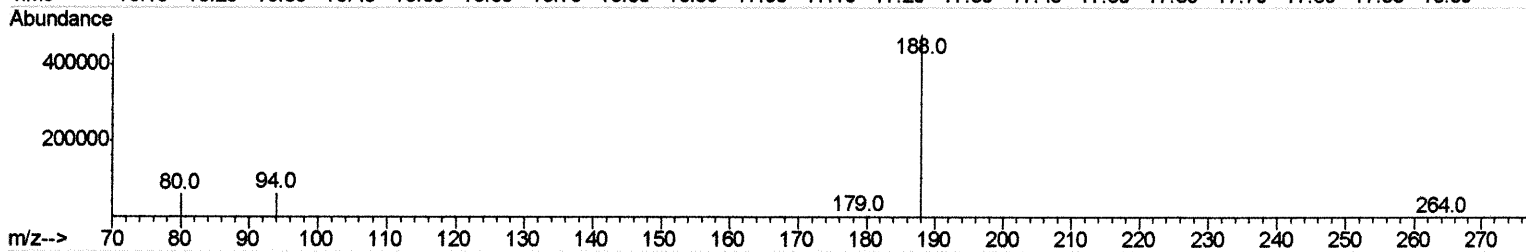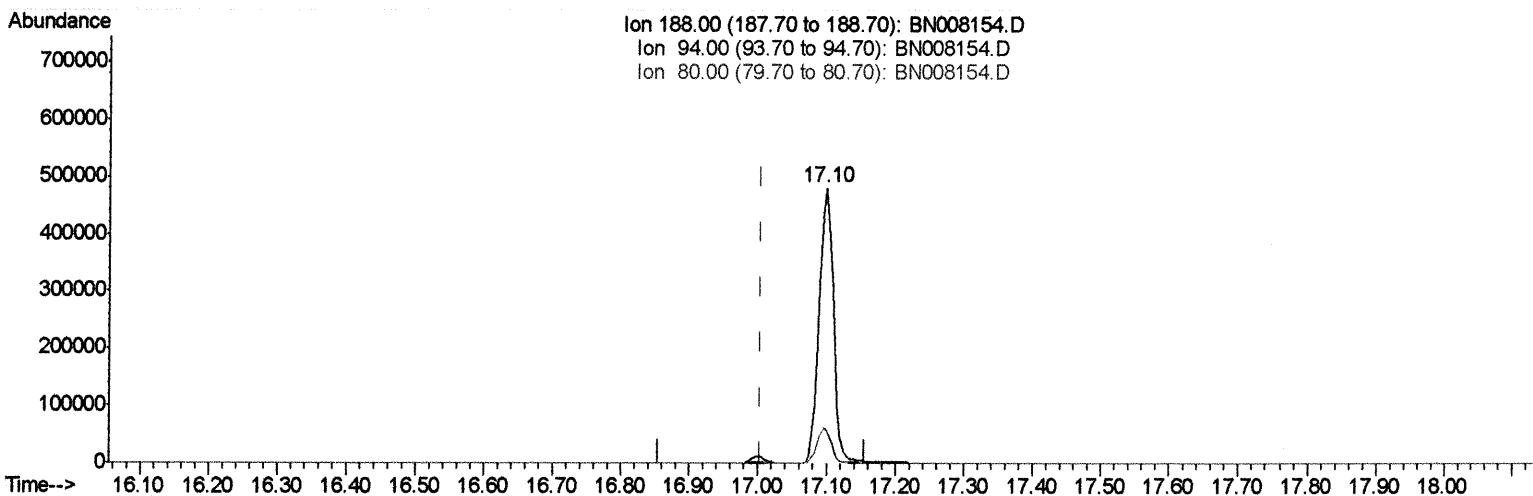

(10) Phenanthrene-d10 (I)

17.097min (+0.093) 0.40ng/ul

response 682594

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	12.56
80.00	12.60	12.30
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:28:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

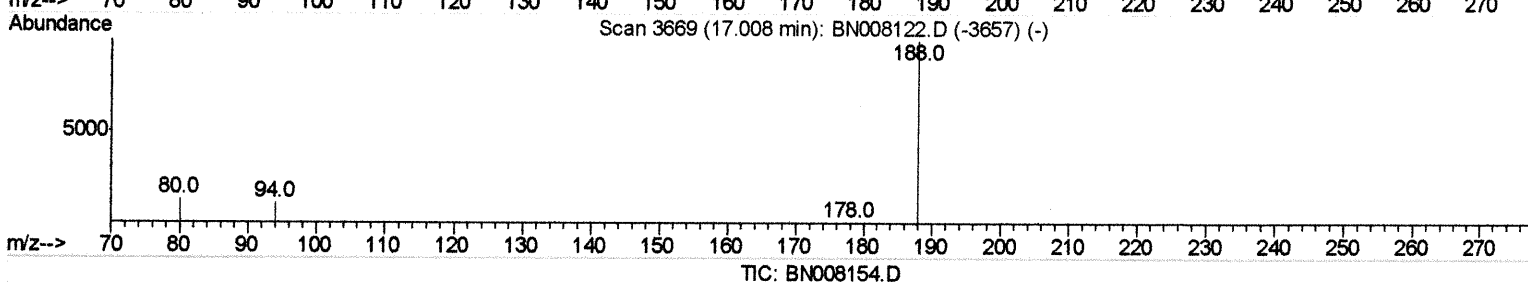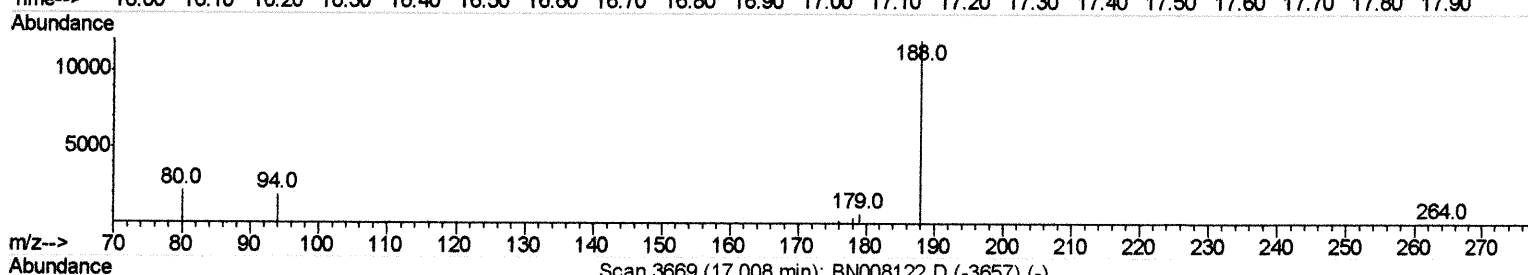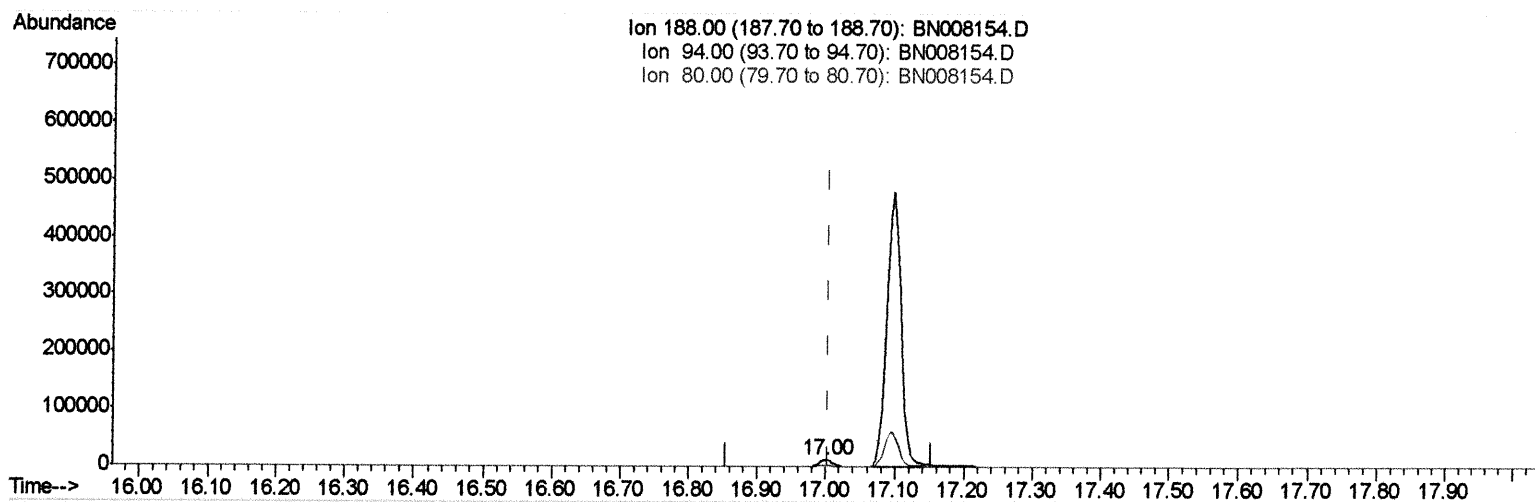

(10) Phenanthrene-d10 (I)

17.000min (-0.004) 0.40ng/ul m *re* 10/16/19

response 16747

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	15.58#
80.00	12.60	17.86#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:34:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

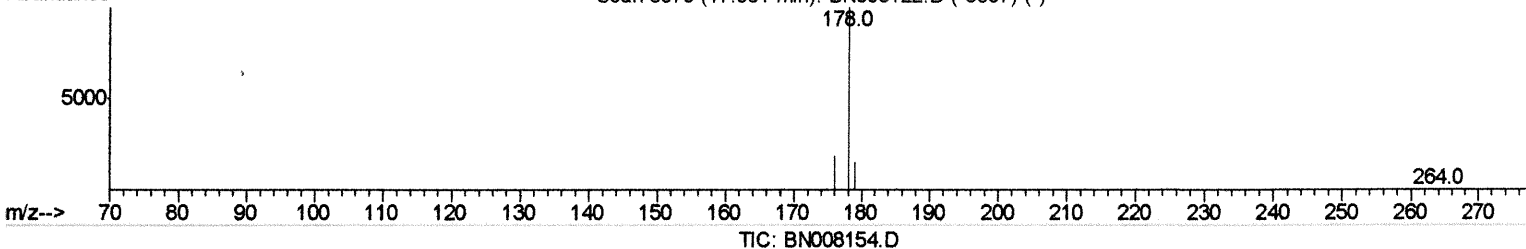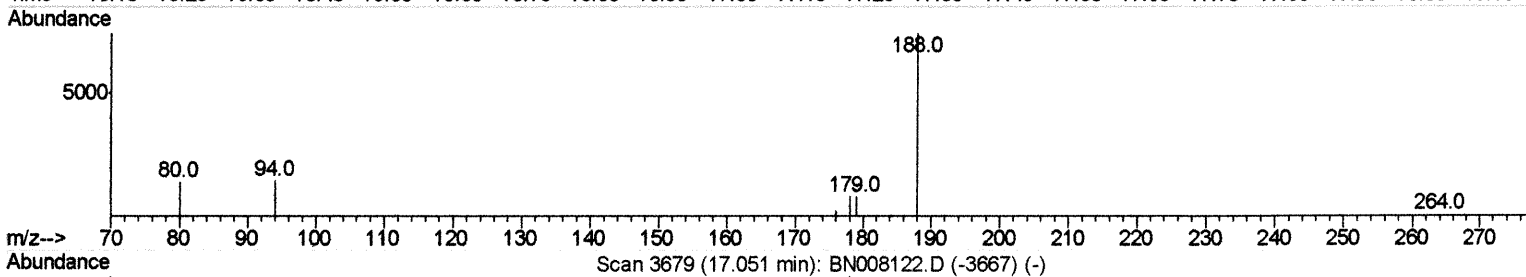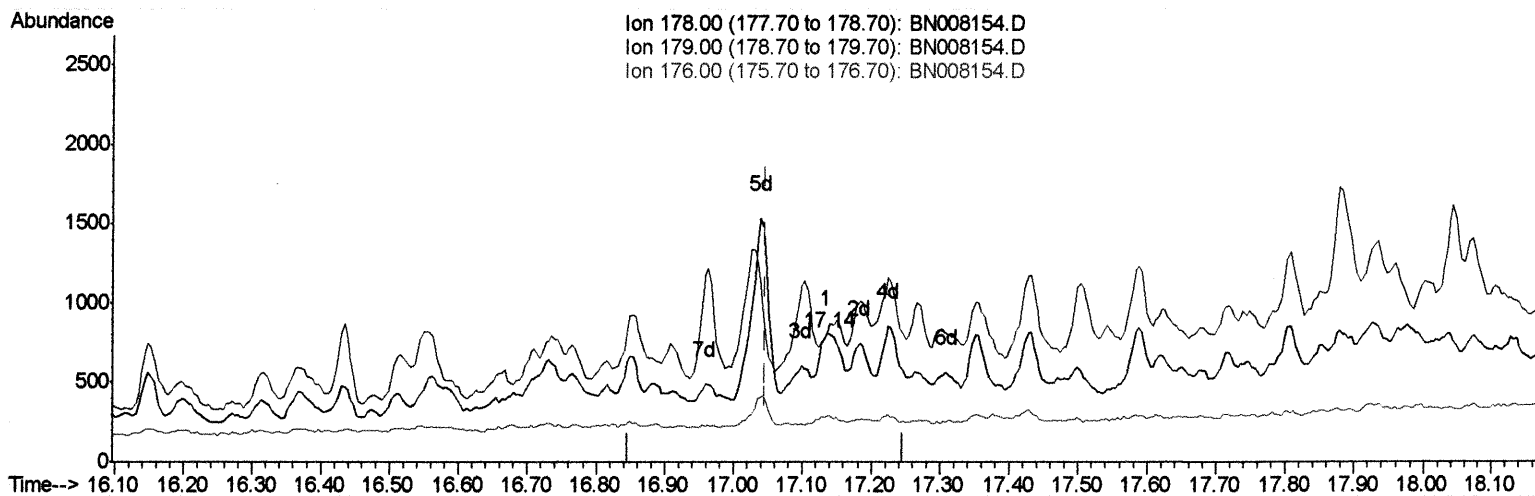

(12) Phenanthrene

17.135min (+0.089) 0.01ng/ul

response 646

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	100.99#
176.00	19.30	36.08#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:34:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

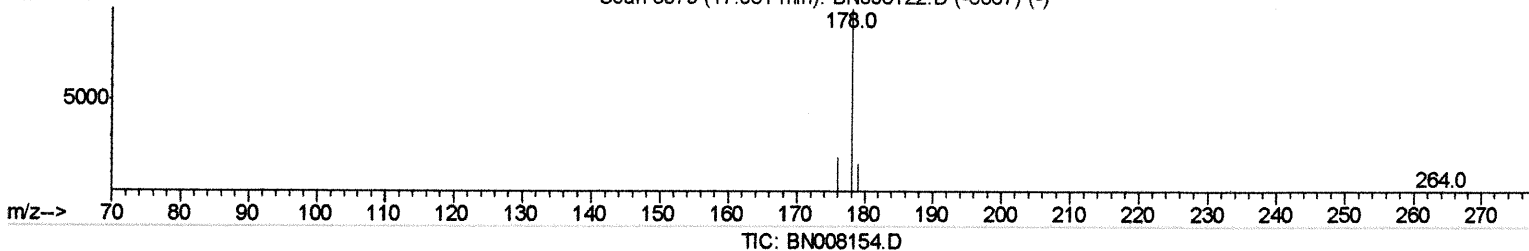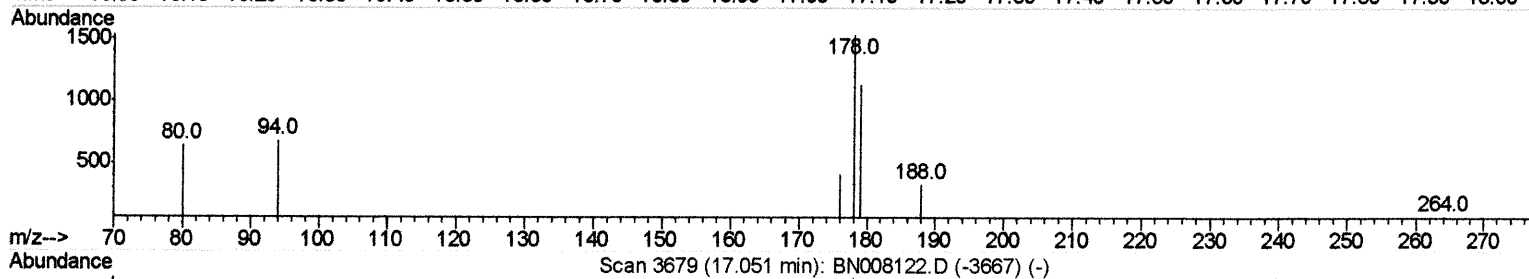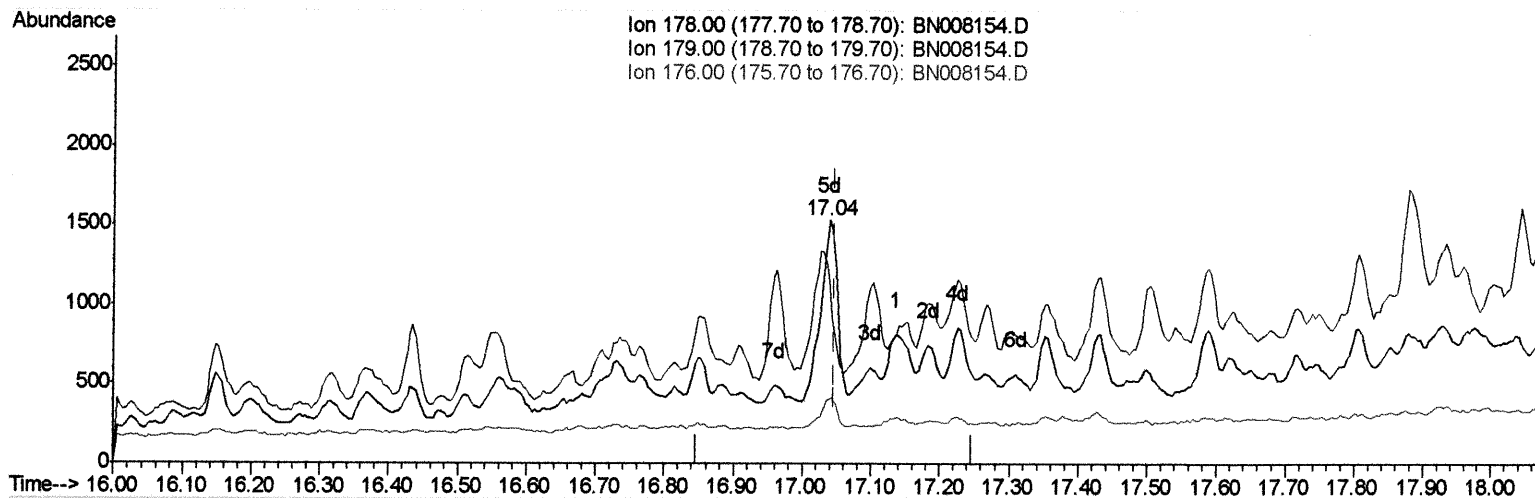

(12) Phenanthrene

17.038min (-0.008) 0.04ng/ul m *De 10/16/19*

response 1912

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	73.86#
176.00	19.30	26.80#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\

Data File : BN008154.D

Acq On : 15 Oct 2019 03:34

Operator : JU

Sample : K5097-05

Misc :

ALS Vial : 22 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

JLMD9

Manual Integrations
APPROVEDmohammad
10/15/2019 1:30:38 PM




Quant Time: Oct 15 04:34:28 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Oct 14 17:19:29 2019

Response via : Initial Calibration

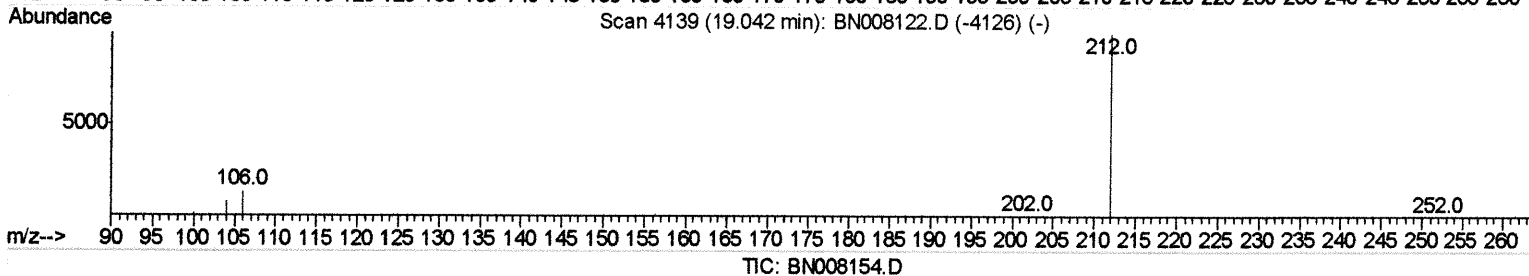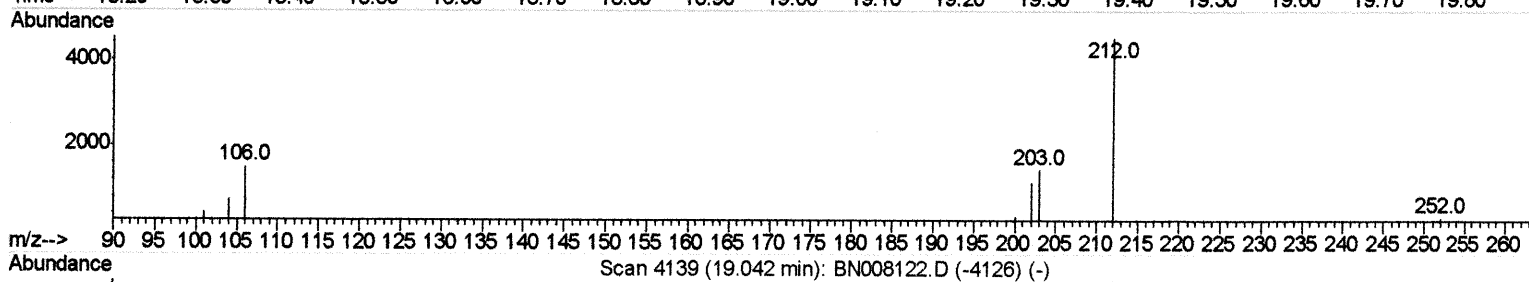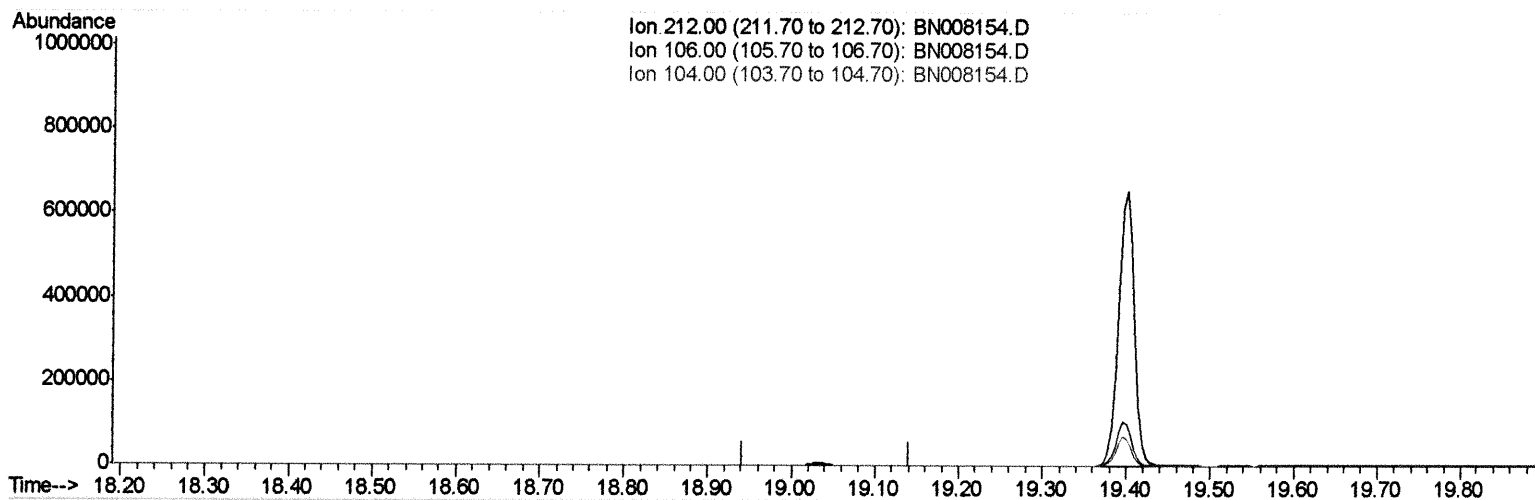

(14) Fluoranthene-d10 (SURR)

19.042min (-19.042) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	12.70	0.00#
104.00	7.20	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:34:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

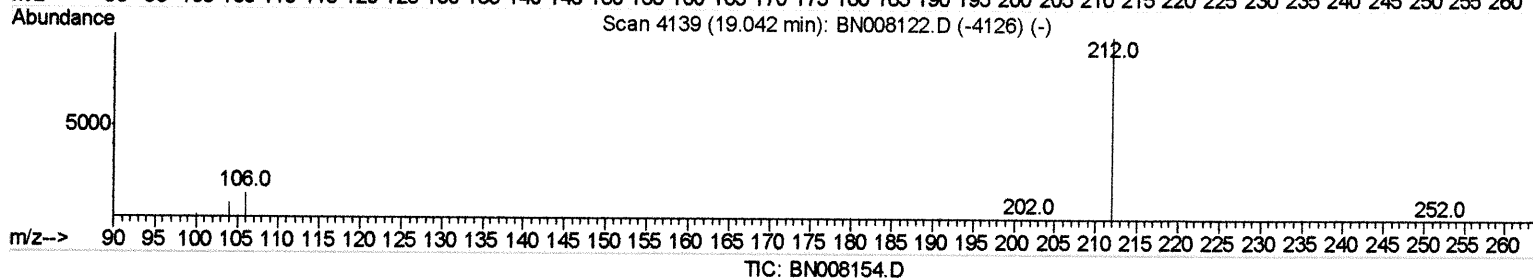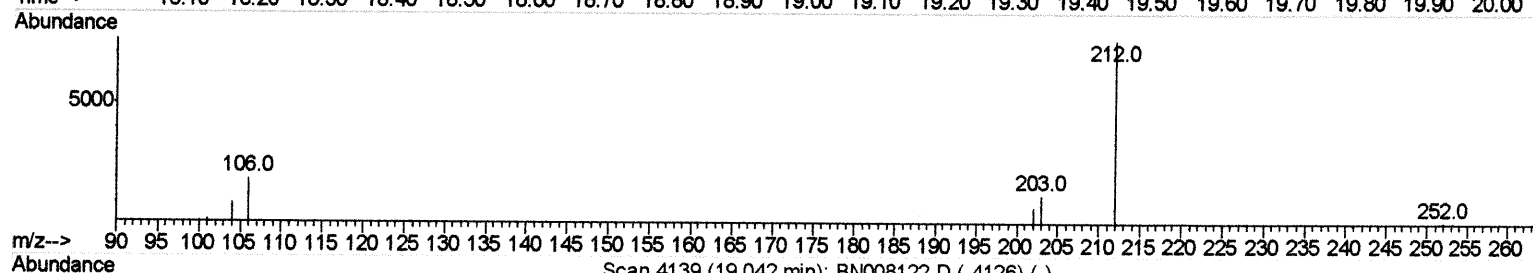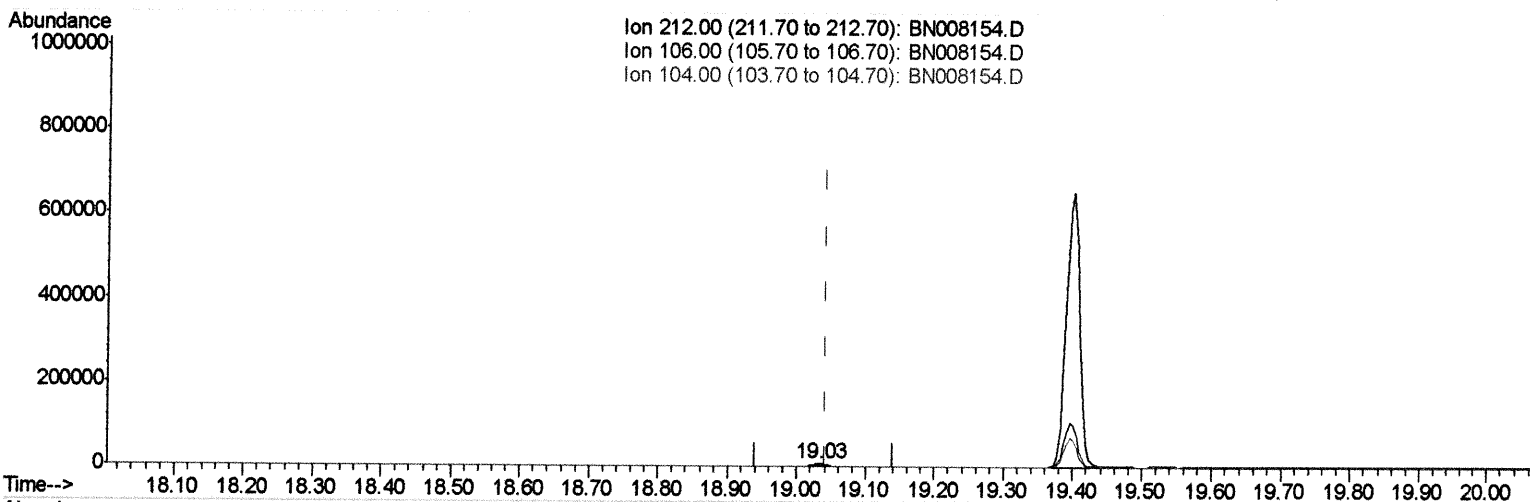

(14) Fluoranthene-d10 (SURR)

19.033min (-0.009) 0.16ng/ul m

JU 10/16/19

response 9510

Ion	Exp%	Act%
212.00	100	100
106.00	12.70	0.00#
104.00	7.20	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:34:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

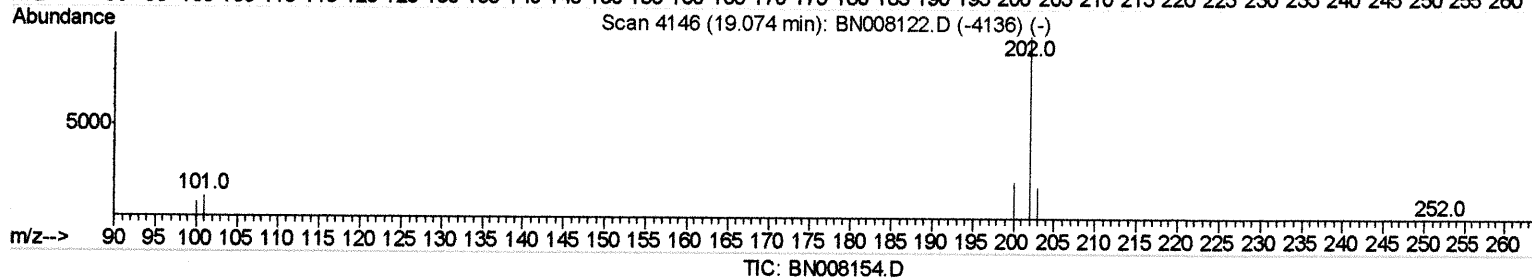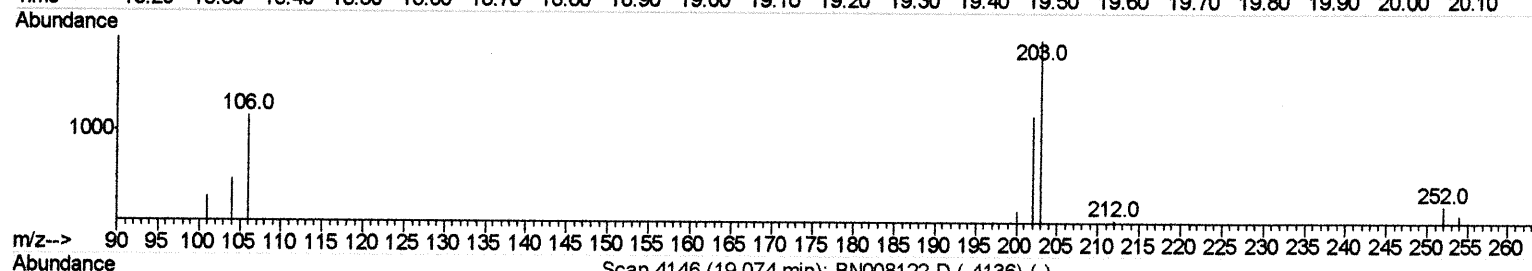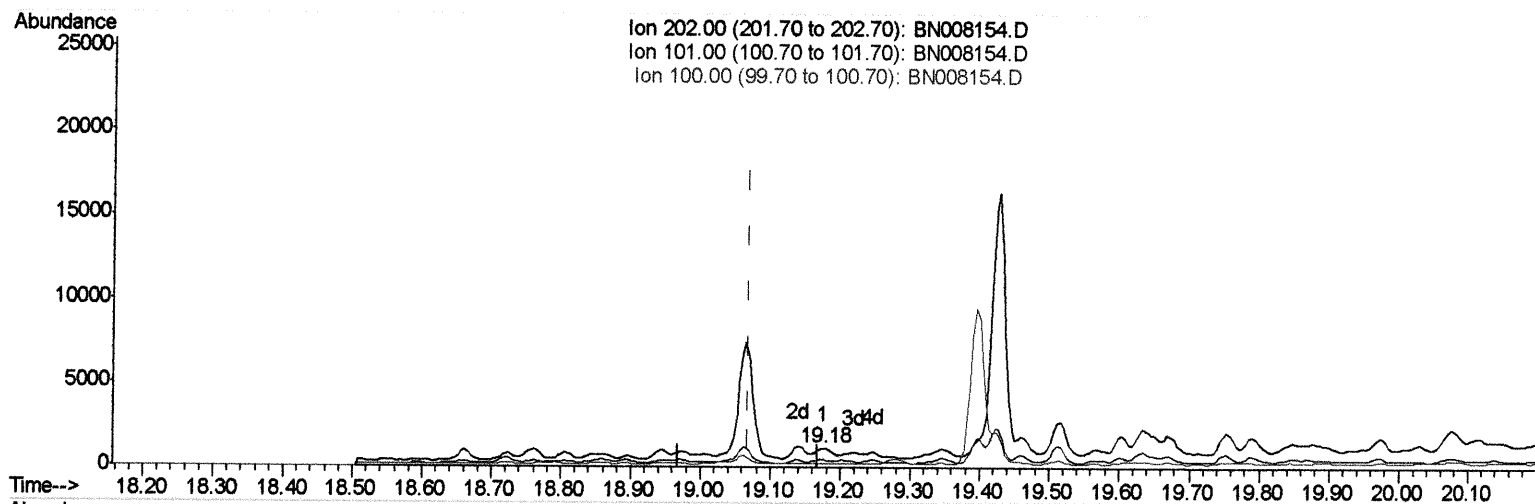

(15) Fluoranthene (C)

19.177min (+0.107) 0.01ng/ul

response 772

Ion	Exp%	Act%
202.00	100	100
101.00	11.20	38.21#
100.00	8.50	19.98
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\

Data File : BN008154.D

Acq On : 15 Oct 2019 03:34

Operator : JU

Sample : K5097-05

Misc :

ALS Vial : 22 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

JLMD9

Manual Integrations
APPROVEDmohammad
10/15/2019 1:30:38 PM



Quant Time: Oct 15 04:34:28 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Oct 14 17:19:29 2019

Response via : Initial Calibration

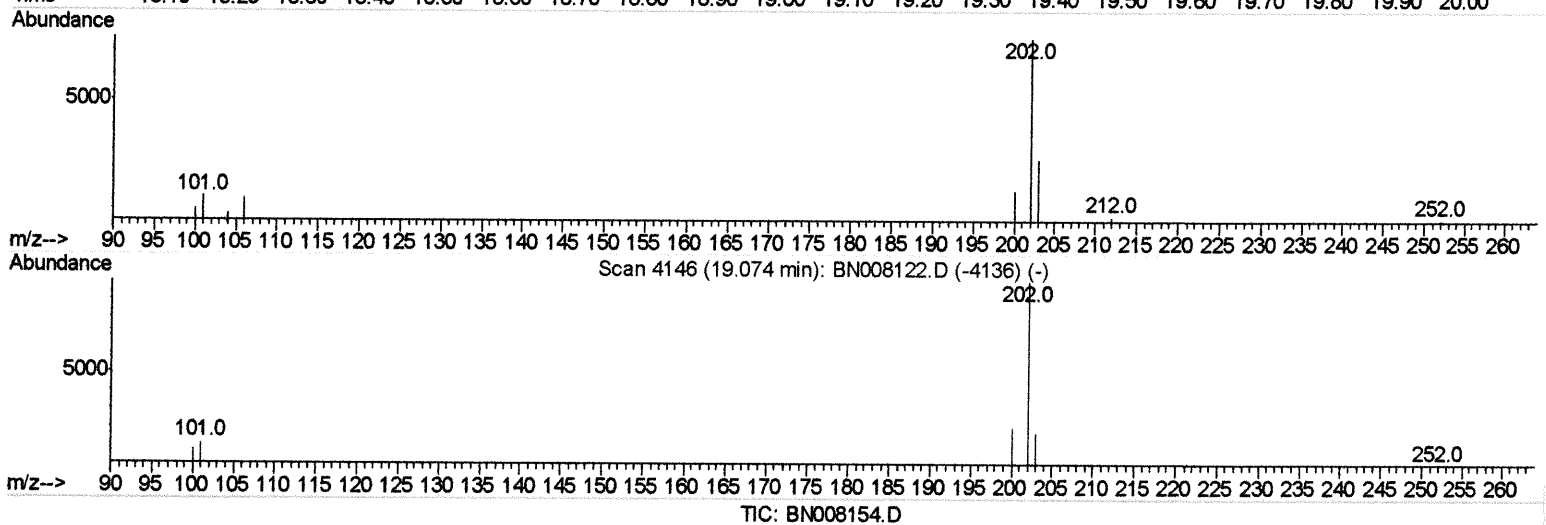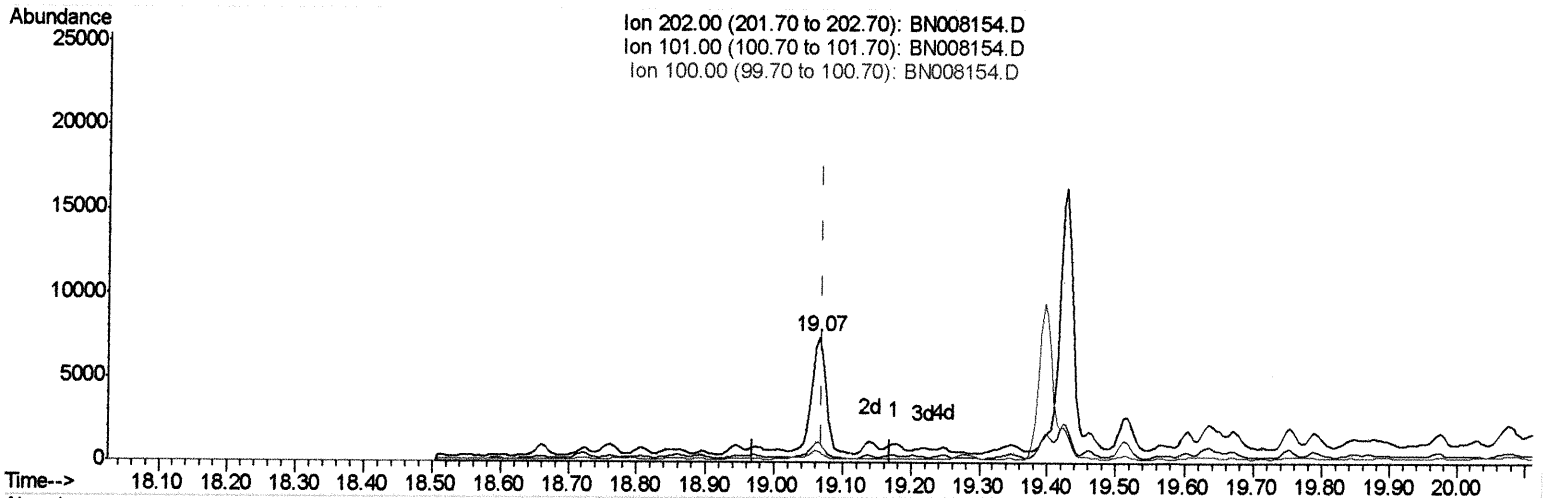

(15) Fluoranthene (C)

19.065min (-0.005) 0.16ng/ul m *Ju 10/16/19*

response 10230

Ion	Exp%	Act%
202.00	100	100
101.00	11.20	15.85
100.00	8.50	9.26
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:34:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

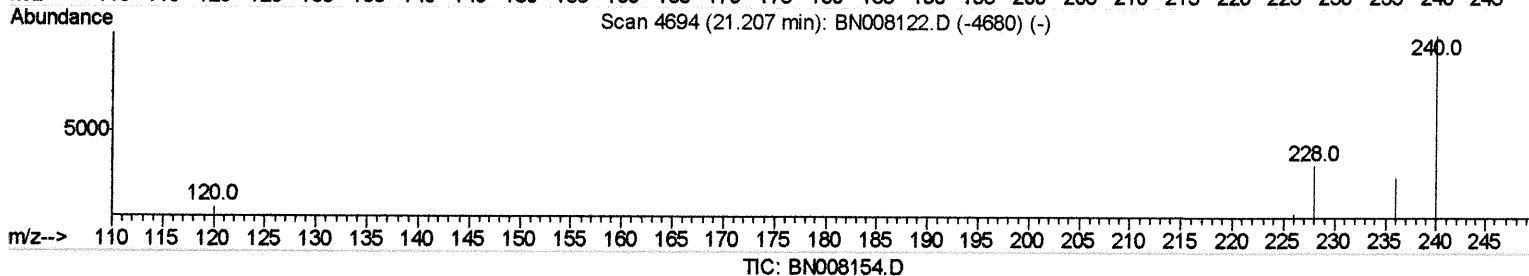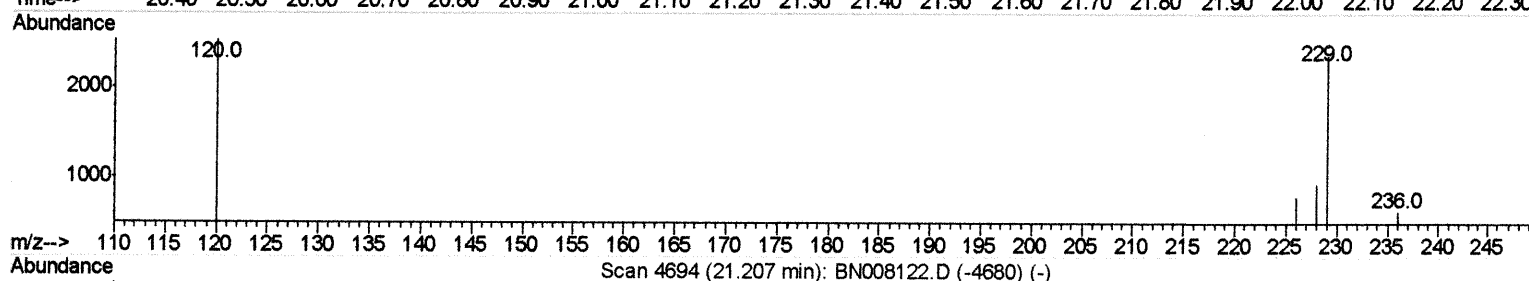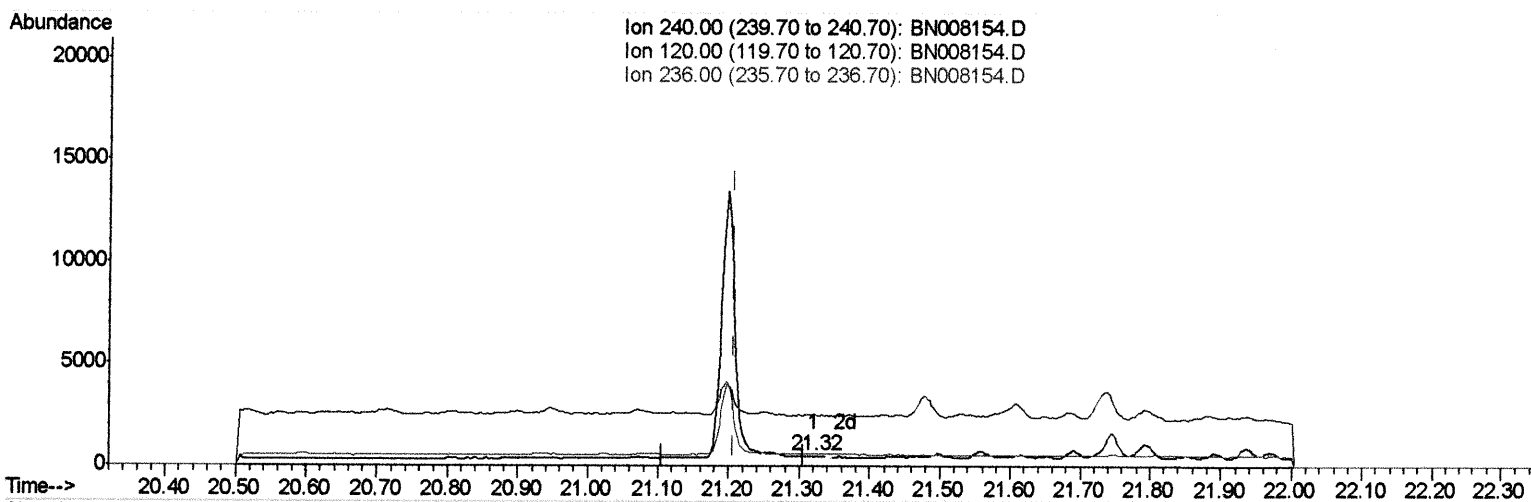

(16) Chrysene-d12 (I)

21.321min (+0.114) 0.40ng/ul

response 56

Ion	Exp%	Act%
240.00	100	100
120.00	14.70	503.78#
236.00	28.40	123.90#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\

Data File : BN008154.D

Acq On : 15 Oct 2019 03:34

Operator : JU

Sample : K5097-05

Misc :

ALS Vial : 22 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

JLMD9

Manual Integrations
APPROVEDmohammad
10/15/2019 1:30:38 PM




Quant Time: Oct 15 04:34:28 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Oct 14 17:19:29 2019

Response via : Initial Calibration

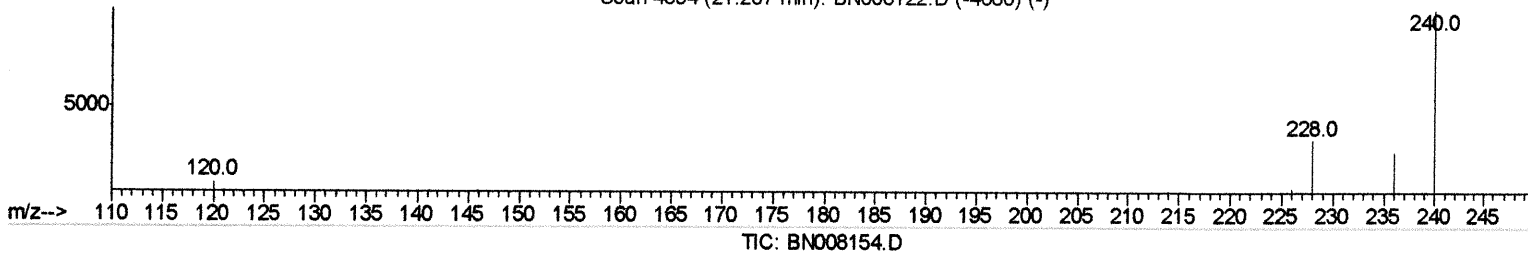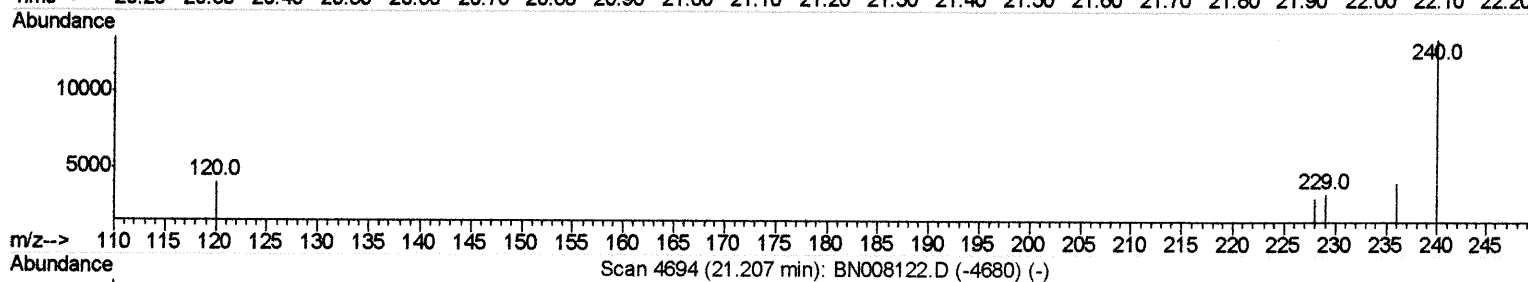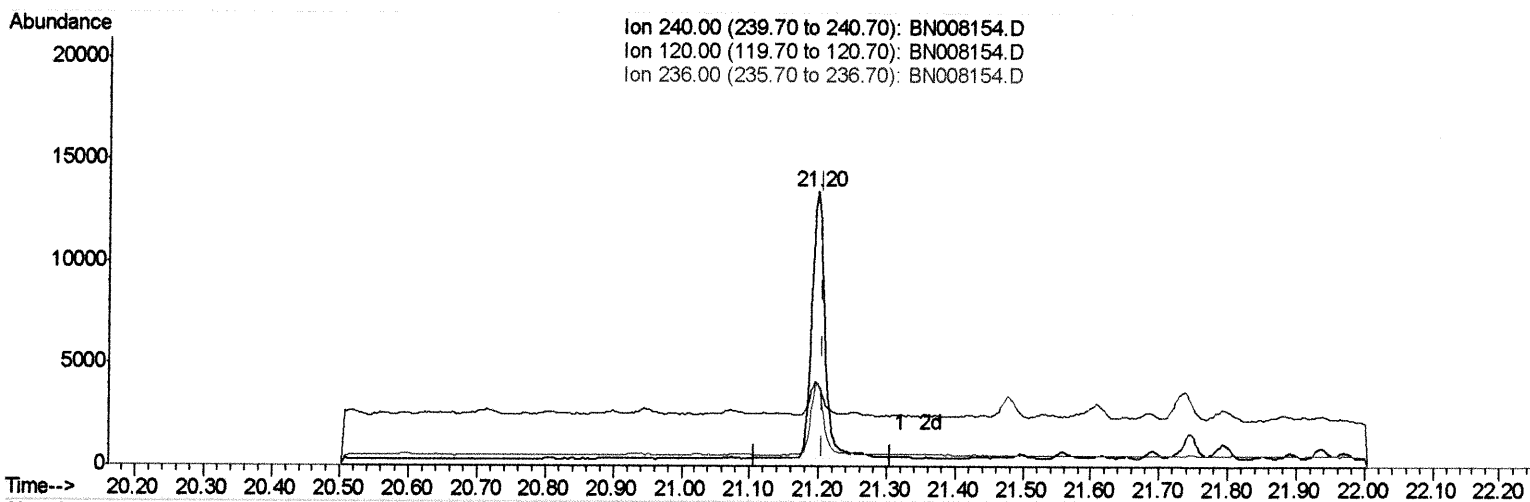

(16) Chrysene-d12 (I)

21.198min (-0.009) 0.40ng/ul m JU 10/16/19

response 17060

Ion	Exp%	Act%
240.00	100	100
120.00	14.70	30.15#
236.00	28.40	30.31
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\

Data File : BN008154.D

Acq On : 15 Oct 2019 03:34

Operator : JU

Sample : K5097-05

Misc :

ALS Vial : 22 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

JLMD9

Manual Integrations
APPROVEDmohammad
10/15/2019 1:30:38 PM




Quant Time: Oct 15 04:36:21 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Oct 14 17:19:29 2019

Response via : Initial Calibration

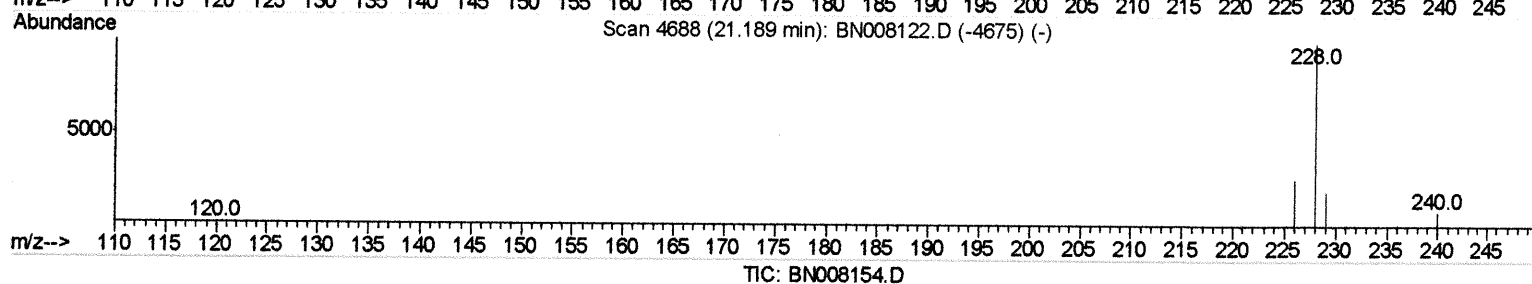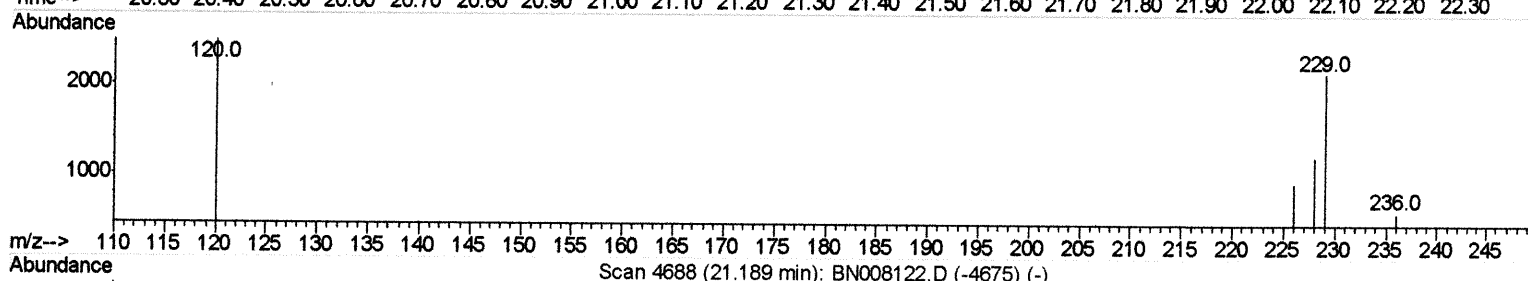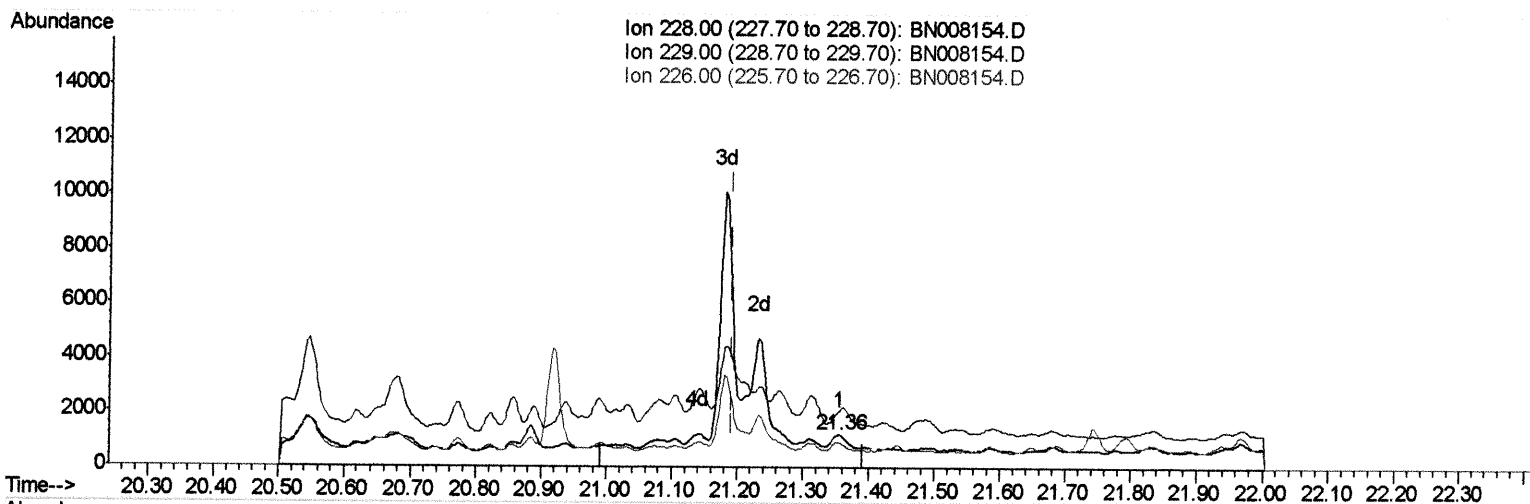

(18) Benzo(a)anthracene

21.356min (+0.164) 0.01ng/ul

response 853

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	175.41#
226.00	26.70	75.16#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\

Data File : BN008154.D

Acq On : 15 Oct 2019 03:34

Operator : JU

Sample : K5097-05

Misc :

ALS Vial : 22 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

JLMD9

Manual Integrations
APPROVEDmohammad
10/15/2019 1:30:38 PM




Quant Time: Oct 15 04:36:21 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Oct 14 17:19:29 2019

Response via : Initial Calibration

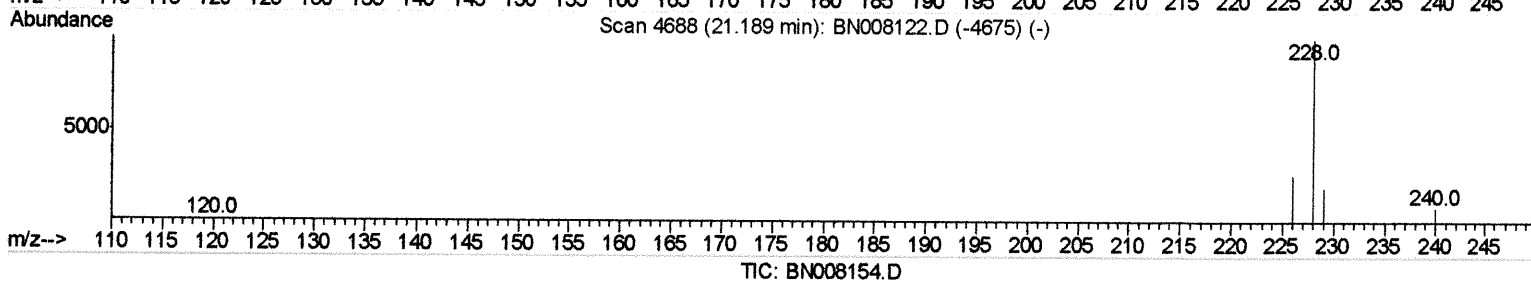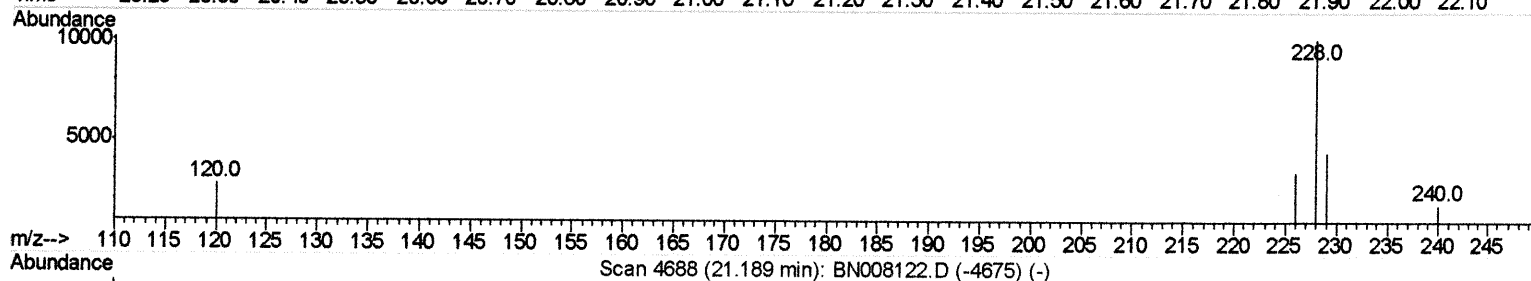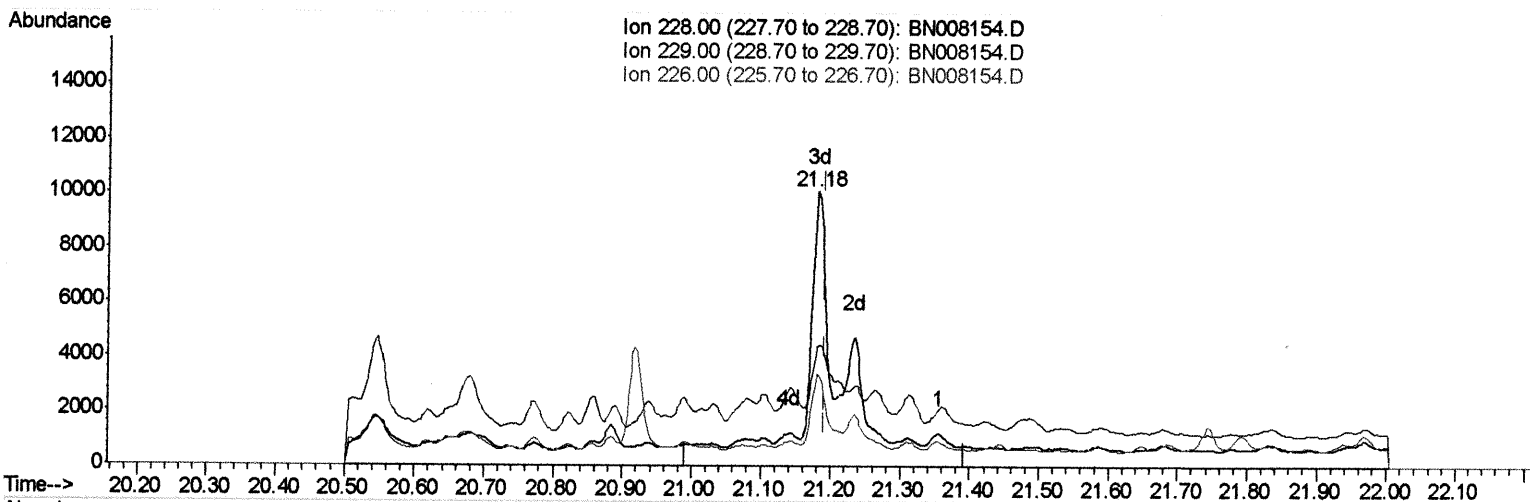

(18) Benzo(a)anthracene

21.180min (-0.012) 0.21ng/ul m *ju 10/16/19*

response 12793

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	43.50#
226.00	26.70	33.50#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:36:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

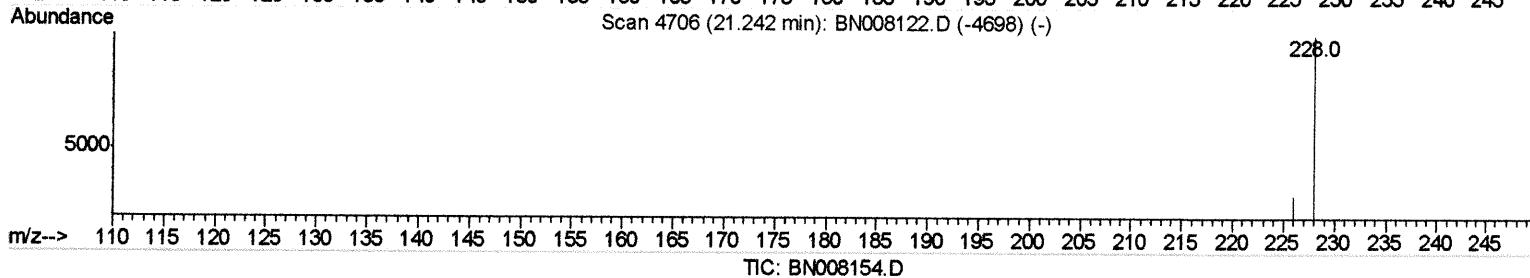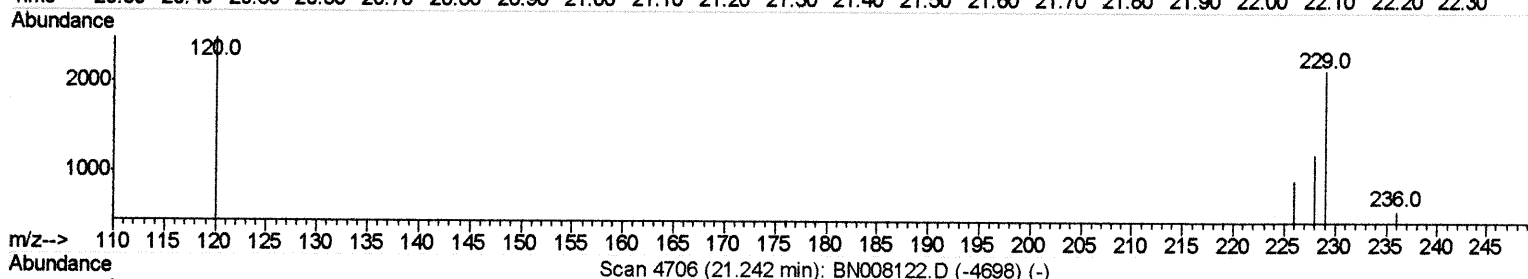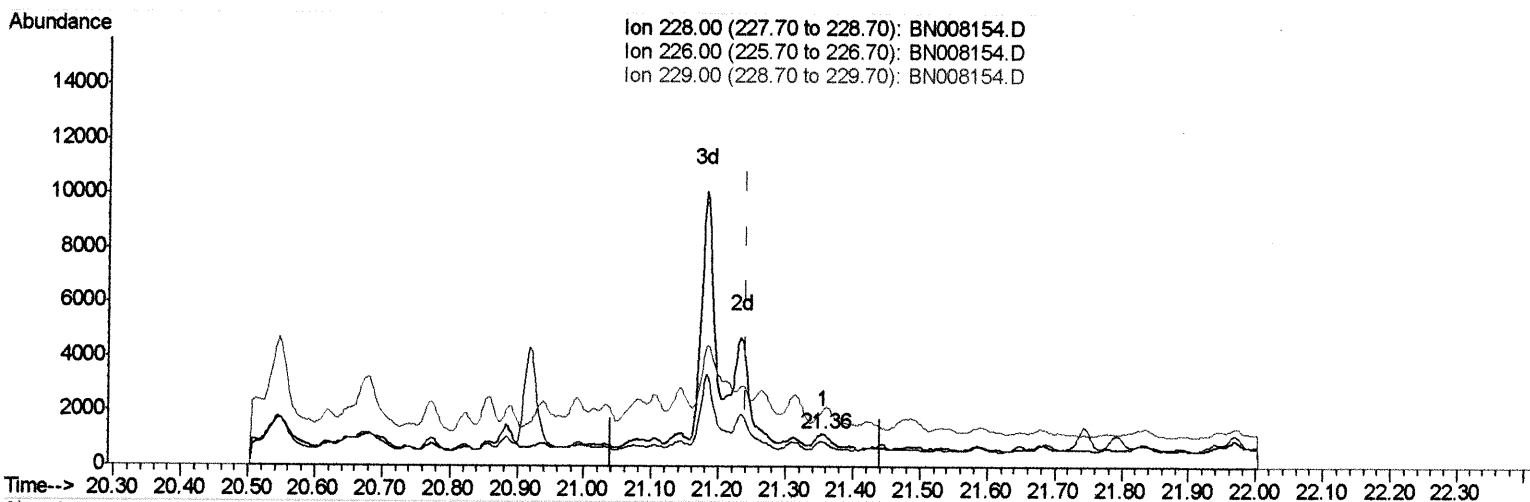

(19) Chrysene

21.356min (+0.114) 0.01ng/ul

response 853

Ion	Exp%	Act%
228.00	100	100
226.00	30.10	75.16#
229.00	20.20	175.41#
0.00	0.00	0.00



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
 Data File : BN008154.D
 Acq On : 15 Oct 2019 03:34
 Operator : JU
 Sample : K5097-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLMD9

Manual Integrations
 APPROVED

mohammad
 10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:36:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:19:29 2019
 Response via : Initial Calibration

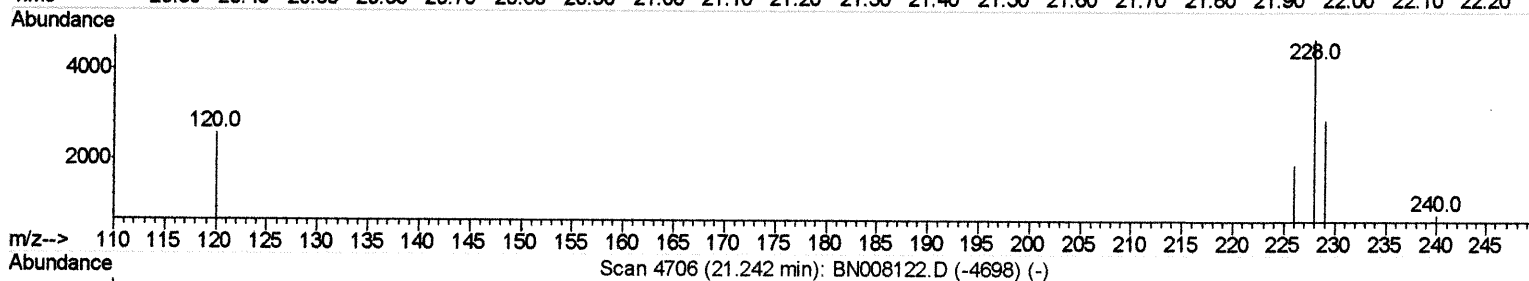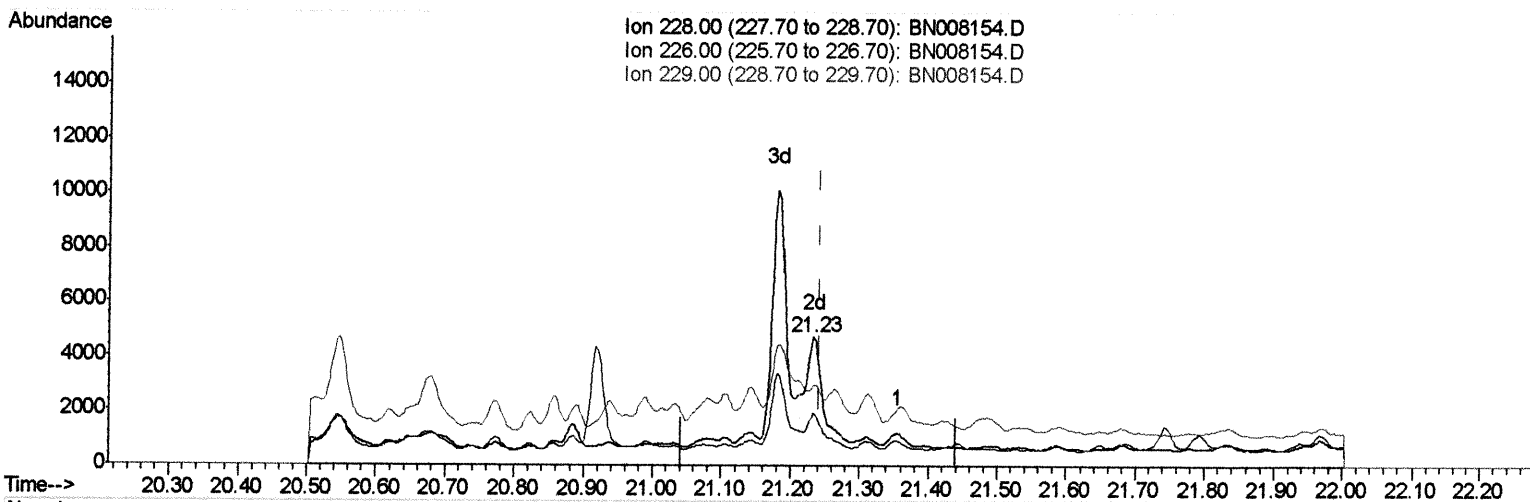

TIC: BN008154.D

(19) Chrysene

21.233min (-0.009) 0.07ng/ul m *PL 10/16/19*

response 5579

Ion	Exp%	Act%
228.00	100	100
226.00	30.10	40.67#
229.00	20.20	62.04#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:36:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

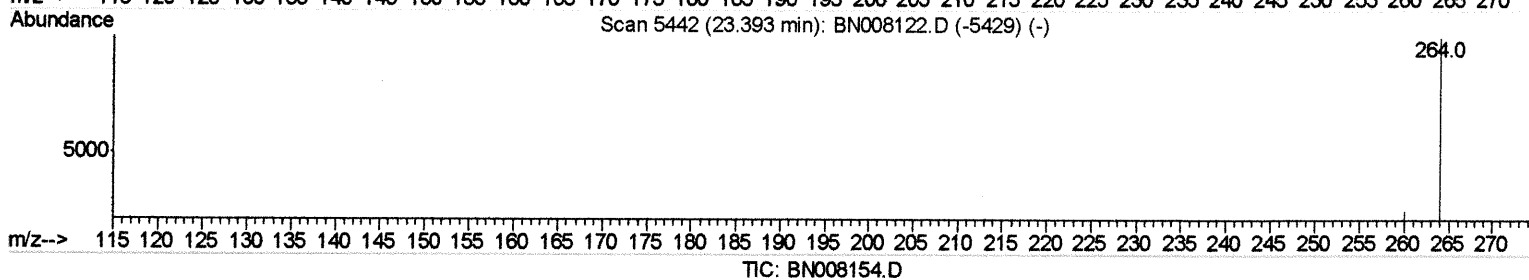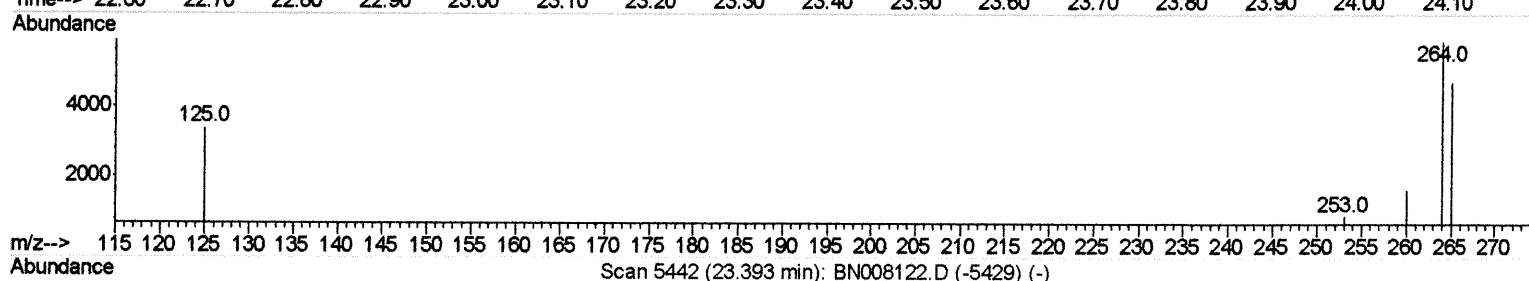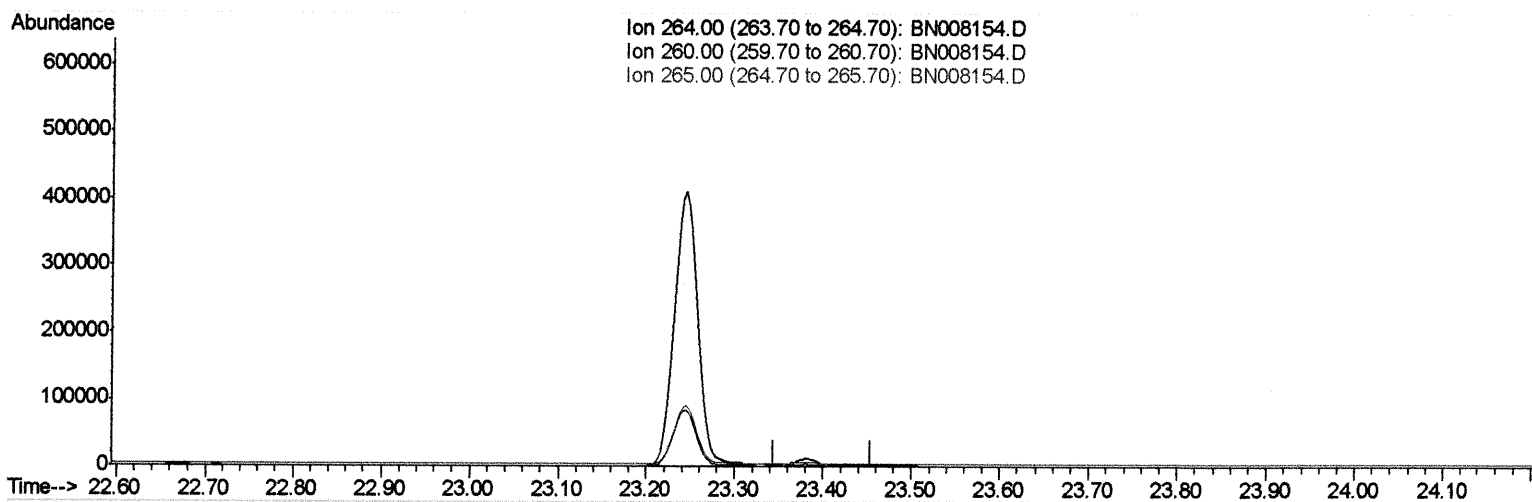

(20) Perylene-d12 (I)

23.396min (-23.396) 0.00ng/ui

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	25.60	0.00#
265.00	74.00	0.00#
0.00	0.00	0.00



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:36:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

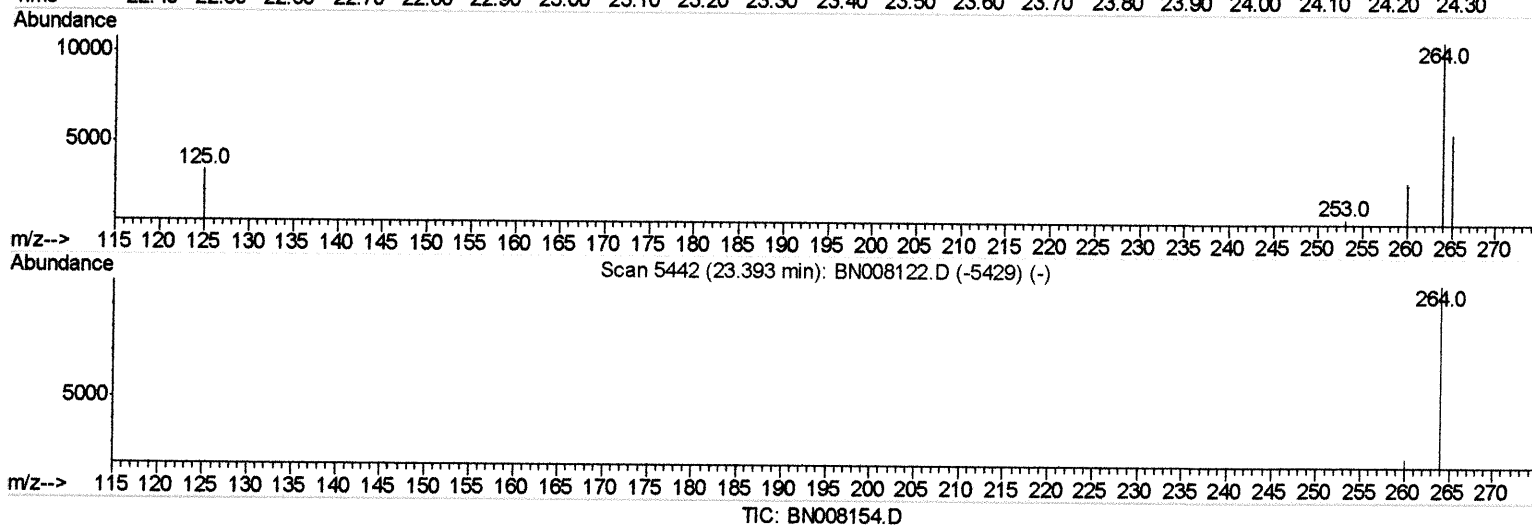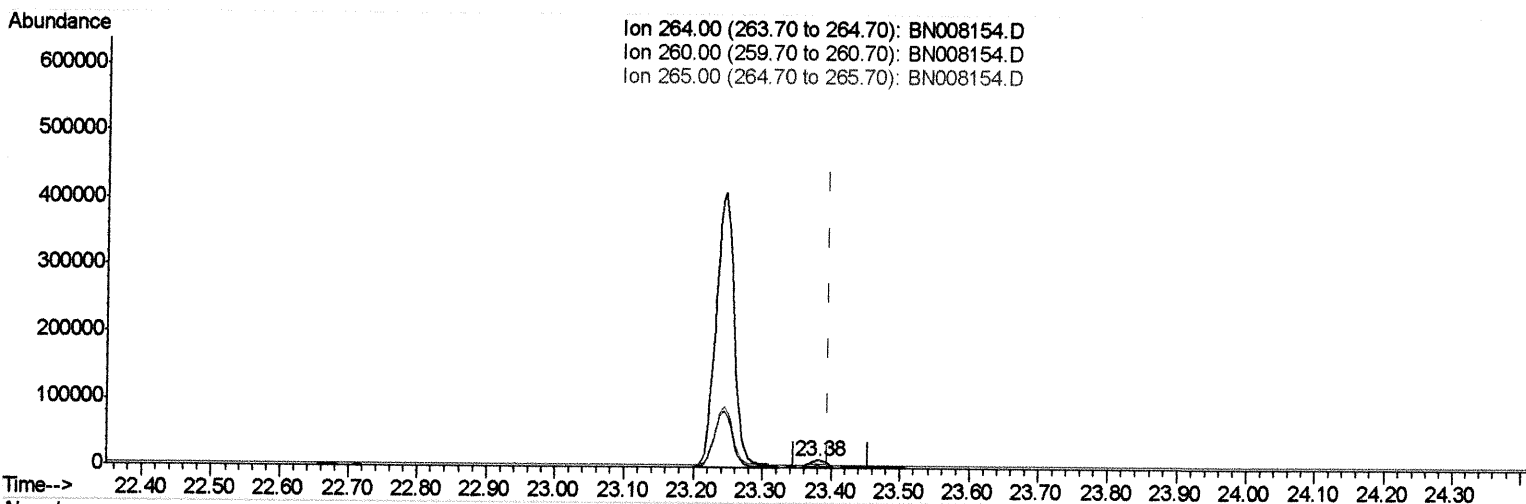

(20) Perylene-d12 (I)

23.381min (-0.015) 0.40ng/ul m *24 10/16/19*

response 14581

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	27.19
265.00	74.00	52.68#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:37:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

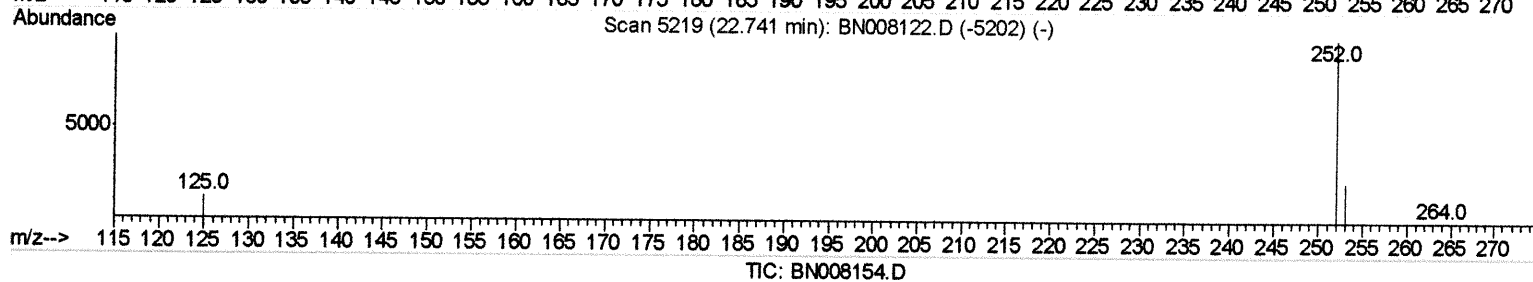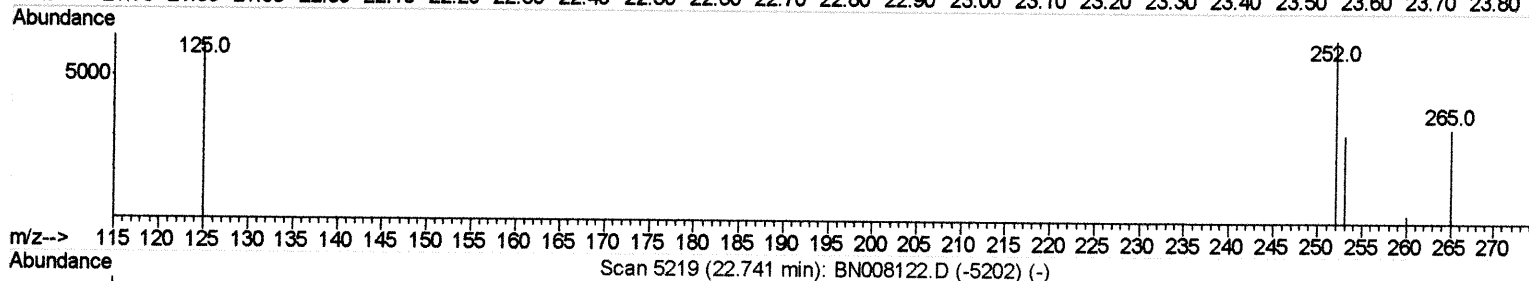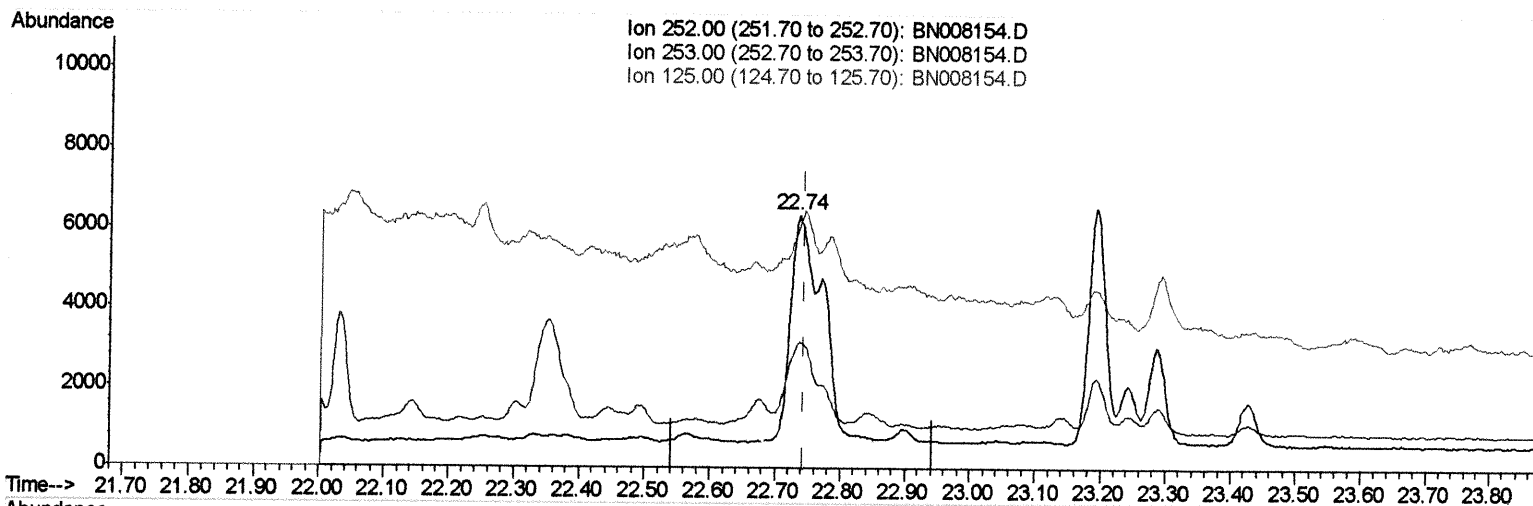

(21) Benzo(b)fluoranthene

22.735min (-0.009) 0.41ng/ul

response 19445

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	49.98
125.00	16.20	95.46#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
 Data File : BN008154.D
 Acq On : 15 Oct 2019 03:34
 Operator : JU
 Sample : K5097-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLMD9

Manual Integrations
 APPROVED

mohammad
 10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:37:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:19:29 2019
 Response via : Initial Calibration

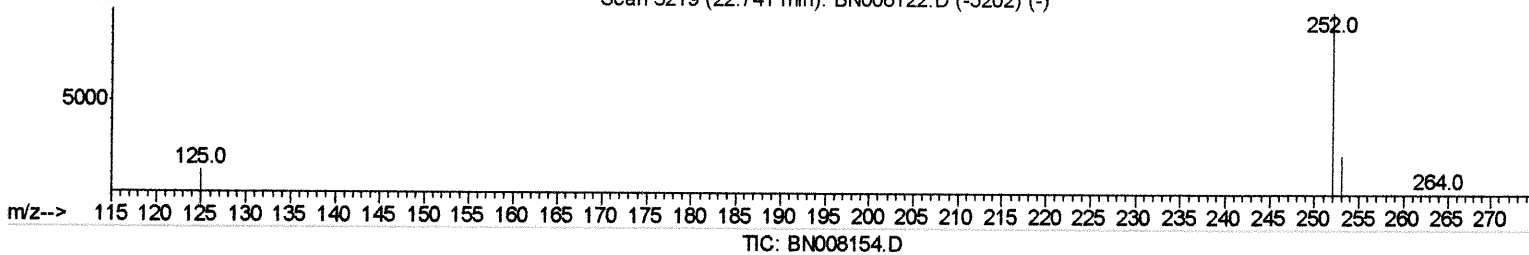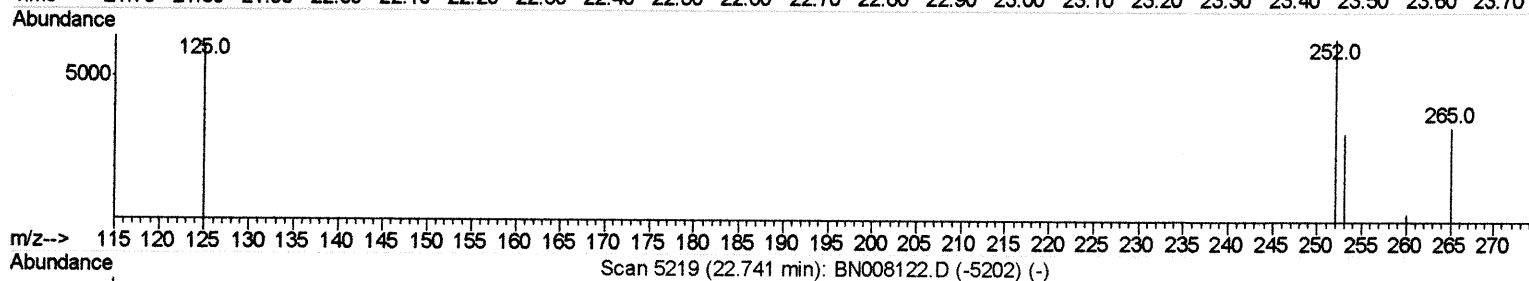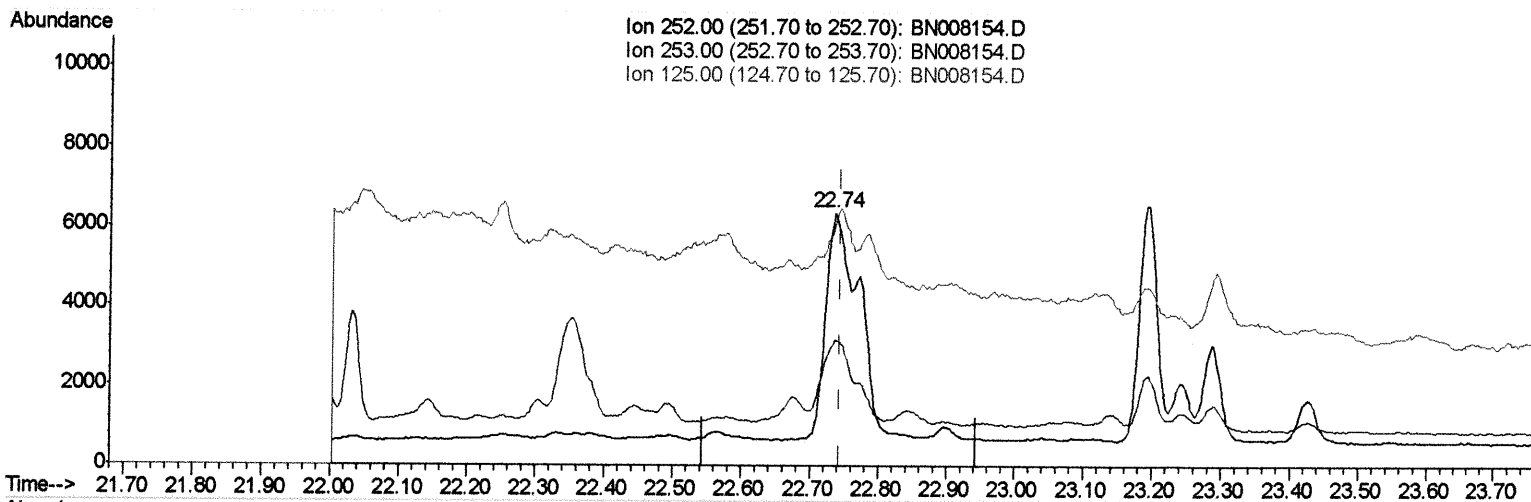

(21) Benzo(b)fluoranthene

22.735min (-0.009) 0.27ng/ul m *JU 10/16/19*

response 12686

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	49.98
125.00	16.20	95.46#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008154.D
Acq On : 15 Oct 2019 03:34
Operator : JU
Sample : K5097-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLMD9

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:37:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:19:29 2019
Response via : Initial Calibration

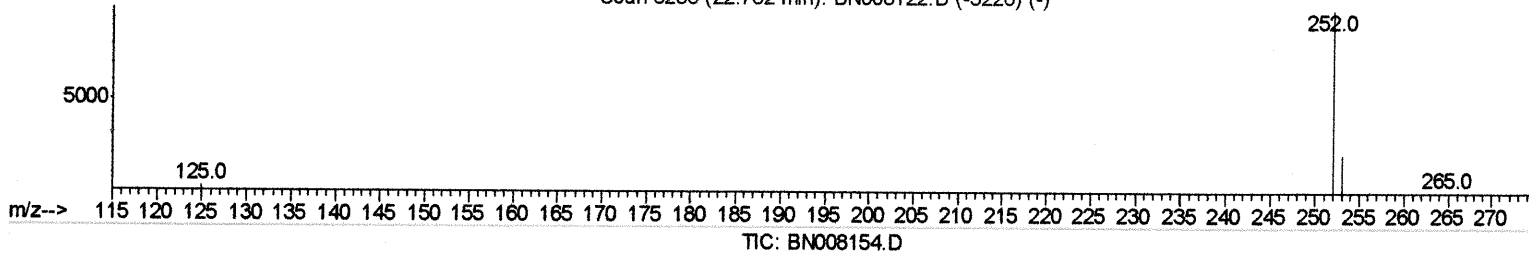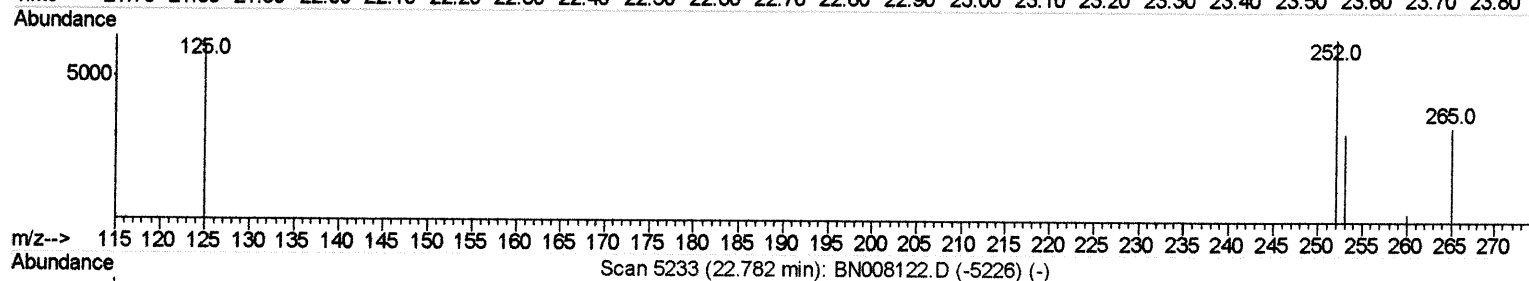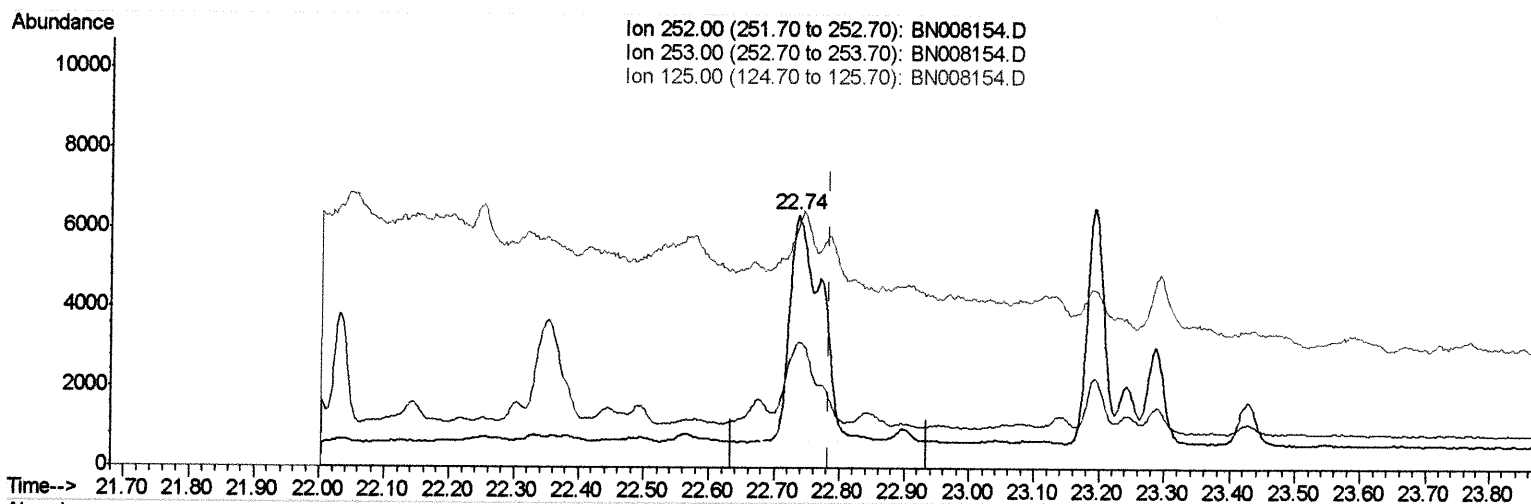

(22) Benzo(k)fluoranthene

22.735min (-0.050) 0.36ng/ul

response 19445

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	49.98#
125.00	15.40	95.46#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
 Data File : BN008154.D
 Acq On : 15 Oct 2019 03:34
 Operator : JU
 Sample : K5097-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLMD9

Manual Integrations
 APPROVED

mohammad
 10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:37:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:19:29 2019
 Response via : Initial Calibration

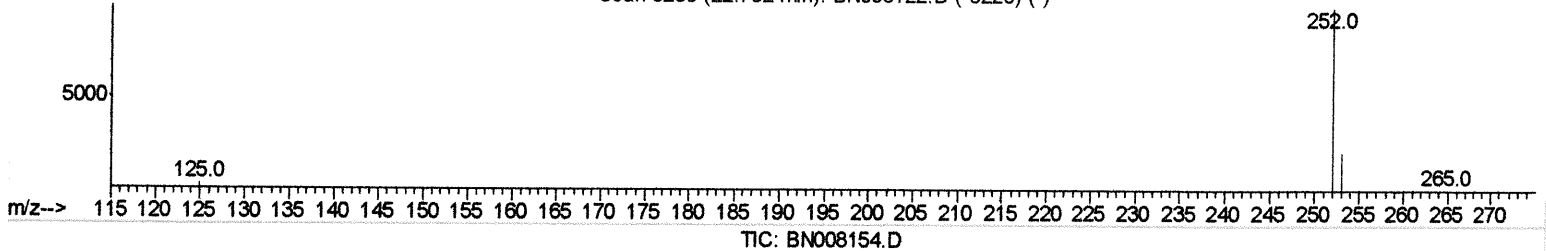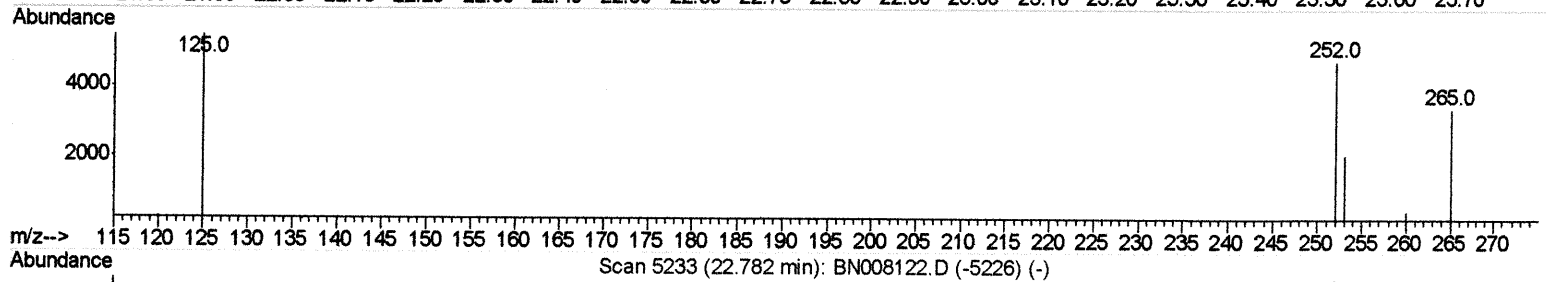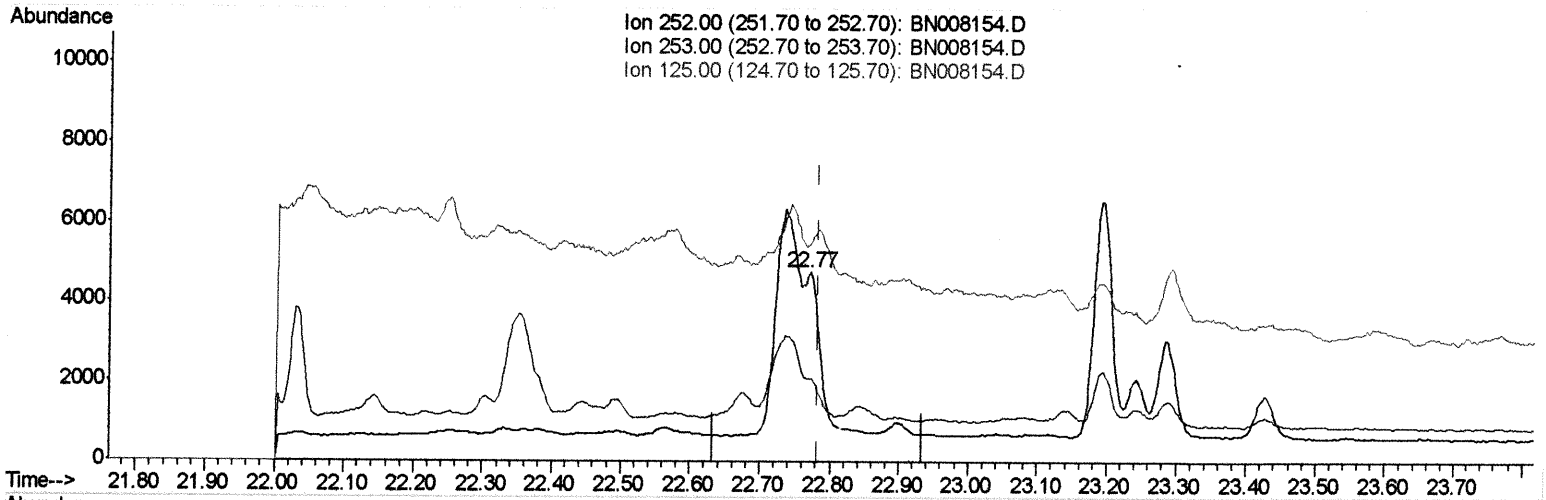

(22) Benzo(k)fluoranthene

22.770min (-0.015) 0.10ng/ul m *DL 10/16/19*

response 5469

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	43.90#
125.00	15.40	114.63#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
 Data File : BN008154.D
 Acq On : 15 Oct 2019 03:34
 Operator : JU
 Sample : K5097-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLMD9

Manual Integrations
 APPROVED

mohammad
 10/15/2019 1:30:38 PM

Quant Time: Oct 15 04:38:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:19:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	2283	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	11249	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	7340	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	16747m	0.40	ng/ul	0.00
16) Chrysene-d12	21.20	240	17060m	0.40	ng/ul	0.00
20) Perylene-d12	23.38	264	14581m	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.98	152	2889	0.15	ng/ul	0.00
14) Fluoranthene-d10	19.03	212	9510m	0.16	ng/ul	0.00

Target Compounds

					Ovalue	
3) Naphthalene	10.43	128	1448	0.045	ng/ul#	85
5) 2-Methylnaphthalene	12.06	142	1522	0.069	ng/ul	99
12) Phenanthrene	17.04	178	1912m	0.039	ng/ul	
15) Fluoranthene	19.07	202	10230m	0.158	ng/ul	
17) Pyrene	19.43	202	22996	0.339	ng/ul	98
18) Benzo(a)anthracene	21.18	228	12793m	0.206	ng/ul	
19) Chrysene	21.23	228	5579m	0.073	ng/ul	
21) Benzo(b)fluoranthene	22.74	252	12686m	0.267	ng/ul	
22) Benzo(k)fluoranthene	22.77	252	5469m	0.102	ng/ul	
23) Benzo(a)pyrene	23.29	252	4320	0.086	ng/ul#	1
24) Indeno(1,2,3-cd)pyrene	25.55	276	3930	0.067	ng/ul#	76
26) Benzo(a,h,i)perylene	26.21	276	14441	0.268	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed