


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008160.D
Acq On : 15 Oct 2019 07:08
Operator : JU
Sample : K5097-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLME7

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:55 PM

Quant Time: Oct 15 07:47:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 05:17:53 2019
Response via : Initial Calibration

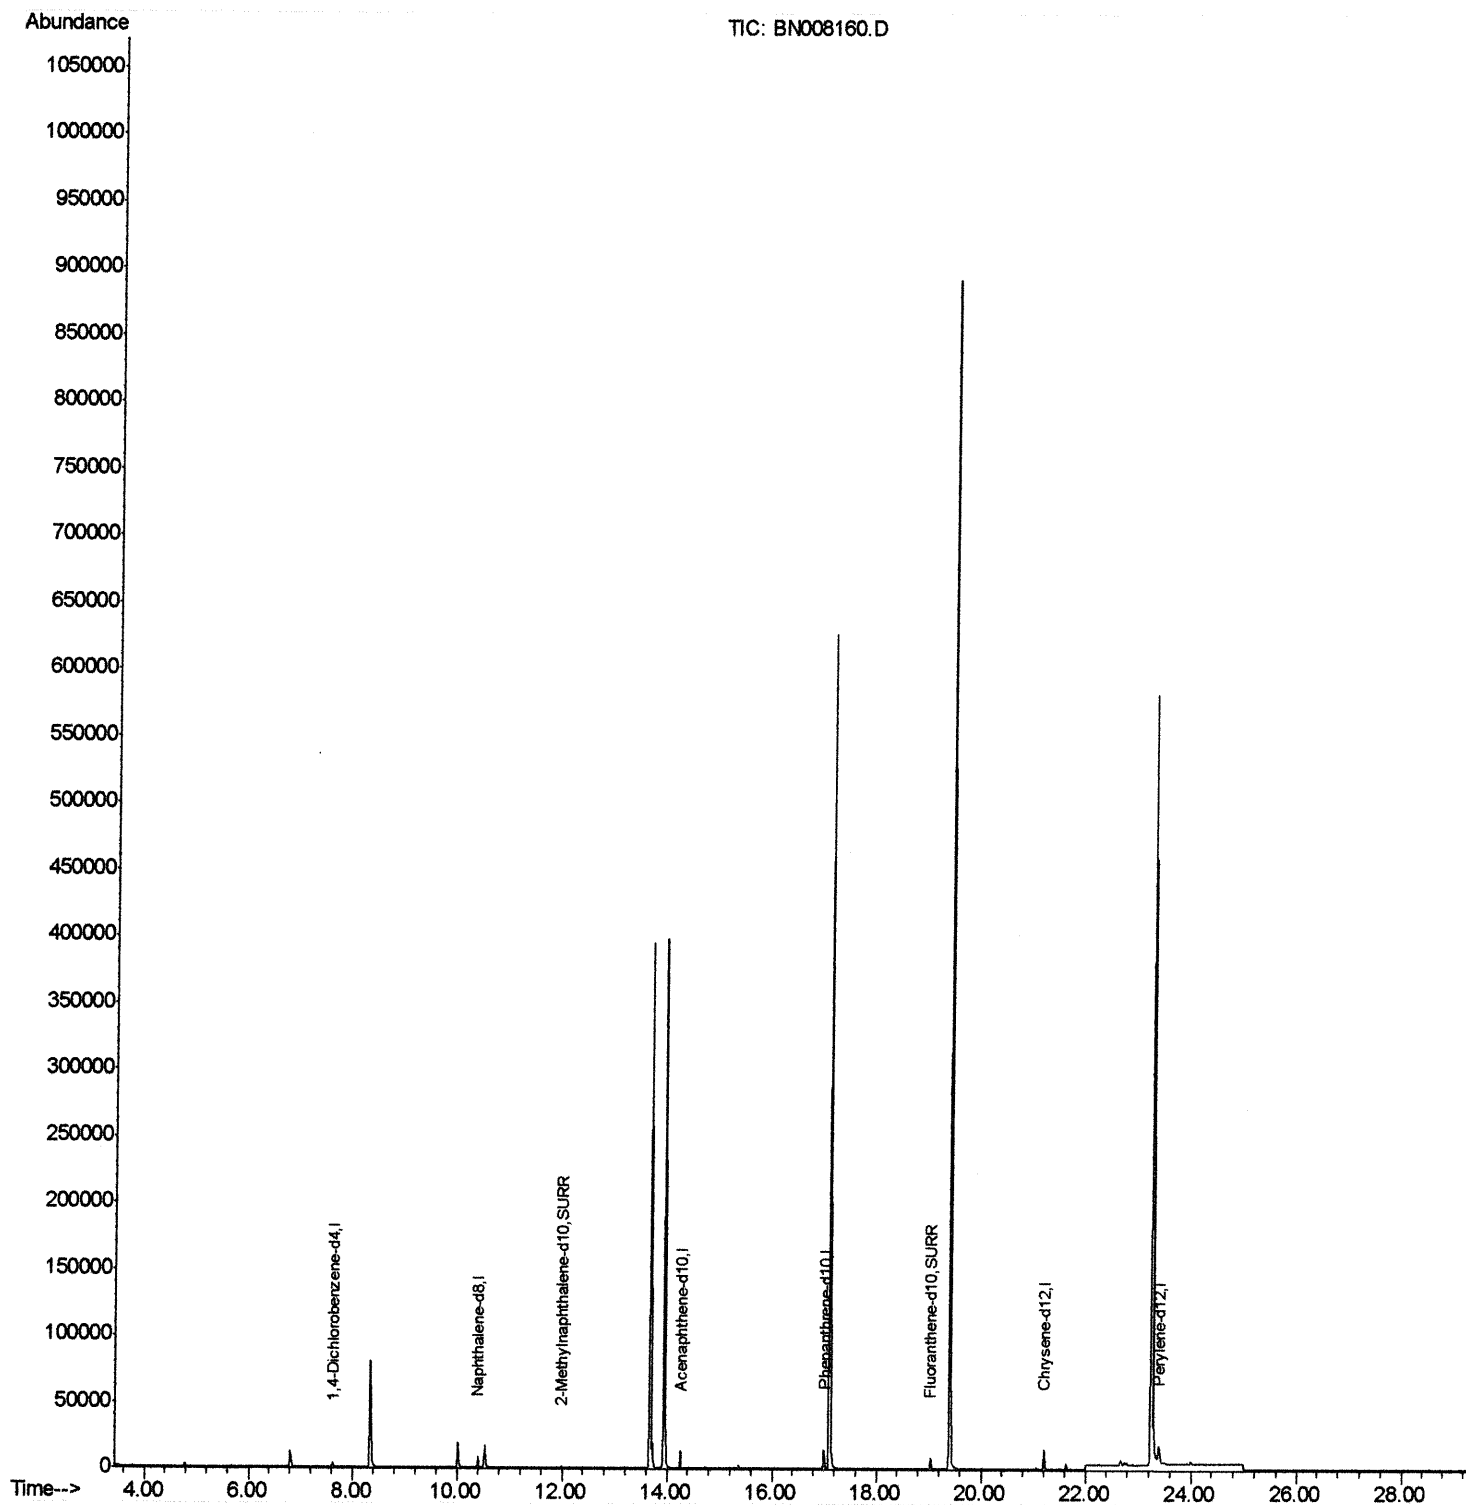


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008160.D
Acq On : 15 Oct 2019 07:08
Operator : JU
Sample : K5097-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLME7

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:55 PM

Quant Time: Oct 15 07:41:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 05:17:53 2019
Response via : Initial Calibration

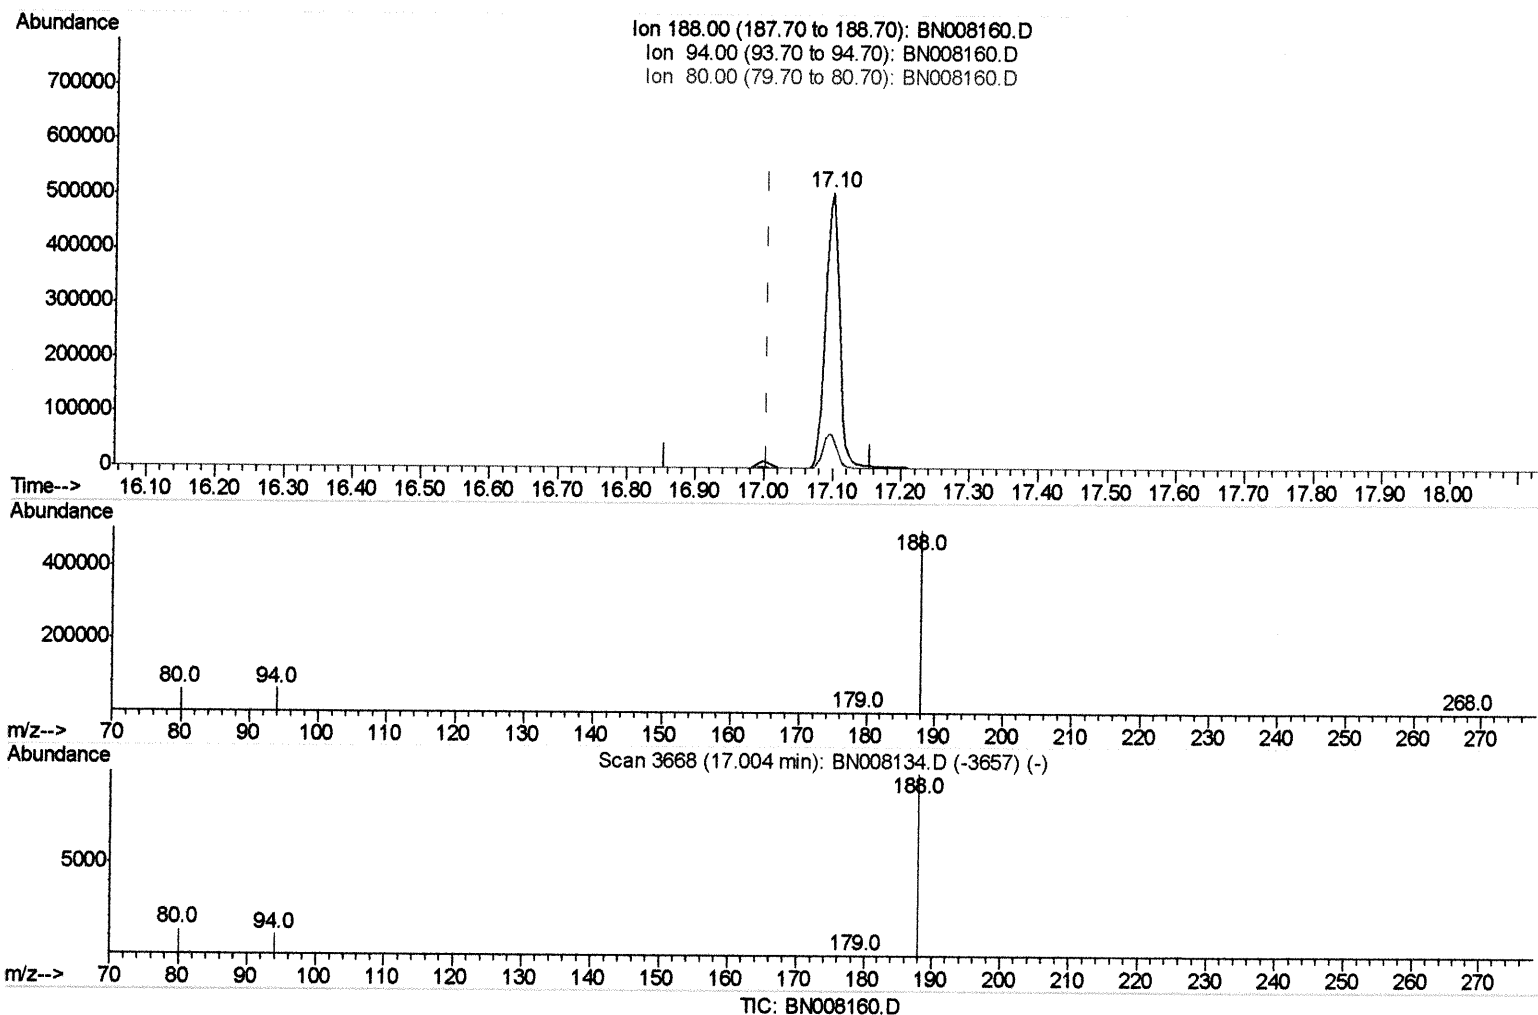

(10) Phenanthrene-d10 (I)

17.097min (+0.093) 0.40ng/ul

response 703109

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	12.28
80.00	12.60	11.95
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008160.D
Acq On : 15 Oct 2019 07:08
Operator : JU
Sample : K5097-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLME7

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:55 PM

Quant Time: Oct 15 07:41:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 05:17:53 2019
Response via : Initial Calibration

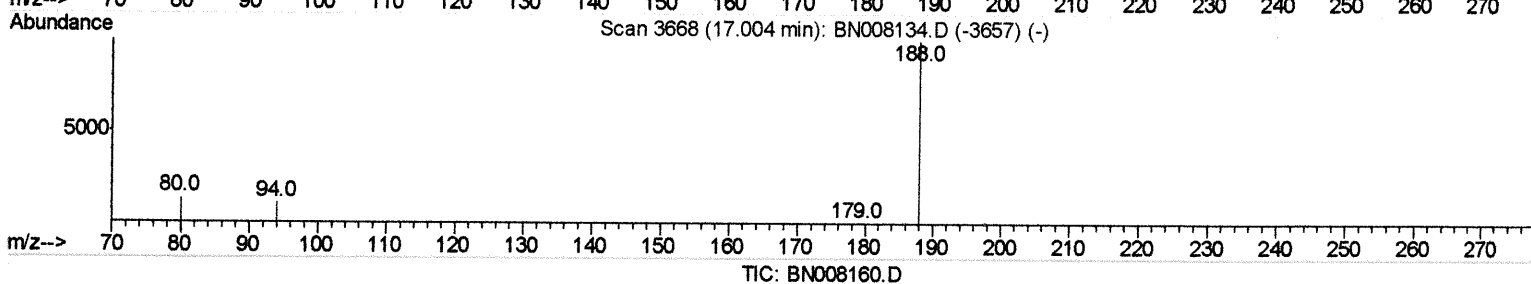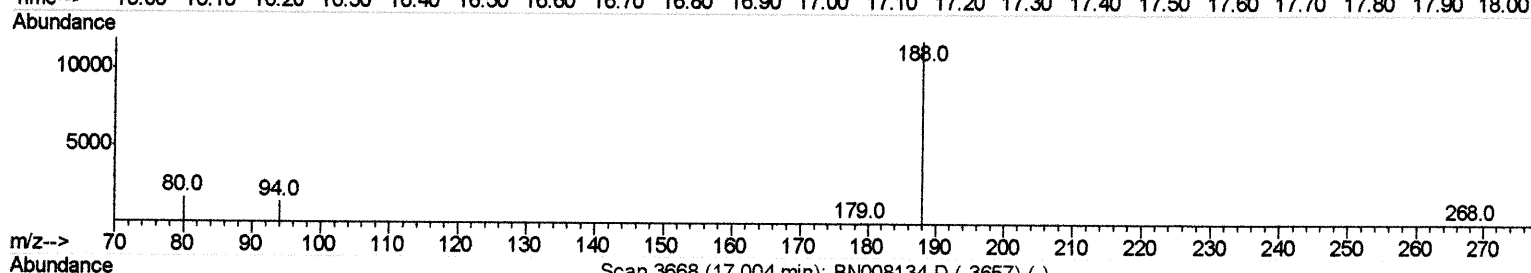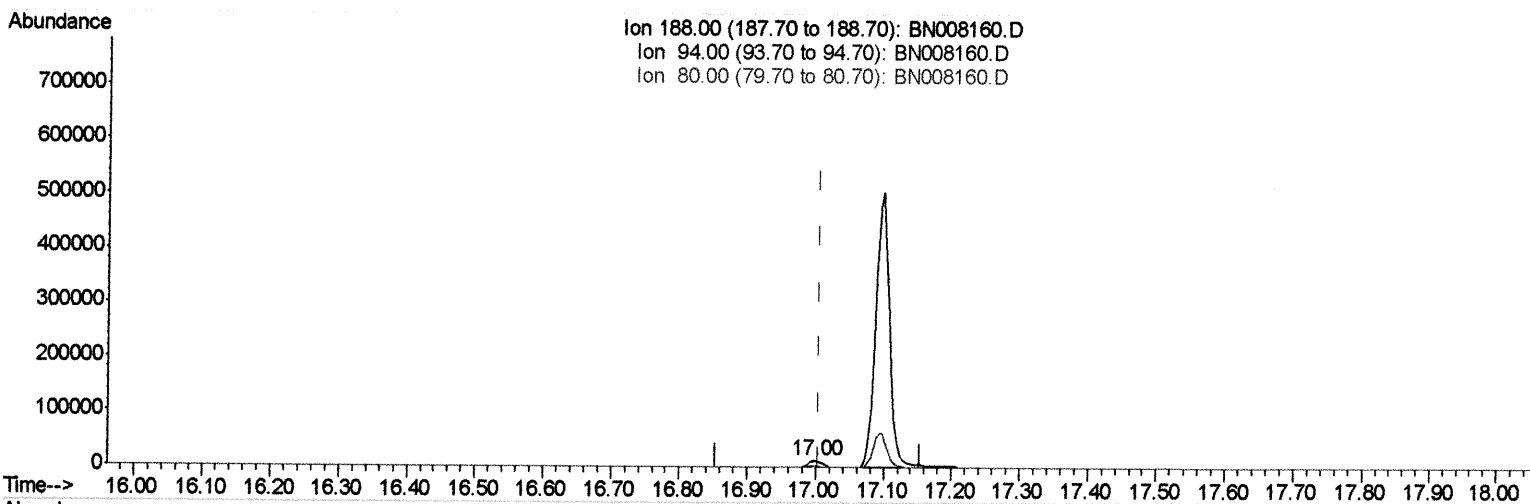

(10) Phenanthrene-d10 (I)

17.000min (-0.004) 0.40ng/ul m *JU 10/16/19*

response 17518

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	11.12
80.00	12.60	13.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\

Data File : BN008160.D

Acq On : 15 Oct 2019 07:08

Operator : JU

Sample : K5097-11

Misc :

ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 15 07:45:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Oct 15 05:17:53 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

JLME7

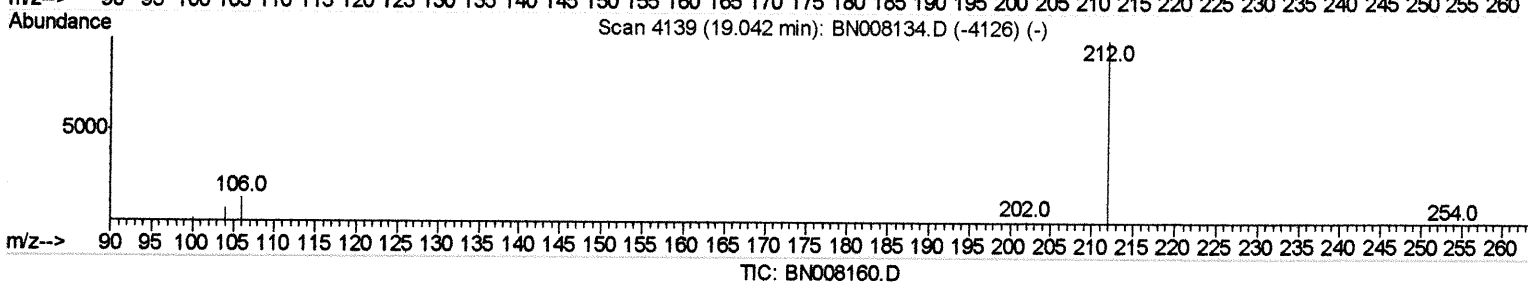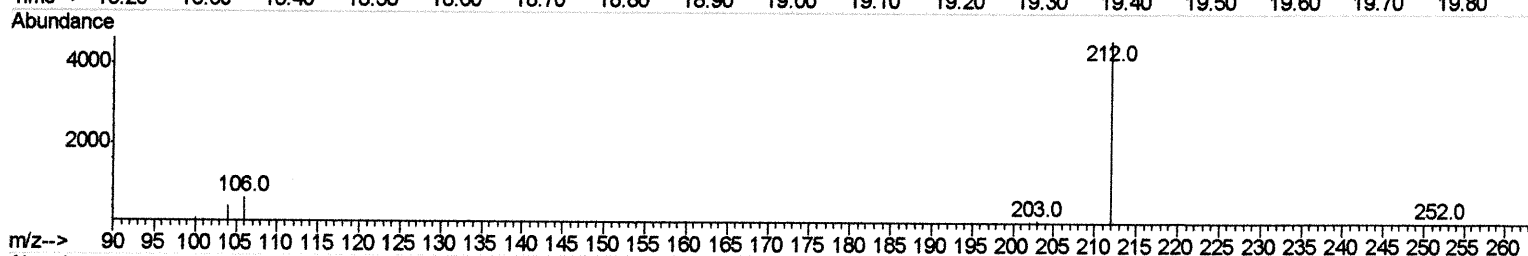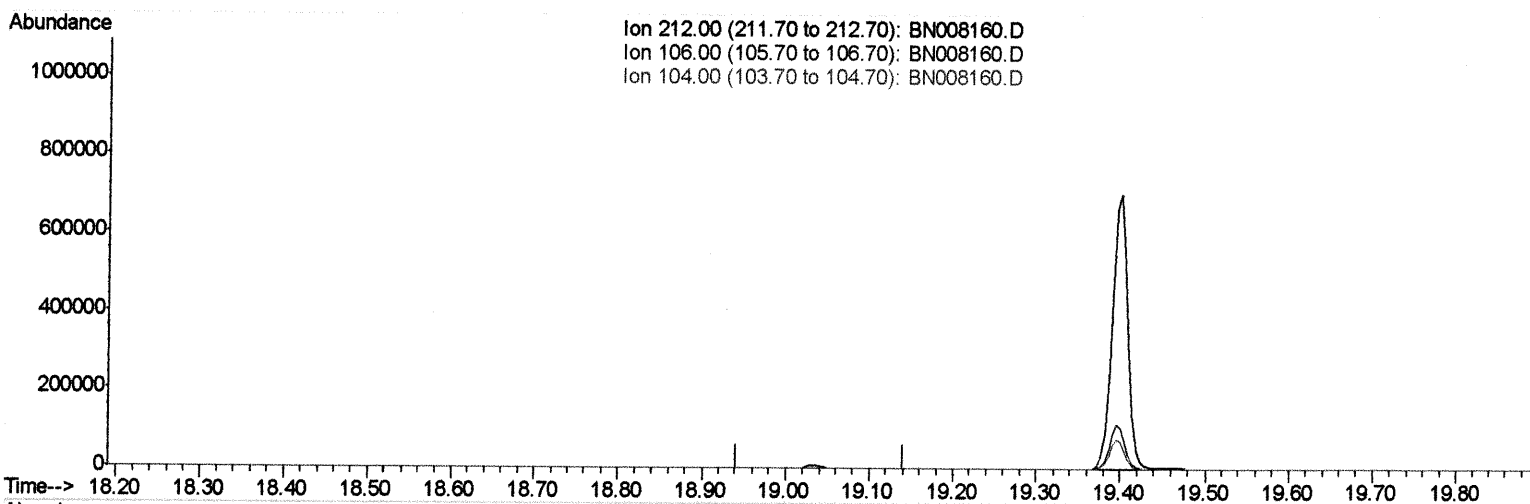Manual Integrations
APPROVEDmohammad
10/15/2019 1:30:55 PM

(14) Fluoranthene-d10 (SURR)

19.042min (-19.042) 0.00ng/ui

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	12.70	0.00#
104.00	7.20	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\

Data File : BN008160.D

Acq On : 15 Oct 2019 07:08

Operator : JU

Sample : K5097-11

Misc :

ALS Vial : 28 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampled :

JLME7

Manual Integrations
APPROVEDmohammad
10/15/2019 1:30:55 PM



Quant Time: Oct 15 07:45:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Oct 15 05:17:53 2019

Response via : Initial Calibration

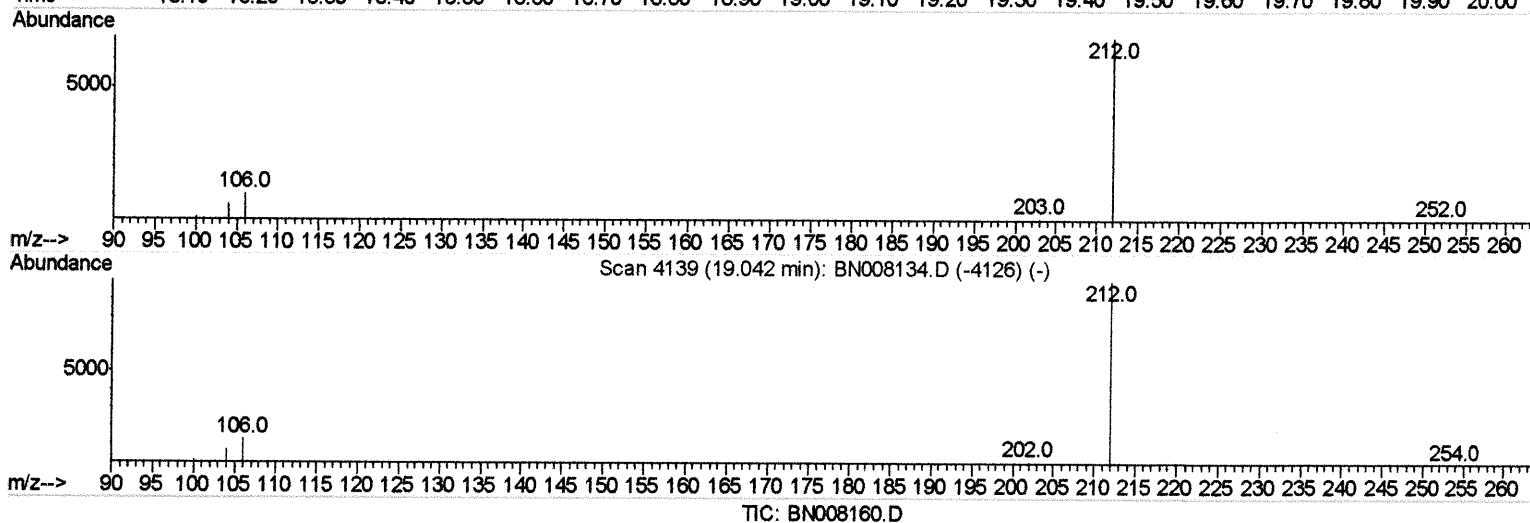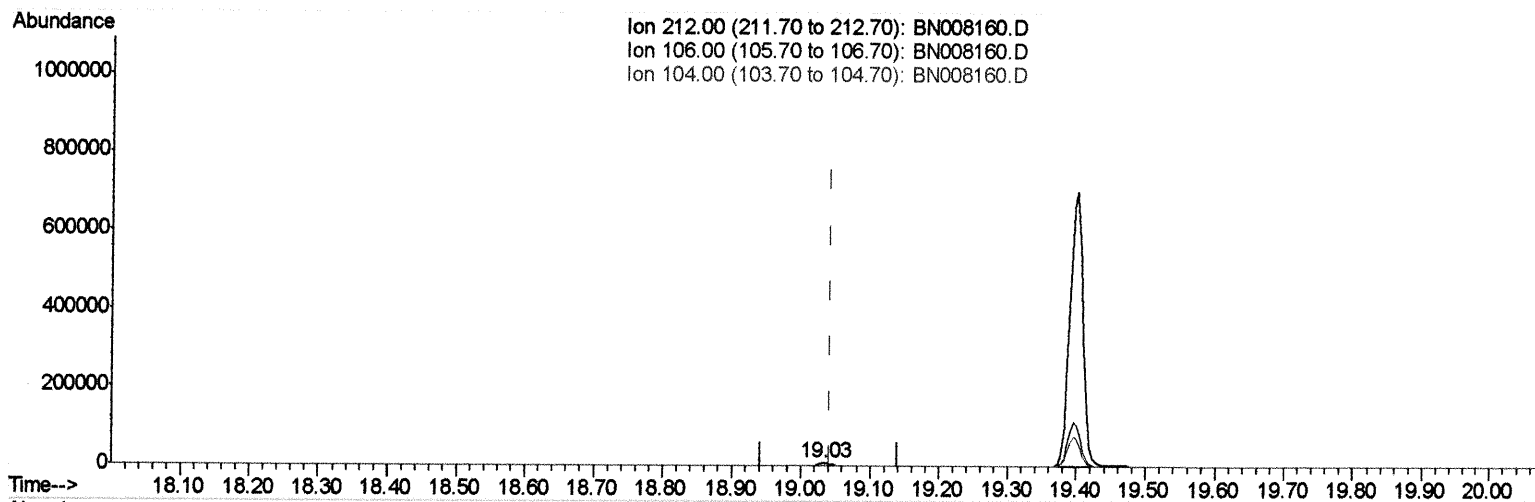

(14) Fluoranthene-d10 (SURR)

19.032min (-0.009) 0.16ng/ul m *JU 10/16/19*

response 9642

Ion	Exp%	Act%
212.00	100	100
106.00	12.70	0.00#
104.00	7.20	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\

Data File : BN008160.D

Acq On : 15 Oct 2019 07:08

Operator : JU

Sample : K5097-11

Misc :

ALS Vial : 28 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

JLME7

Manual Integrations
APPROVEDmohammad
10/15/2019 1:30:55 PM



Quant Time: Oct 15 07:45:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Oct 15 05:17:53 2019

Response via : Initial Calibration

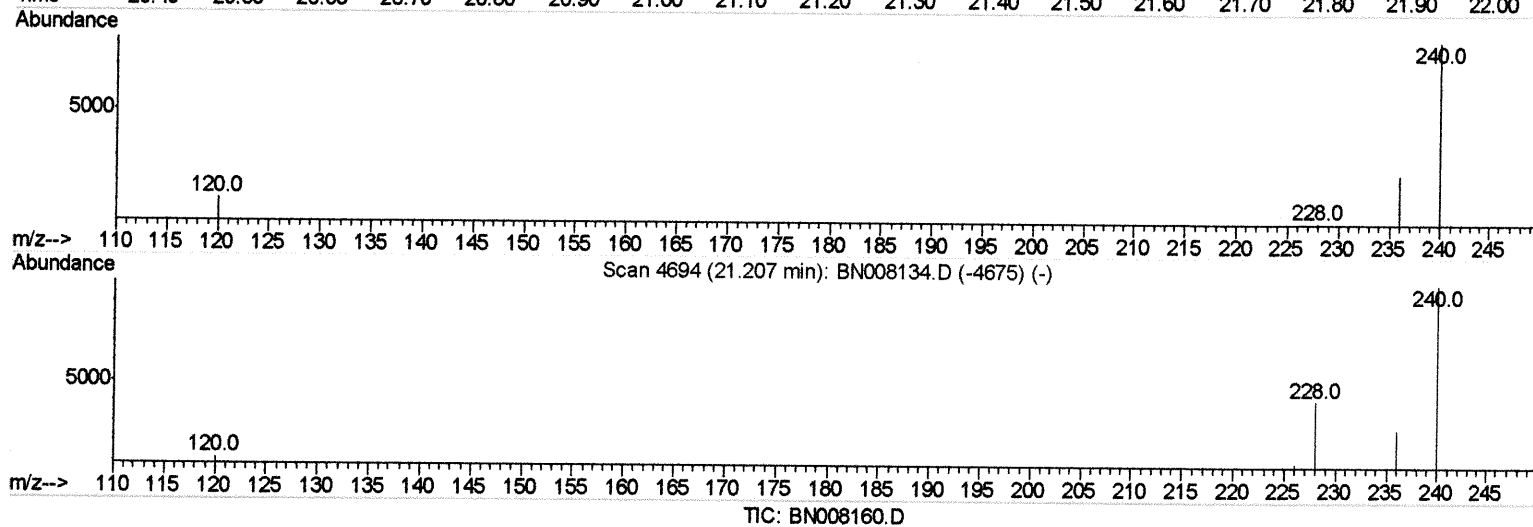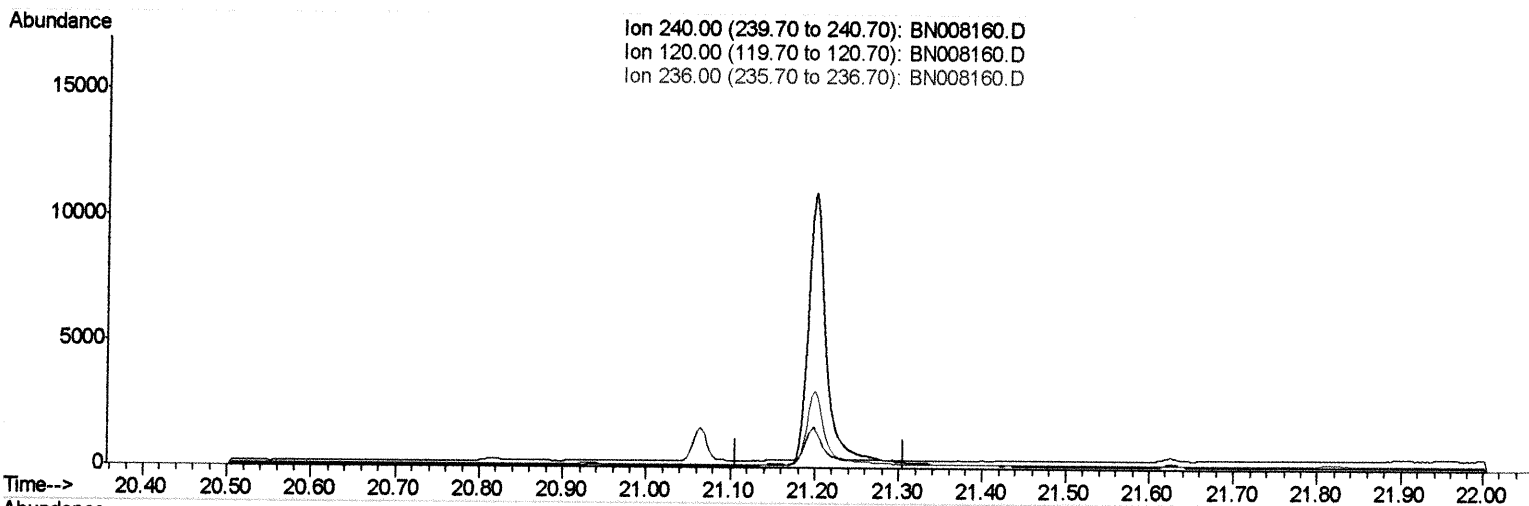

(16) Chrysene-d12 (I)

21.207min (-21.207) 0.00ng/ui

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.70	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
Data File : BN008160.D
Acq On : 15 Oct 2019 07:08
Operator : JU
Sample : K5097-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLME7

Manual Integrations
APPROVED

mohammad
10/15/2019 1:30:55 PM

Quant Time: Oct 15 07:45:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 05:17:53 2019
Response via : Initial Calibration

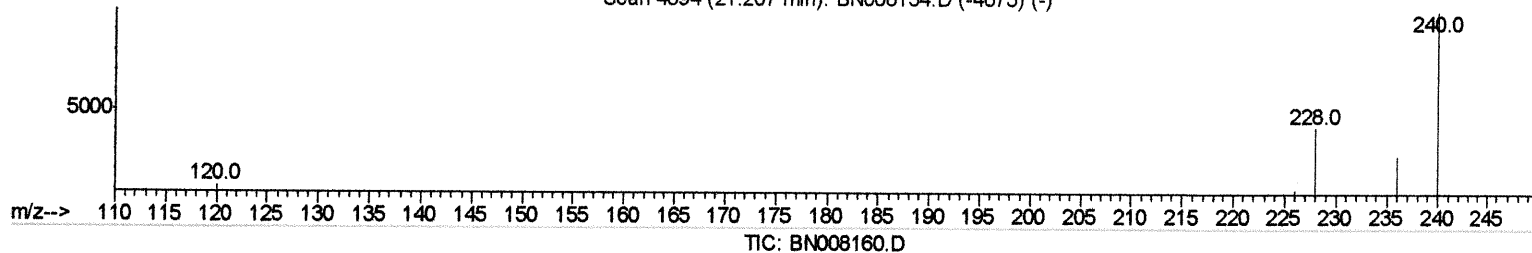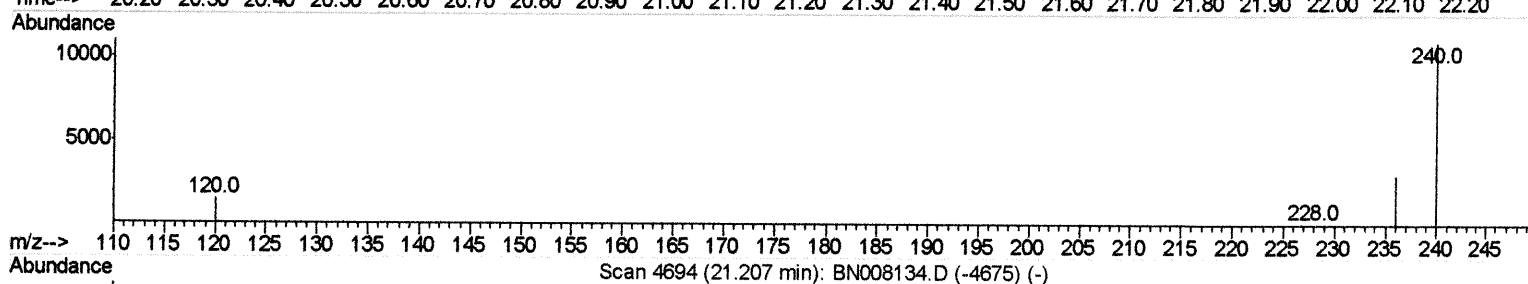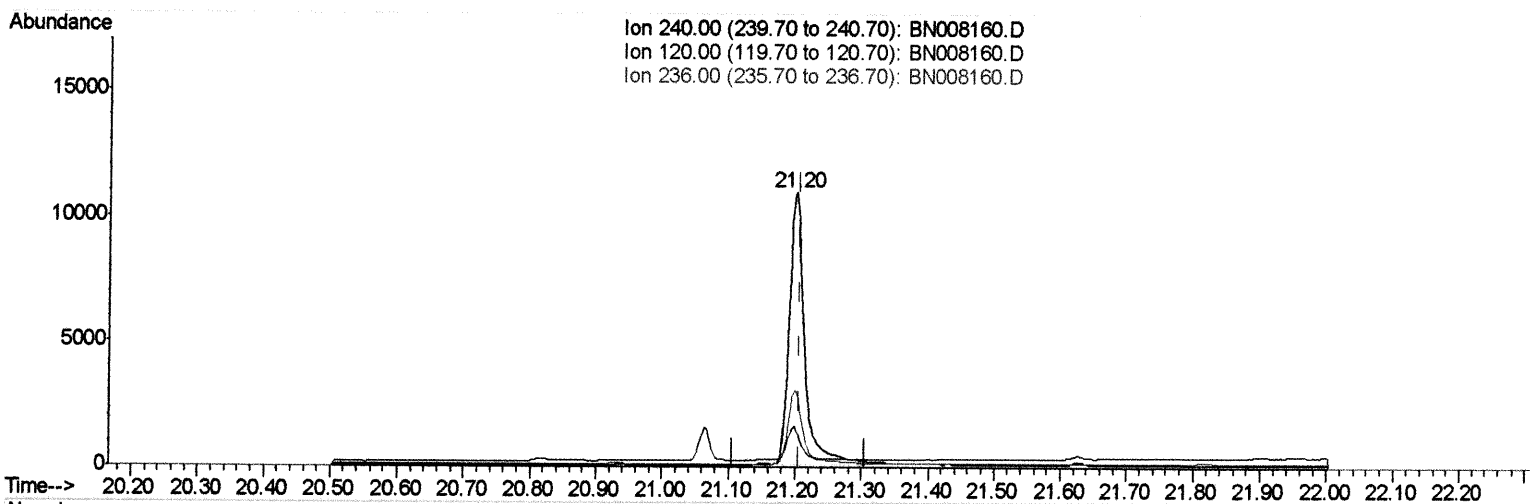

(16) Chrysene-d12 (I)

21.201min (-0.006) 0.40ng/ul m

JU 10/16/19

response 17651

Ion	Exp%	Act%
240.00	100	100
120.00	14.70	13.72
236.00	28.40	27.76
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101419\
 Data File : BN008160.D
 Acq On : 15 Oct 2019 07:08
 Operator : JU
 Sample : K5097-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLME7

Manual Integrations
 APPROVED

mohammad
 10/15/2019 1:30:55 PM

Quant Time: Oct 15 07:47:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 15 05:17:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	2339	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	11751	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.25	164	7717	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	17518m	0.40	ng/ul	0.00
16) Chrysene-d12	21.20	240	17651m	0.40	ng/ul	0.00
20) Perylene-d12	23.38	264	17093	0.40	ng/ul	-0.02

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.98	152	2972	0.15	ng/ul	0.00
14) Fluoranthene-d10	19.03	212	9642m	0.16	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed