


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101619\
Data File : BN008201.D
Acq On : 16 Oct 2019 16:41
Operator : JU
Sample : PB123577BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Oct 16 18:27:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 16 17:43:36 2019
Response via : Initial Calibration

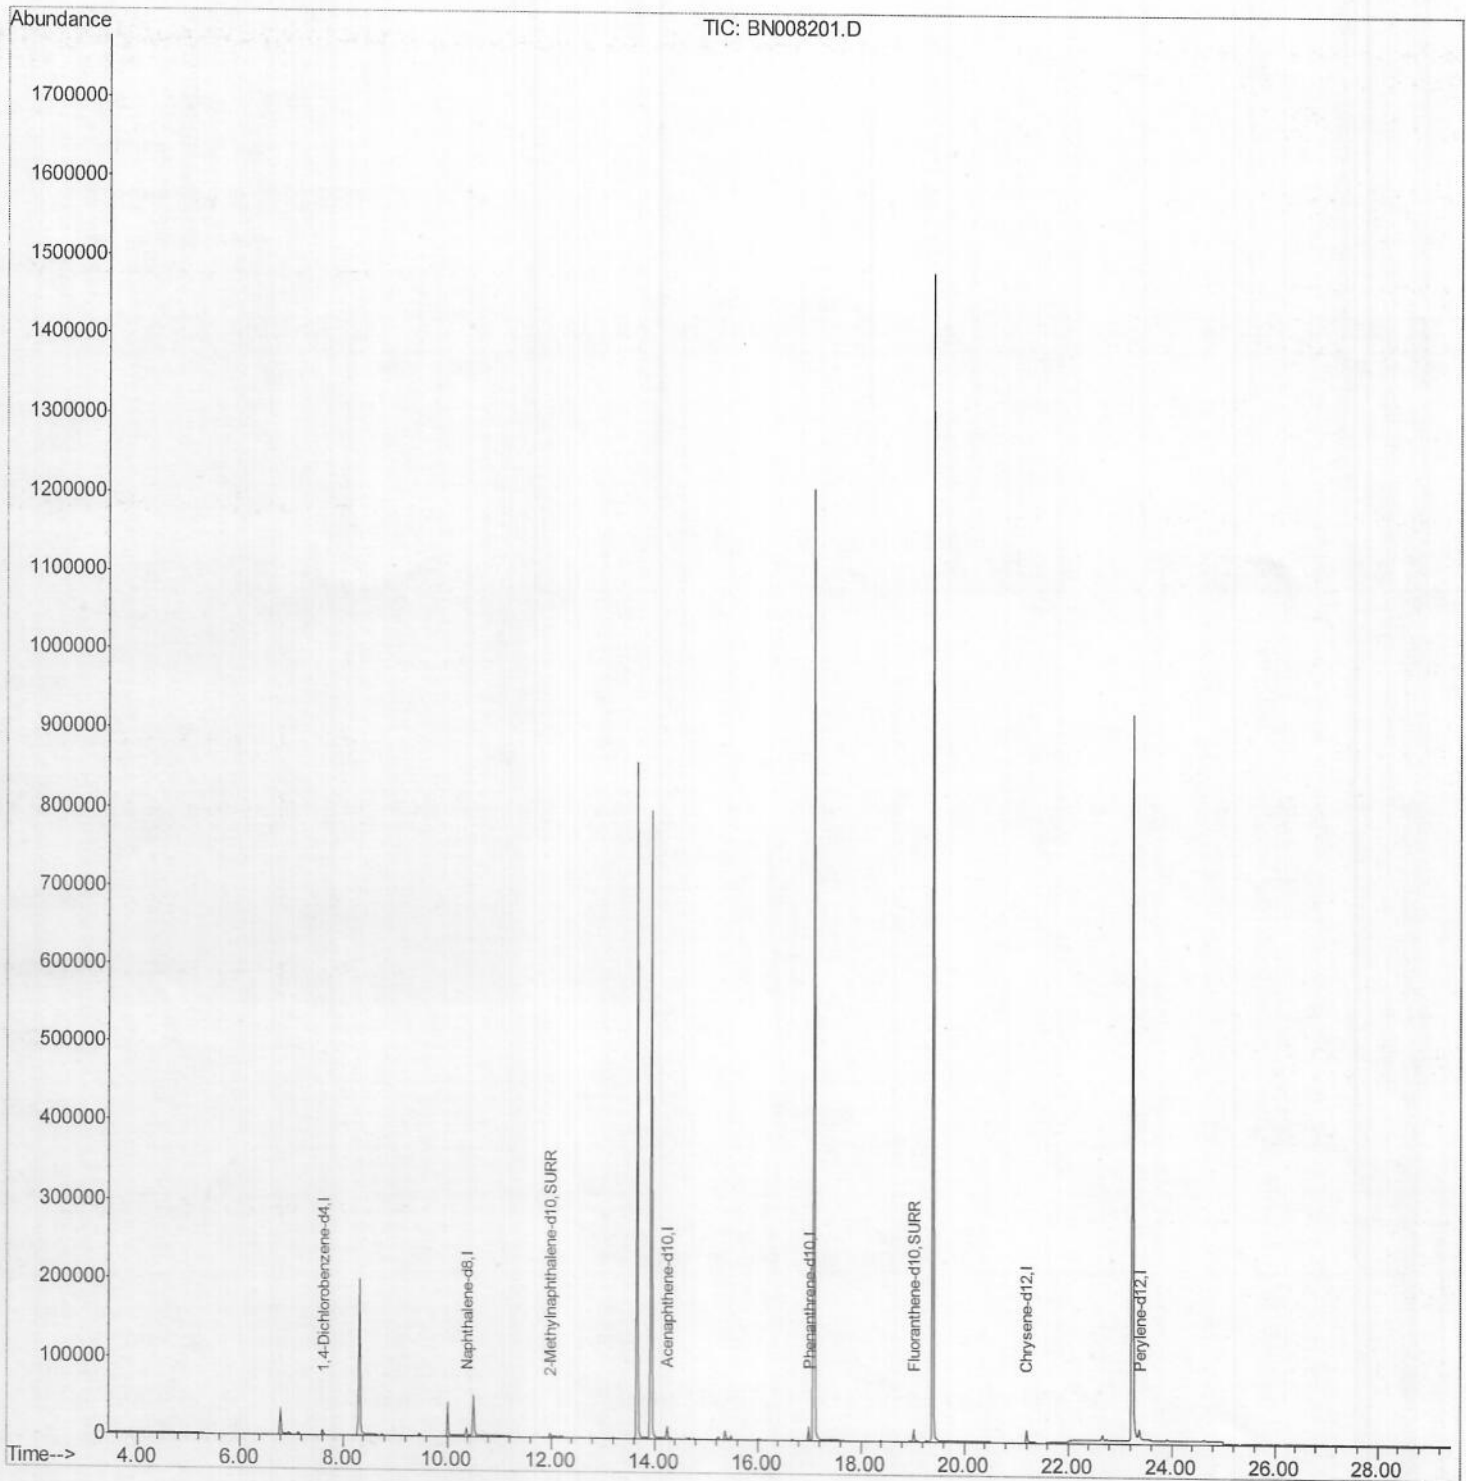

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101619\

Data File : BN008201.D

Acq On : 16 Oct 2019 16:41

Operator : JU

Sample : PB123577BL

Misc :

ALS Vial : 12 Sample Multiplier: 1




Quant Time: Oct 16 18:26:44 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Oct 16 17:43:36 2019

Response via : Initial Calibration

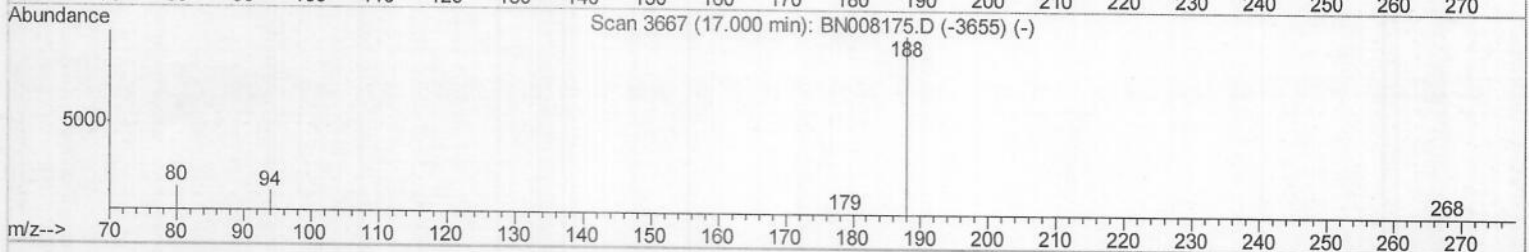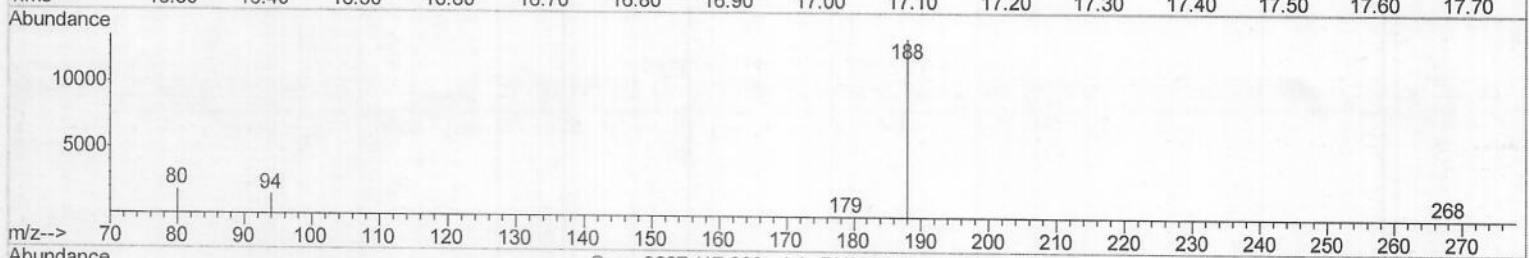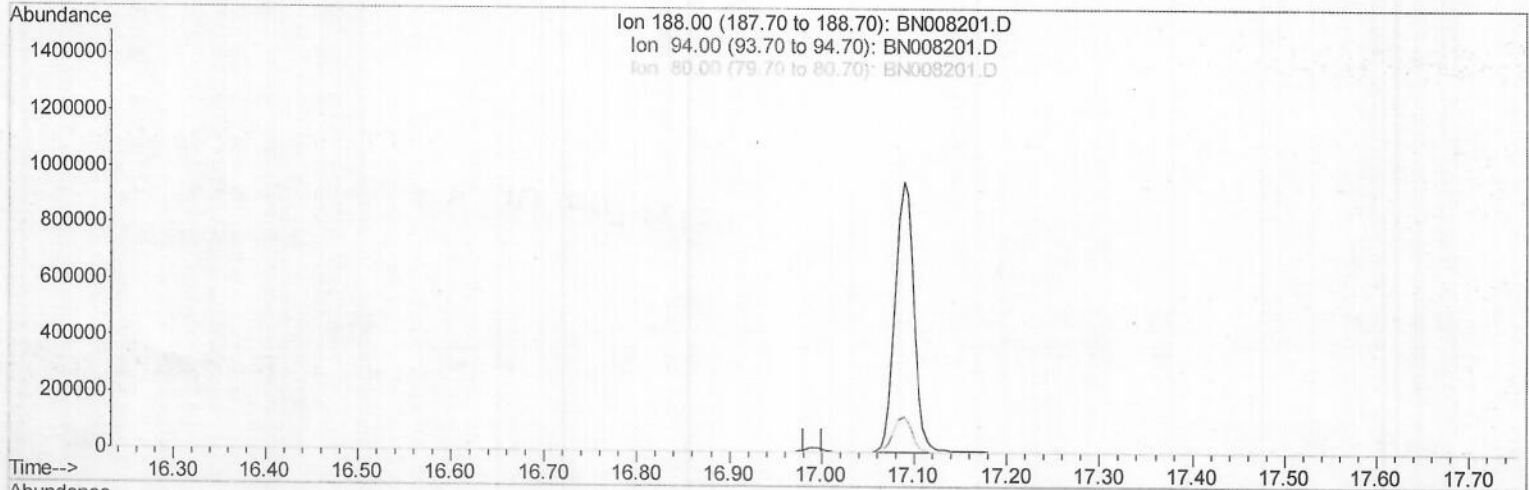

TIC: BN008201.D

(10) Phenanthrene-d10 (I)

16.991min (-16.991) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.90	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101619\

Data File : BN008201.D

Acq On : 16 Oct 2019 16:41

Operator : JU

Sample : PB123577BL

Misc :

ALS Vial : 12 Sample Multiplier: 1




Quant Time: Oct 16 18:26:44 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Oct 16 17:43:36 2019

Response via : Initial Calibration

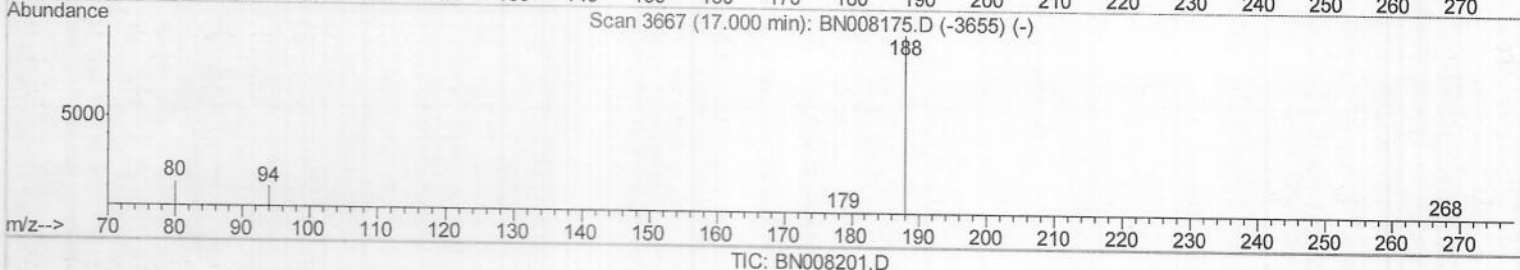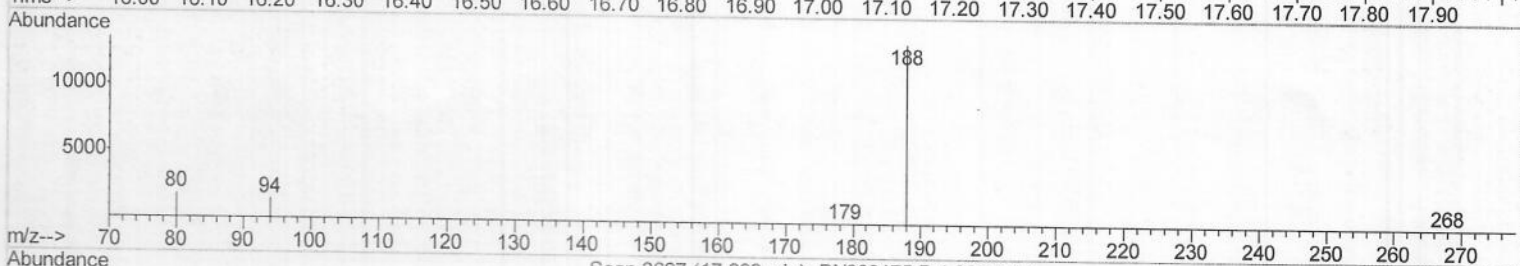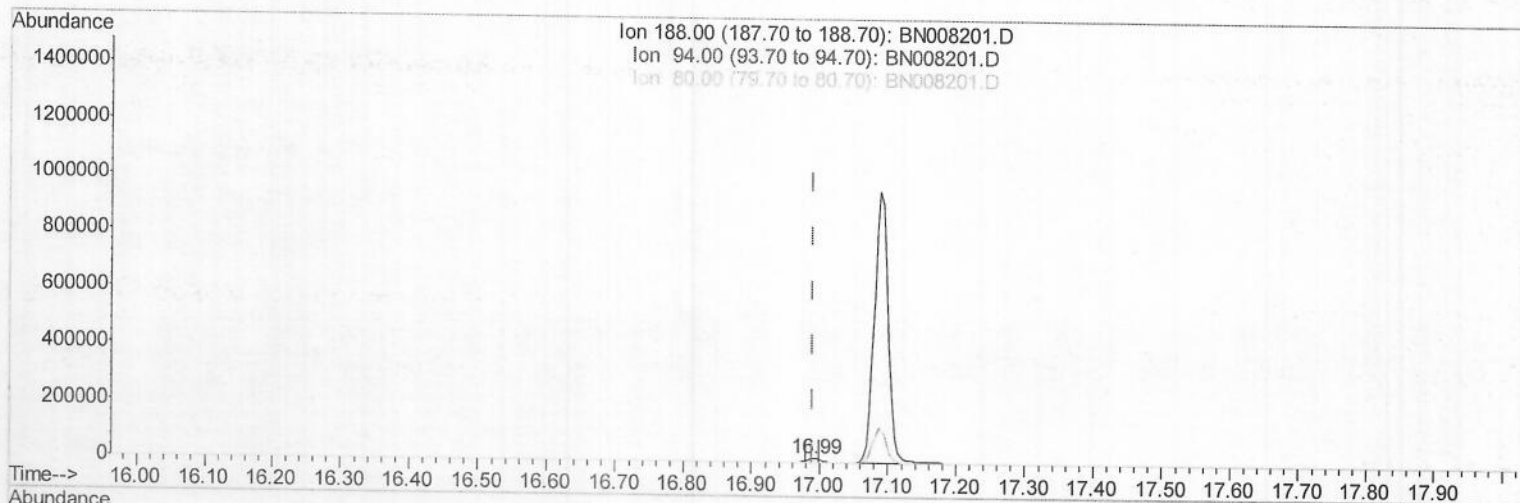

(10) Phenanthrene-d10 (I)

16.992min (+0.001) 0.40ng/ul m

response 19345

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	11.00
80.00	12.60	13.49
0.00	0.00	0.00

JU 20148119

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101619\
Data File : BN008201.D
Acq On : 16 Oct 2019 16:41
Operator : JU
Sample : PB123577BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Oct 16 18:27:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 16 17:43:36 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	2939	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	13839	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	8701	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188	19345m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	17064	0.40	ng/ul	0.00
20) Perylene-d12	23.37	264	15314	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	6357	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.03	212	17592	0.26	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

3 JU
40/28/19