





Data File : BN008211.D
Acq On : 16 Oct 2019 22:44
Operator : JU
Sample : PB123769BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Oct 17 03:02:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 17 01:48:53 2019
Response via : Initial Calibration

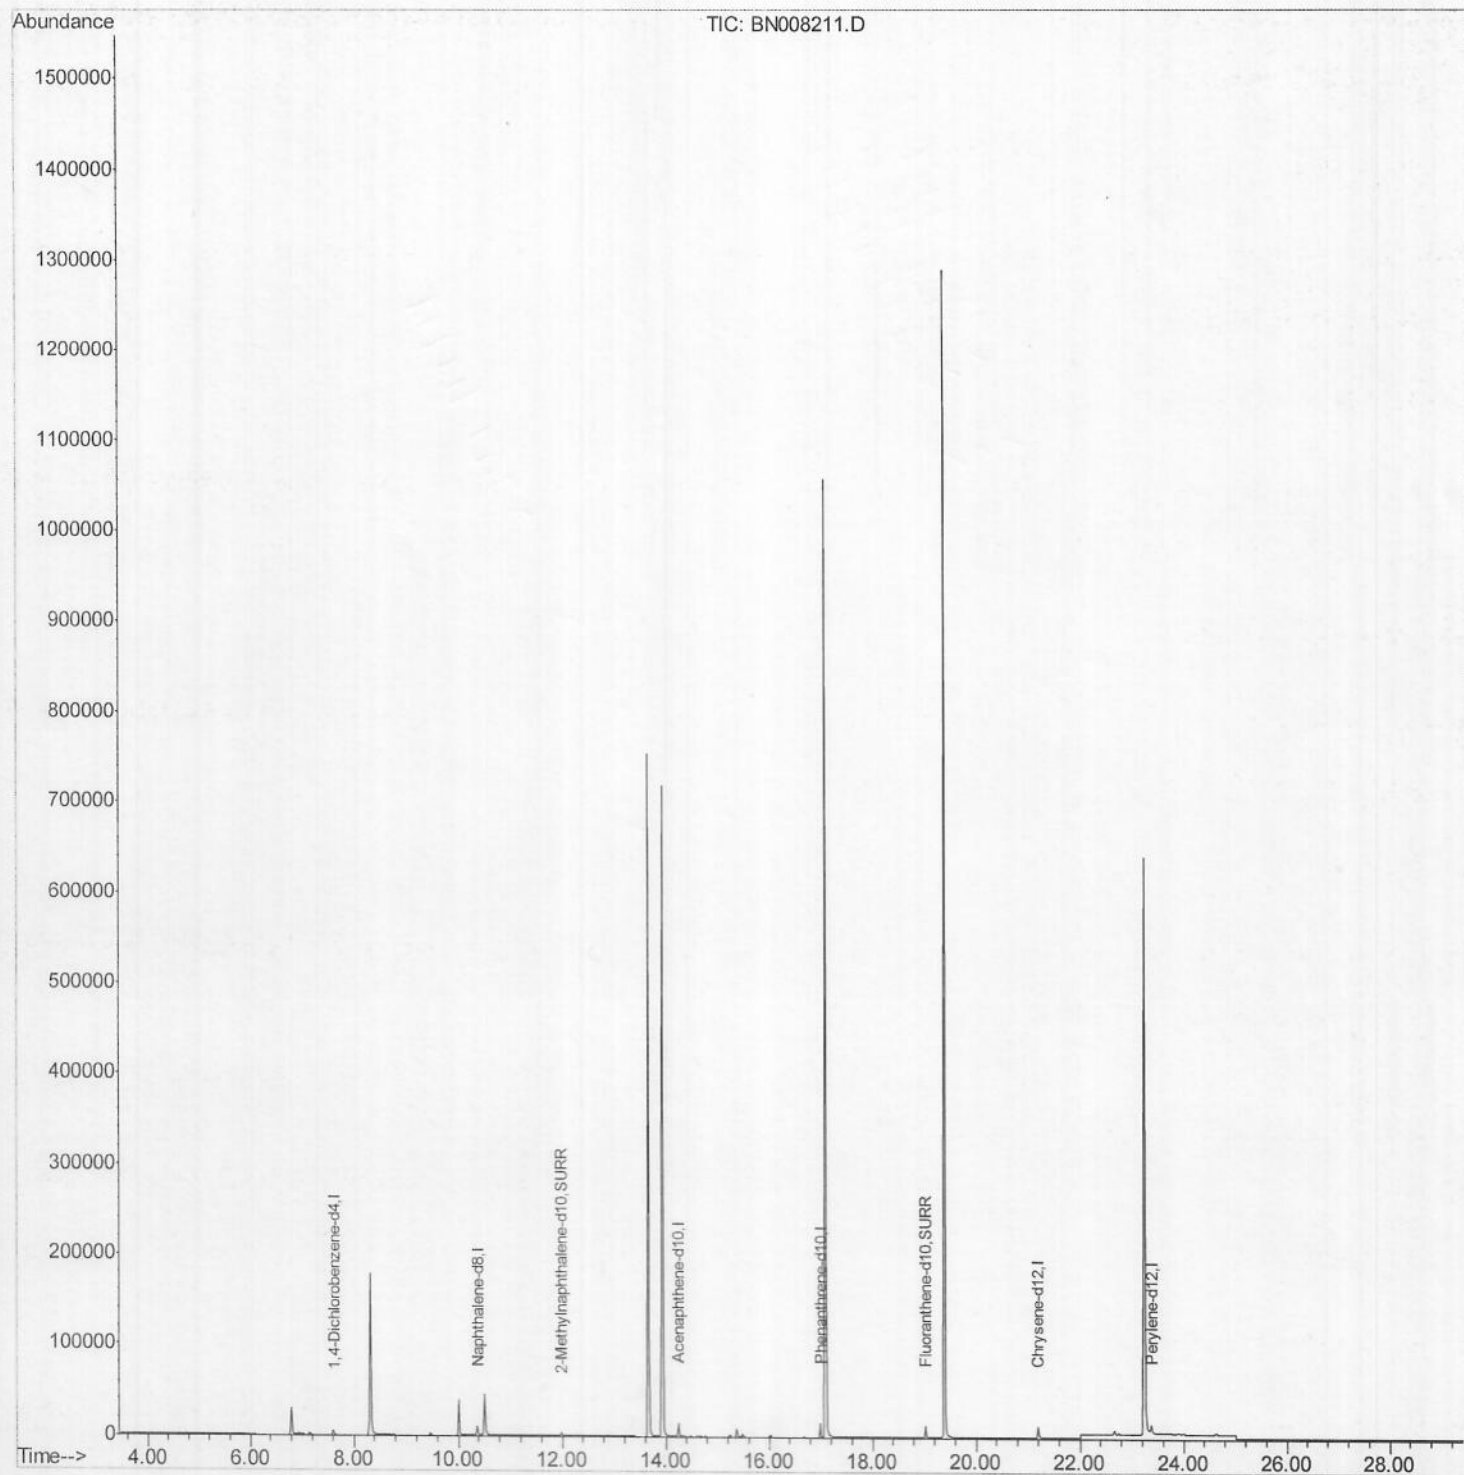

Data File : BN008211.D
Acq On : 16 Oct 2019 22:44
Operator : JU
Sample : PB123769BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Oct 17 01:53:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 17 01:48:53 2019
Response via : Initial Calibration

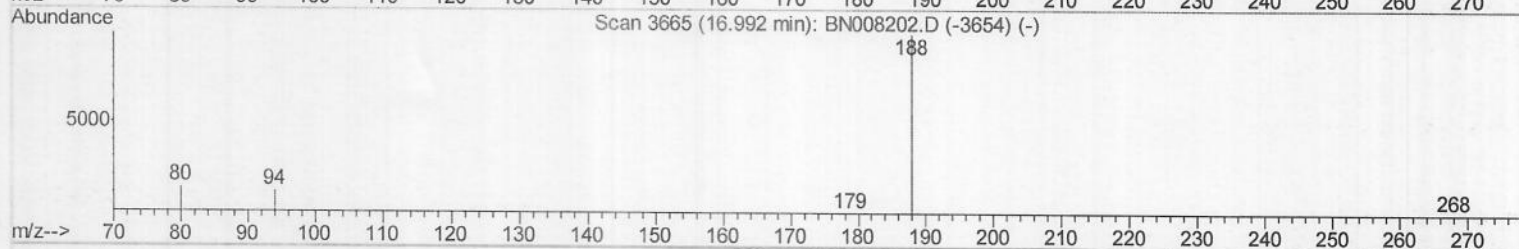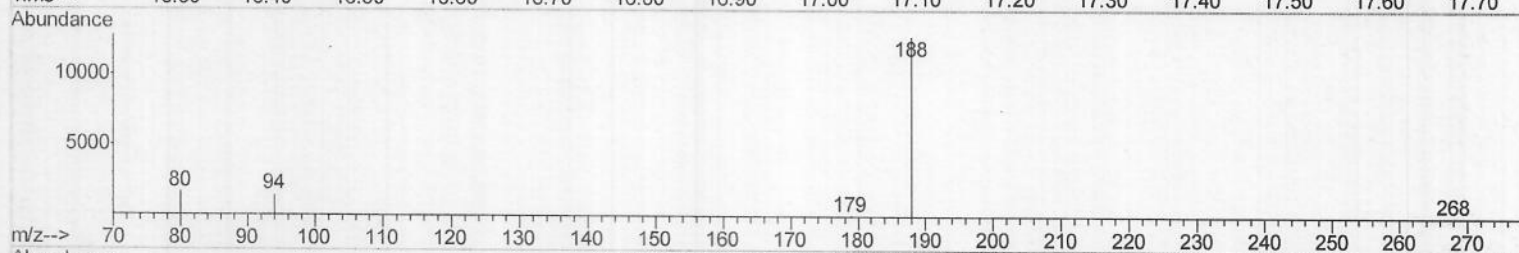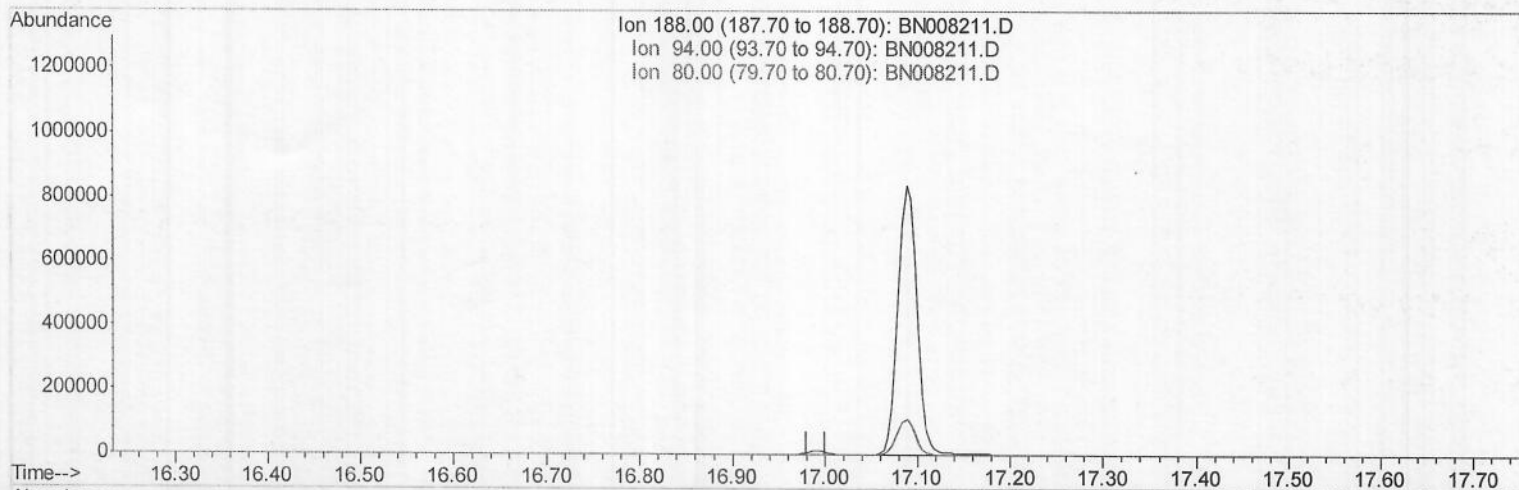

TIC: BN008211.D

(10) Phenanthrene-d10 (I)

16.992min (-16.992) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.90	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data File : BN008211.D

Acq On : 16 Oct 2019 22:44

Operator : JU

Sample : PB123769BL

Misc :

ALS Vial : 21 Sample Multiplier: 1




Quant Time: Oct 17 01:53:47 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Oct 17 01:48:53 2019

Response via : Initial Calibration

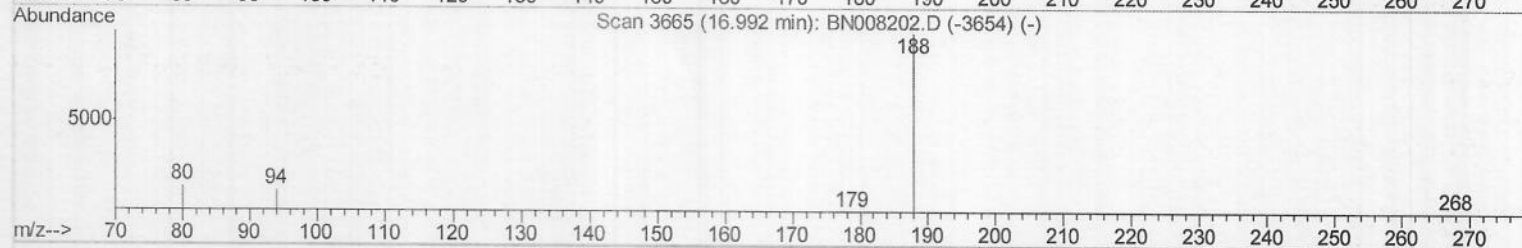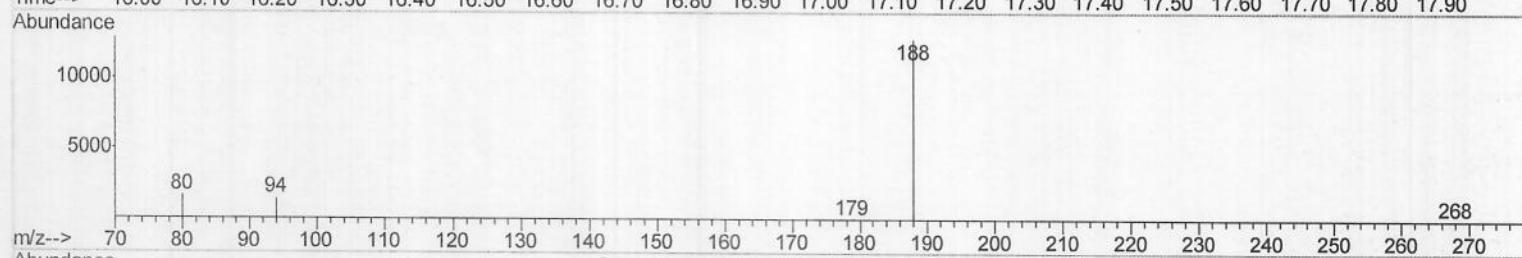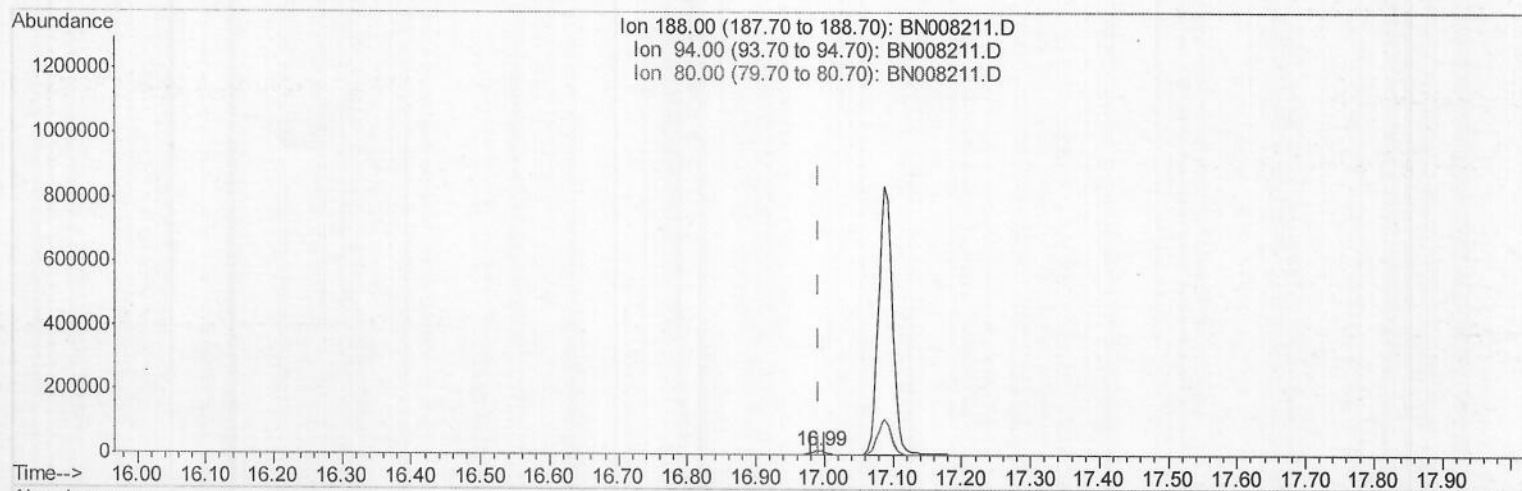

TIC: BN008211.D

(10) Phenanthrene-d10 (I)

16.992min (+0.000) 0.40ng/ul m JU 10/19/19

response 17654

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	11.30
80.00	12.60	13.21
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101619\
Quantitation Report (QT Reviewed)

Data File : BN008211.D
Acq On : 16 Oct 2019 22:44
Operator : JU
Sample : PB123769BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Oct 17 03:02:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 17 01:48:53 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	2744	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	13157	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	8270	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188	17654m	0.40	ng/ul	0.00
16) Chrysene-d12	21.20	240	13326	0.40	ng/ul	0.00
20) Perylene-d12	23.38	264	11939	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	5728	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.03	212	15360	0.25	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 10/19/19