

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101623\
 Data File : BN028293.D
 Acq On : 16 Oct 2023 16:49
 Operator : MA/JU
 Sample : PB156405BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK405

Quant Time: Oct 17 02:10:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 16 16:16:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	2282	0.400	ng/ul	0.00
4) Naphthalene-d8	10.697	136	7866	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.536	164	4874	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.295	188	10980	0.400	ng/ul	0.00
17) Chrysene-d12	21.507	240	10017	0.400	ng/ul	0.00
23) Perylene-d12	23.953	264	12093	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	18362	6.406	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.313	152	3918	0.309	ng/ul	0.01
18) Fluoranthene-d10	19.329	212	10146	0.319	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.531	166	1374	0.070	ng/ul#	16
20) Pyrene	19.696	202	1746	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.787	252	3659	0.096	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101623\
Data File : BN028293.D
Acq On : 16 Oct 2023 16:49
Operator : MA/JU
Sample : PB156405BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK405

Quant Time: Oct 17 02:10:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 16:16:04 2023
Response via : Initial Calibration




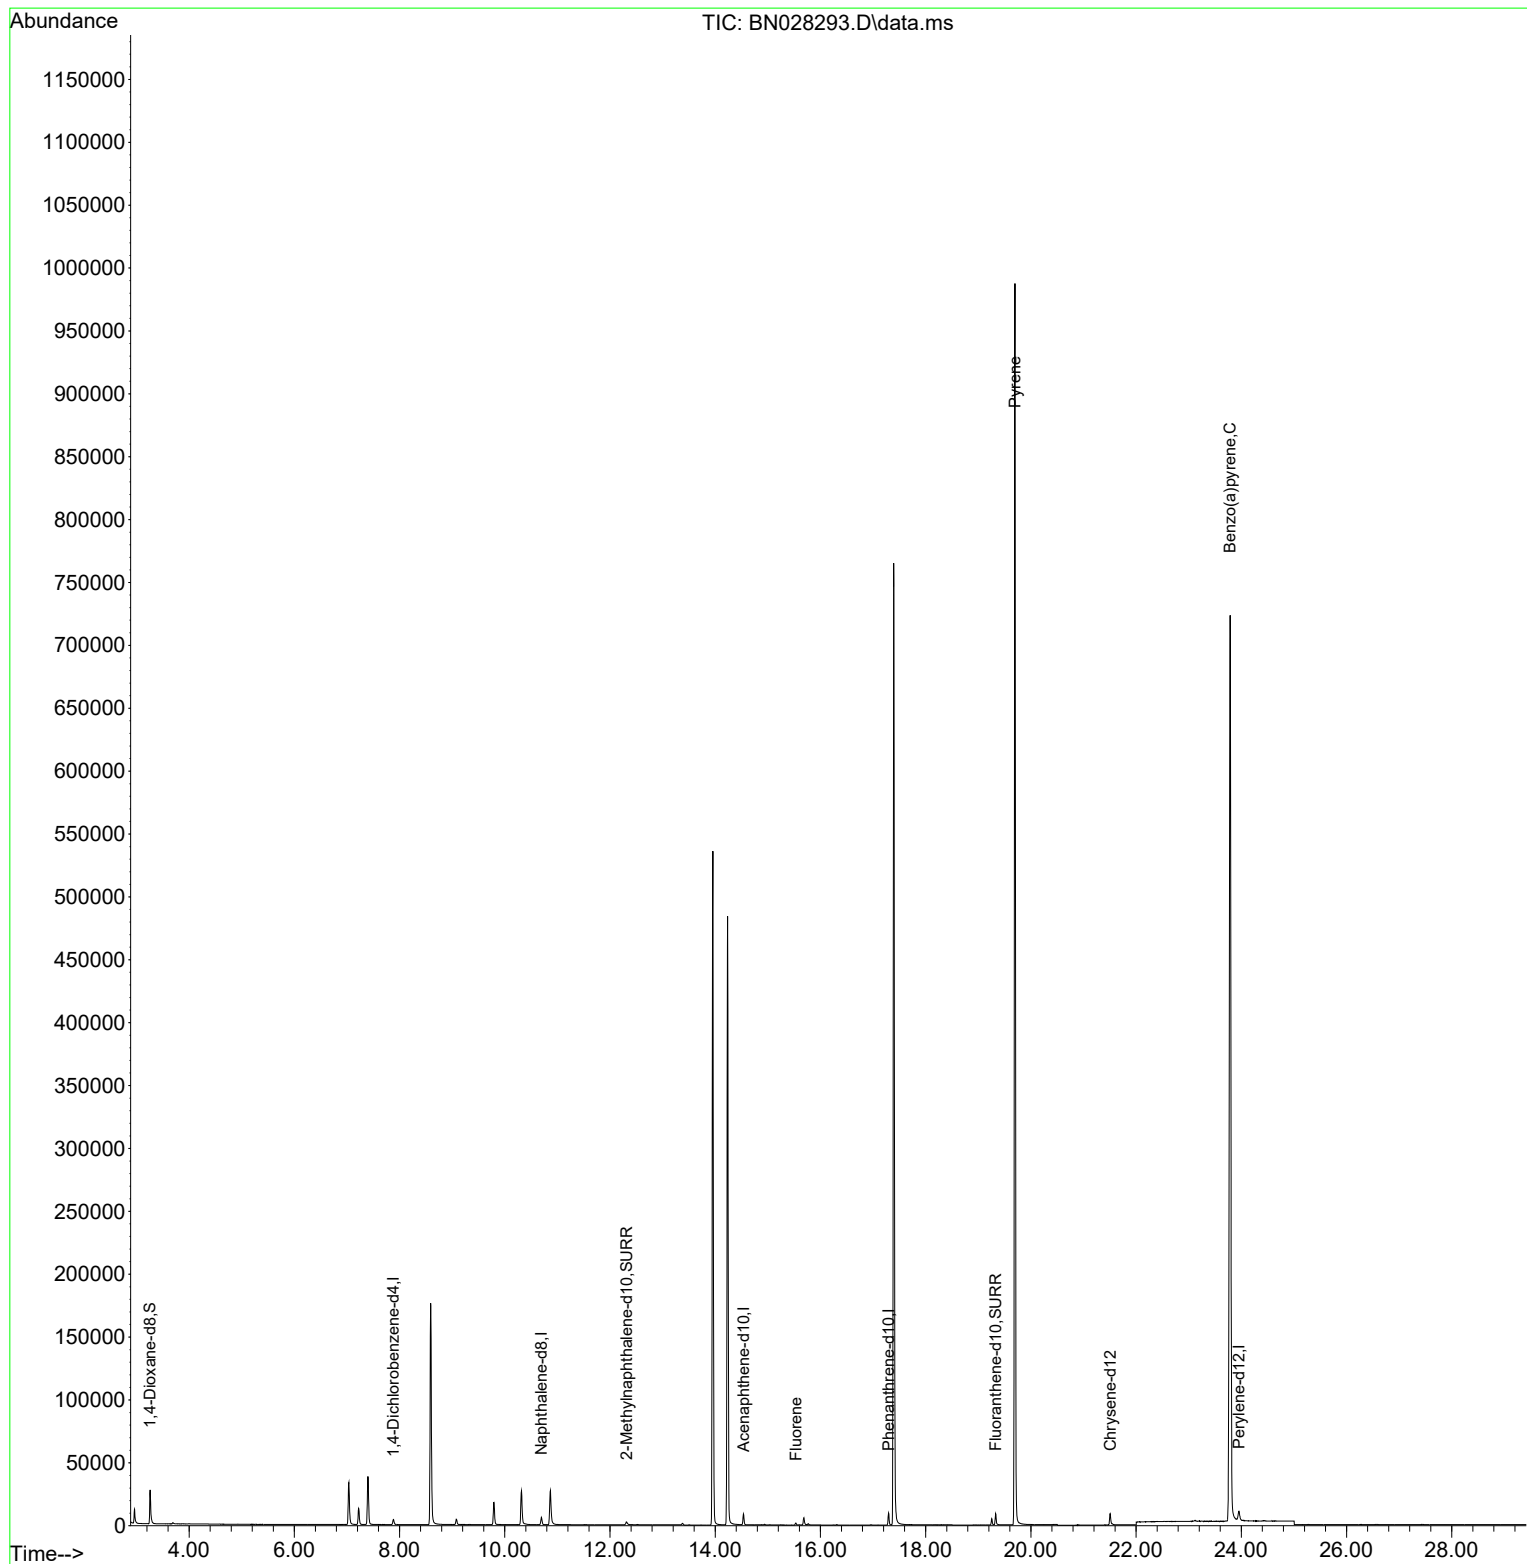


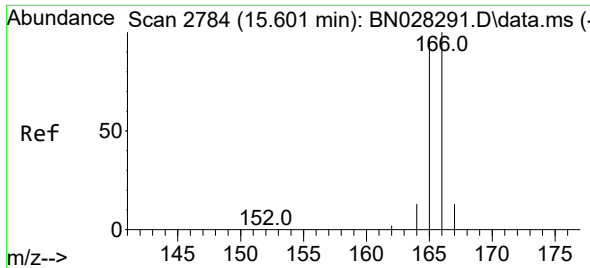

#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.531 min Scan# 21
Delta R.T. -0.069 min
Lab File: BN028293.D
Acq: 16 Oct 2023 16:49




Instrument :
BNA_N
ClientSampleId :
SBLK405


Tgt Ion:166 Resp: 1374
Ion Ratio Lower Upper
166 100
165 10.9 78.5 117.7#
167 35.7 11.2 16.8#

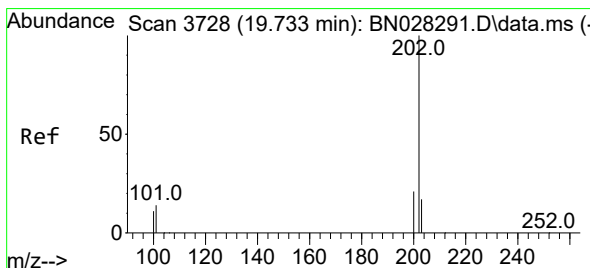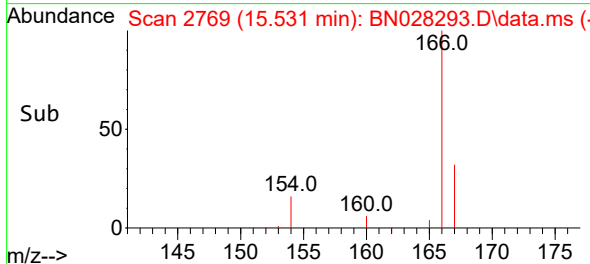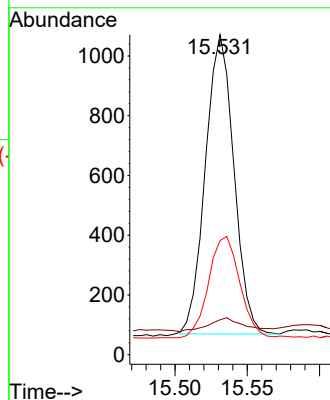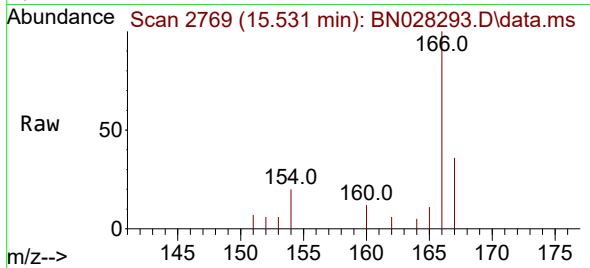

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.696 min Scan# 3720
Delta R.T. -0.037 min
Lab File: BN028293.D
Acq: 16 Oct 2023 16:49


Tgt Ion:202 Resp: 1746
Ion Ratio Lower Upper
202 100
101 170.9 11.2 16.8#
100 1226.7 9.1 13.7#

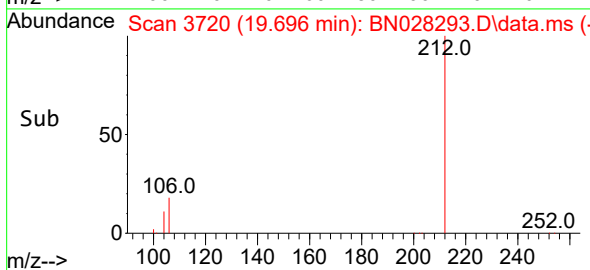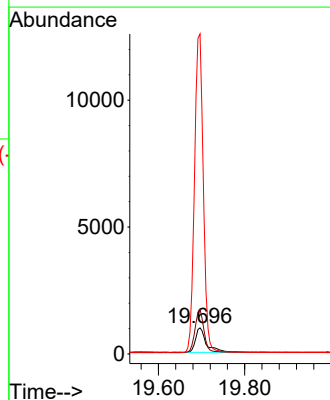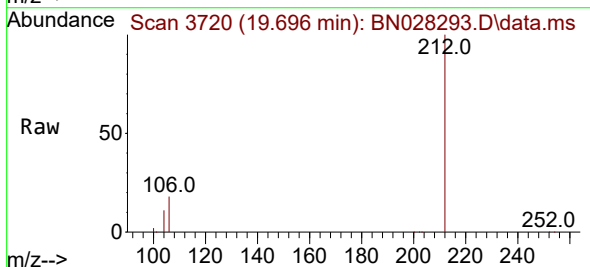

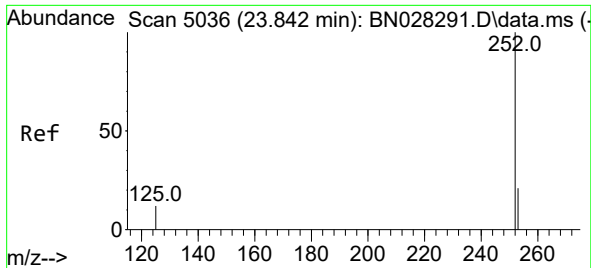

#26
Benzo(a)pyrene
Concen: 0.096 ng/ul
RT: 23.787 min Scan# 50
Delta R.T. -0.056 min
Lab File: BN028293.D
Acq: 16 Oct 2023 16:49

Instrument :
BNA_N
ClientSampleId :
SBLK405

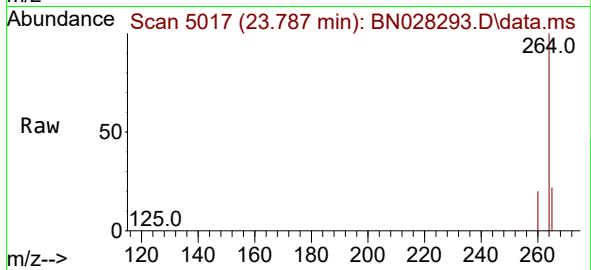

Tgt Ion:252 Resp: 3659
Ion Ratio Lower Upper
252 100
253 52.6 23.4 35.2#
125 44.2 15.3 22.9#

