

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101623\
 Data File : BN028296.D
 Acq On : 16 Oct 2023 18:39
 Operator : MA/JU
 Sample : 04900-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AT3

Quant Time: Oct 17 02:10:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 16 16:16:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.886	152	2121	0.400	ng/ul	0.00
4) Naphthalene-d8	10.696	136	7221	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.536	164	4501	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.295	188	10289	0.400	ng/ul	0.00
17) Chrysene-d12	21.498	240	9736	0.400	ng/ul	0.00
23) Perylene-d12	23.945	264	11753	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.262	96	10801	4.054	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.308	152	4382	0.377	ng/ul	0.00
18) Fluoranthene-d10	19.329	212	12077	0.391	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.300	88	412	0.146	ng/ul#	73
20) Pyrene	19.696	202	1951	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.781	252	4245	0.114	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101623\
Data File : BN028296.D
Acq On : 16 Oct 2023 18:39
Operator : MA/JU
Sample : 04900-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT3

Quant Time: Oct 17 02:10:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN100323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 16:16:04 2023
Response via : Initial Calibration




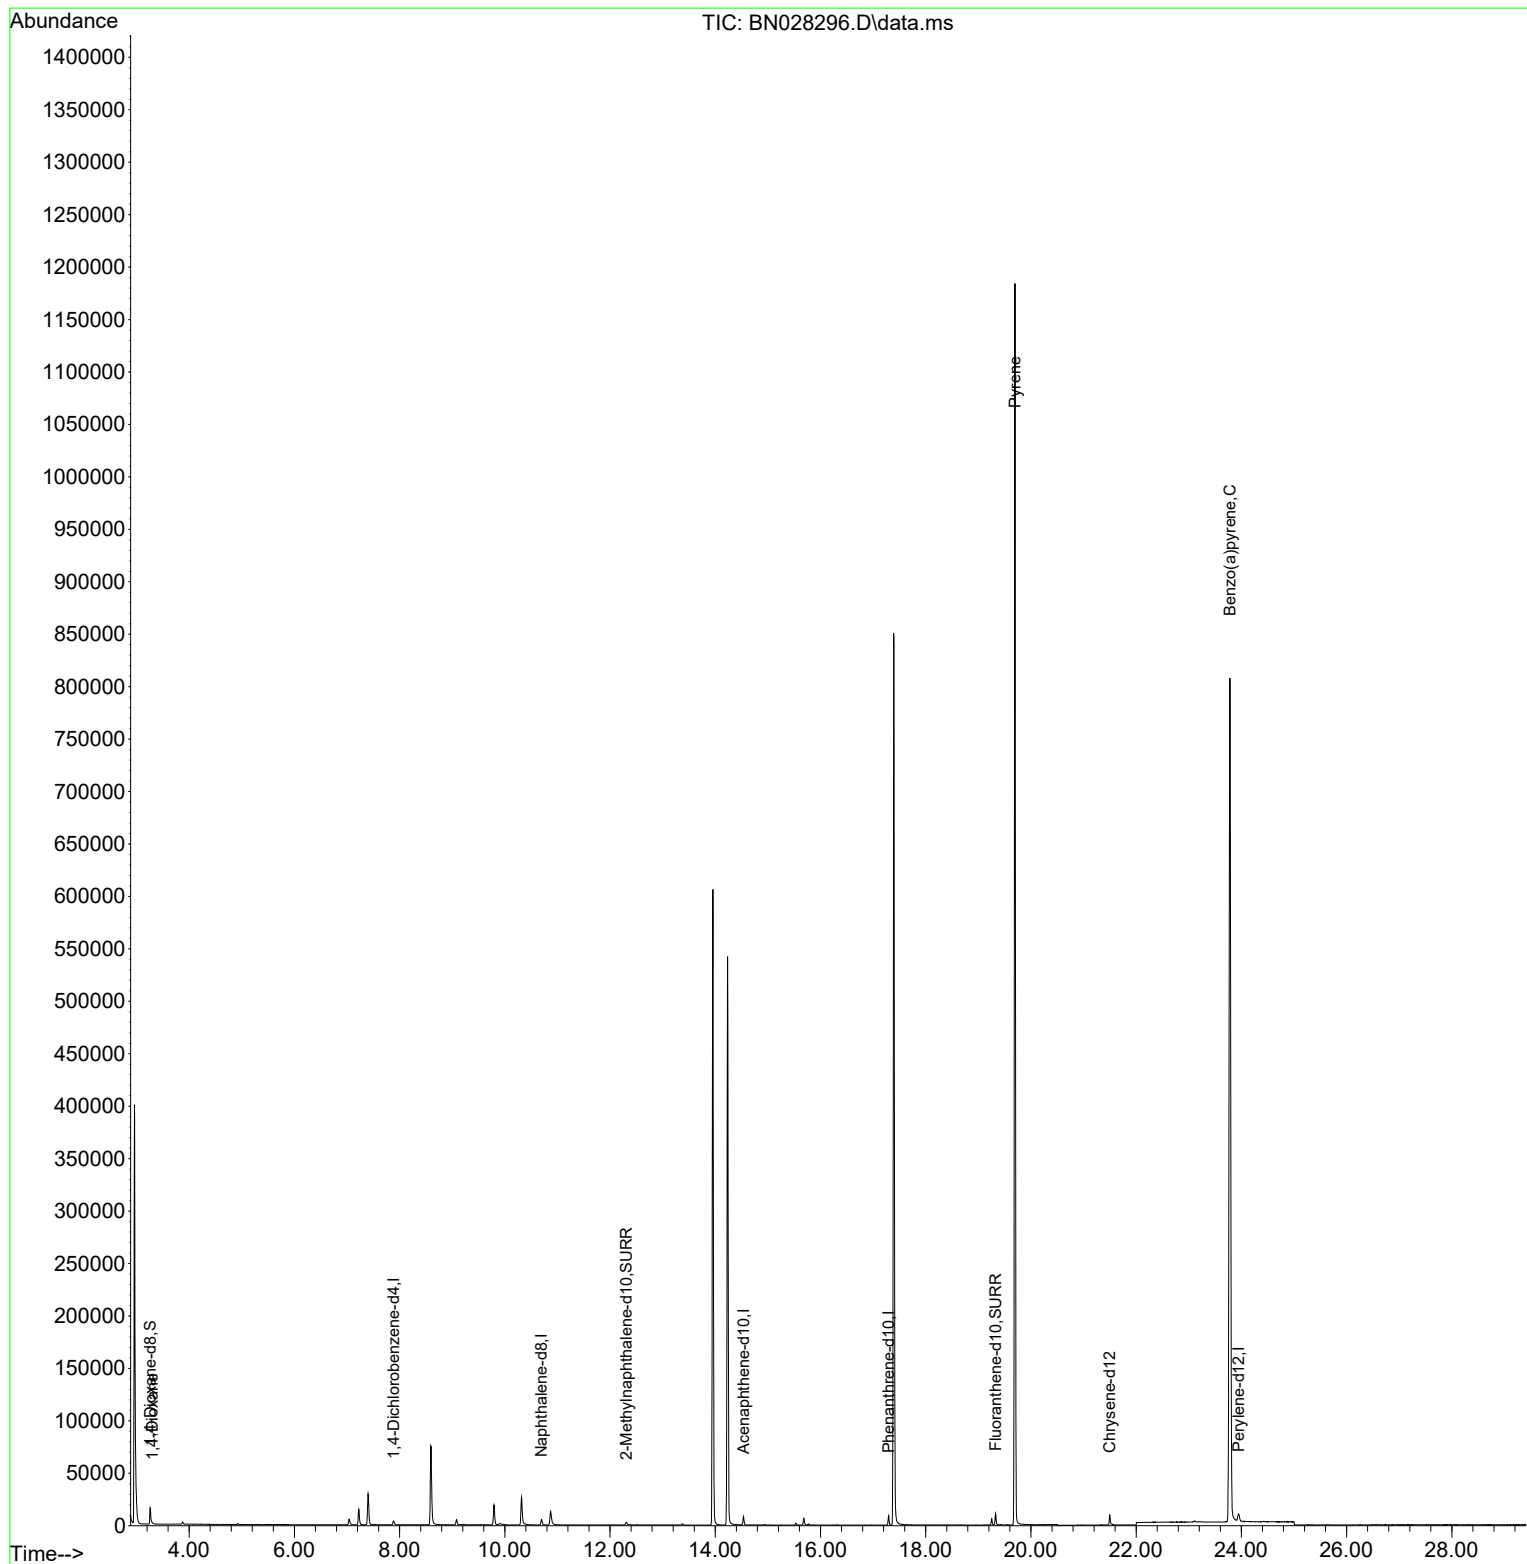


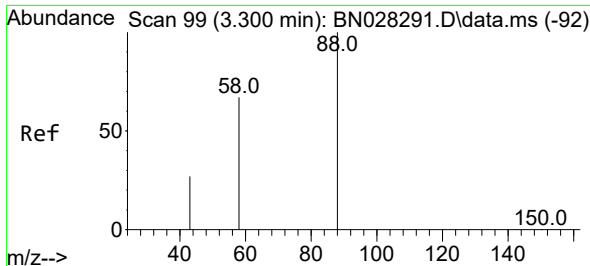

#2
1,4-Dioxane
Concen: 0.146 ng/ul
RT: 3.300 min Scan# 99
Delta R.T. -0.000 min
Lab File: BN028296.D
Acq: 16 Oct 2023 18:39




Instrument :
BNA_N
ClientSampleId :
COAT3


Tgt Ion: 88 Resp: 412
Ion Ratio Lower Upper
88 100
43 72.2 33.4 50.2#
58 48.7 45.7 68.5

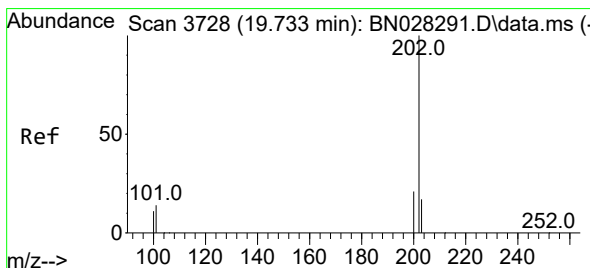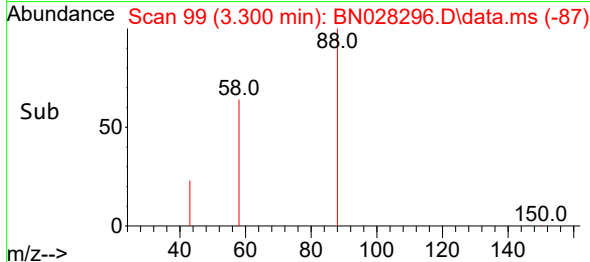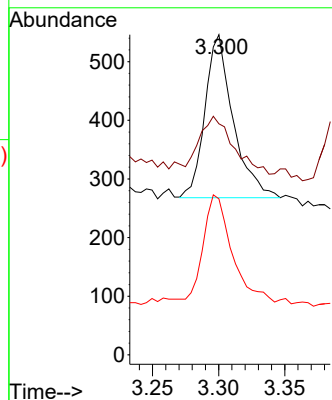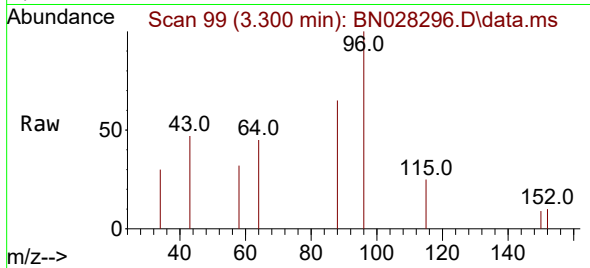

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.696 min Scan# 3720
Delta R.T. -0.037 min
Lab File: BN028296.D
Acq: 16 Oct 2023 18:39


Tgt Ion: 202 Resp: 1951
Ion Ratio Lower Upper
202 100
101 170.2 11.2 16.8#
100 1220.1 9.1 13.7#

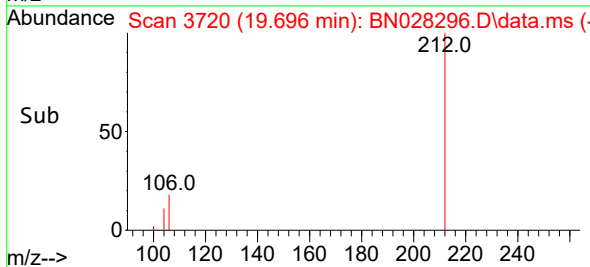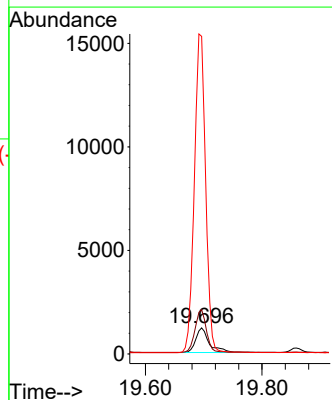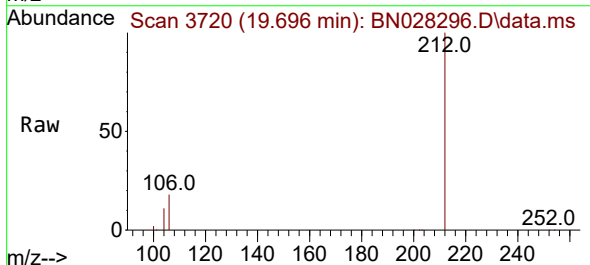

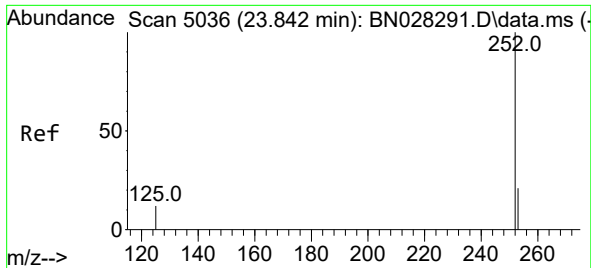

#26
 Benzo(a)pyrene
 Concen: 0.114 ng/ul
 RT: 23.781 min Scan# 50
 Delta R.T. -0.061 min
 Lab File: BN028296.D
 Acq: 16 Oct 2023 18:39

Instrument :
 BNA_N
 ClientSampleId :
 C0AT3

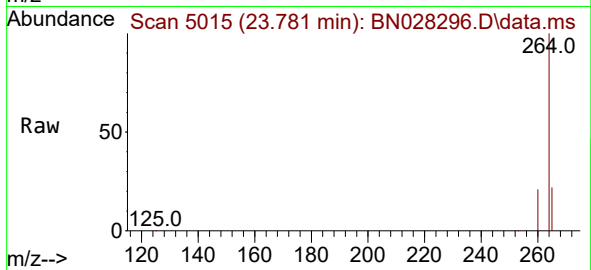

Tgt Ion:252 Resp: 4245
 Ion Ratio Lower Upper
 252 100
 253 51.9 23.4 35.2#
 125 41.6 15.3 22.9#

