


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101718\
 Data File : BN003180.D
 Acq On : 17 Oct 2018 14:40
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 15:26:23 2018

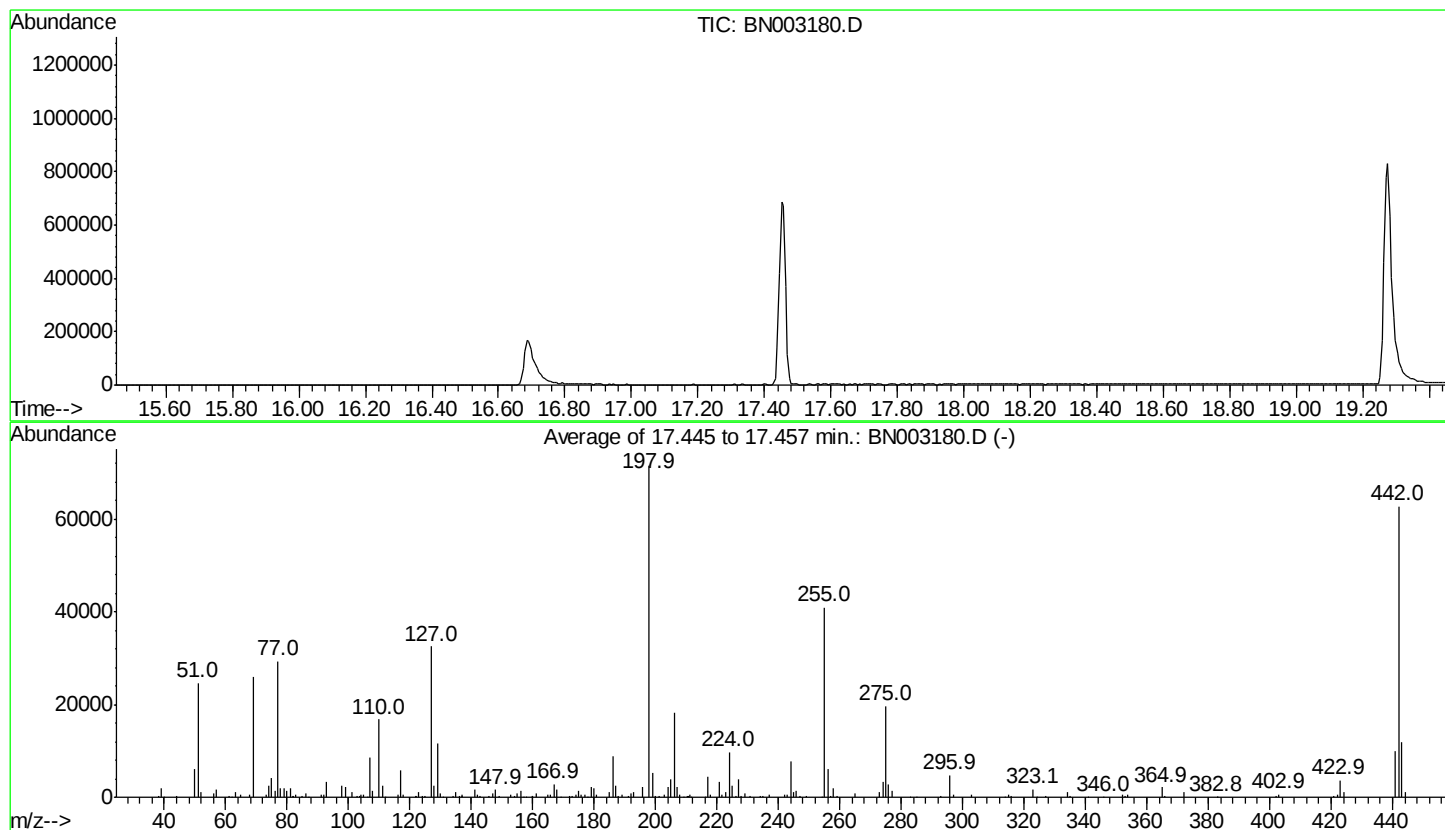

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	24637	PASS
68	69	0.00	2	1.8	456	PASS
69	198	0.00	100	36.2	25904	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.5	32506	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71472	PASS
199	198	5	9	7.4	5303	PASS
275	198	10	60	27.5	19623	PASS
365	198	1	100	3.1	2183	PASS
441	198	0.01	100	13.7	9811	PASS
442	198	50	100	87.8	62736	PASS
443	442	15	24	18.9	11835	PASS