

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101719\
 Data File : BN008240.D
 Acq On : 18 Oct 2019 02:33
 Operator : JU
 Sample : K5177-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 18 04:07:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 17 01:48:53 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	2947	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	14328	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	8926	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.99
16) Chrysene-d12	21.19	240	14530	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	12464	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	6073	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	16402	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.39	202	2222	0.038	ng/ul#	1
23) Benzo(a)pyrene	23.23	252	3129	0.073	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101719\
Data File : BN008240.D
Acq On : 18 Oct 2019 02:33
Operator : JU
Sample : K5177-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 18 04:07:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 17 01:48:53 2019
Response via : Initial Calibration

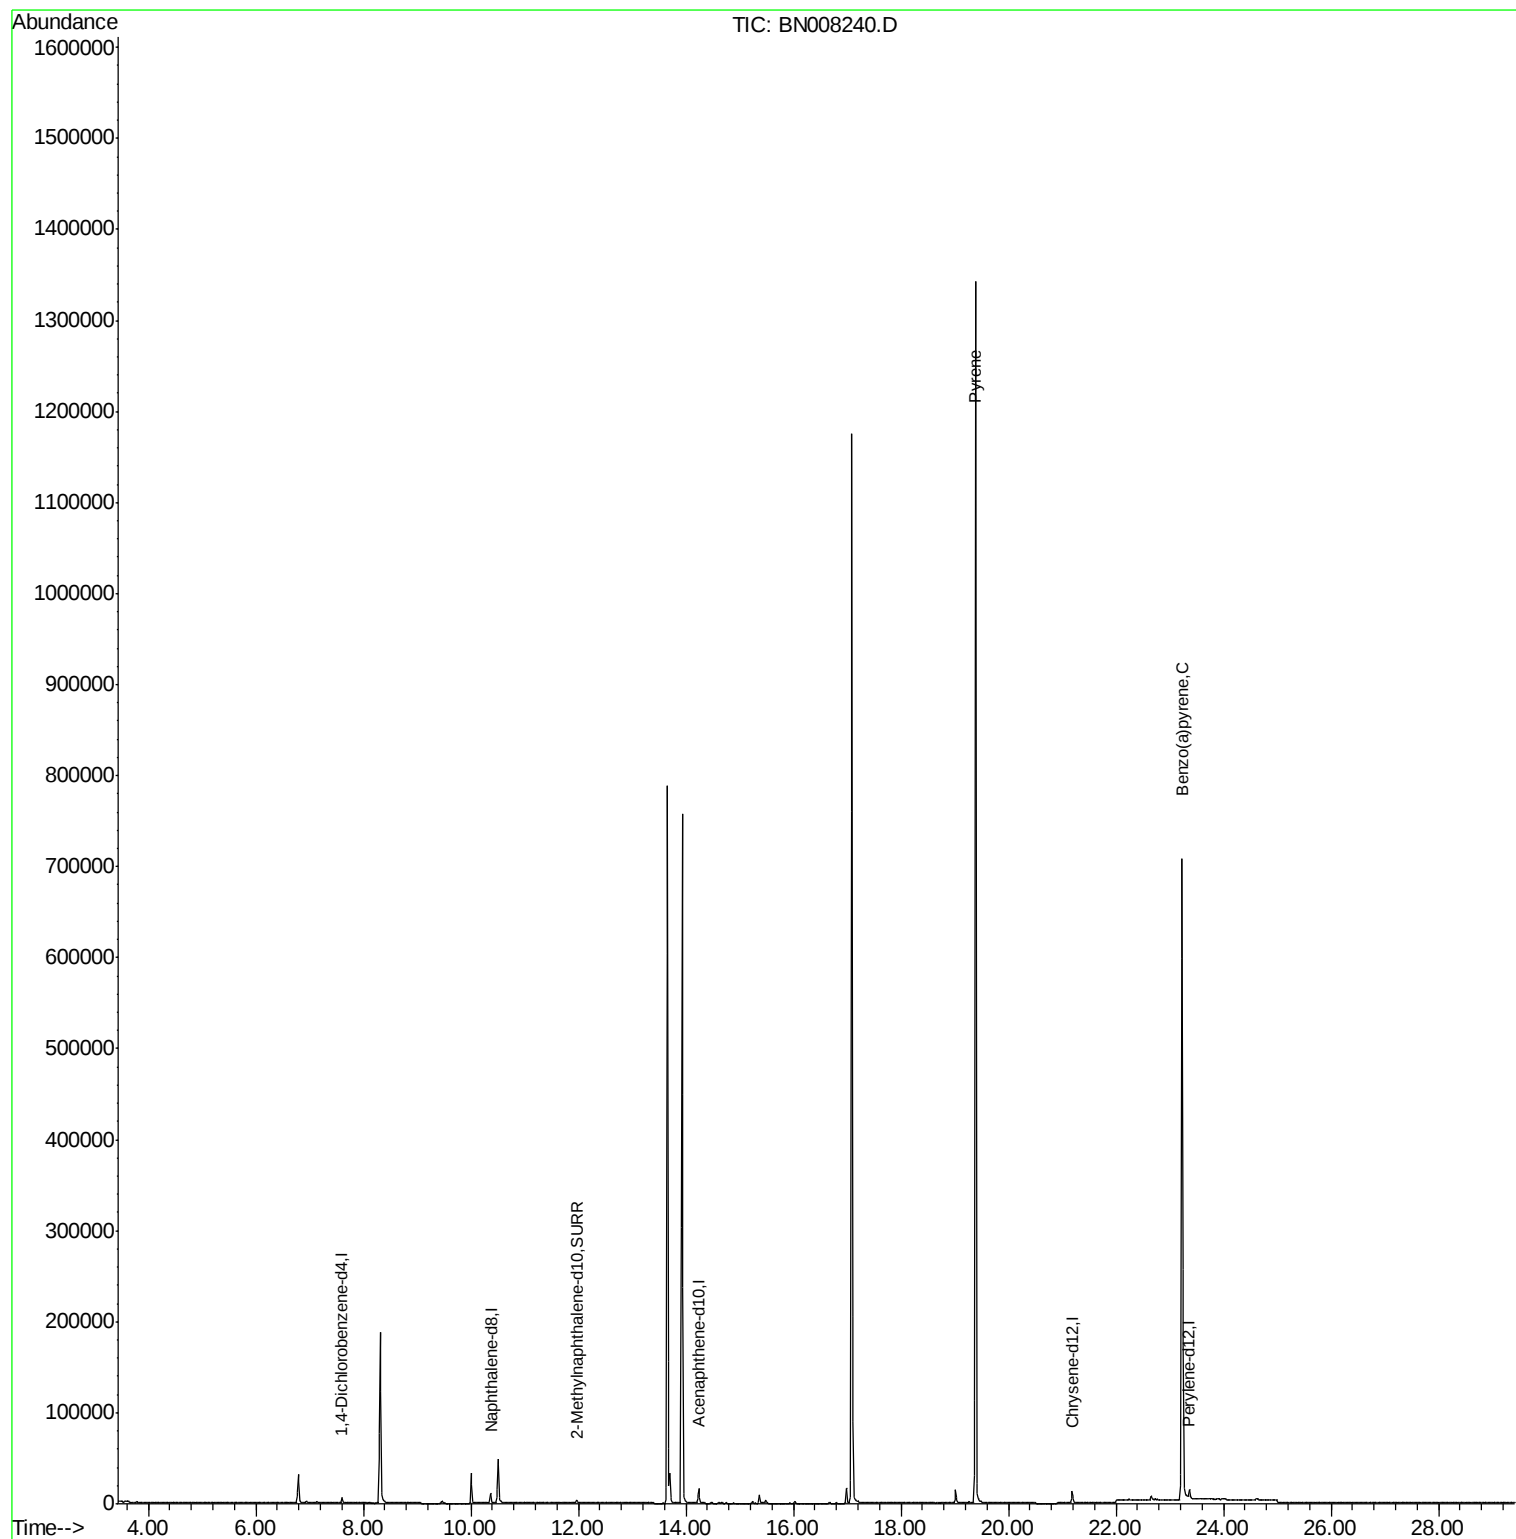

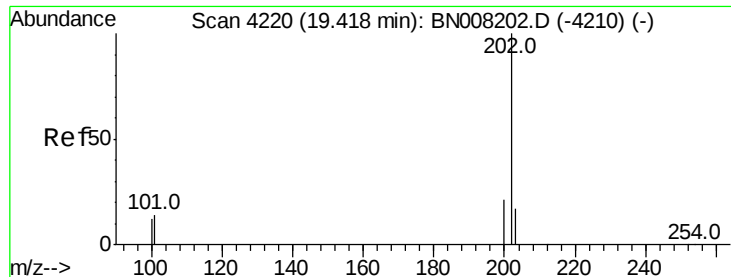

#17

Pvrene

Concen: 0.038 ng/ul

RT: 19.39 min Scan# 4213

Delta R.T. -0.03 min

Lab File: BN008240.D

Acq: 18 Oct 2019 02:33





Instrument :

BNA_N

ClientSampleId :

Tot Ion:202 Resp: 2222

Ion	Ratio	Lower	Upper
202	100		
101	156.2	10.9	16.3#
100	1064.4	8.7	13.1#

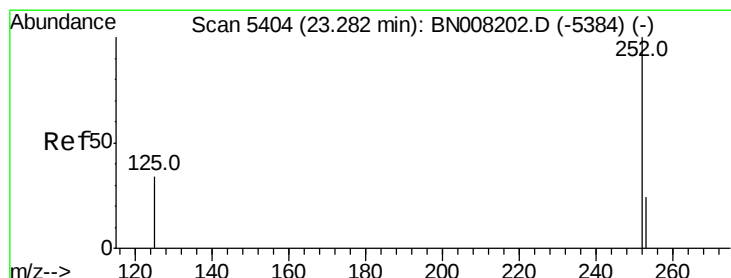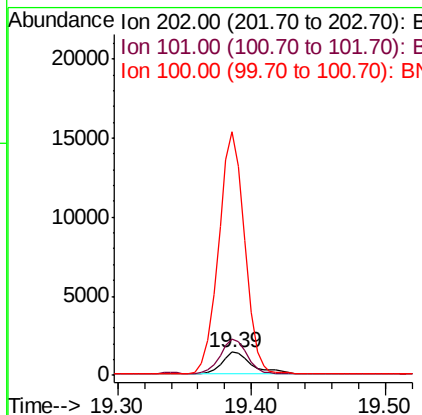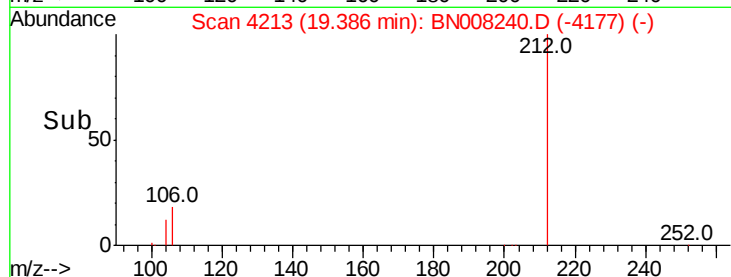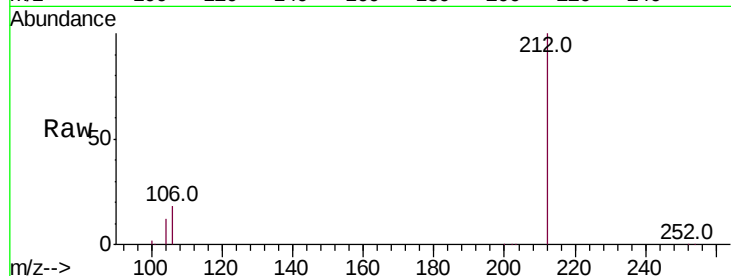

#23

Benzo(a)pyrene

Concen: 0.073 ng/ul

RT: 23.23 min Scan# 5386

Delta R.T. -0.05 min

Lab File: BN008240.D

Acq: 18 Oct 2019 02:33

Tgt Ion:252 Resp: 3129

Ion	Ratio	Lower	Upper
252	100		
253	48.6	22.8	34.2#
125	49.6	18.4	27.6#

