


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101719\
Data File : BN008240.D
Acq On : 18 Oct 2019 02:33
Operator : JU
Sample : K5177-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 18 04:11:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 17 01:48:53 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
BEPA1

Manual Integrations
APPROVED

mohammad
10/20/2019 8:09:55 PM

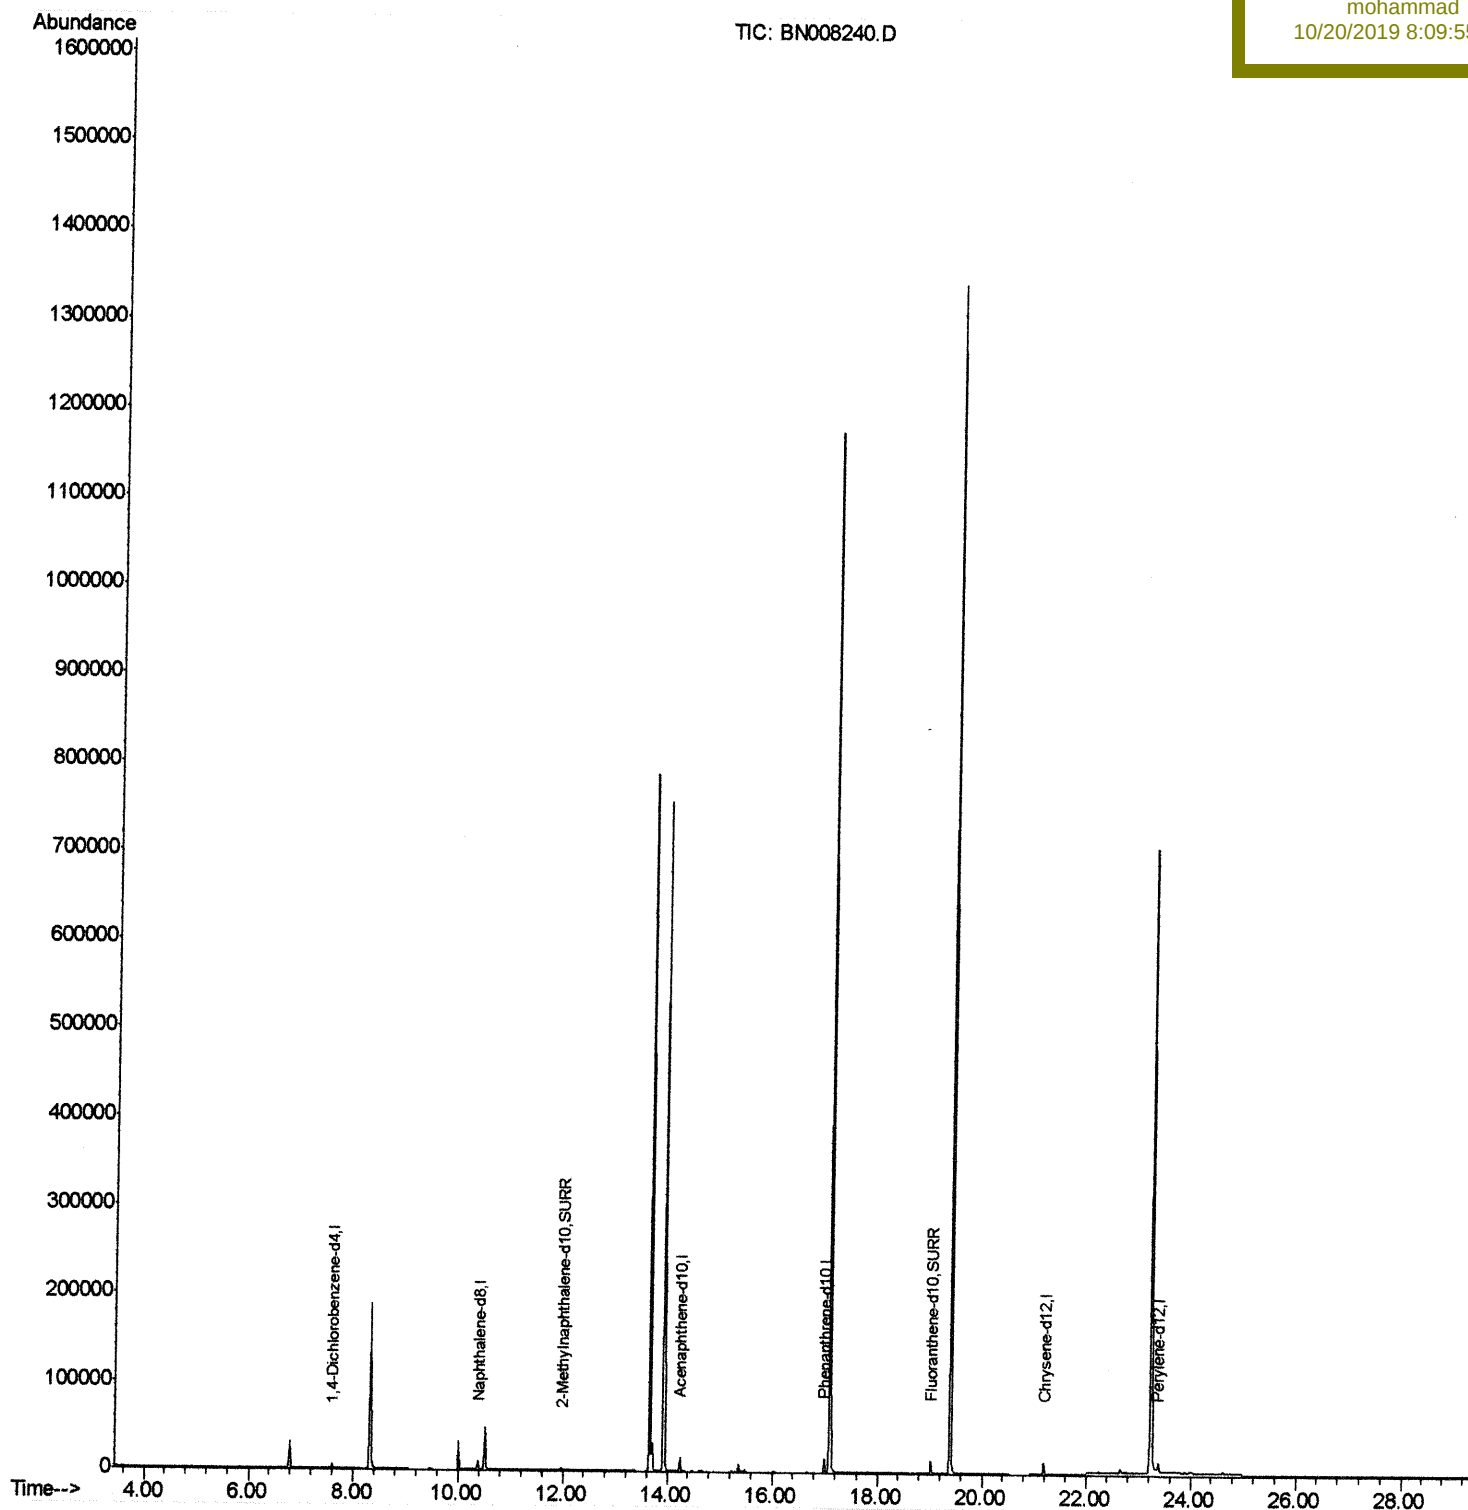


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101719\
Data File : BN008240.D
Acq On : 18 Oct 2019 02:33
Operator : JU
Sample : K5177-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 18 04:07:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 17 01:48:53 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
BEPA1

Manual Integrations
APPROVED

mohammad
10/20/2019 8:09:55 PM

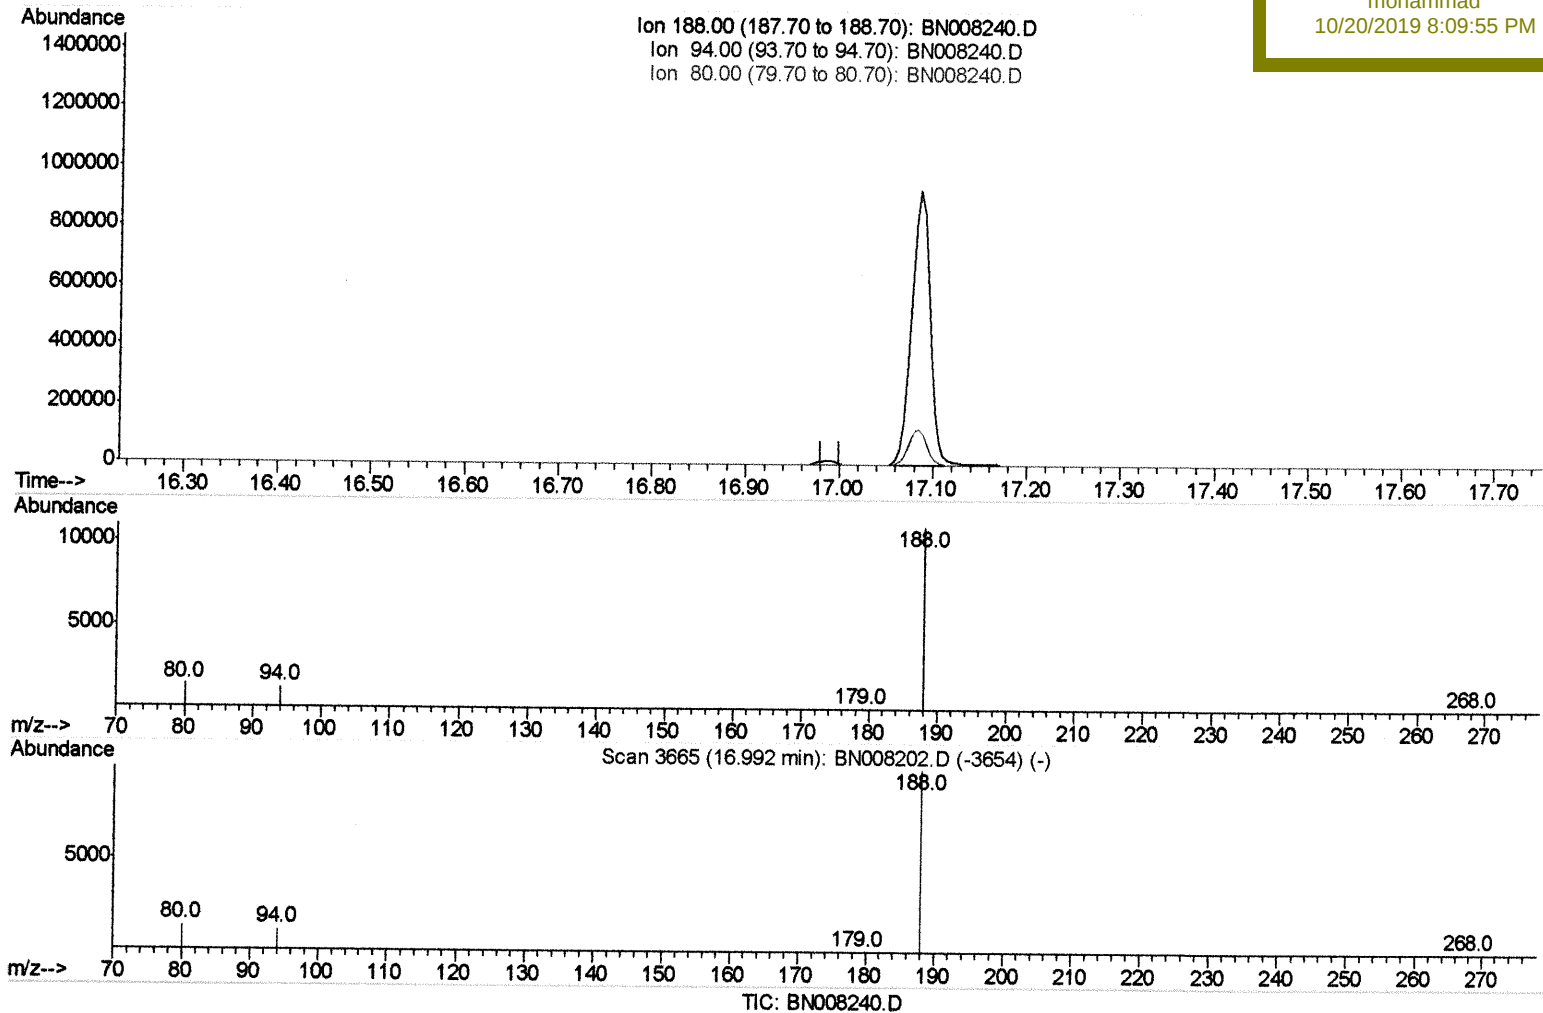

(10) Phenanthrene-d10 (I)

16.992min (-16.992) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.90	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101719\
 Data File : BN008240.D
 Acq On : 18 Oct 2019 02:33
 Operator : JU
 Sample : K5177-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BEPA1

Manual Integrations
 APPROVED

mohammad
 10/20/2019 8:09:55 PM

Quant Time: Oct 18 04:07:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 17 01:48:53 2019
 Response via : Initial Calibration

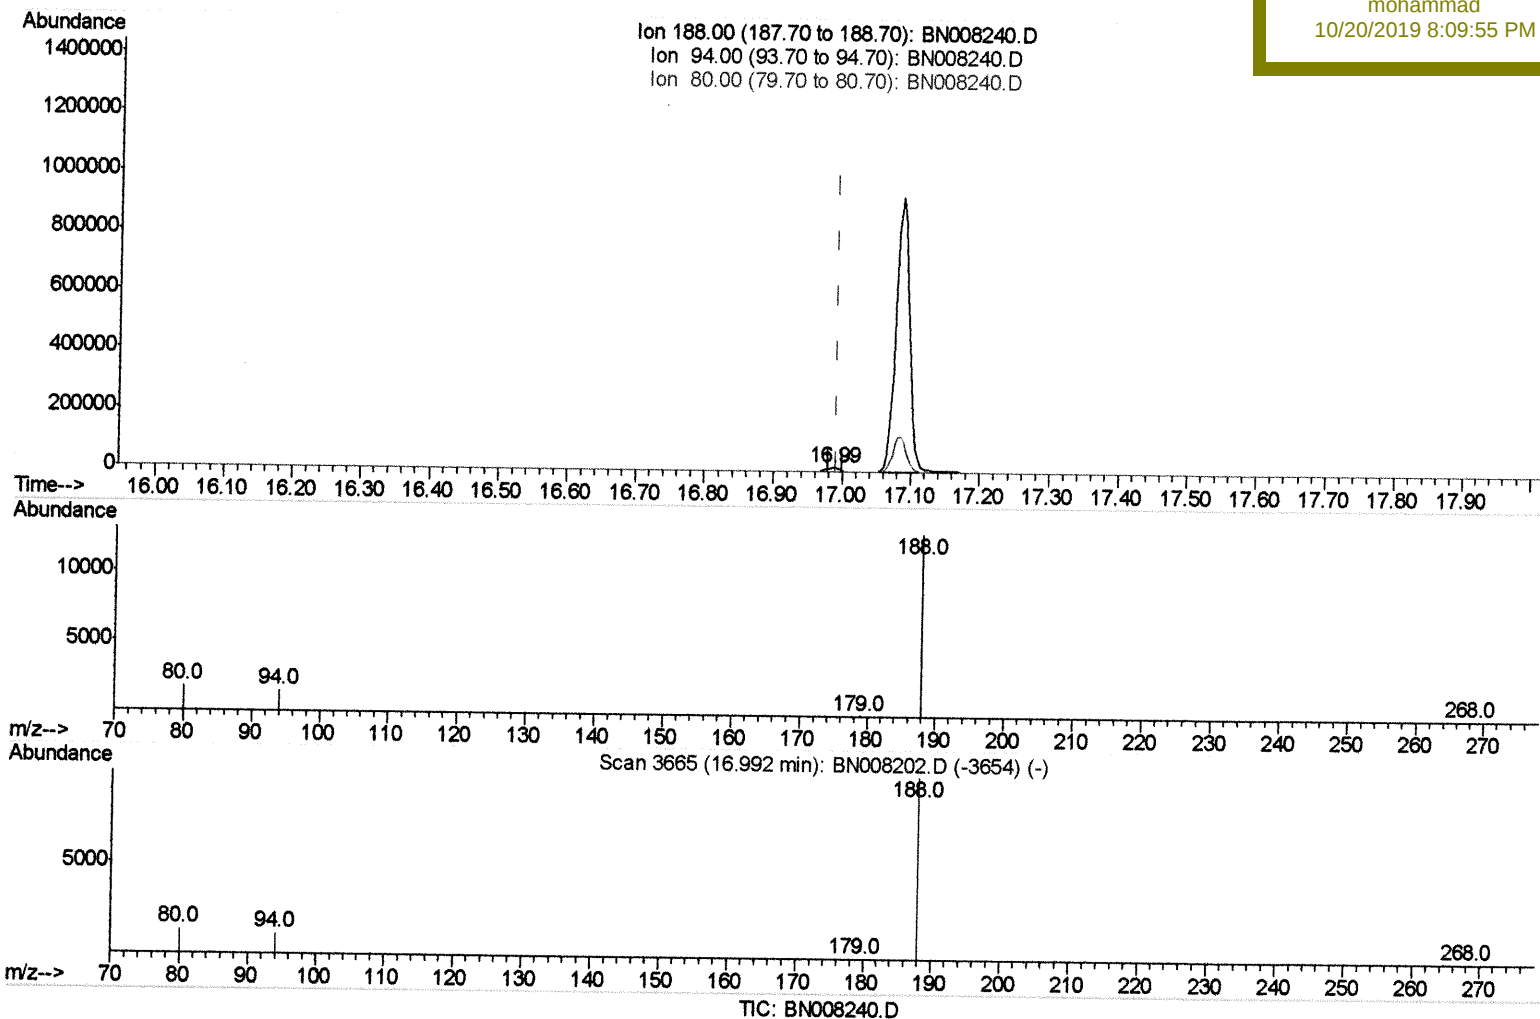

(10) Phenanthrene-d10 (I)

16.988min (-0.004) 0.40ng/ul m

response 19221

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	11.33
80.00	12.60	13.67
0.00	0.00	0.00

JUC 10/21/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101719\
 Data File : BN008240.D
 Acq On : 18 Oct 2019 02:33
 Operator : JU
 Sample : K5177-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BEPA1

Quant Time: Oct 18 04:11:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 17 01:48:53 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 10/20/2019 8:09:55 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	2947	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	14328	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	8926	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.99	188	19221m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	14530	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	12464	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.97	152	6073	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	16402	0.25	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 10/21/19