

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101725\
 Data File : BN038097.D
 Acq On : 17 Oct 2025 15:57
 Operator : RC/JU
 Sample : PB169495BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK495

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101725.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN038097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	31	rVB	81394	110216	1.71%	0.157%
2	3.640	90	94	116	rBV	1026975	1633835	25.42%	2.321%
3	3.969	145	150	159	rVB	38063	54934	0.85%	0.078%
4	4.599	255	257	261	rVB3	5759	8036	0.13%	0.011%
5	6.940	648	655	666	rBV	1242928	1910921	29.73%	2.715%
6	7.110	676	684	692	rBV	1024872	1559758	24.26%	2.216%
7	7.310	711	718	728	rBV	1262162	1980611	30.81%	2.814%
8	7.781	791	798	808	rVB	1036297	1612032	25.08%	2.290%
9	8.487	910	918	931	rBV	1541887	2402191	37.37%	3.413%
10	8.940	987	995	1003	rBV	1165478	1878905	29.23%	2.669%
11	9.057	1010	1015	1020	rVB5	7130	10799	0.17%	0.015%
12	9.663	1110	1118	1133	rBV	920578	1480471	23.03%	2.103%
13	10.204	1202	1210	1225	rBV	1415449	2375923	36.96%	3.376%
14	10.587	1267	1275	1285	rVB	1383544	2290508	35.63%	3.254%
15	10.716	1289	1297	1313	rBV	1205740	2179678	33.91%	3.097%
16	11.245	1381	1387	1389	rBV4	8771	14545	0.23%	0.021%
17	12.187	1541	1547	1552	rVB	25415	42663	0.66%	0.061%
18	13.428	1752	1758	1763	rBV	31735	47305	0.74%	0.067%
19	13.851	1824	1830	1845	rBV	2651320	3517991	54.73%	4.998%
20	14.133	1870	1878	1888	rBV	2963869	4279856	66.58%	6.081%
21	14.286	1896	1904	1911	rBV5	23505	68769	1.07%	0.098%
22	14.445	1923	1931	1941	rBV	2066693	3003507	46.72%	4.267%
23	14.522	1941	1944	1949	rVB7	7777	10739	0.17%	0.015%
24	14.633	1955	1963	1983	rBV	1135799	1773314	27.59%	2.519%
25	14.857	1996	2001	2006	rVB8	9472	17210	0.27%	0.024%
26	15.439	2093	2100	2108	rBV	3779037	5207476	81.01%	7.398%
27	15.551	2113	2119	2136	rVV	1054718	1414186	22.00%	2.009%
28	15.680	2136	2141	2146	rVV	16878	24857	0.39%	0.035%
29	16.222	2229	2233	2239	rBV6	3908	6521	0.10%	0.009%
30	16.980	2357	2362	2370	rVB5	9592	16871	0.26%	0.024%
31	17.192	2392	2398	2407	rBV2	2266039	3331412	51.82%	4.733%
32	17.292	2408	2415	2432	rVV	3975511	5499849	85.56%	7.814%
33	17.580	2455	2464	2468	rBV10	4580	14244	0.22%	0.020%
34	17.851	2506	2510	2511	rBV4	6014	6821	0.11%	0.010%
35	18.092	2548	2551	2559	rBV7	11315	16247	0.25%	0.023%
36	19.157	2727	2732	2738	rBV3	42928	62292	0.97%	0.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101725\
Data File : BN038097.D
Acq On : 17 Oct 2025 15:57
Operator : RC/JU
Sample : PB169495BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101725.MA.M
Title : SVOA CALIBRATION

37	19.227	2740	2744	2747	rVV2	42207	58474	0.91%	0.083%
38	19.292	2751	2755	2759	rVB	63772	73856	1.15%	0.105%
39	19.533	2792	2796	2800	rBV	134201	156196	2.43%	0.222%
40	19.592	2800	2806	2813	rVV	4644838	6199969	96.45%	8.809%
41	19.645	2813	2815	2824	rVB7	22640	38012	0.59%	0.054%
42	20.374	2936	2939	2943	rBV4	33409	36229	0.56%	0.051%
43	20.580	2970	2974	2979	rBV2	92941	108780	1.69%	0.155%
44	21.445	3115	3121	3134	rBV	2416965	3630458	56.48%	5.158%
45	24.292	3596	3605	3620	rBV	2581654	6428375	100.00%	9.133%
46	24.498	3632	3640	3650	rBV	1461579	3789854	58.96%	5.384%




Sum of corrected areas: 70385696

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101725\
Data File : BN038097.D
Acq On : 17 Oct 2025 15:57
Operator : RC/JU
Sample : PB169495BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101725.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

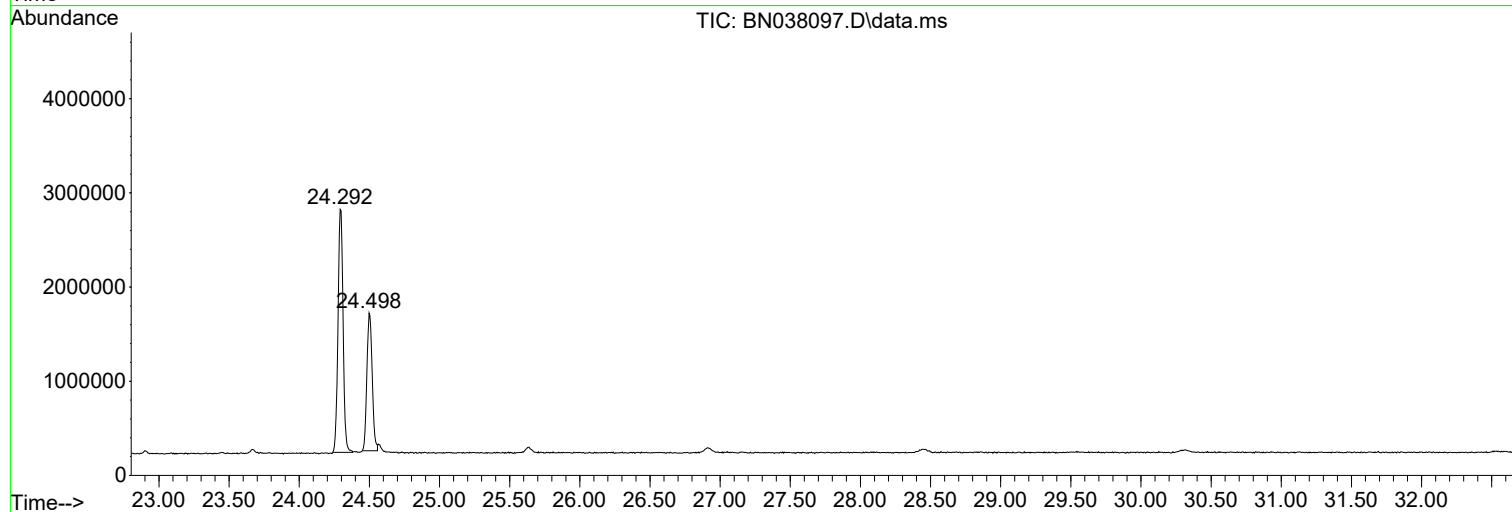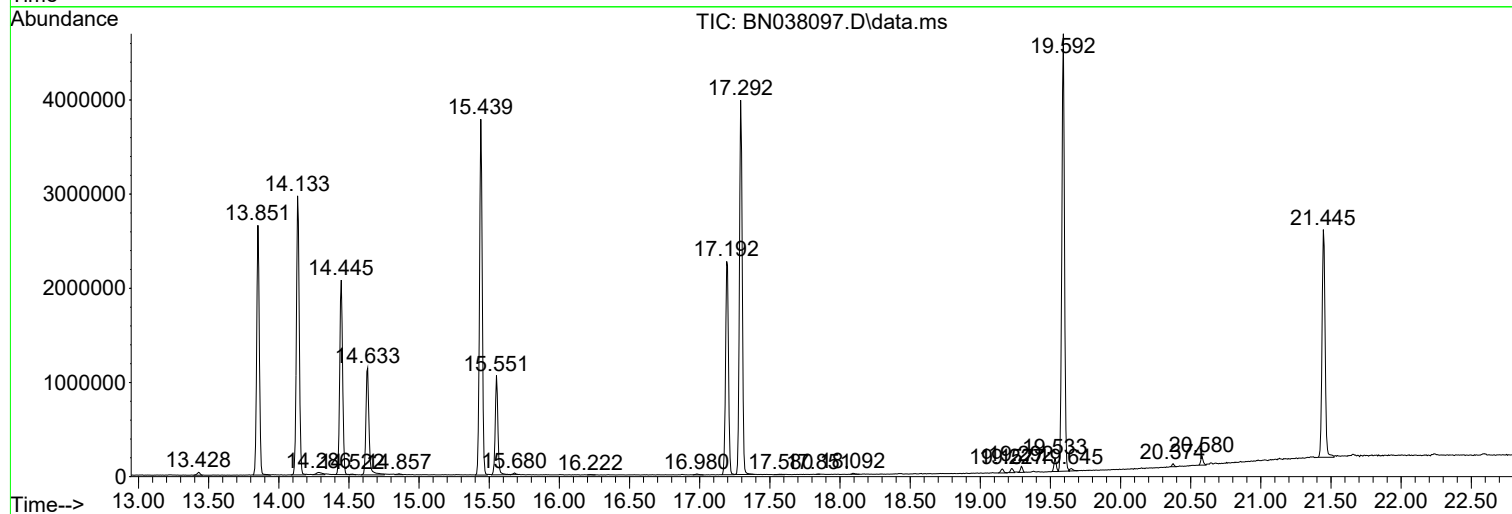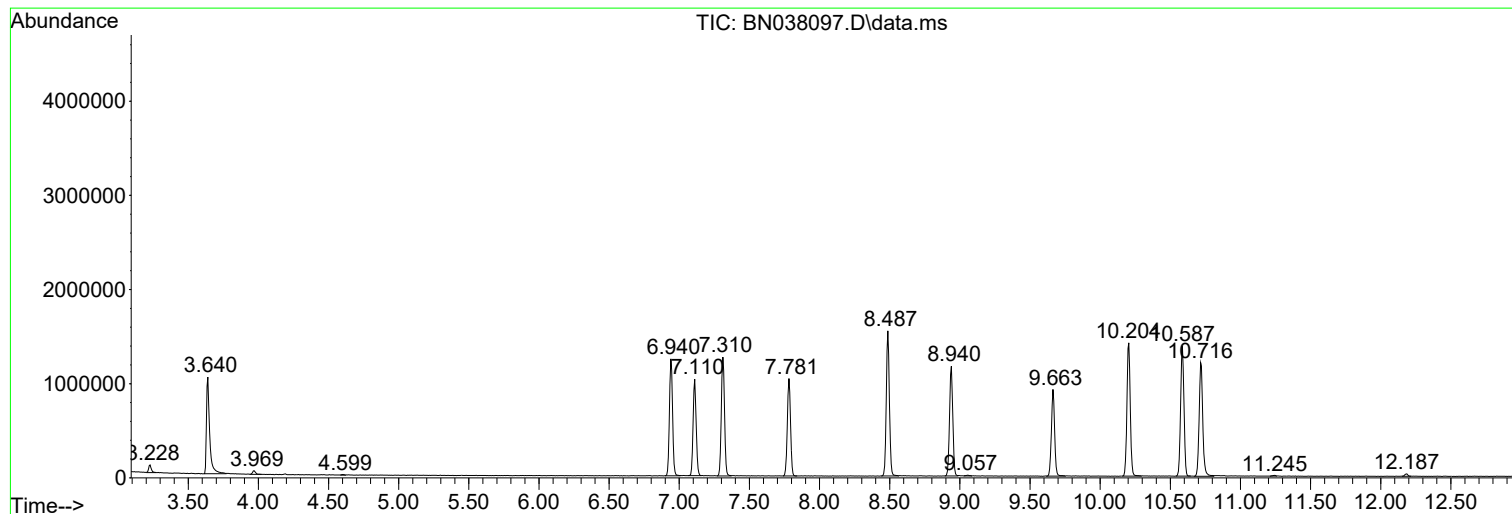

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101725\
Data File : BN038097.D
Acq On : 17 Oct 2025 15:57
Operator : RC/JU
Sample : PB169495BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101725.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101725\
Data File : BN038097.D
Acq On : 17 Oct 2025 15:57
Operator : RC/JU
Sample : PB169495BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101725.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc