


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101818\
 Data File : BN003197.D
 Acq On : 18 Oct 2018 08:44
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 15:26:23 2018

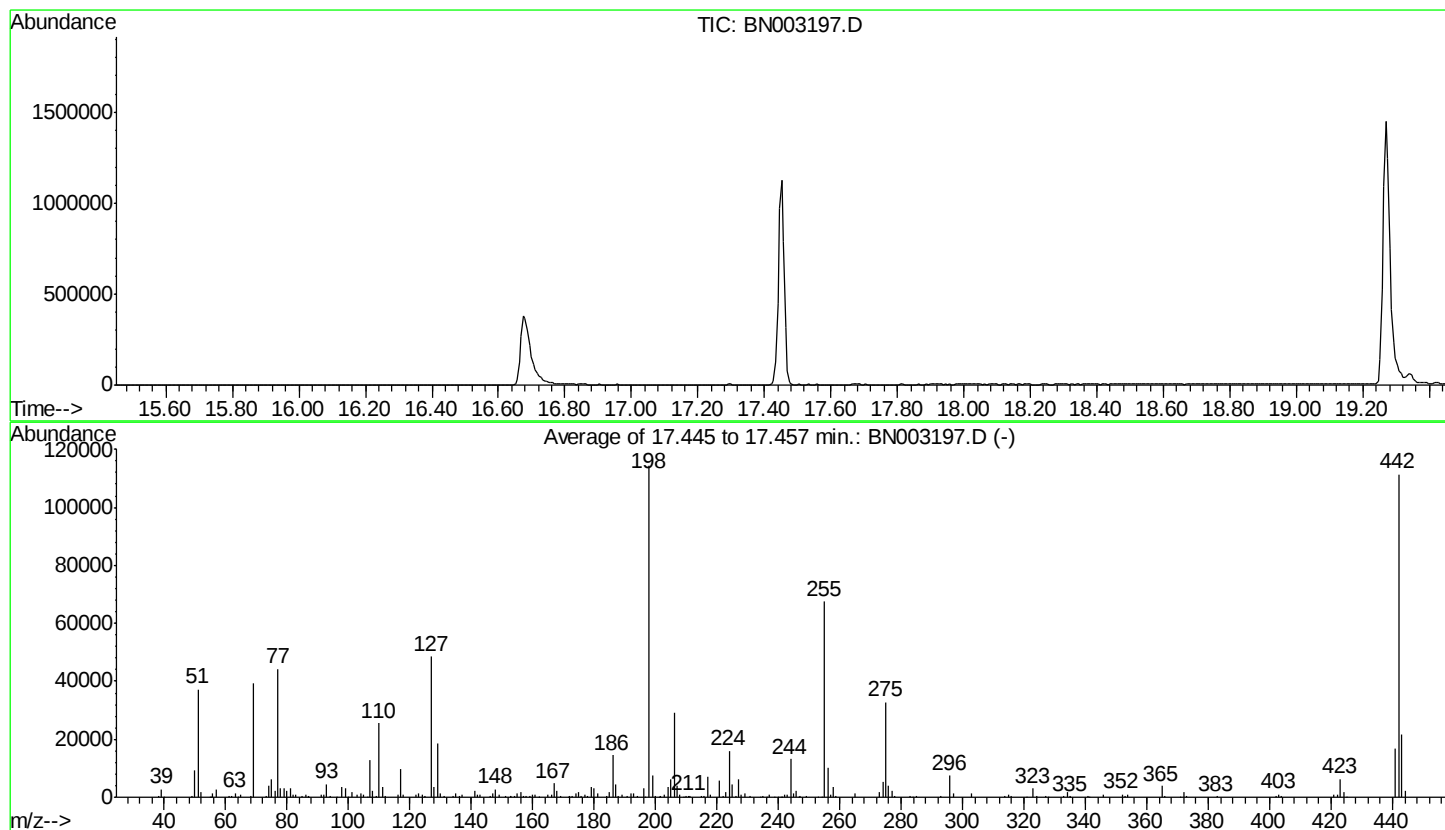

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	37096	PASS
68	69	0.00	2	1.6	637	PASS
69	198	0.00	100	34.4	39402	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	48525	PASS
197	198	0.00	2	0.2	231	PASS
198	198	100	100	100.0	114389	PASS
199	198	5	9	6.7	7656	PASS
275	198	10	60	28.6	32709	PASS
365	198	1	100	3.5	3951	PASS
441	198	0.01	100	14.9	16993	PASS
442	198	50	100	97.4	111442	PASS
443	442	15	24	19.3	21469	PASS