

Data File : BN008257.D
Acq On : 18 Oct 2019 20:58
Operator : JU
Sample : K5175-01RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BEPG7

Quant Time: Oct 18 23:50:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 23:47:17 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2250	0.40	ng/ul	0.00
2) Naphthalene-d8	10.36	136	10663	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.23	164	6501	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.98
16) Chrysene-d12	21.18	240	13463	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	12818	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	5139	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.01	212	14010	0.00	ng/ul	0.00
Target Compounds				Qvalue		
7) Acenaphthylene	13.94	152	668	0.022	ng/ul#	69
17) Pyrene	19.41	202	9974	0.186	ng/ul	97
18) Benzo(a)anthracene	21.17	228	4753	0.097	ng/ul	94
19) Chrysene	21.22	228	5062	0.084	ng/ul	95
21) Benzo(b)fluoranthene	22.71	252	8600	0.206	ng/ul#	71
22) Benzo(k)fluoranthene	22.71	252	8600	0.182	ng/ul#	70
23) Benzo(a)pyrene	23.26	252	4123	0.094	ng/ul#	72
24) Indeno(1,2,3-cd)pyrene	25.51	276	2428	0.047	ng/ul	92
26) Benzo(g,h,i)perylene	26.17	276	2295	0.048	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN008257.D
Acq On : 18 Oct 2019 20:58
Operator : JU
Sample : K5175-01RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BEPG7

Quant Time: Oct 18 23:50:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 23:47:17 2019
Response via : Initial Calibration

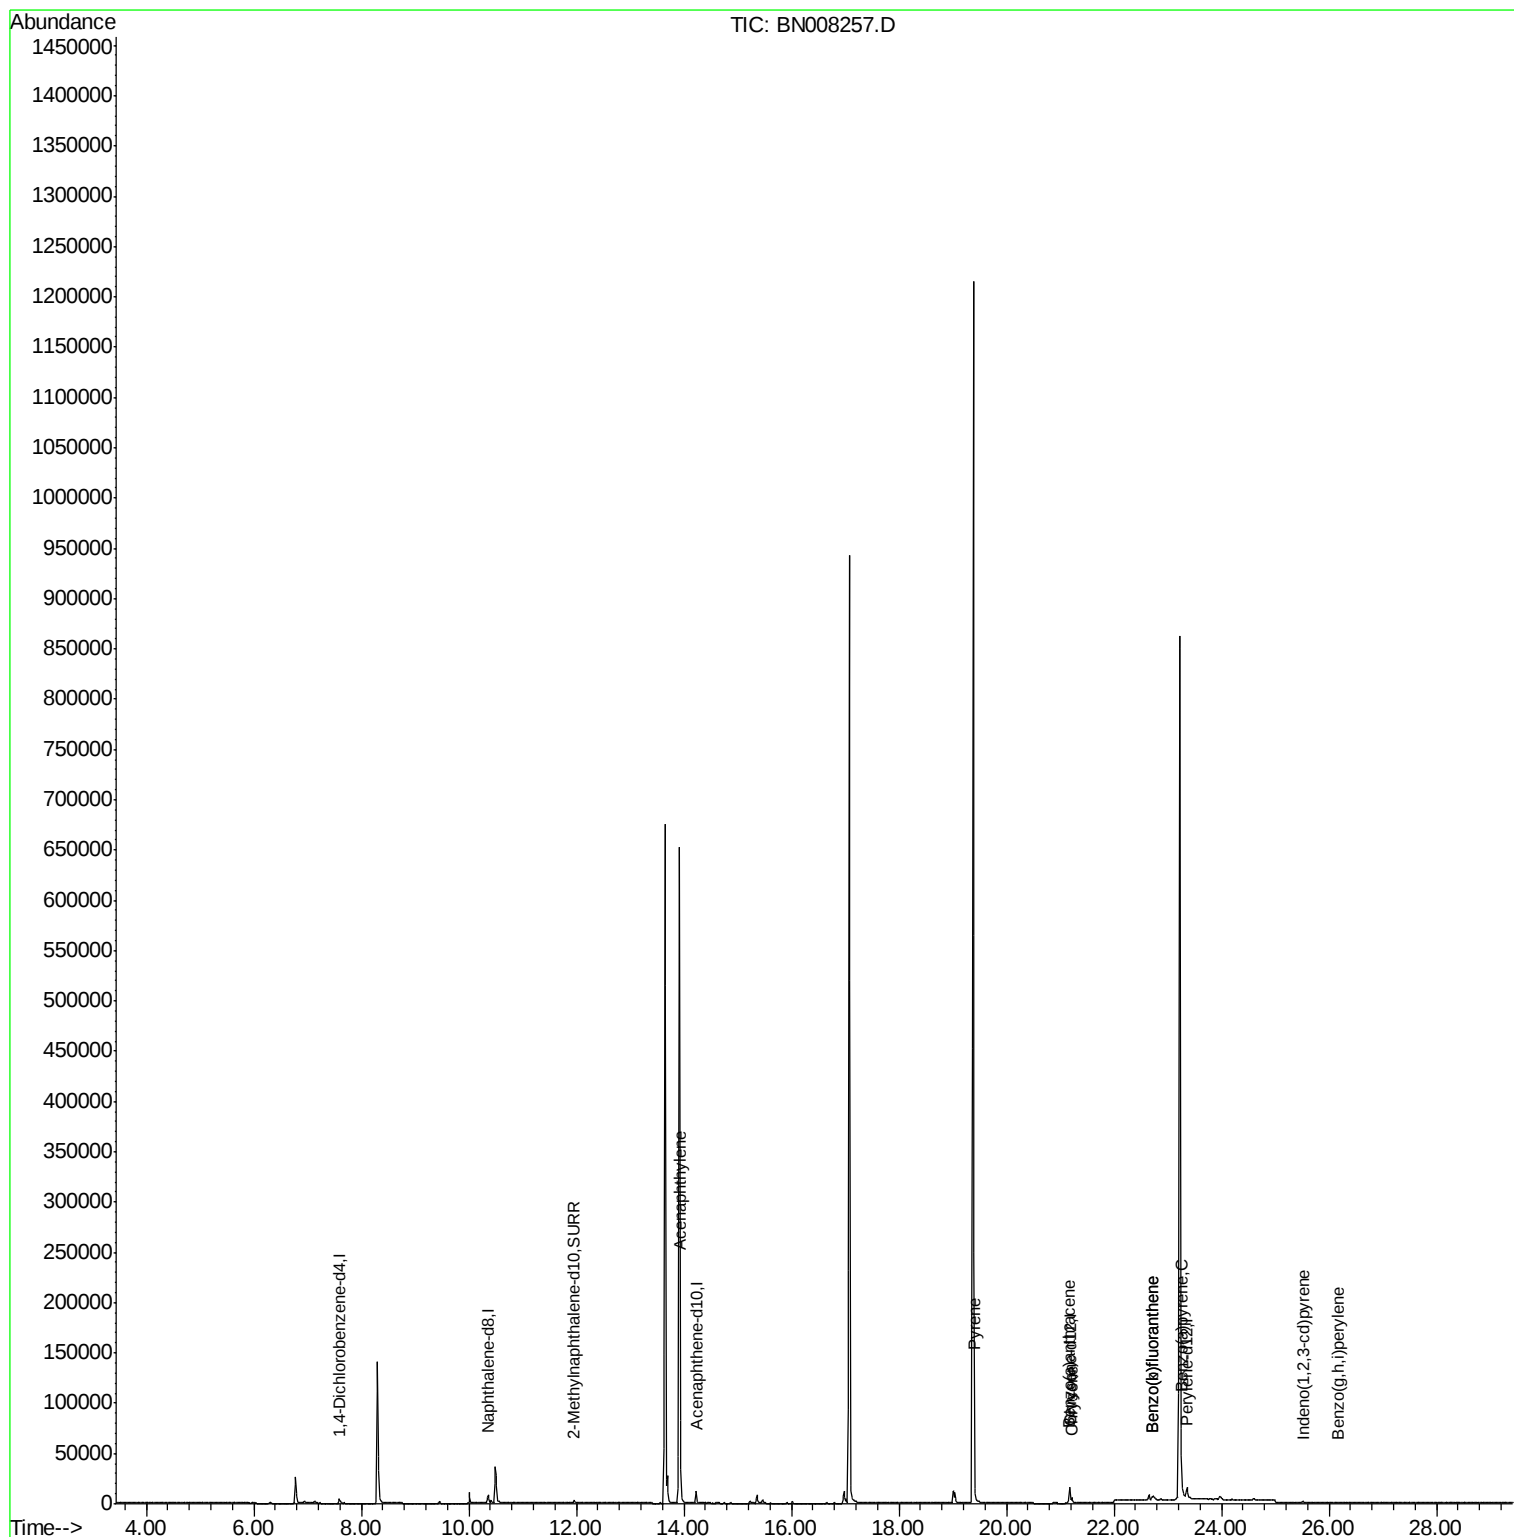

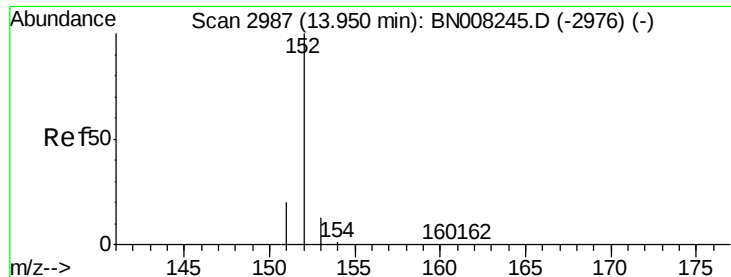

#7

Acenaphthylene

Concen: 0.022 ng/ul

RT: 13.94 min Scan# 2985

Delta R.T. -0.01 min

Lab File: BN008257.D

Acq: 18 Oct 2019 20:58

Instrument :

BNA_N

ClientSampled :

BEPG7


Tgt Ion:152 Resp: 668

Ion Ratio Lower Upper

152 100

151 29.9 16.2 24.4#




153 31.9 11.0 16.4#

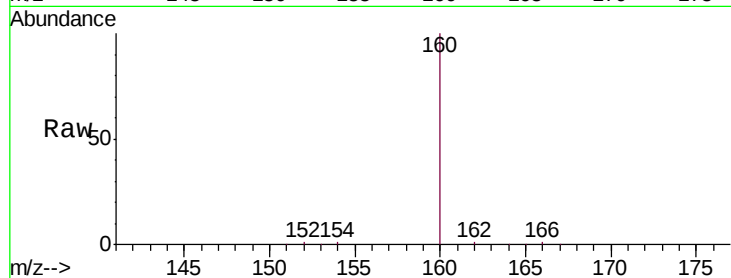

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

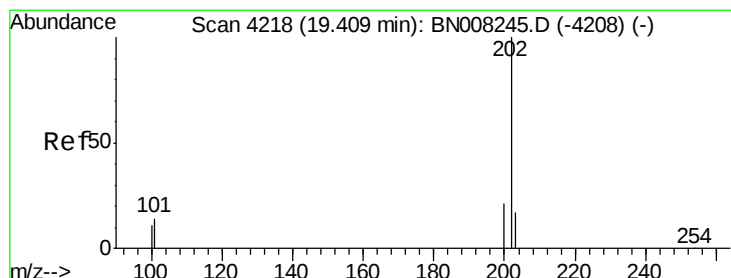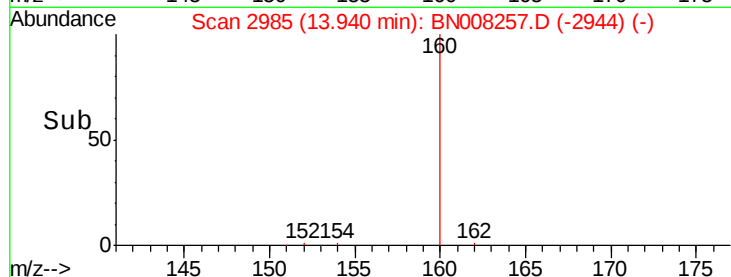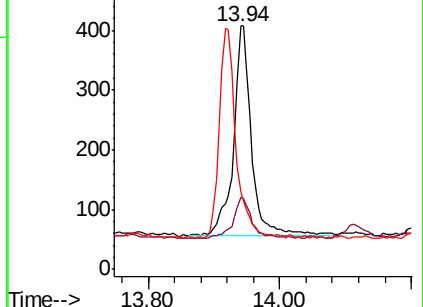

#17

Pyrene

Concen: 0.186 ng/ul

RT: 19.41 min Scan# 4218

Delta R.T. 0.00 min

Lab File: BN008257.D

Acq: 18 Oct 2019 20:58


Tgt Ion:202 Resp: 9974

Ion Ratio Lower Upper

202 100

101 14.1 10.9 16.3



100 12.8 8.7 13.1

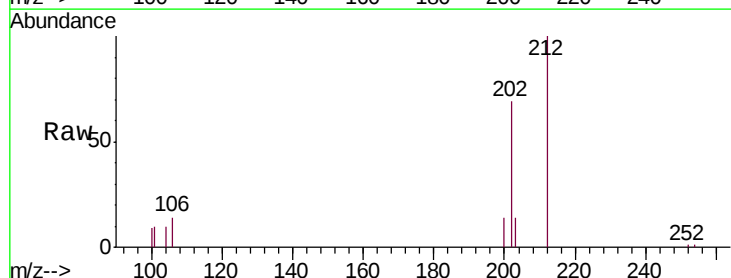


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

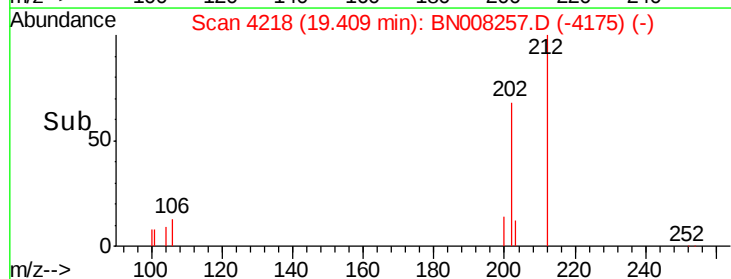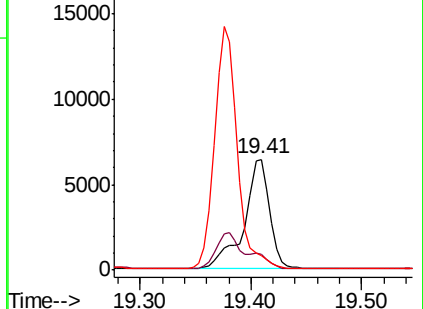

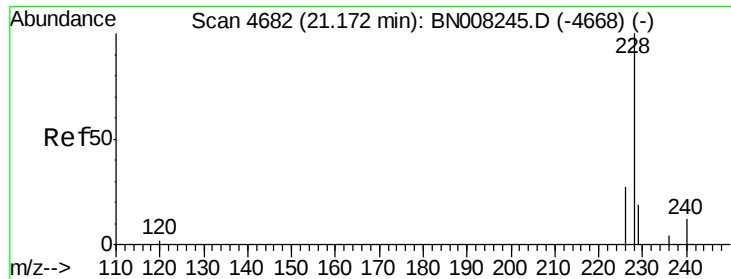

#18

Benzo(a)anthracene

Concen: 0.097 ng/ul

RT: 21.17 min Scan# 4680

Delta R.T. -0.01 min

Lab File: BN008257.D

Acq: 18 Oct 2019 20:58

Instrument :

BNA_N

ClientSampleId :

BEPG7


Tgt Ion:228 Resp: 4753

Ion Ratio Lower Upper




228 100

229 22.6 16.2 24.2

226 30.2 21.4 32.0

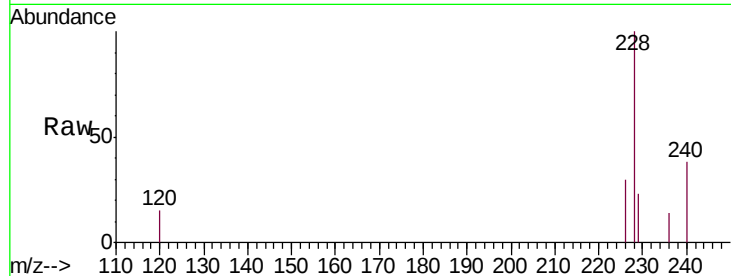

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

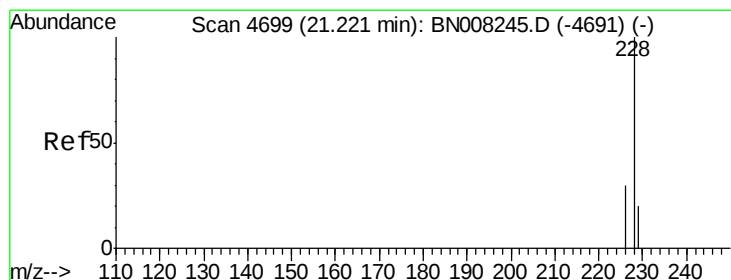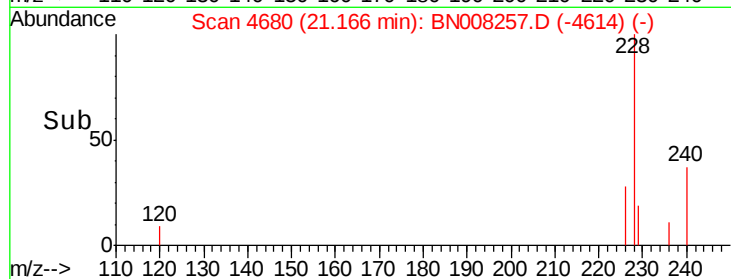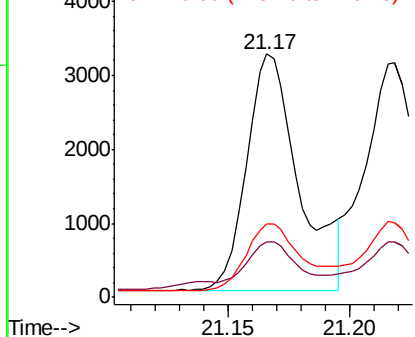

#19

Chrysene

Concen: 0.084 ng/ul

RT: 21.22 min Scan# 4698

Delta R.T. -0.00 min

Lab File: BN008257.D

Acq: 18 Oct 2019 20:58


Tgt Ion:228 Resp: 5062

Ion Ratio Lower Upper



228 100


226 31.6 24.1 36.1

229 23.6 16.2 24.2

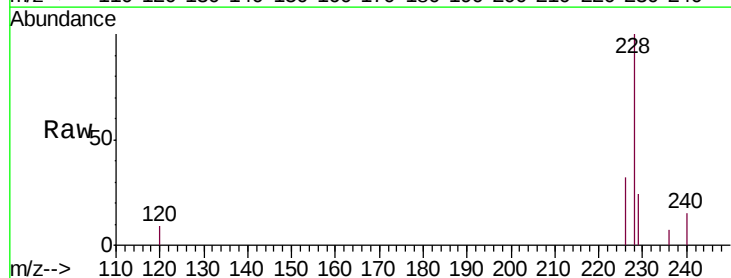

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

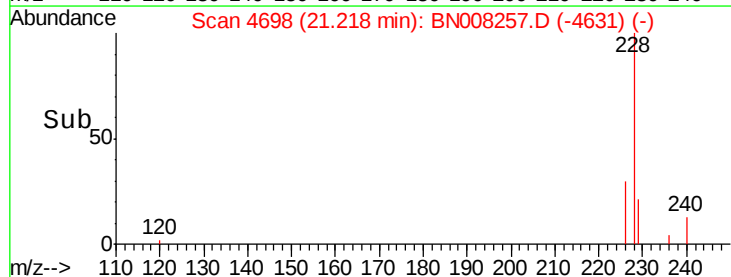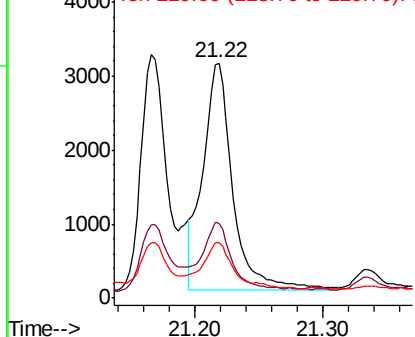

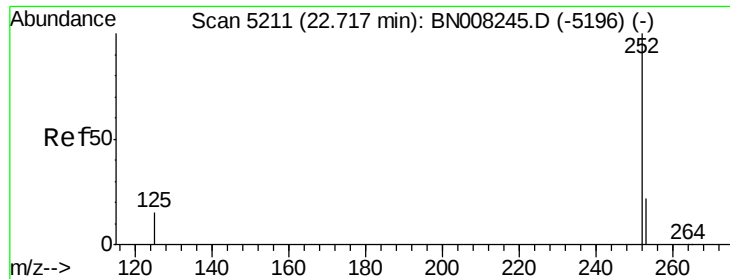

#21

Benzo(b)fluoranthene

Concen: 0.206 ng/ul

RT: 22.71 min Scan# 5210

Delta R.T. -0.00 min

Lab File: BN008257.D

Acq: 18 Oct 2019 20:58

Instrument :

BNA_N

ClientSampleId :

BEPG7


Tgt Ion:252 Resp: 8600

Ion Ratio Lower Upper

252 100

253 35.3 0.0 53.4




125 37.6 0.0 32.4#

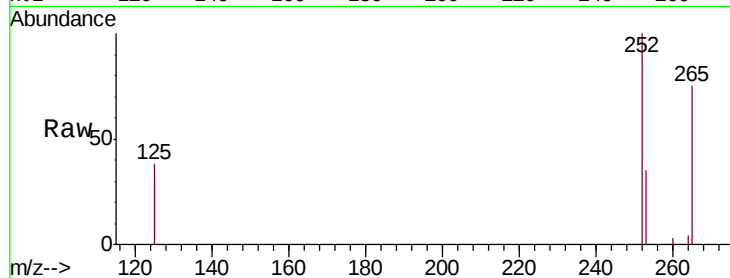

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

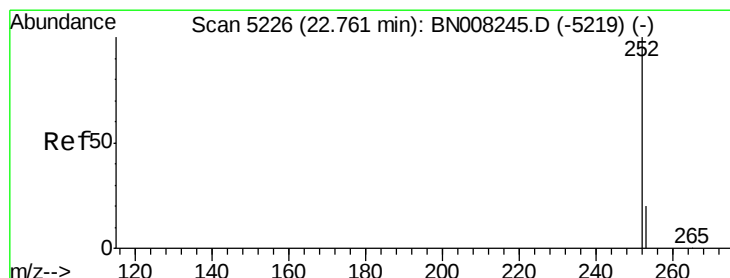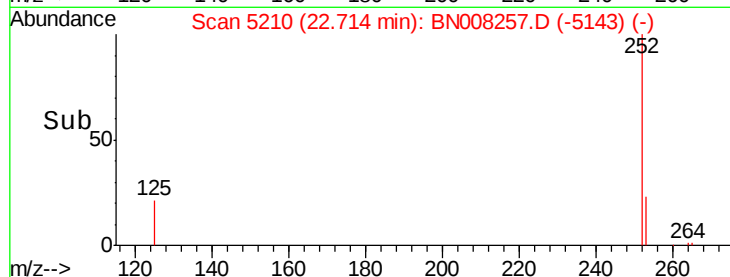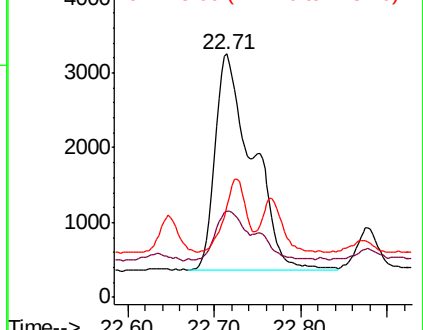

#22

Benzo(k)fluoranthene

Concen: 0.182 ng/ul

RT: 22.71 min Scan# 5210

Delta R.T. -0.05 min

Lab File: BN008257.D

Acq: 18 Oct 2019 20:58


Tgt Ion:252 Resp: 8600

Ion Ratio Lower Upper

252 100

253 35.3 21.3 31.9#



125 37.6 12.3 18.5#

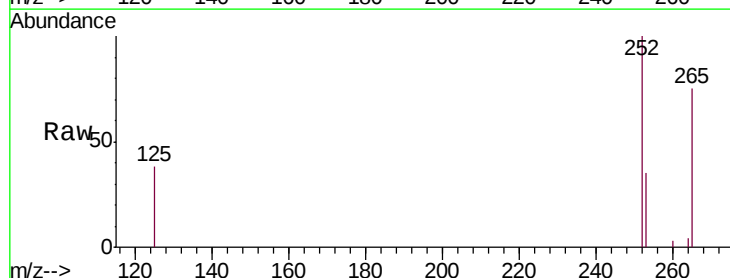


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

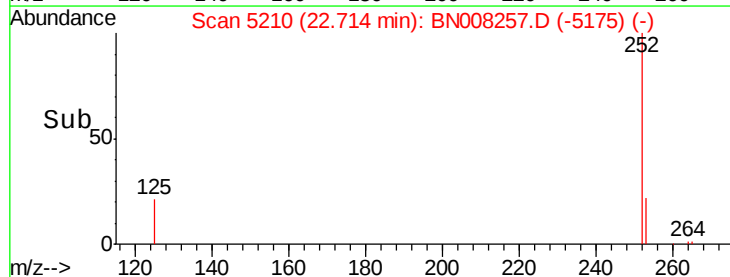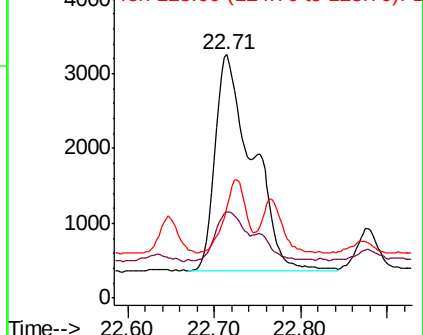

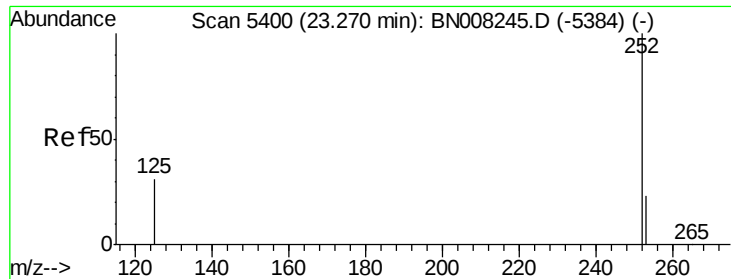

#23

Benzo(a)pyrene

Concen: 0.094 ng/u1

RT: 23.26 min Scan# 5397

Delta R.T. -0.01 min

Lab File: BN008257.D

Acq: 18 Oct 2019 20:58

Instrument :

BNA_N

ClientSampleId :

BEPG7


Tgt Ion:252 Resp: 4123

Ion Ratio Lower Upper

252 100

253 37.8 22.8 34.2#




125 43.2 18.4 27.6#

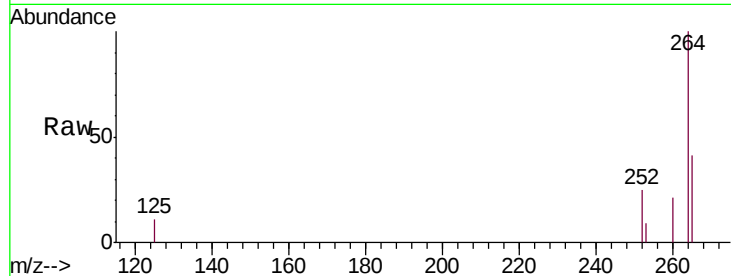

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

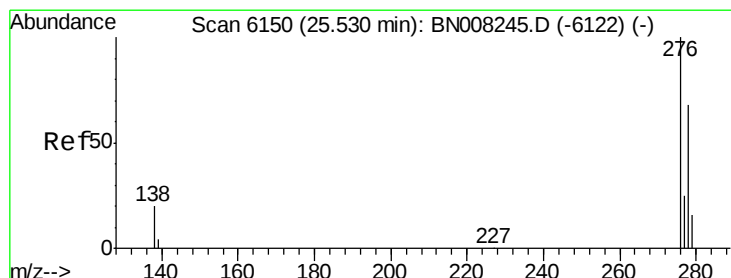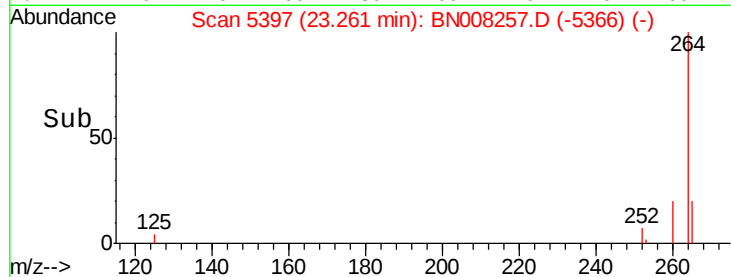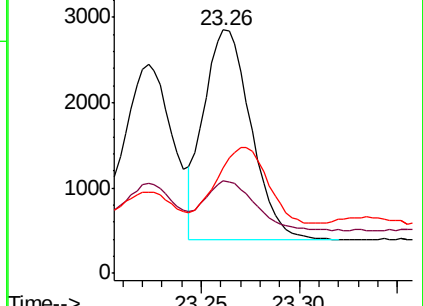

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.047 ng/u1

RT: 25.51 min Scan# 6145

Delta R.T. -0.02 min

Lab File: BN008257.D

Acq: 18 Oct 2019 20:58


Tgt Ion:276 Resp: 2428

Ion Ratio Lower Upper

276 100

138 16.4 16.1 24.1



227 0.2 0.2 0.2

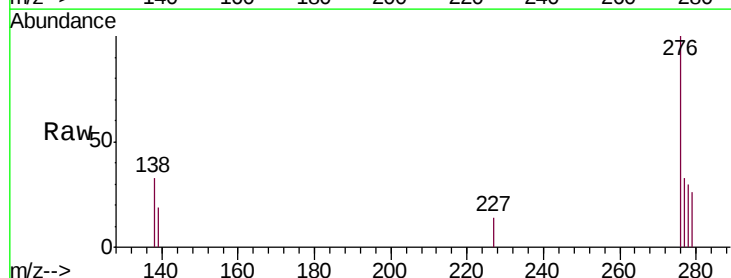


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

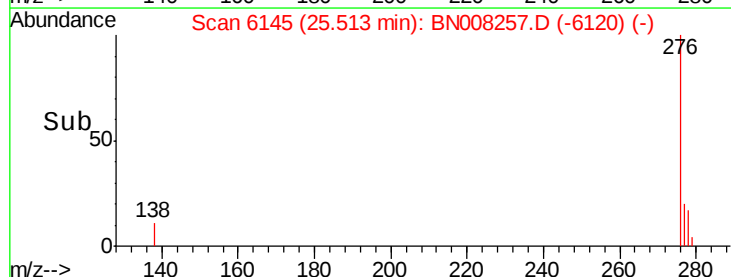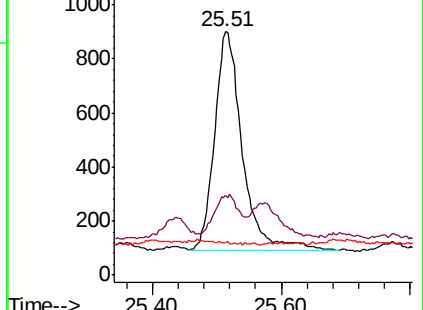

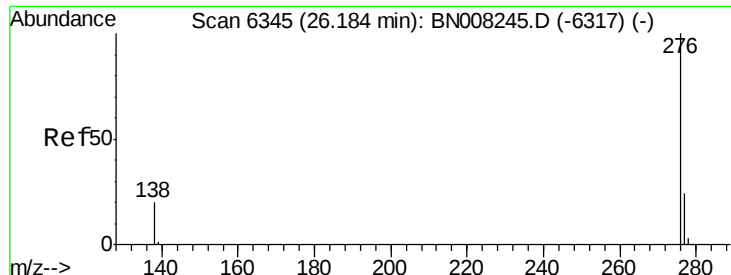

#26

Benzo(g,h,i)perylene

Concen: 0.048 ng/ul

RT: 26.17 min Scan# 6342

Delta R.T. -0.01 min

Lab File: BN008257.D

Acq: 18 Oct 2019 20:58

Instrument :

BNA_N

ClientSampleId :

BEPG7


Tgt Ion: 276 Resp: 2295

Ion Ratio Lower Upper

276 100

138 34.6 17.0 25.4#

277 35.1 20.4 30.6#

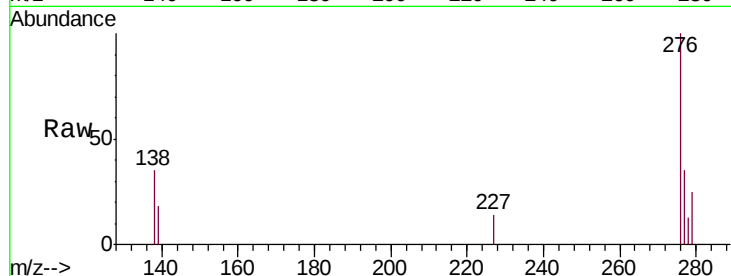

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

