

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101819\
 Data File : BN008249.D
 Acq On : 18 Oct 2019 16:12
 Operator : JU
 Sample : K5178-02DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Quant Time: Oct 18 17:38:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 17:22:25 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 BEPD1DL

Manual Integrations
 APPROVED

mohammad

10/22/2019 1:40:23 AM

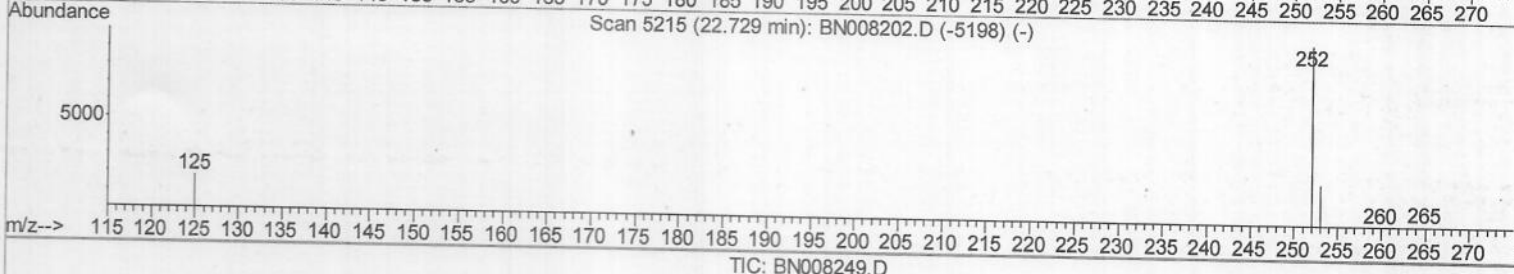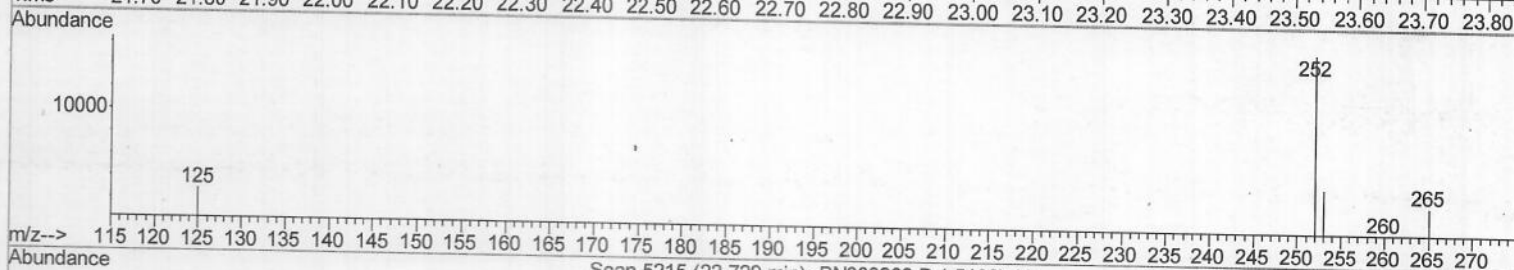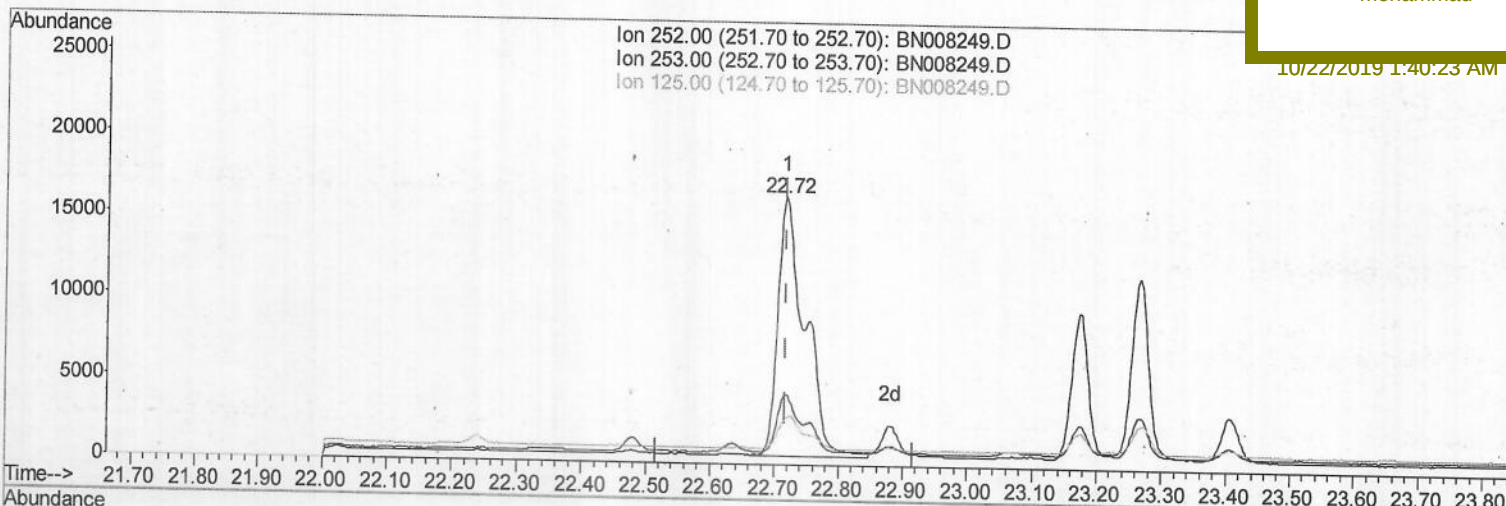

(21) Benzo(b)fluoranthene
 22.717min (+0.000) 1.01ng/ul
 response 46668

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	26.32
125.00	16.20	17.26
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101819\

Data File : BN008249.D

Acq On : 18 Oct 2019 16:12

Operator : JU

Sample : K5178-02DL 5X

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Oct 18 17:38:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Oct 18 17:22:25 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




BEPD1DL

Manual Integrations

APPROVED

mohammad

10/22/2019 1:40:23 AM

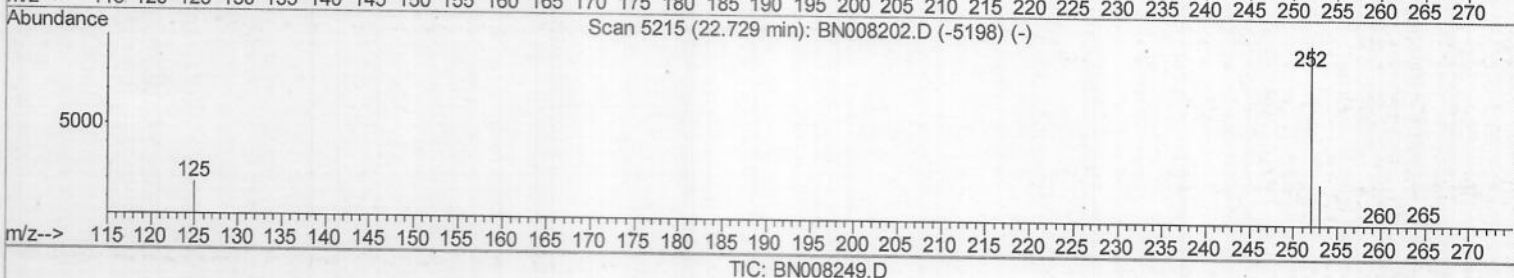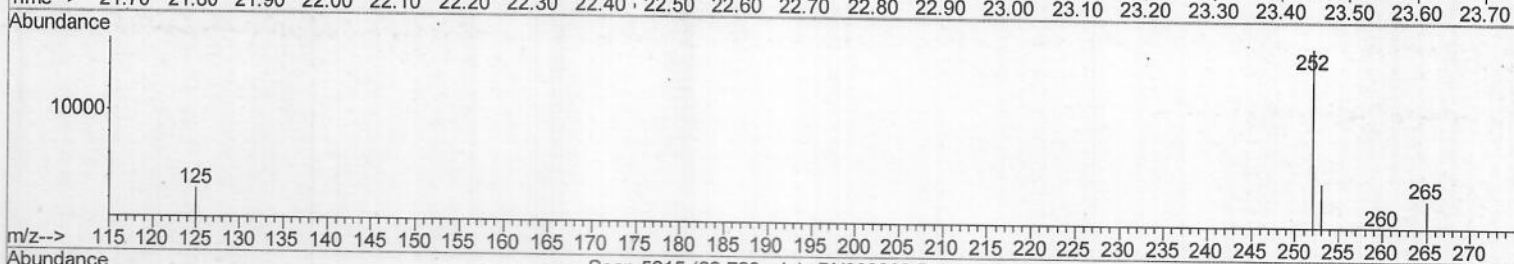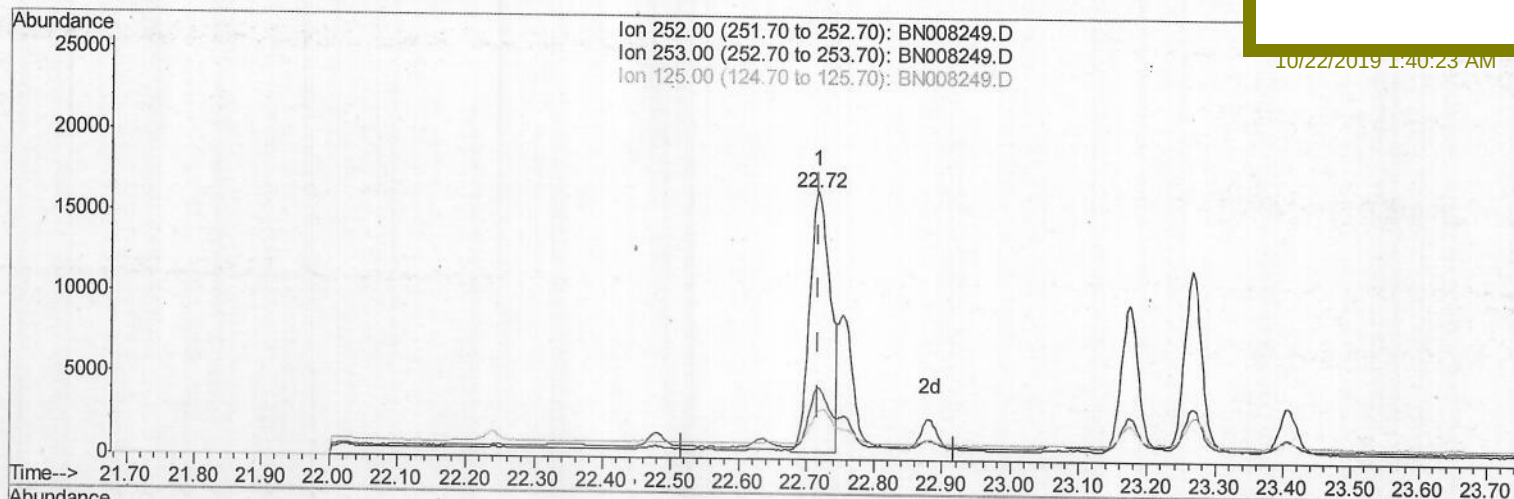

(21) Benzo(b)fluoranthene

22.717min (+0.000) 0.73ng/ul m > JU 10/23/19

response 33578

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	26.32
125.00	16.20	17.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101819\
Data File : BN008249.D

Acq On : 18 Oct 2019 16:12

Operator : JU

Sample : K5178-02DL 5X

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Oct 18 17:38:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Oct 18 17:22:25 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

BEPD1DL

Manual Integrations
APPROVED

mohammad

10/22/2019 1:40:23 AM

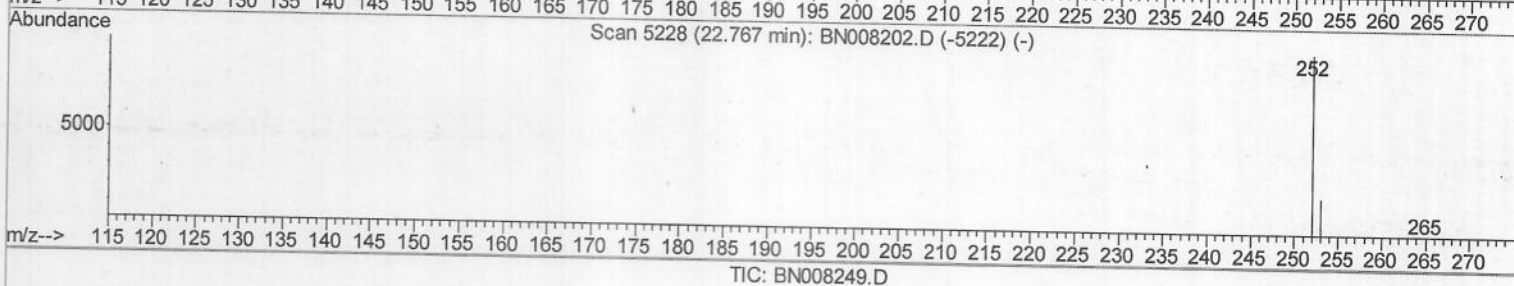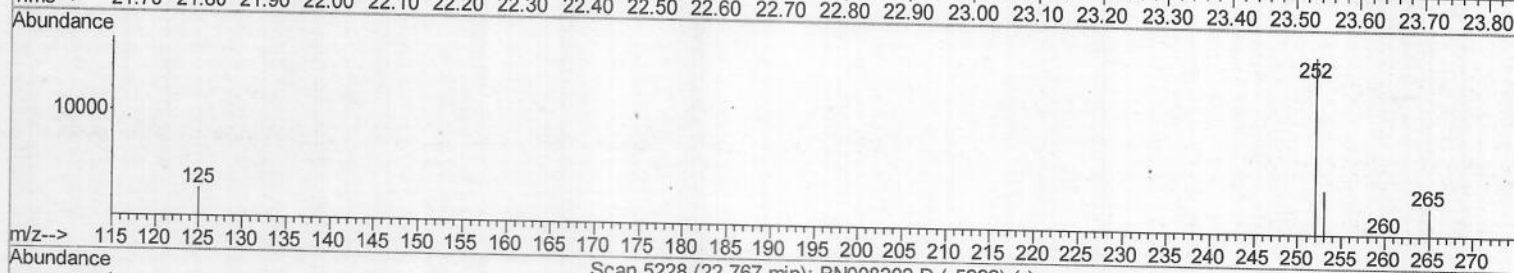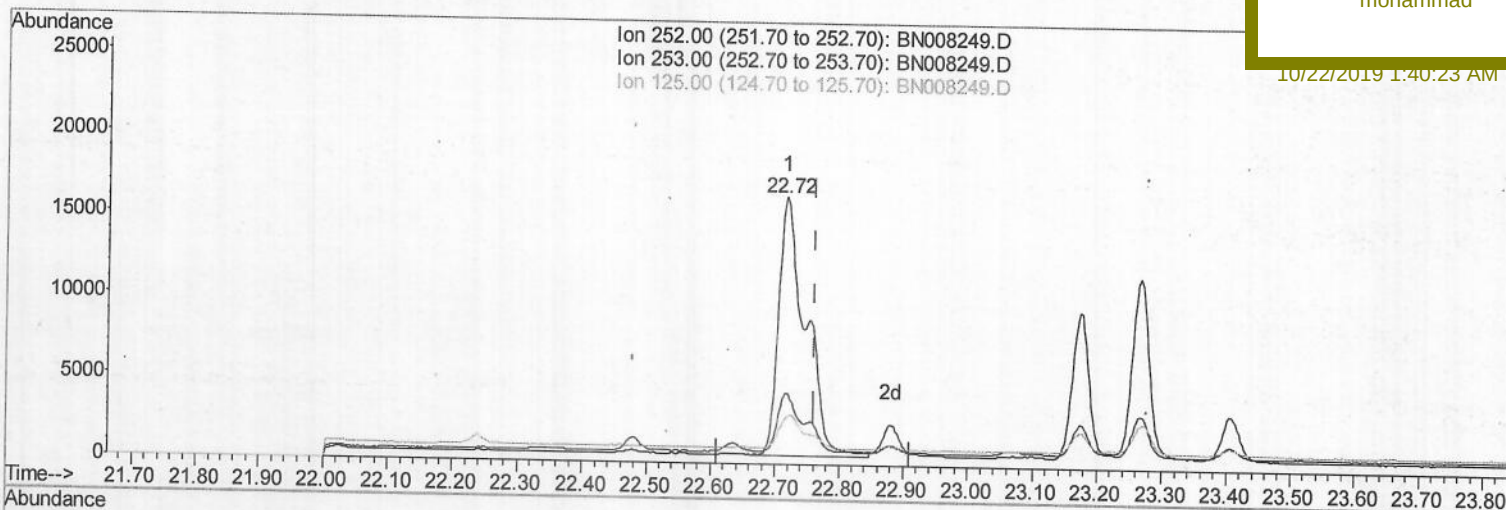

(22) Benzo(k)fluoranthene

22.717min (-0.044) 0.89ng/ul

response 46668

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	26.32
125.00	15.40	17.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101819\

Data File : BN008249.D

Acq On : 18 Oct 2019 16:12

Operator : JU

Sample : K5178-02DL 5X

Misc :

ALS Vial : 6 Sample Multiplier: 1

Quant Time: Oct 18 17:38:29 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Oct 18 17:22:25 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




BEPD1DL

Manual Integrations

APPROVED

mohammad

10/22/2019 1:40:23 AM

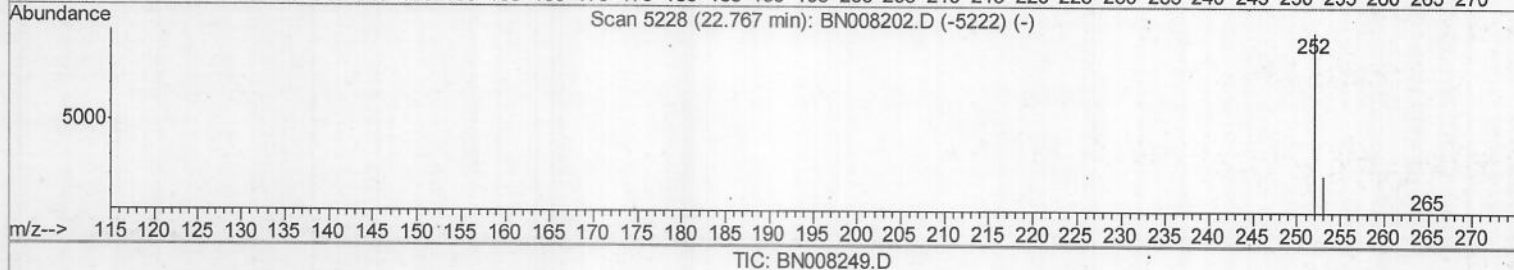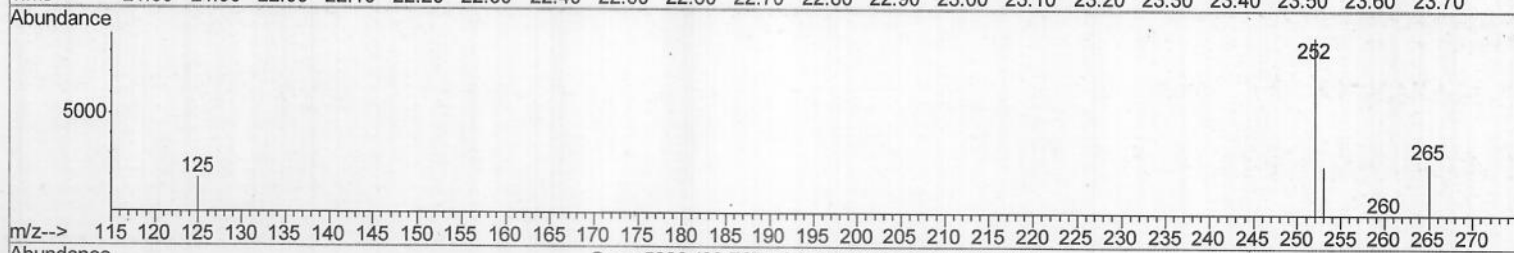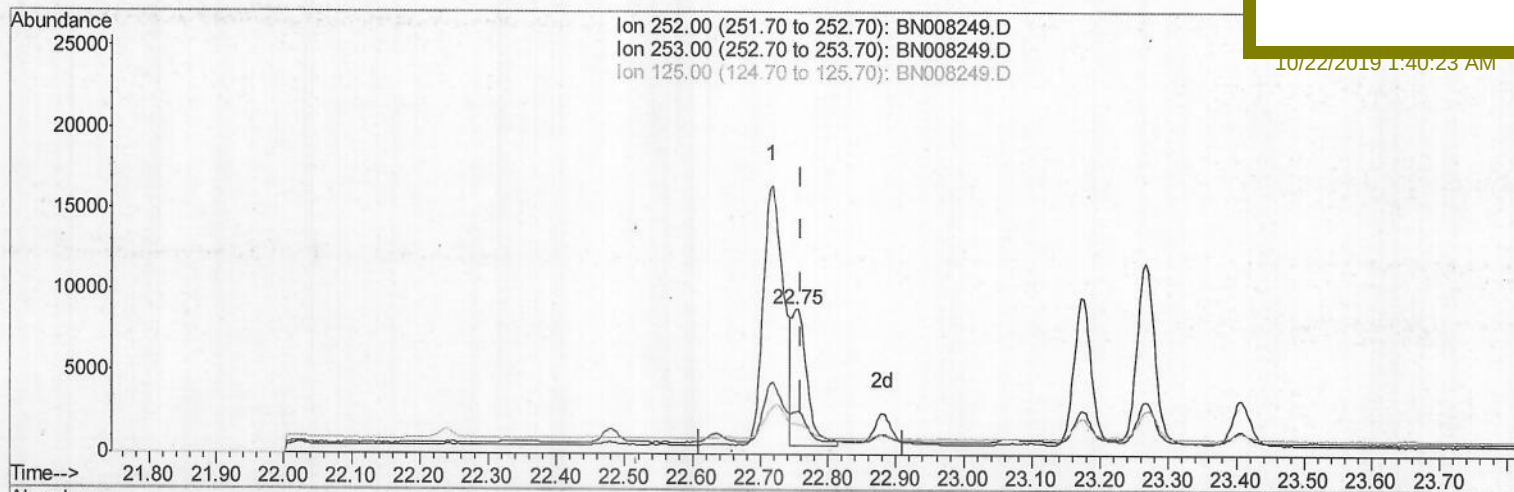

(22) Benzo(k)fluoranthene

22.752min (-0.009) 0.25ng/ul m

response 13075

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	29.12
125.00	15.40	20.92#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101819\
 Data File : BN008249.D
 Acq On : 18 Oct 2019 16:12
 Operator : JU
 Sample : K5178-02DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Oct 18 17:39:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 17:22:25 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 BEPD1DL

Manual Integrations
 APPROVED

mohammad

10/22/2019 1:40:23 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2672	0.40	ng/ul	0.00
2) Naphthalene-d8	10.36	136	13268	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.23	164	8407	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	17527	0.40	ng/ul	0.00
16) Chrysene-d12	21.18	240	16409	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	14165	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.96	152	631	0.03	ng/ul	0.00
14) Fluoranthene-d10	19.01	212	1986	0.03	ng/ul	0.00

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
7) Acenaphthylene	13.95	152	886	0.022	ng/ul#	72
12) Phenanthrene	17.02	178	15837	0.309	ng/ul	99
13) Anthracene	17.11	178	1668	0.037	ng/ul#	88
15) Fluoranthene	19.04	202	57414	0.847	ng/ul	97
17) Pyrene	19.41	202	47506	0.727	ng/ul	100
18) Benzo(a)anthracene	21.17	228	20373	0.341	ng/ul	96
19) Chrysene	21.22	228	27237	0.372	ng/ul	98
21) Benzo(b)fluoranthene	22.72	252	33578m	0.728	ng/ul	98
22) Benzo(k)fluoranthene	22.75	252	13075m	0.250	ng/ul	99
23) Benzo(a)pyrene	23.27	252	19887	0.410	ng/ul	97
24) Indeno(1,2,3-cd)pyrene	25.52	276	14391	0.252	ng/ul#	97
25) Dibenzo(a,h)anthracene	25.52	278	2727	0.060	ng/ul#	56
26) Benzo(g,h,i)perylene	26.18	276	14103	0.269	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101819\
Data File : BN008249.D
Acq On : 18 Oct 2019 16:12
Operator : JU
Sample : K5178-02DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Oct 18 17:39:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 17:22:25 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
BEPD1DL

Manual Integrations
APPROVED

mohammad

