

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101819\
 Data File : BN008258.D
 Acq On : 18 Oct 2019 21:34
 Operator : JU
 Sample : K5177-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BEPK2

Manual Integrations
 APPROVED

mohammad
 10/22/2019 1:41:05 AM

Quant Time: Oct 19 00:58:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 23:47:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2446	0.40	ng/ul	0.00
2) Naphthalene-d8	10.36	136	11529	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.23	164	6966	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.97	188	14540	0.40	ng/ul	0.00
16) Chrysene-d12	21.18	240	13478	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	12243	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	3633	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.01	212	9565	0.19	ng/ul	0.00
Target Compounds				Ovalue		
12) Phenanthrene	17.02	178	1372	0.032	ng/ul#	88
15) Fluoranthene	19.04	202	2951	0.052	ng/ul	89
17) Pyrene	19.40	202	3254m	0.061	ng/ul	
18) Benzo(a)anthracene	21.17	228	1521	0.031	ng/ul#	84
19) Chrysene	21.22	228	2097	0.035	ng/ul#	88
21) Benzo(b)fluoranthene	22.72	252	2340m	0.059	ng/ul	
23) Benzo(a)pyrene	23.26	252	1409	0.034	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101819\
Data File : BN008258.D
Acq On : 18 Oct 2019 21:34
Operator : JU
Sample : K5177-16
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BEPK2

Manual Integrations
APPROVED

mohammad
10/22/2019 1:41:05 AM

Quant Time: Oct 19 00:58:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 23:47:17 2019
Response via : Initial Calibration

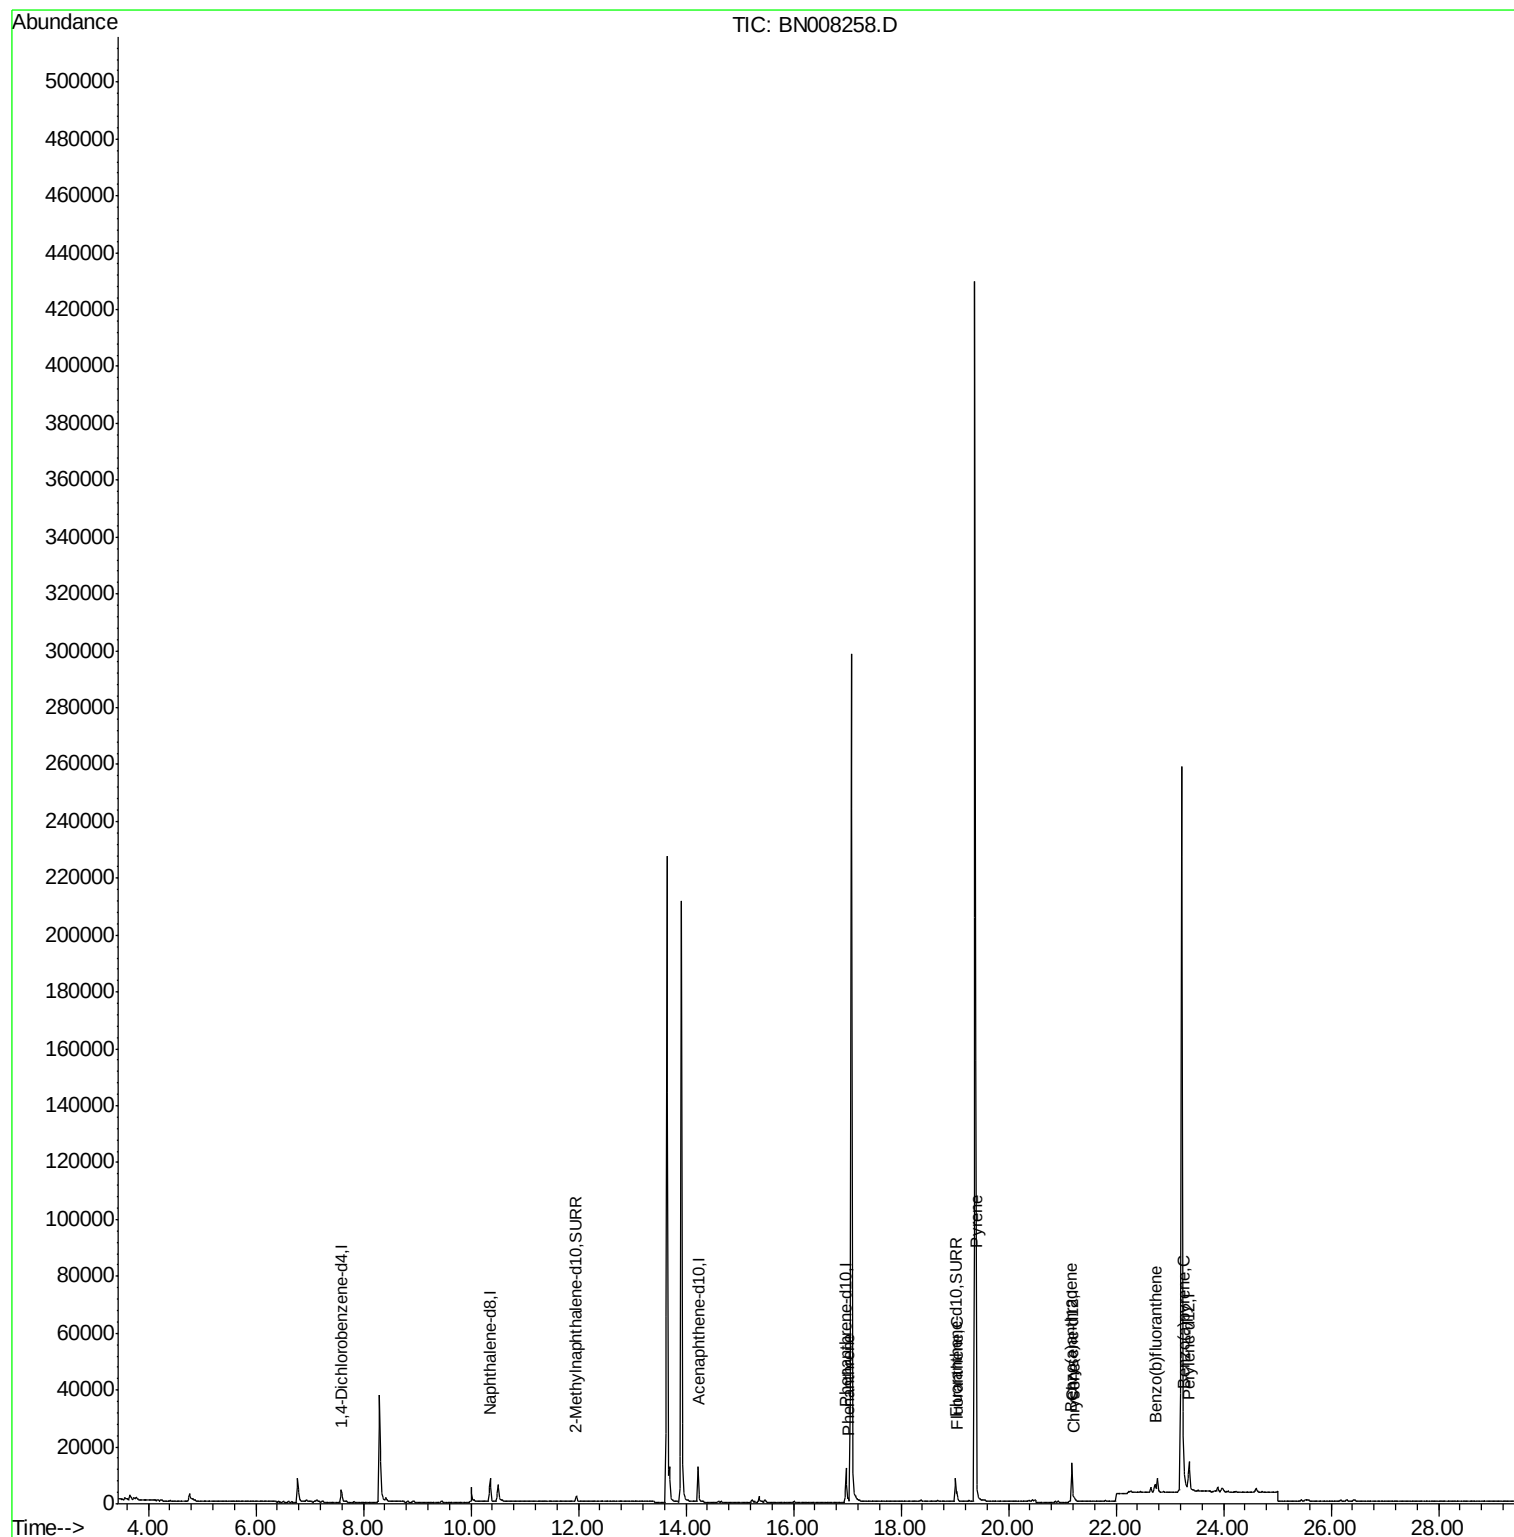

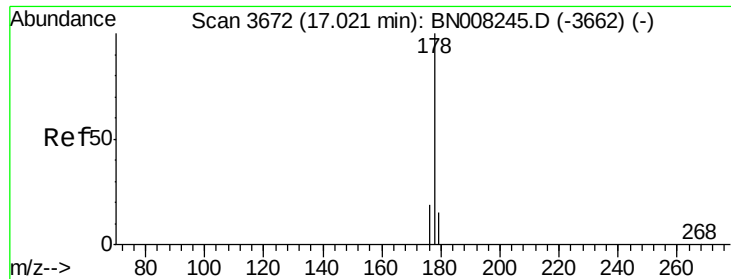





#12
Phenanthrene
Concen: 0.032 ng/ul
RT: 17.02 min Scan# 3671
Delta R.T. -0.00 min
Lab File: BN008258.D
Acq: 18 Oct 2019 21:34

Instrument :
BNA_N
ClientSampled :
BEPK2

Tot Ion	Ratio	Lower	Upper
178	100		
179	22.7	12.8	19.2#
176	23.4	15.4	23.2#




Manual Integrations
APPROVED


mohammad
10/22/2019 1:41:05 AM

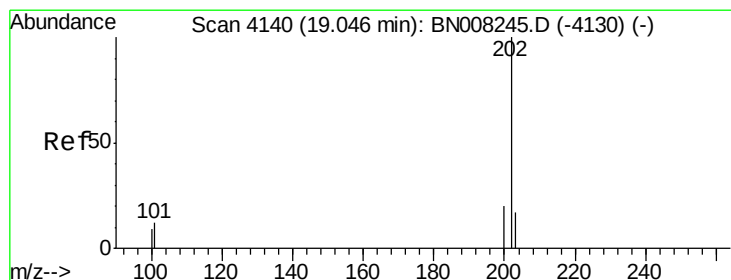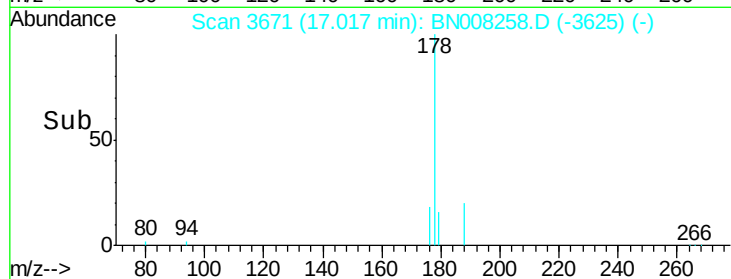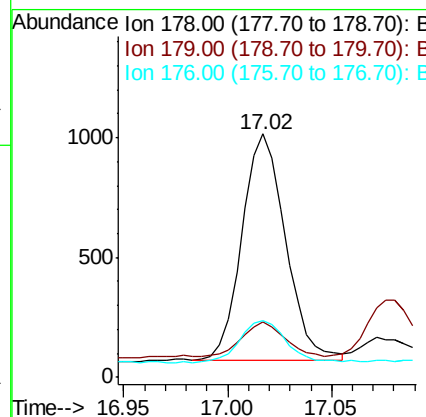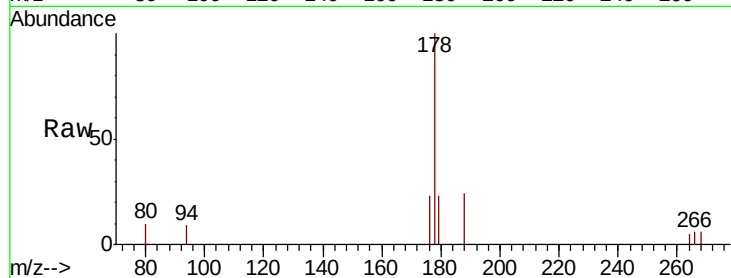

#15
Fluoranthene
Concen: 0.052 ng/ul
RT: 19.04 min Scan# 4139
Delta R.T. -0.00 min
Lab File: BN008258.D
Acq: 18 Oct 2019 21:34

Tgt Ion	Ratio	Lower	Upper
202	100		
101	16.0	0.0	31.2
100	11.8	0.0	28.5

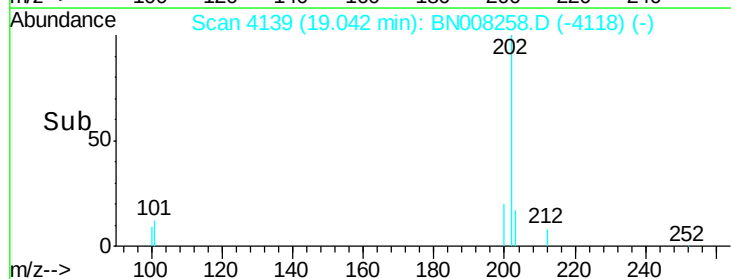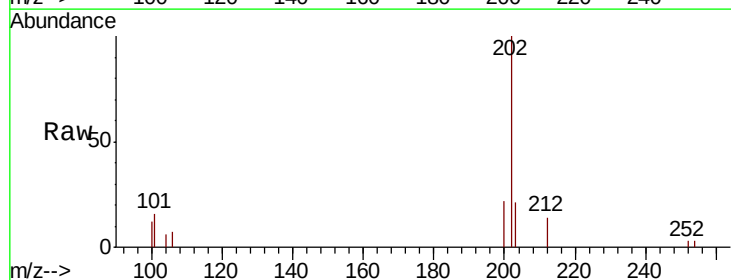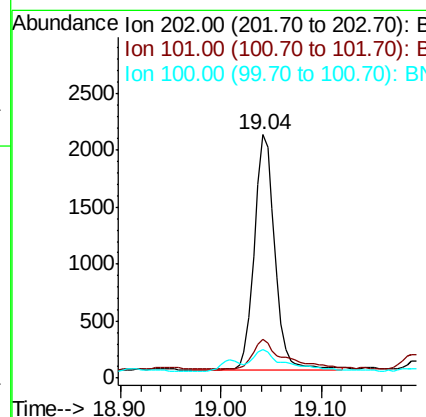

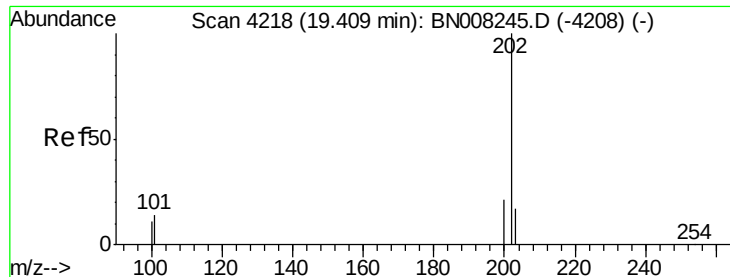

#17

Pvrene

Concen: 0.061 ng/ul m

RT: 19.40 min Scan# 4217

Delta R.T. -0.00 min

Lab File: BN008258.D

Acq: 18 Oct 2019 21:34

Instrument :

BNA_N





ClientSampled :

BEPK2

Tot Ion	Ratio	Lower	Upper
202	100		
101	17.5	10.9	16.3#
100	17.6	8.7	13.1#

Manual Integrations
APPROVED

mohammad
10/22/2019 1:41:05 AM

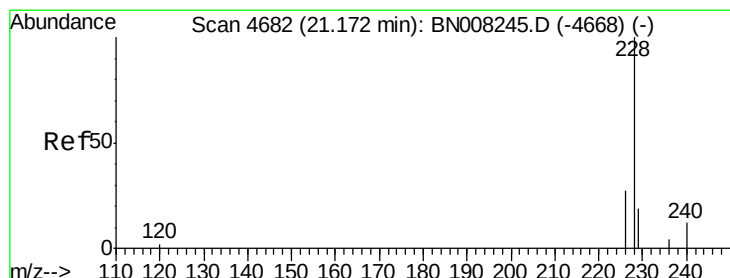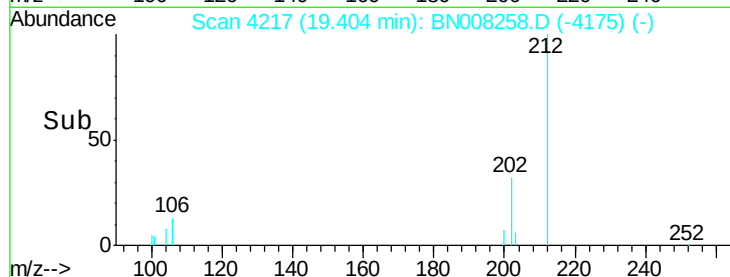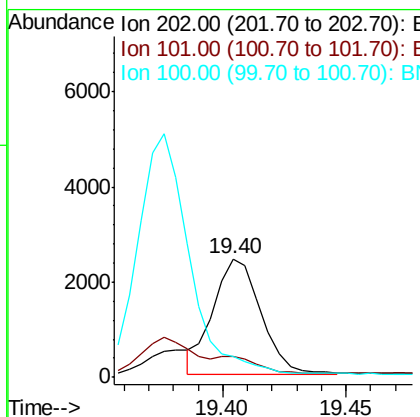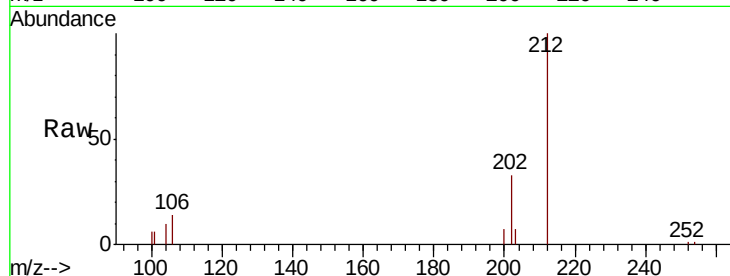

#18

Benzo(a)anthracene

Concen: 0.031 ng/ul




RT: 21.17 min Scan# 4680


Delta R.T. -0.01 min

Lab File: BN008258.D

Acq: 18 Oct 2019 21:34

Tgt Ion	Ratio	Lower	Upper
228	100		
229	27.9	16.2	24.2#
226	34.6	21.4	32.0#

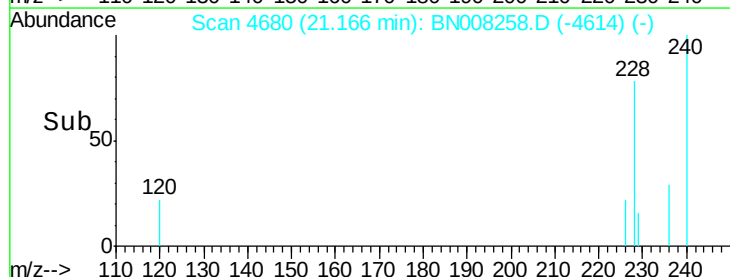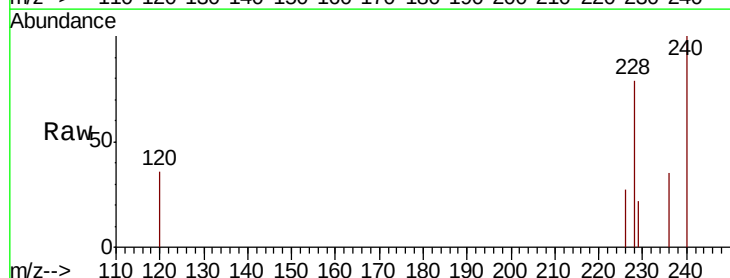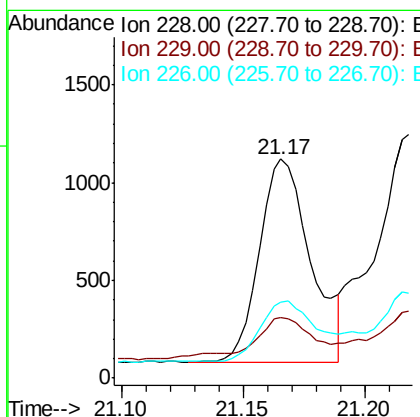

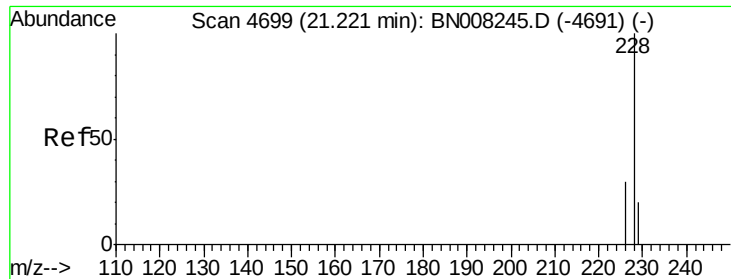

#19

Chrysene

Concen: 0.035 ng/ul

RT: 21.22 min Scan# 4698

Delta R.T. -0.00 min

Lab File: BN008258.D

Acq: 18 Oct 2019 21:34

Instrument :

BNA_N

ClientSampled :

BEPK2

Tot Ion:228 Resp: 2097

Ion Ratio Lower Upper





228 100

226 35.0 24.1 36.1

229 27.6 16.2 24.2#

Manual Integrations
APPROVED

mohammad
10/22/2019 1:41:05 AM

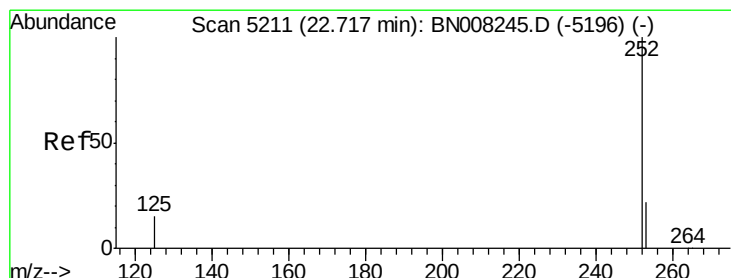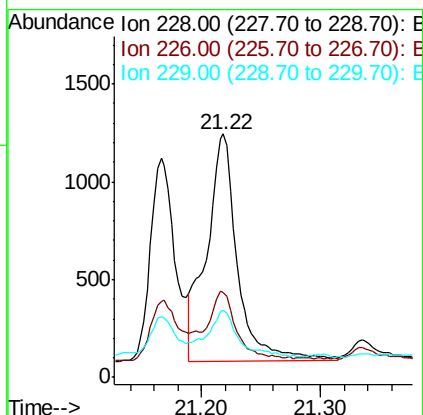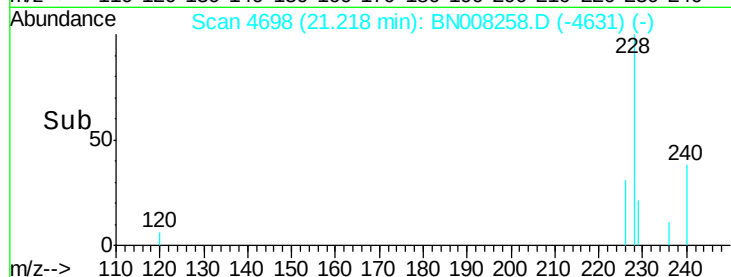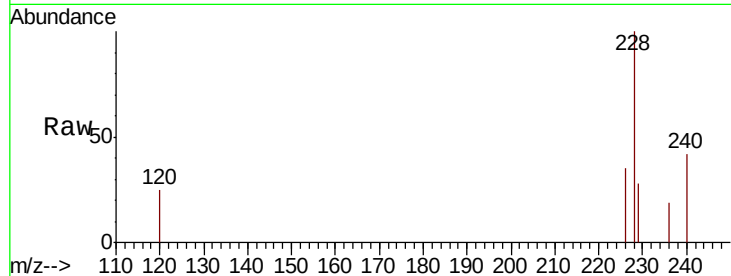

#21

Benzo(b)fluoranthene

Concen: 0.059 ng/ul m

RT: 22.72 min Scan# 5211

Delta R.T. 0.00 min

Lab File: BN008258.D

Acq: 18 Oct 2019 21:34




Tgt Ion:252 Resp: 2340




Ion Ratio Lower Upper

252 100

253 59.0 0.0 53.4#

125 121.4 0.0 32.4#

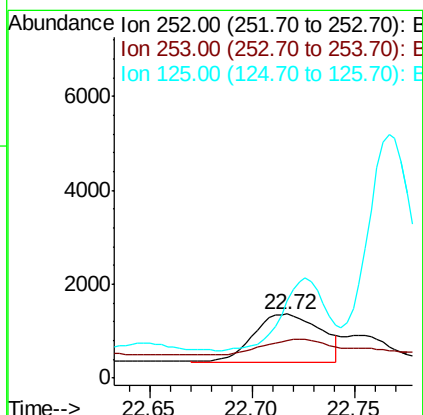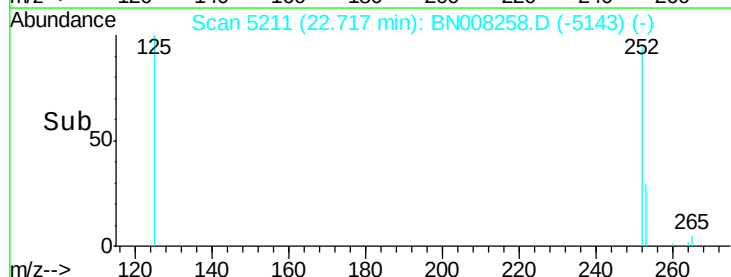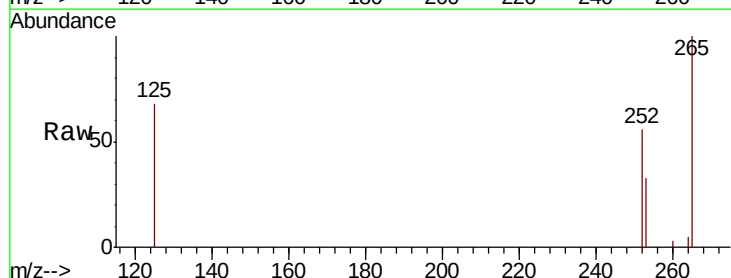

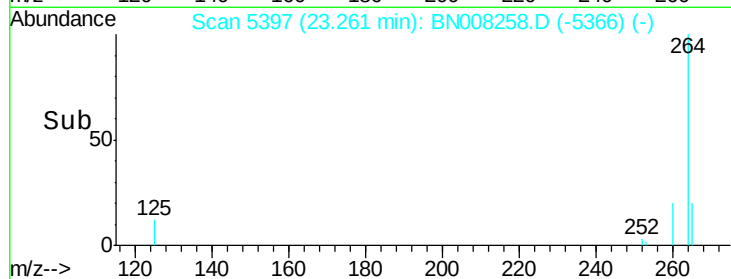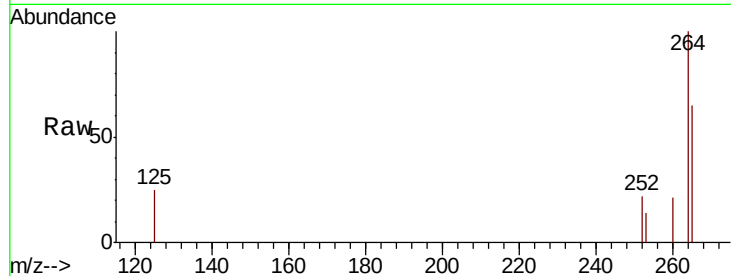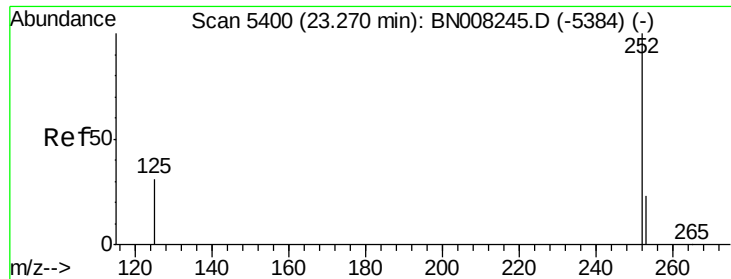

#23

Benzo(a)pyrene

Concen: 0.034 ng/ul

RT: 23.26 min Scan# 5397

Delta R.T. -0.01 min

Lab File: BN008258.D

Acq: 18 Oct 2019 21:34

Instrument :

BNA_N

ClientSampleId :

BEPK2

Tot Ion	Ratio	Lower	Upper
252	100		
253	62.7	22.8	34.2#
125	114.3	18.4	27.6#

Manual Integrations
APPROVED

mohammad
10/22/2019 1:41:05 AM

