

Data File : BN003229.D
Acq On : 20 Oct 2018 04:26
Operator : MJ/SJ
Sample : J5567-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ1

Quant Time: Oct 20 07:13:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 20 06:06:40 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	98732	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	487804	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	313677	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	736150	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	814031	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	792702	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	832	0.43	ng/uL	0.00
5) Phenol-d5	6.83	99	22101	2.36	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	6.96	67	13164	2.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	19061	2.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	18610	2.44	ng/ul	0.03
19) Nitrobenzene-d5	8.78	128	7541	1.99	ng/ul	0.02
22) 2-Nitrophenol-d4	9.49	143	9073	2.07	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	10.08	165	14375	1.81	ng/ul	0.05
29) 4-Chloroaniline-d4	10.56	131	20834	3.24	ng/ul	0.03
43) Dimethylphthalate-d6	13.67	166	62779	2.35	ng/ul	0.00
46) Acenaphthylene-d8	13.94	160	81462	2.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.60	143	1351	0.37	ng/ul	0.09
57) Fluorene-d10	15.26	176	61952	2.65	ng/ul	0.01
62) 4,6-Dinitro-2-methylphenol	15.44	200	4210	0.85	ng/ul	0.04
70) Anthracene-d10	17.11	188	94000	2.58	ng/ul	0.01
78) Pyrene-d10	19.42	212	107838	2.73	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	114478	2.67	ng/ul	0.00


Target Compounds					Qvalue	
44) Dimethylphthalate	13.72	163	32971	1.262	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003229.D
Acq On : 20 Oct 2018 04:26
Operator : MJ/SJ
Sample : J5567-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ1

Quant Time: Oct 20 07:13:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 20 06:06:40 2018
Response via : Initial Calibration

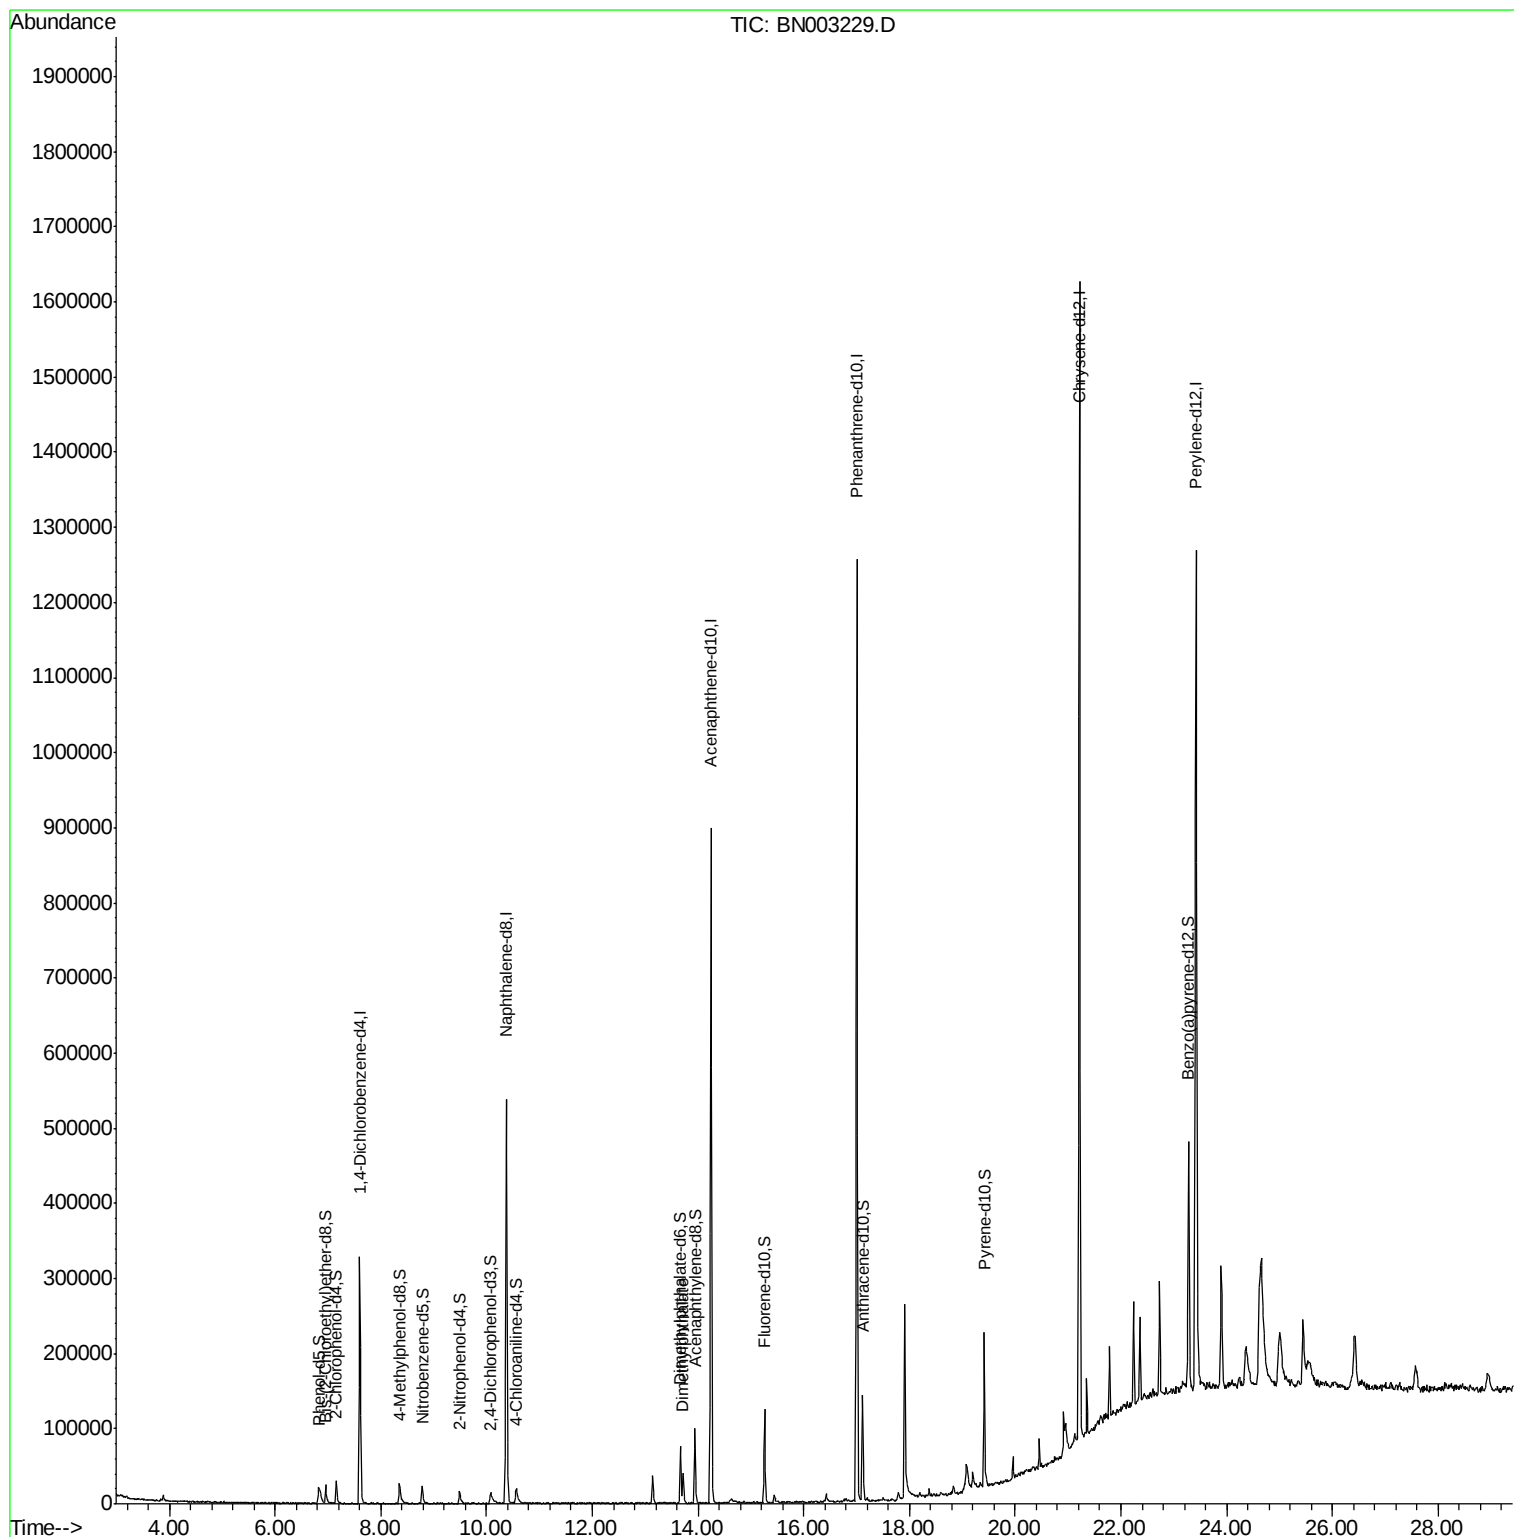

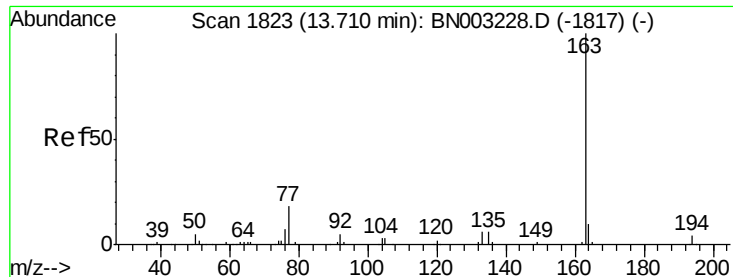

#44

Dimethylphthalate

Concen: 1.262 ng/ul

RT: 13.72 min Scan# 1824

Delta R.T. 0.01 min

Lab File: BN003229.D

Acq: 20 Oct 2018 04:26

Instrument :

BNA_N

ClientSampleId :

C0AJ1


Tgt Ion:163 Resp: 32971

Ion Ratio Lower Upper

163 100

194 3.6 3.7 5.5#

164 12.0 8.3 12.5

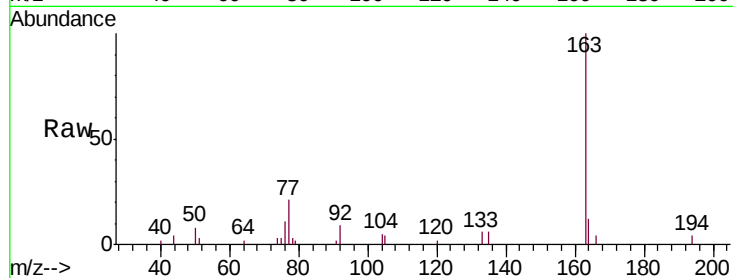

Abundance Ion 163.00 (162.70 to 163.70): E

25000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

