

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101918\
 Data File : BN003218.D
 Acq On : 19 Oct 2018 21:57
 Operator : MJ/SJ
 Sample : J5567-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH1

Manual Integrations
 APPROVED

Sohil
 10/22/2018 4:52:51 PM

Quant Time: Oct 20 05:34:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 20 05:04:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	89944	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	436418	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	274531	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	640651	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	736647	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	789956	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	5548	3.18	ng/uL	0.00
5) Phenol-d5	6.80	99	139677	16.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	92139	18.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	121102	18.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	123696	17.84	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	61484	18.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	72974	18.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	131293	18.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	142863	24.87	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	443555	18.96	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	552696	19.13	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	61222m	18.99	ng/ul	0.02
57) Fluorene-d10	15.25	176	401900	19.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.41	200	65743	15.28	ng/ul	0.00
70) Anthracene-d10	17.10	188	629579	19.85	ng/ul	0.00
78) Pyrene-d10	19.40	212	710734	19.91	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	848851	19.88	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	6.83	94	46493	5.424	ng/ul	96
44) Dimethylphthalate	13.71	163	112254	4.909	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101918\
Data File : BN003218.D
Acq On : 19 Oct 2018 21:57
Operator : MJ/SJ
Sample : J5567-03
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AH1

Quant Time: Oct 20 05:34:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 20 05:04:06 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
10/22/2018 4:52:51 PM

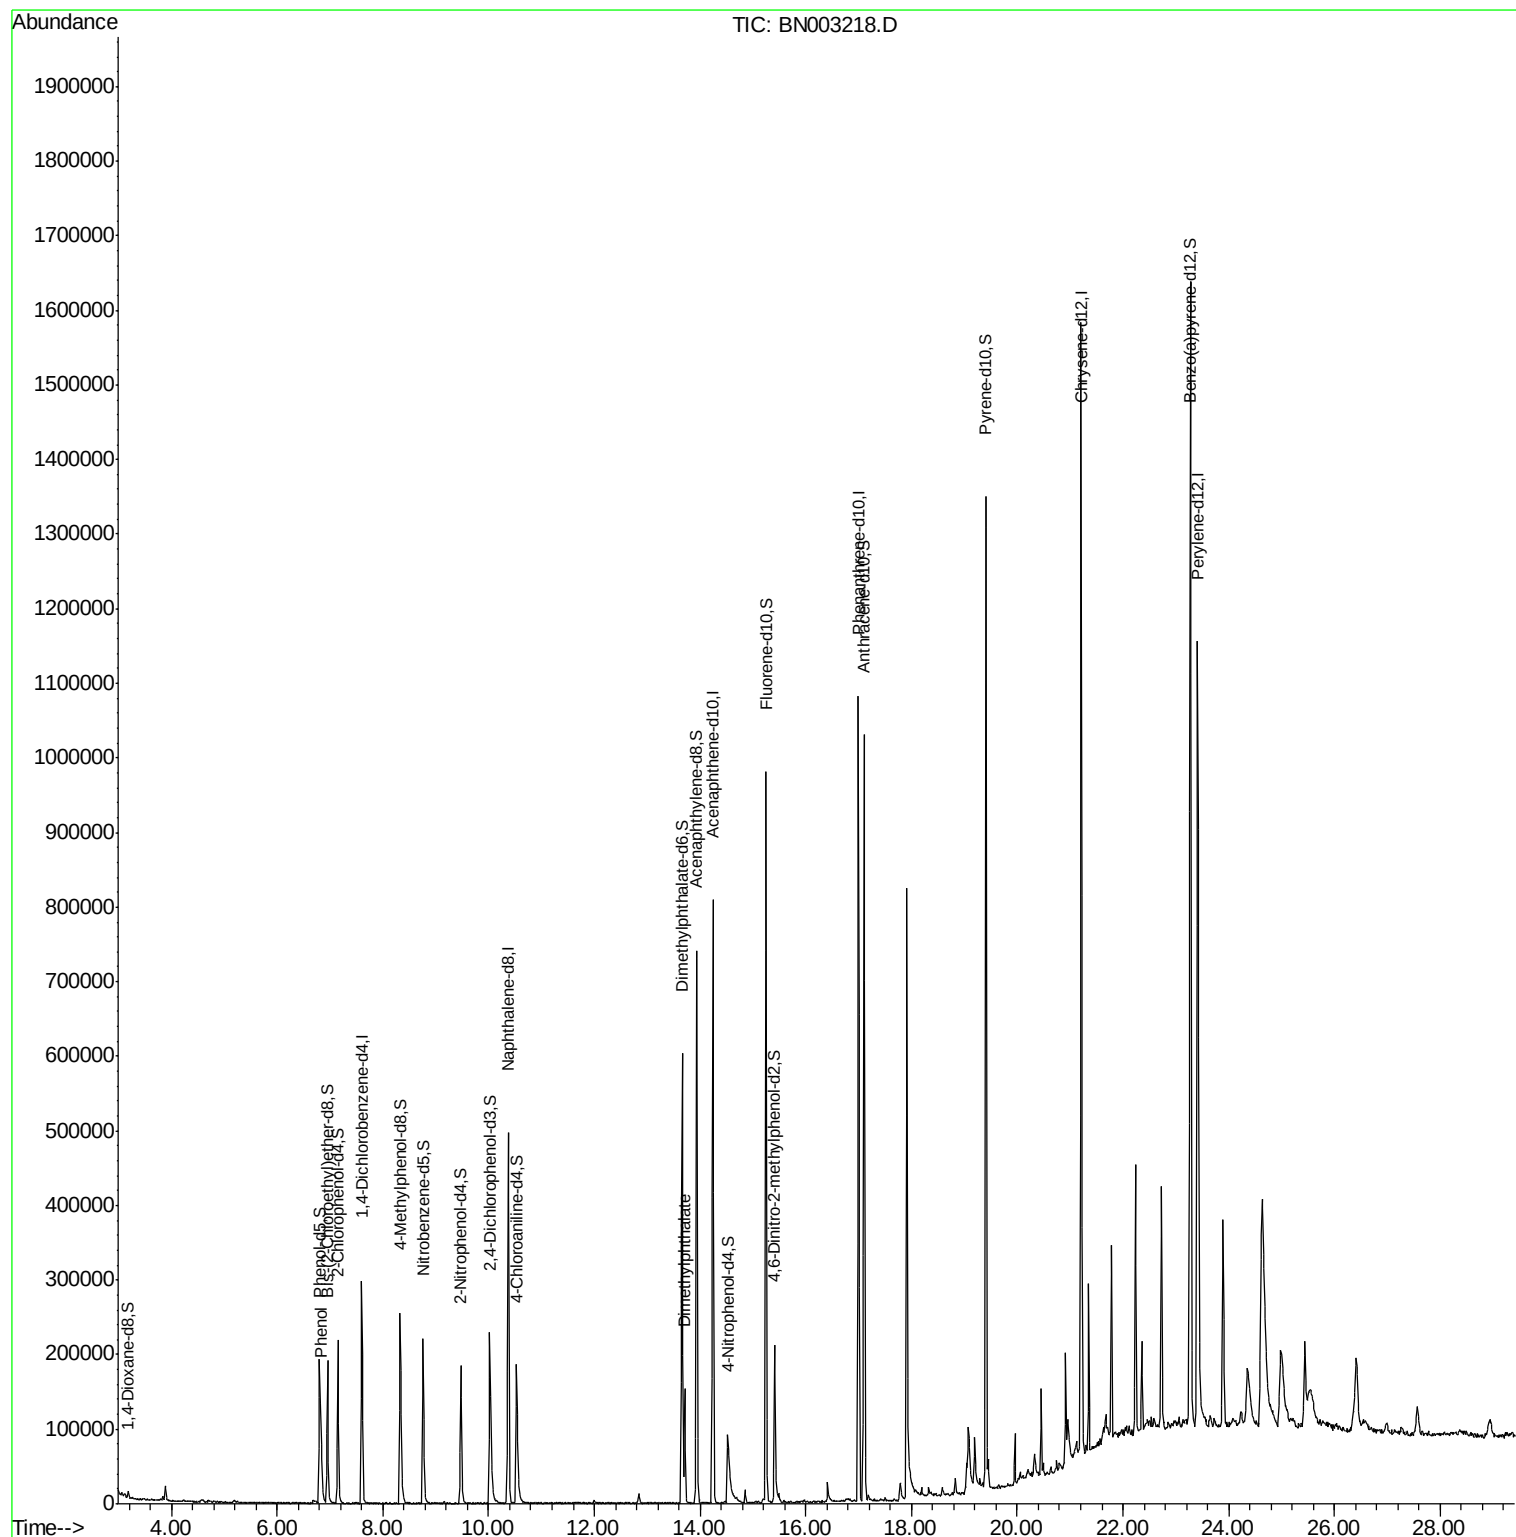

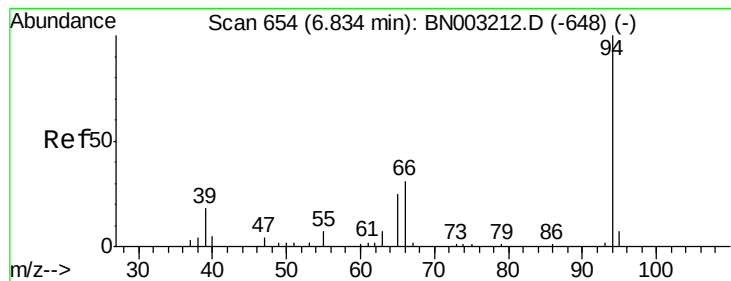


#6

Phenol

Concen: 5.424 ng/ul
 RT: 6.83 min Scan# 654
 Delta R.T. -0.00 min
 Lab File: BN003218.D
 Acq: 19 Oct 2018 21:57




Instrument :
 BNA_N
 ClientSampled :
 C0AH1

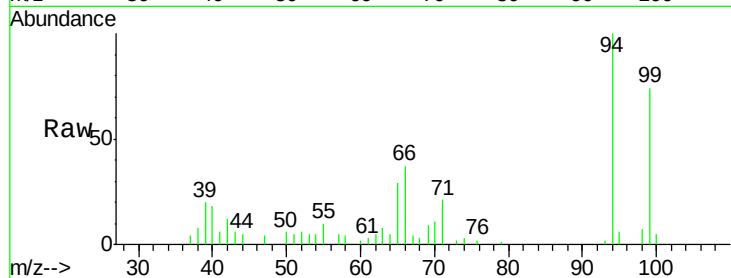

Tgt Ion: 94 Resp: 46493
 Ion Ratio Lower Upper
 94 100
 65 28.7 21.2 31.8
 66 36.9 27.4 41.2

Manual Integrations
 APPROVED

Sohil
 10/22/2018 4:52:51 PM

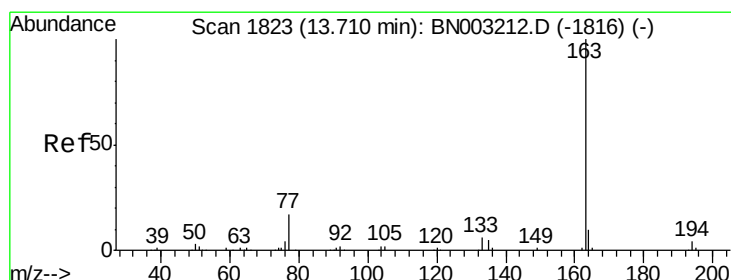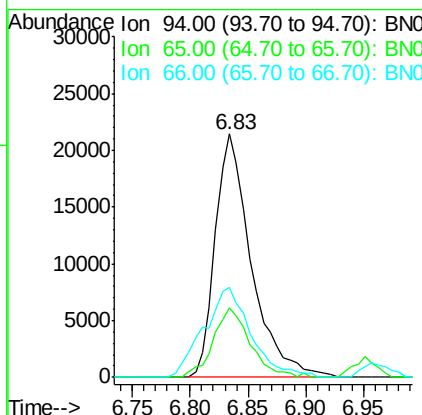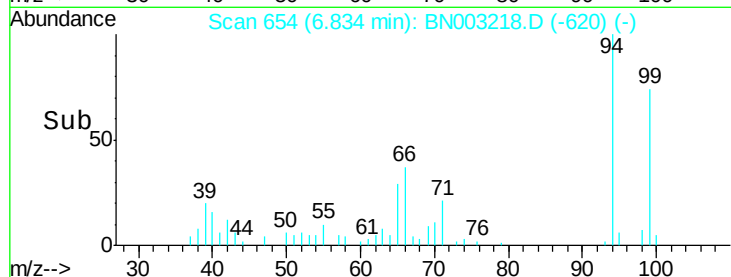

#44

Dimethylphthalate

Concen: 4.909 ng/ul
 RT: 13.71 min Scan# 1823
 Delta R.T. -0.00 min
 Lab File: BN003218.D
 Acq: 19 Oct 2018 21:57

Tgt Ion: 163 Resp: 112254
 Ion Ratio Lower Upper
 163 100
 194 4.2 3.7 5.5
 164 9.8 8.3 12.5

