

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101918\
 Data File : BN003220.D
 Acq On : 19 Oct 2018 23:07
 Operator : MJ/SJ
 Sample : J5567-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE8

Quant Time: Oct 20 05:08:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 20 05:04:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	101245	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	488520	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	295770	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	683599	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	725136	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	689664	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	9650	4.92	ng/uL	0.00
5) Phenol-d5	6.80	99	256194	26.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	163842	29.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	216975	29.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	226429	29.01	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	111947	29.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	134332	30.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	234349	29.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	245236	38.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	724277	28.74	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	934866	30.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	101544	29.24	ng/ul	0.01
57) Fluorene-d10	15.25	176	657515	29.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	118301	25.77	ng/ul	0.00
70) Anthracene-d10	17.10	188	999323	29.53	ng/ul	0.00
78) Pyrene-d10	19.40	212	1106822	31.50	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	1121734	30.08	ng/ul	0.00

Target Compounds


					Qvalue
6) Phenol	6.83	94	87396	9.058 ng/ul	99
44) Dimethylphthalate	13.71	163	159665	6.481 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101918\
Data File : BN003220.D
Acq On : 19 Oct 2018 23:07
Operator : MJ/SJ
Sample : J5567-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE8

Quant Time: Oct 20 05:08:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 20 05:04:06 2018
Response via : Initial Calibration

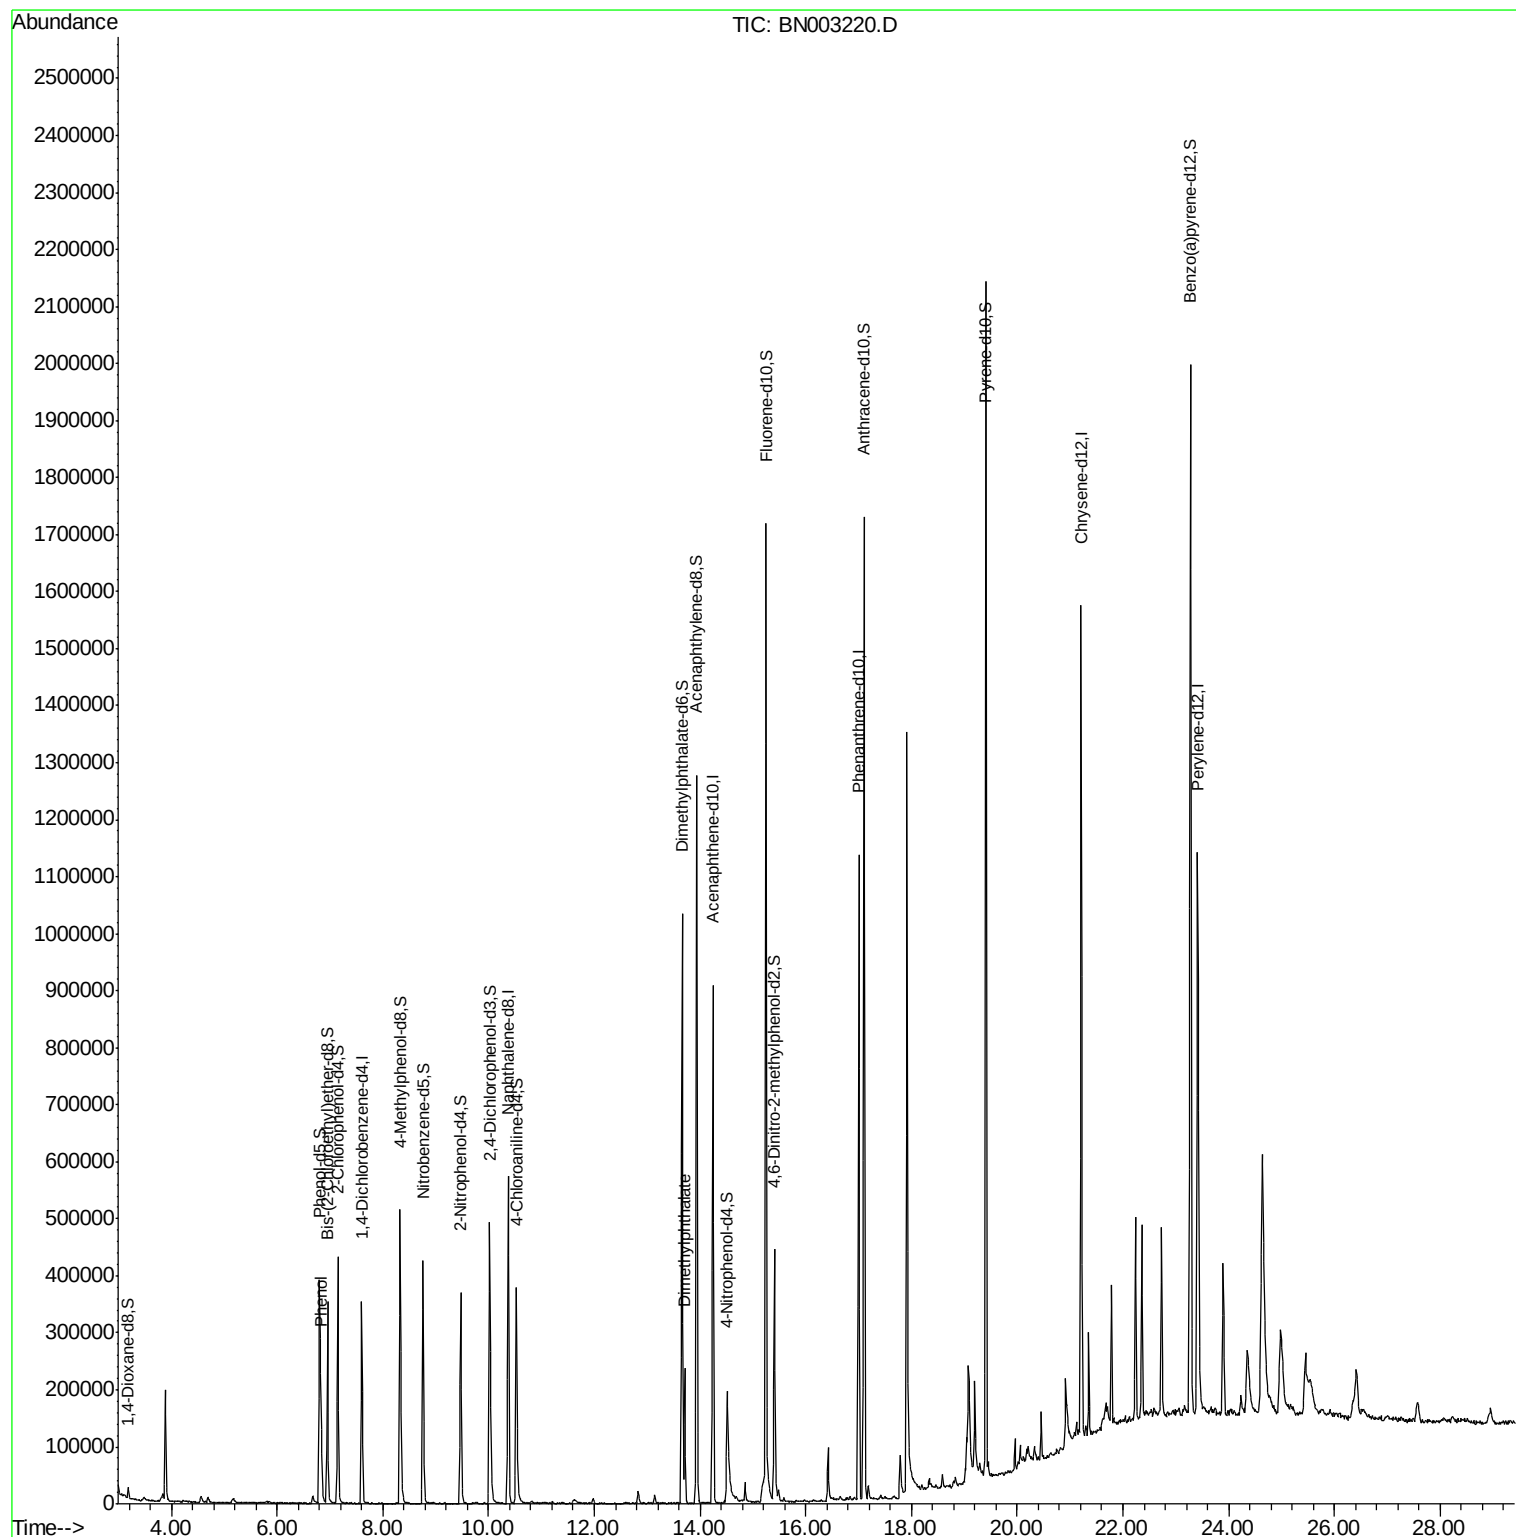

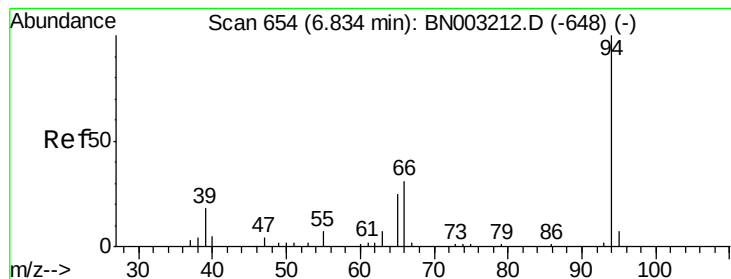

#6

Phenol

Concen: 9.058 ng/ul

RT: 6.83 min Scan# 654

Delta R.T. 0.00 min

Lab File: BN003220.D

Acq: 19 Oct 2018 23:07

Instrument :

BNA_N

ClientSampleId :

C0AE8


Tgt Ion: 94 Resp: 87396

Ion Ratio Lower Upper




94 100

65 26.9 21.2 31.8

66 35.4 27.4 41.2

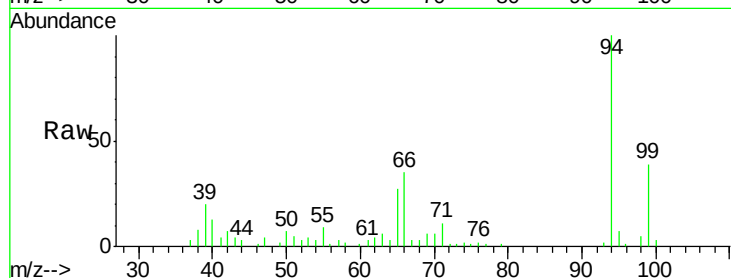

Abundance Ion 94.00 (93.70 to 94.70): BN003212.D (-648) (-)

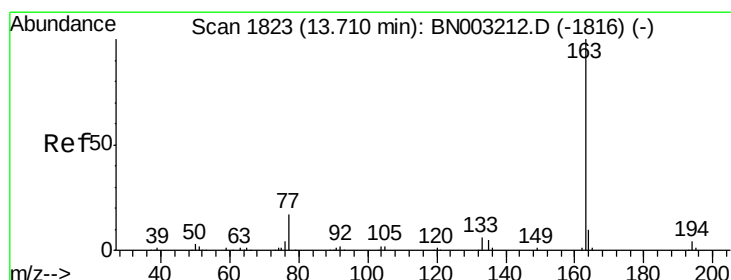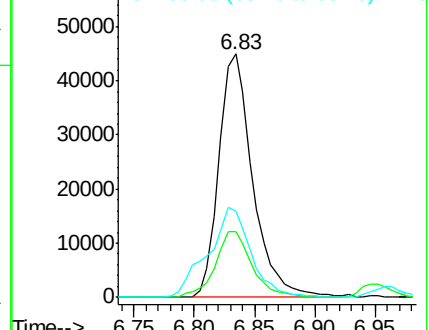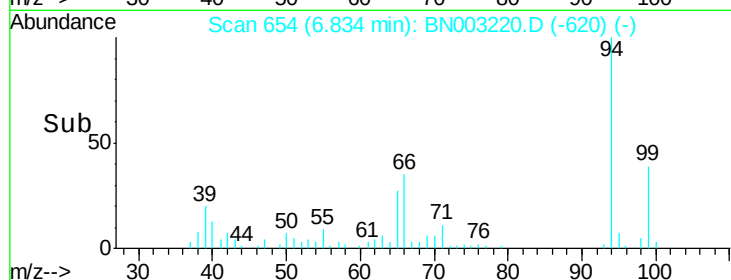

#44

Dimethylphthalate

Concen: 6.481 ng/ul

RT: 13.71 min Scan# 1823

Delta R.T. 0.00 min

Lab File: BN003220.D

Acq: 19 Oct 2018 23:07


Tgt Ion: 163 Resp: 159665

Ion Ratio Lower Upper

163 100

194 4.4 3.7 5.5

164 10.9 8.3 12.5

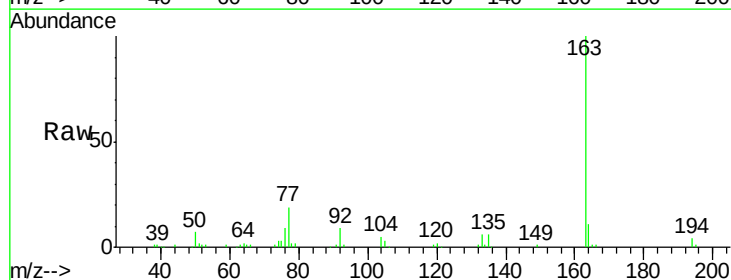

Abundance Ion 163.00 (162.70 to 163.70): BN003212.D (-1816) (-)

