

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101918\
 Data File : BN003222.D
 Acq On : 20 Oct 2018 00:17
 Operator : MJ/SJ
 Sample : J5567-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH8

Quant Time: Oct 20 05:09:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 20 05:04:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	97485	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	467977	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	284935	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	647689	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	701456	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	650421	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	11679	6.18	ng/uL	0.00
5) Phenol-d5	6.80	99	311929	33.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	186882	34.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	255792	35.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	262378	34.91	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	128712	35.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	153727	36.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	268852	35.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	352501	57.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	816849	33.64	ng/ul	0.00
46) Acenaphthylene-d8	13.94	160	1059631	35.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	124989	37.36	ng/ul	0.00
57) Fluorene-d10	15.24	176	748644	35.20	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	133615	30.71	ng/ul	0.00
70) Anthracene-d10	17.10	188	1151989	35.93	ng/ul	0.00
78) Pyrene-d10	19.41	212	1243767	36.59	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	1259156	35.81	ng/ul	0.00

Target Compounds


					Qvalue
6) Phenol	6.83	94	101010	10.873 ng/ul	97
44) Dimethylphthalate	13.71	163	171074	7.208 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101918\
Data File : BN003222.D
Acq On : 20 Oct 2018 00:17
Operator : MJ/SJ
Sample : J5567-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH8

Quant Time: Oct 20 05:09:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 20 05:04:06 2018
Response via : Initial Calibration

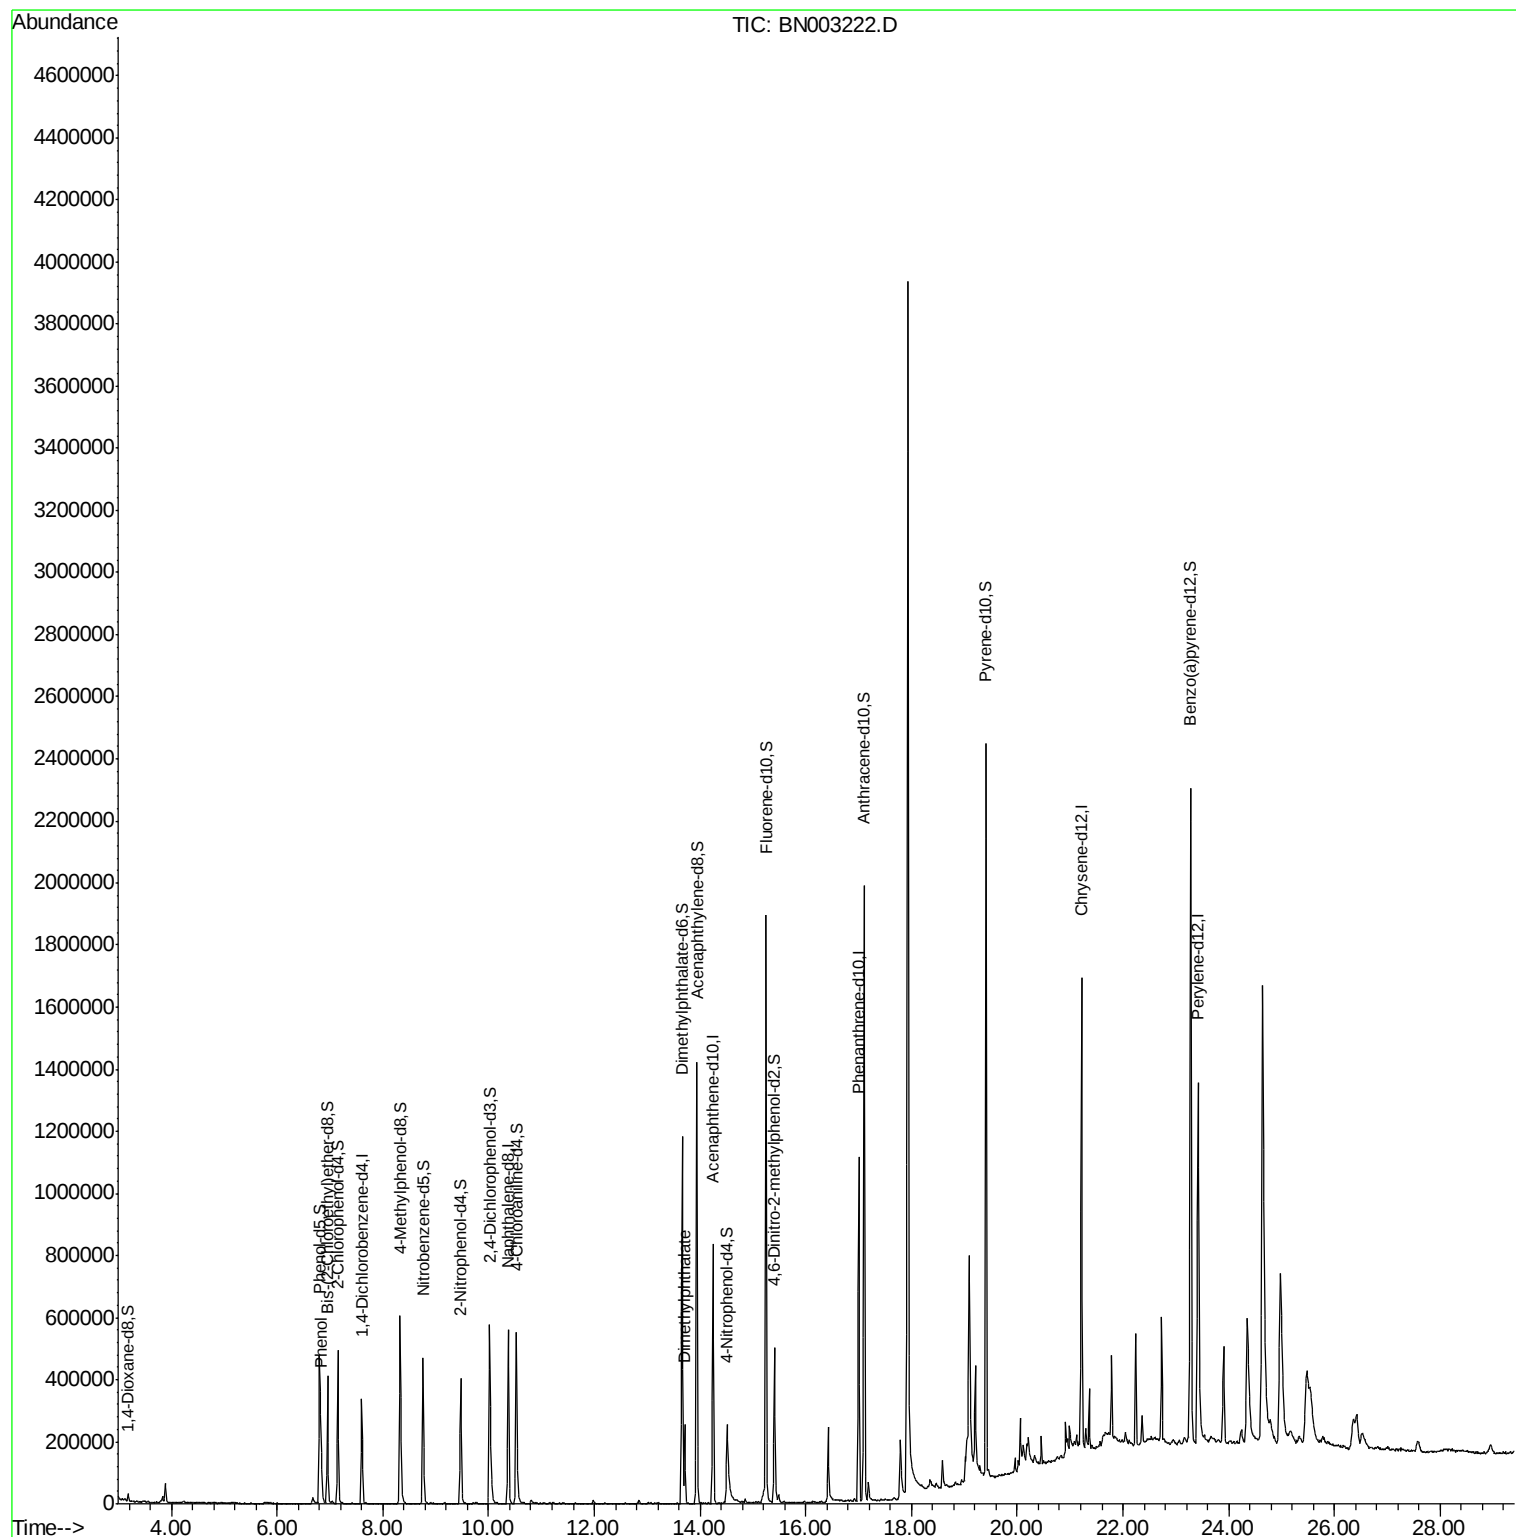

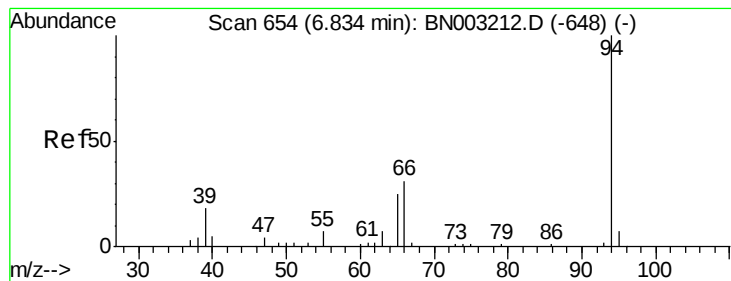


#6

Phenol




Concen: 10.873 ng/ul
 RT: 6.83 min Scan# 654
 Delta R.T. -0.00 min
 Lab File: BN003222.D
 Acq: 20 Oct 2018 00:17

Instrument :
 BNA_N
 ClientSampleId :
 C0AH8

Tgt Ion: 94 Resp: 101010
 Ion Ratio Lower Upper
 94 100
 65 28.3 21.2 31.8
 66 36.1 27.4 41.2

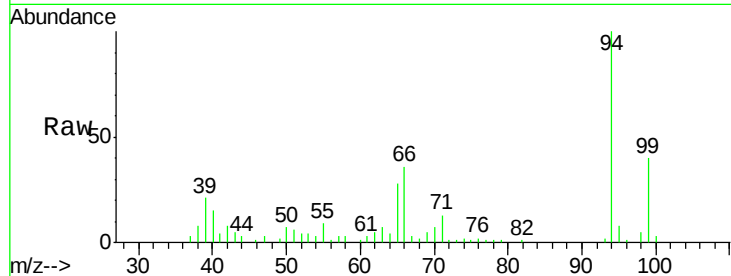

Abundance Ion 94.00 (93.70 to 94.70): BN0
 Ion 65.00 (64.70 to 65.70): BN0
 Ion 66.00 (65.70 to 66.70): BN0

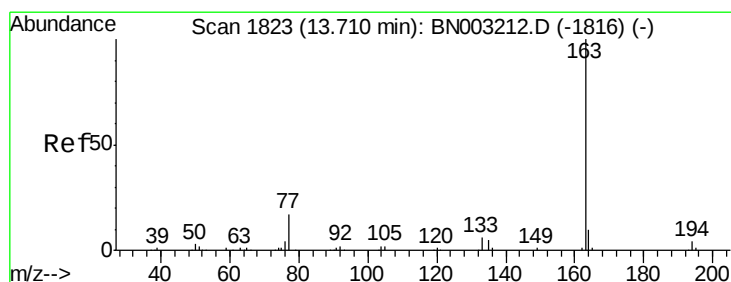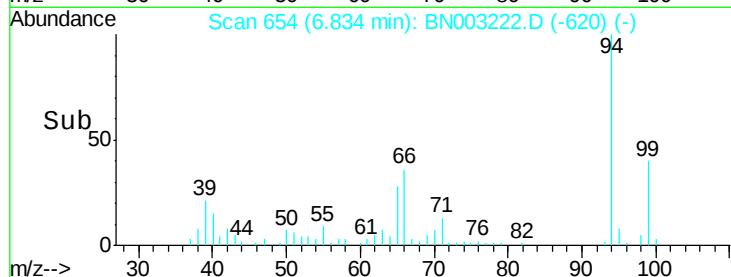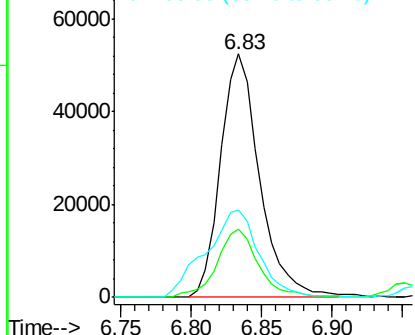


#44

Dimethylphthalate

Concen: 7.208 ng/ul
 RT: 13.71 min Scan# 1823
 Delta R.T. -0.00 min
 Lab File: BN003222.D
 Acq: 20 Oct 2018 00:17

Tgt Ion: 163 Resp: 171074
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.7 5.5
 164 9.9 8.3 12.5

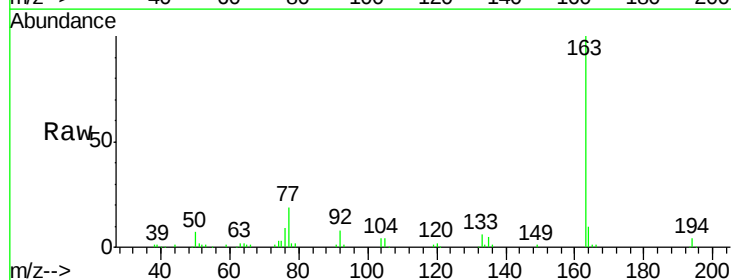

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

