

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101918\
 Data File : BN003229.D
 Acq On : 20 Oct 2018 04:26
 Operator : MJ/SJ
 Sample : J5567-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ1

Manual Integrations
 APPROVED

Sohil
 10/22/2018 4:53:03 PM

Quant Time: Oct 20 06:46:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 20 06:06:40 2018
 Response via : Initial Calibration




Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	98732	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	487804	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	313677	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	736150	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	814031	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	792702	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	832	0.43	ng/uL	0.00
5) Phenol-d5	6.83	99	22101	2.36	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	6.96	67	13164	2.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	19061	2.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	18610	2.44	ng/ul	0.03
19) Nitrobenzene-d5	8.78	128	7541	1.99	ng/ul	0.02
22) 2-Nitrophenol-d4	9.49	143	9073	2.07	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	10.08	165	17808m	2.24	ng/ul	0.05
29) 4-Chloroaniline-d4	10.56	131	24126m	3.76	ng/ul	0.03
43) Dimethylphthalate-d6	13.67	166	62779	2.35	ng/ul	0.00
46) Acenaphthylene-d8	13.94	160	81462	2.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	5230m	1.42	ng/ul	0.12
57) Fluorene-d10	15.26	176	61952	2.65	ng/ul	0.01
62) 4,6-Dinitro-2-methylphenol	15.44	200	4210	0.85	ng/ul	0.04
70) Anthracene-d10	17.11	188	94000	2.58	ng/ul	0.01
78) Pyrene-d10	19.42	212	107838	2.73	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	114478	2.67	ng/ul	0.00

Target Compounds					Qvalue	
44) Dimethylphthalate	13.72	163	32971	1.262	ng/ul#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

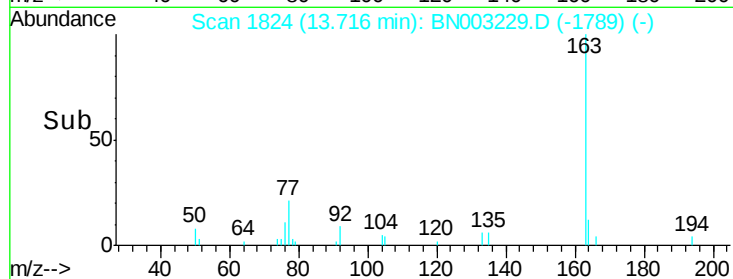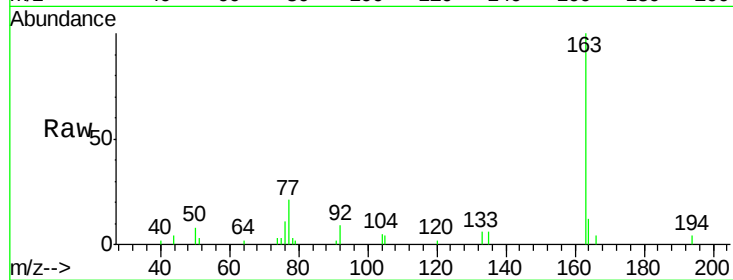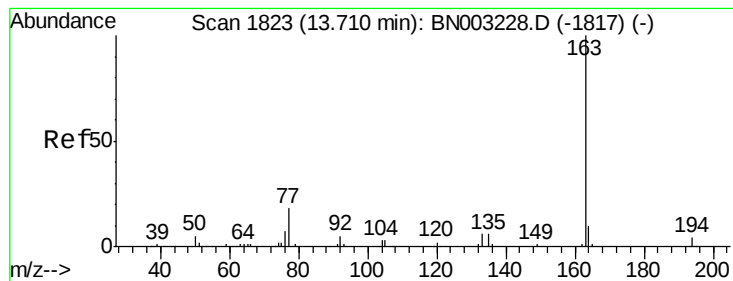

#44

Dimethylphthalate

Concen: 1.262 ng/ul

RT: 13.72 min Scan# 1824

Delta R.T. 0.01 min

Lab File: BN003229.D

Acq: 20 Oct 2018 04:26

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.6	3.7	5.5#
164	12.0	8.3	12.5

Instrument :

BNA_N

ClientSampleId :

C0AJ1

Manual Integrations
APPROVED

Sohil
10/22/2018 4:53:03 PM

