

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101919\  
 Data File : BN008262.D  
 Acq On : 19 Oct 2019 10:29  
 Operator : JU  
 Sample : K5177-05DL 5X  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 BEP94DL

Quant Time: Oct 19 20:51:24 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Oct 18 23:47:17 2019  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|---------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.59  | 152  | 1801     | 0.40 | ng/ul | 0.00     |
| 2) Naphthalene-d8         | 10.36 | 136  | 8294     | 0.40 | ng/ul | 0.00     |
| 6) Acenaphthene-d10       | 14.23 | 164  | 5137     | 0.40 | ng/ul | 0.00     |
| 10) Phenanthrene-d10      | 16.97 | 188  | 11184    | 0.40 | ng/ul | 0.00     |
| 16) Chrysene-d12          | 21.18 | 240  | 12469    | 0.40 | ng/ul | 0.00     |
| 20) Perylene-d12          | 23.35 | 264  | 12912    | 0.40 | ng/ul | -0.01    |

|                             |       |     |      |      |       |      |
|-----------------------------|-------|-----|------|------|-------|------|
| System Monitoring Compounds |       |     |      |      |       |      |
| 4) 2-Methylnaphthalene-d10  | 11.96 | 152 | 473  | 0.03 | ng/ul | 0.00 |
| 14) Fluoranthene-d10        | 19.01 | 212 | 2228 | 0.06 | ng/ul | 0.00 |


|                            |       |     |        |        |        |     |
|----------------------------|-------|-----|--------|--------|--------|-----|
| Target Compounds           |       |     |        | Ovalue |        |     |
| 3) Naphthalene             | 10.41 | 128 | 1136   | 0.048  | ng/ul# | 82  |
| 5) 2-Methylnaphthalene     | 12.03 | 142 | 661    | 0.041  | ng/ul  | 98  |
| 7) Acenaphthylene          | 13.94 | 152 | 3812   | 0.156  | ng/ul  | 96  |
| 8) Acenaphthene            | 14.29 | 153 | 1854   | 0.097  | ng/ul  | 97  |
| 9) Fluorene                | 15.28 | 166 | 2476   | 0.115  | ng/ul# | 97  |
| 12) Phenanthrene           | 17.02 | 178 | 53536  | 1.635  | ng/ul  | 99  |
| 13) Anthracene             | 17.11 | 178 | 10390  | 0.361  | ng/ul  | 98  |
| 15) Fluoranthene           | 19.04 | 202 | 144437 | 3.340  | ng/ul  | 99  |
| 17) Pyrene                 | 19.40 | 202 | 158398 | 3.190  | ng/ul  | 100 |
| 18) Benzo(a)anthracene     | 21.16 | 228 | 94019  | 2.074  | ng/ul  | 98  |
| 19) Chrysene               | 21.22 | 228 | 105583 | 1.898  | ng/ul  | 98  |
| 21) Benzo(b)fluoranthene   | 22.71 | 252 | 169239 | 4.026  | ng/ul  | 92  |
| 22) Benzo(k)fluoranthene   | 22.88 | 252 | 14184  | 0.298  | ng/ul  | 93  |
| 23) Benzo(a)pyrene         | 23.26 | 252 | 93007  | 2.103  | ng/ul# | 85  |
| 24) Indeno(1,2,3-cd)pyrene | 25.51 | 276 | 53983  | 1.036  | ng/ul# | 99  |
| 25) Dibenzo(a,h)anthracene | 25.52 | 278 | 13604  | 0.330  | ng/ul  | 96  |
| 26) Benzo(a,h,i)perylene   | 26.17 | 276 | 48865  | 1.023  | ng/ul  | 98  |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101919\  
Data File : BN008262.D  
Acq On : 19 Oct 2019 10:29  
Operator : JU  
Sample : K5177-05DL 5X  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
BEP94DL

Quant Time: Oct 19 20:51:24 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 18 23:47:17 2019  
Response via : Initial Calibration

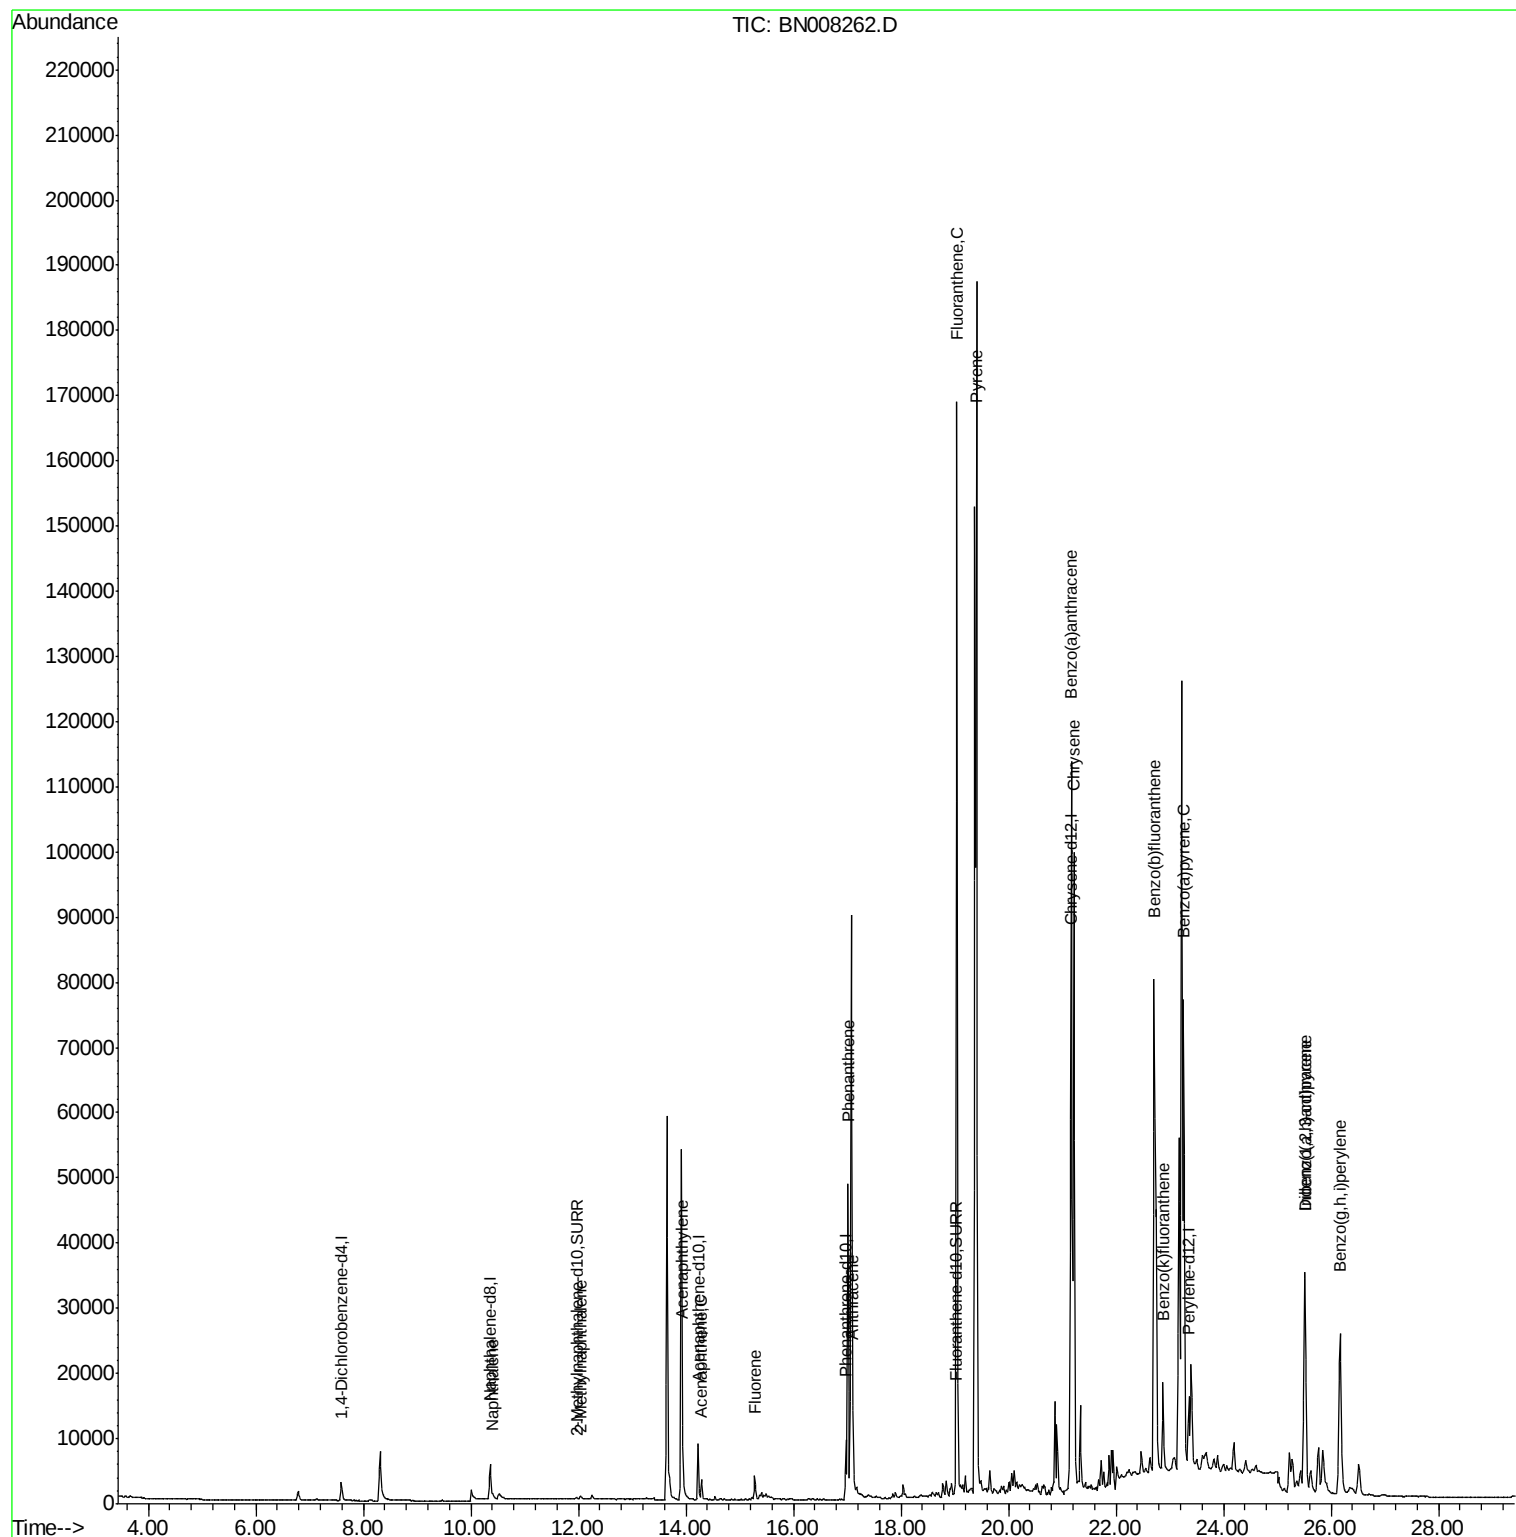

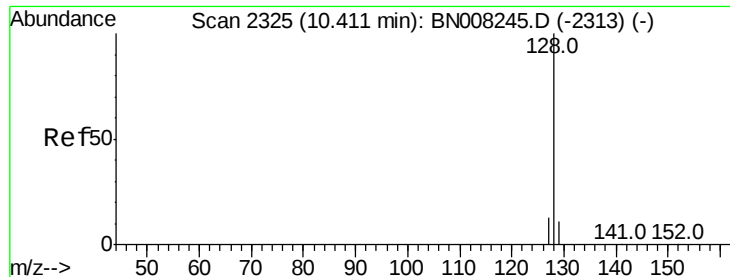

#3

Naphthalene

Concen: 0.048 ng/ul

RT: 10.41 min Scan# 2324

Delta R.T. -0.01 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29

Instrument :

BNA\_N

ClientSampleId :

BEP94DL


Tot Ion:128 Resp: 1136

Ion Ratio Lower Upper

128 100

129 20.3 9.8 14.8#

127 20.5 11.1 16.7#

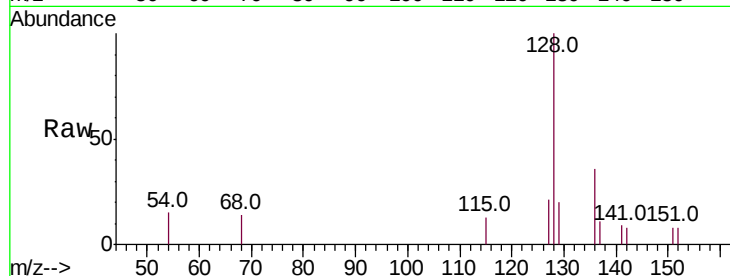

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

10.41

600



400

200

0

Time-->

10.30 10.40 10.50

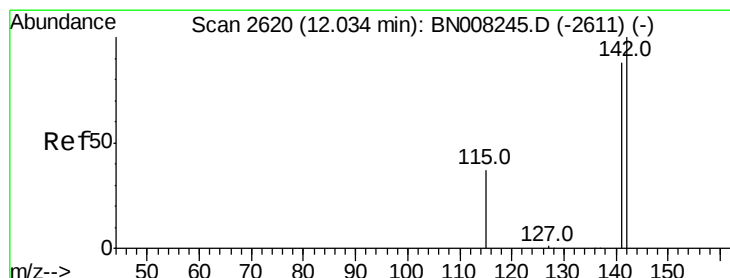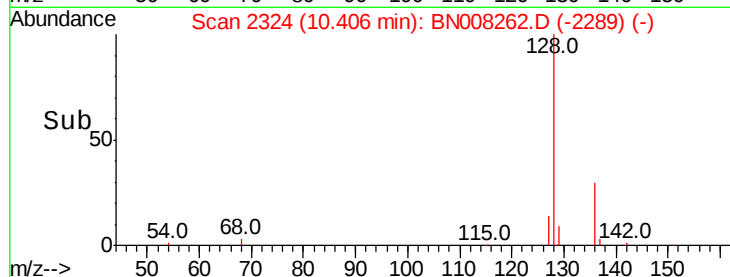

#5

2-Methylnaphthalene

Concen: 0.041 ng/ul

RT: 12.03 min Scan# 2620

Delta R.T. 0.00 min

Lab File: BN008262.D


Acq: 19 Oct 2019 10:29

Tgt Ion:142 Resp: 661

Ion Ratio Lower Upper

142 100

141 87.7 71.4 107.2

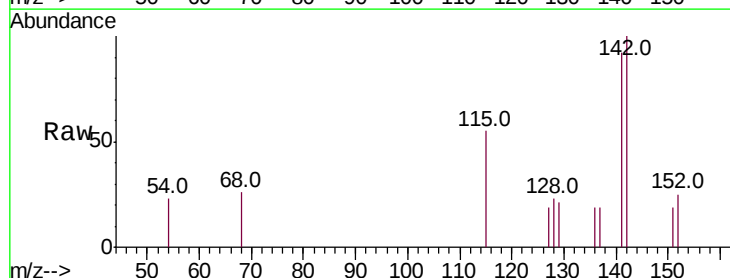

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

12.03

300

250

200


150


100

50

Time-->

12.00 12.10 12.20

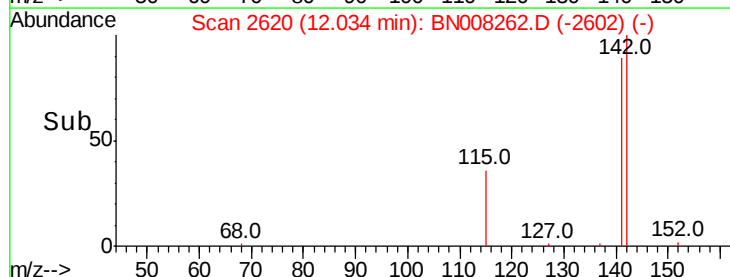

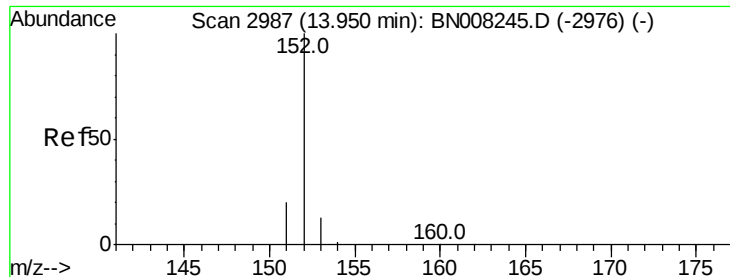

#7

Acenaphthylene

Concen: 0.156 ng/ul

RT: 13.94 min Scan# 2985

Delta R.T. -0.01 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29

Instrument :

BNA\_N

ClientSampleId :

BEP94DL


Tot Ion:152 Resp: 3812

Ion Ratio Lower Upper

152 100

151 21.7 16.2 24.4




153 16.0 11.0 16.4

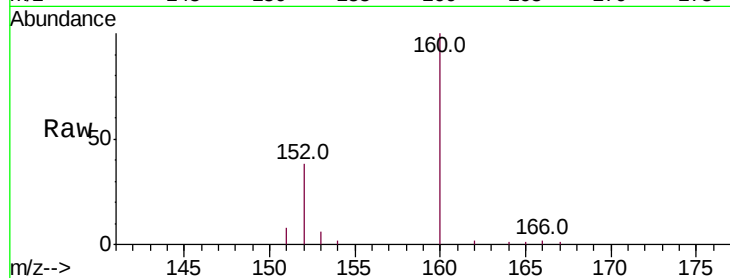

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

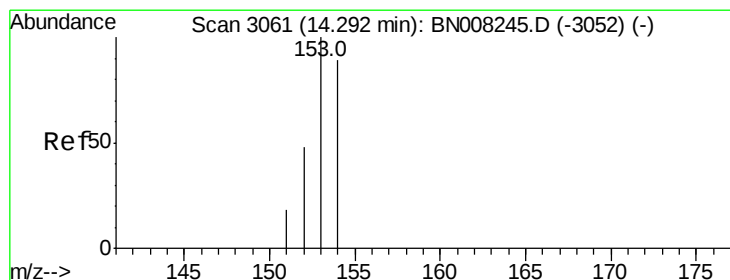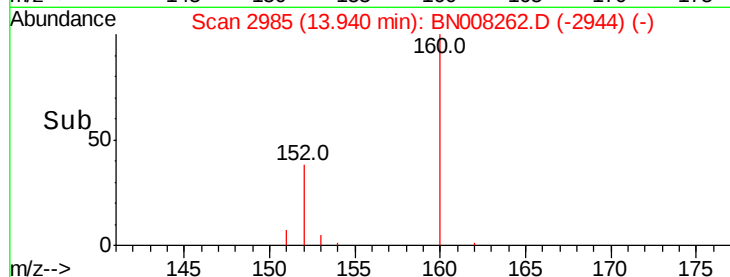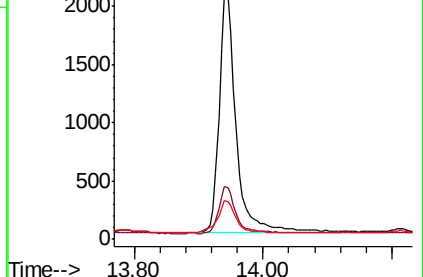

#8

Acenaphthene

Concen: 0.097 ng/ul

RT: 14.29 min Scan# 3060

Delta R.T. -0.00 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29


Tgt Ion:153 Resp: 1854

Ion Ratio Lower Upper

153 100

152 51.5 38.2 57.2



154 91.4 71.8 107.8

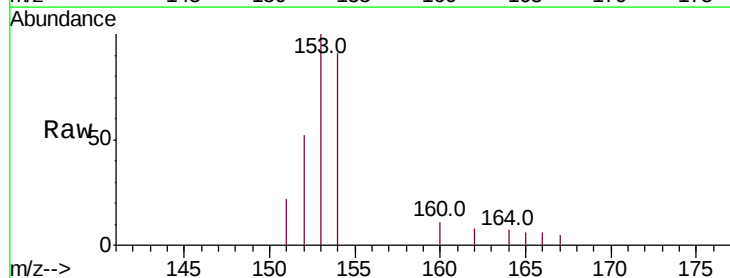


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

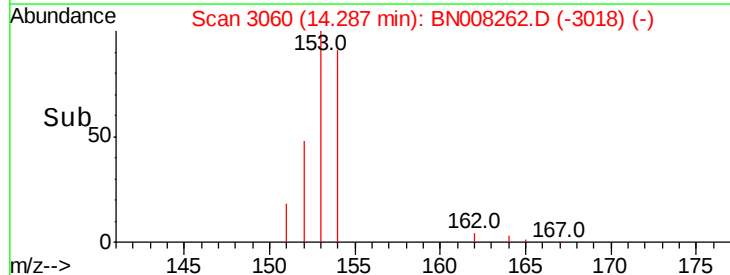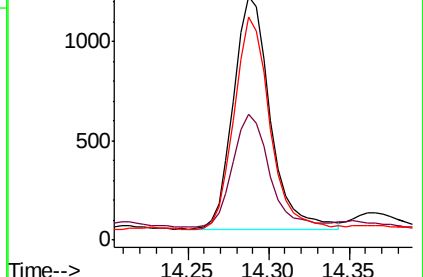

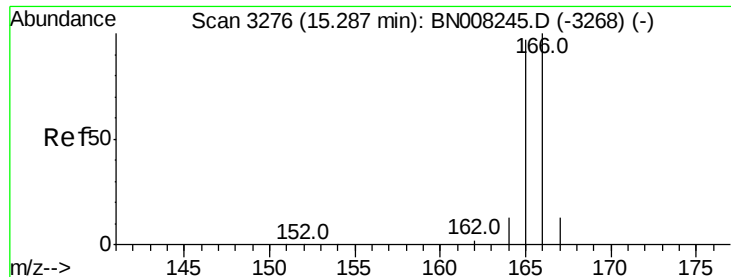

#9

Fluorene

Concen: 0.115 ng/ul

RT: 15.28 min Scan# 3275

Delta R.T. -0.00 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29

Instrument :

BNA\_N

ClientSampleId :

BEP94DL





Tot Ion:166 Resp: 2476

Ion Ratio Lower Upper

166 100

165 98.2 76.6 115.0

167 18.2 11.7 17.5#

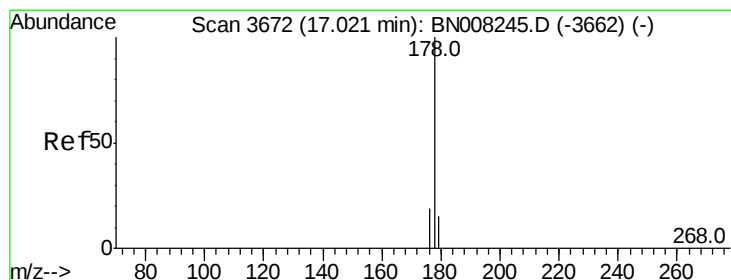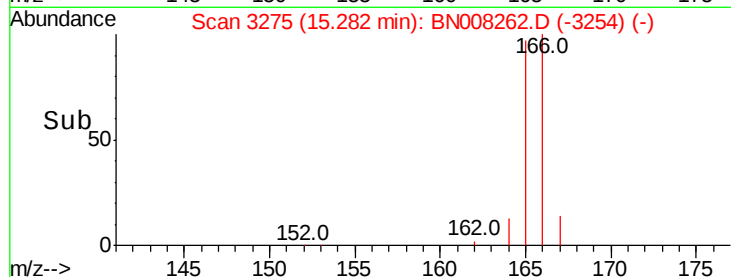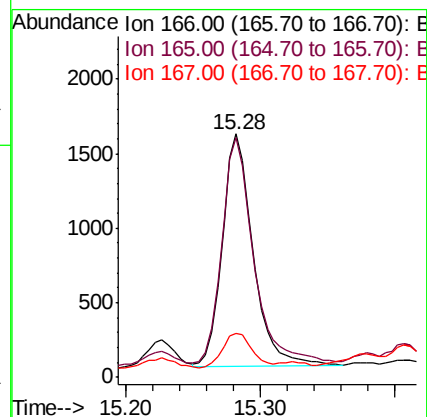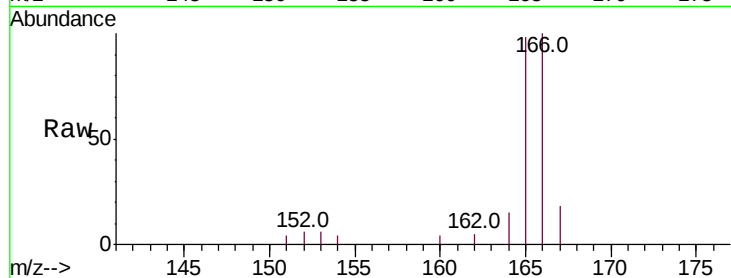

#12

Phenanthrene

Concen: 1.635 ng/ul

RT: 17.02 min Scan# 3671

Delta R.T. -0.00 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29




Tgt Ion:178 Resp: 53536


Ion Ratio Lower Upper

178 100

179 15.7 12.8 19.2

176 18.5 15.4 23.2

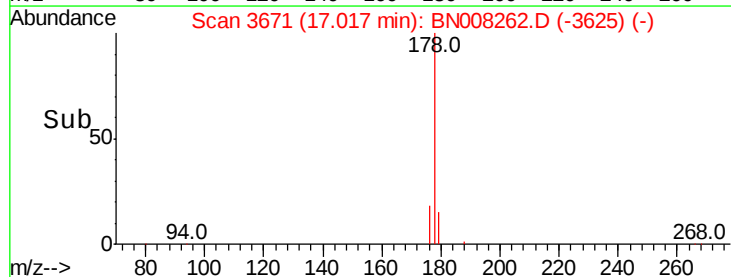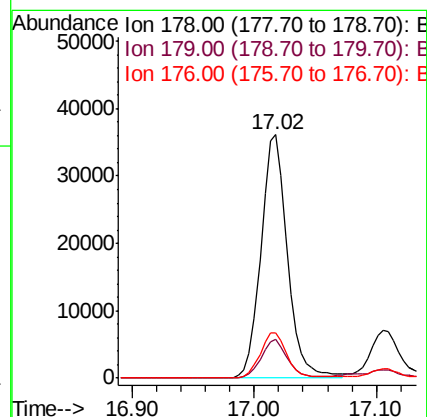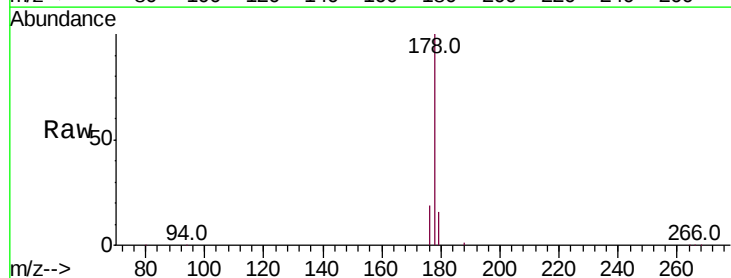

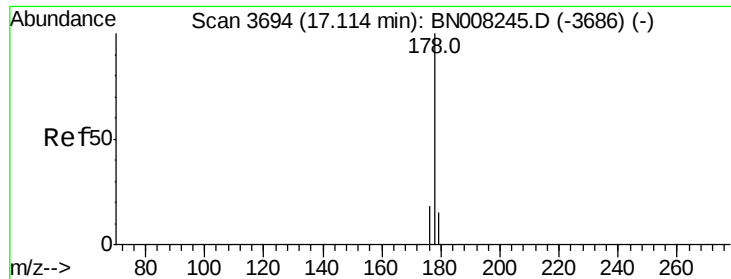

#13

Anthracene

Concen: 0.361 ng/ul

RT: 17.11 min Scan# 3692

Delta R.T. -0.01 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29

Instrument :

BNA\_N

ClientSampleId :

BEP94DL


Tot Ion:178 Resp: 10390

Ion Ratio Lower Upper

178 100

179 17.4 13.0 19.6




176 19.1 15.0 22.6

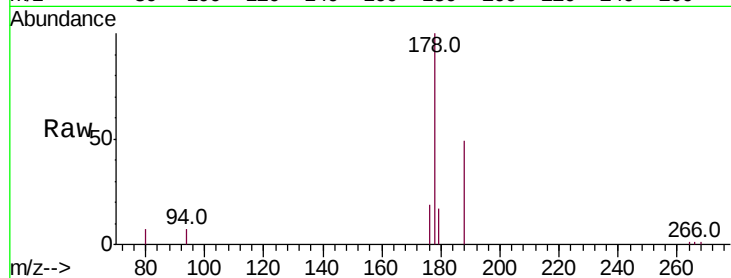

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

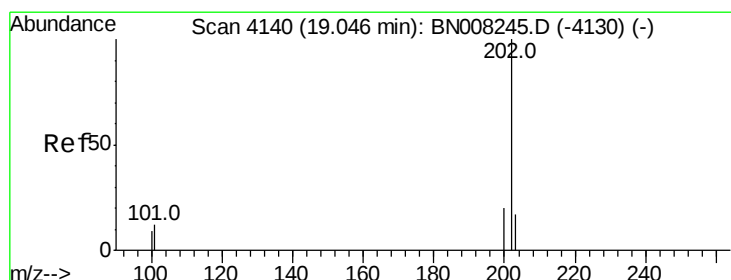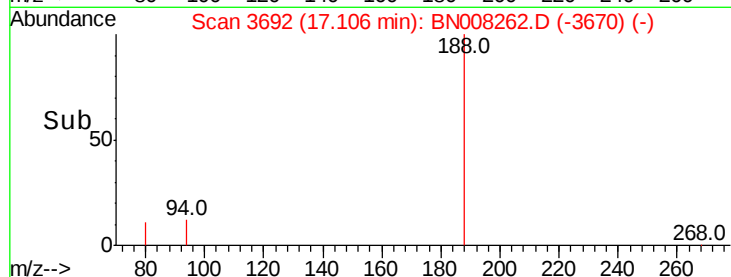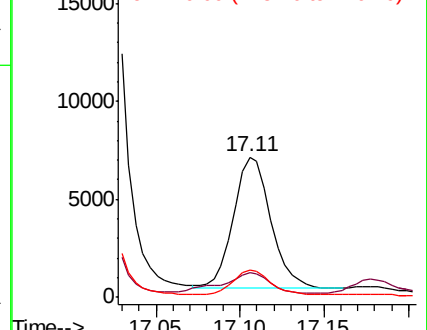

#15

Fluoranthene

Concen: 3.340 ng/ul

RT: 19.04 min Scan# 4139

Delta R.T. -0.00 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29


Tgt Ion:202 Resp: 144437

Ion Ratio Lower Upper

202 100

101 11.7 0.0 31.2



100 8.7 0.0 28.5

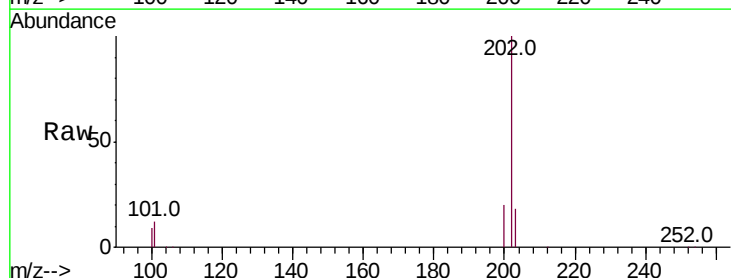


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

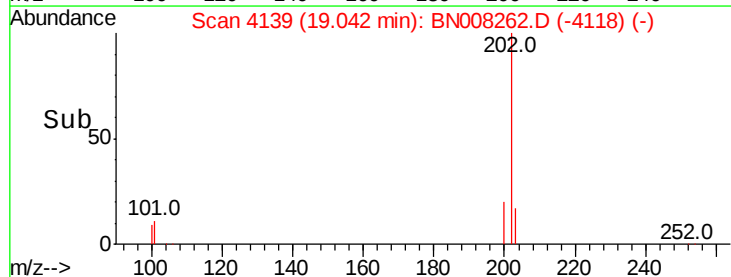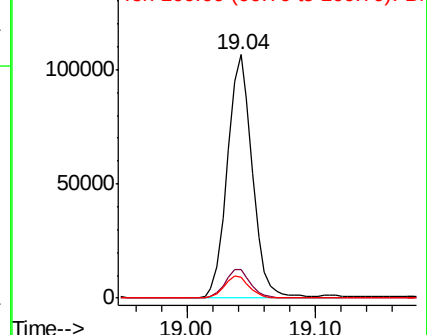

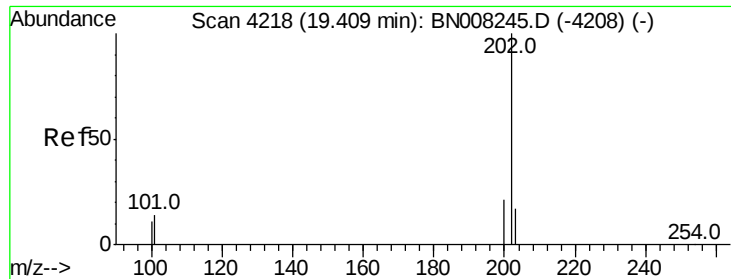

#17

Pvrene

Concen: 3.190 ng/ul

RT: 19.40 min Scan# 4217

Delta R.T. -0.00 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29

Instrument :

BNA\_N

ClientSampleId :

BEP94DL


Tot Ion:202 Resp: 158398

Ion Ratio Lower Upper

202 100

101 13.7 10.9 16.3




100 11.0 8.7 13.1

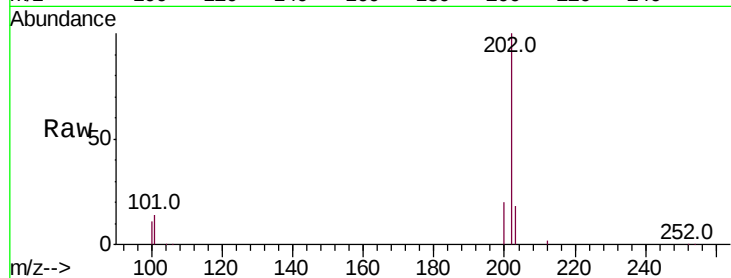

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

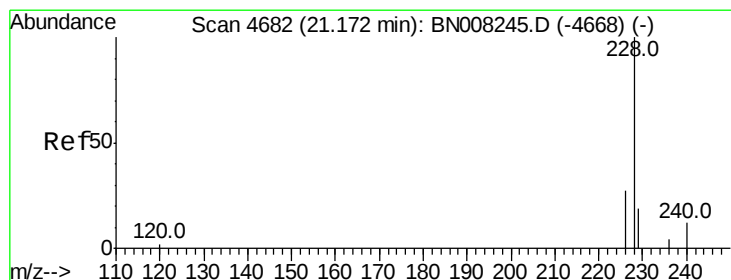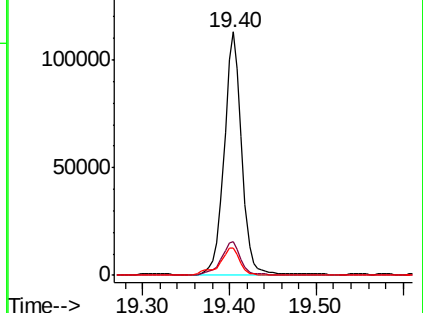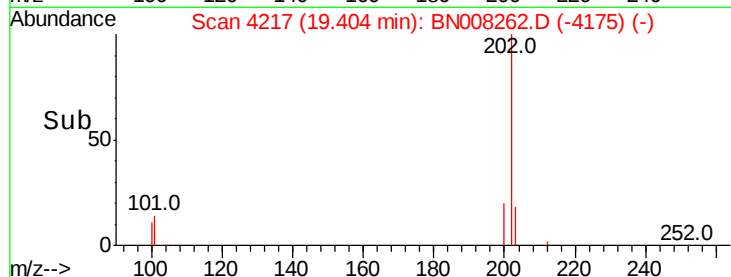

#18

Benzo(a)anthracene

Concen: 2.074 ng/ul

RT: 21.16 min Scan# 4679

Delta R.T. -0.01 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29


Tgt Ion:228 Resp: 94019

Ion Ratio Lower Upper

228 100

229 20.9 16.2 24.2



226 27.7 21.4 32.0

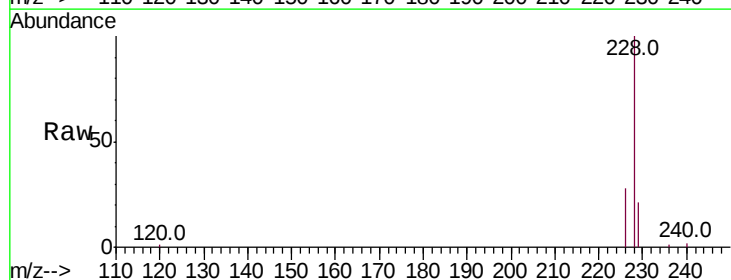


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

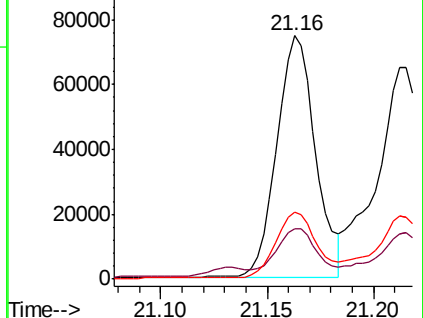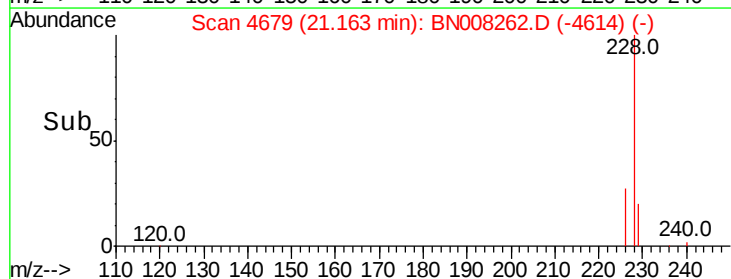

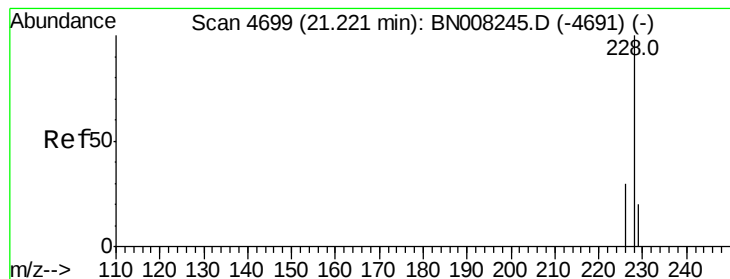

#19

Chrysene

Concen: 1.898 ng/ul

RT: 21.22 min Scan# 4697

Delta R.T. -0.01 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29

Instrument :

BNA\_N

ClientSampleId :

BEP94DL


Tot Ion:228 Resp: 105583

Ion Ratio Lower Upper

228 100

226 29.3 24.1 36.1




229 21.8 16.2 24.2

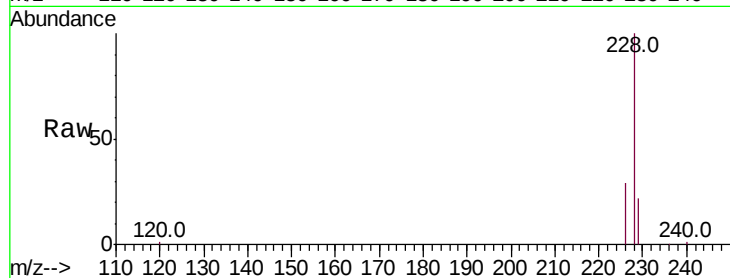

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

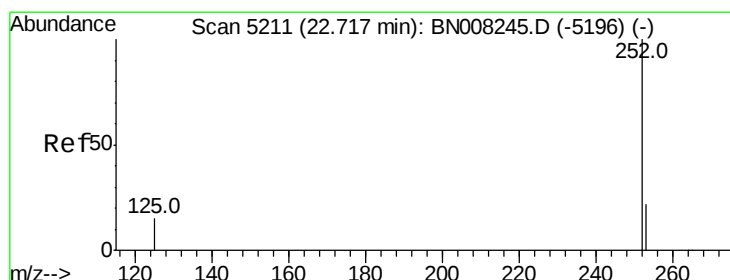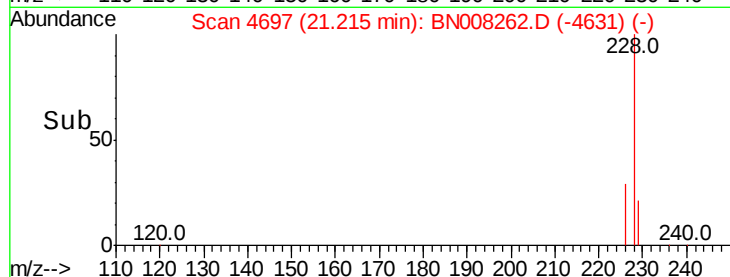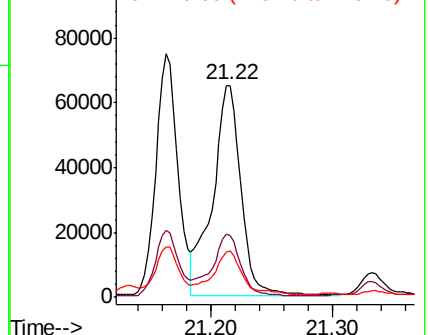

#21

Benzo(b)fluoranthene

Concen: 4.026 ng/ul

RT: 22.71 min Scan# 5208

Delta R.T. -0.01 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29


Tgt Ion:252 Resp: 169239

Ion Ratio Lower Upper

252 100

253 23.2 0.0 53.4



125 11.9 0.0 32.4

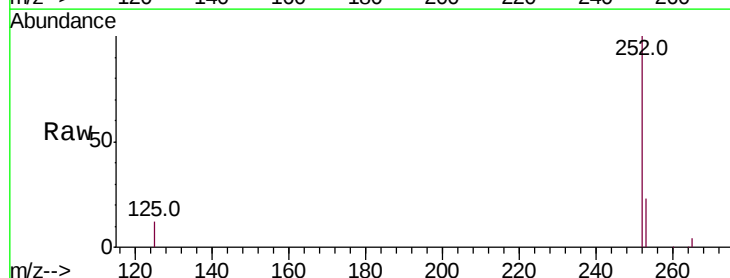


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

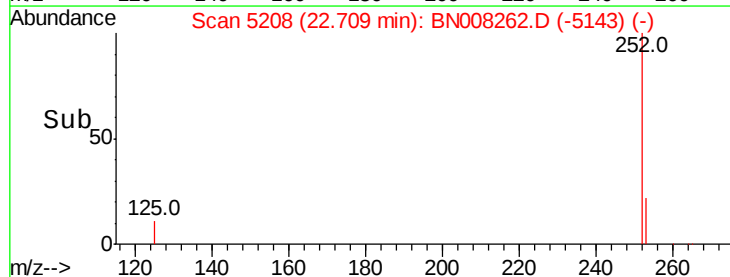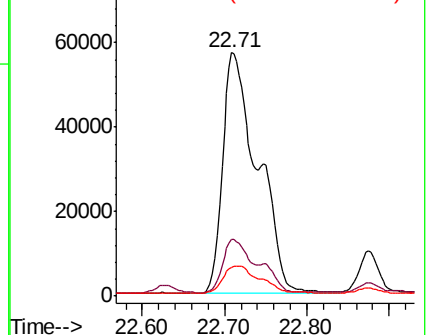

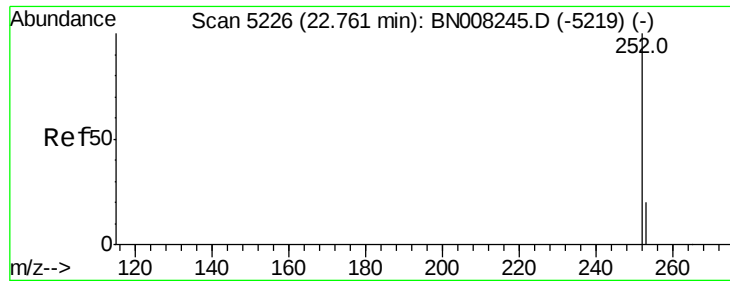

#22

Benzo(k)fluoranthene

Concen: 0.298 ng/ul

RT: 22.88 min Scan# 5265

Delta R.T. 0.11 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29

Instrument :

BNA\_N

ClientSampleId :

BEP94DL


Tot Ion:252 Resp: 14184

Ion Ratio Lower Upper

252 100

253 29.9 21.3 31.9




125 18.5 12.3 18.5

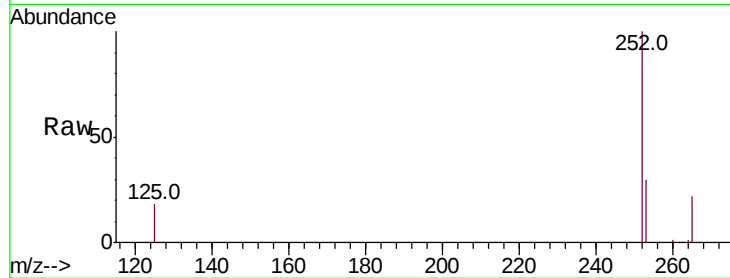

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

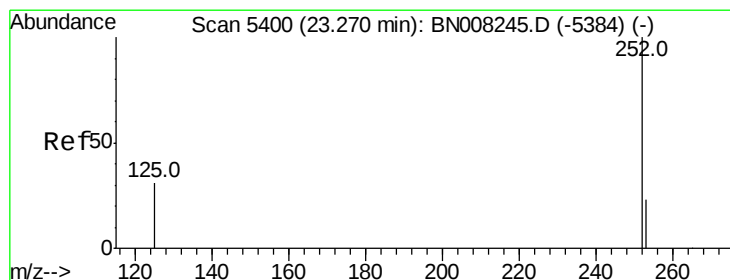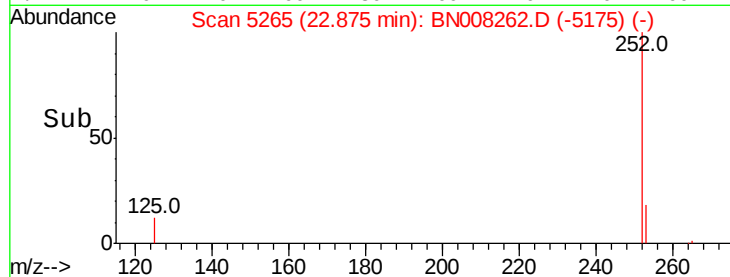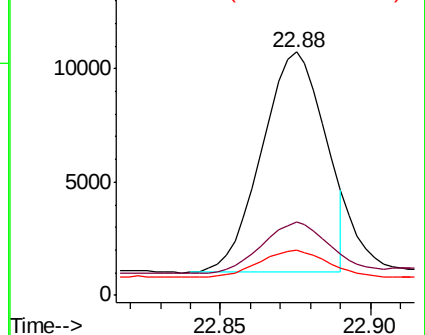

#23

Benzo(a)pyrene

Concen: 2.103 ng/ul

RT: 23.26 min Scan# 5396

Delta R.T. -0.01 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29


Tgt Ion:252 Resp: 93007

Ion Ratio Lower Upper

252 100

253 23.3 22.8 34.2



125 13.0 18.4 27.6#

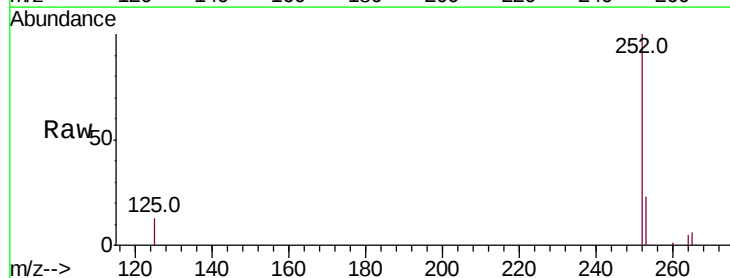


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

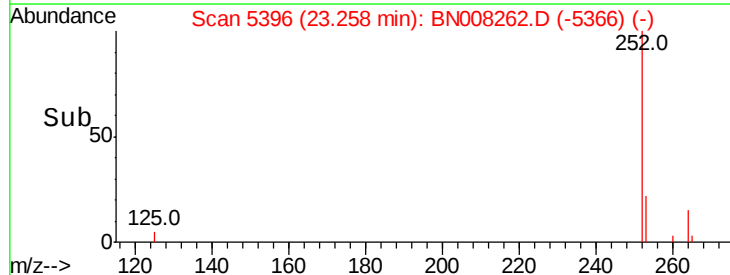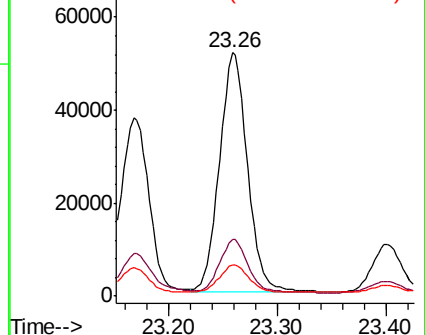


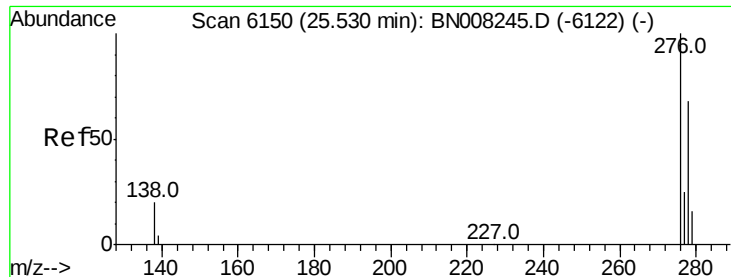




#24  
 Indeno(1,2,3-cd)pyrene  
 Concen: 1.036 ng/ul  
 RT: 25.51 min Scan# 6144  
 Delta R.T. -0.02 min  
 Lab File: BN008262.D  
 Acq: 19 Oct 2019 10:29

Instrument :  
 BNA\_N  
 ClientSampleId :  
 BEP94DL

Tot Ion:276 Resp: 53983  
 Ion Ratio Lower Upper  
 276 100  
 138 19.4 16.1 24.1  
 227 0.1 0.2 0.2#

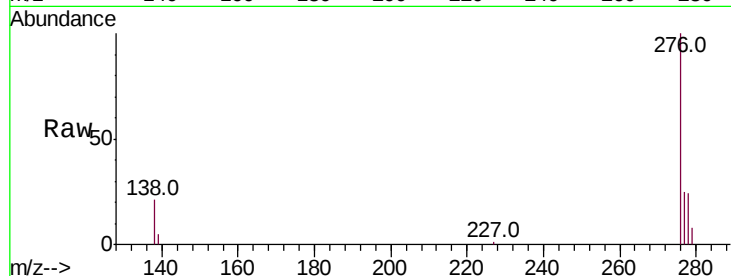


Abundance Ion 276.00 (275.70 to 276.70): E  
 Ion 138.00 (137.70 to 138.70): E  
 Ion 227.00 (226.70 to 227.70): E

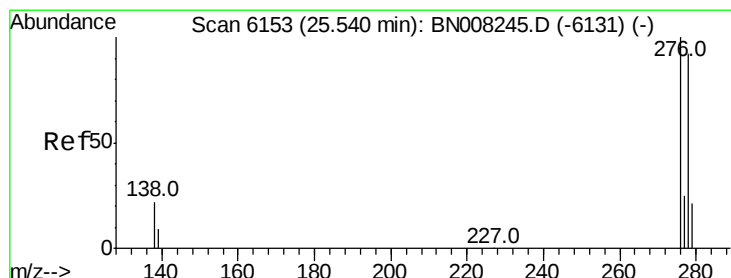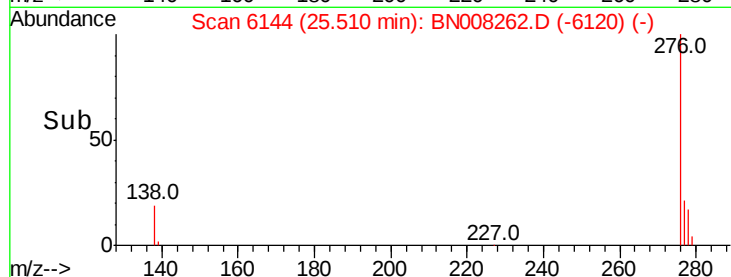
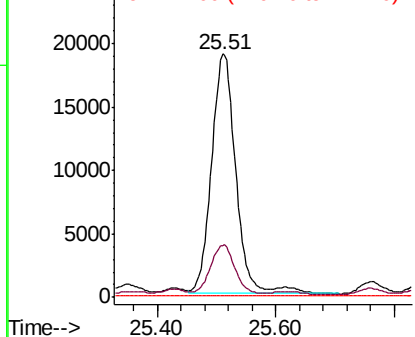



#25  
 Dibenzo(a,h)anthracene  
 Concen: 0.330 ng/ul  
 RT: 25.52 min Scan# 6146  
 Delta R.T. -0.02 min  
 Lab File: BN008262.D  
 Acq: 19 Oct 2019 10:29

Tgt Ion:278 Resp: 13604  
 Ion Ratio Lower Upper  
 278 100  
 139 20.1 15.0 22.6  
 279 30.8 22.4 33.6

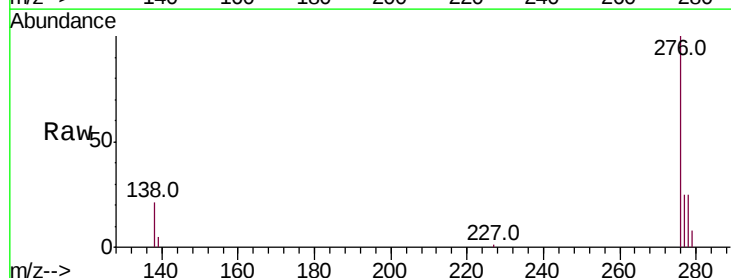

Abundance Ion 278.00 (277.70 to 278.70): E  
 Ion 139.00 (138.70 to 139.70): E  
 Ion 279.00 (278.70 to 279.70): E

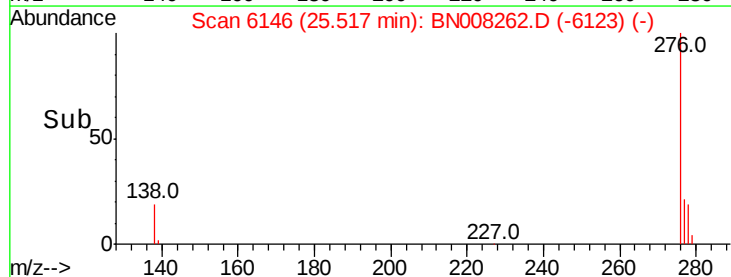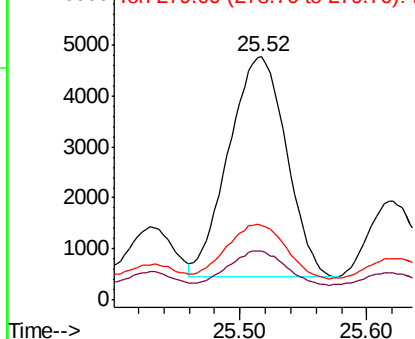

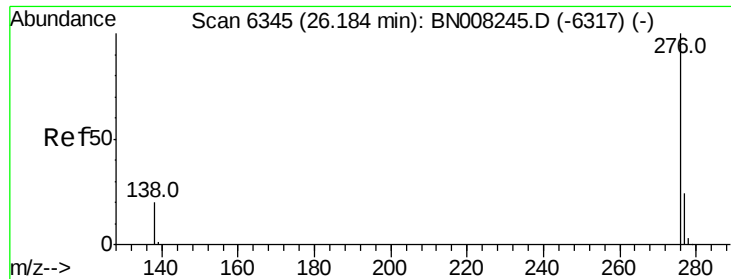

#26

Benzo(a,h,i)perylene

Concen: 1.023 ng/ul

RT: 26.17 min Scan# 6340

Delta R.T. -0.02 min

Lab File: BN008262.D

Acq: 19 Oct 2019 10:29

Instrument :

BNA\_N

ClientSampleId :

BEP94DL


Tot Ion:276 Resp: 48865

Ion Ratio Lower Upper

276 100

138 21.9 17.0 25.4

277 24.6 20.4 30.6

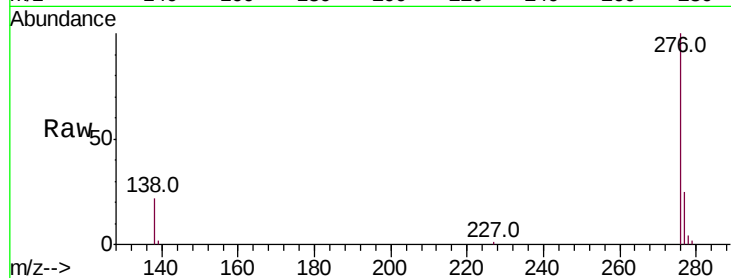

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

