

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101919\
 Data File : BN008269.D
 Acq On : 19 Oct 2019 14:40
 Operator : JU
 Sample : K5177-19DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BEPC8DL

Quant Time: Oct 19 20:52:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 23:47:17 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	1985	0.40	ng/ul	0.00
2) Naphthalene-d8	10.36	136	9670	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.23	164	6573	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.97	188	14642	0.40	ng/ul	0.00
16) Chrysene-d12	21.18	240	15500	0.40	ng/ul	0.00
20) Perylene-d12	23.35	264	14559	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	403	0.02	ng/ul	0.00
14) Fluoranthene-d10	19.01	212	1457	0.03	ng/ul	0.00
Target Compounds				Ovalue		
12) Phenanthrene	17.01	178	17125	0.399	ng/ul	100
13) Anthracene	17.11	178	2400	0.064	ng/ul#	92
15) Fluoranthene	19.04	202	51564	0.911	ng/ul	99
17) Pyrene	19.40	202	43464	0.704	ng/ul	100
18) Benzo(a)anthracene	21.16	228	17818	0.316	ng/ul	98
19) Chrysene	21.22	228	23437	0.339	ng/ul	98
21) Benzo(b)fluoranthene	22.71	252	40746	0.860	ng/ul	97
22) Benzo(k)fluoranthene	22.71	252	40746	0.759	ng/ul	98
23) Benzo(a)pyrene	23.26	252	17763	0.356	ng/ul#	93
24) Indeno(1,2,3-cd)pyrene	25.51	276	11932	0.203	ng/ul#	99
25) Dibenzo(a,h)anthracene	25.52	278	2150	0.046	ng/ul#	73
26) Benzo(g,h,i)perylene	26.16	276	10856	0.202	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101919\
Data File : BN008269.D
Acq On : 19 Oct 2019 14:40
Operator : JU
Sample : K5177-19DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BEPC8DL

Quant Time: Oct 19 20:52:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 23:47:17 2019
Response via : Initial Calibration

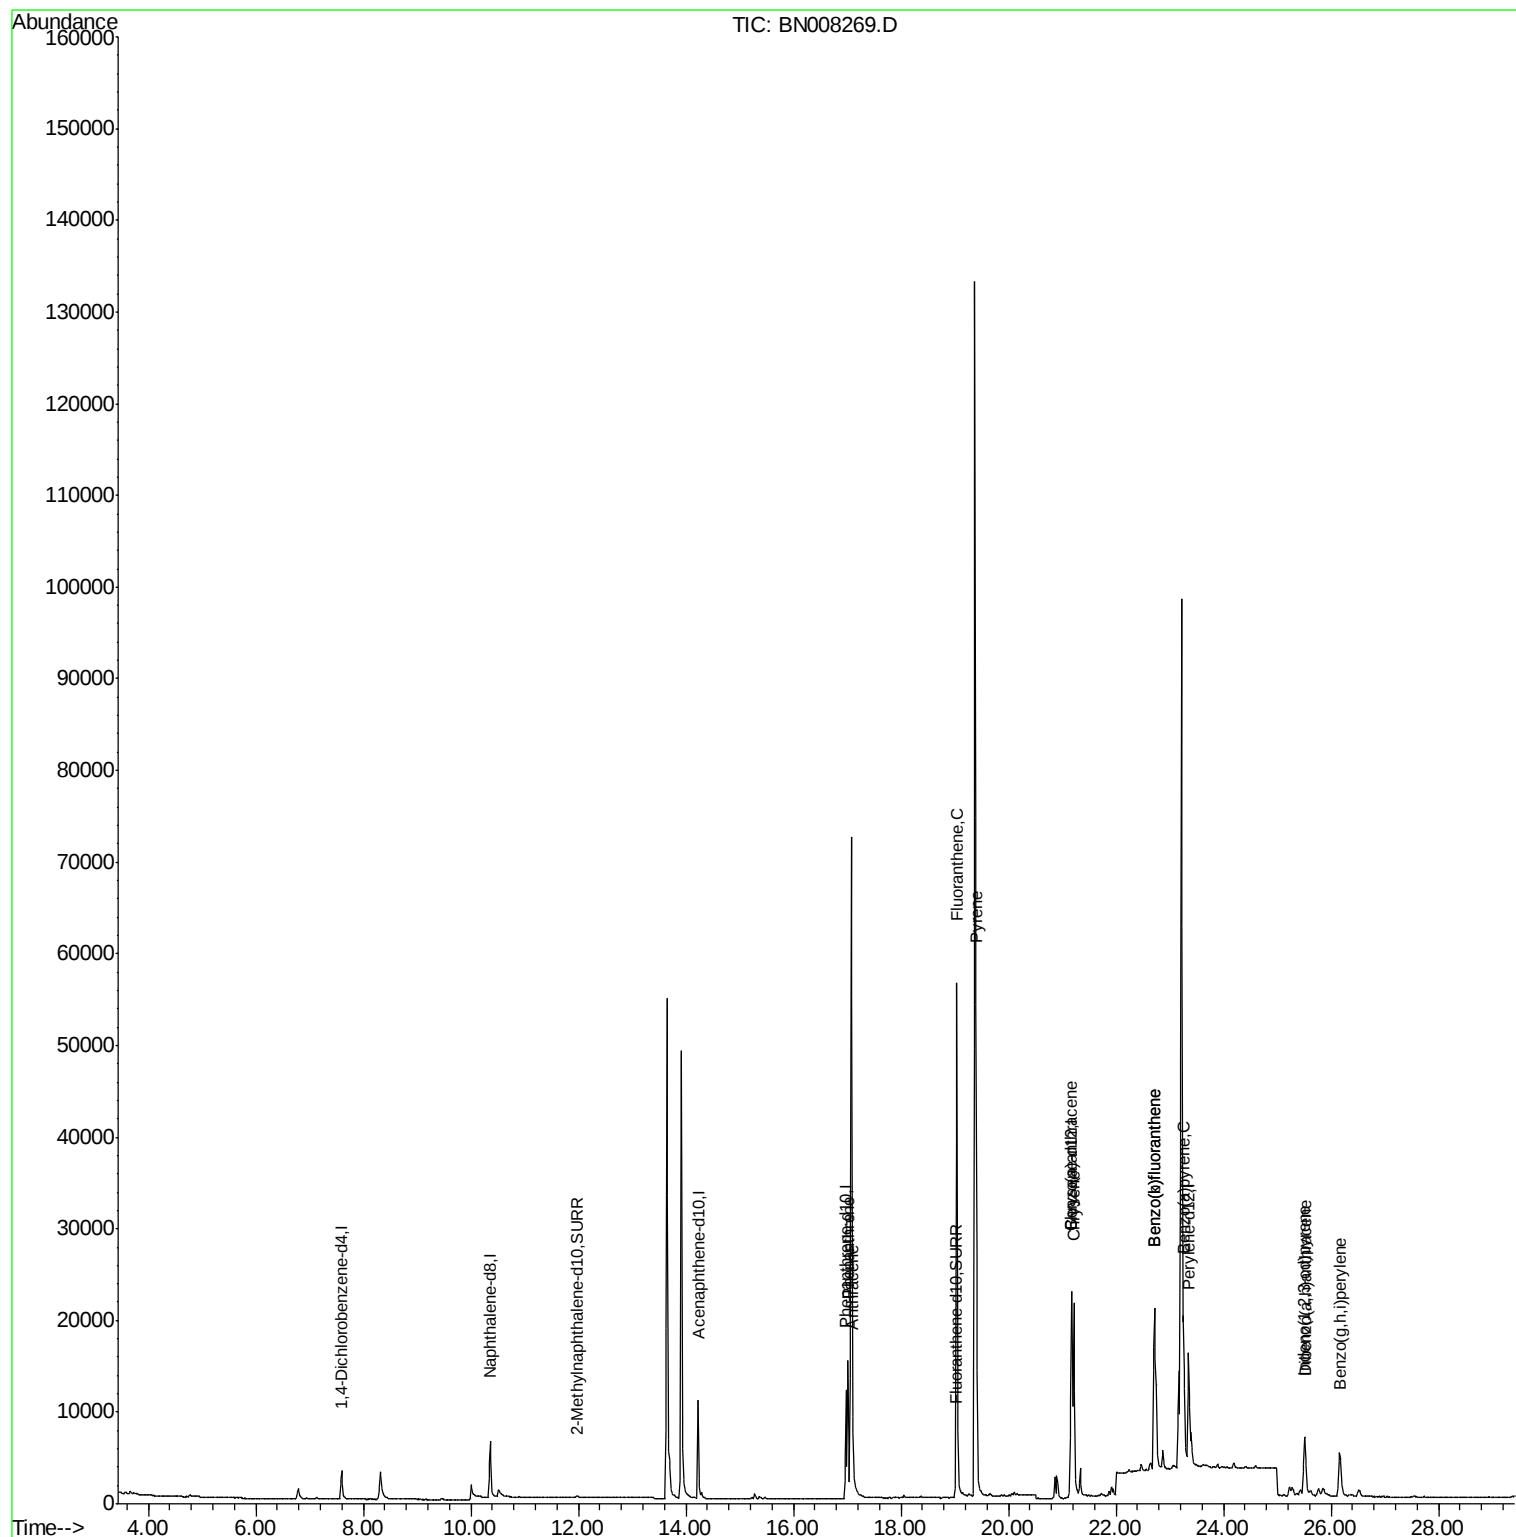

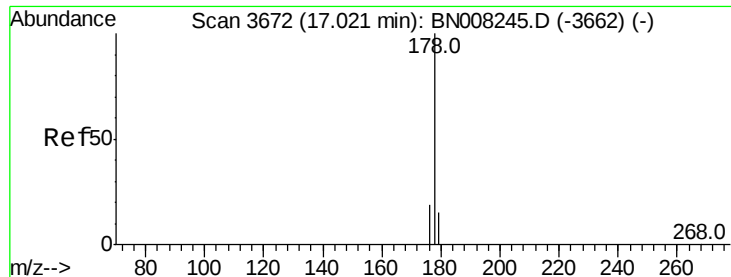

#12

Phenanthrene

Concen: 0.399 ng/ul

RT: 17.01 min Scan# 3670

Delta R.T. -0.01 min

Lab File: BN008269.D

Acq: 19 Oct 2019 14:40

Instrument :

BNA_N

ClientSampleId :

BEPC8DL





Tot Ion:178 Resp: 17125

Ion Ratio Lower Upper

178 100

179 15.8 12.8 19.2

176 19.3 15.4 23.2

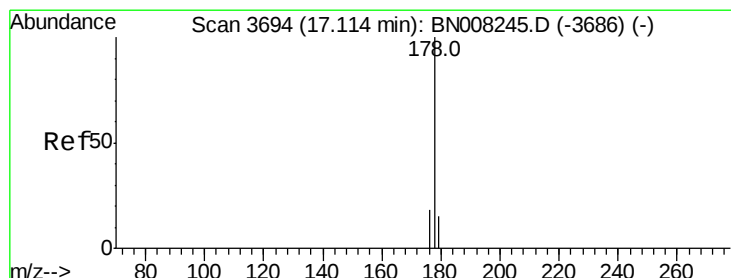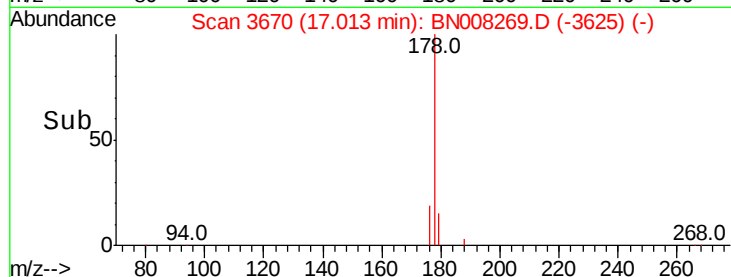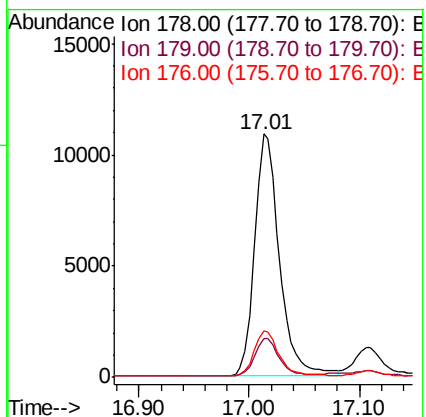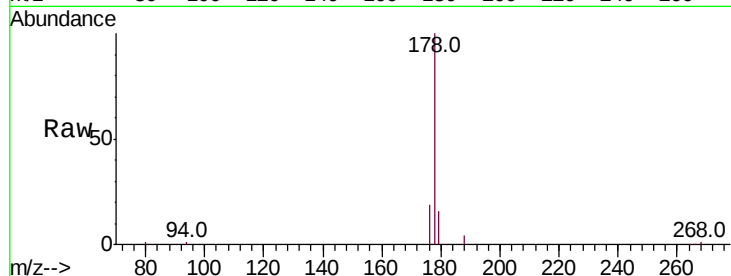

#13

Anthracene

Concen: 0.064 ng/ul

RT: 17.11 min Scan# 3692

Delta R.T. -0.01 min

Lab File: BN008269.D

Acq: 19 Oct 2019 14:40




Tgt Ion:178 Resp: 2400


Ion Ratio Lower Upper

178 100

179 21.0 13.0 19.6#

176 21.5 15.0 22.6

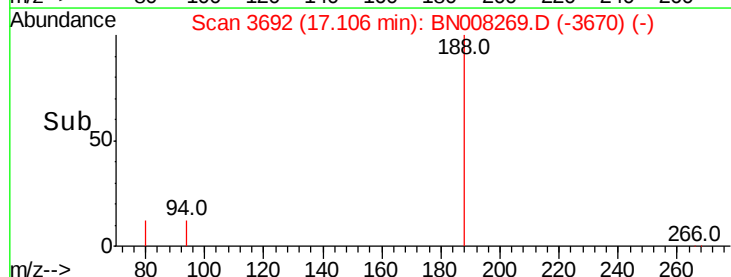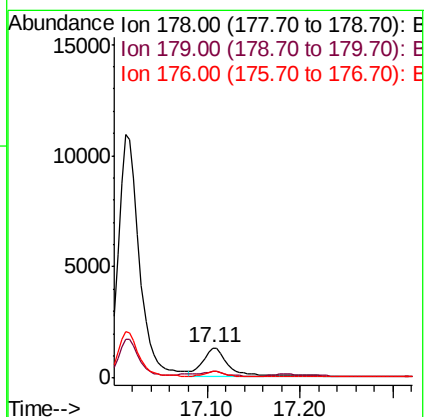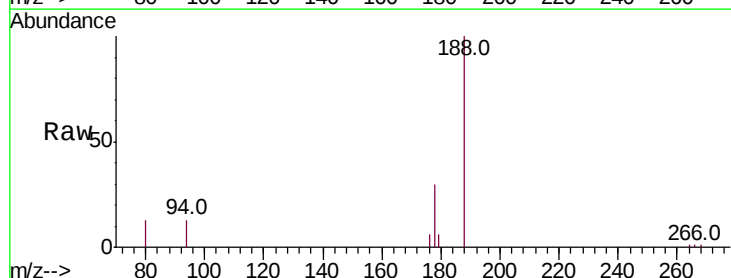


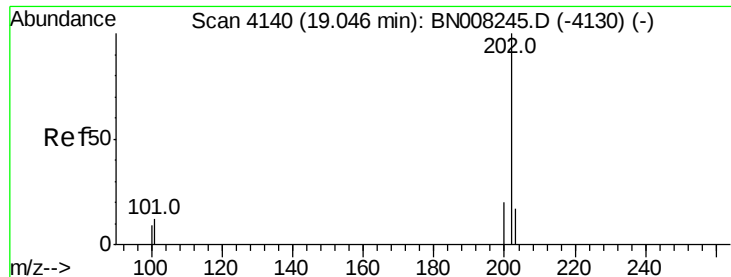




#15
Fluoranthene
 Concen: 0.911 ng/ul
 RT: 19.04 min Scan# 4139
 Delta R.T. -0.00 min
 Lab File: BN008269.D
 Acq: 19 Oct 2019 14:40

Instrument :
 BNA_N
 ClientSampleId :
 BEPC8DL

Tot Ion:202 Resp: 51564
 Ion Ratio Lower Upper
 202 100
 101 11.6 0.0 31.2
 100 8.8 0.0 28.5

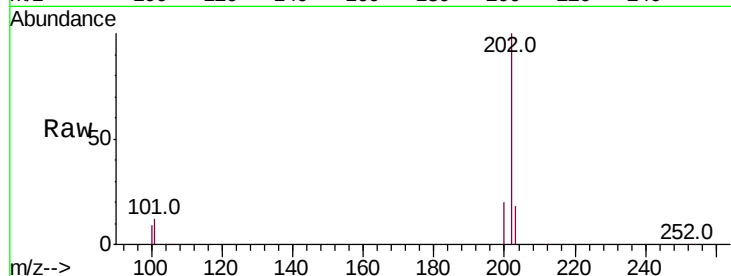


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

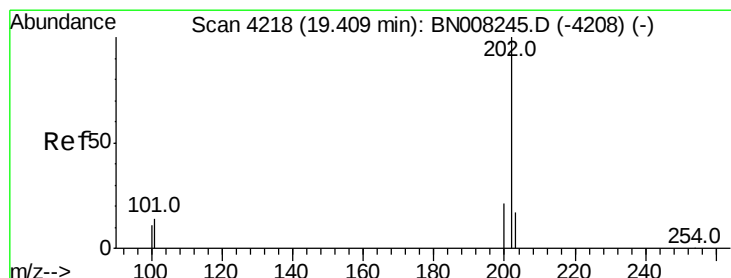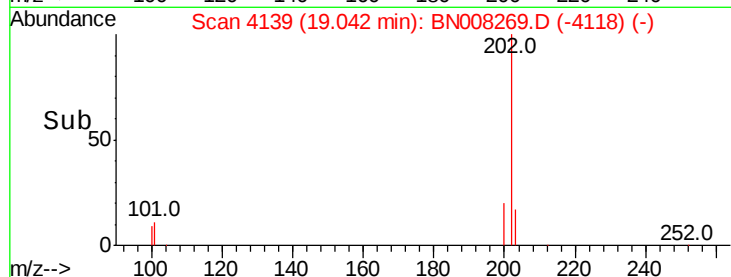
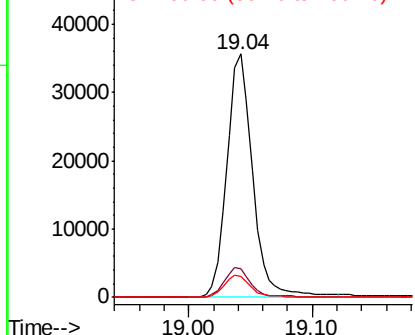



#17
Pyrene
 Concen: 0.704 ng/ul
 RT: 19.40 min Scan# 4217
 Delta R.T. -0.00 min
 Lab File: BN008269.D
 Acq: 19 Oct 2019 14:40

Tgt Ion:202 Resp: 43464
 Ion Ratio Lower Upper
 202 100
 101 13.5 10.9 16.3
 100 11.0 8.7 13.1

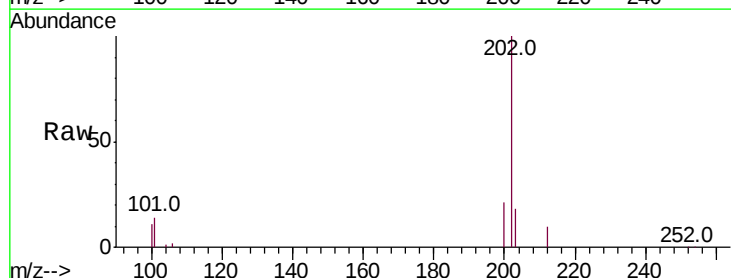

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

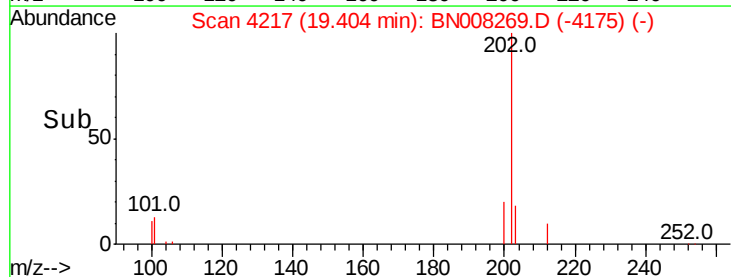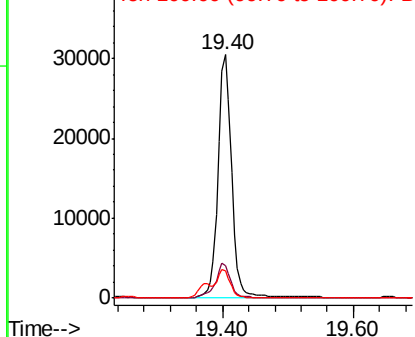

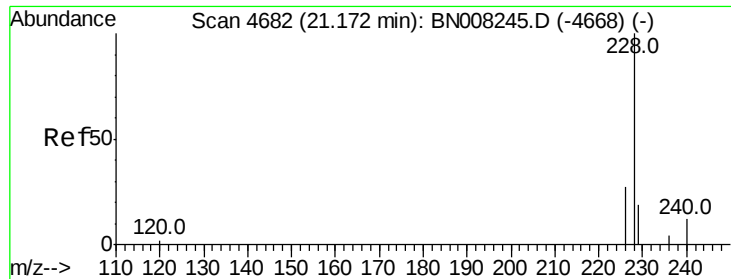

#18

Benzo(a)anthracene

Concen: 0.316 ng/ul

RT: 21.16 min Scan# 4679

Delta R.T. -0.01 min

Lab File: BN008269.D

Acq: 19 Oct 2019 14:40

Instrument :

BNA_N

ClientSampleId :

BEPC8DL


Tot Ion:228 Resp: 17818

Ion Ratio Lower Upper




228 100

229 20.9 16.2 24.2

226 27.5 21.4 32.0

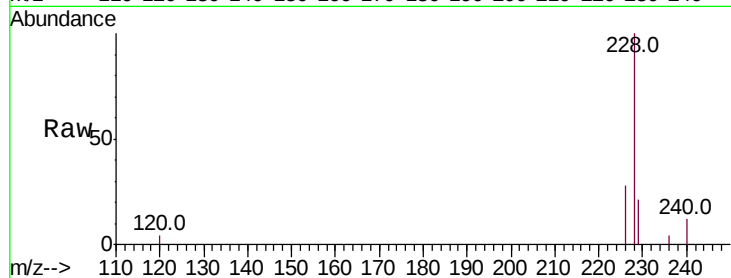

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

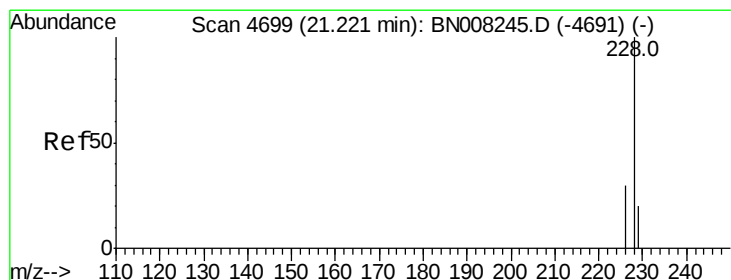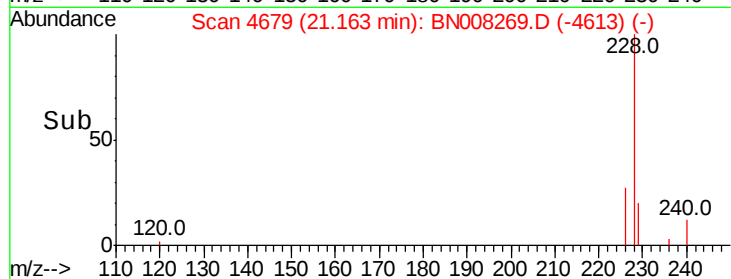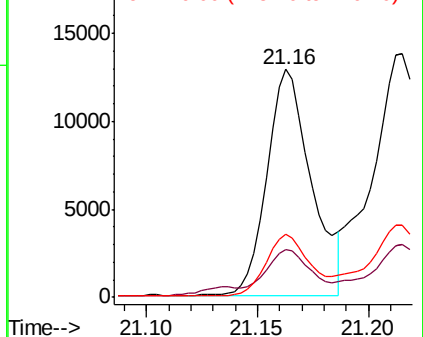

#19

Chrysene

Concen: 0.339 ng/ul

RT: 21.22 min Scan# 4697

Delta R.T. -0.01 min

Lab File: BN008269.D

Acq: 19 Oct 2019 14:40


Tgt Ion:228 Resp: 23437

Ion Ratio Lower Upper



228 100


226 29.6 24.1 36.1

229 21.5 16.2 24.2

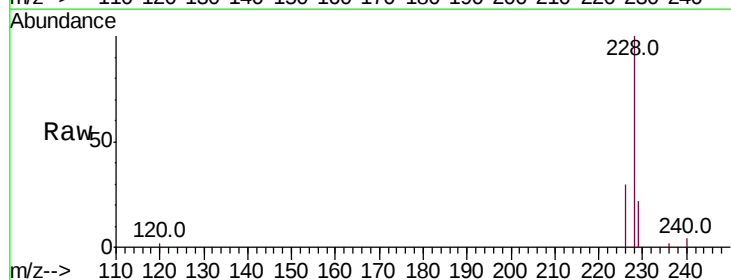

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

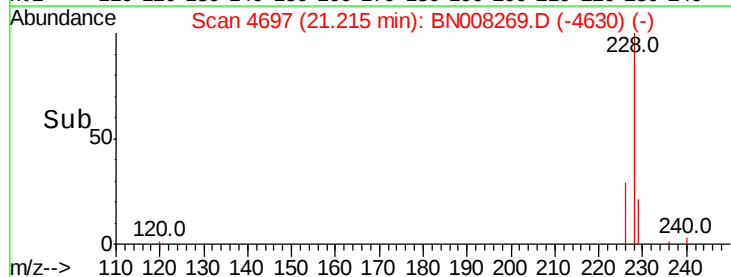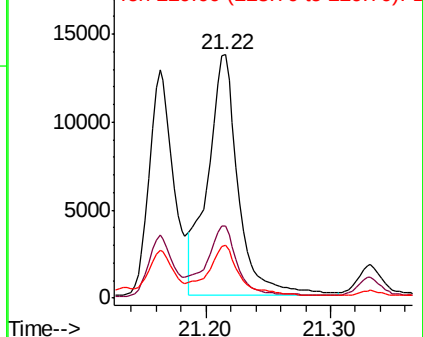

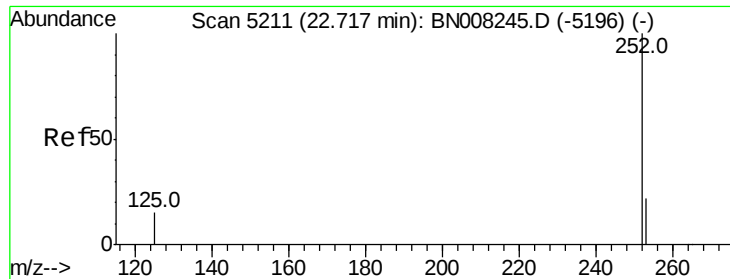

#21

Benzo(b)fluoranthene

Concen: 0.860 ng/u1

RT: 22.71 min Scan# 5209

Delta R.T. -0.01 min

Lab File: BN008269.D

Acq: 19 Oct 2019 14:40

Instrument :

BNA_N

ClientSampleId :

BEPC8DL


Tot Ion:252 Resp: 40746

Ion Ratio Lower Upper

252 100

253 25.0 0.0 53.4




125 14.9 0.0 32.4

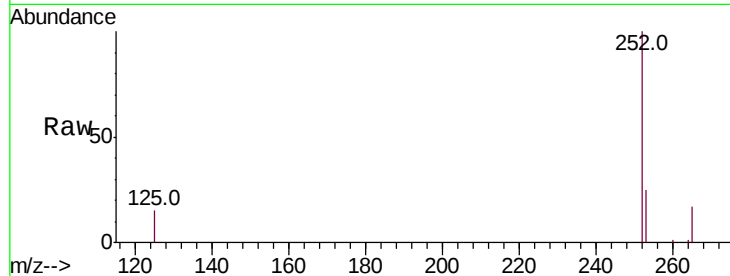

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

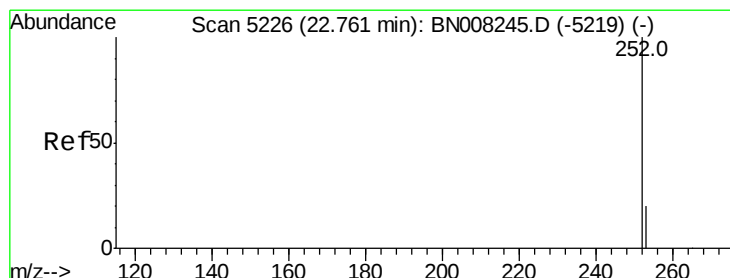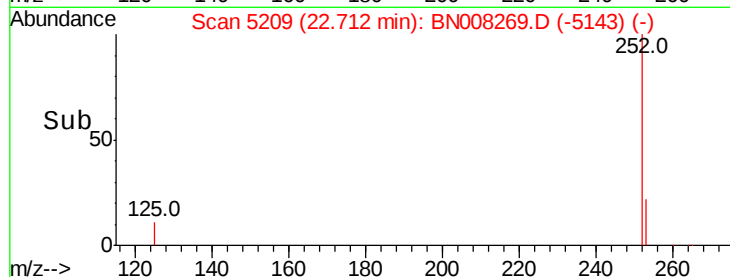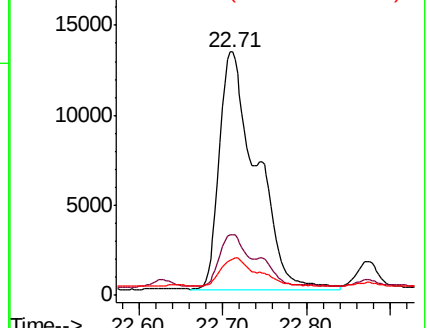

#22

Benzo(k)fluoranthene

Concen: 0.759 ng/u1

RT: 22.71 min Scan# 5209

Delta R.T. -0.05 min

Lab File: BN008269.D

Acq: 19 Oct 2019 14:40


Tgt Ion:252 Resp: 40746

Ion Ratio Lower Upper

252 100

253 25.0 21.3 31.9



125 14.9 12.3 18.5

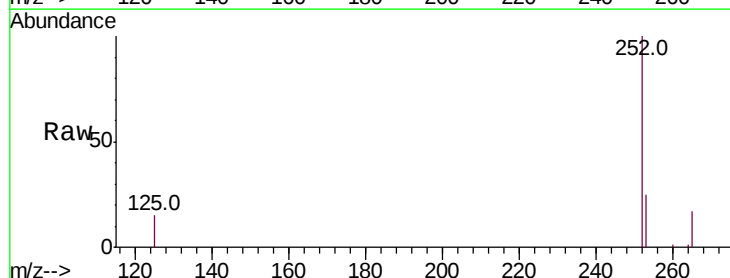


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

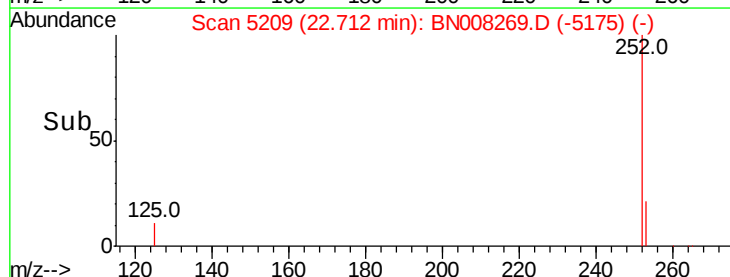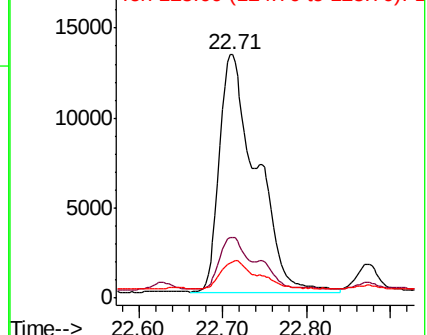

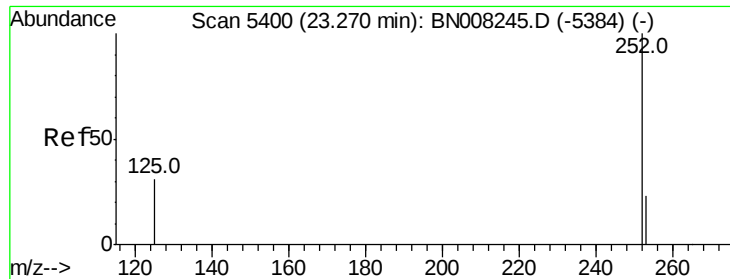

#23

Benzo(a)pyrene

Concen: 0.356 ng/u1

RT: 23.26 min Scan# 5396

Delta R.T. -0.01 min

Lab File: BN008269.D

Acq: 19 Oct 2019 14:40

Instrument :

BNA_N

ClientSampleId :

BEPC8DL


Tot Ion:252 Resp: 17763

Ion Ratio Lower Upper

252 100

253 26.2 22.8 34.2




125 17.8 18.4 27.6#

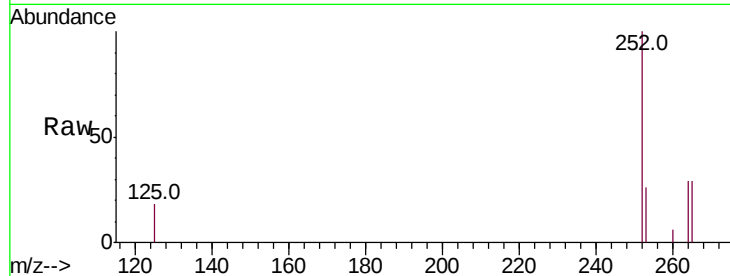

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

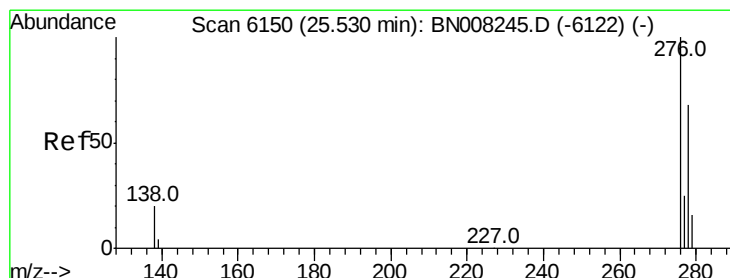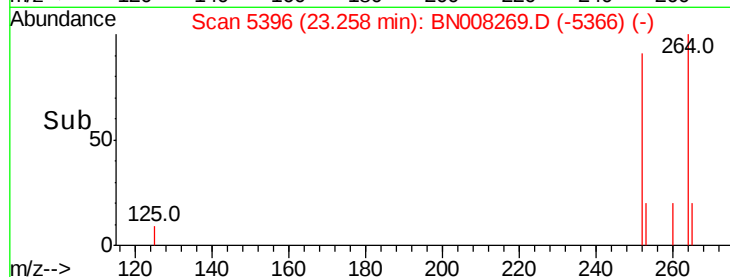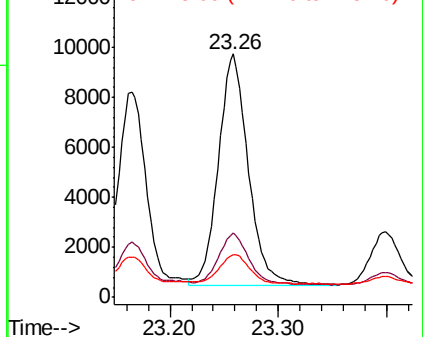

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.203 ng/u1

RT: 25.51 min Scan# 6143

Delta R.T. -0.02 min

Lab File: BN008269.D

Acq: 19 Oct 2019 14:40


Tgt Ion:276 Resp: 11932

Ion Ratio Lower Upper

276 100

138 20.5 16.1 24.1



227 0.0 0.2 0.2#

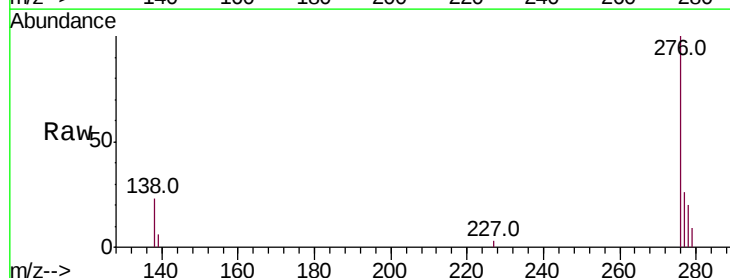


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E



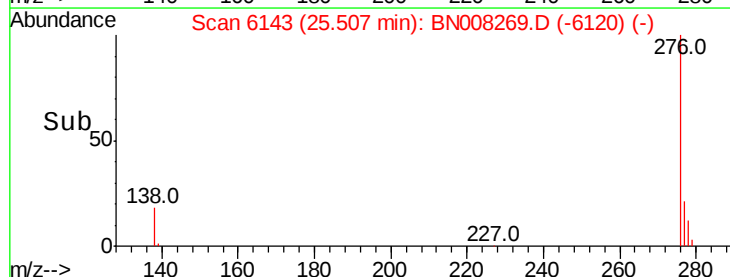
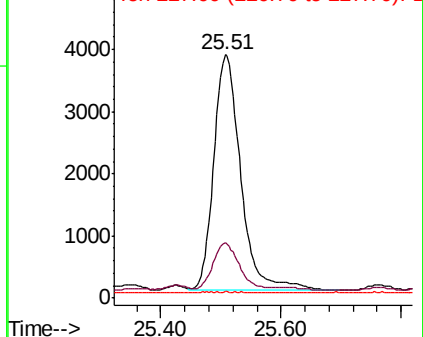


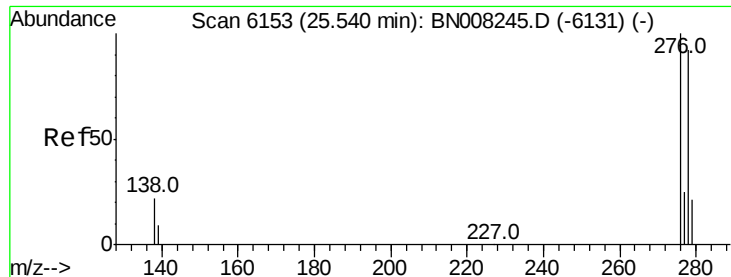

#25
Dibenzo(a,h)anthracene
Concen: 0.046 ng/u1
RT: 25.52 min Scan# 6146
Delta R.T. -0.02 min
Lab File: BN008269.D
Acq: 19 Oct 2019 14:40

Instrument :
BNA_N
ClientSampleId :
BEPC8DL

Tot Ion:278 Resp: 2150
Ion Ratio Lower Upper
278 100
139 28.5 15.0 22.6#
279 43.8 22.4 33.6#

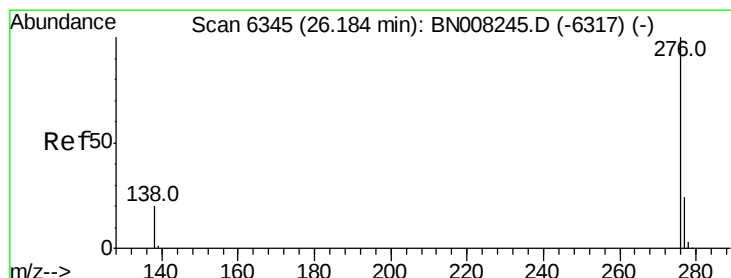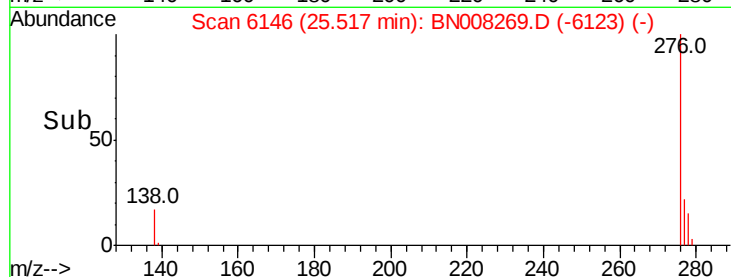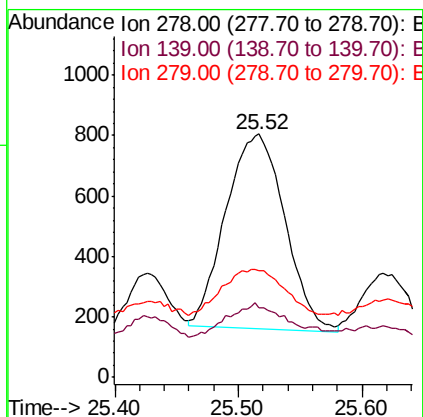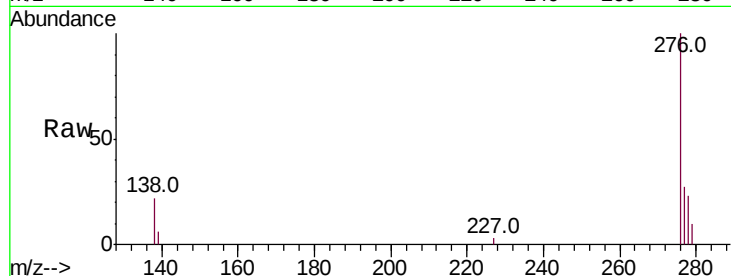

#26
Benzo(g,h,i)perylene
Concen: 0.202 ng/u1
RT: 26.16 min Scan# 6339
Delta R.T. -0.02 min
Lab File: BN008269.D
Acq: 19 Oct 2019 14:40

Tgt Ion:276 Resp: 10856
Ion Ratio Lower Upper
276 100
138 23.8 17.0 25.4
277 26.2 20.4 30.6

