

Data File : BN003248.D
Acq On : 22 Oct 2018 20:23
Operator : MJ/SJ
Sample : J5568-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK3

Quant Time: Oct 23 05:09:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 23 05:03:53 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	72905	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	350525	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	233998	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	560504	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	669359	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	676169	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	2505	1.77	ng/uL	0.00
5) Phenol-d5	6.82	99	66655	9.65	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.95	67	32546	8.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	44792	8.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	52201	9.29	ng/ul	0.01
19) Nitrobenzene-d5	8.77	128	19884	7.31	ng/ul	0.01
22) 2-Nitrophenol-d4	9.49	143	23207	7.35	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.05	165	41033	7.17	ng/ul	0.02
29) 4-Chloroaniline-d4	10.55	131	51735	11.21	ng/ul	0.01
43) Dimethylphthalate-d6	13.66	166	148677	7.46	ng/ul	0.00
46) Acenaphthylene-d8	13.94	160	128482	5.22	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	30199	10.99	ng/ul	0.04
57) Fluorene-d10	15.25	176	80720	4.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	24717	6.57	ng/ul	0.02
70) Anthracene-d10	17.10	188	114204	4.12	ng/ul	0.00
78) Pyrene-d10	19.41	212	130032	4.01	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	174906	4.78	ng/ul	0.00


Target Compounds					Qvalue
6) Phenol	6.84	94	25661	3.694 ng/ul	95
44) Dimethylphthalate	13.71	163	35578	1.825 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003248.D
Acq On : 22 Oct 2018 20:23
Operator : MJ/SJ
Sample : J5568-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK3

Quant Time: Oct 23 05:09:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 23 05:03:53 2018
Response via : Initial Calibration




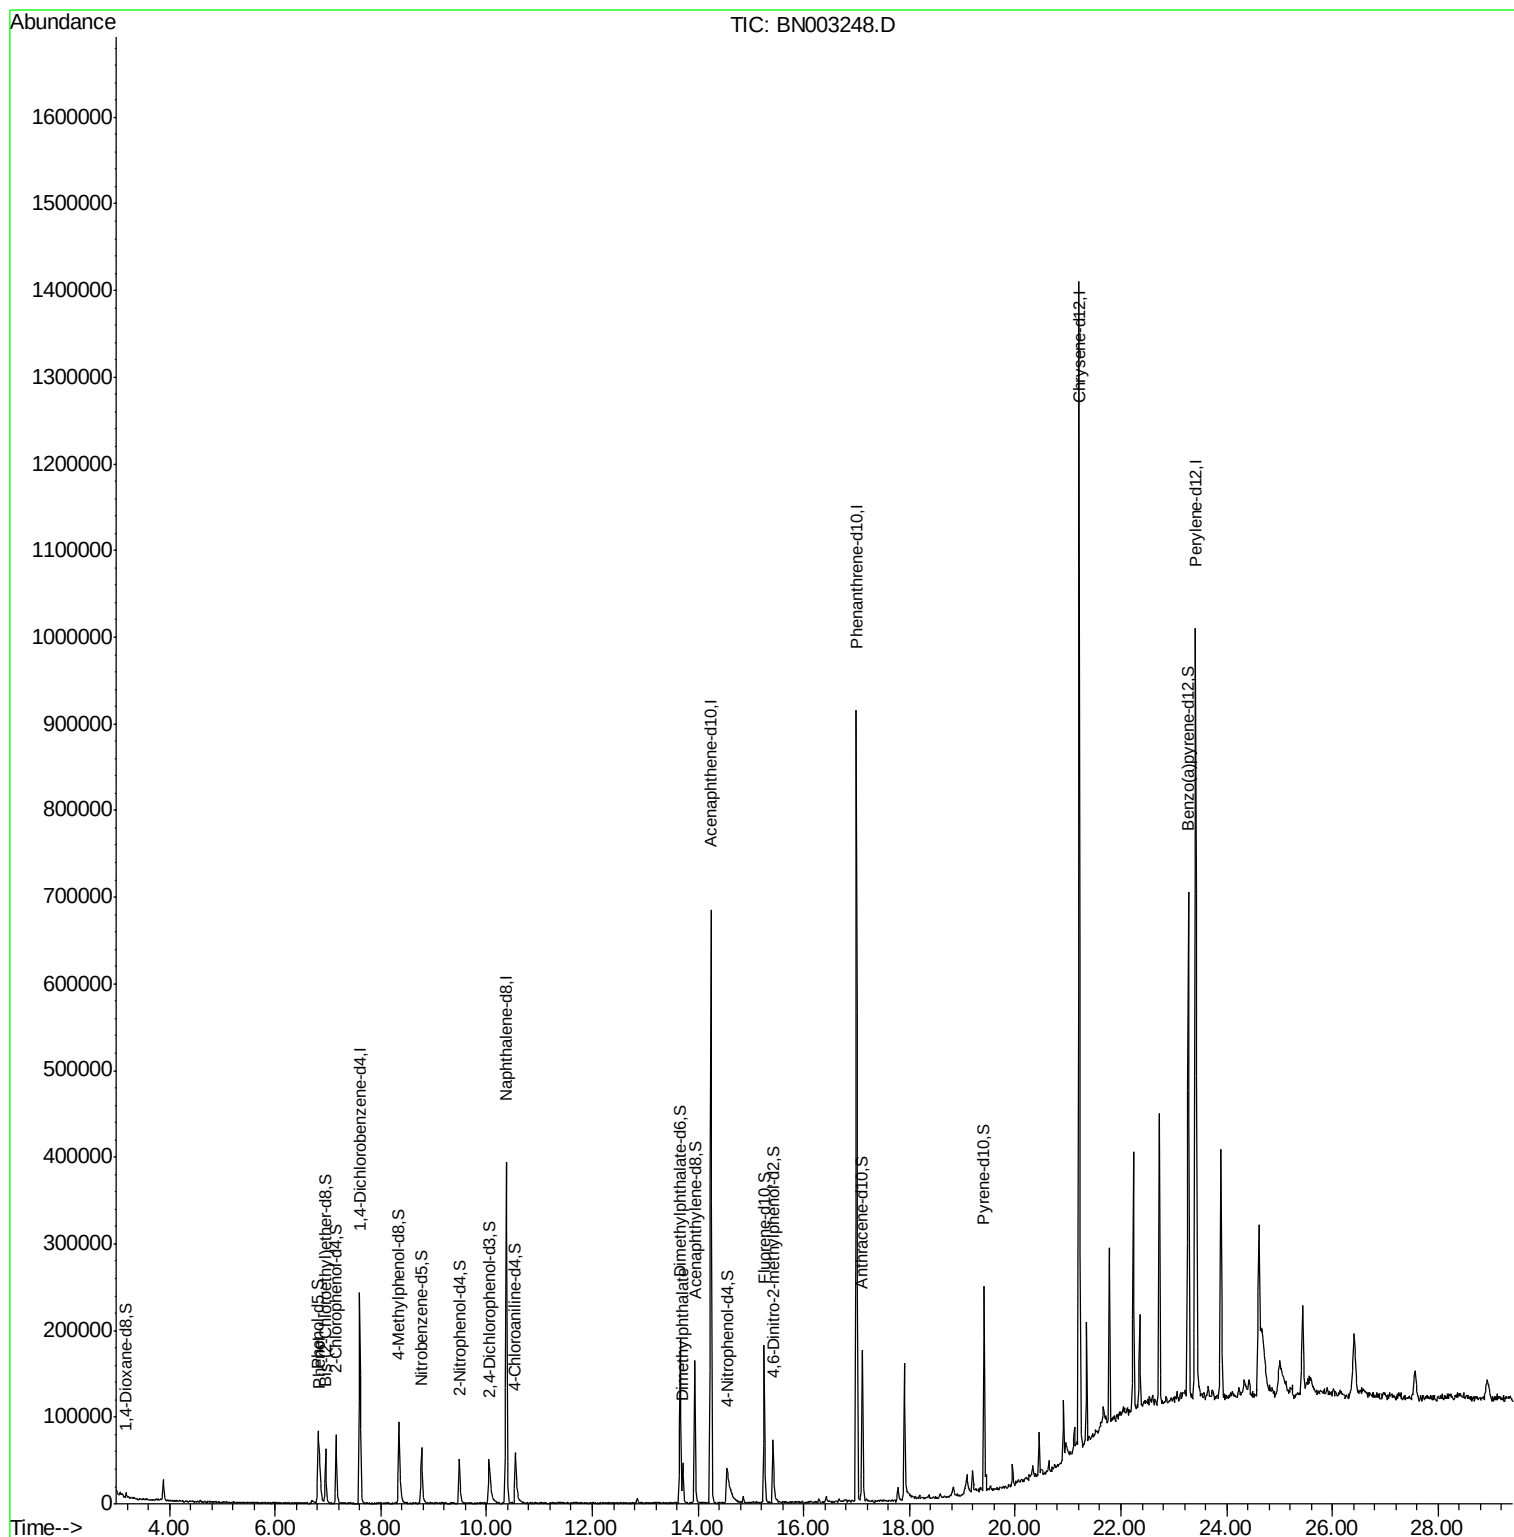


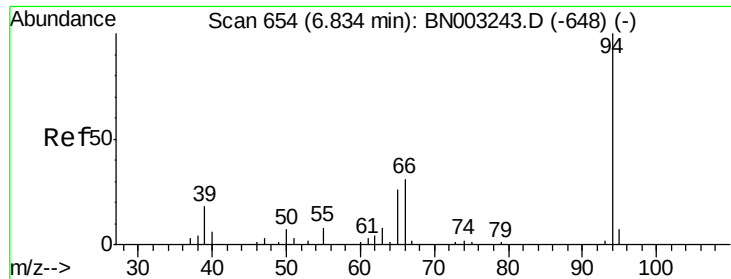

#6
 Phenol
 Concen: 3.694 ng/ul
 RT: 6.84 min Scan# 655
 Delta R.T. 0.01 min
 Lab File: BN003248.D
 Acq: 22 Oct 2018 20:23

Instrument :
 BNA_N
 ClientSampleId :
 C0AK3

Tgt Ion: 94 Resp: 25661
 Ion Ratio Lower Upper
 94 100
 65 25.9 21.2 31.8
 66 38.6 27.4 41.2

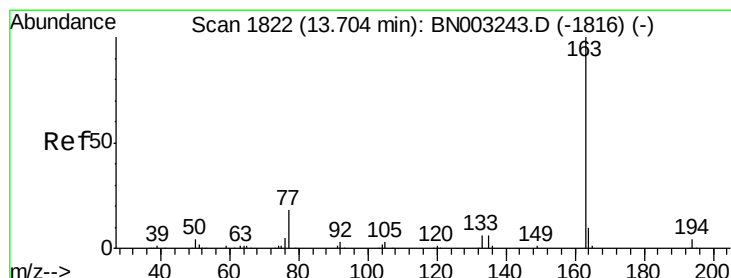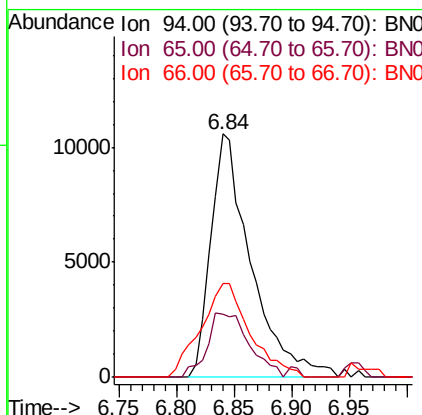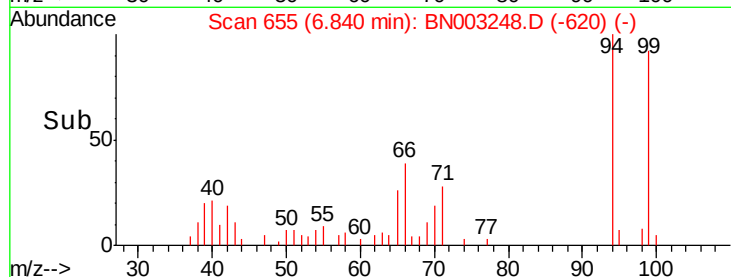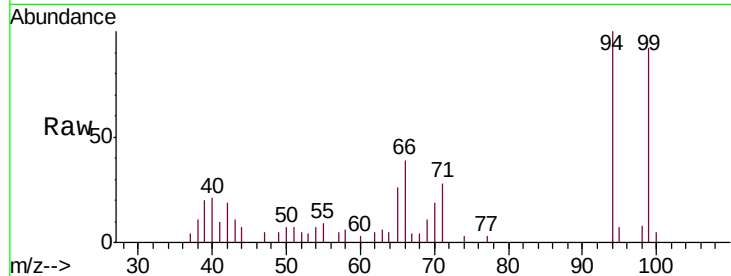

#44
 Dimethylphthalate
 Concen: 1.825 ng/ul
 RT: 13.71 min Scan# 1823
 Delta R.T. 0.01 min
 Lab File: BN003248.D
 Acq: 22 Oct 2018 20:23

Tgt Ion: 163 Resp: 35578
 Ion Ratio Lower Upper
 163 100
 194 3.6 3.7 5.5#
 164 10.9 8.3 12.5

