

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN102218\
 Data File : BN003253.D
 Acq On : 22 Oct 2018 23:18
 Operator : MJ/SJ
 Sample : J5568-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK6

Quant Time: Oct 23 05:09:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 23 05:03:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	73285	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	358305	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	233726	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	566595	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	662516	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	696991	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	5892	4.15	ng/uL	0.00
5) Phenol-d5	6.81	99	144772	20.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	88006	21.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	118975	21.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	128848	22.81	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	61045	21.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	72976	22.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	131417	22.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	148628	31.52	ng/ul	0.00
43) Dimethylphthalate-d6	13.66	166	447681	22.48	ng/ul	0.00
46) Acenaphthylene-d8	13.93	160	566748	23.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	68544	24.98	ng/ul	0.01
57) Fluorene-d10	15.25	176	416565	23.88	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.41	200	69633	18.30	ng/ul	0.00
70) Anthracene-d10	17.10	188	667521	23.80	ng/ul	0.00
78) Pyrene-d10	19.40	212	766803	23.88	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	905300	24.02	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.83	94	58181	8.331 ng/ul	95
44) Dimethylphthalate	13.71	163	121283	6.230 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN102218\
Data File : BN003253.D
Acq On : 22 Oct 2018 23:18
Operator : MJ/SJ
Sample : J5568-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK6

Quant Time: Oct 23 05:09:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 23 05:03:53 2018
Response via : Initial Calibration

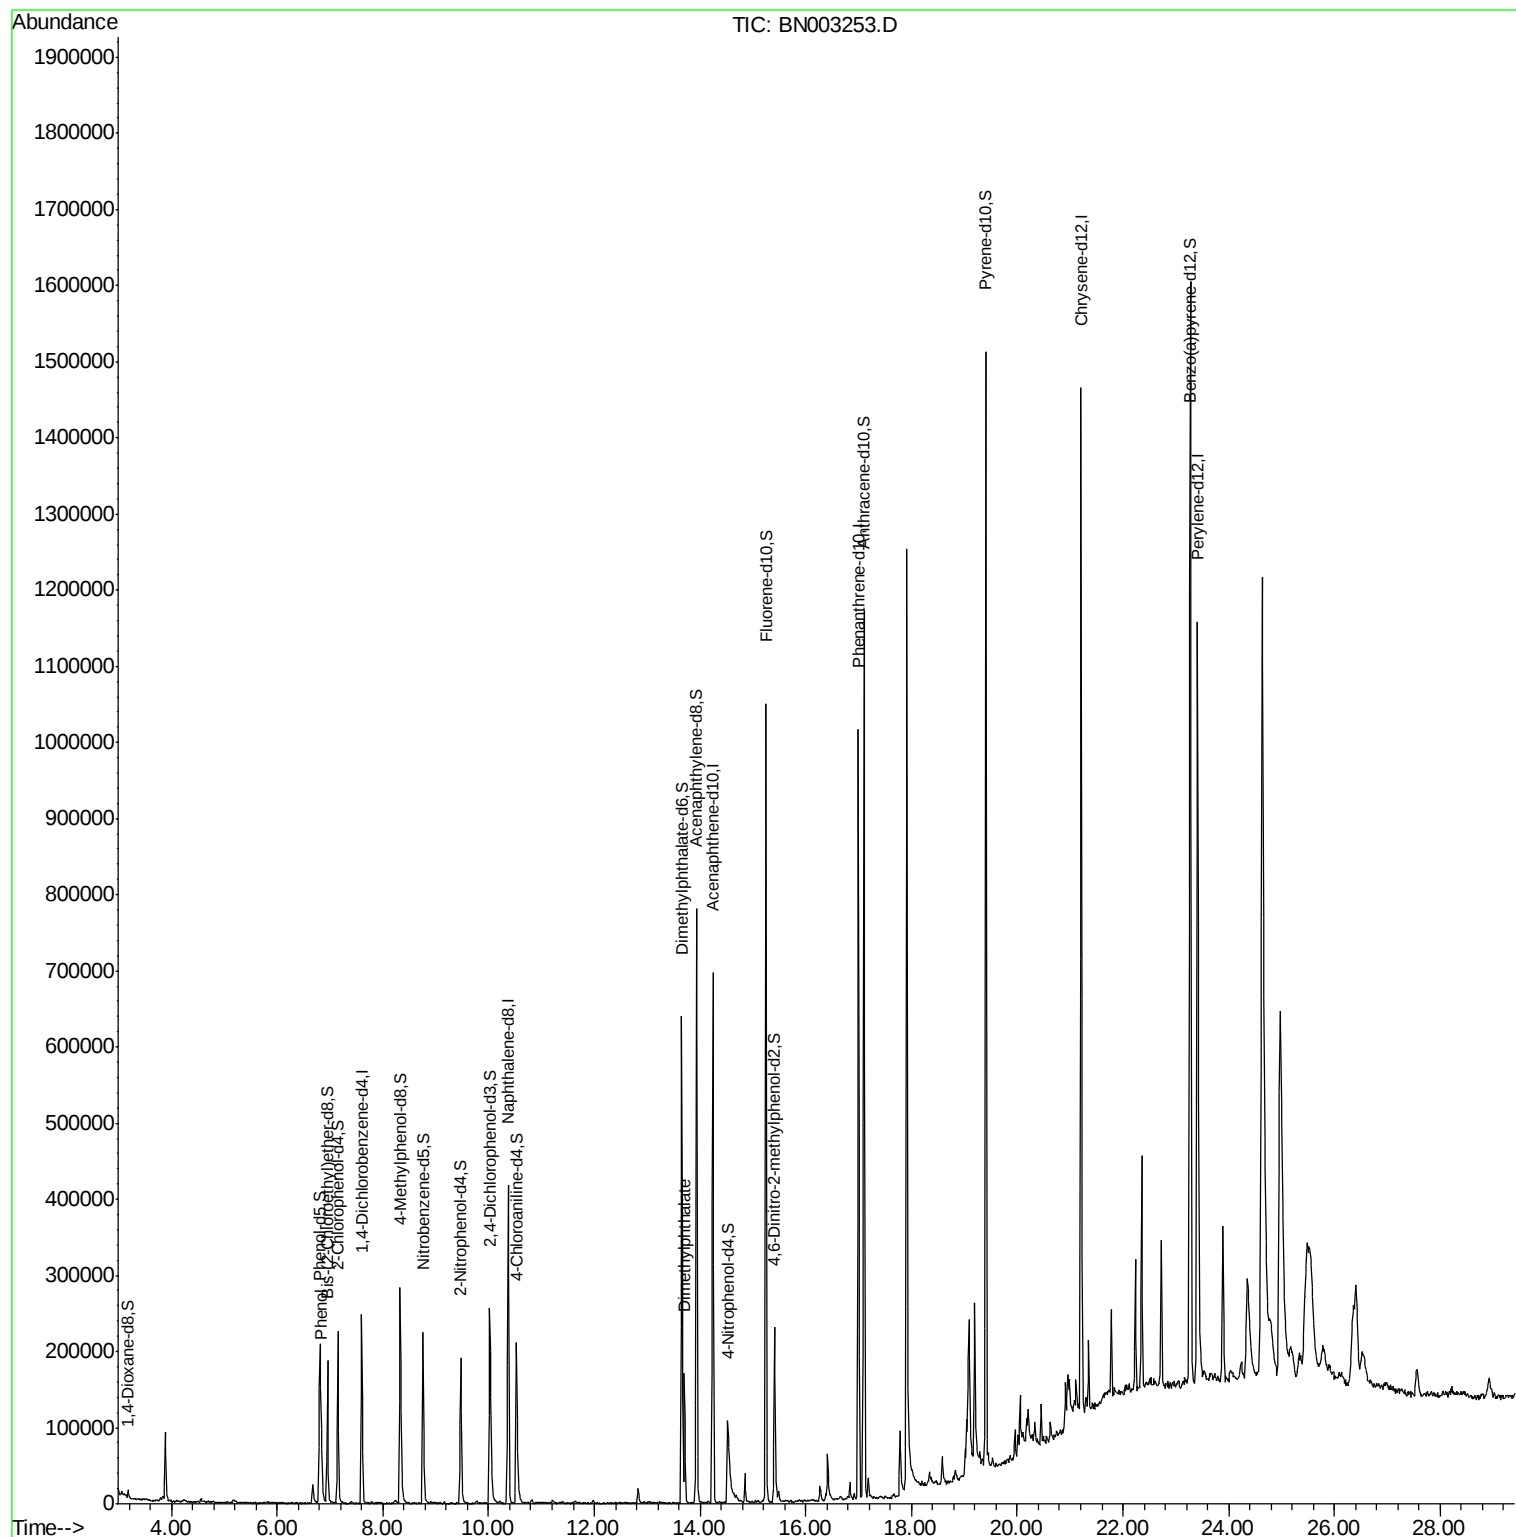

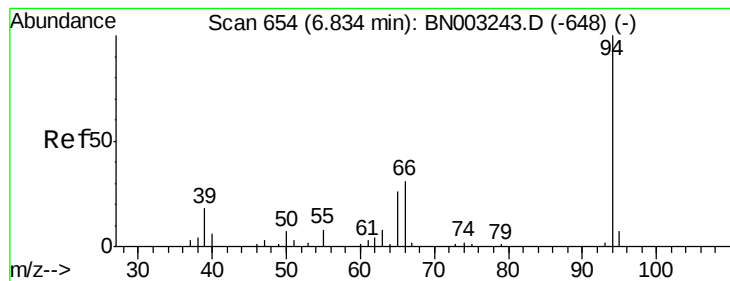


#6

Phenol




Concen: 8.331 ng/ul
 RT: 6.83 min Scan# 654
 Delta R.T. -0.00 min
 Lab File: BN003253.D
 Acq: 22 Oct 2018 23:18

Instrument :
 BNA_N
 ClientSampleId :
 C0AK6

Tot Ion: 94 Resp: 58181
 Ion Ratio Lower Upper
 94 100
 65 28.3 21.2 31.8
 66 38.1 27.4 41.2

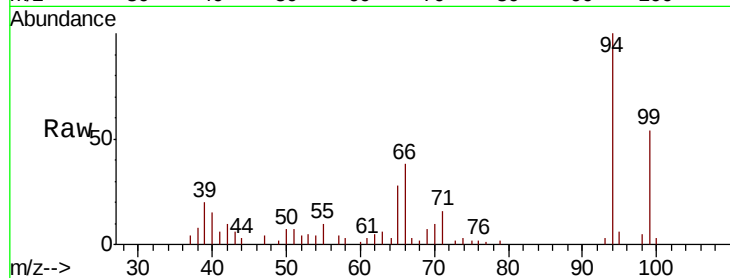

Abundance Ion 94.00 (93.70 to 94.70): BN0
 Ion 65.00 (64.70 to 65.70): BN0
 Ion 66.00 (65.70 to 66.70): BN0

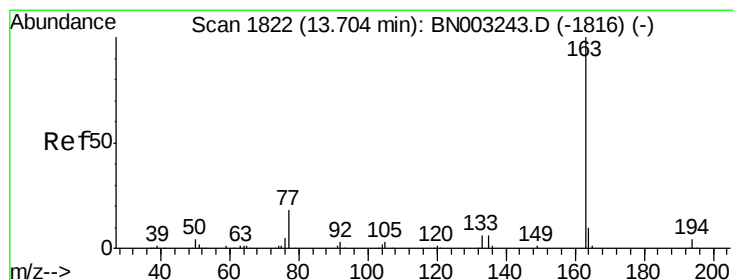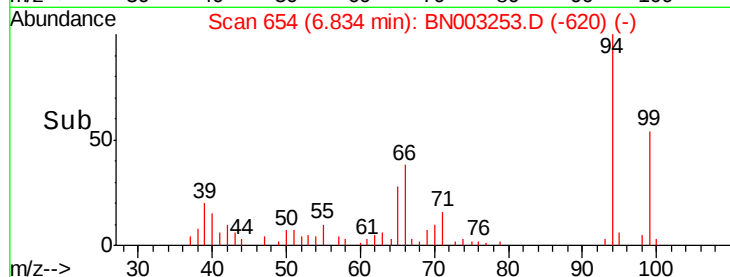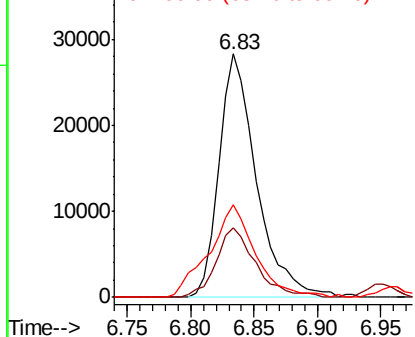


#44

Dimethylphthalate

Concen: 6.230 ng/ul
 RT: 13.71 min Scan# 1823
 Delta R.T. 0.01 min
 Lab File: BN003253.D
 Acq: 22 Oct 2018 23:18

Tgt Ion:163 Resp: 121283
 Ion Ratio Lower Upper
 163 100
 194 4.2 3.7 5.5
 164 10.1 8.3 12.5

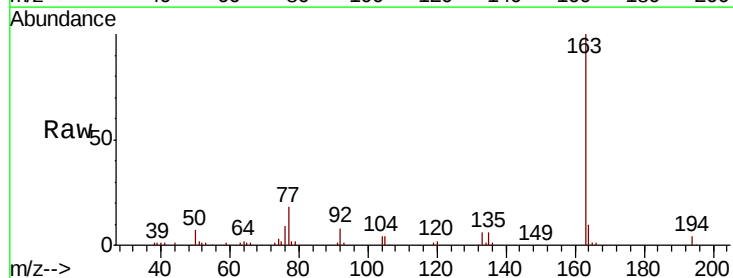

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

