


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102219\
Data File : BN008347.D
Acq On : 23 Oct 2019 13:09
Operator : JU
Sample : K5346-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Oct 23 14:19:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 11:13:51 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
ETON4

Manual Integrations
APPROVED

mohammad
10/24/2019 8:06:32 AM

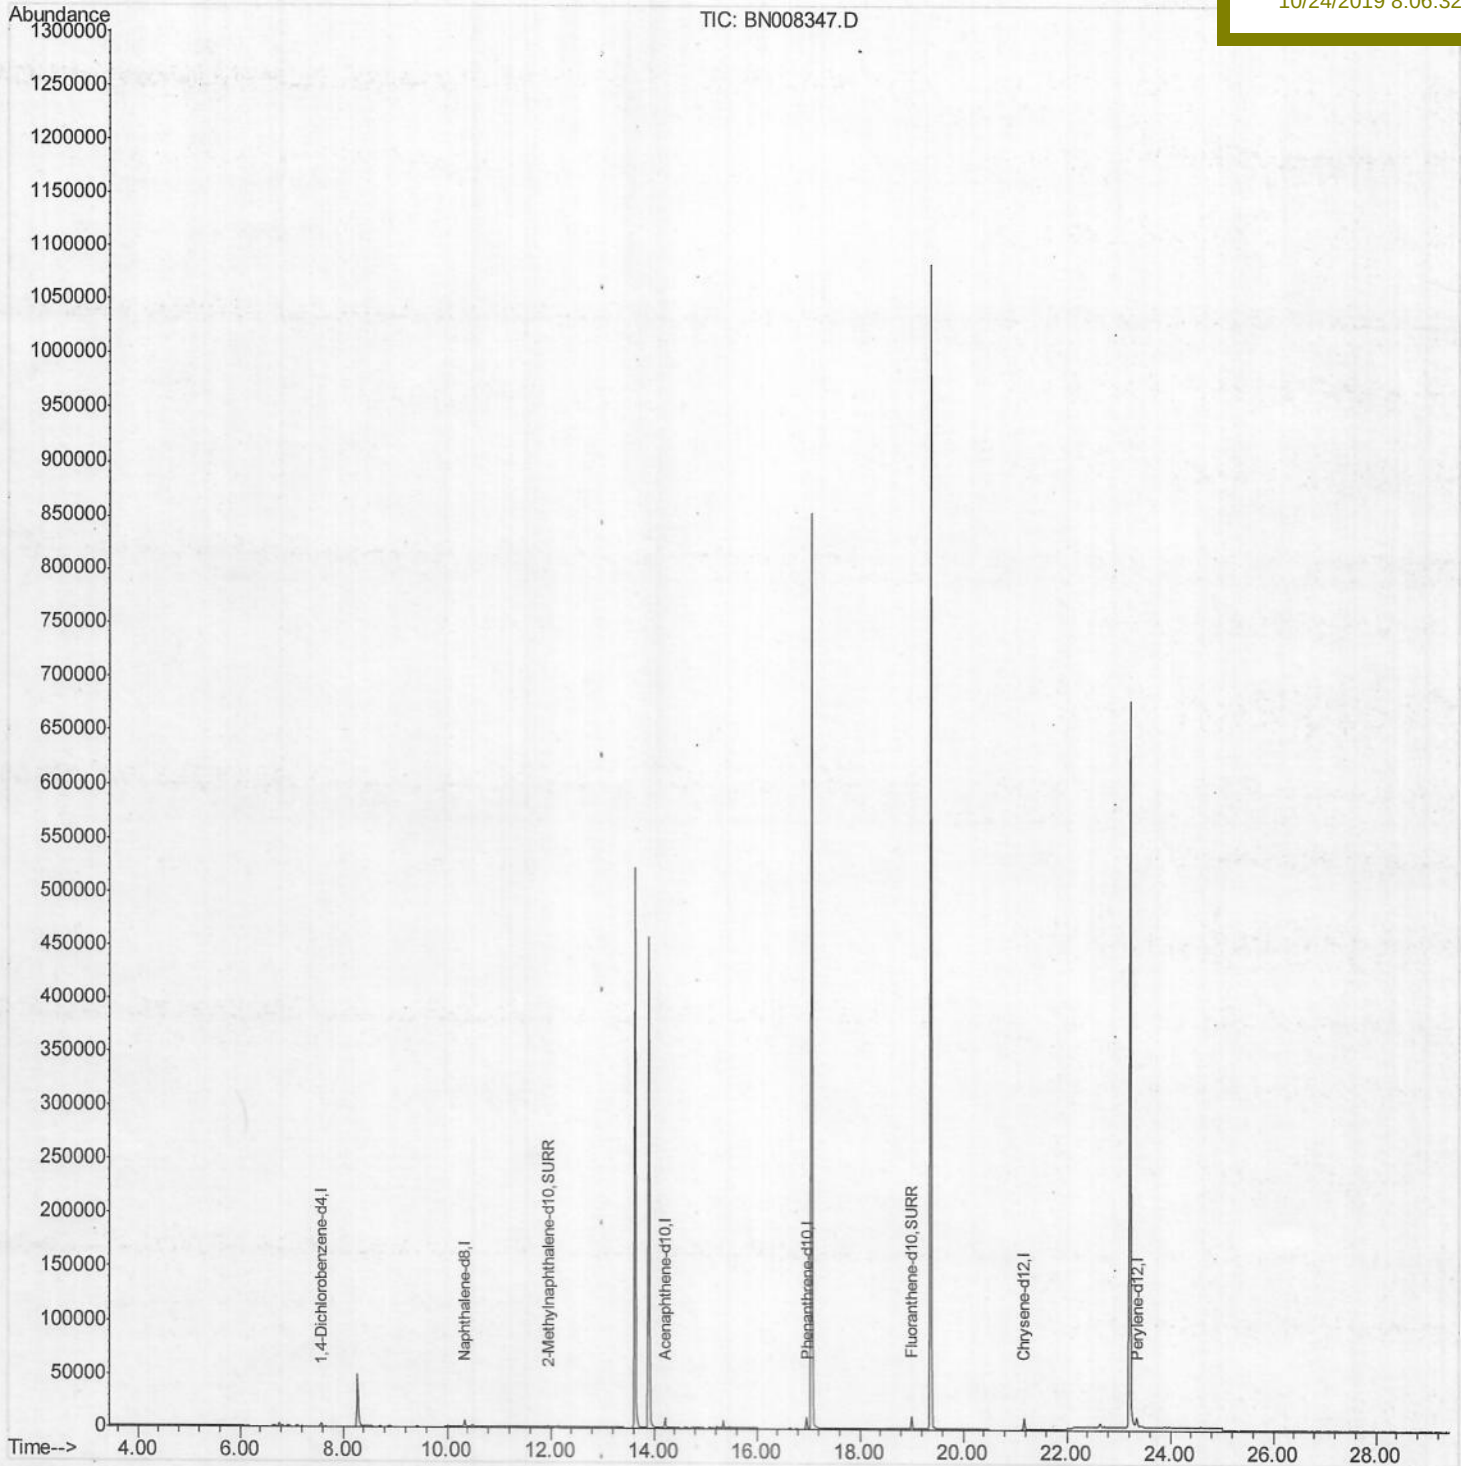

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102219\

Data File : BN008347.D

Acq On : 23 Oct 2019 13:09

Operator : JU

Sample : K5346-10

Misc :

ALS Vial : 41 Sample Multiplier: 1

Quant Time: Oct 23 14:17:05 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Oct 23 11:13:51 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :


ETON4

Manual Integrations

APPROVED

mohammad

10/24/2019 8:06:32 AM

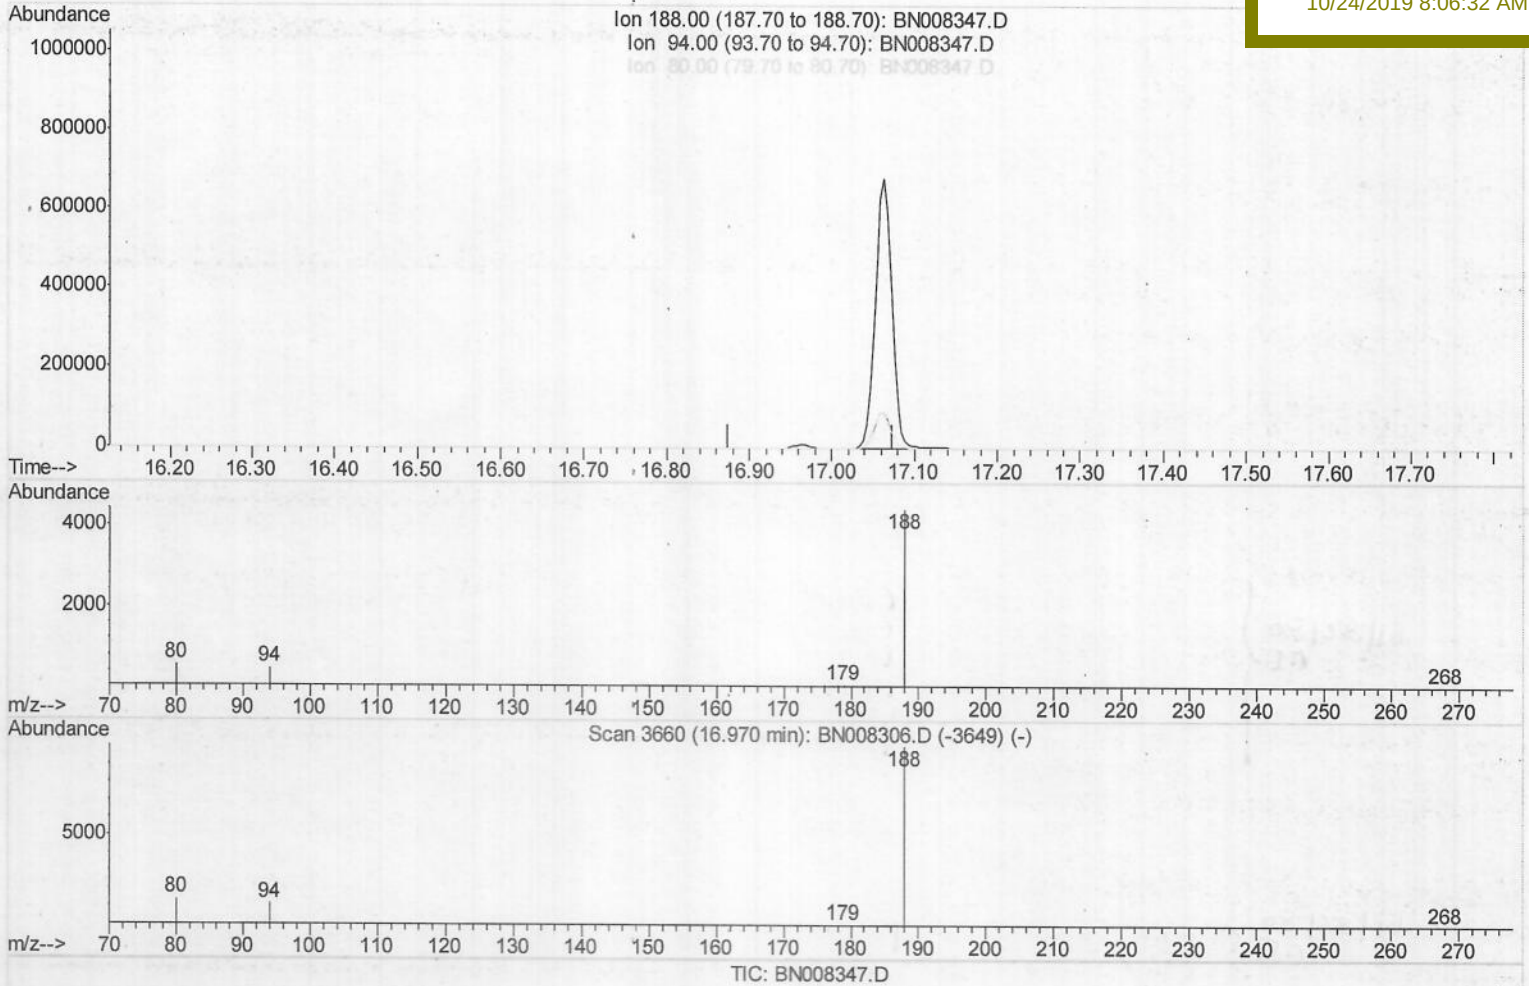

(10) Phenanthrene-d10 (I)

16.975min (-16.975) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.90	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102219\
 Data File : BN008347.D
 Acq On : 23 Oct 2019 13:09
 Operator : JU
 Sample : K5346-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 ETON4

Manual Integrations
APPROVED

mohammad
 10/24/2019 8:06:32 AM

Quant Time: Oct 23 14:17:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 23 11:13:51 2019
 Response via : Initial Calibration

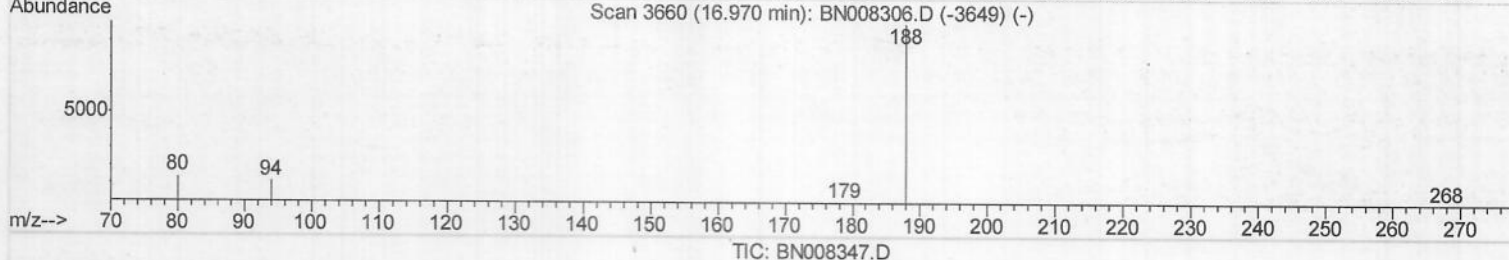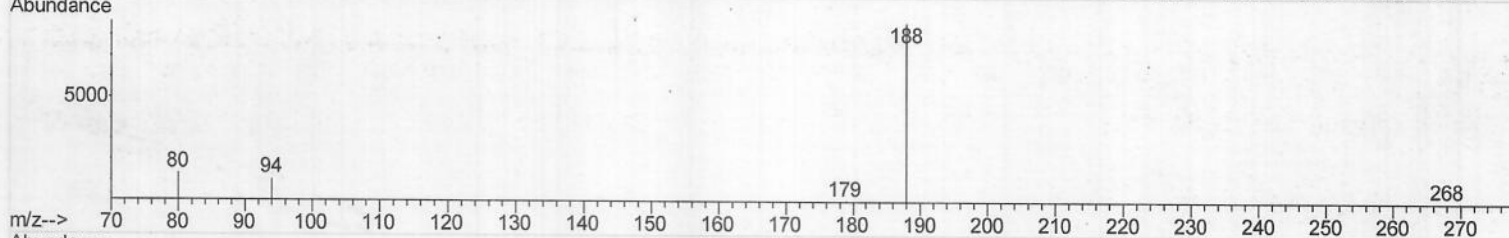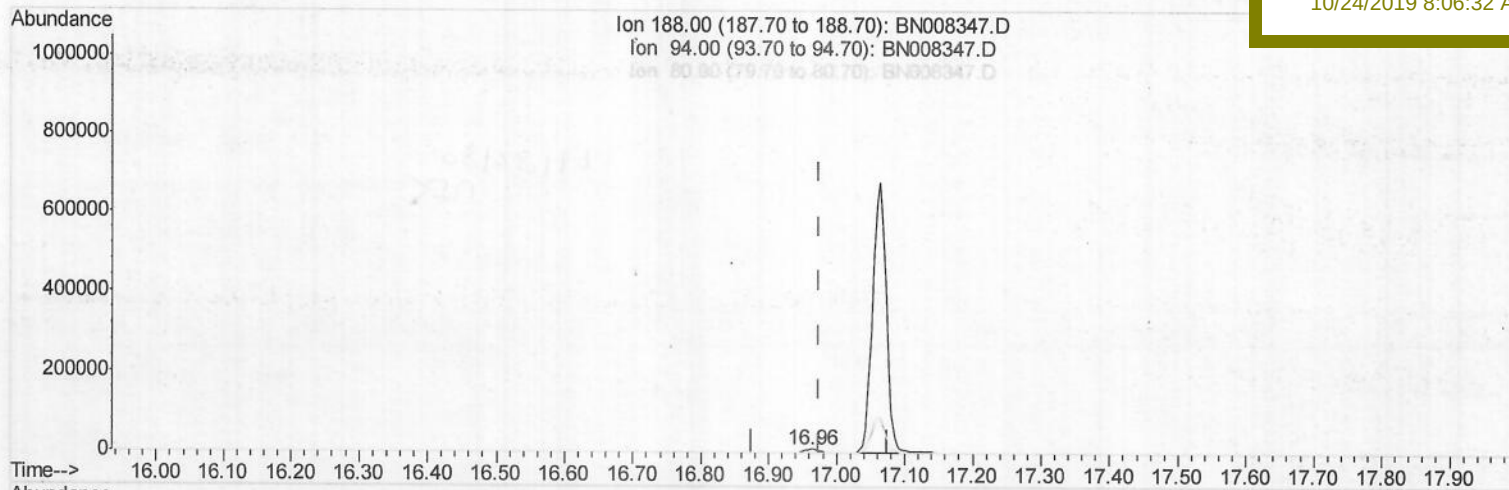

(10) Phenanthrene-d10 (I)

16.962min (-0.012) 0.40ng/ul m) JU
 10/24/19

response 12620

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	12.46
80.00	12.60	15.38#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102219\
Data File : BN008347.D
Acq On : 23 Oct 2019 13:09
Operator : JU
Sample : K5346-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Oct 23 14:19:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 11:13:51 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
ETON4

Manual Integrations
APPROVED

mohammad
10/24/2019 8:06:32 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	1821	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.33	136	8799	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.21	164	5566	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.96	188	12620m)	0.40	ng/ul	-0.01
16) Chrysene-d12	21.17	240	10924	0.40	ng/ul	0.00
20) Perylene-d12	23.35	264	12081	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.94	152	3544	0.24	ng/ul	-0.02
14) Fluoranthene-d10	19.00	212	13006	0.30	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
10/24/19