


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102219\
Data File : BN008351.D
Acq On : 23 Oct 2019 15:32
Operator : JU
Sample : K5346-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Oct 23 16:56:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 14:07:55 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
ETON6

Manual Integrations
APPROVED

mohammad
10/24/2019 8:06:41 AM

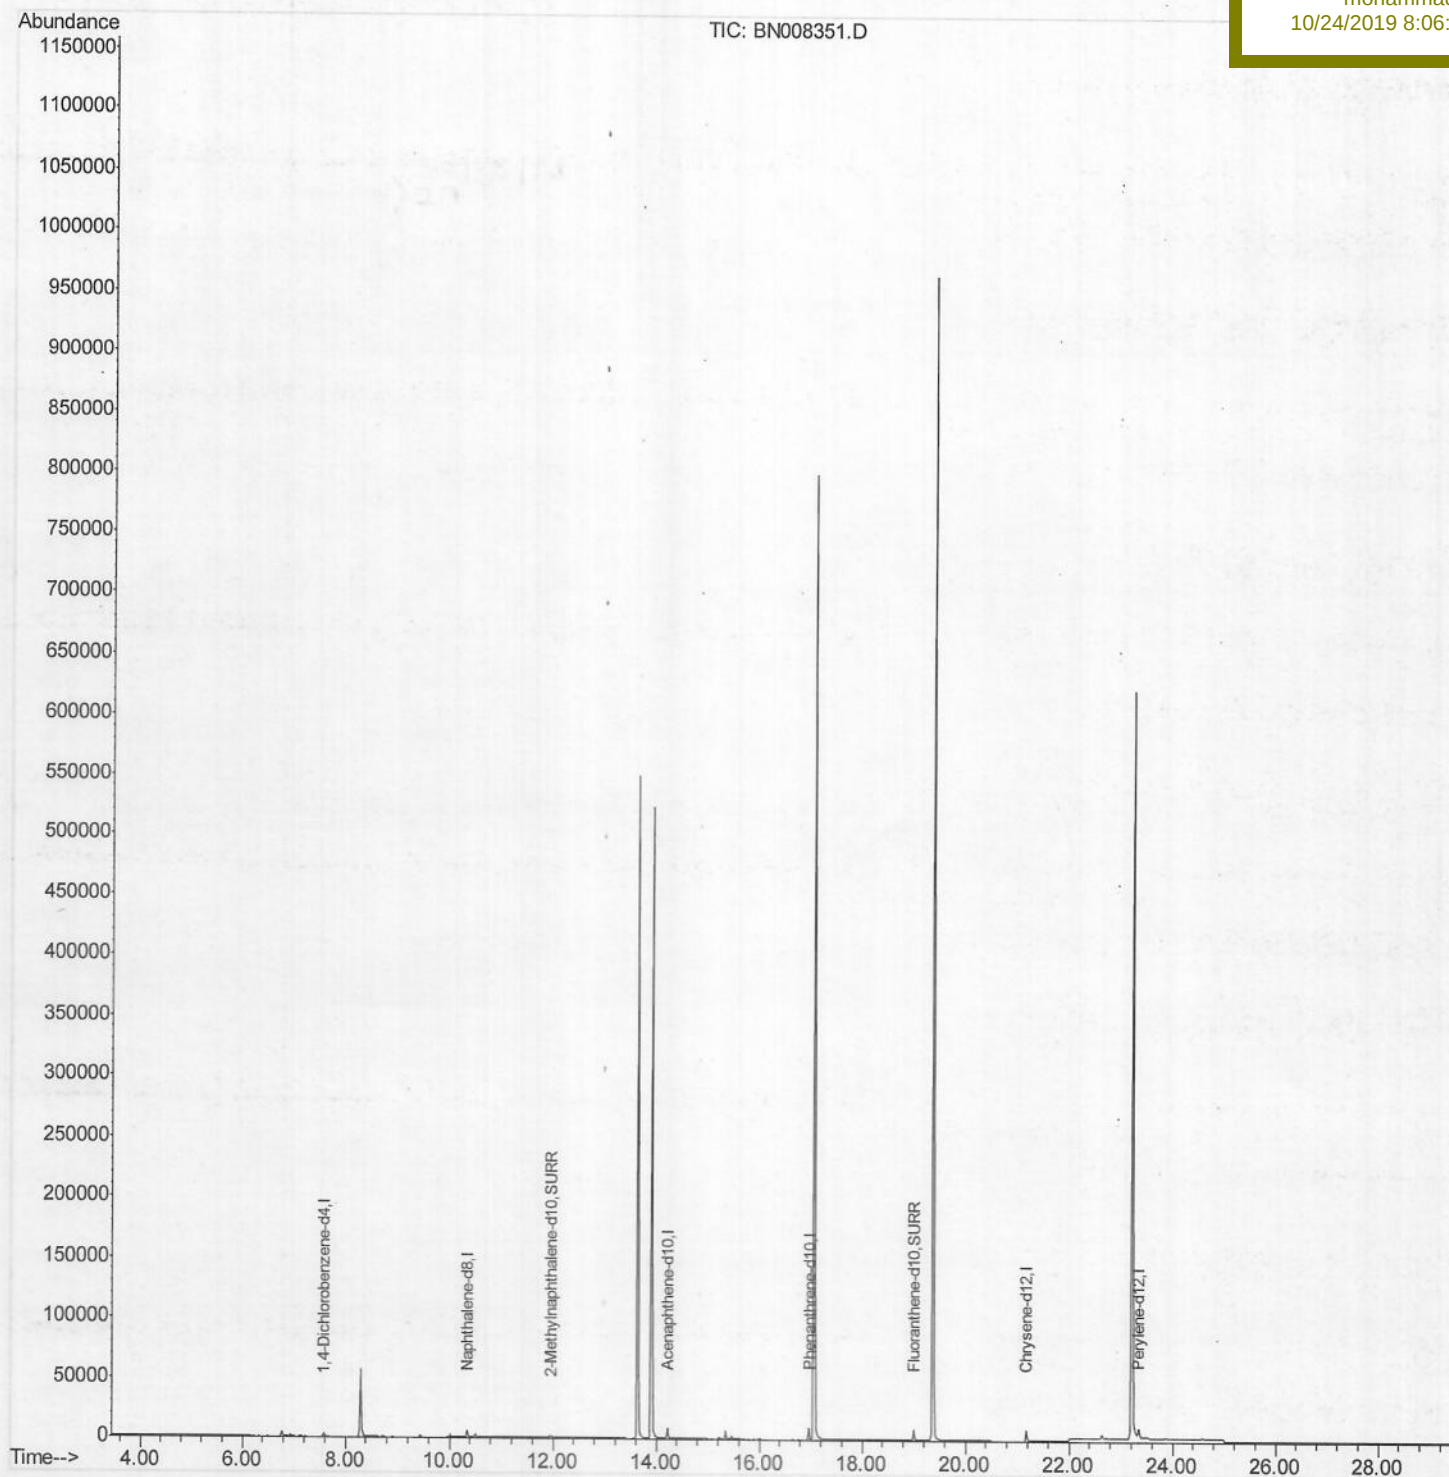

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102219\

Data File : BN008351.D

Acq On : 23 Oct 2019 15:32

Operator : JU

Sample : K5346-14

Misc :

ALS Vial : 45 Sample Multiplier: 1

Quant Time: Oct 23 16:55:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Oct 23 14:07:55 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :


ETON6

Manual Integrations

APPROVED

mohammad

10/24/2019 8:06:41 AM

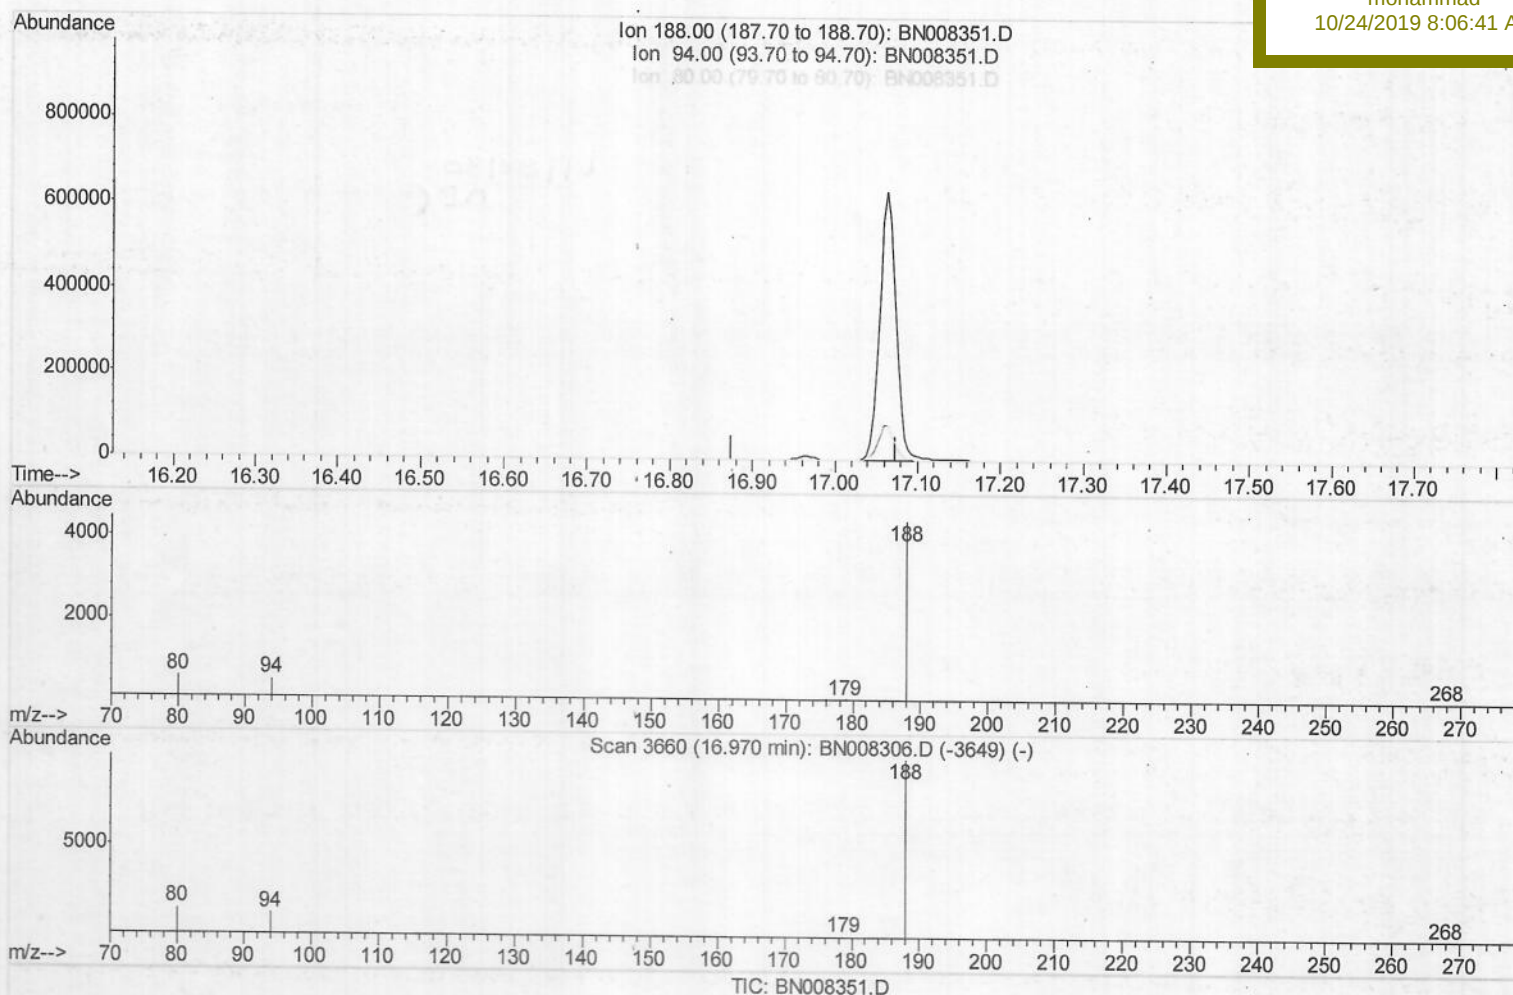

(10) Phenanthrene-d10 (I)

16.975min (-16.975) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.90	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102219\

Data File : BN008351.D

Acq On : 23 Oct 2019 15:32

Operator : JU

Sample : K5346-14

Misc :

ALS Vial : 45 Sample Multiplier: 1

Quant Time: Oct 23 16:55:30 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Oct 23 14:07:55 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

ETON6

Manual Integrations
APPROVED

mohammad

10/24/2019 8:06:41 AM

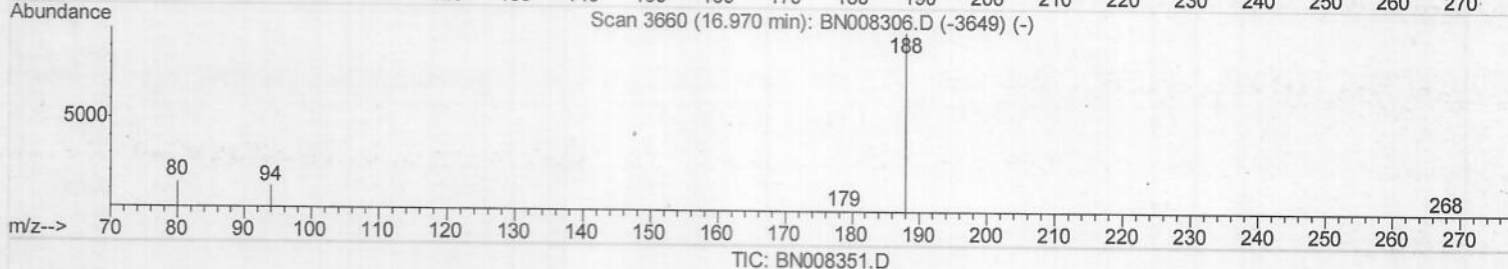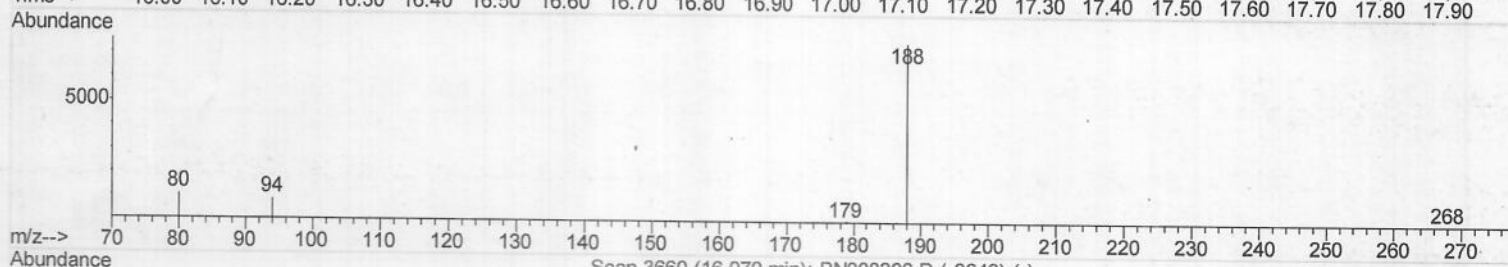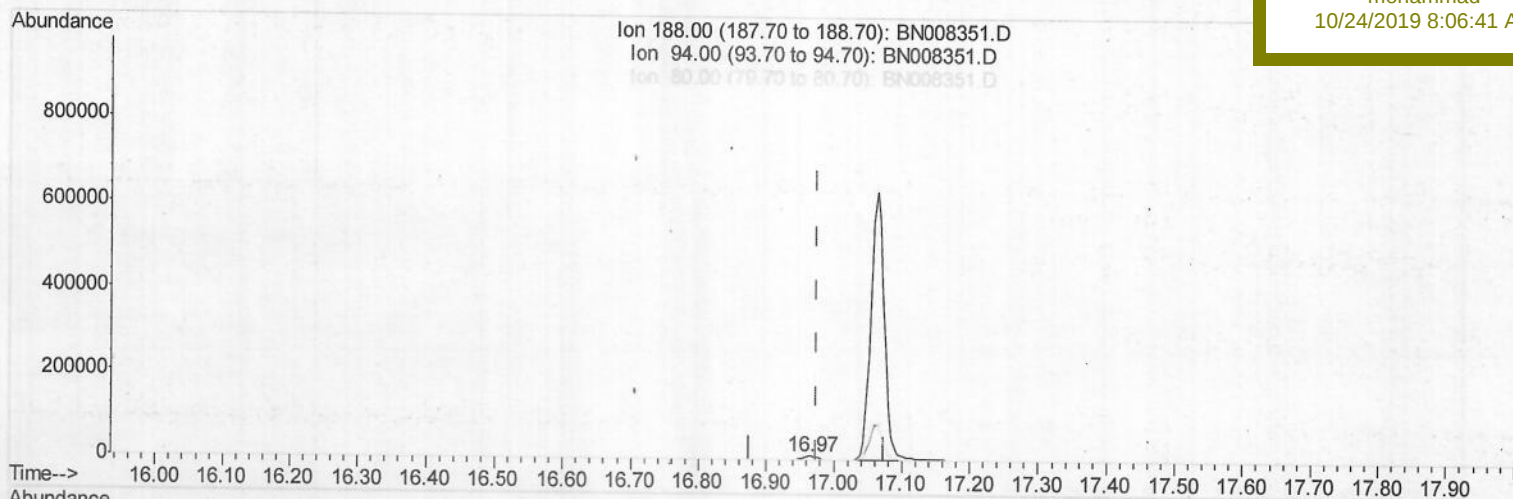

(10) Phenanthrene-d10 (I)

16.966min (-0.008) 0.40ng/ul m

response 10868

Ion Exp% Act%

188.00 100 100

94.00 10.90 11.65

80.00 12.60 14.23

0.00 0.00 0.00

JU
10/24/19

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102219\
Data File : BN008351.D
Acq On : 23 Oct 2019 15:32
Operator : JU
Sample : K5346-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Oct 23 16:56:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 14:07:55 2019
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
ETON6

Manual Integrations
APPROVED

mohammad
10/24/2019 8:06:41 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	1633	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.34	136	7876	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.21	164	4939	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.97	188	10868m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.17	240	9434	0.40	ng/ul	0.00
20) Perylene-d12	23.34	264	9012	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.95	152	3754	0.28	ng/ul	-0.01
14) Fluoranthene-d10	19.00	212	10599	0.28	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed