
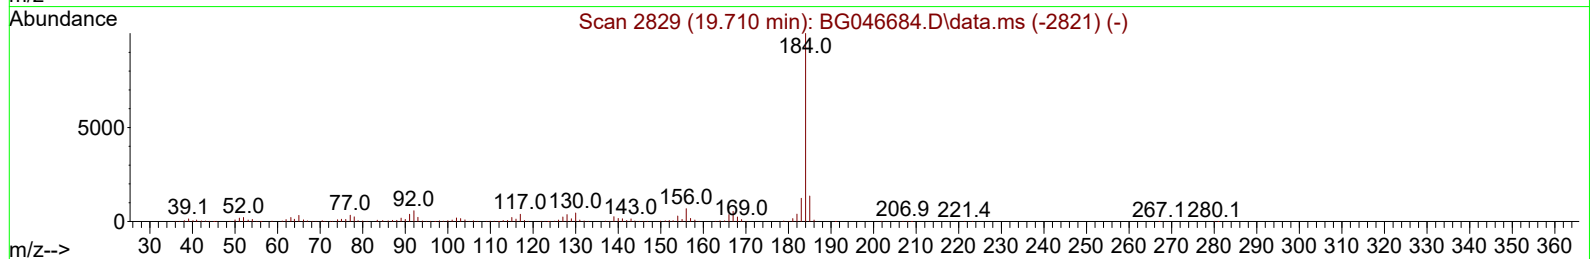
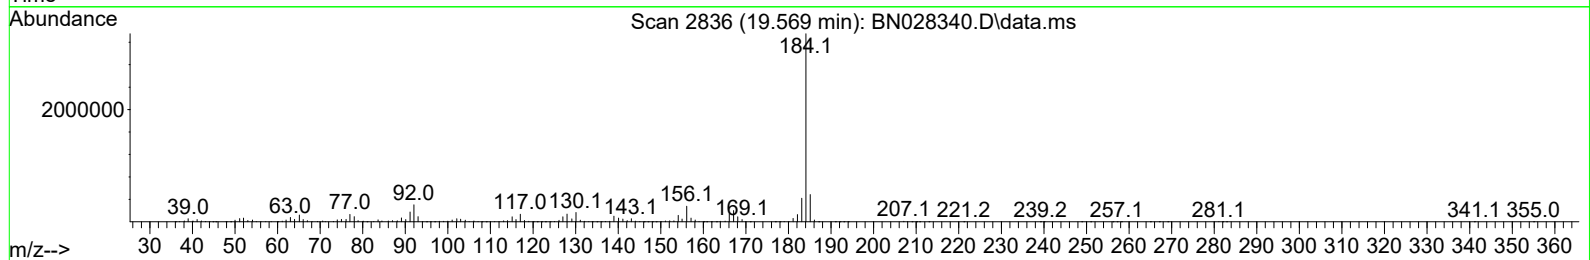


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
 Data File : BN028340.D
 Acq On : 23 Oct 2023 08:51
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 19:17:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 02:49:17 2023
 Response via : Initial Calibration

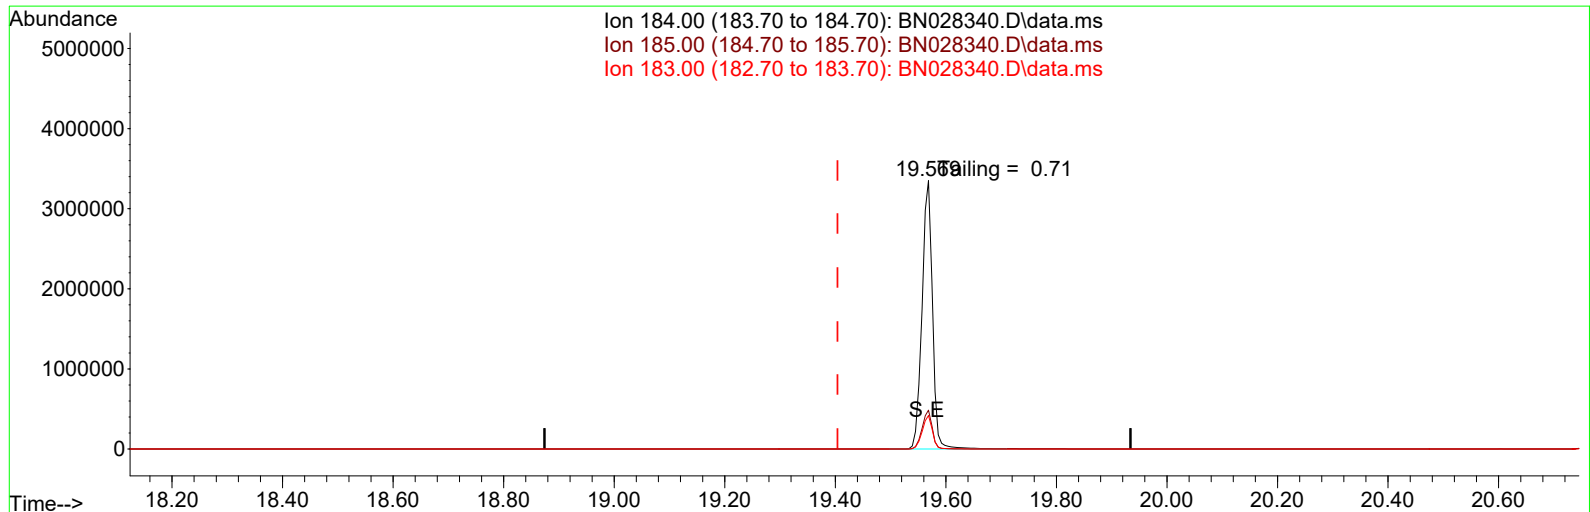

TIC: BN028340.D\data.ms

(77) Benzidine




19.569min (+ 0.165) 0.00 ng

response 4420615

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	12.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
Data File : BN028340.D
Acq On : 23 Oct 2023 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 19:17:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:49:17 2023
Response via : Initial Calibration

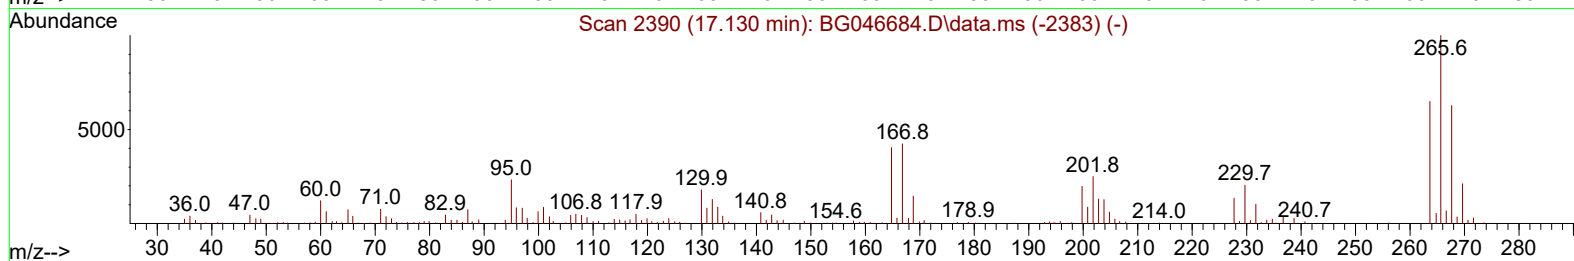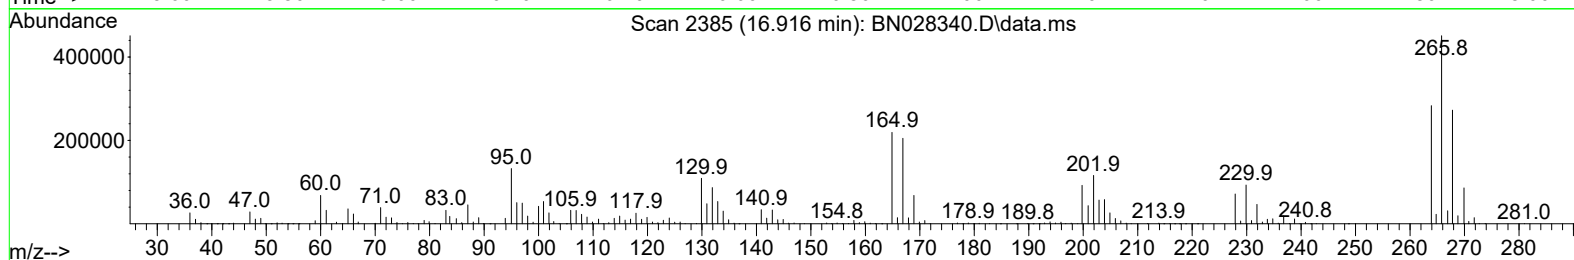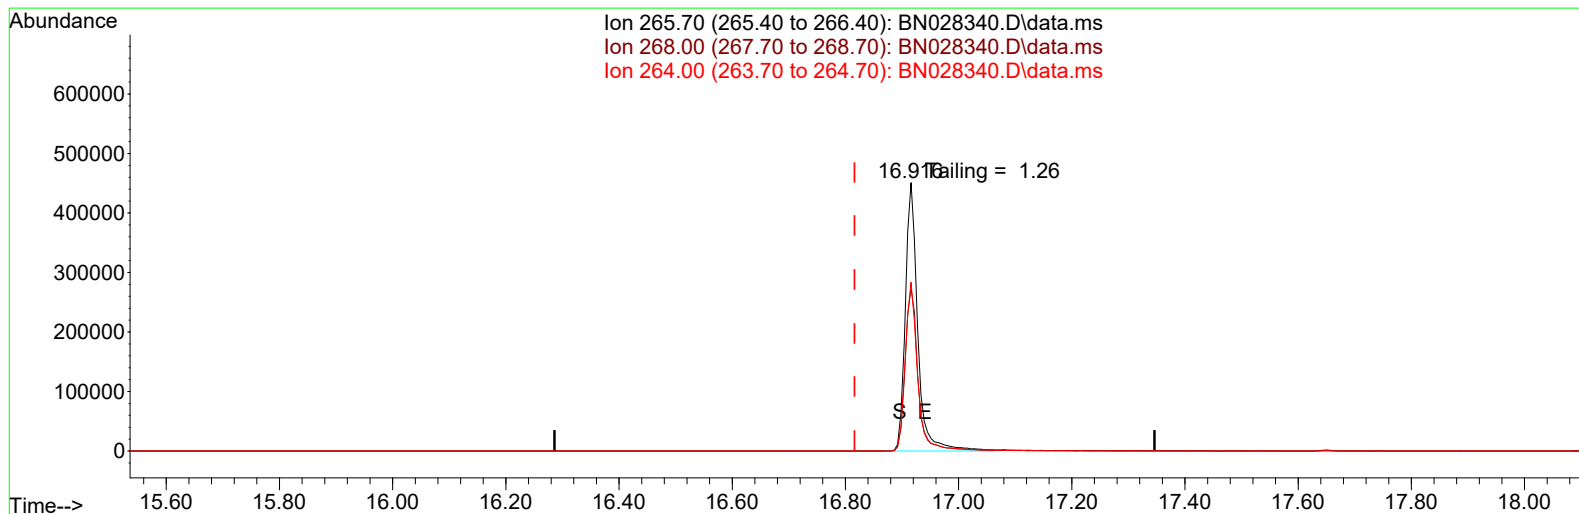

TIC: BN028340.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.100) 20798.85 ng

response 691744

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.45
264.00	61.60	62.85
0.00	0.00	0.00