

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
 Data File : BN028362.D
 Acq On : 24 Oct 2023 01:37
 Operator : MA/JU
 Sample : 04913-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-48S

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/24/2023
 Supervised By :mohammad ahmed 10/25/2023

Quant Time: Oct 24 03:23:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 23 15:14:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	2820	0.400	ng	0.01
7) Naphthalene-d8	10.724	136	9159	0.400	ng	# 0.02
13) Acenaphthene-d10	14.533	164	6131	0.400	ng	0.00
19) Phenanthrene-d10	17.294	188	14357	0.400	ng	# 0.00
29) Chrysene-d12	21.488	240	14616	0.400	ng	0.00
35) Perylene-d12	23.928	264	14326	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.430	112	1193	0.136	ng	0.00
5) Phenol-d6	7.156	99	724m	0.067	ng	0.10
8) Nitrobenzene-d5	9.144	82	2359	0.290	ng	0.04
11) 2-Methylnaphthalene-d10	12.313	152	5329	0.387	ng	0.02
14) 2,4,6-Tribromophenol	16.052	330	906	0.303	ng	-0.01
15) 2-Fluorobiphenyl	13.176	172	7589	0.352	ng	0.01
27) Fluoranthene-d10	19.323	212	18611	0.485	ng	0.00
31) Terphenyl-d14	19.908	244	16039	0.517	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.299	88	431	0.126	ng	# 60
34) Bis(2-ethylhexyl)phtha...	21.336	149	4025	0.101	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
Data File : BN028362.D
Acq On : 24 Oct 2023 01:37
Operator : MA/JU
Sample : 04913-01
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
MW-48S

Quant Time: Oct 24 03:23:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 23 15:14:08 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/24/2023
Supervised By :mohammad ahmed 10/25/2023

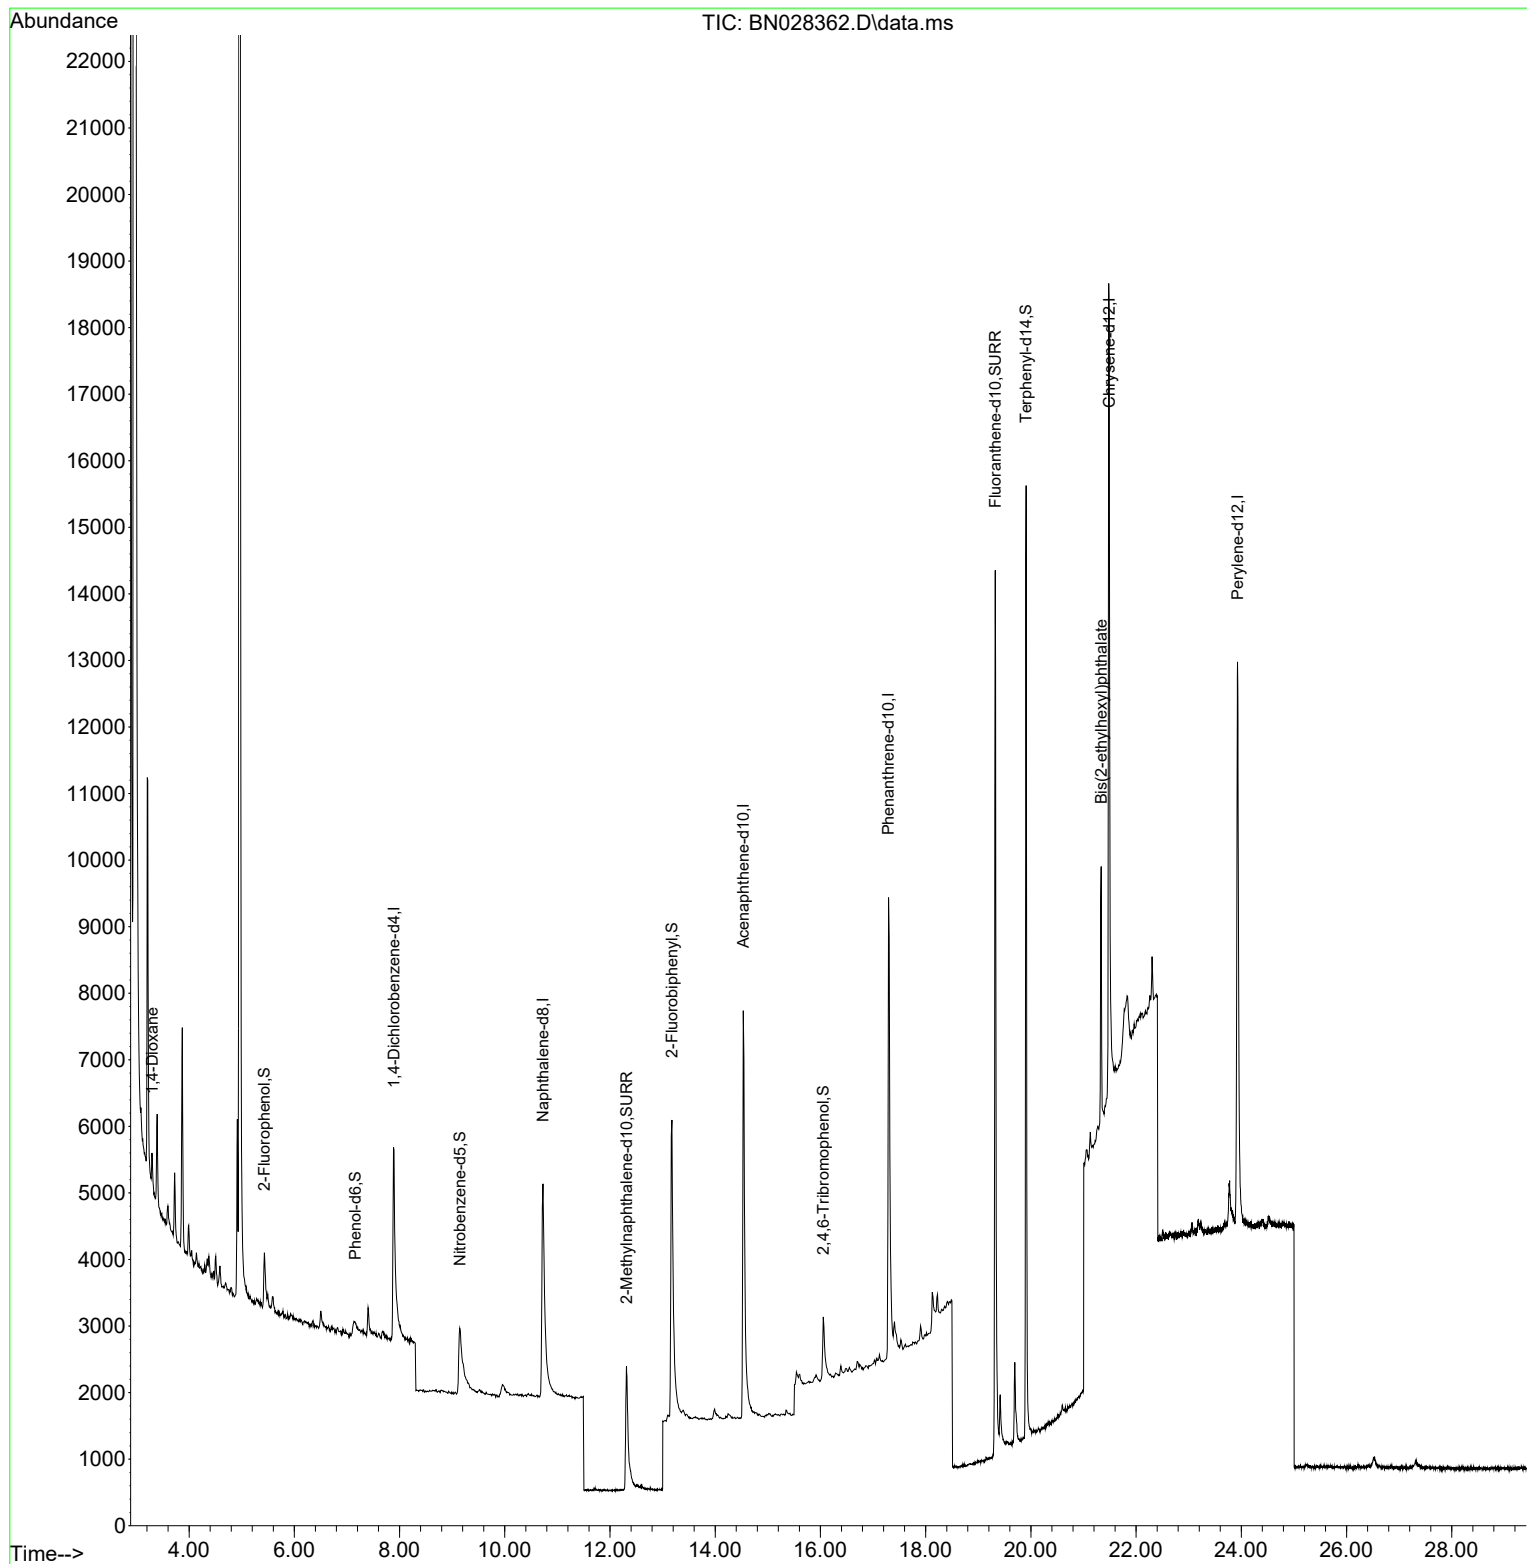

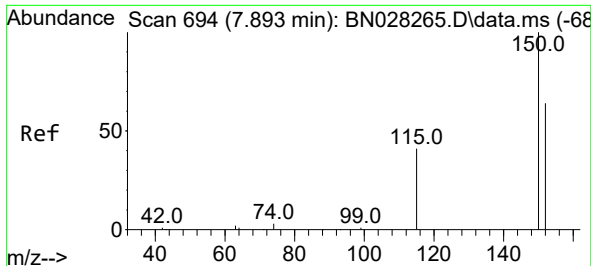

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.893 min Scan# 694
 Delta R.T. 0.015 min
 Lab File: BN028362.D
 Acq: 24 Oct 2023 01:37




Instrument :
 BNA_N
 ClientSampleId :
 MW-48S

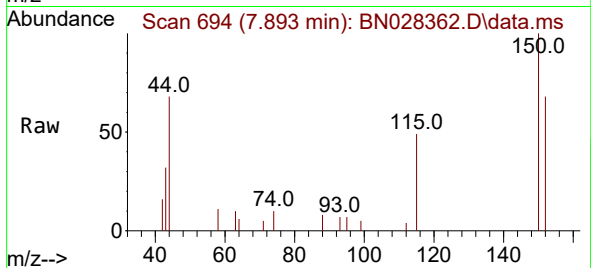


Tgt Ion: 152 Resp: 2820
 Ion Ratio Lower Upper
 152 100
 150 147.0 121.6 182.4
 115 72.7 54.3 81.5

Manual Integrations
 APPROVED



Reviewed By :Yogesh Patel 10/24/2023
 Supervised By :mohammad ahmed 10/25/2023

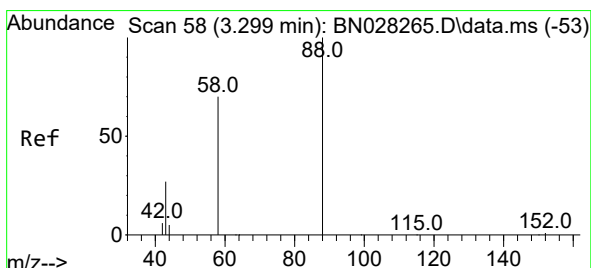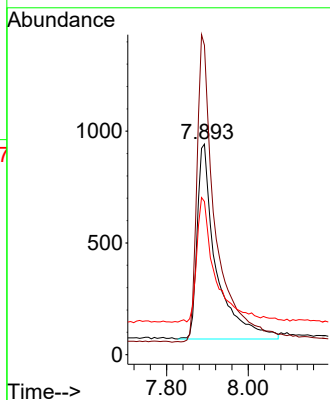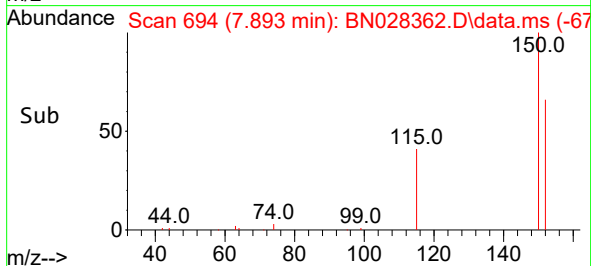


#2
 1,4-Dioxane
 Concen: 0.126 ng
 RT: 3.299 min Scan# 58
 Delta R.T. -0.000 min
 Lab File: BN028362.D
 Acq: 24 Oct 2023 01:37

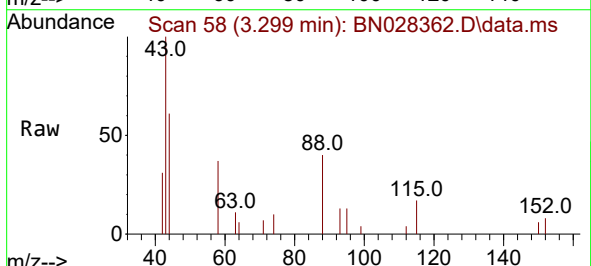

Tgt Ion: 88 Resp: 431
 Ion Ratio Lower Upper
 88 100
 43 88.4 26.6 39.8
 58 78.9 55.4 83.0

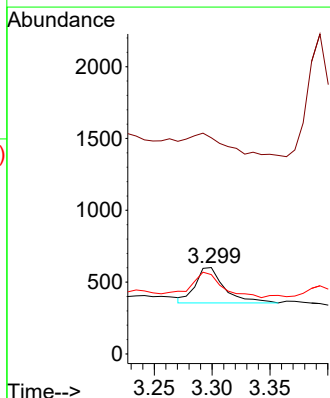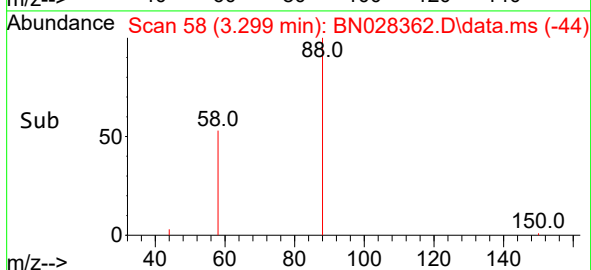

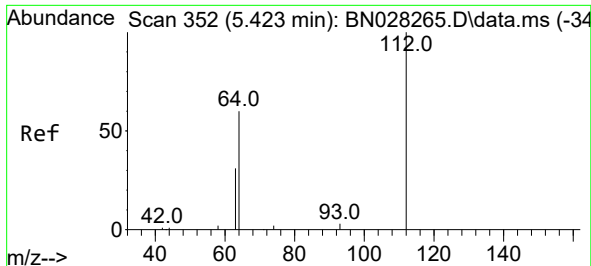





#4
2-Fluorophenol
Concen: 0.136 ng
RT: 5.430 min Scan# 352
Delta R.T. -0.000 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37

Instrument :
BNA_N
ClientSampleId :
MW-48S

Tgt Ion:112 Resp: 119
Ion Ratio Lower Upper
112 100
64 56.3 46.9 70.3
63 34.0 25.0 37.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/24/2023
Supervised By :mohammad ahmed 10/25/2023

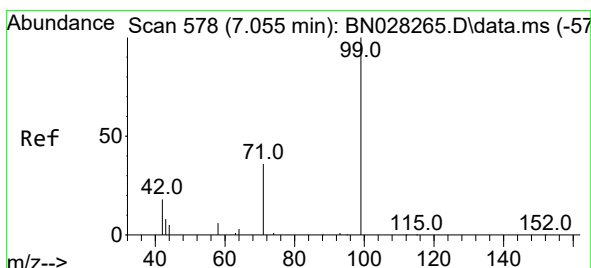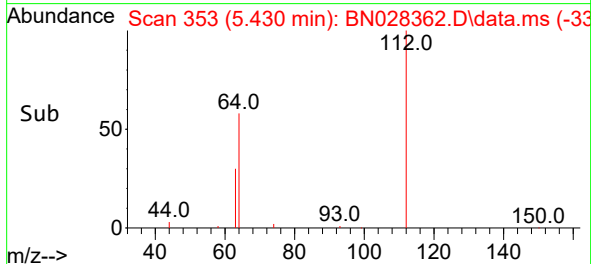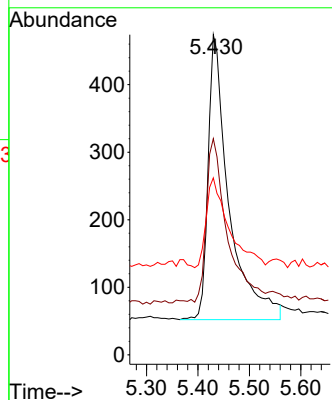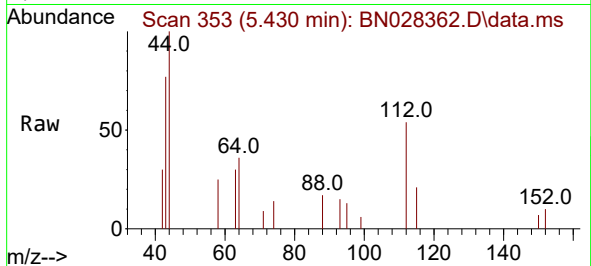

#5
Phenol-d6
Concen: 0.067 ng m
RT: 7.156 min Scan# 592
Delta R.T. 0.101 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37


Tgt Ion: 99 Resp: 724
Ion Ratio Lower Upper
99 100
42 2.6 15.9 23.9#
71 20.6 28.6 42.8#

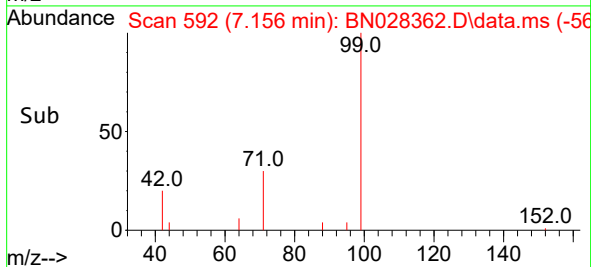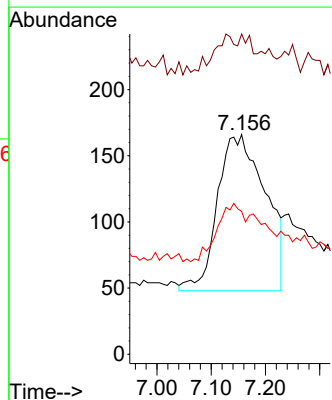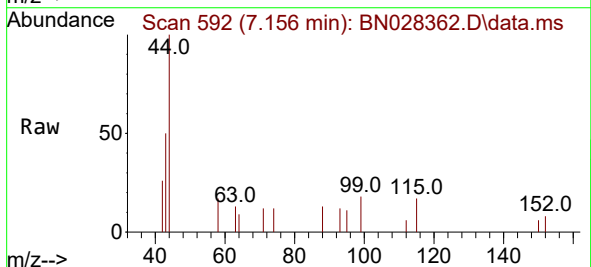

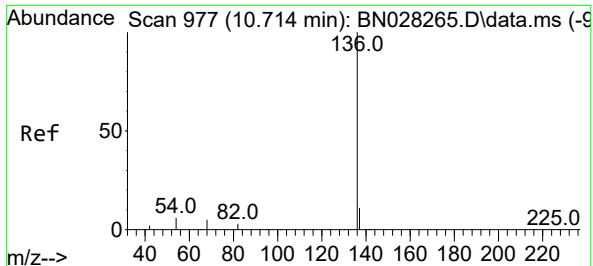

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.724 min Scan# 915
Delta R.T. 0.021 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37




Instrument :
BNA_N
ClientSampleId :
MW-48S

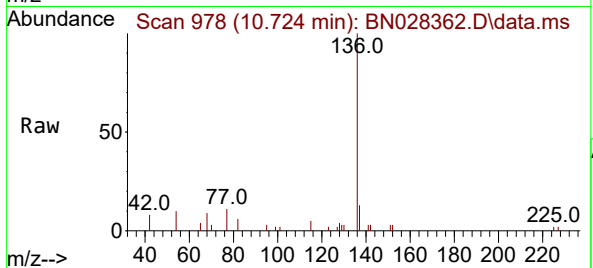

Tgt Ion:136 Resp: 915
Ion Ratio Lower Upper
136 100
137 12.8 9.8 14.8
54 10.4 6.2 9.4
68 9.2 5.7 8.5#




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 10/24/2023
Supervised By :mohammad ahmed 10/25/2023

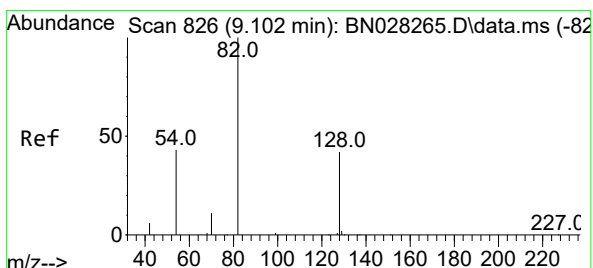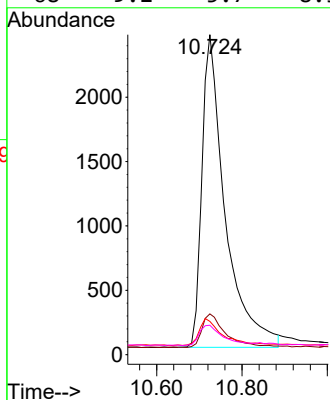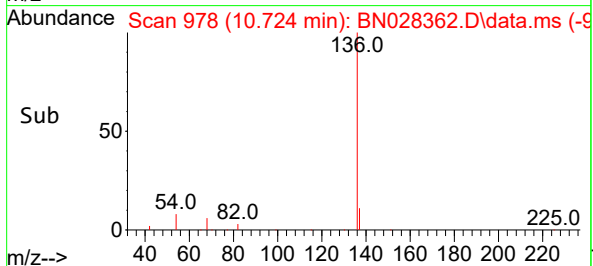

#8
Nitrobenzene-d5
Concen: 0.290 ng
RT: 9.144 min Scan# 830
Delta R.T. 0.043 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37


Tgt Ion: 82 Resp: 2359
Ion Ratio Lower Upper
82 100
128 49.9 36.8 55.2
54 57.0 37.4 56.2#

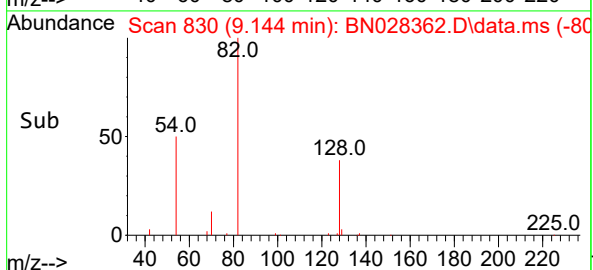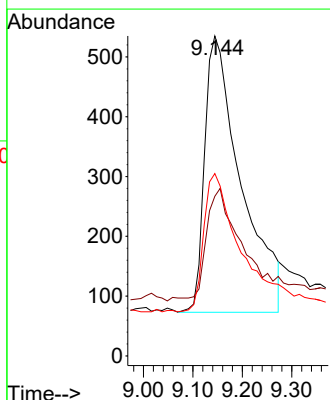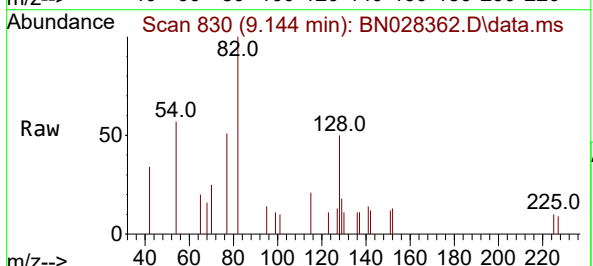

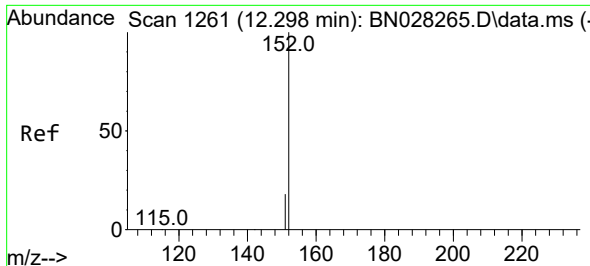

#11
2-Methylnaphthalene-d10
Concen: 0.387 ng
RT: 12.313 min Scan# 151
Delta R.T. 0.019 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37




Instrument :
BNA_N
ClientSampleId :
MW-48S

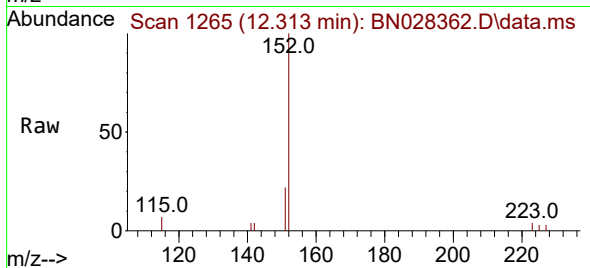


Tgt Ion:152 Resp: 5329
Ion Ratio Lower Upper
152 100
151 20.2 16.1 24.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 10/24/2023
Supervised By :mohammad ahmed 10/25/2023

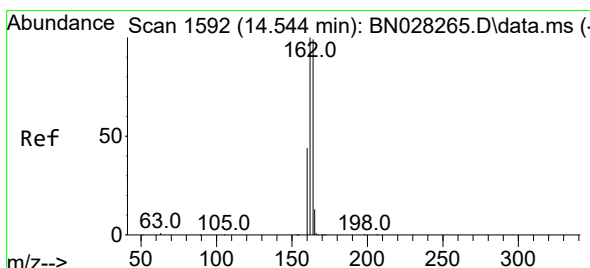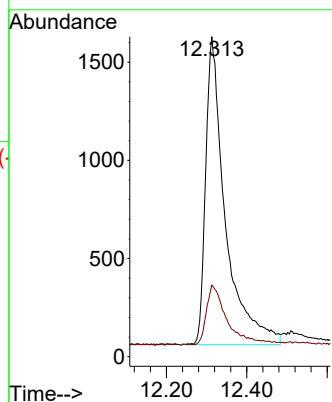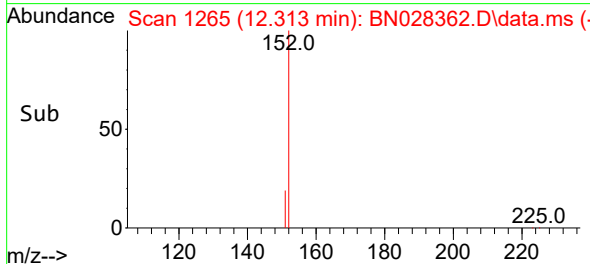


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.533 min Scan# 1591
Delta R.T. -0.000 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37

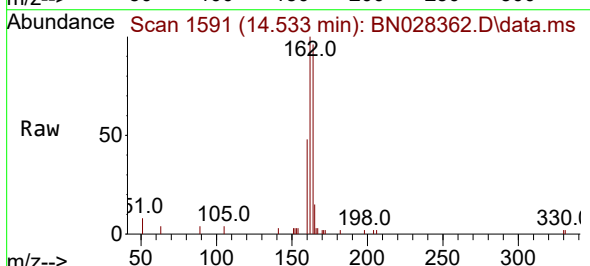


Tgt Ion:164 Resp: 6131
Ion Ratio Lower Upper
164 100
162 104.5 81.1 121.7
160 49.8 36.6 54.8

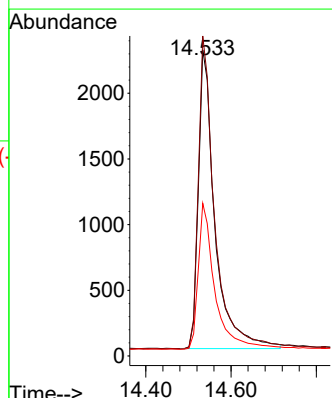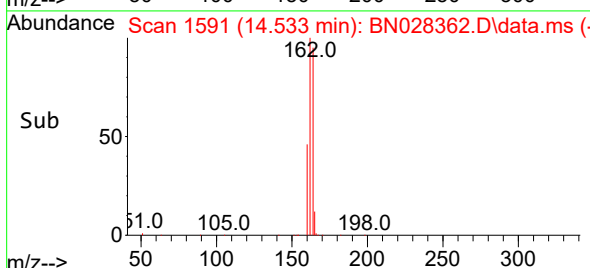

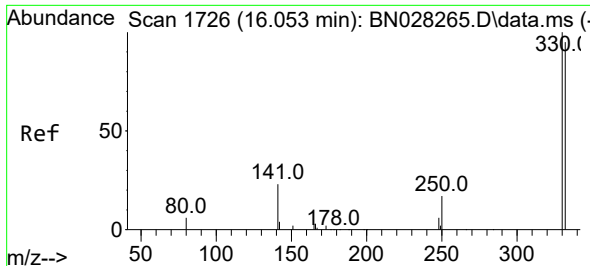

#14
2,4,6-Tribromophenol
Concen: 0.303 ng
RT: 16.052 min Scan# 11
Delta R.T. -0.012 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37




Instrument :
BNA_N
ClientSampleId :
MW-48S

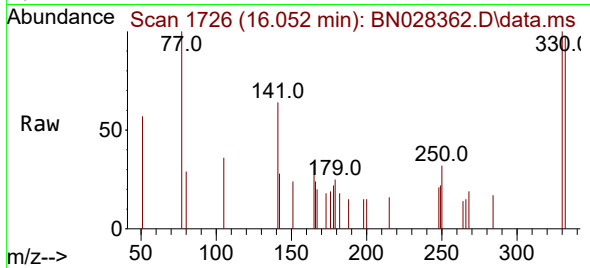


Tgt Ion:330 Resp: 900
Ion Ratio Lower Upper
330 100
332 97.7 74.1 111.1
141 50.4 32.1 48.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 10/24/2023
Supervised By :mohammad ahmed 10/25/2023

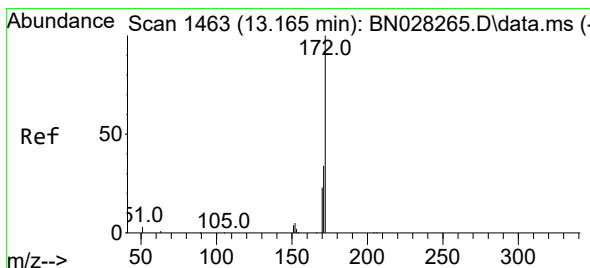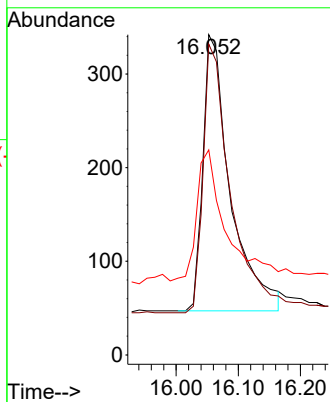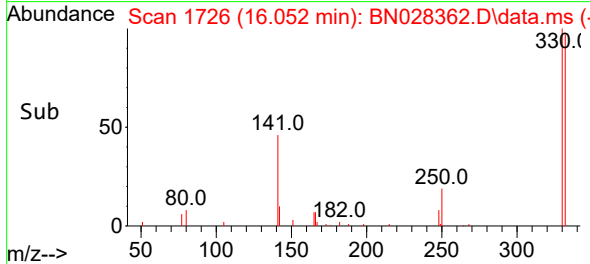


#15
2-Fluorobiphenyl
Concen: 0.352 ng
RT: 13.176 min Scan# 1464
Delta R.T. 0.011 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37

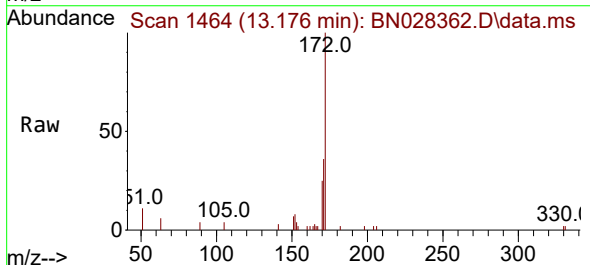


Tgt Ion:172 Resp: 7589
Ion Ratio Lower Upper
172 100
171 36.0 28.3 42.5
170 25.3 18.7 28.1

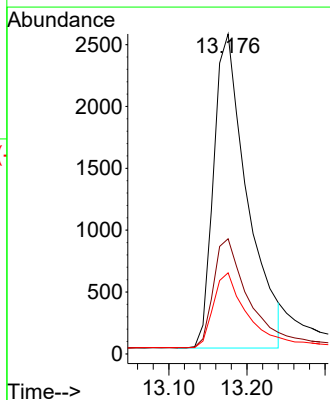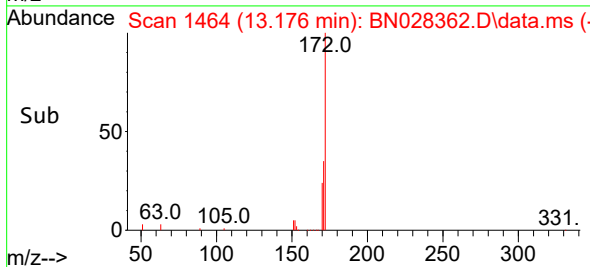

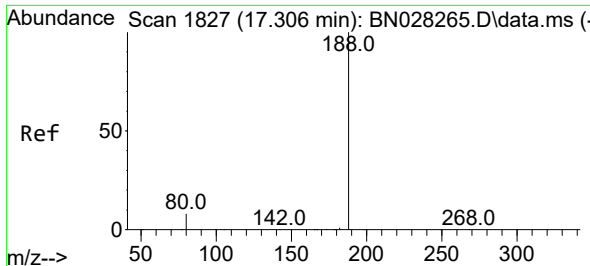

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.294 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37




Instrument :
BNA_N
ClientSampleId :
MW-48S

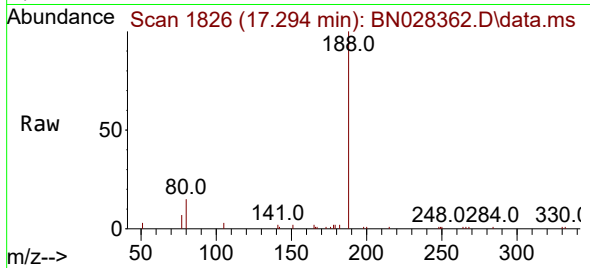


Tgt Ion:188 Resp: 1435
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.6 7.1 10.7

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 10/24/2023
Supervised By :mohammad ahmed 10/25/2023

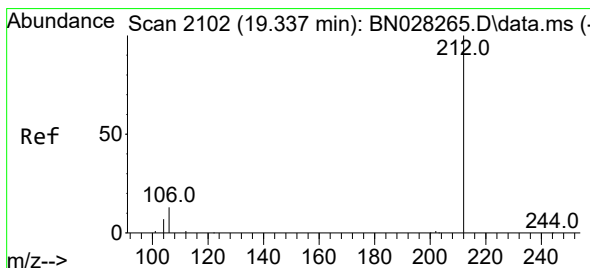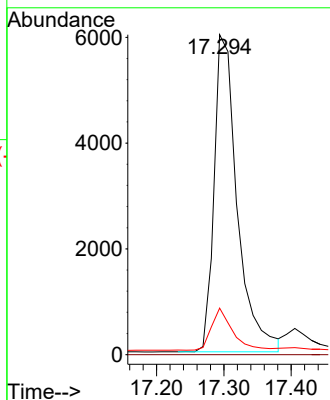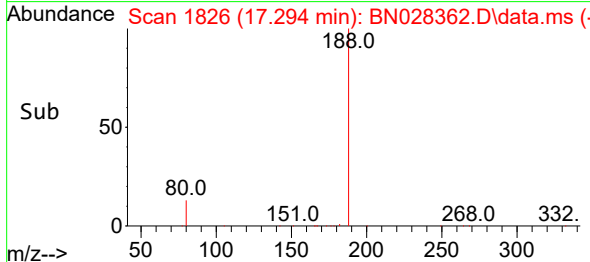


#27
Fluoranthene-d10
Concen: 0.485 ng
RT: 19.323 min Scan# 2099
Delta R.T. -0.005 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37

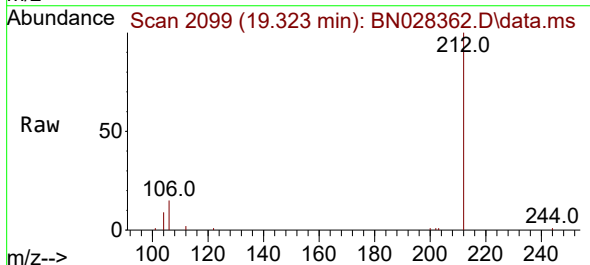


Tgt Ion:212 Resp: 18611
Ion Ratio Lower Upper
212 100
106 14.3 11.5 17.3
104 8.2 6.7 10.1

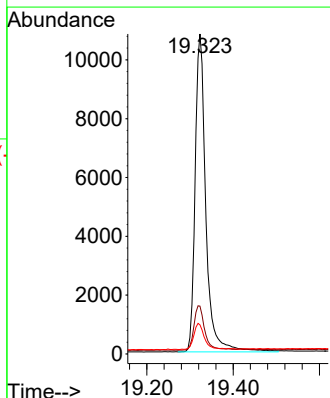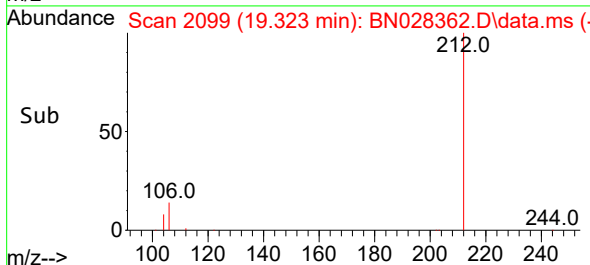

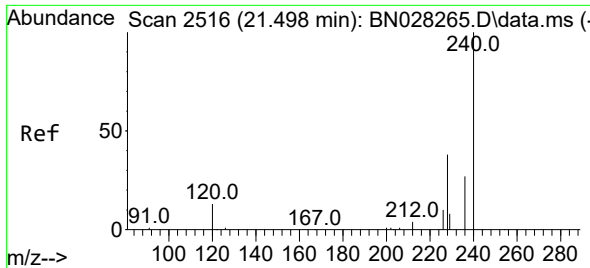

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.488 min Scan# 21488
Delta R.T. -0.000 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37




Instrument :
BNA_N
ClientSampleId :
MW-48S

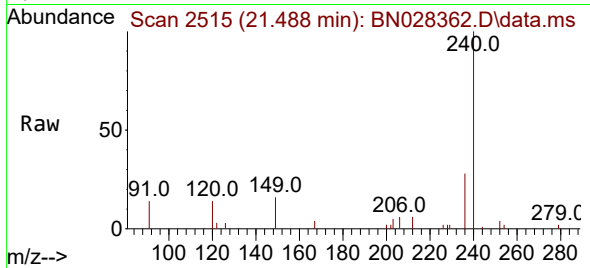


Tgt Ion:240 Resp: 14610
Ion Ratio Lower Upper
240 100
120 13.6 13.4 20.0
236 27.6 22.7 34.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 10/24/2023
Supervised By :mohammad ahmed 10/25/2023

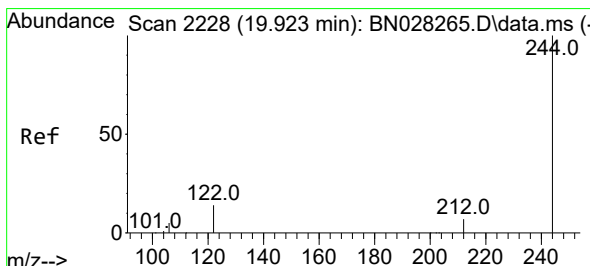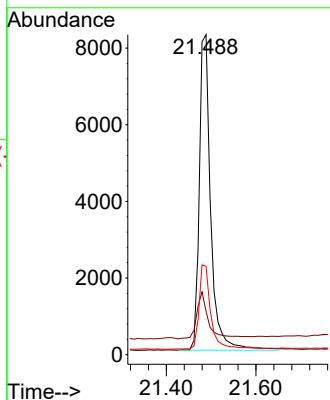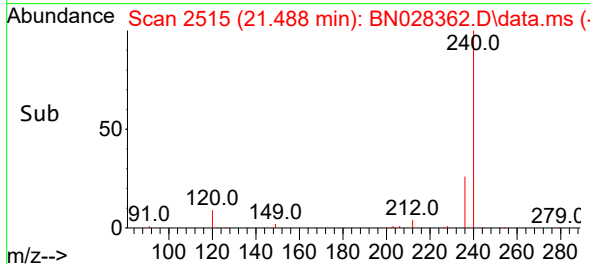


#31
Terphenyl-d14
Concen: 0.517 ng
RT: 19.908 min Scan# 2225
Delta R.T. -0.009 min
Lab File: BN028362.D
Acq: 24 Oct 2023 01:37

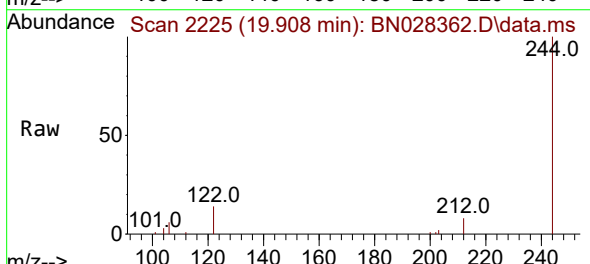

Tgt Ion:244 Resp: 16039
Ion Ratio Lower Upper
244 100
212 8.5 6.6 10.0
122 14.3 11.7 17.5

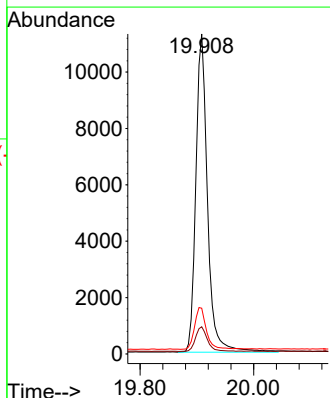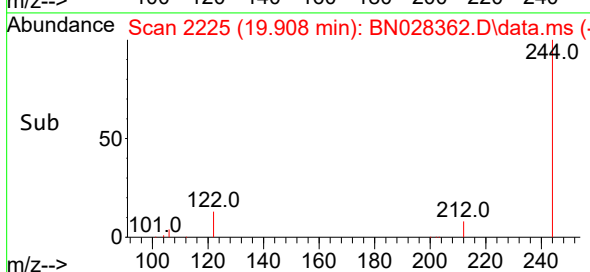

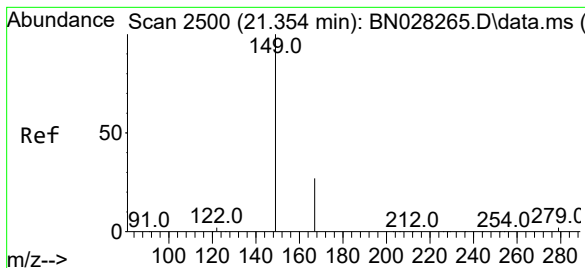

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.101 ng

RT: 21.336 min Scan# 2498

Delta R.T. -0.009 min

Lab File: BN028362.D

Acq: 24 Oct 2023 01:37

Instrument :

BNA_N

ClientSampleId :

MW-48S

Tgt Ion:149 Resp: 4025





Ion	Ratio	Lower	Upper
149	100		
167	26.6	22.6	34.0
279	4.3	4.2	6.2

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 10/24/2023

Supervised By :mohammad ahmed 10/25/2023

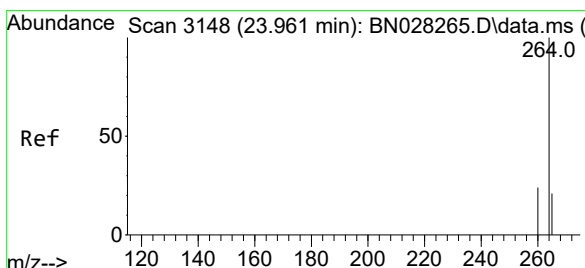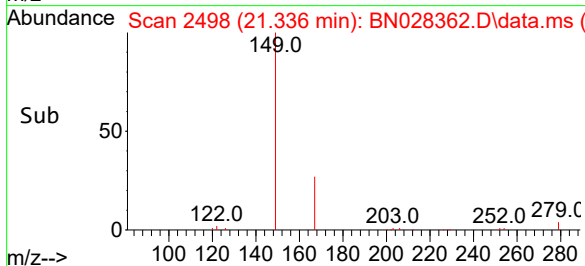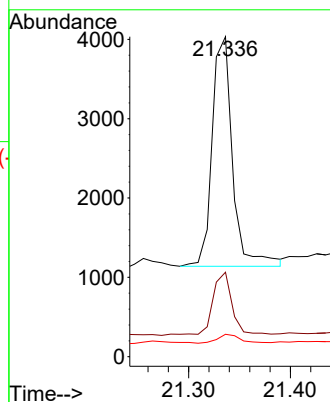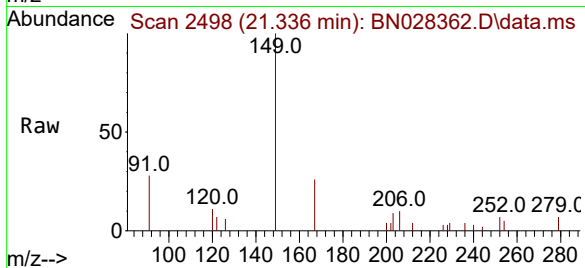

#35

Perylene-d12

Concen: 0.400 ng

RT: 23.928 min Scan# 3137

Delta R.T. -0.009 min

Lab File: BN028362.D

Acq: 24 Oct 2023 01:37

Tgt Ion:264 Resp: 14326

Ion	Ratio	Lower	Upper
264	100		
260	25.3	20.7	31.1
265	62.4	38.3	57.5

