
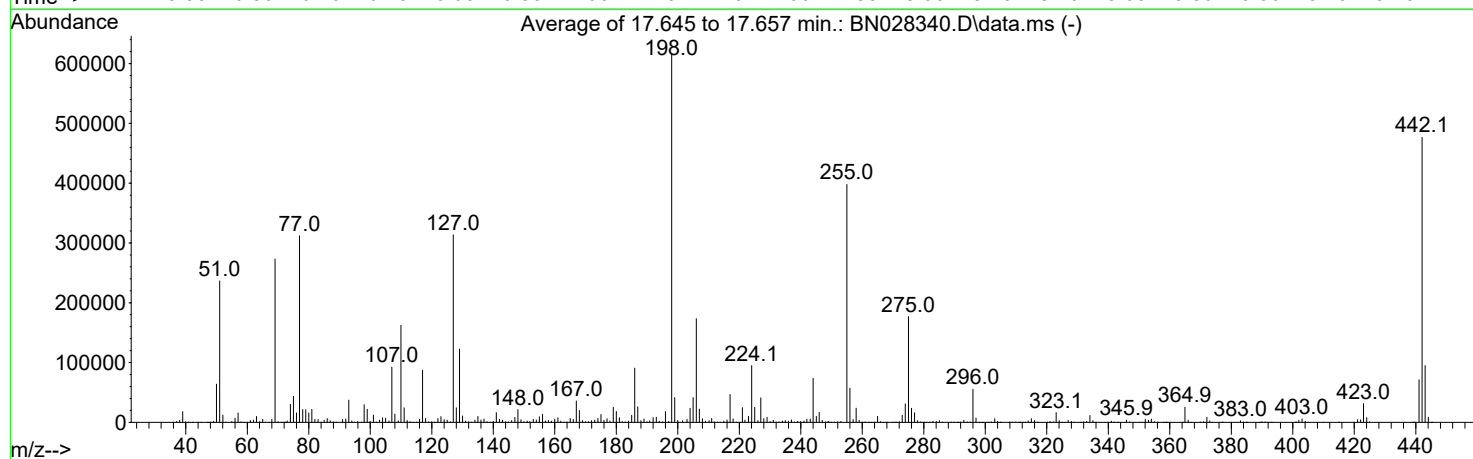


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
 Data File : BN028340.D
 Acq On : 23 Oct 2023 08:51
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP386

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 23 15:14:08 2023

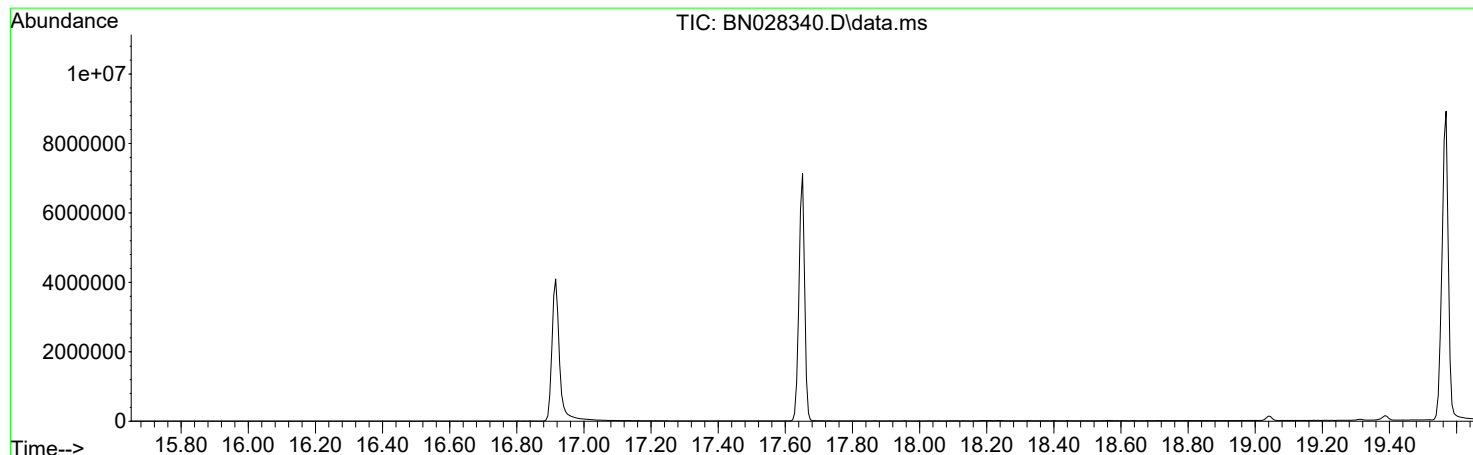




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	236437	PASS
68	69	0.00	2	1.9	5080	PASS
69	198	0.00	100	44.4	273173	PASS
70	69	0.00	2	0.5	1453	PASS
127	198	10	80	51.0	313515	PASS
197	198	0.00	2	0.3	1649	PASS
198	198	100	100	100.0	615147	PASS
199	198	5	9	6.8	41613	PASS
275	198	10	60	28.8	176939	PASS
365	198	1	100	4.1	25488	PASS
441	198	0.01	100	11.6	71195	PASS
442	442	50	100	100.0	476565	PASS
443	442	15	24	20.0	95093	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
Data File : BN028340.D
Acq On : 23 Oct 2023 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP386

Quant Time: Oct 24 19:17:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:49:17 2023
Response via : Initial Calibration

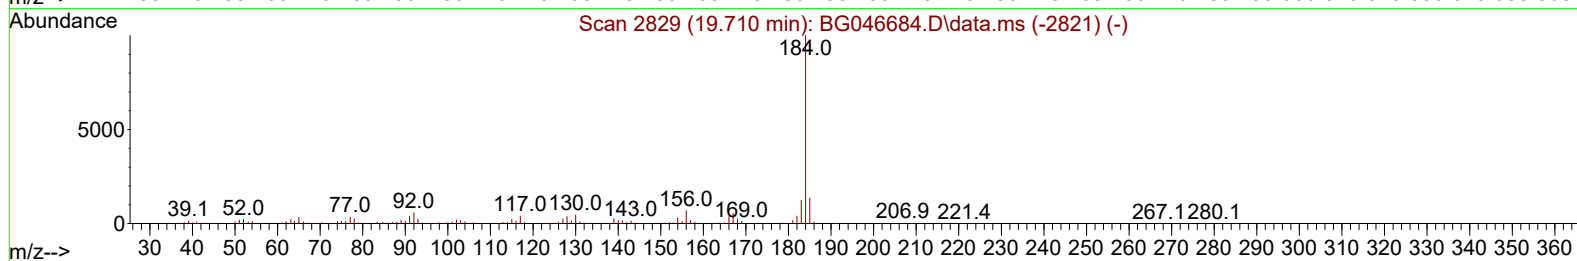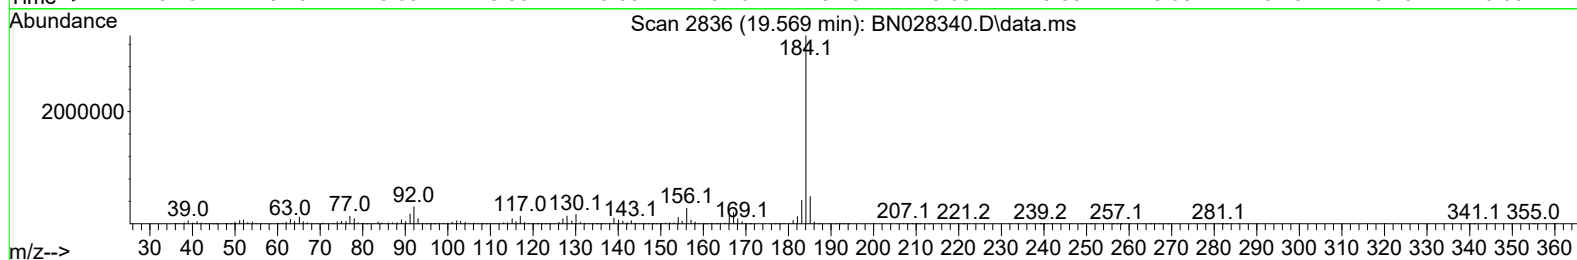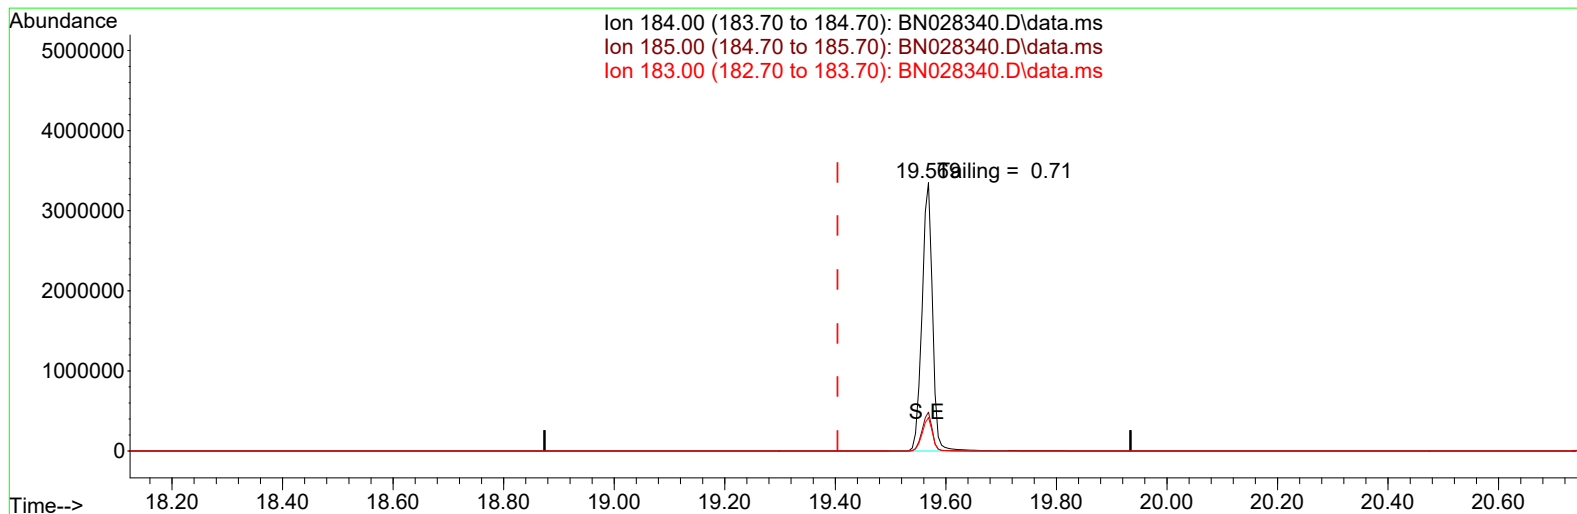

TIC: BN028340.D\data.ms

(77) Benzidine

19.569min (+ 0.165) 0.00 ng




response 4420615

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	12.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
Data File : BN028340.D
Acq On : 23 Oct 2023 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP386

Quant Time: Oct 24 19:17:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:49:17 2023
Response via : Initial Calibration

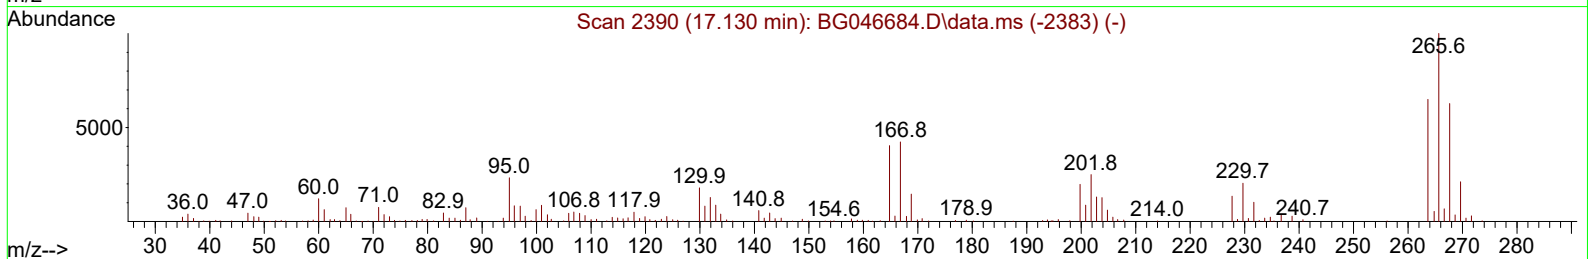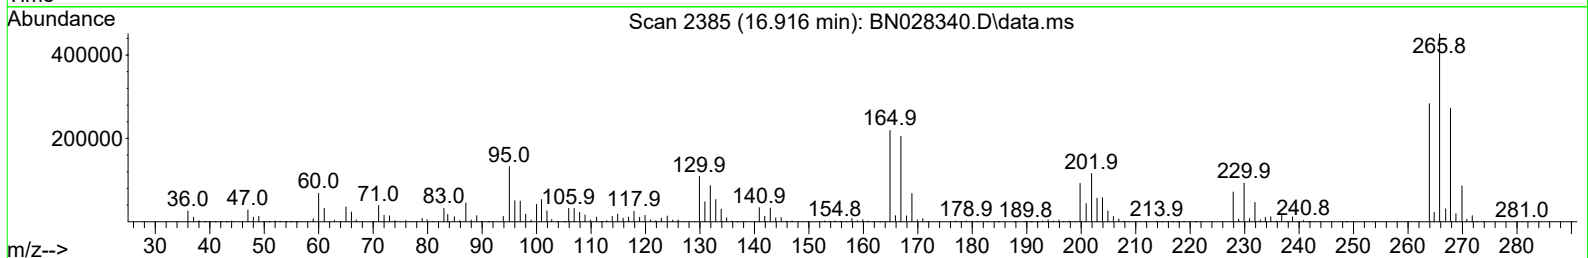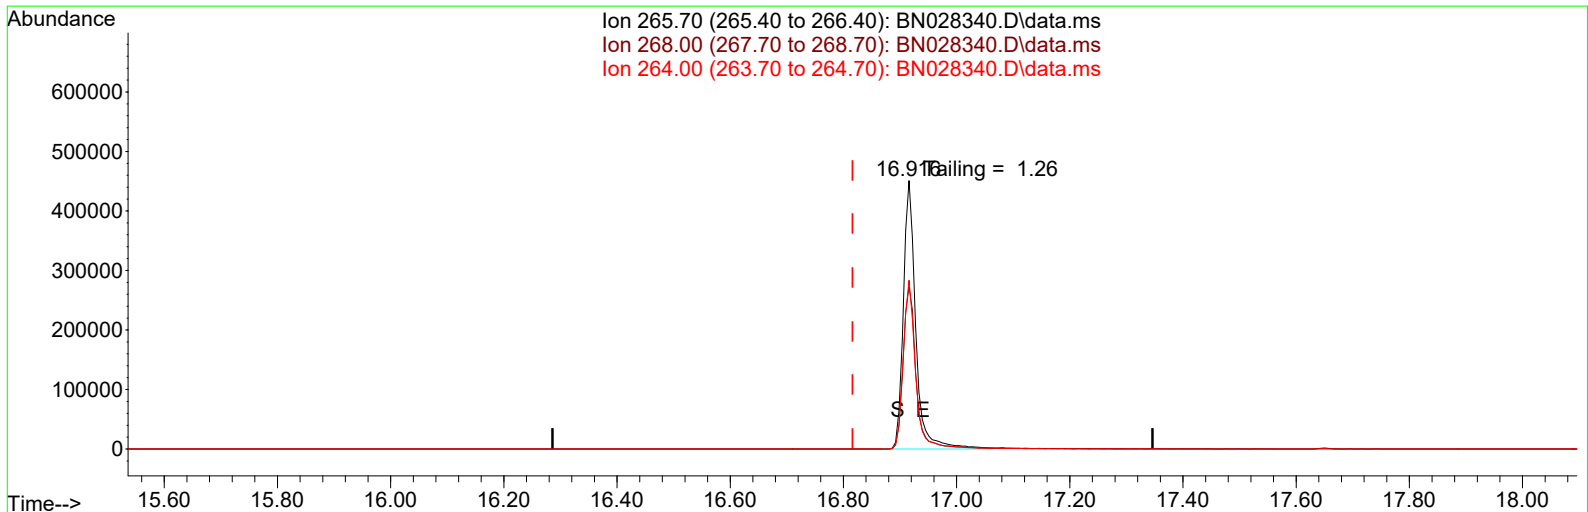

TIC: BN028340.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.100) 20798.85 ng

response 691744

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.45
264.00	61.60	62.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/23/2023	BNA_N	<u>BN028340.D</u>
Compound Name	Response	Retention Time
DDT	2271128	20.751
DDD	24407	20.351
DDE	254	19.045
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24661	2295789	1.07

Instrument :
BNA_N
ClientSampleId :
DFTPP386