


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
Data File : BN028350.D
Acq On : 23 Oct 2023 18:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 23 15:14:08 2023

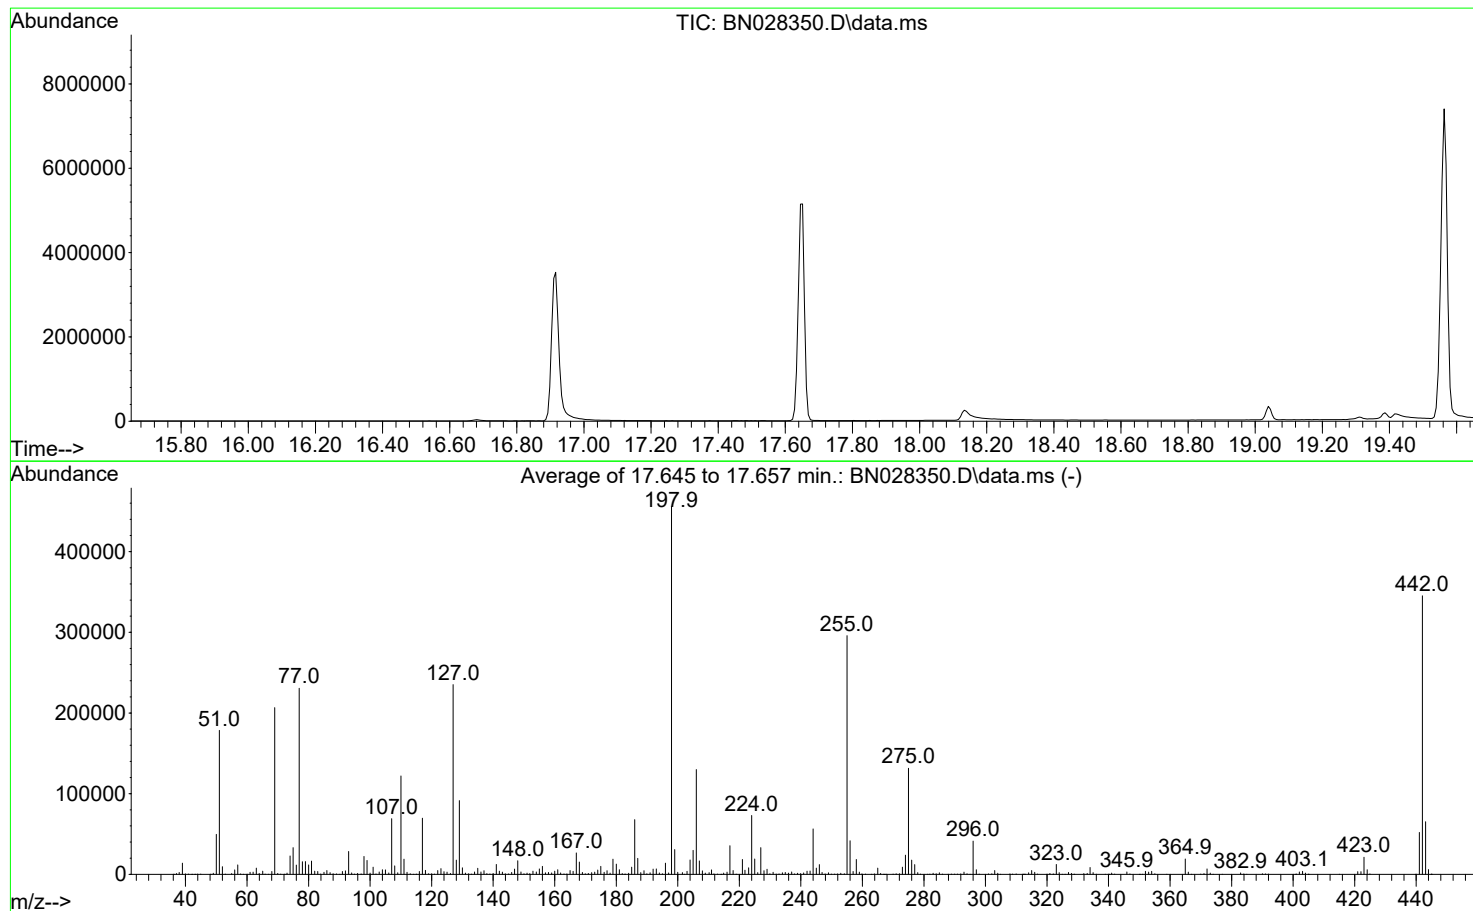




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	178475	PASS
68	69	0.00	2	1.7	3591	PASS
69	198	0.00	100	45.3	206701	PASS
70	69	0.00	2	0.6	1176	PASS
127	198	10	80	51.6	235285	PASS
197	198	0.00	2	0.4	1726	PASS
198	198	100	100	100.0	455936	PASS
199	198	5	9	6.8	30787	PASS
275	198	10	60	28.8	131488	PASS
365	198	1	100	4.2	19067	PASS
441	198	0.01	100	11.4	52005	PASS
442	442	50	100	100.0	345195	PASS
443	442	15	24	18.9	65328	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
Data File : BN028350.D
Acq On : 23 Oct 2023 18:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 24 09:09:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:49:17 2023
Response via : Initial Calibration

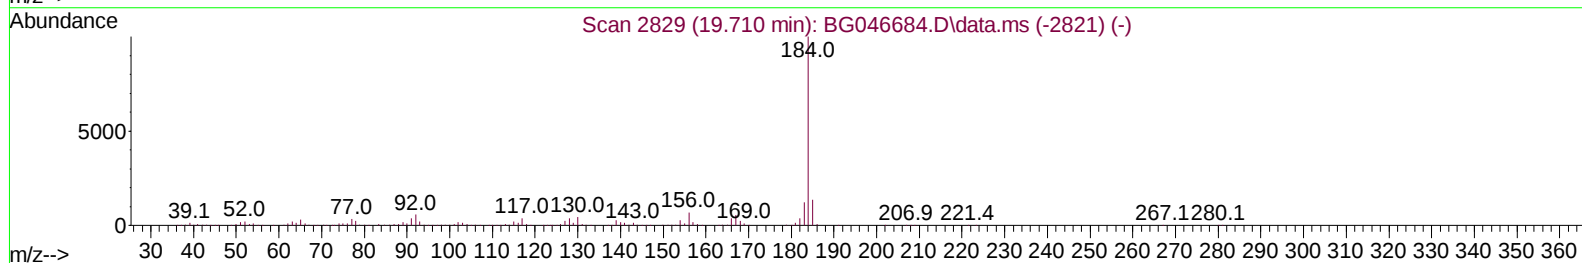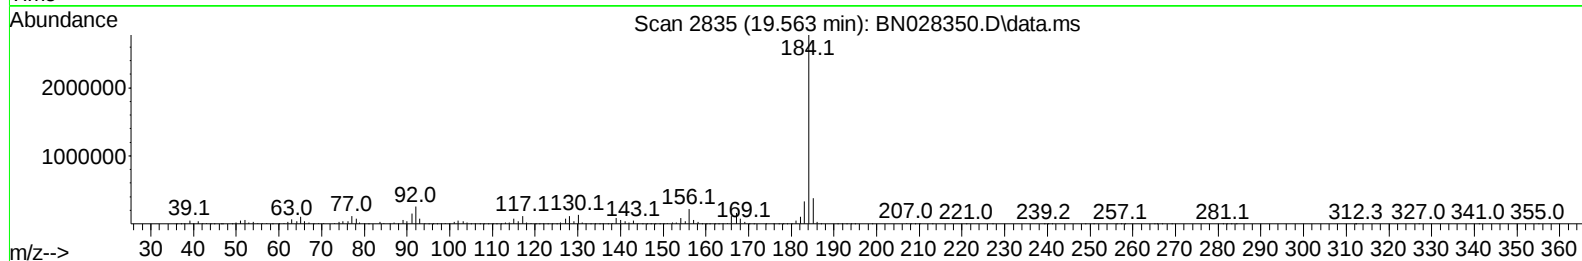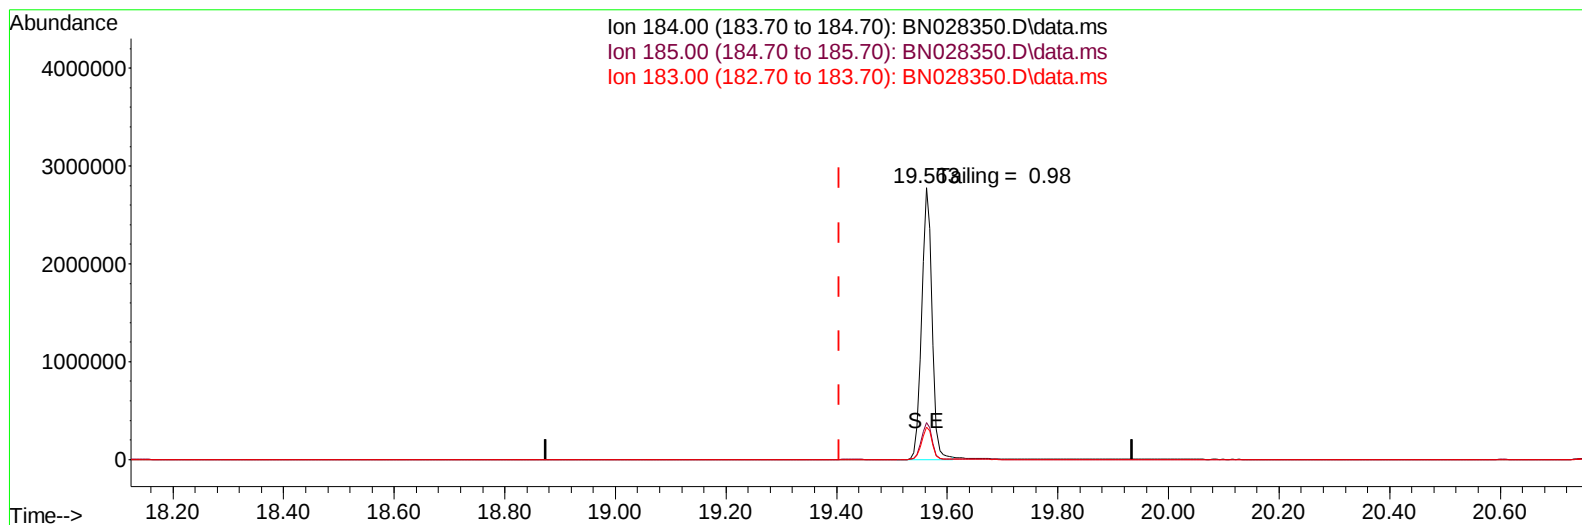

TIC: BN028350.D\data.ms

(77) Benzidine

19.563min (+ 0.159) 0.00 ng




response 3707381

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.69
183.00	13.20	11.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102323\
Data File : BN028350.D
Acq On : 23 Oct 2023 18:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 24 09:09:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:49:17 2023
Response via : Initial Calibration

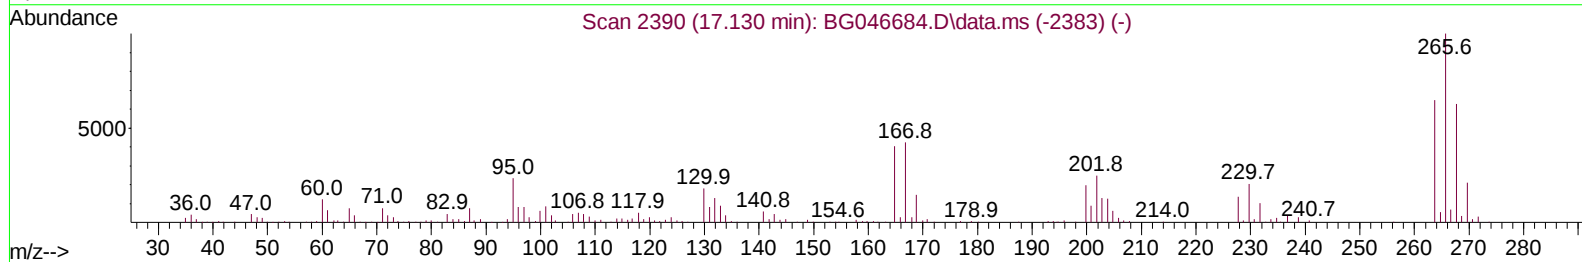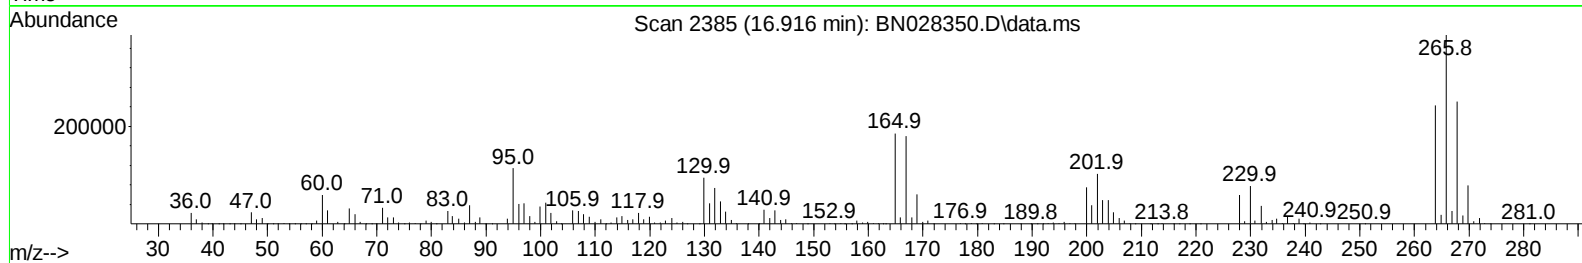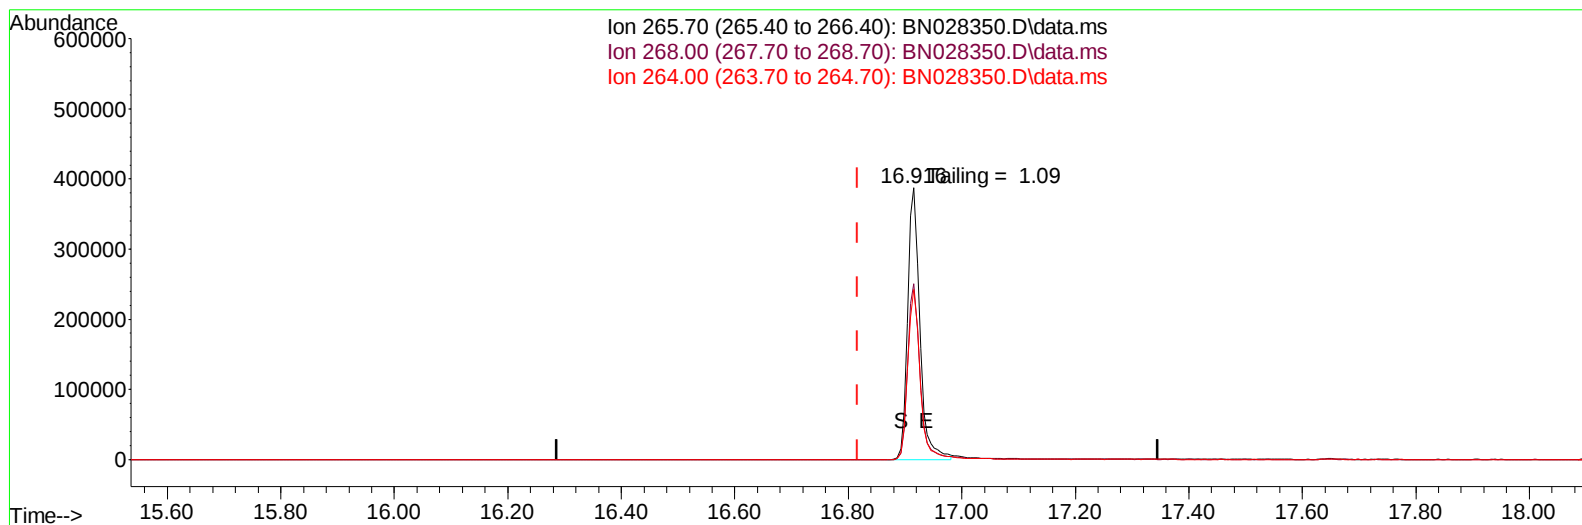

TIC: BN028350.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.100) 21292.65 ng

response 591866

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.76
264.00	61.60	62.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/23/2023	BNA_N	BN028350.D
Compound Name	Response	Retention Time
DDT	1868218	20.745
DDD	19919	20.351
DDE	789	19.039
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20708	1888926	1.10

Instrument :
BNA_N
ClientSampleId :
DFTPP