



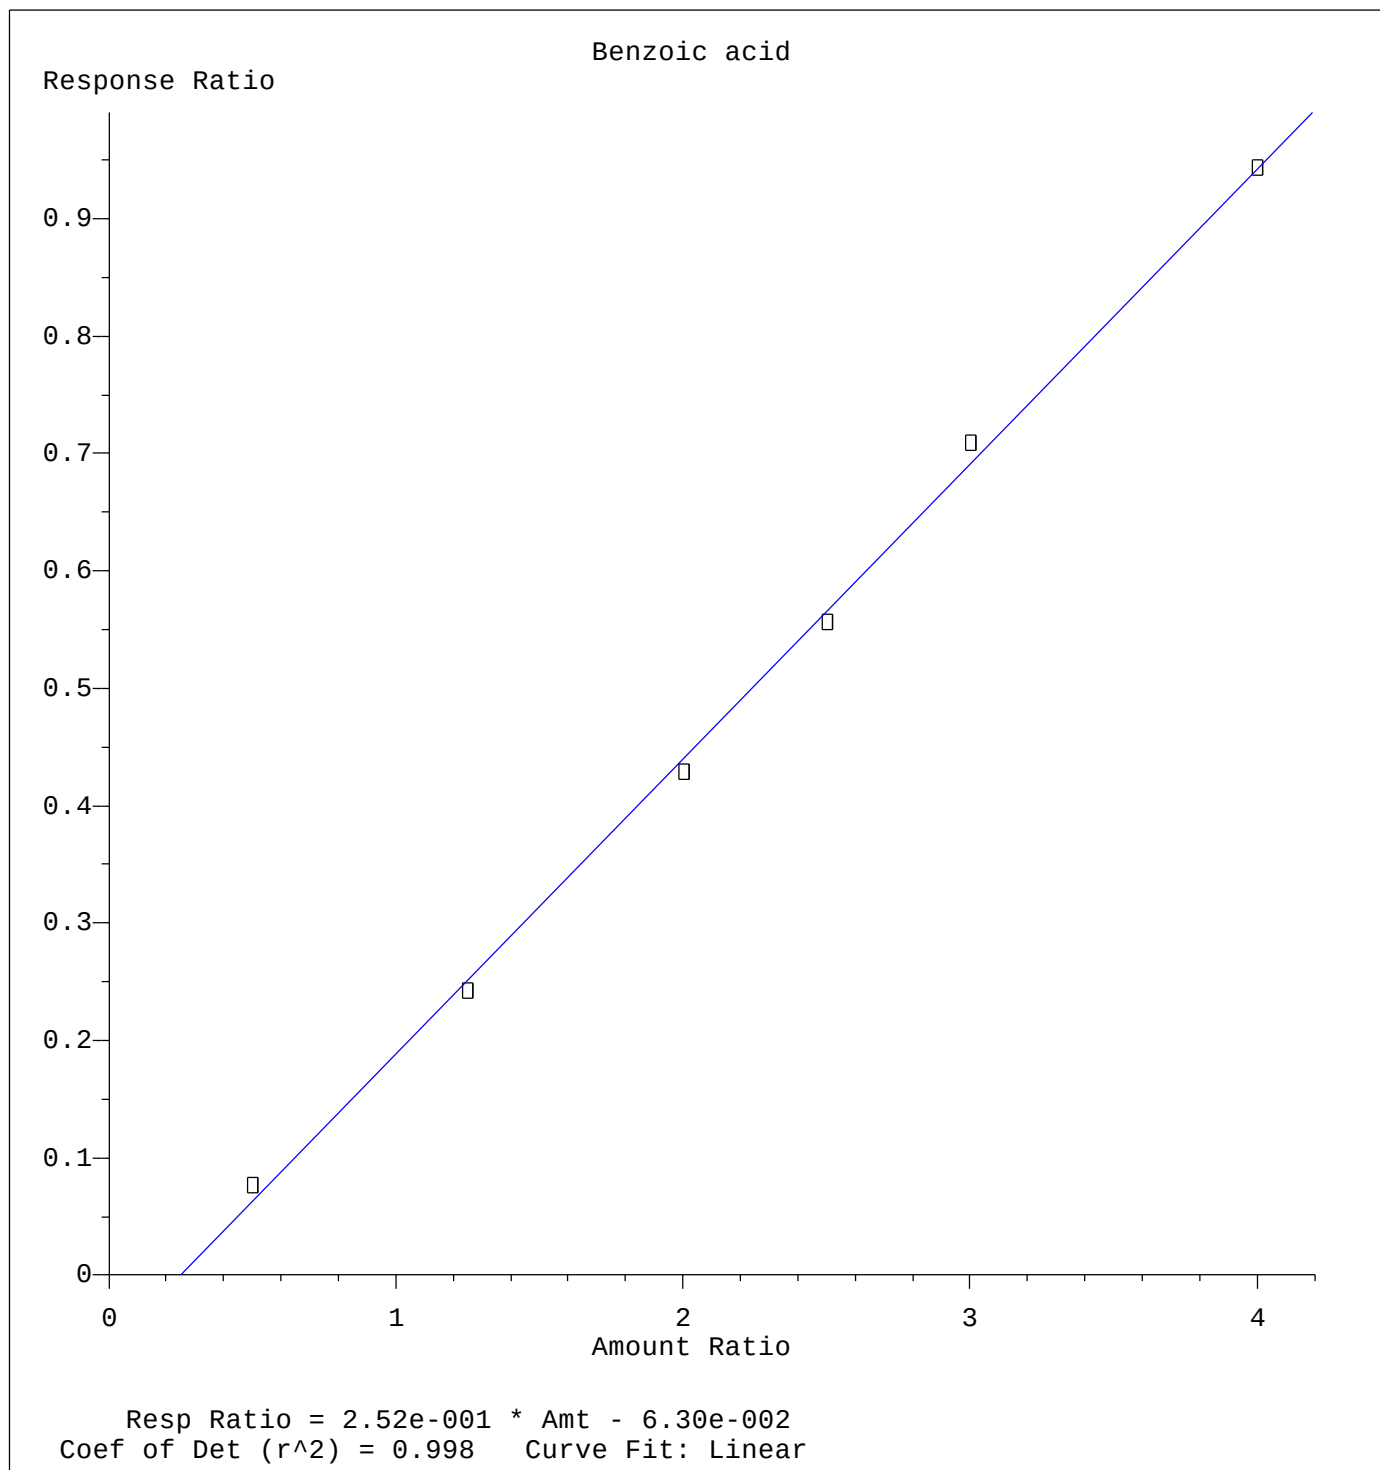

Method Name: Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
Calibration Table Last Updated: Wed Oct 24 14:21:25 2018

Hexachlorocyclopentadiene

Response Ratio

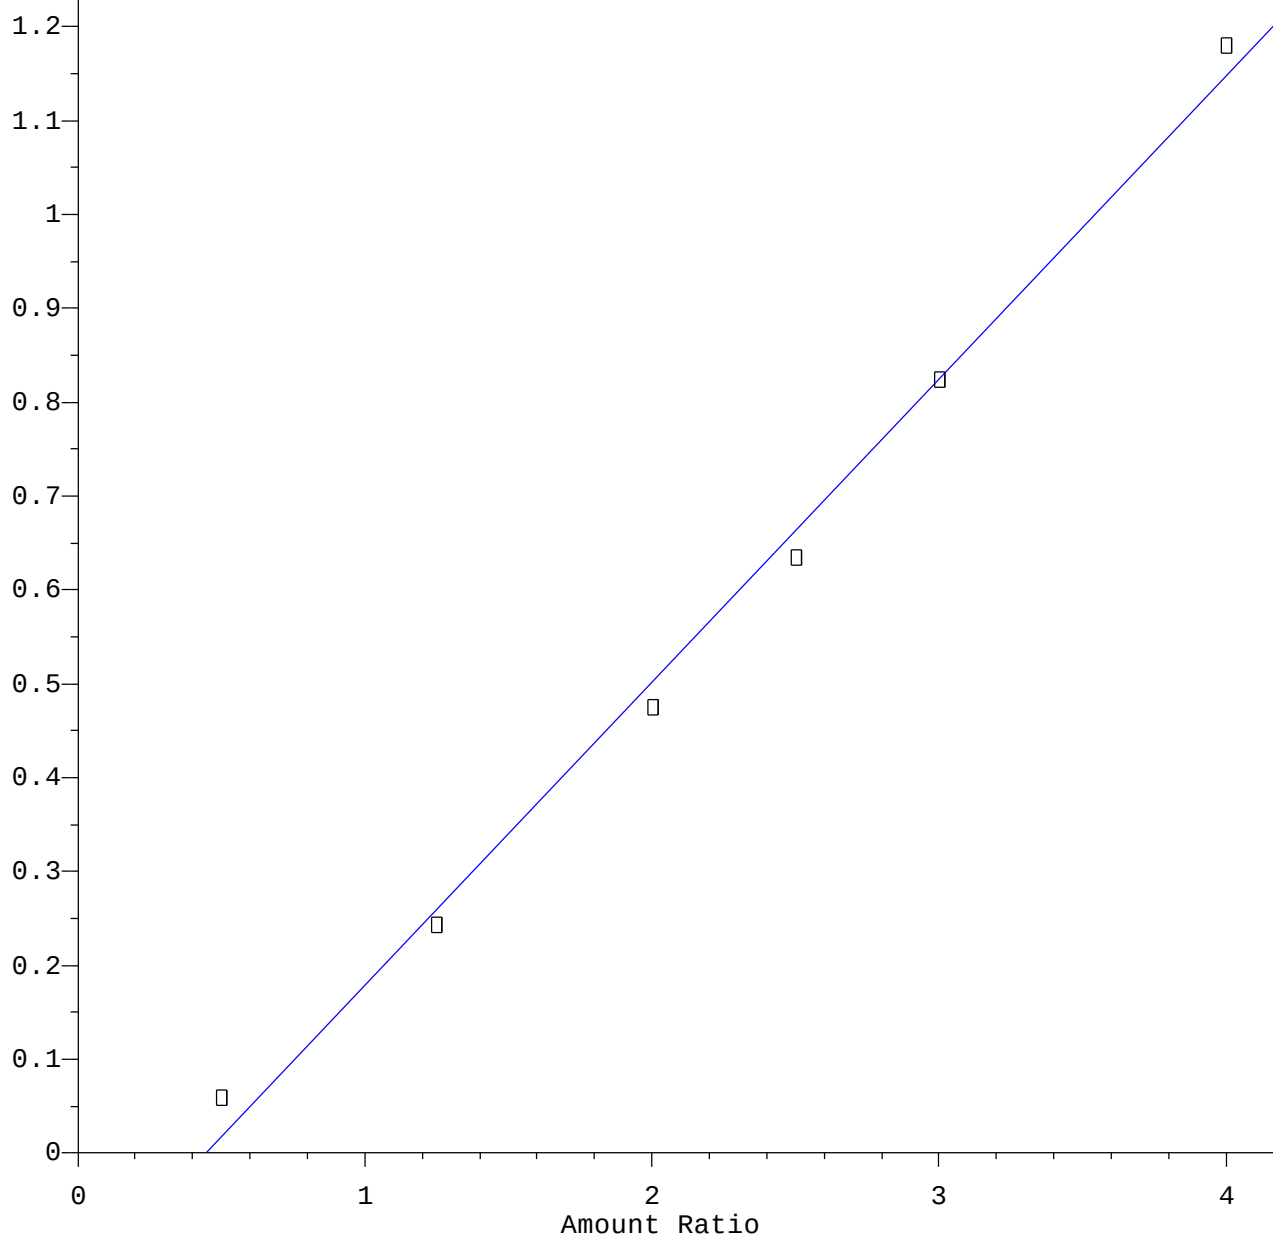


Resp Ratio = $3.23 \times 10^{-1} \times \text{Amt} - 1.44 \times 10^{-1}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
Calibration Table Last Updated: Wed Oct 24 14:21:25 2018


2,4-Dinitrophenol

Response Ratio

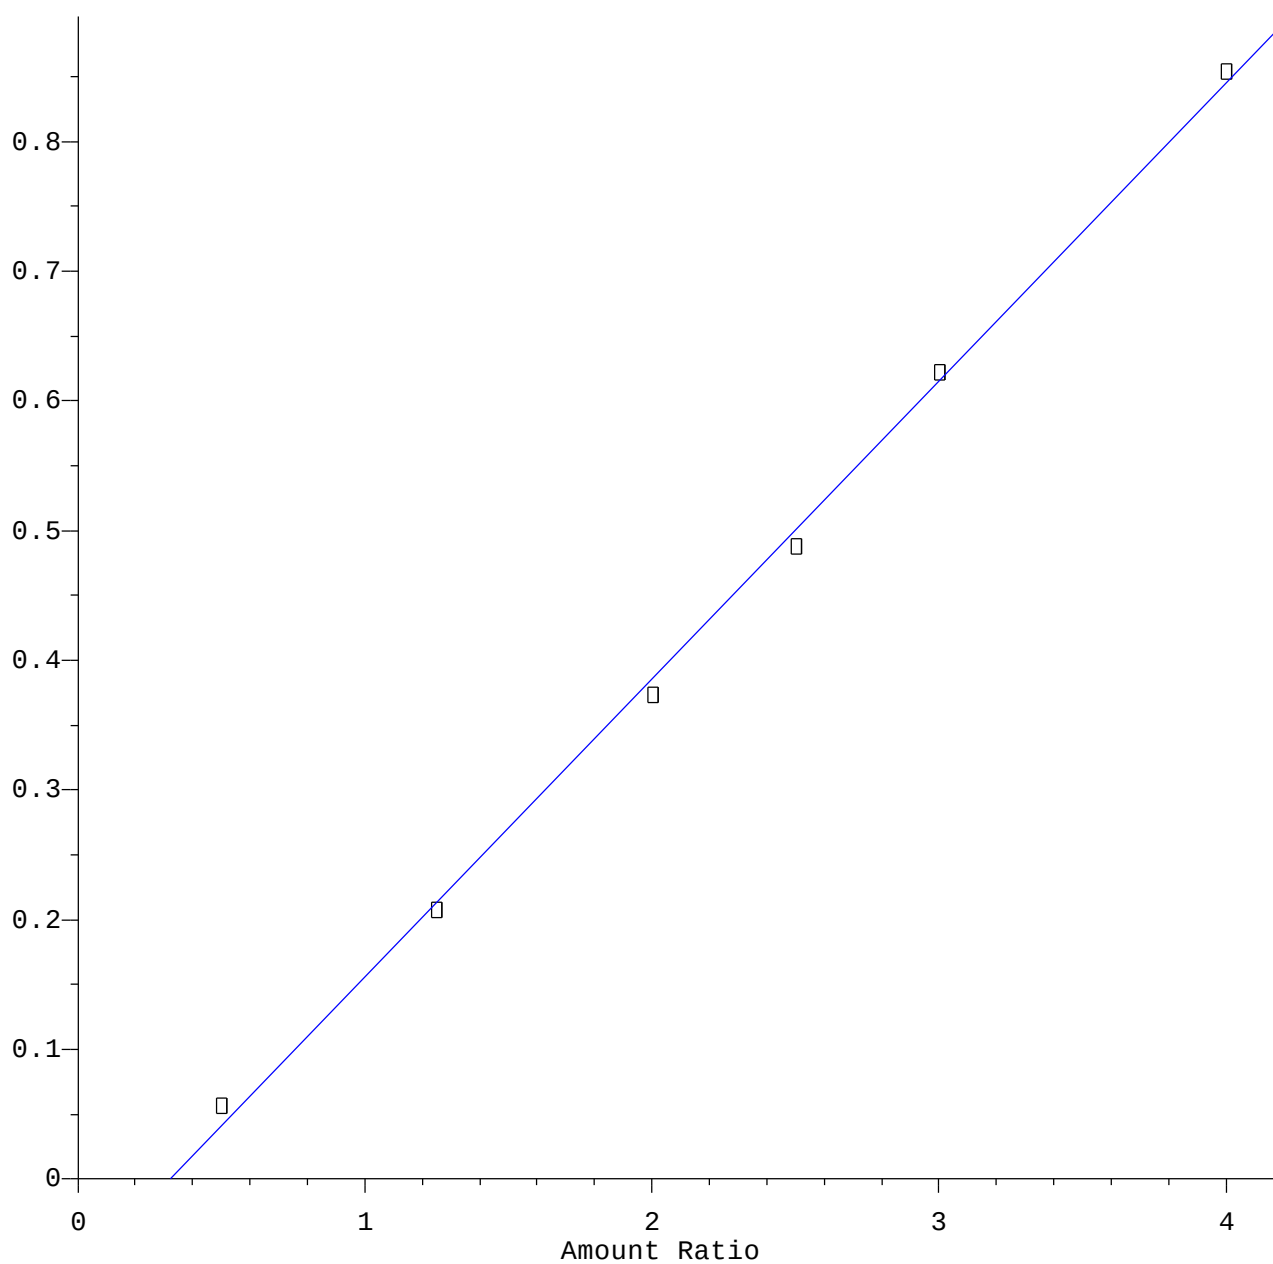


Resp Ratio = 2.30e-001 * Amt - 7.42e-002
Coef of Det (r²) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
Calibration Table Last Updated: Wed Oct 24 14:21:25 2018

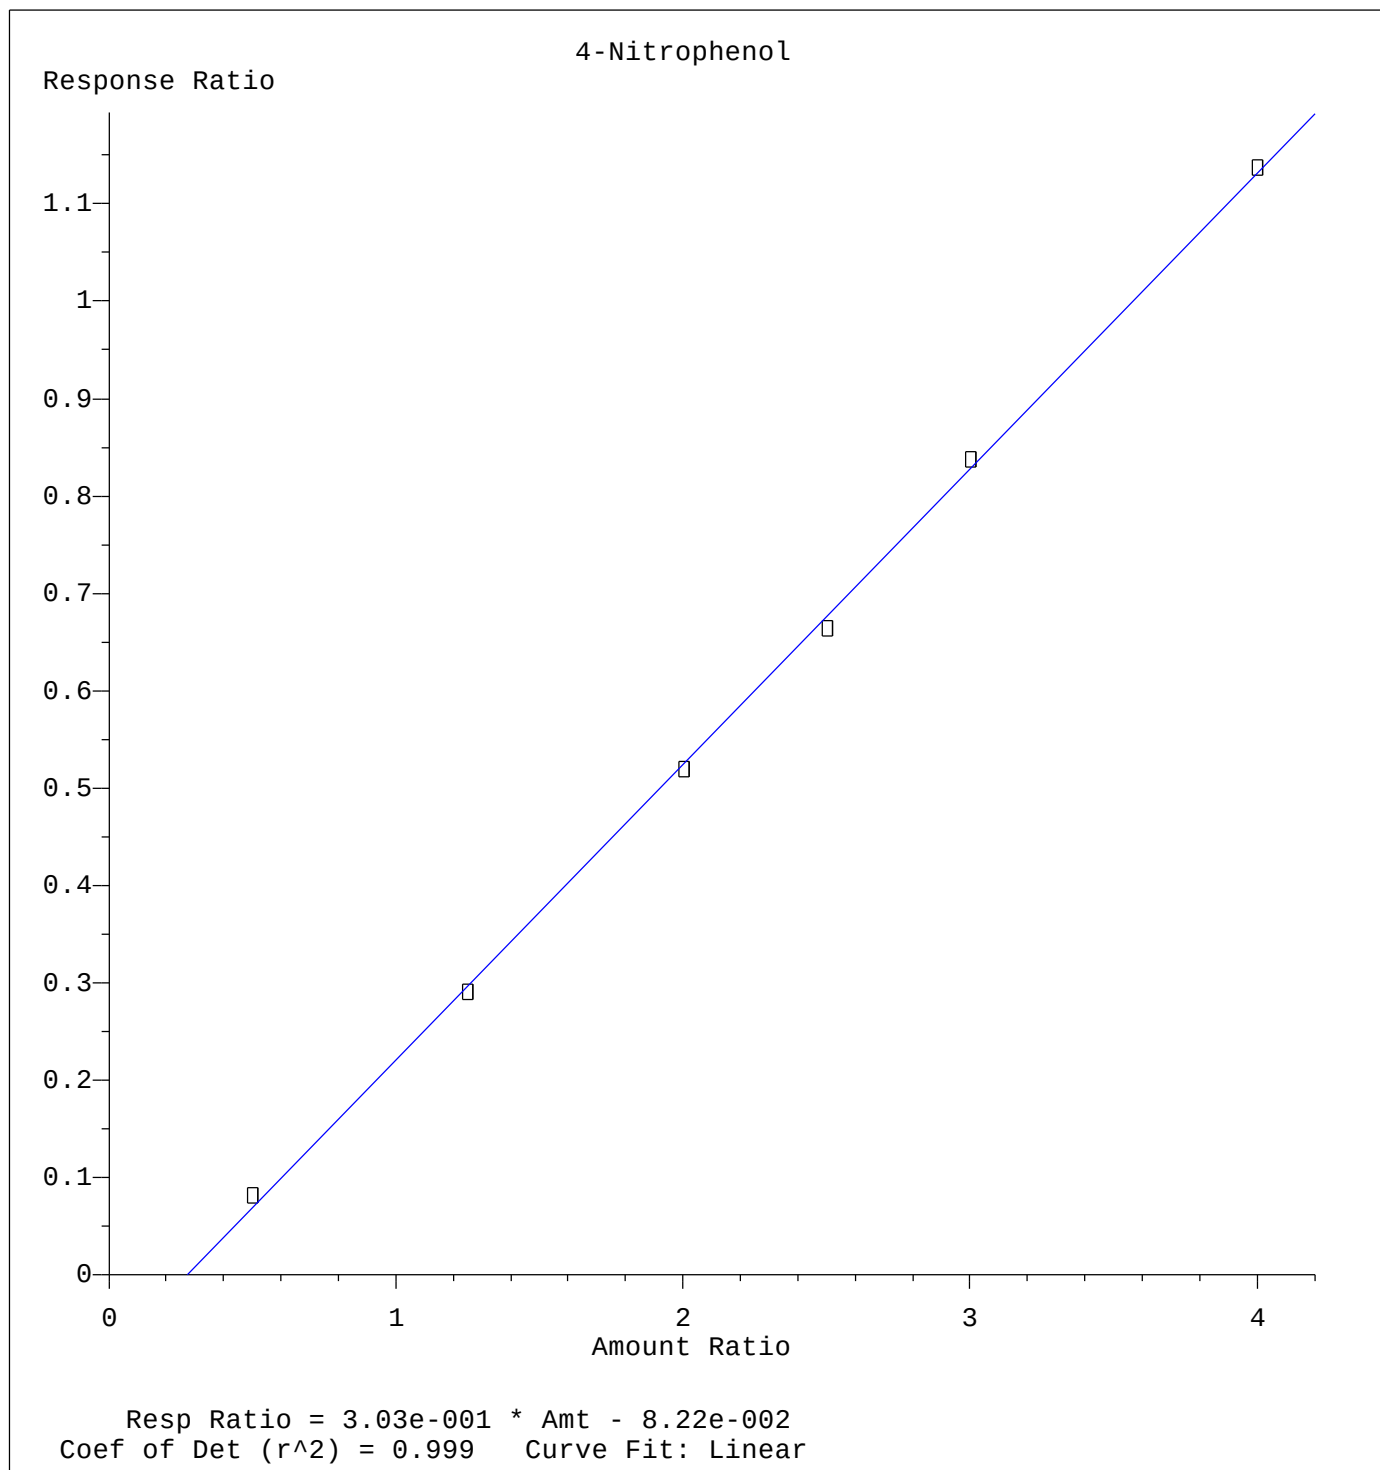

Method Name: Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
Calibration Table Last Updated: Wed Oct 24 14:21:25 2018

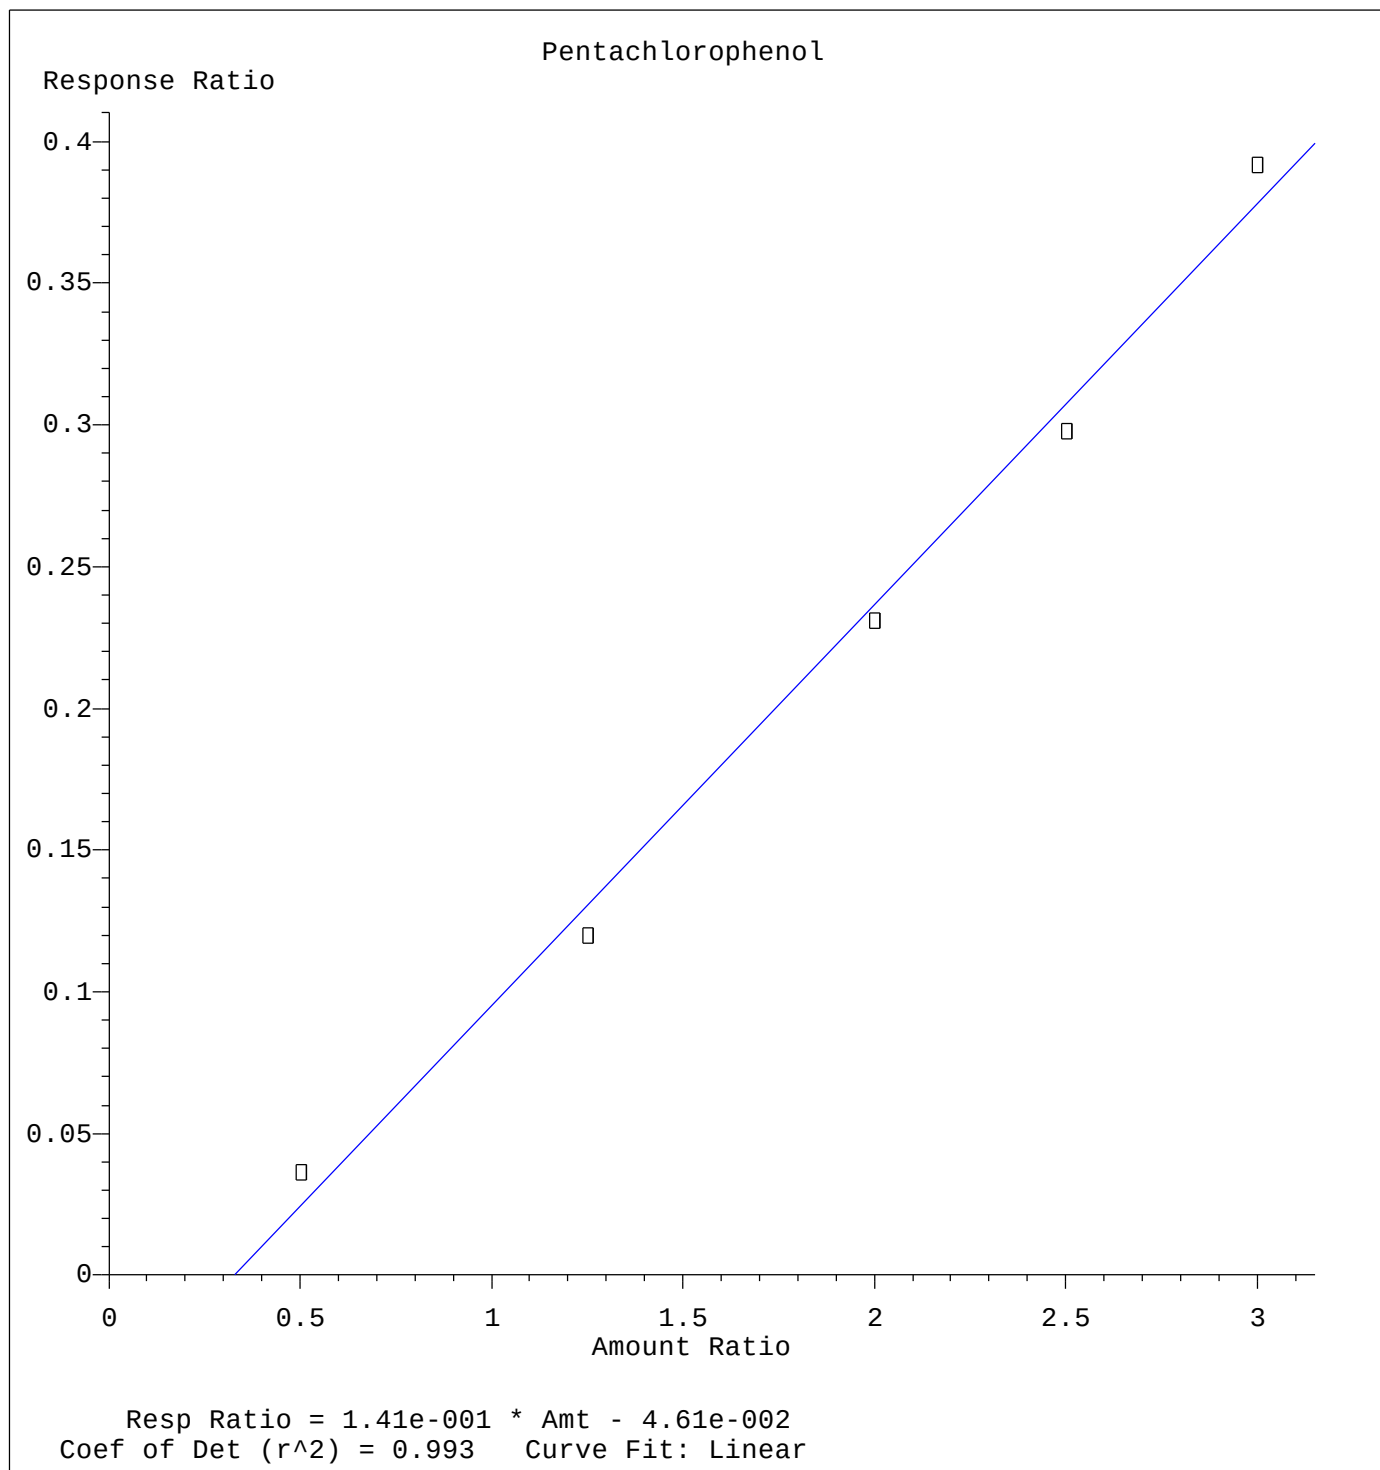

Method Name: Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
Calibration Table Last Updated: Wed Oct 24 14:21:25 2018