


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN102418\  
 Data File : BN003263.D  
 Acq On : 24 Oct 2018 09:31  
 Operator : MJ/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-BN102418.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Oct 24 14:21:25 2018

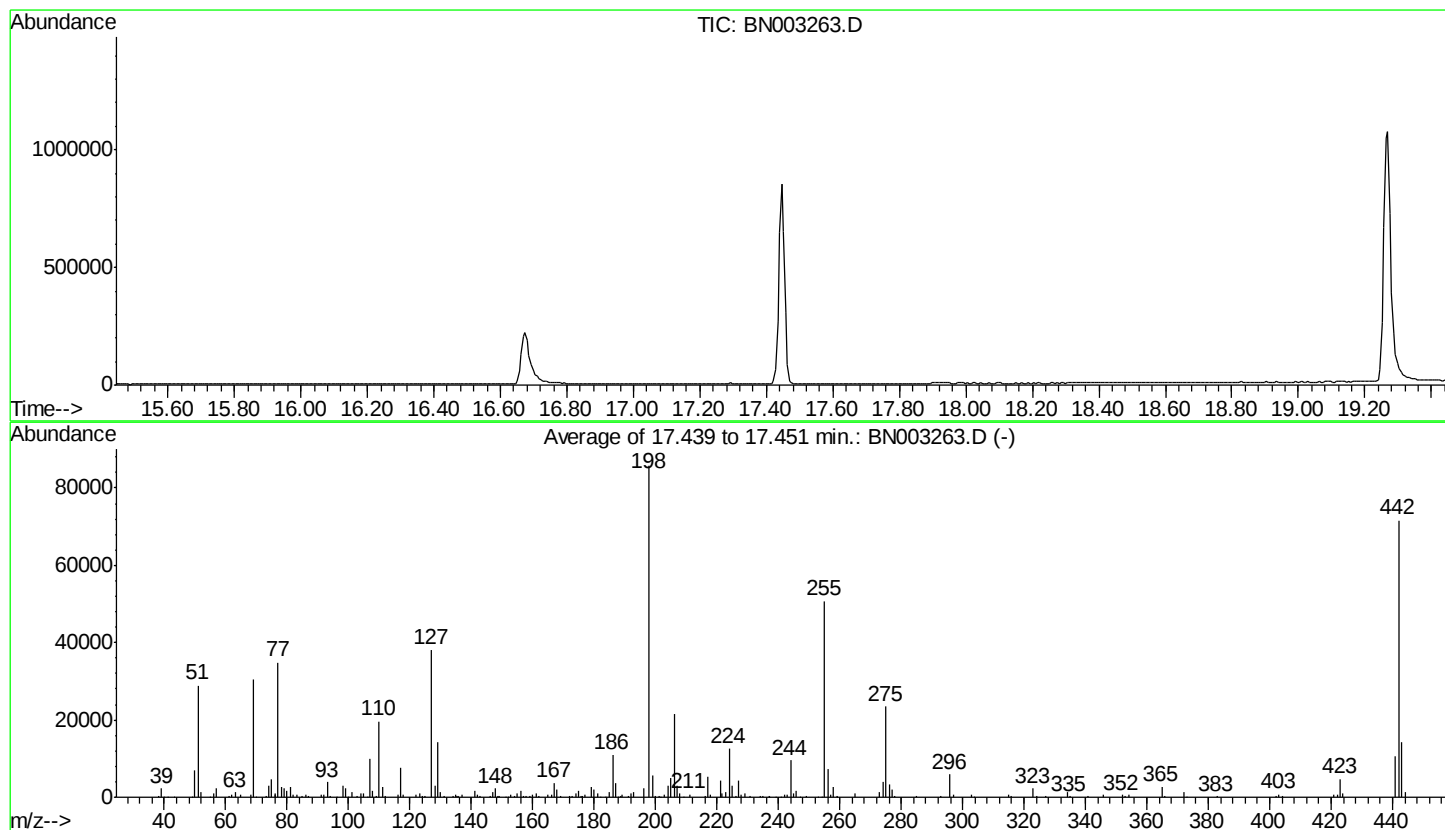

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 33.6      | 28824   | PASS             |
| 68          | 69           | 0.00         | 2            | 2.0       | 613     | PASS             |
| 69          | 198          | 0.00         | 100          | 35.5      | 30488   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 119     | PASS             |
| 127         | 198          | 10           | 80           | 44.6      | 38240   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 85778   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 5731    | PASS             |
| 275         | 198          | 10           | 60           | 27.3      | 23386   | PASS             |
| 365         | 198          | 1            | 100          | 3.1       | 2692    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.5      | 10727   | PASS             |
| 442         | 198          | 50           | 100          | 83.5      | 71602   | PASS             |
| 443         | 442          | 15           | 24           | 19.8      | 14154   | PASS             |