


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN102418\
 Data File : BN003272.D
 Acq On : 24 Oct 2018 15:19
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 24 14:21:25 2018

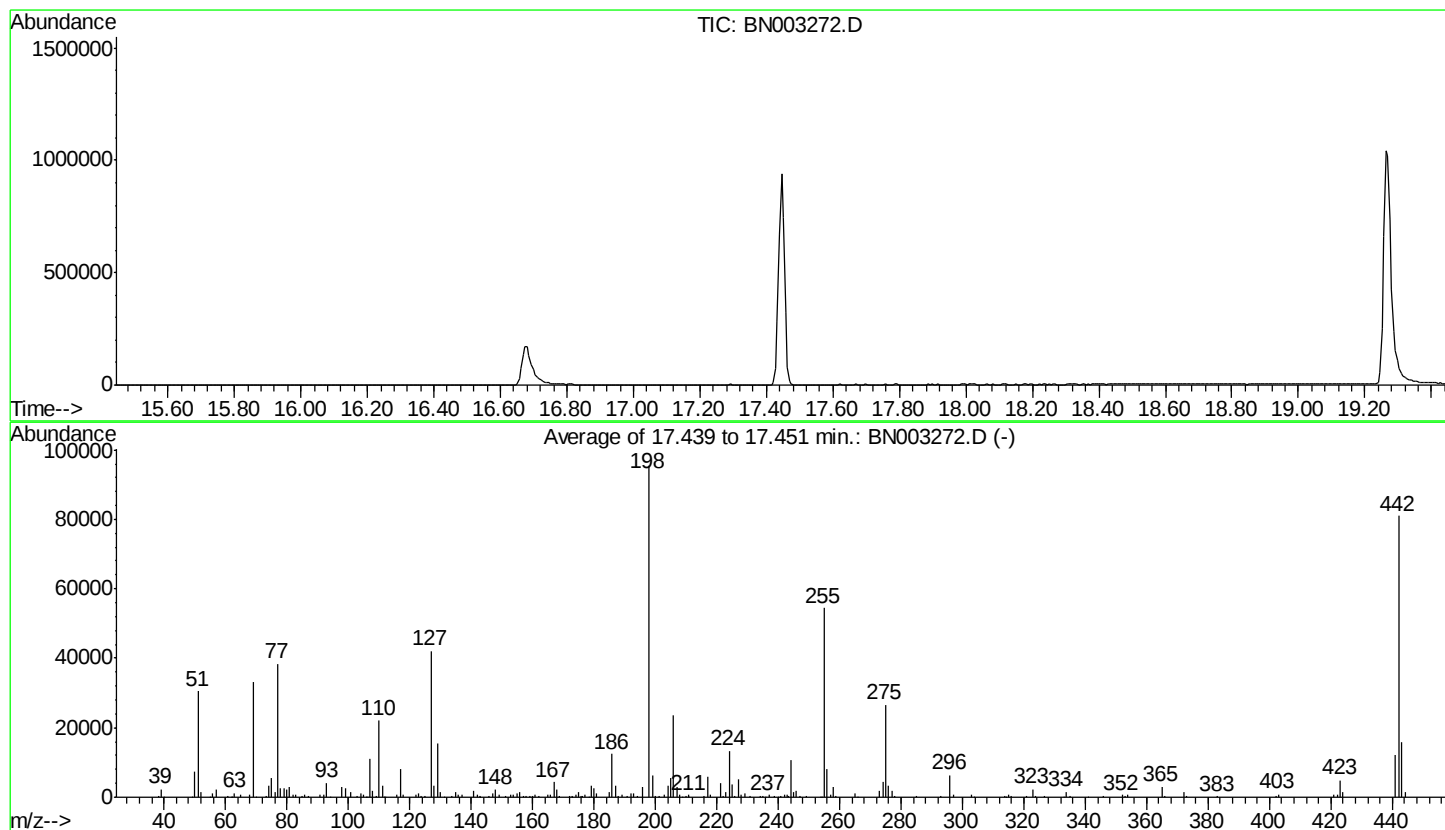

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	30480	PASS
68	69	0.00	2	1.9	643	PASS
69	198	0.00	100	34.6	33066	PASS
70	69	0.00	2	0.3	101	PASS
127	198	10	80	44.1	42069	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95458	PASS
199	198	5	9	6.7	6376	PASS
275	198	10	60	27.8	26557	PASS
365	198	1	100	3.3	3103	PASS
441	198	0.01	100	12.7	12151	PASS
442	198	50	100	84.9	81024	PASS
443	442	15	24	19.5	15776	PASS