


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN102418\
 Data File : BN003289.D
 Acq On : 25 Oct 2018 01:41
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 24 14:21:25 2018

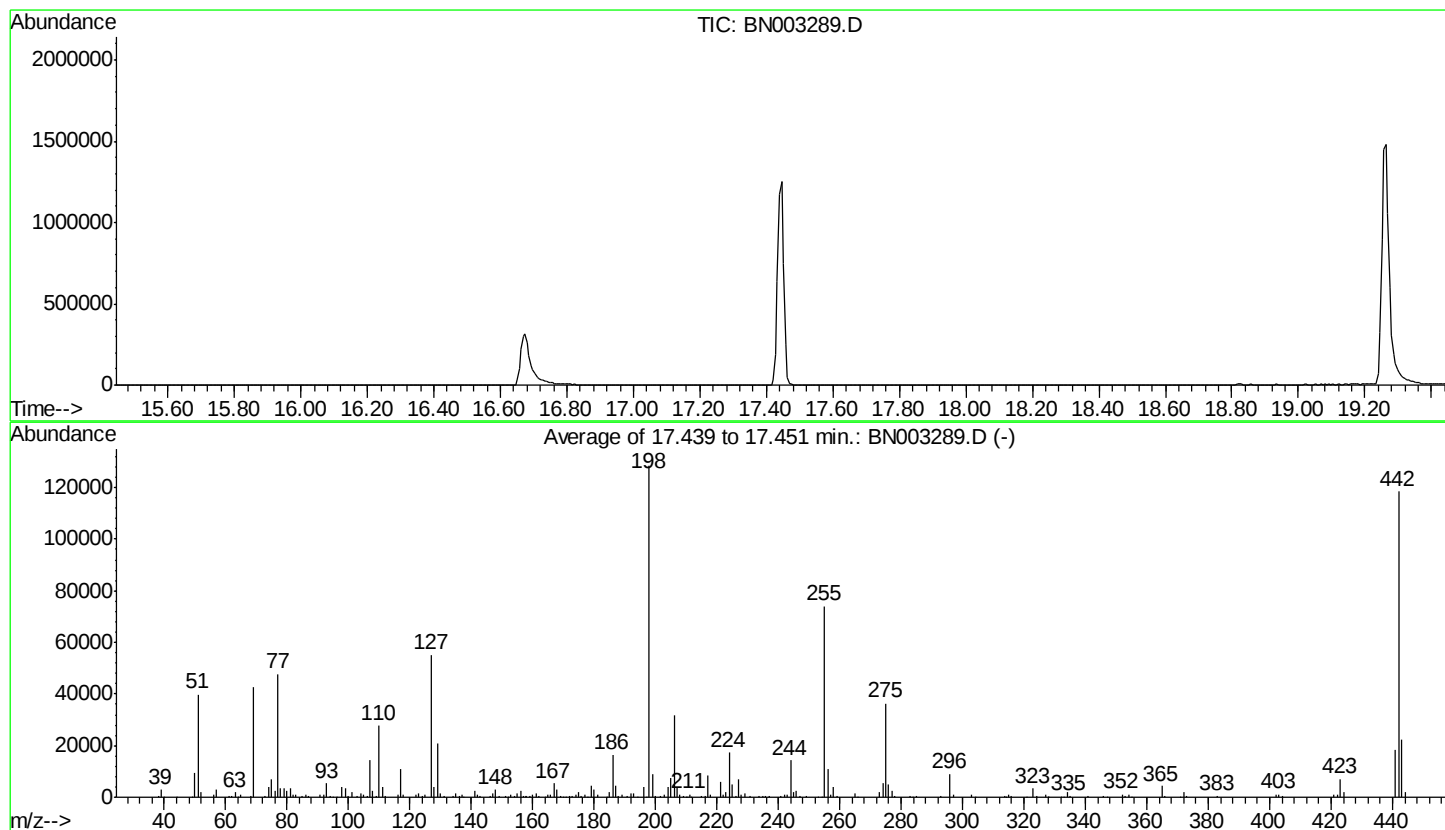

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	39917	PASS
68	69	0.00	2	1.7	730	PASS
69	198	0.00	100	33.3	42808	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.9	55069	PASS
197	198	0.00	2	0.1	187	PASS
198	198	100	100	100.0	128498	PASS
199	198	5	9	7.0	8944	PASS
275	198	10	60	28.2	36253	PASS
365	198	1	100	3.4	4405	PASS
441	198	0.01	100	14.1	18128	PASS
442	198	50	100	92.1	118338	PASS
443	442	15	24	18.9	22413	PASS