
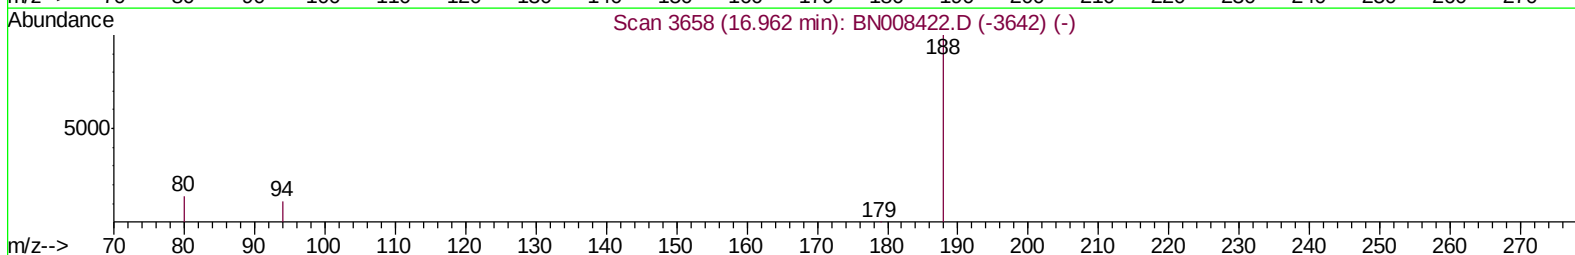
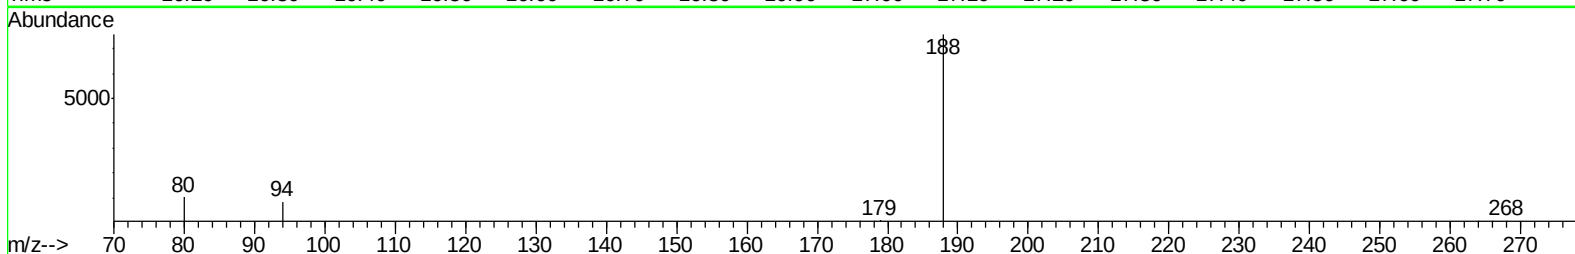


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\
Data File : BN008431.D
Acq On : 25 Oct 2019 17:39
Operator : JU
Sample : PB123997BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 25 18:10:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 13:14:06 2019
Response via : Initial Calibration

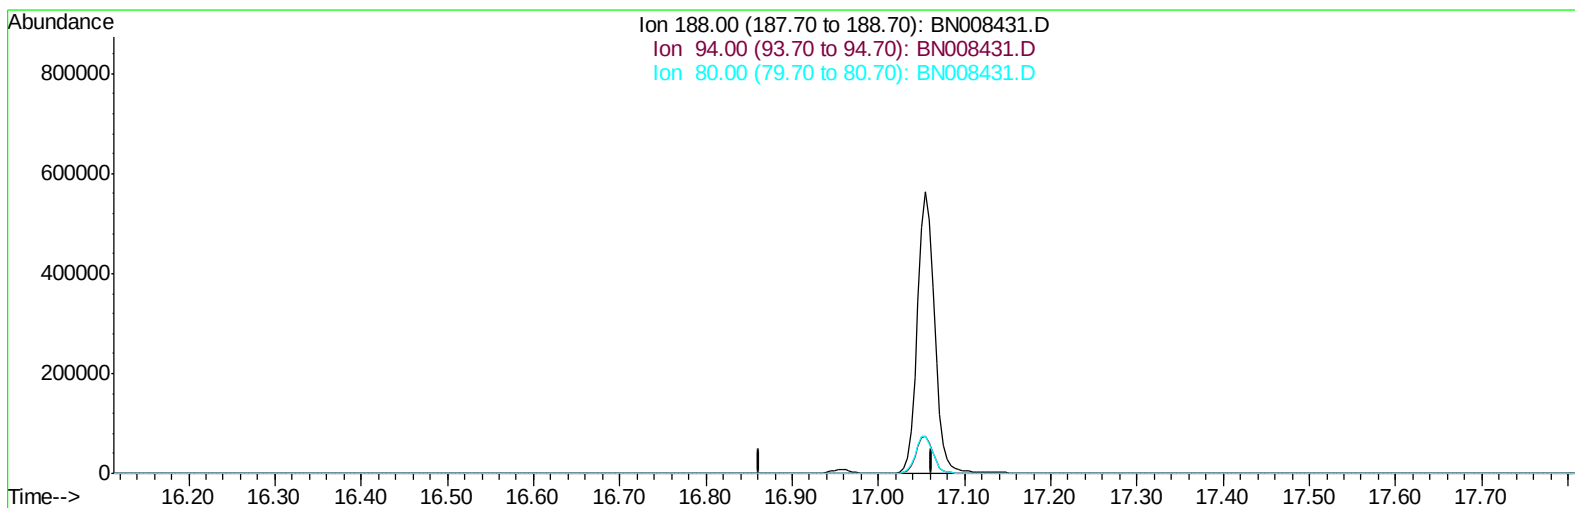

TIC: BN008431.D

(10) Phenanthrene-d10 (I)




16.962min (-16.962) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.90	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\
Data File : BN008431.D
Acq On : 25 Oct 2019 17:39
Operator : JU
Sample : PB123997BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 25 18:10:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 13:14:06 2019
Response via : Initial Calibration

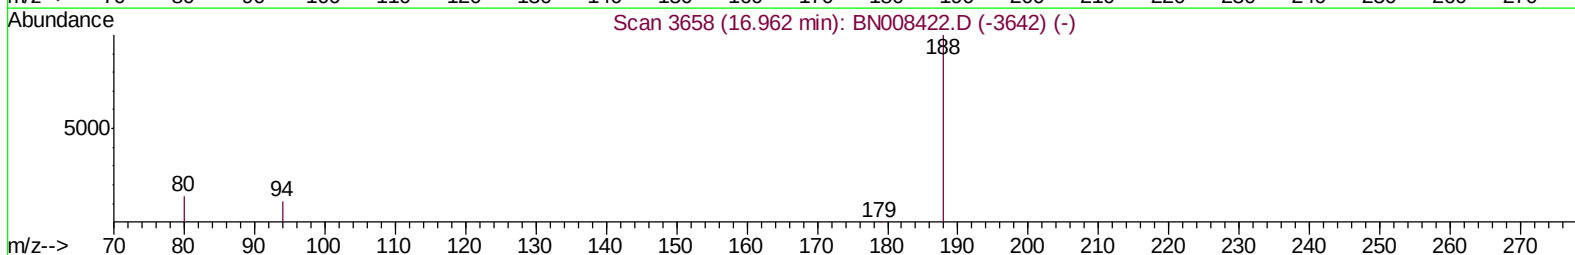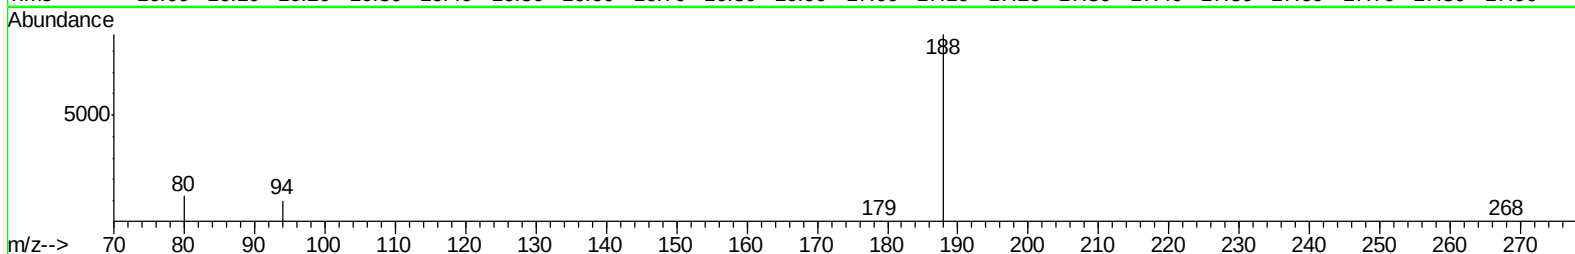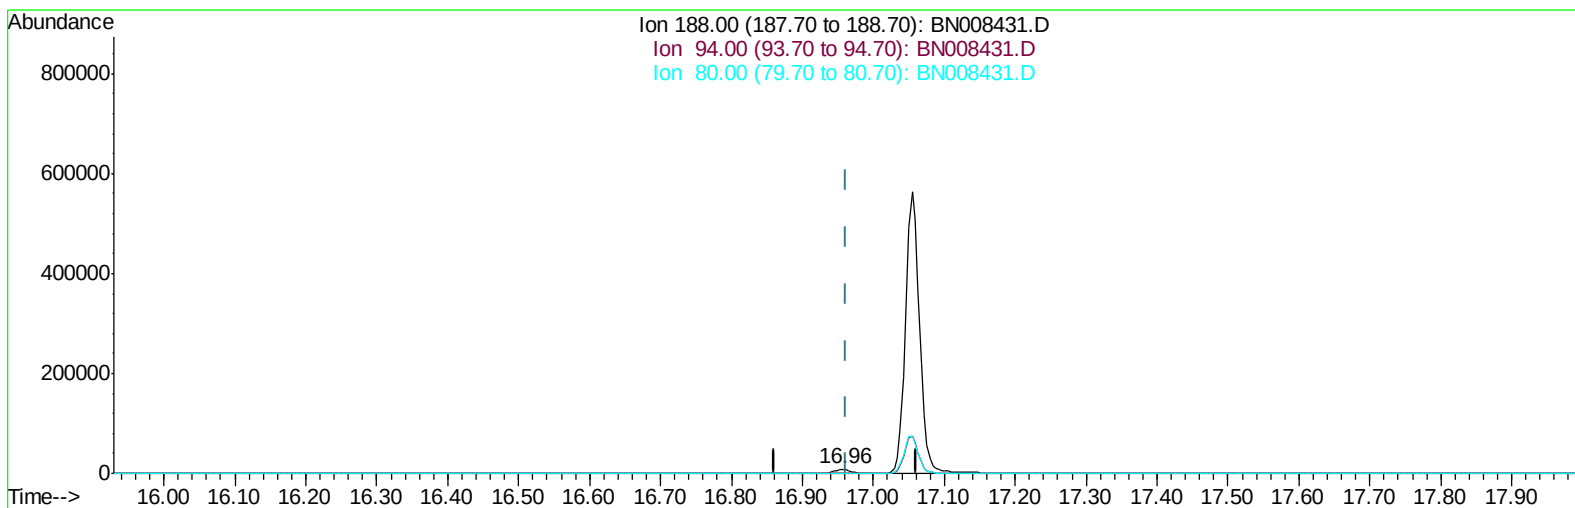

TIC: BN008431.D

(10) Phenanthrene-d10 (I)




16.957min (-0.005) 0.40ng/ul m

response 13033

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	11.71
80.00	12.60	14.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\
Data File : BN008431.D
Acq On : 25 Oct 2019 17:39
Operator : JU
Sample : PB123997BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 25 18:12:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 13:14:06 2019
Response via : Initial Calibration

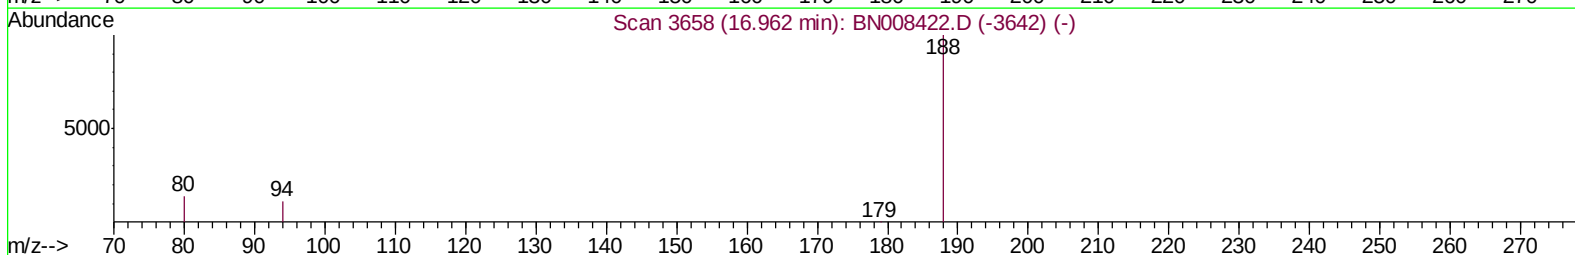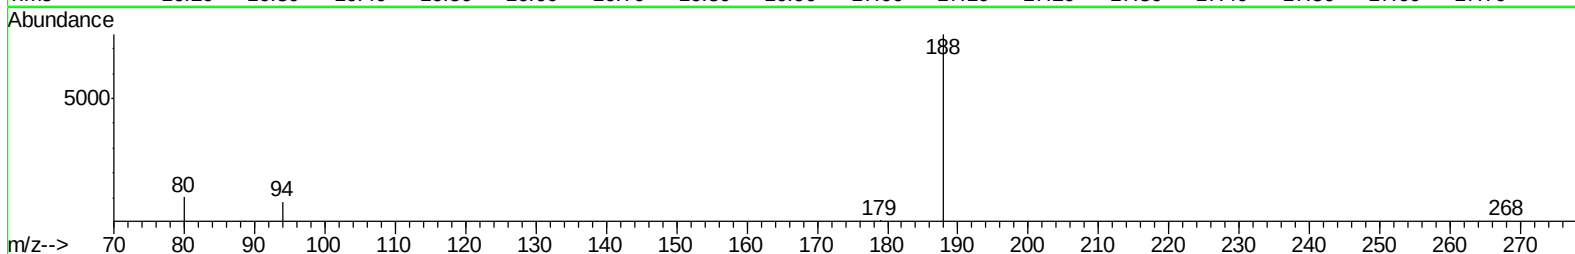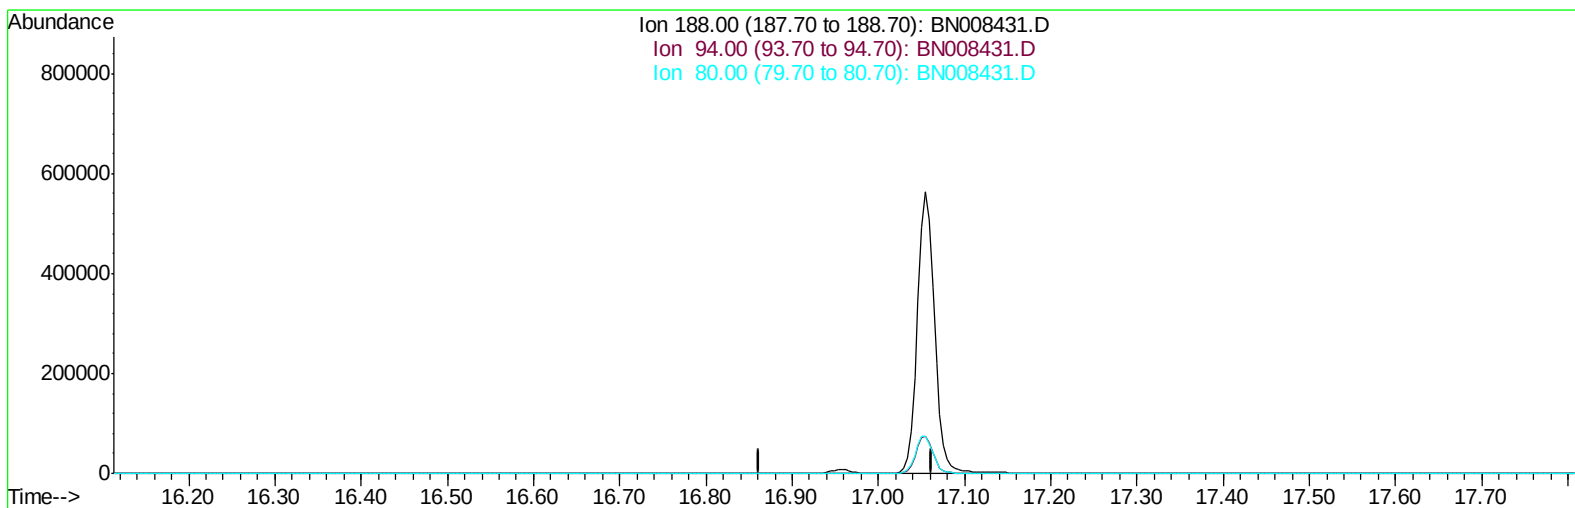

TIC: BN008431.D

(10) Phenanthrene-d10 (I)




16.962min (-16.962) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.90	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\
Data File : BN008431.D
Acq On : 25 Oct 2019 17:39
Operator : JU
Sample : PB123997BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 25 18:12:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 13:14:06 2019
Response via : Initial Calibration

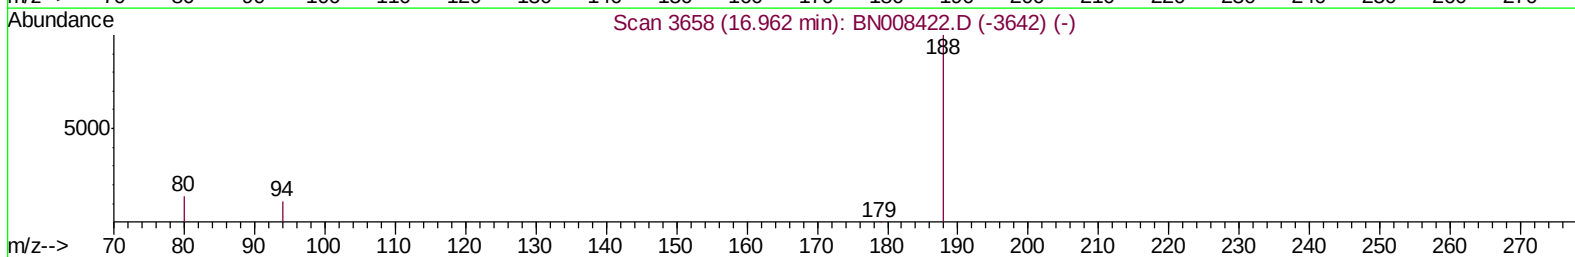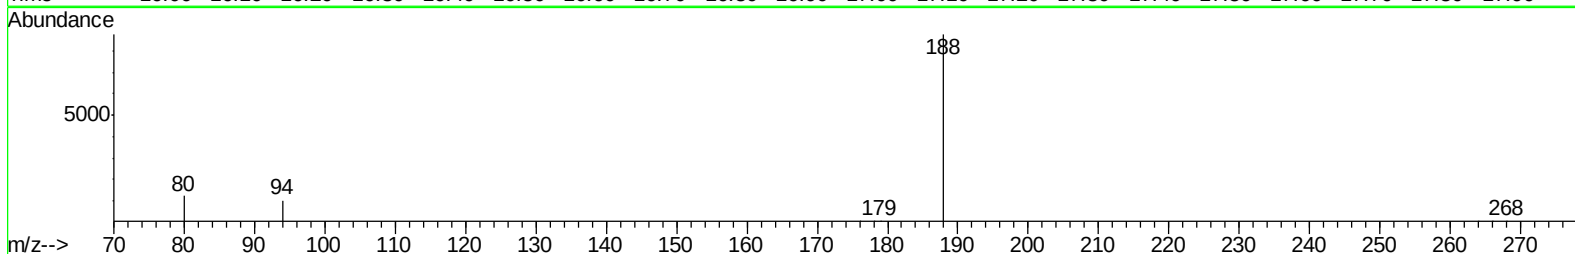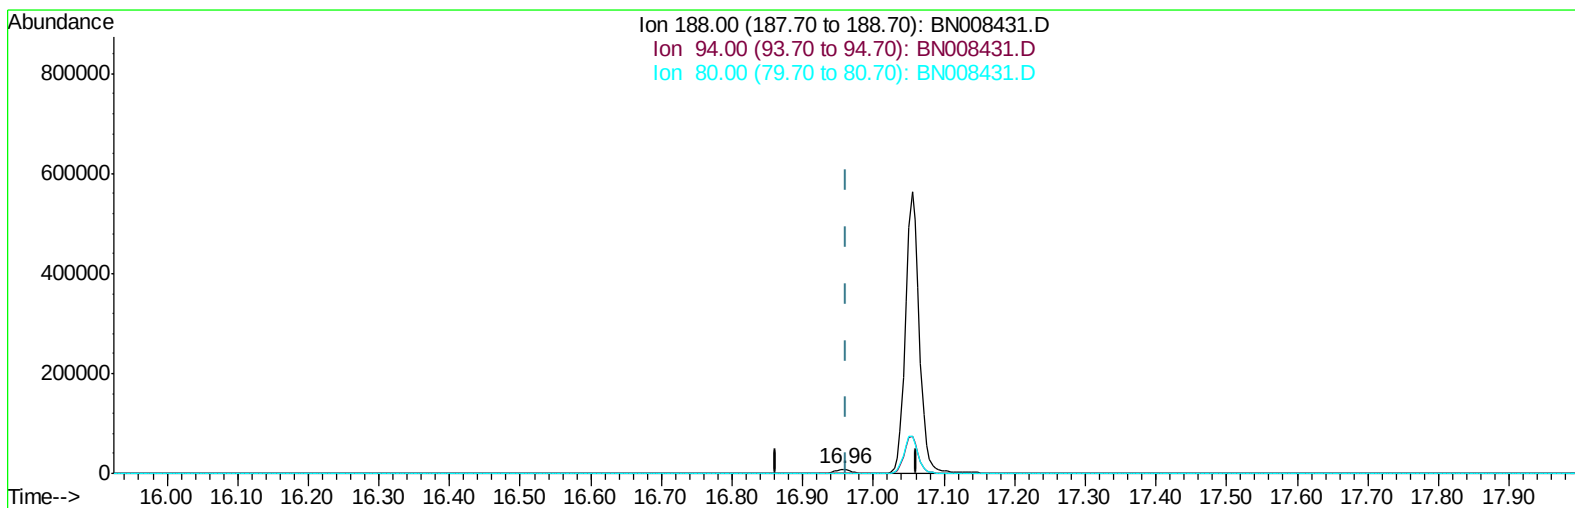

TIC: BN008431.D

(10) Phenanthrene-d10 (I)

16.957min (-0.005) 0.40ng/ul m

response 13111

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	11.71
80.00	12.60	14.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\
Data File : BN008431.D
Acq On : 25 Oct 2019 17:39
Operator : JU
Sample : PB123997BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 25 18:12:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 13:14:06 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	1774	0.40	ng/ul	0.00
2) Naphthalene-d8	10.33	136	9126	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.21	164	5910	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.96	188	13111m	0.40	ng/ul	0.00
16) Chrysene-d12	21.17	240	9991	0.40	ng/ul	0.00
20) Perylene-d12	23.33	264	9252	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.94	152	3281	0.21	ng/ul	0.00
14) Fluoranthene-d10	18.99	212	9617	0.21	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\
Data File : BN008431.D
Acq On : 25 Oct 2019 17:39
Operator : JU
Sample : PB123997BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 25 18:12:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 13:14:06 2019
Response via : Initial Calibration

