

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\

Data File : BN008432.D

Acq On : 25 Oct 2019 18:31

Operator : JU

Sample : K5236-15DL2 10X

Misc :

ALS Vial : 51 Sample Multiplier: 1




Quant Time: Oct 25 19:04:01 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Oct 25 17:59:21 2019

Response via : Initial Calibration

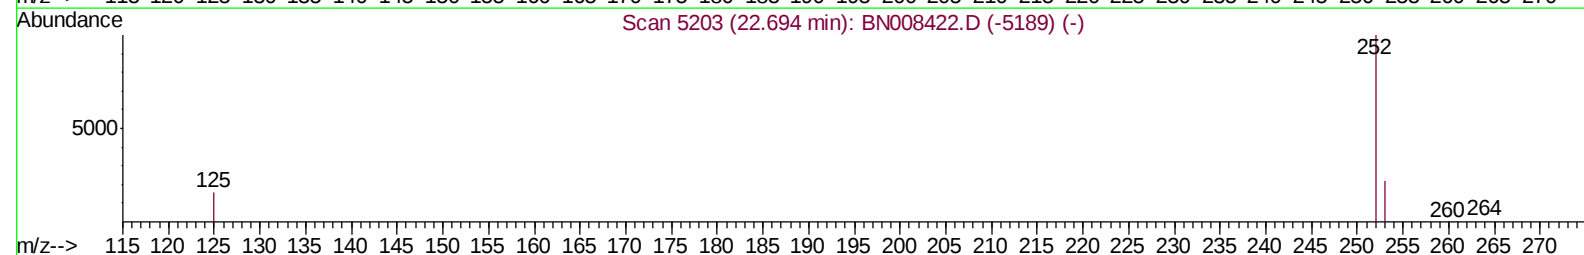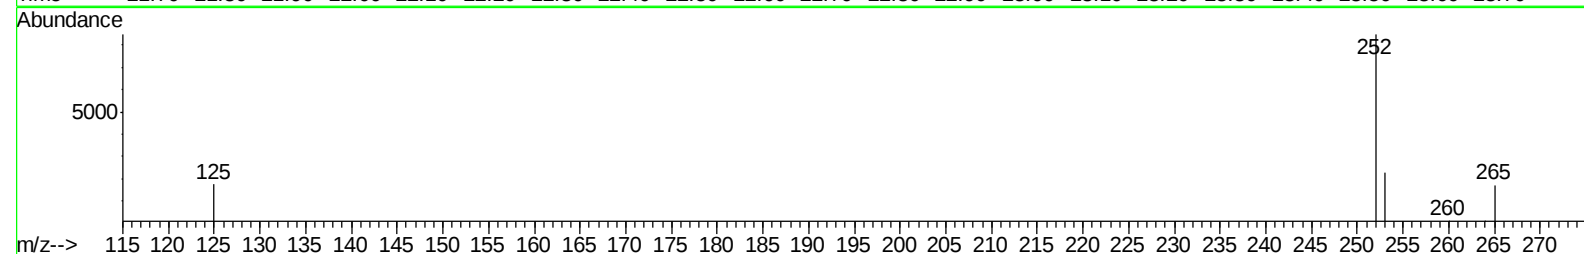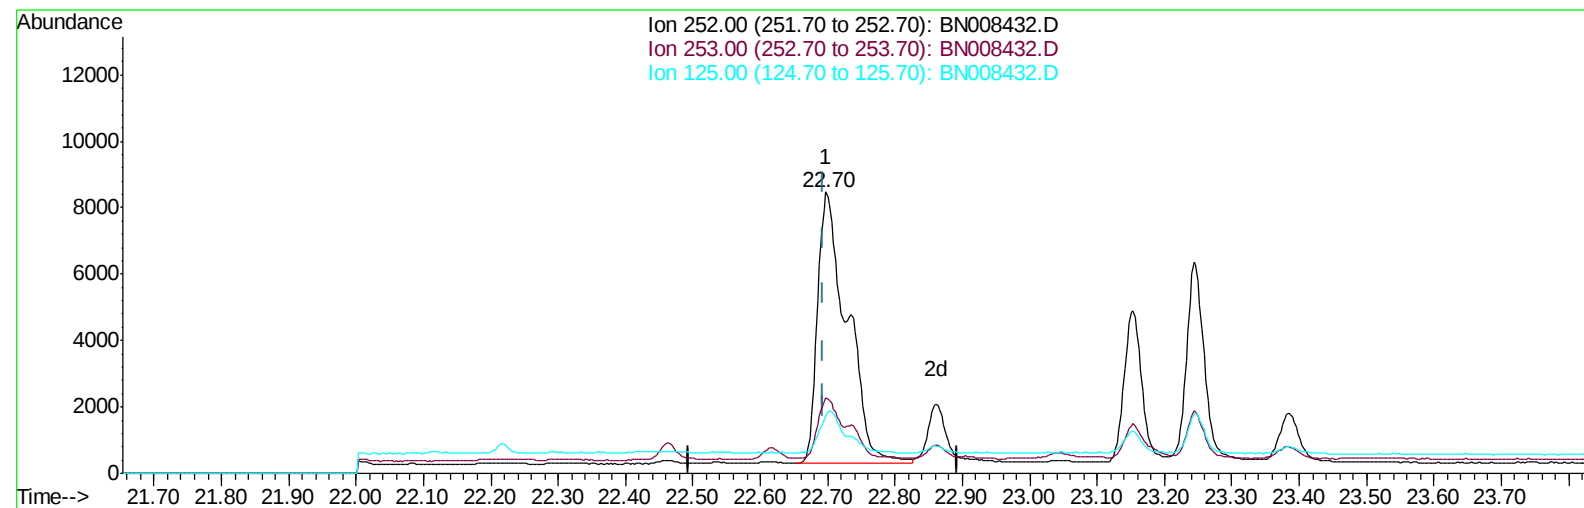

TIC: BN008432.D

(21) Benzo(b)fluoranthene

22.697min (+0.003) 1.00ng/ul

response 24808

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	26.80
125.00	16.20	20.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\

Data File : BN008432.D

Acq On : 25 Oct 2019 18:31

Operator : JU

Sample : K5236-15DL2 10X

Misc :

ALS Vial : 51 Sample Multiplier: 1




Quant Time: Oct 25 19:04:01 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Oct 25 17:59:21 2019

Response via : Initial Calibration

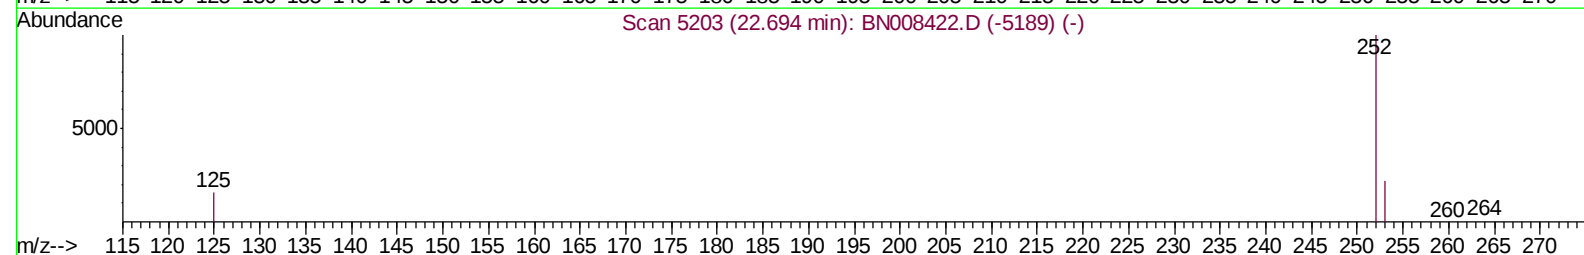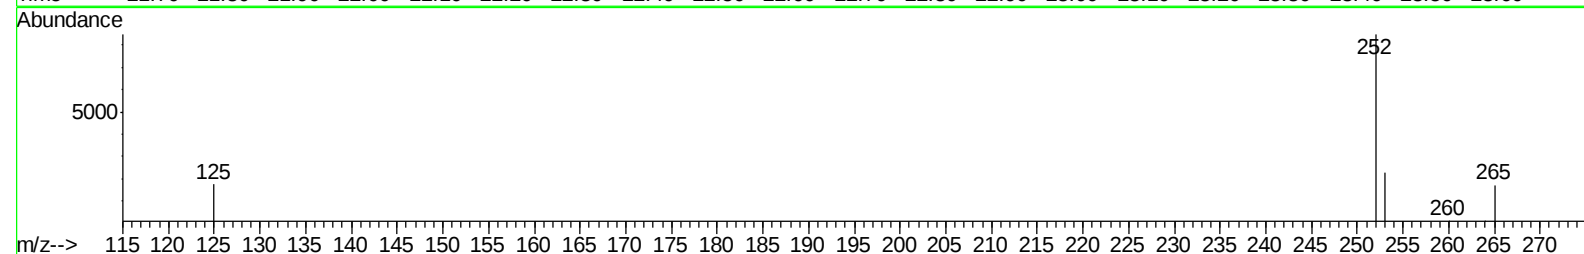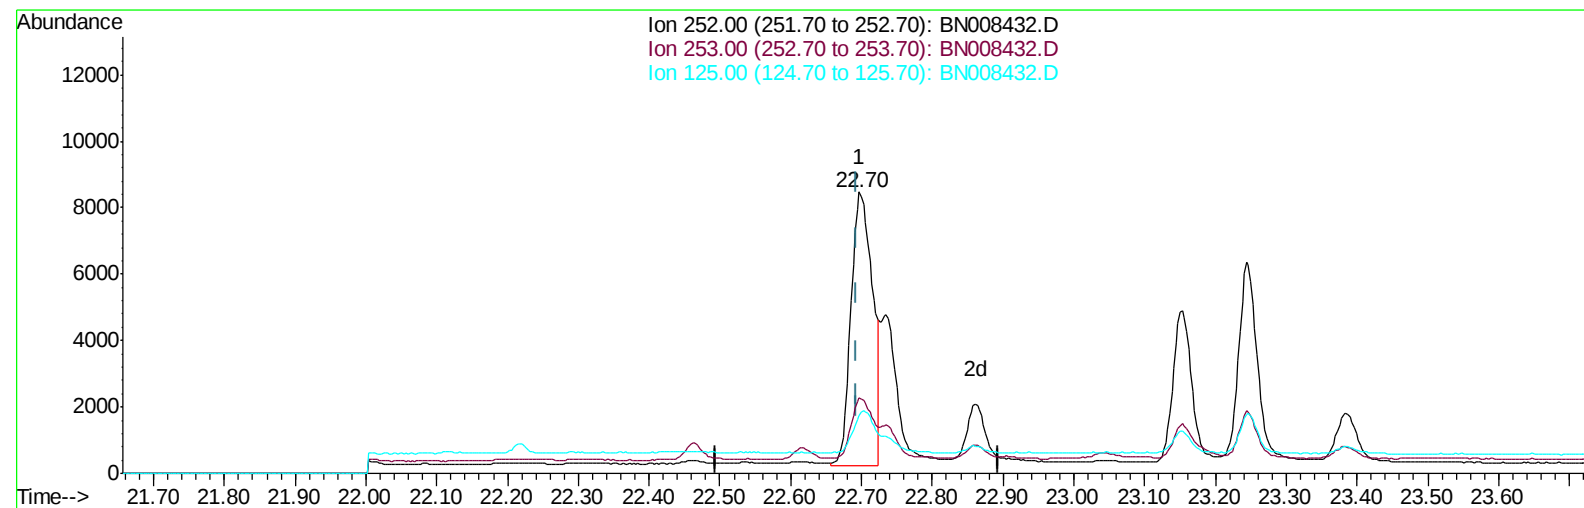

TIC: BN008432.D

(21) Benzo(b)fluoranthene

22.697min (+0.003) 0.70ng/ul m

response 17406

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	26.80
125.00	16.20	20.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\

Data File : BN008432.D

Acq On : 25 Oct 2019 18:31

Operator : JU

Sample : K5236-15DL2 10X

Misc :

ALS Vial : 51 Sample Multiplier: 1




Quant Time: Oct 25 19:04:01 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Oct 25 17:59:21 2019

Response via : Initial Calibration

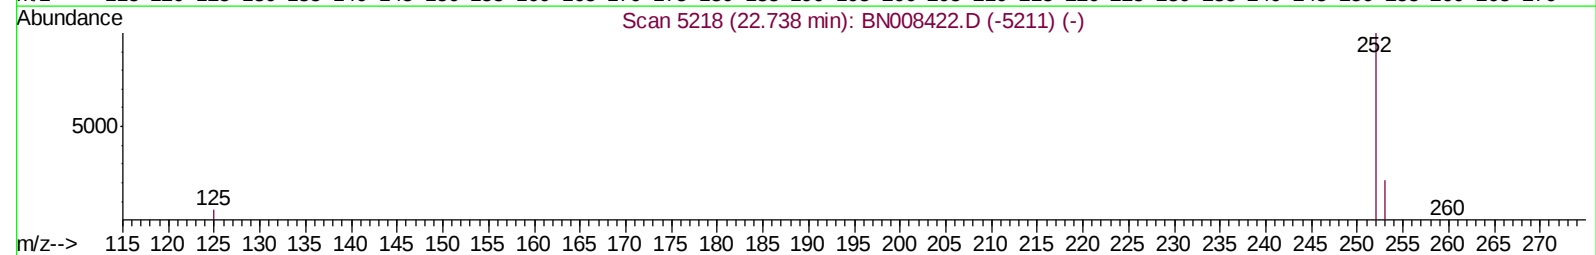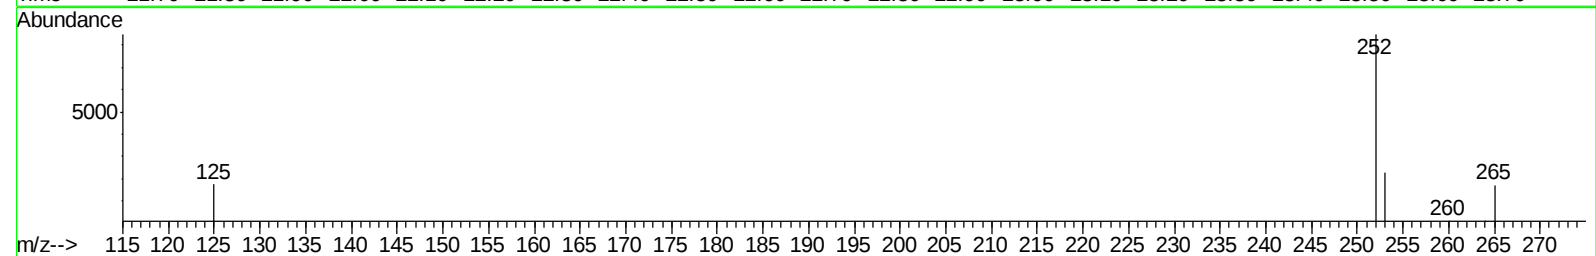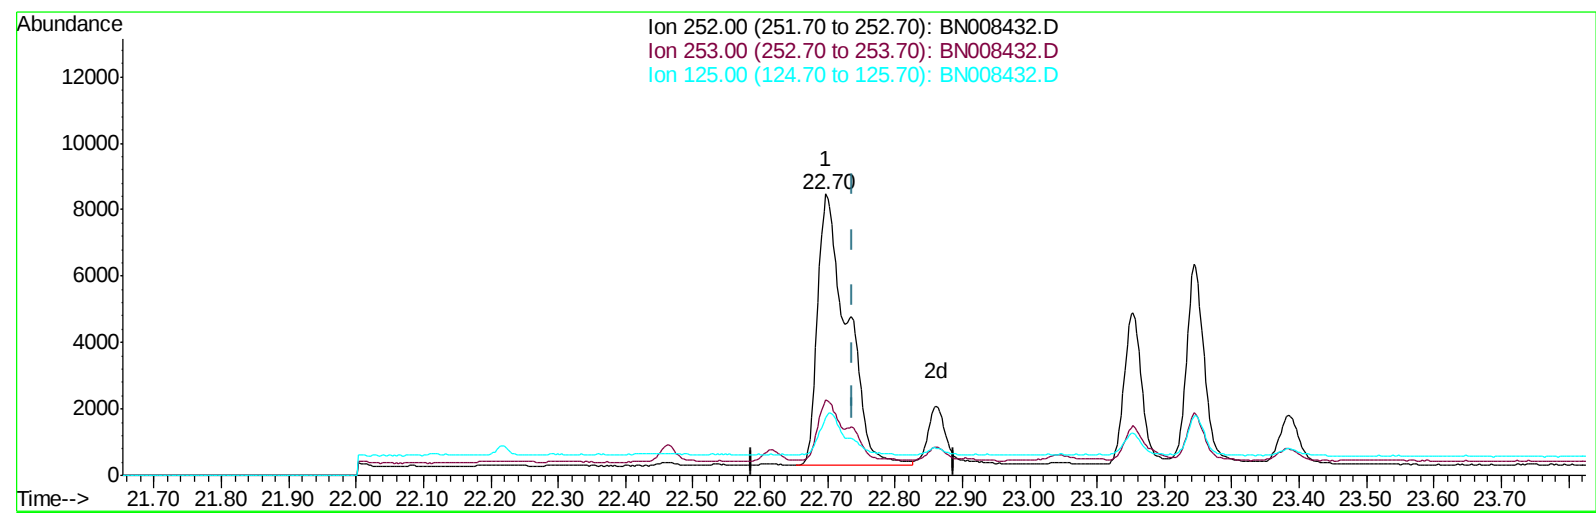

TIC: BN008432.D

(22) Benzo(k)fluoranthene

22.697min (-0.041) 0.88ng/ul

response 24808

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	26.80
125.00	15.40	20.50#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\

Data File : BN008432.D

Acq On : 25 Oct 2019 18:31

Operator : JU

Sample : K5236-15DL2 10X

Misc :

ALS Vial : 51 Sample Multiplier: 1




Quant Time: Oct 25 19:04:01 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Oct 25 17:59:21 2019

Response via : Initial Calibration

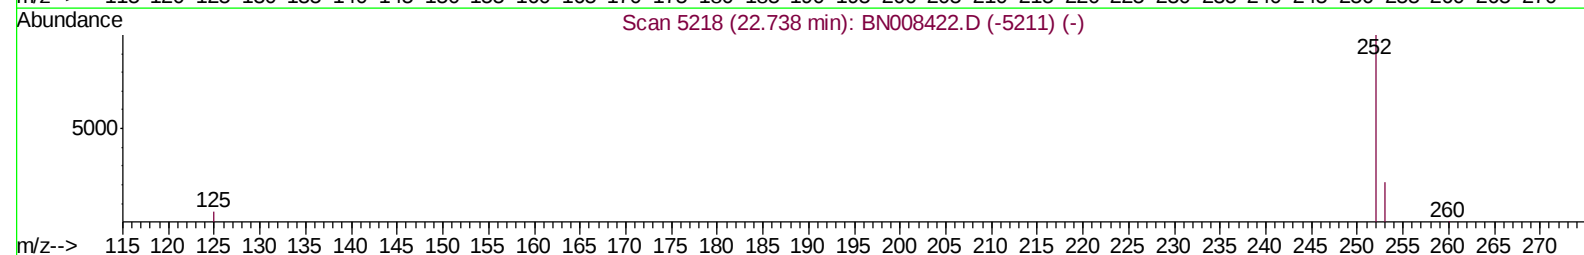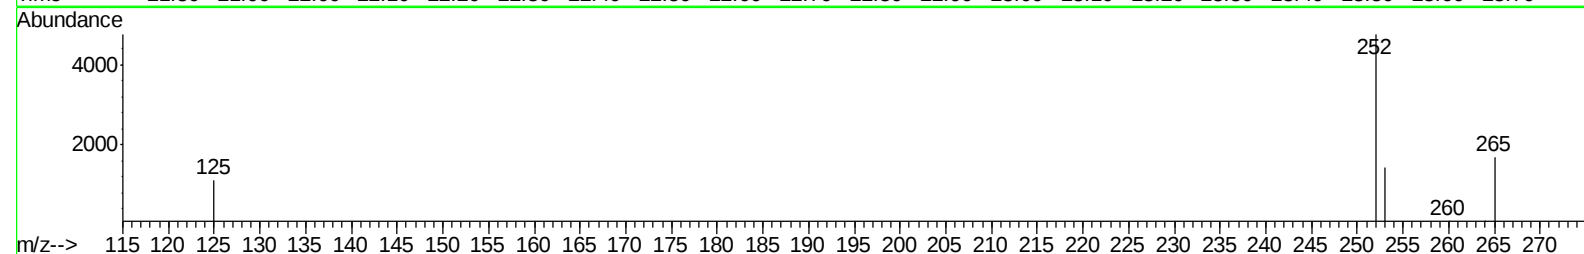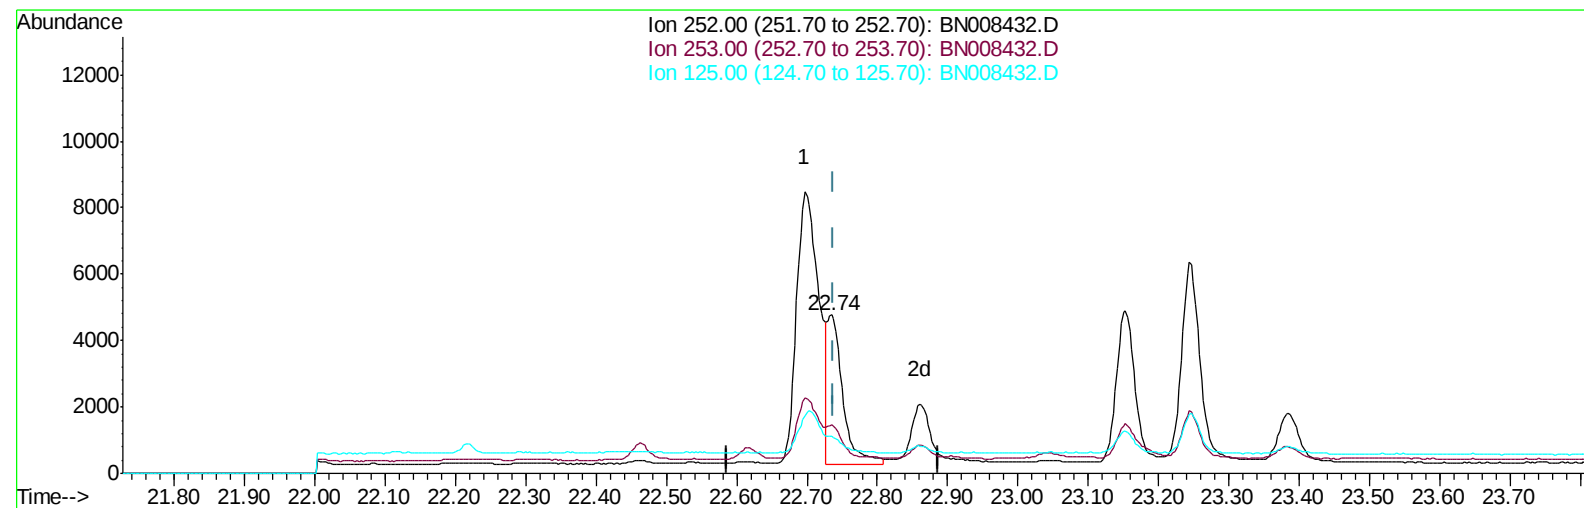

TIC: BN008432.D

(22) Benzo(k)fluoranthene

22.735min (-0.003) 0.25ng/ul m

response 6909

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	30.46
125.00	15.40	23.62#
0.00	0.00	0.00