


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\
Data File : BN008433.D
Acq On : 25 Oct 2019 19:06
Operator : JU
Sample : PB124037BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Quant Time: Oct 25 19:38:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 17:59:21 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK37

Manual Integrations
APPROVED

mohammad
10/25/2019 9:29:34 PM

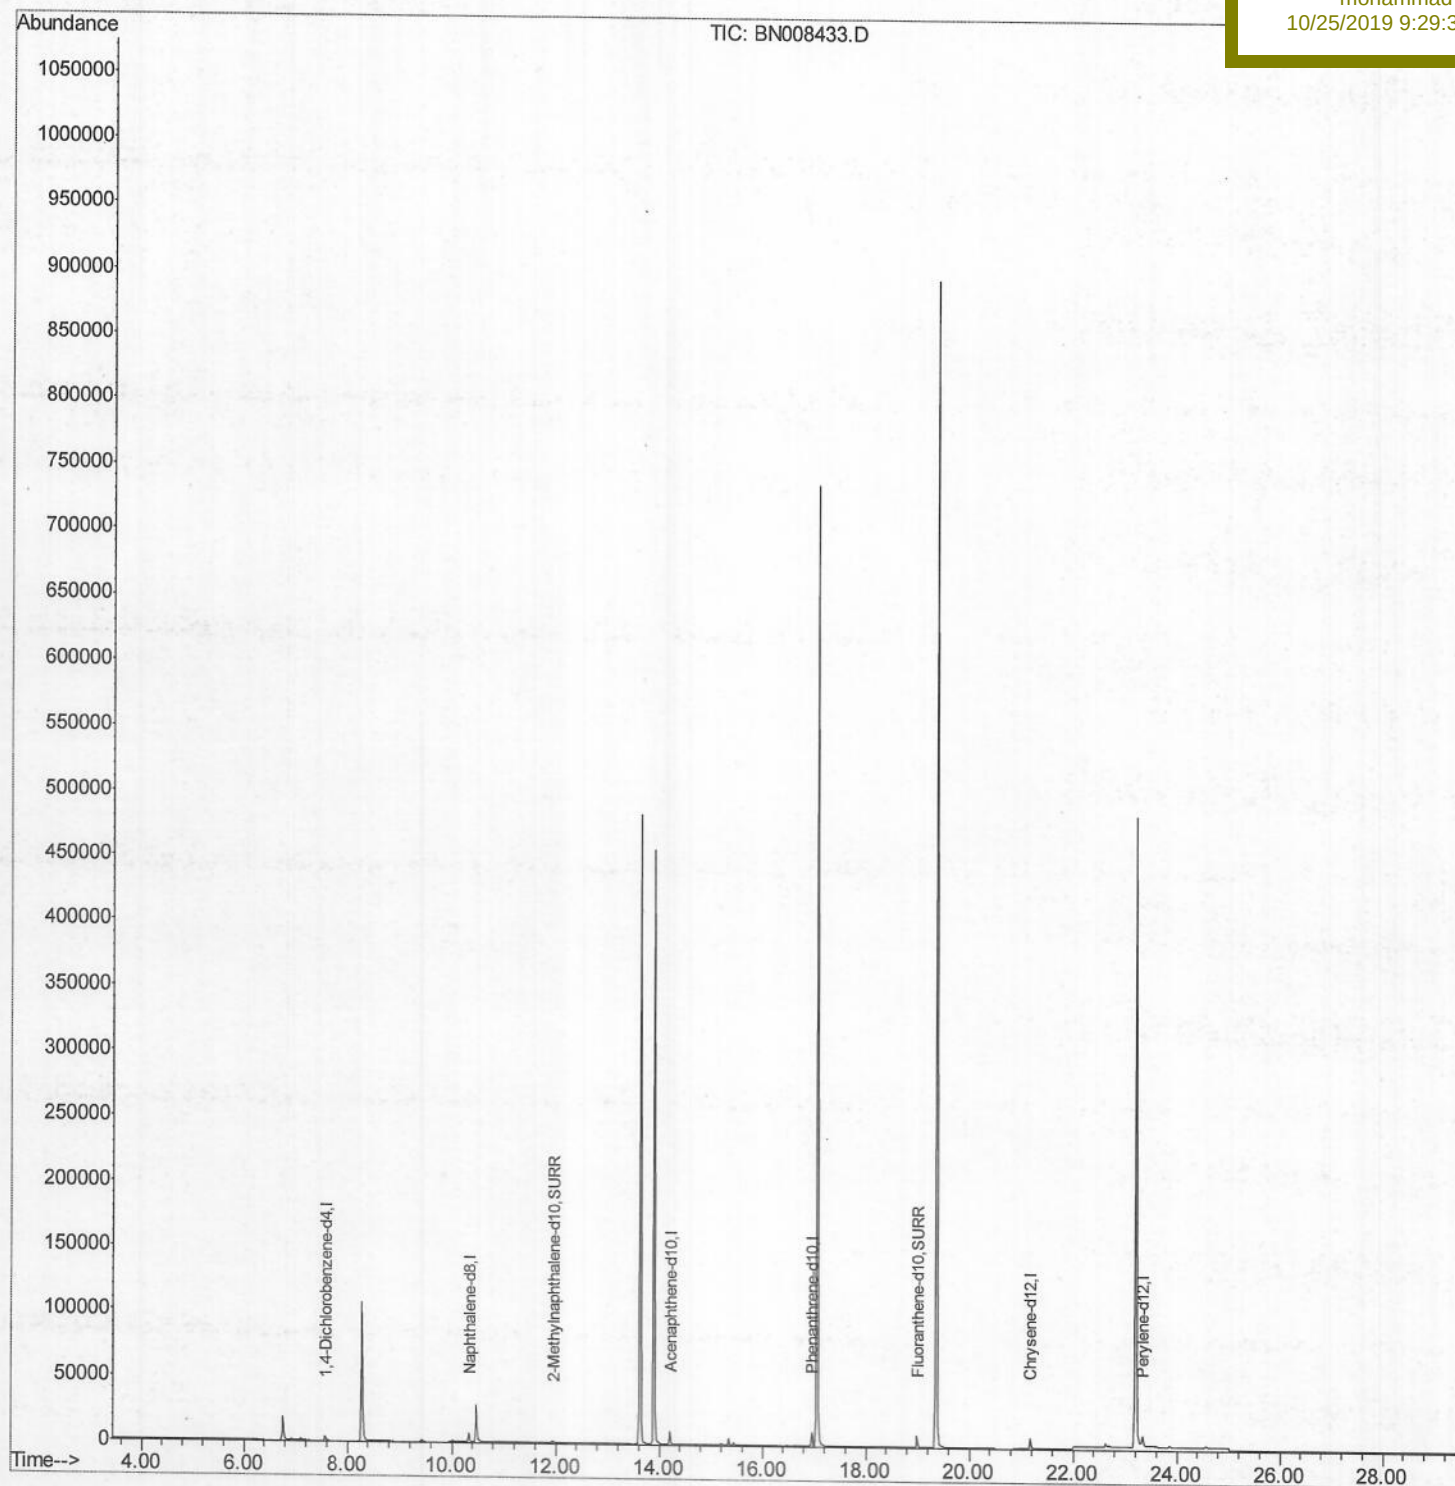

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\

Data File : BN008433.D

Acq On : 25 Oct 2019 19:06

Operator : JU

Sample : PB124037BL

Misc :

ALS Vial : 54 Sample Multiplier: 1

Quant Time: Oct 25 19:37:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Oct 25 17:59:21 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

SBLK37

Manual Integrations
APPROVED

mohammad

10/25/2019 9:29:34 PM

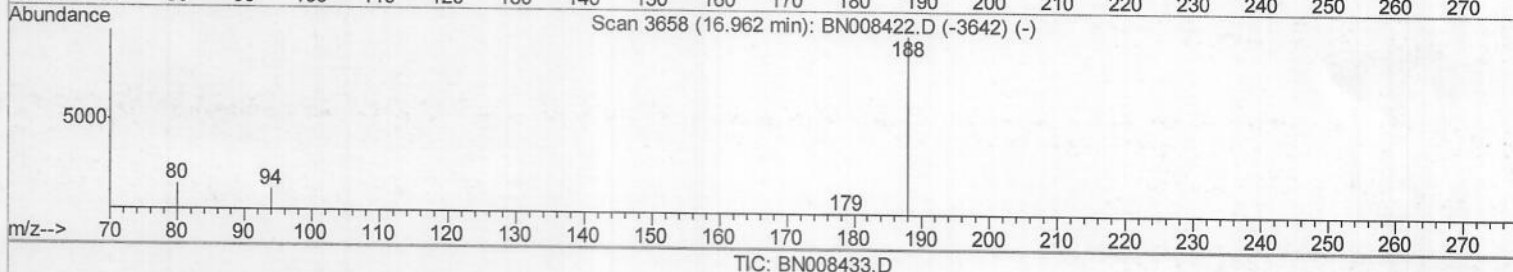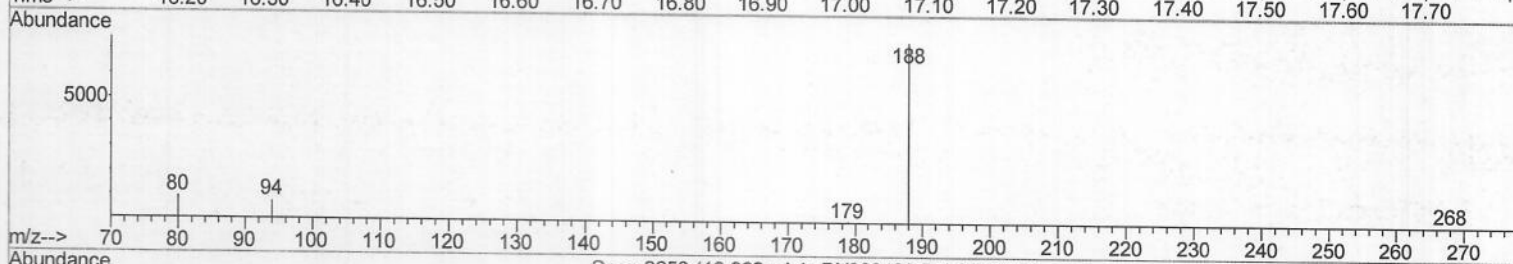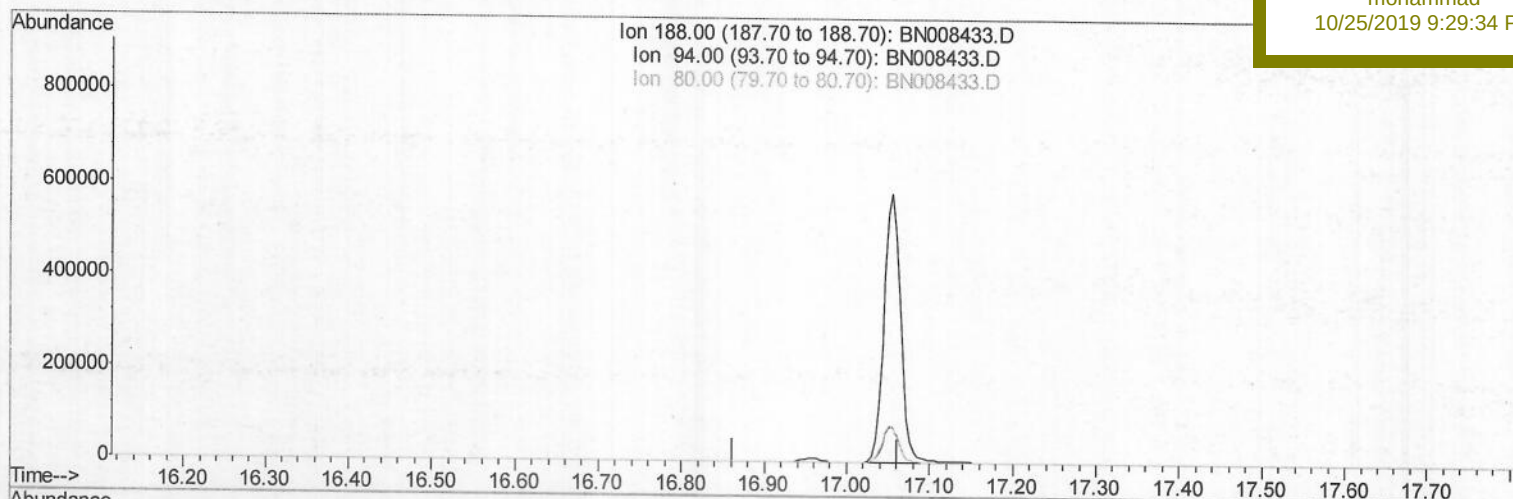

TIC: BN008433.D

(10) Phenanthrene-d10 (I)

16.962min (-16.962) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.90	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\

Data File : BN008433.D

Acq On : 25 Oct 2019 19:06

Operator : JU

Sample : PB124037BL

Misc :

ALS Vial : 54 Sample Multiplier: 1

Quant Time: Oct 25 19:37:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Oct 25 17:59:21 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

SBLK37

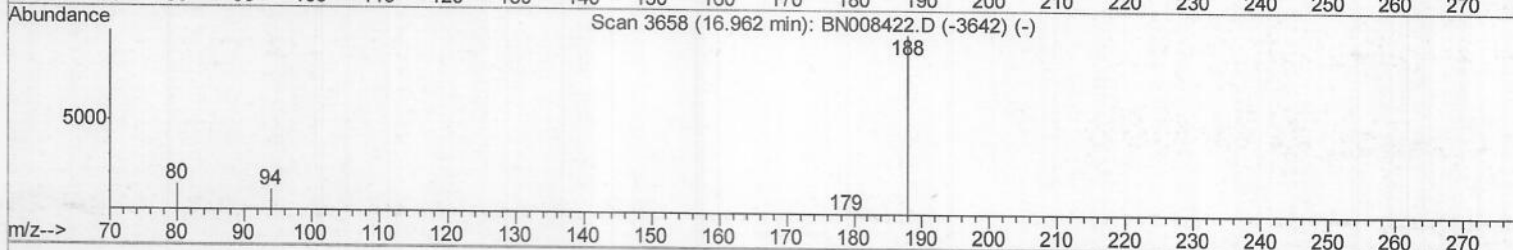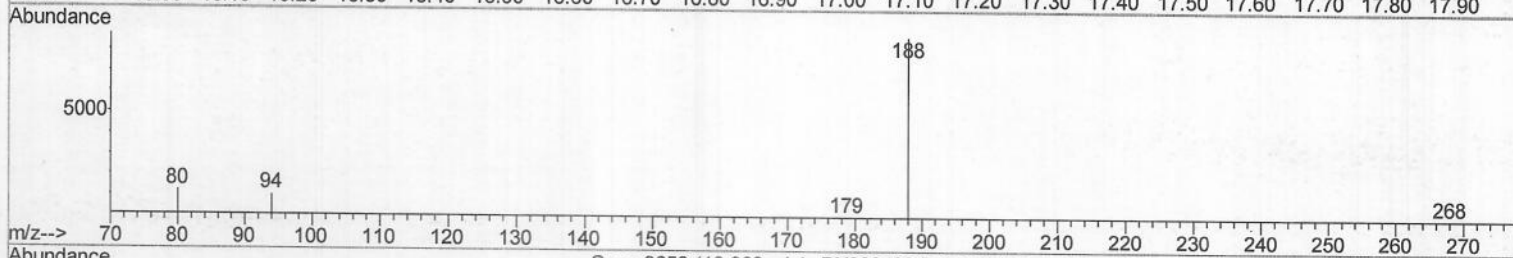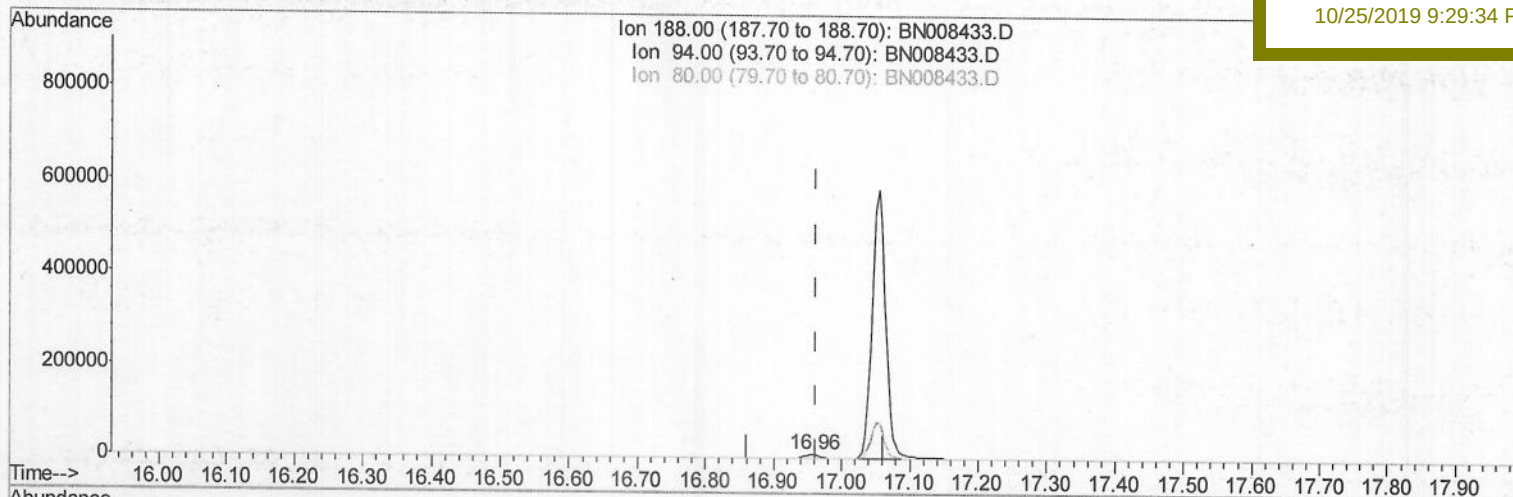Manual Integrations
APPROVEDmohammad
10/25/2019 9:29:34 PM

TIC: BN008433.D

(10) Phenanthrene-d10 (I)

16.958min (-0.004) 0.40ng/ul m

response 12761

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	11.48
80.00	12.60	14.11
0.00	0.00	0.00

JU
10/26/19

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102419\
Data File : BN008433.D
Acq On : 25 Oct 2019 19:06
Operator : JU
Sample : PB124037BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Quant Time: Oct 25 19:38:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 17:59:21 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK37

Manual Integrations
APPROVED

mohammad
10/25/2019 9:29:34 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	1772	0.40	ng/ul	0.00
2) Naphthalene-d8	10.33	136	8902	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.20	164	5742	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.96	188	12761m	0.40	ng/ul	0.00
16) Chrysene-d12	21.17	240	9663	0.40	ng/ul	0.00
20) Perylene-d12	23.33	264	9326	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.94	152	3428	0.23	ng/ul	0.00
14) Fluoranthene-d10	19.00	212	10040	0.23	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
10/26/19