
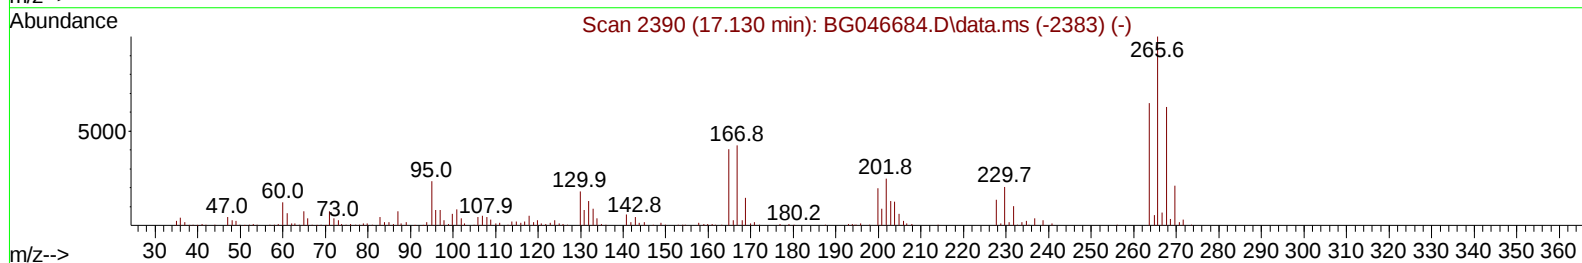
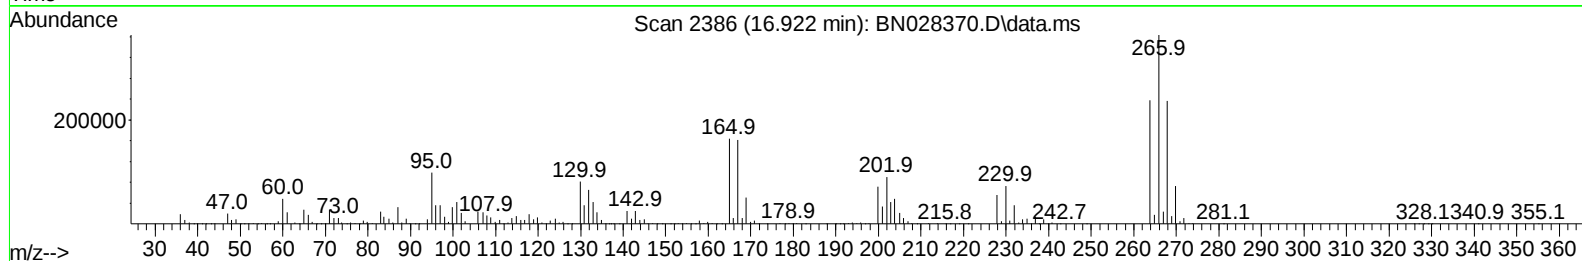


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028370.D
Acq On : 24 Oct 2023 10:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 05:13:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 05:13:40 2023
Response via : Initial Calibration

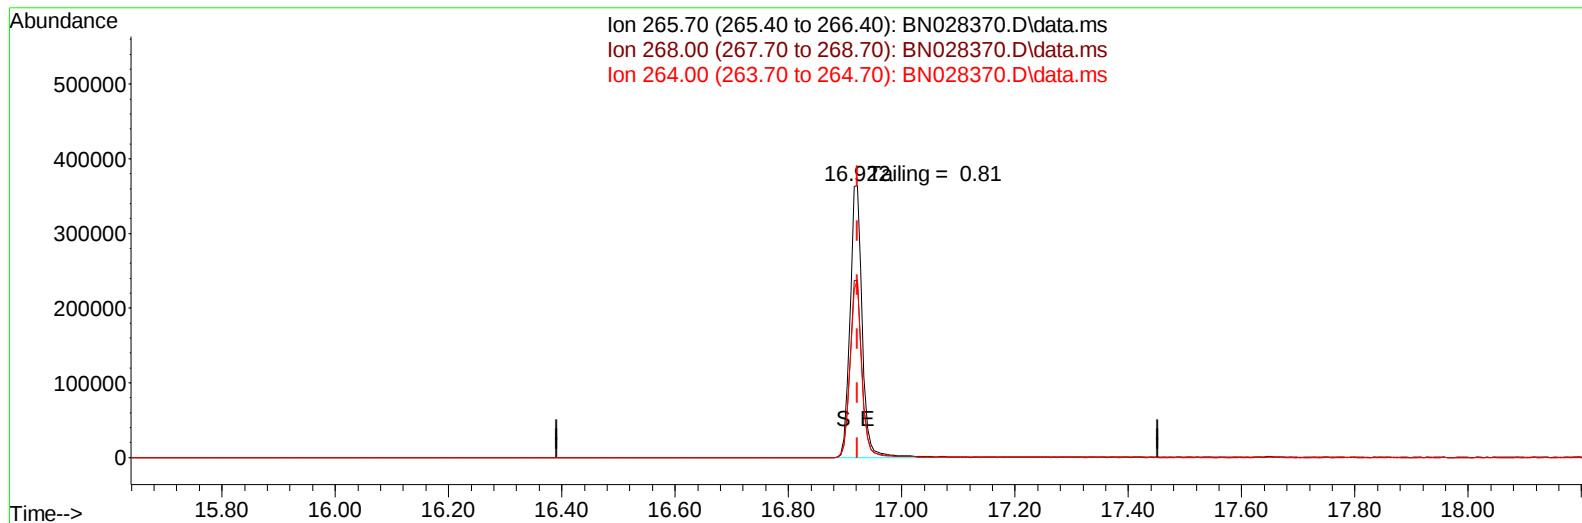

TIC: BN028370.D\data.ms

(70) Pentachlorophenol (C)




16.922min (0.000) 23264.19 ng

response 547897

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.17
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028370.D
Acq On : 24 Oct 2023 10:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 05:13:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 05:13:40 2023
Response via : Initial Calibration

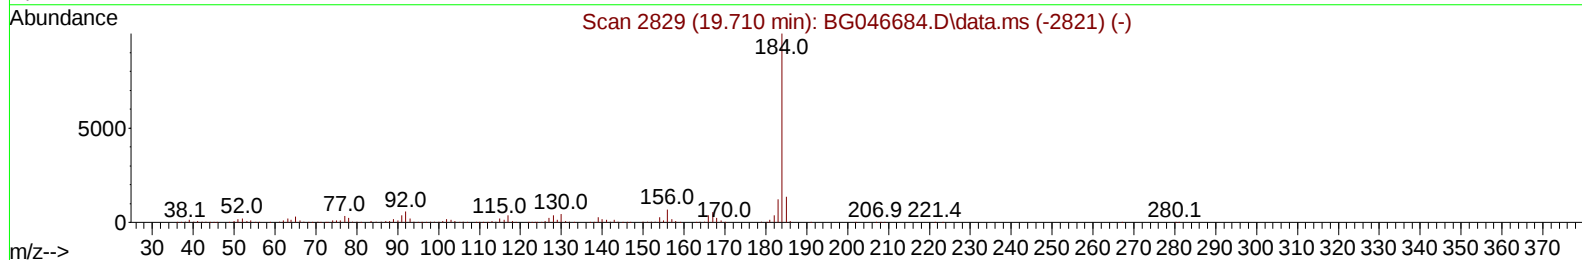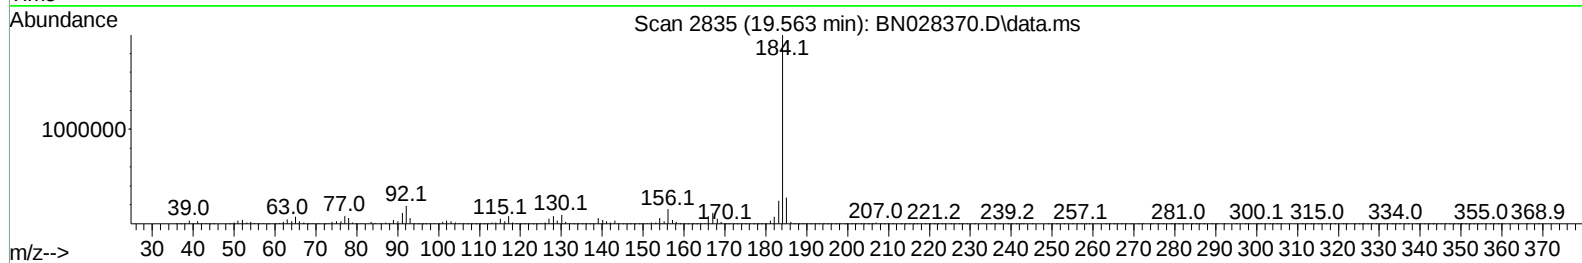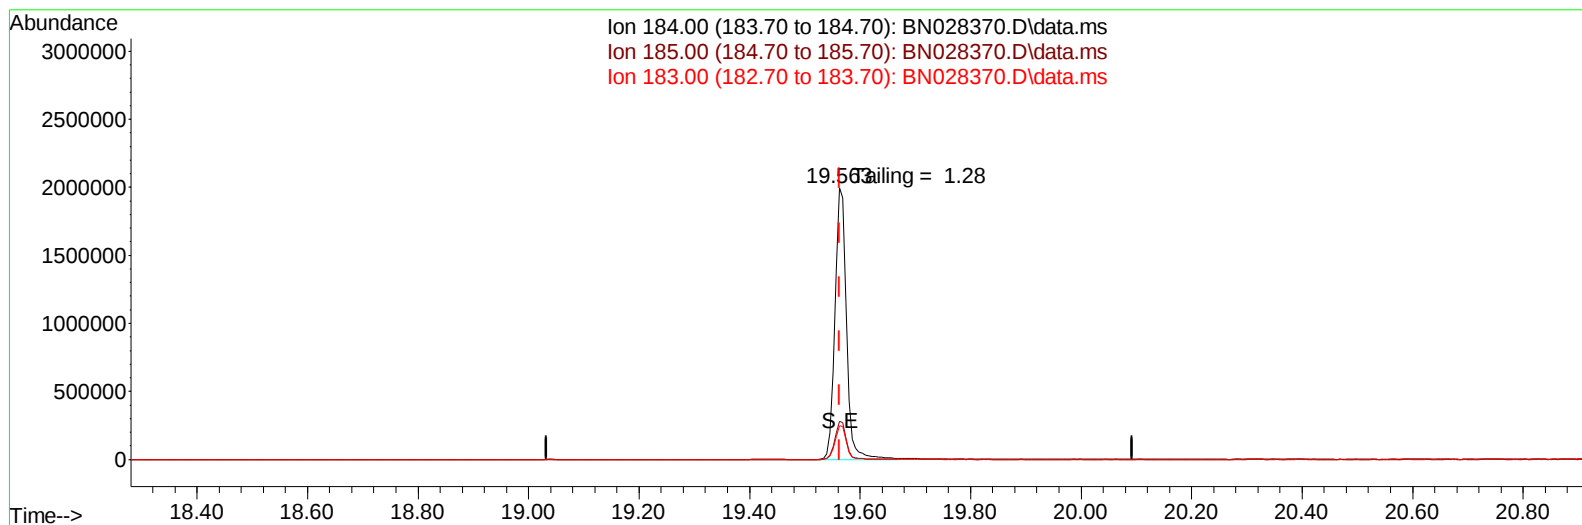

TIC: BN028370.D\data.ms

(77) Benzidine**19.563min (0.000) 675556.71 ng****response 2977873**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	12.35
0.00	0.00	0.00