
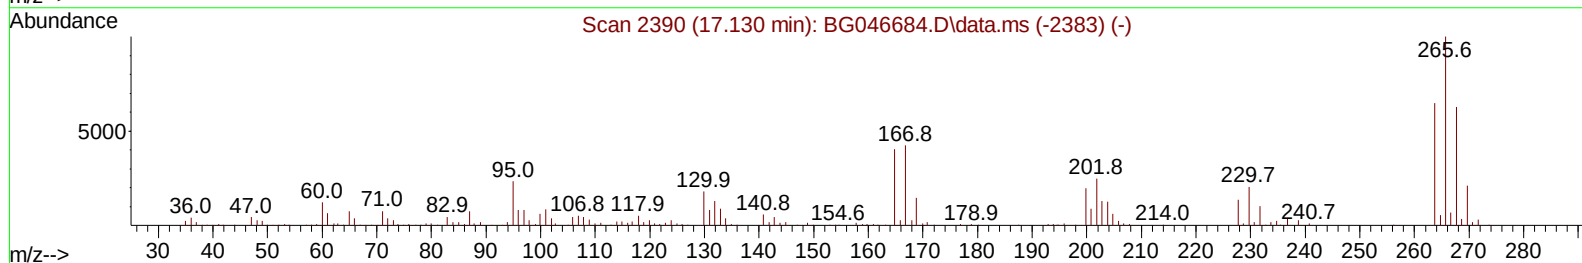
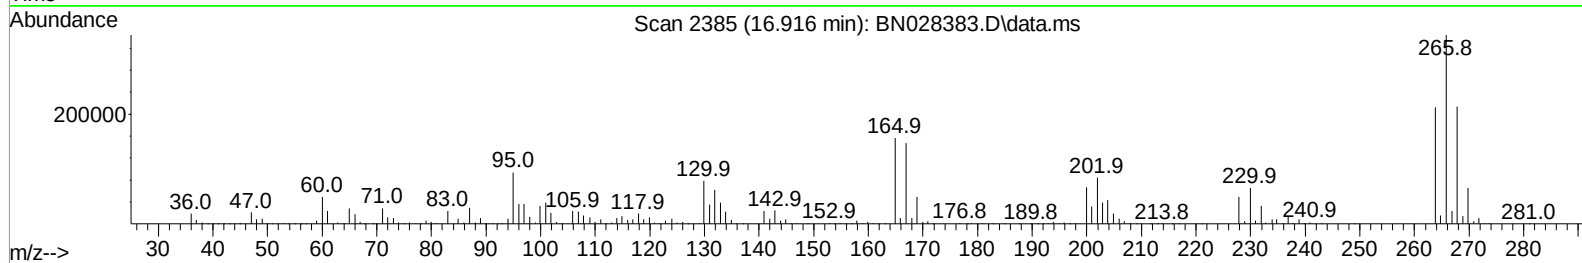


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028383.D
Acq On : 24 Oct 2023 19:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 05:15:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 05:13:40 2023
Response via : Initial Calibration

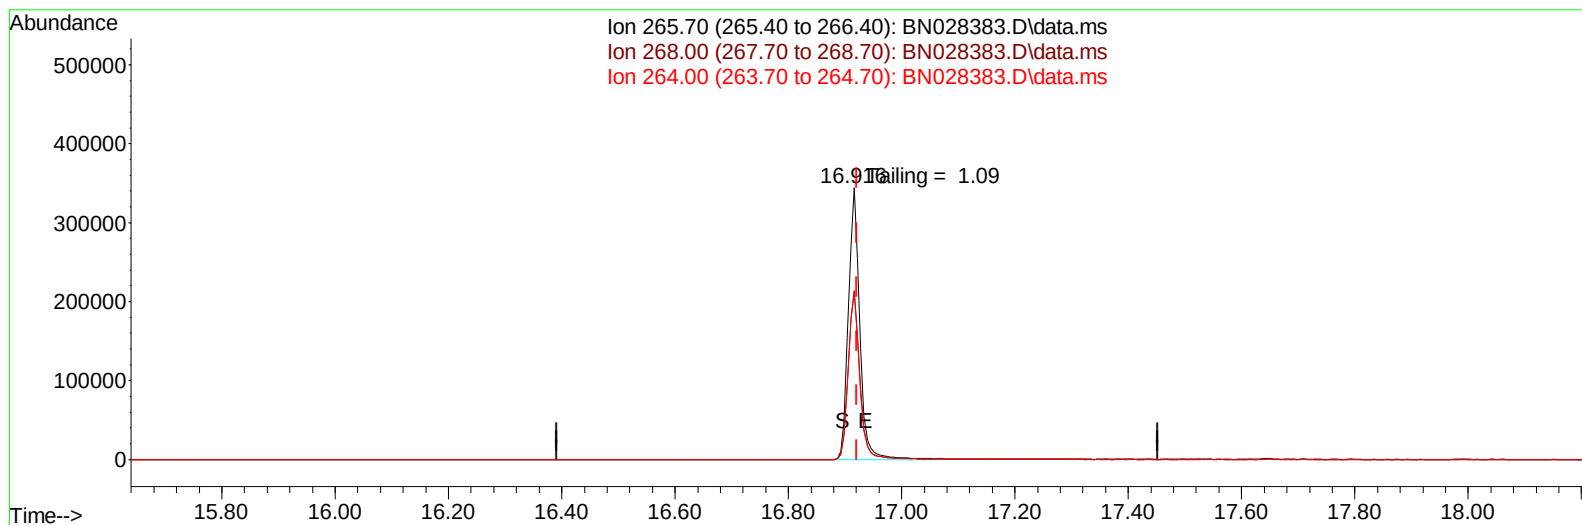




TIC: BN028383.D\data.ms

(70) Pentachlorophenol (C)**16.916min (-0.006) 19923.86 ng****response 483770**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.08
264.00	61.60	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028383.D
Acq On : 24 Oct 2023 19:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 05:15:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 05:13:40 2023
Response via : Initial Calibration

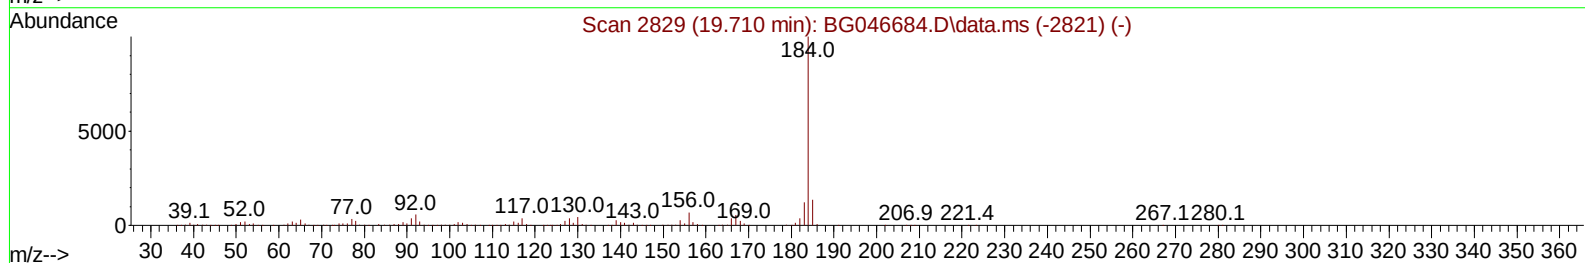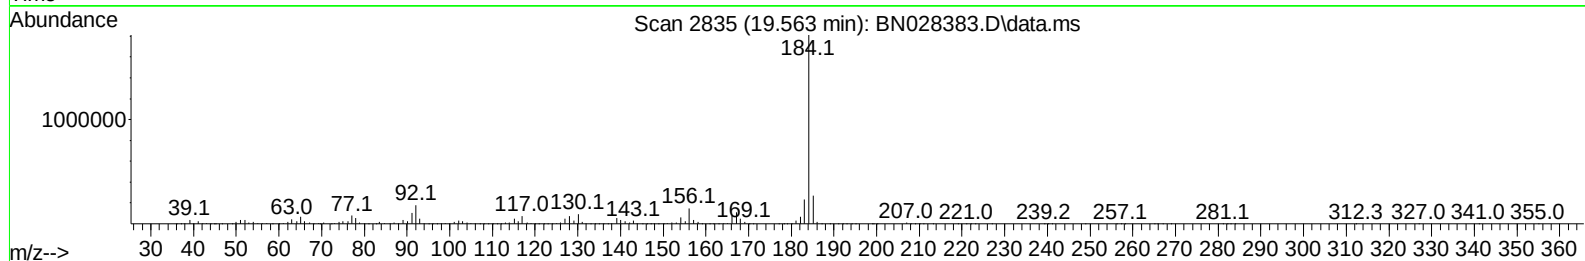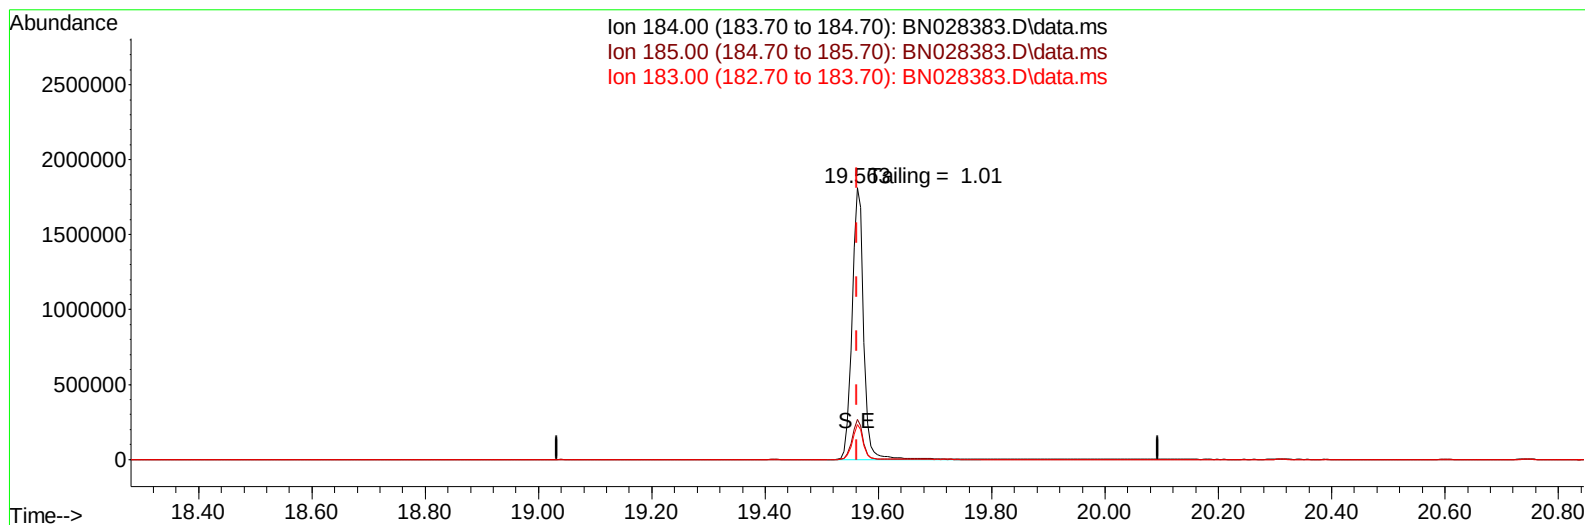

TIC: BN028383.D\data.ms

(77) Benzidine**19.563min (+ 0.000) 657411.98 ng****response 2593916**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.80
183.00	13.20	12.91
0.00	0.00	0.00