Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028380.D
Acq On : 24 Oct 2023 16:12
Operator : MA/JU
Sample : 04938-17MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations APPROVED
Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

Quant Time: Oct 25 01:05:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 23 15:14:08 2023
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.871	152	4621	0.400	ng	# 0.00
7) Naphthalene-d8	10.682	136	14145	0.400	ng	#-0.02
13) Acenaphthene-d10	14.523	164	9527	0.400	ng	-0.01
19) Phenanthrene-d10	17.281	188	11064	0.400	ng	#-0.01
29) Chrysene-d12	21.480	240	10881	0.400	ng	# 0.00
35) Perylene-d12	23.925	264	12754	0.400	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.423	112	2864	0.200	ng	0.00
5) Phenol-d6	7.048	99	3699	0.209	ng	0.00
8) Nitrobenzene-d5	9.070	82	3277	0.261	ng	-0.03
11) 2-Methylnaphthalene-d10	12.271	152	4484	0.211	ng	-0.02
14) 2,4,6-Tribromophenol	16.028	330	535	0.115	ng	-0.04
15) 2-Fluorobiphenyl	13.144	172	6068	0.181	ng	-0.02
27) Fluoranthene-d10	19.323	212	4948	0.167	ng	0.00
31) Terphenyl-d14	19.909	244	5111	0.221	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.299	88	1977	0.354	ng	# 66
3) n-Nitrosodimethylamine	3.653	42	2768	0.454	ng	97
6) bis(2-Chloroethyl)ether	7.315	93	6771	0.497	ng	# 89
9) Naphthalene	10.735	128	1694799	46.192	ng	97
10) Hexachlorobutadiene	10.960	225	3087	0.490	ng	# 100
12) 2-Methylnaphthalene	12.351	142	918072	35.212	ng	99
16) Acenaphthylene	14.256	152	239660	5.598	ng	# 92
17) Acenaphthene	14.587	154	111843	4.146	ng	92
18) Fluorene	15.569	166	212923	5.996	ng	# 97
20) 4,6-Dinitro-2-methylph...	15.792	198	815	1.052	ng	# 1
21) 4-Bromophenyl-phenylether	16.462	248	3107	0.545	ng	# 1
22) Hexachlorobenzene	16.549	284	2927	0.499	ng	# 35
23) Atrazine	16.748	200	3242	0.607	ng	# 5
24) Pentachlorophenol	17.008	266	395	0.147	ng	# 55
25) Phenanthrene	17.331	178	781815	25.815	ng	99
26) Anthracene	17.418	178	202139	6.988	ng	# 96
28) Fluoranthene	19.351	202	482831	12.690	ng	99
30) Pyrene	19.718	202	594036	15.955	ng	# 96
32) Benzo(a)anthracene	21.462	228	295174	7.636	ng	99
33) Chrysene	21.515	228	271568	7.340	ng	98
34) Bis(2-ethylhexyl)phtha...	21.336	149	14708	0.498	ng	99
36) Indeno(1,2,3-cd)pyrene	26.487	276	217483	4.230	ng	96
37) Benzo(b)fluoranthene	23.174	252	334068	8.380	ng	# 90
38) Benzo(k)fluoranthene	23.218	252	130906m	3.228	ng	
39) Benzo(a)pyrene	23.814	252	276733m	6.978	ng	
40) Dibenzo(a,h)anthracene	26.495	278	67411	1.615	ng	99
41) Benzo(g,h,i)perylene	27.294	276	263420	6.112	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102423\
Data File : BN028380.D
Acq On : 24 Oct 2023 16:12
Operator : MA/JU
Sample : 04938-17MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 25 01:05:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 23 15:14:08 2023
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

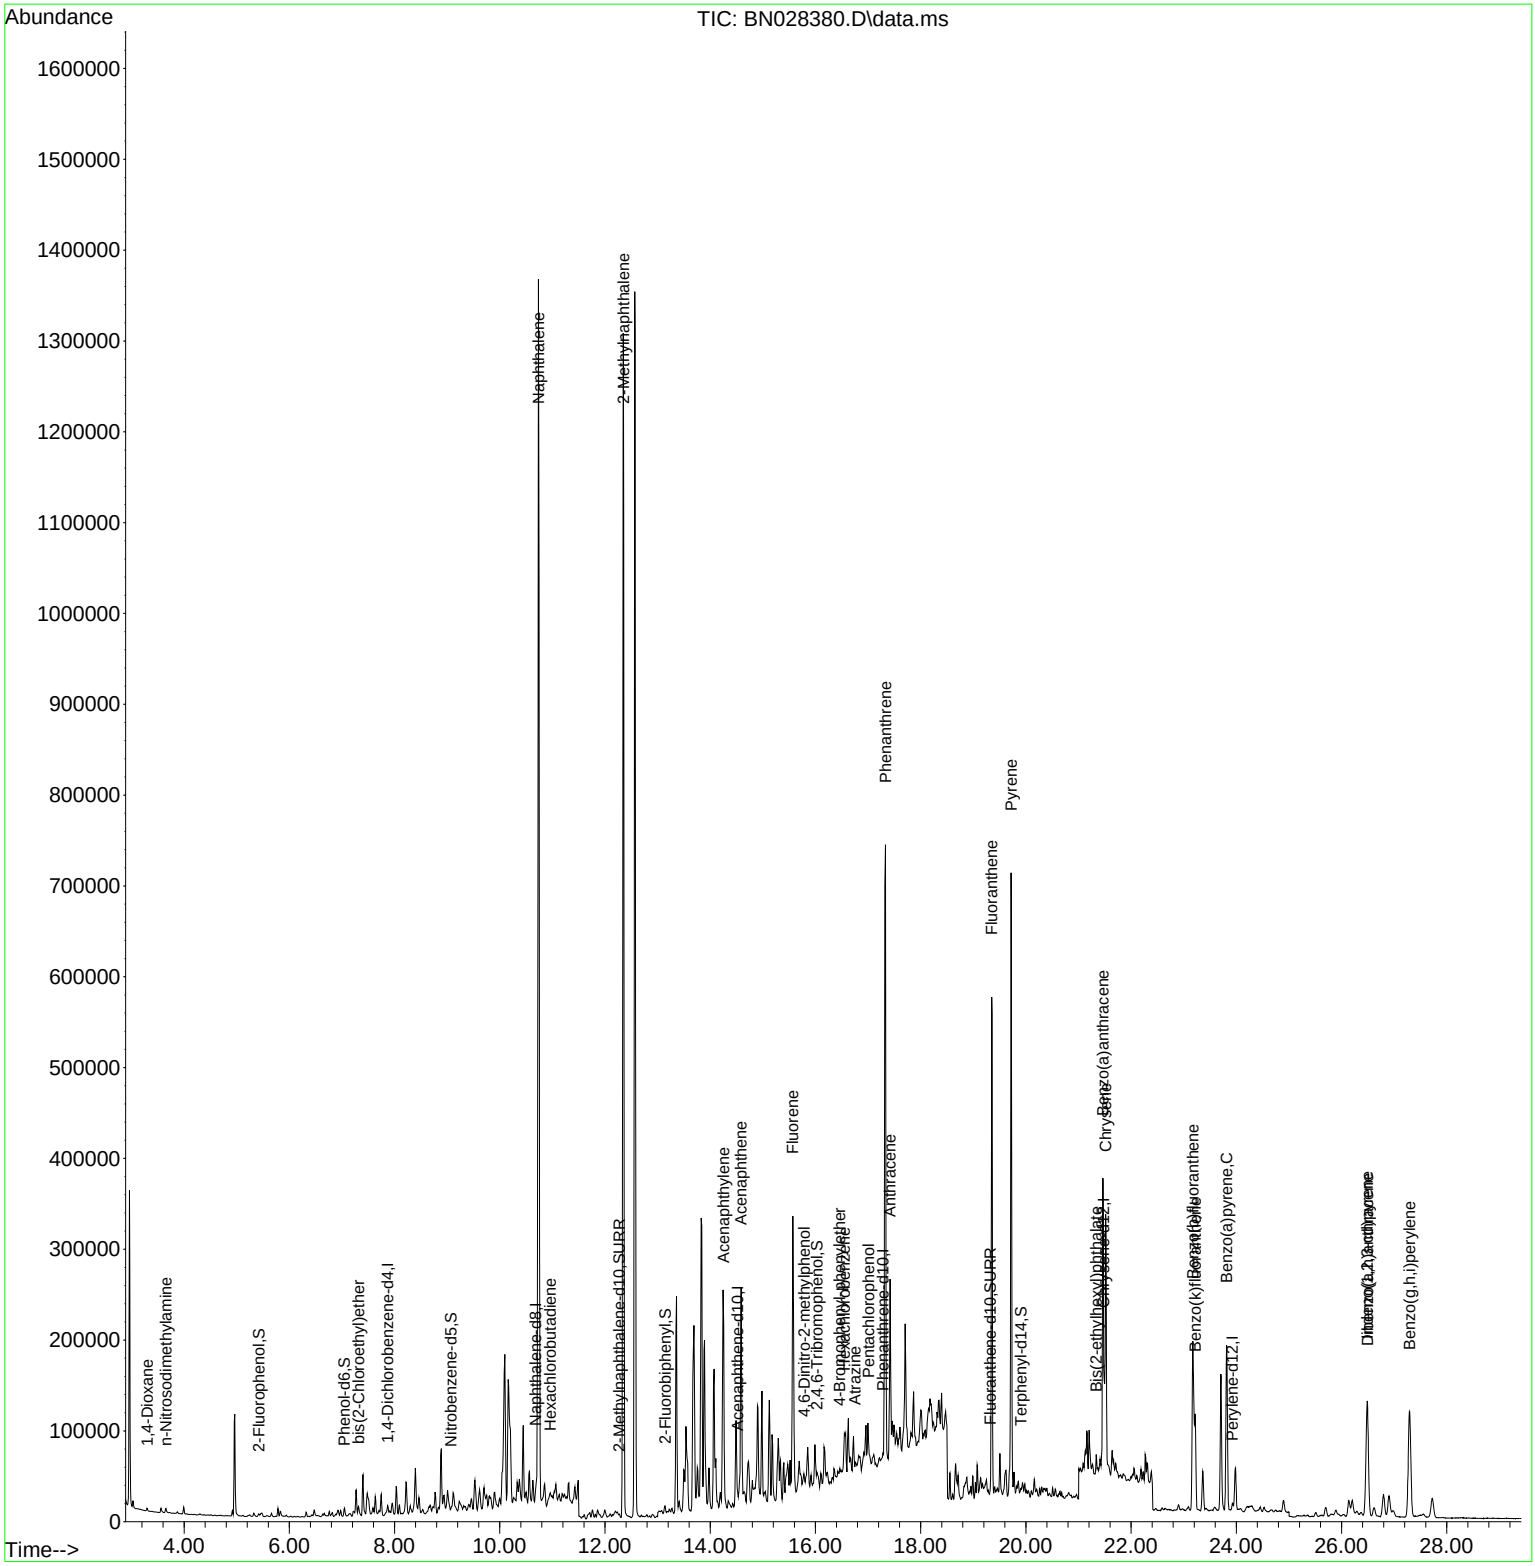

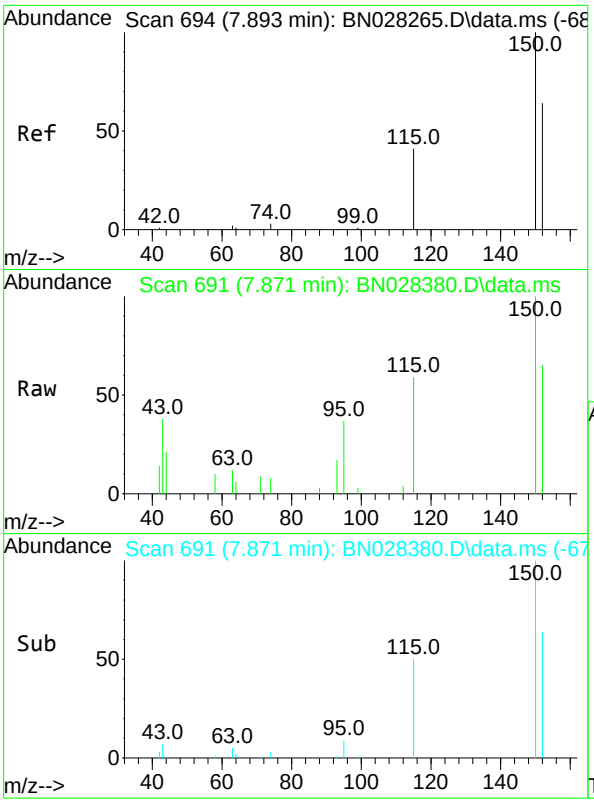

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.871 min Scan# 6
Delta R.T. -0.007 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:152 Resp: 462

Ion	Ratio	Lower	Upper
152	100		
150	153.7	121.6	182.4
115	90.8	54.3	81.5#



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

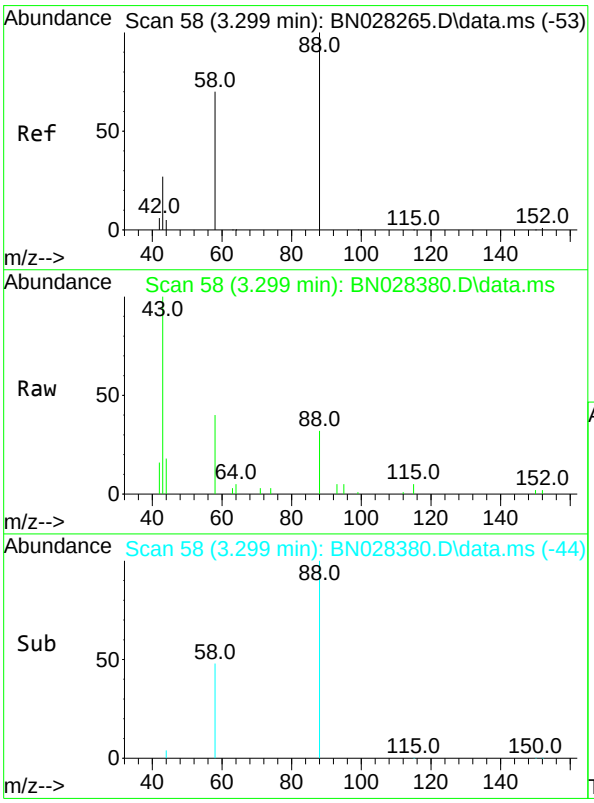

#2
1,4-Dioxane
Concen: 0.354 ng
RT: 3.299 min Scan# 58
Delta R.T. 0.000 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion: 88 Resp: 1977

Ion	Ratio	Lower	Upper
88	100		
43	81.9	26.6	39.8#
58	77.1	55.4	83.0



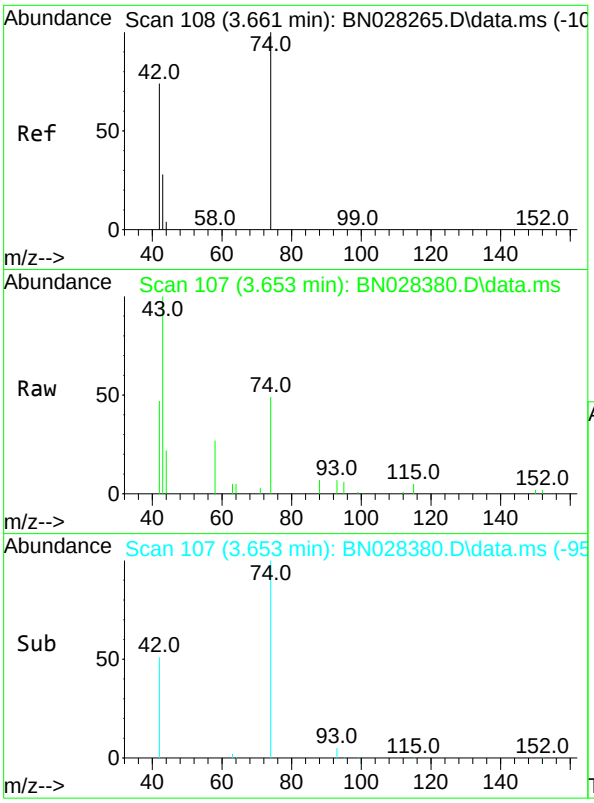

#3
n-Nitrosodimethylamine
Concen: 0.454 ng
RT: 3.653 min Scan# 1
Delta R.T. -0.014 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion: 42 Resp: 276

Ion	Ratio	Lower	Upper
42	100		
74	144.9	112.6	168.8
44	10.5	7.8	11.6



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

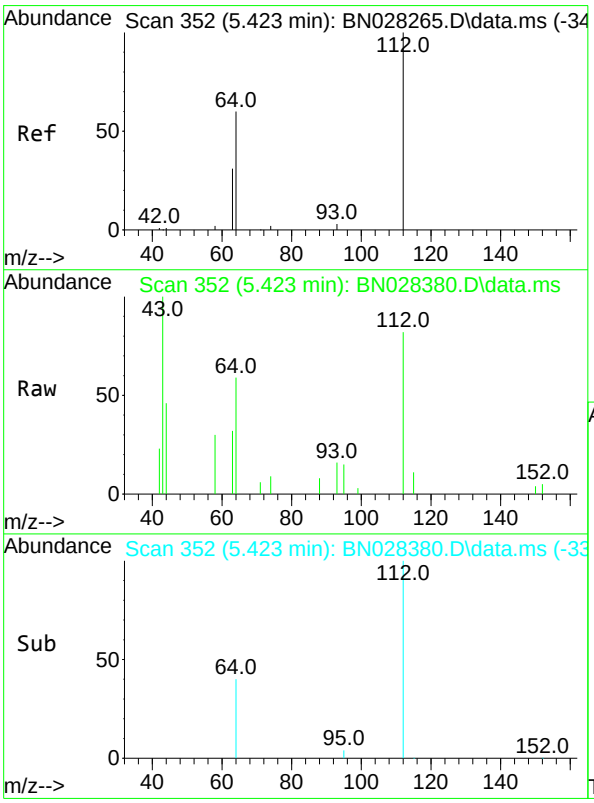

#4
2-Fluorophenol
Concen: 0.200 ng
RT: 5.423 min Scan# 352
Delta R.T. -0.007 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:112 Resp: 2864

Ion	Ratio	Lower	Upper
112	100		
64	62.8	46.9	70.3
63	26.5	25.0	37.4



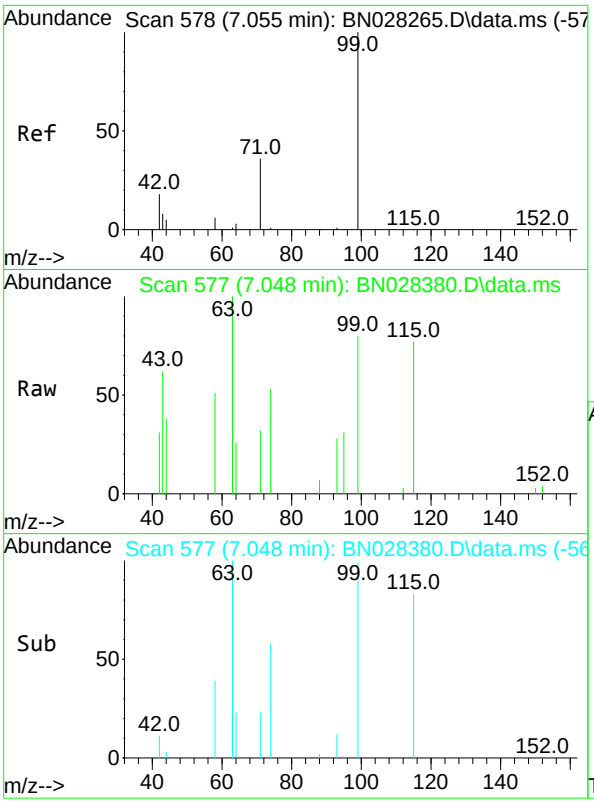

#5
Phenol-d6
Concen: 0.209 ng
RT: 7.048 min Scan# 5
Delta R.T. -0.007 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion: 99 Resp: 369

Ion	Ratio	Lower	Upper
99	100		
42	17.6	15.9	23.9
71	35.1	28.6	42.8



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

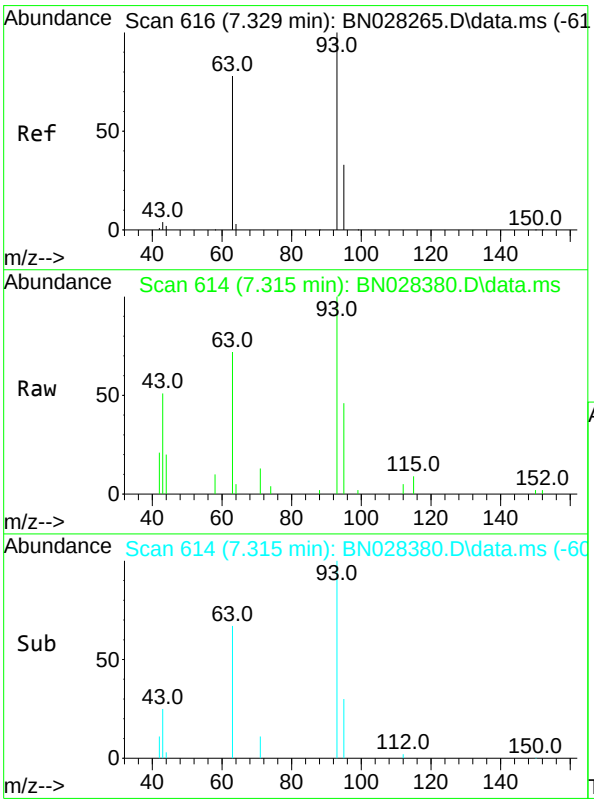

#6
bis(2-Chloroethyl)ether
Concen: 0.497 ng
RT: 7.315 min Scan# 614
Delta R.T. -0.007 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion: 93 Resp: 6771

Ion	Ratio	Lower	Upper
93	100		
63	75.7	62.6	93.8
95	51.2	27.2	40.8#



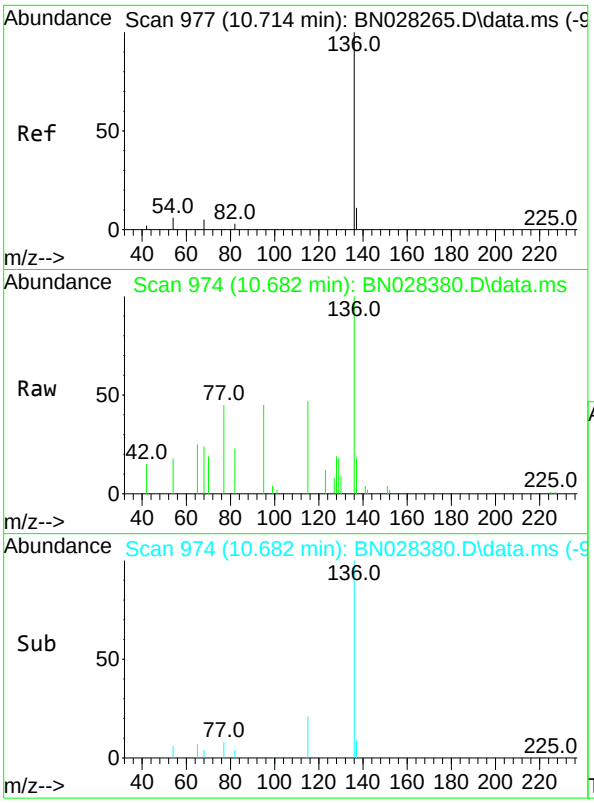

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.682 min Scan# 9
Delta R.T. -0.021 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:136 Resp: 1414

Ion	Ratio	Lower	Upper
136	100		
137	17.9	9.8	14.8#
54	18.5	6.2	9.4#
68	23.9	5.7	8.5#



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

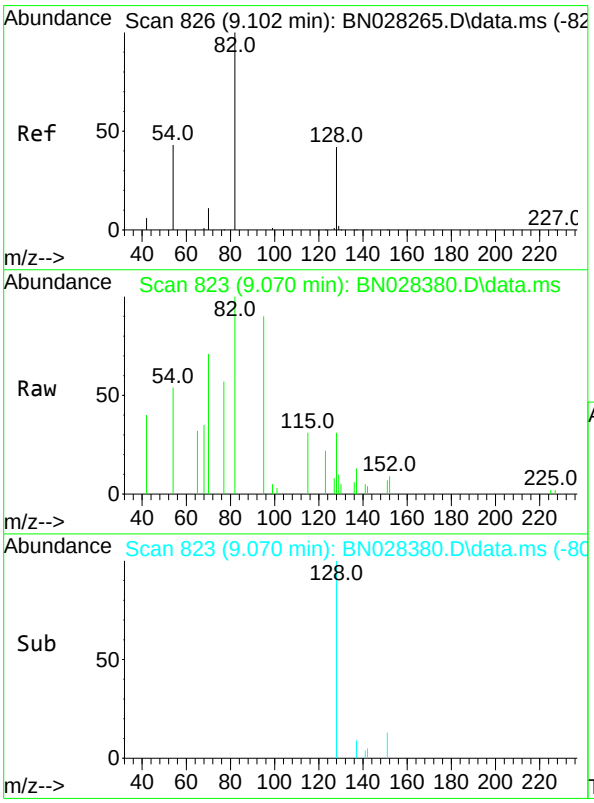

#8
Nitrobenzene-d5
Concen: 0.261 ng
RT: 9.070 min Scan# 823
Delta R.T. -0.032 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion: 82 Resp: 3277

Ion	Ratio	Lower	Upper
82	100		
128	30.7	36.8	55.2#
54	53.6	37.4	56.2



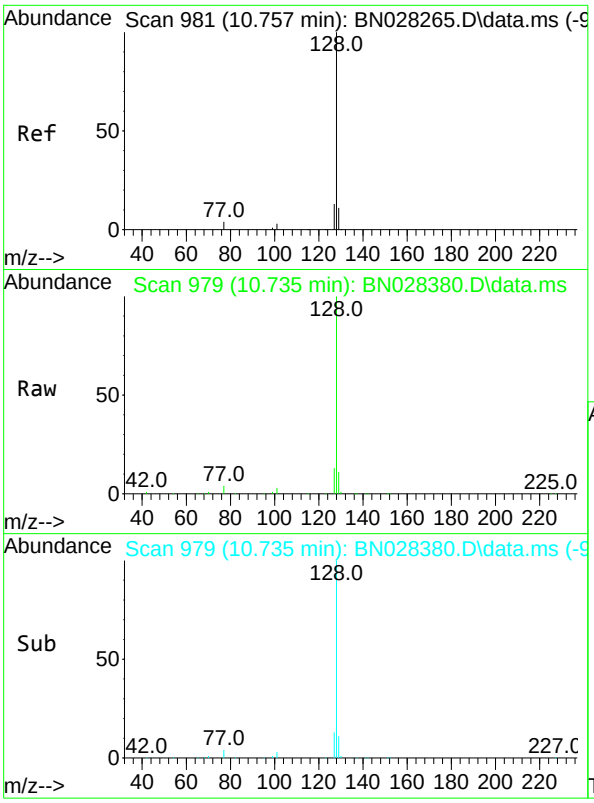

#9
Naphthalene
Concen: 46.192 ng
RT: 10.735 min Scan# 9
Delta R.T. -0.021 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:128 Resp: 169479

Ion	Ratio	Lower	Upper
128	100		
129	11.1	9.8	14.6
127	13.2	11.4	17.0



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

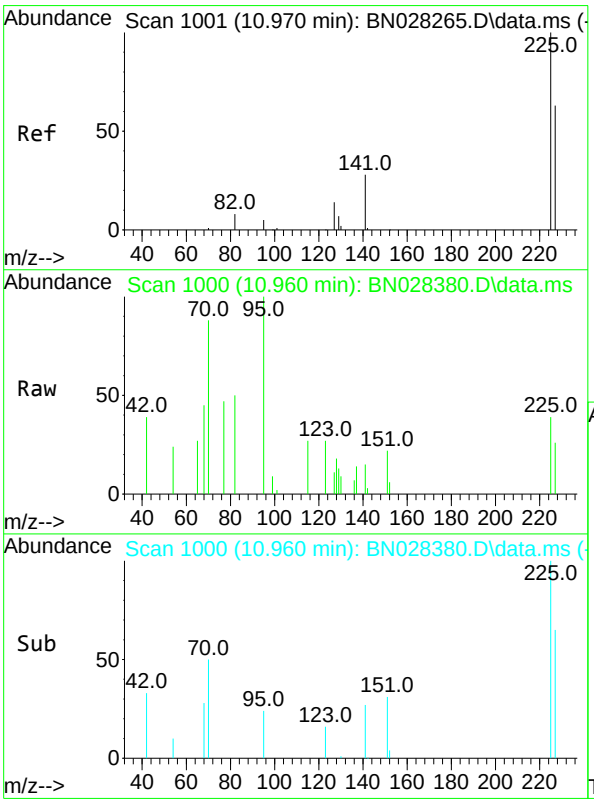

#10
Hexachlorobutadiene
Concen: 0.490 ng
RT: 10.960 min Scan# 1000
Delta R.T. 0.000 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:225 Resp: 3087

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.2	51.6	77.4



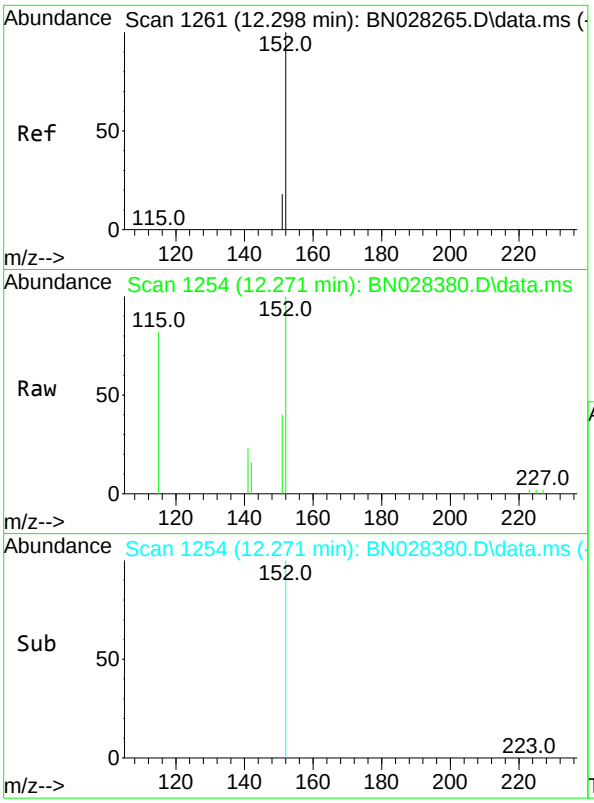

#11
2-Methylnaphthalene-d10
Concen: 0.211 ng
RT: 12.271 min Scan# 1
Delta R.T. -0.023 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:152 Resp: 448

Ion	Ratio	Lower	Upper
152	100		
151	40.6	16.1	24.1#



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

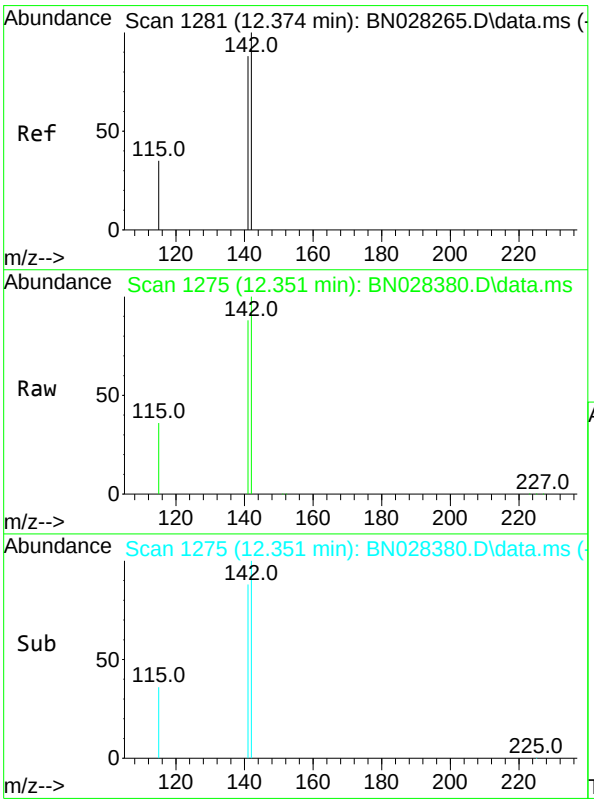

#12
2-Methylnaphthalene
Concen: 35.212 ng
RT: 12.351 min Scan# 1275
Delta R.T. -0.019 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:142 Resp: 918072

Ion	Ratio	Lower	Upper
142	100		
141	88.1	71.1	106.7
115	36.1	29.9	44.9



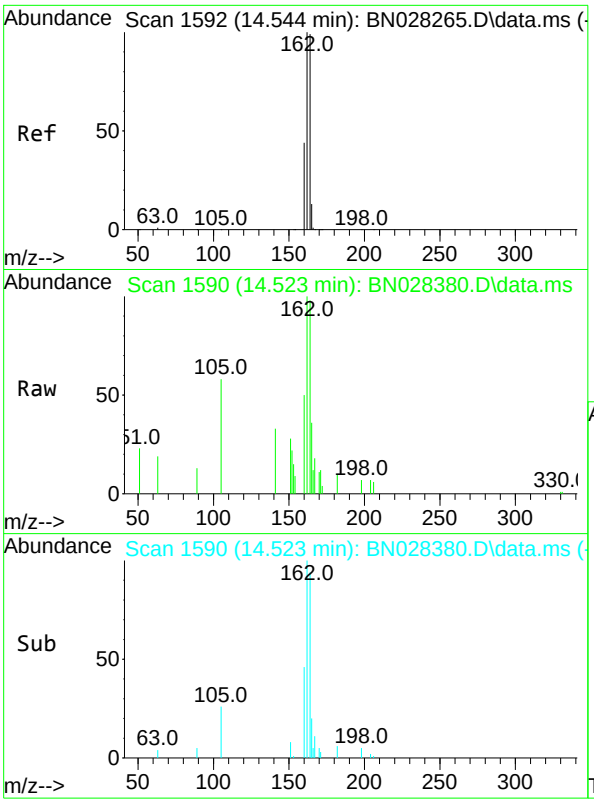

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.523 min Scan# 1
Delta R.T. -0.011 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:164 Resp: 952

Ion	Ratio	Lower	Upper
164	100		
162	102.2	81.1	121.7
160	51.1	36.6	54.8



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

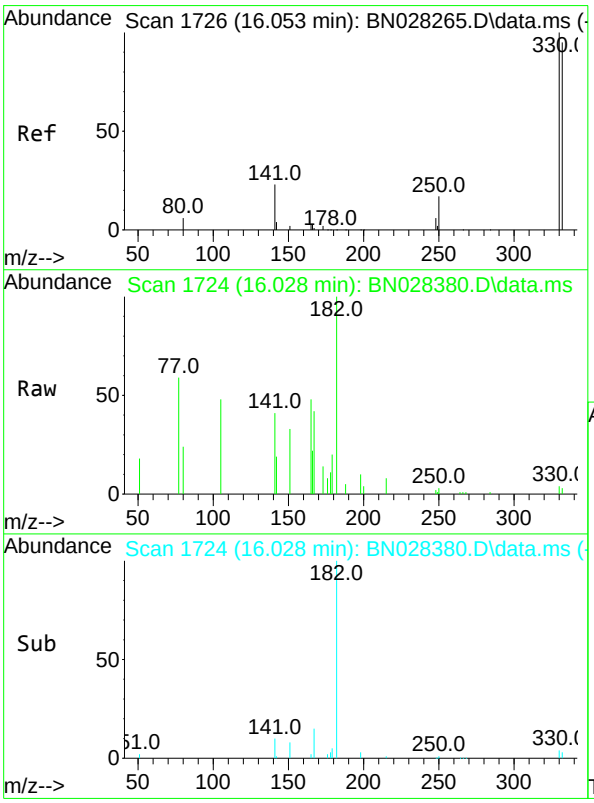

#14
2,4,6-Tribromophenol
Concen: 0.115 ng
RT: 16.028 min Scan# 1724
Delta R.T. -0.037 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:330 Resp: 535

Ion	Ratio	Lower	Upper
330	100		
332	95.1	74.1	111.1
141	0.0	32.1	48.1#



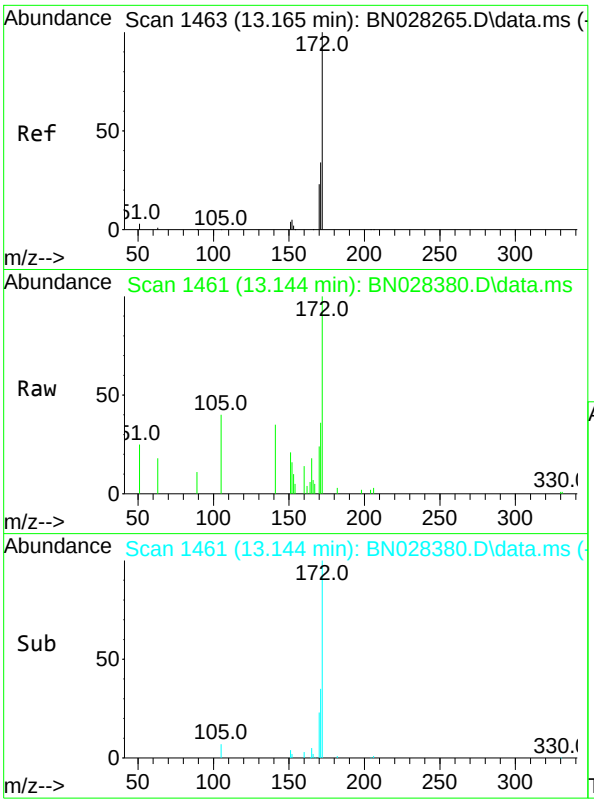

#15
2-Fluorobiphenyl
Concen: 0.181 ng
RT: 13.144 min Scan# 14
Delta R.T. -0.021 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:172 Resp: 606

Ion	Ratio	Lower	Upper
172	100		
171	36.4	28.3	42.5
170	23.5	18.7	28.1



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

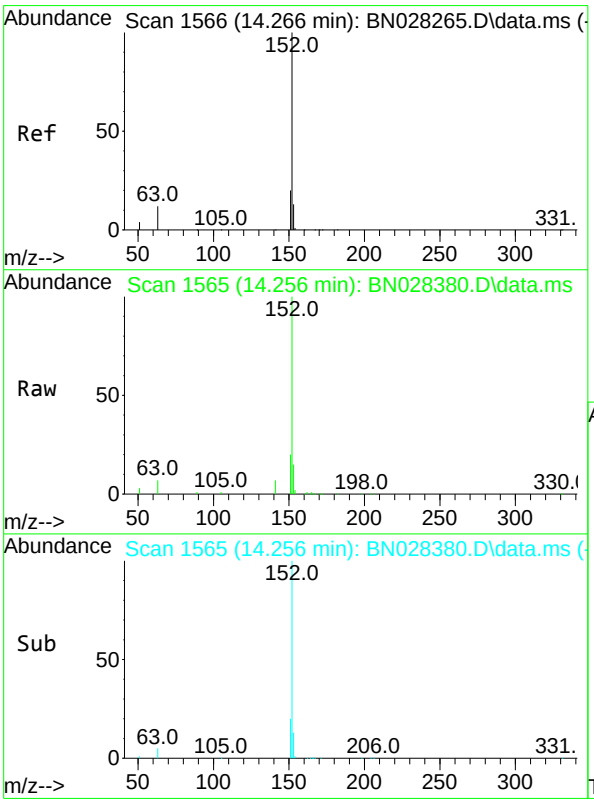

#16
Acenaphthylene
Concen: 5.598 ng
RT: 14.256 min Scan# 1565
Delta R.T. 0.000 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:152 Resp: 239660

Ion	Ratio	Lower	Upper
152	100		
151	21.0	15.6	23.4
153	19.5	10.6	16.0#



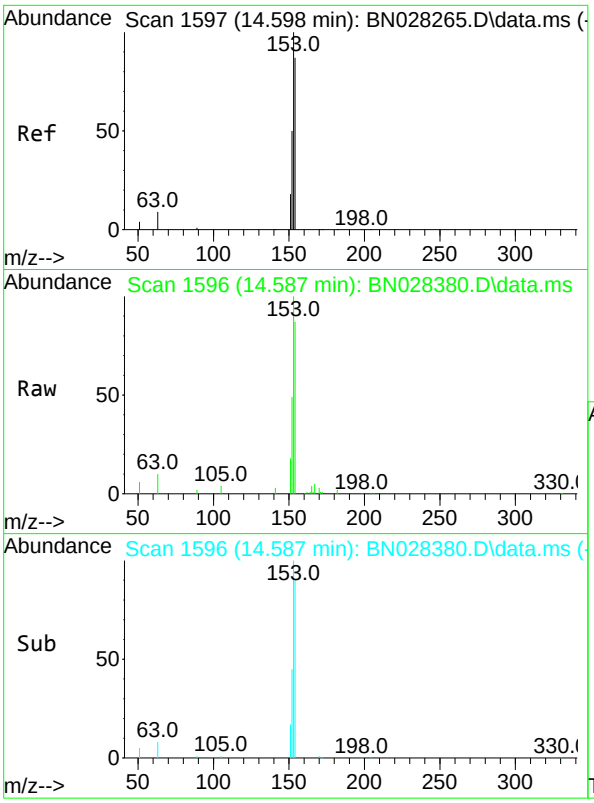

#17
Acenaphthene
Concen: 4.146 ng
RT: 14.587 min Scan# 1
Delta R.T. -0.011 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:154 Resp: 11184

Ion	Ratio	Lower	Upper
154	100		
153	120.9	90.7	136.1
152	62.2	43.6	65.4



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

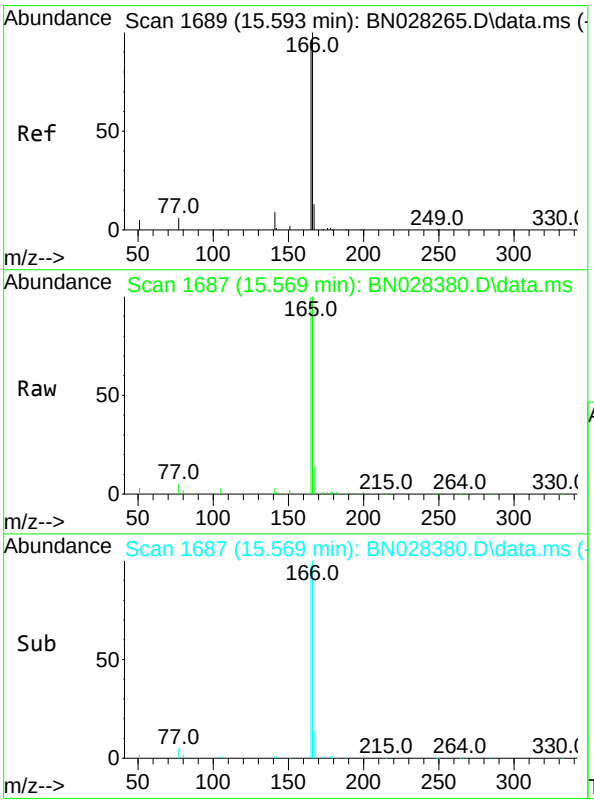

#18
Fluorene
Concen: 5.996 ng
RT: 15.569 min Scan# 1687
Delta R.T. -0.012 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:166 Resp: 212923

Ion	Ratio	Lower	Upper
166	100		
165	101.0	79.3	118.9
167	18.0	10.9	16.3#



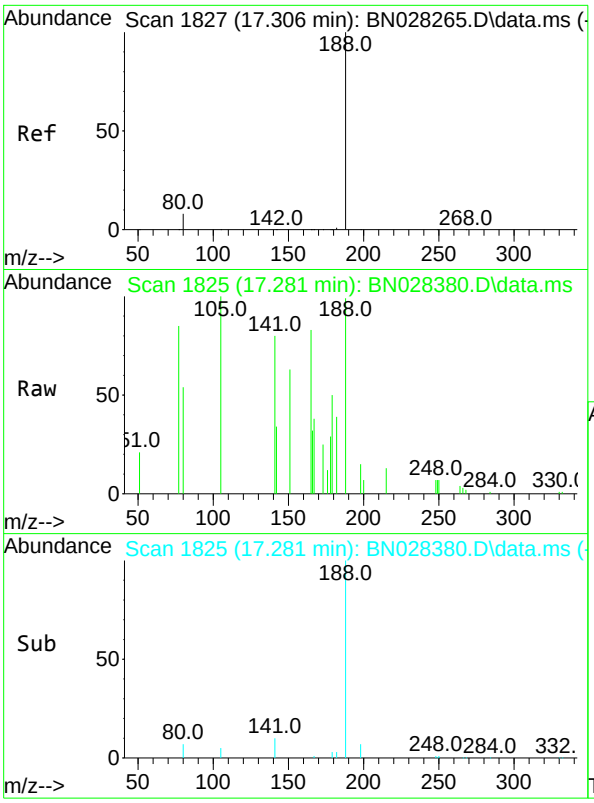

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.281 min Scan# 1
Delta R.T. -0.012 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:188 Resp: 1106

Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	54.0	7.1	10.7#



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

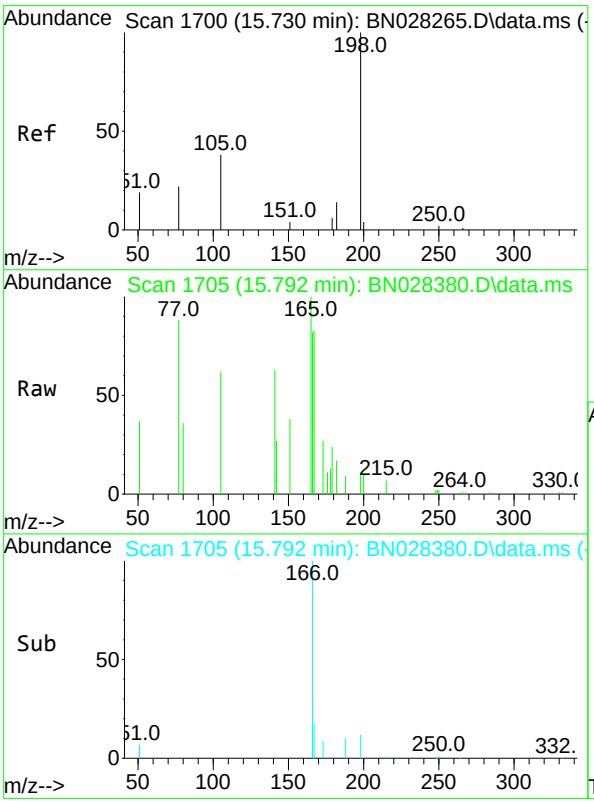

#20
4,6-Dinitro-2-methylphenol
Concen: 1.052 ng
RT: 15.792 min Scan# 1705
Delta R.T. -0.012 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:198 Resp: 815

Ion	Ratio	Lower	Upper
198	100		
51	352.5	96.1	144.1#
105	602.2	75.4	113.0#



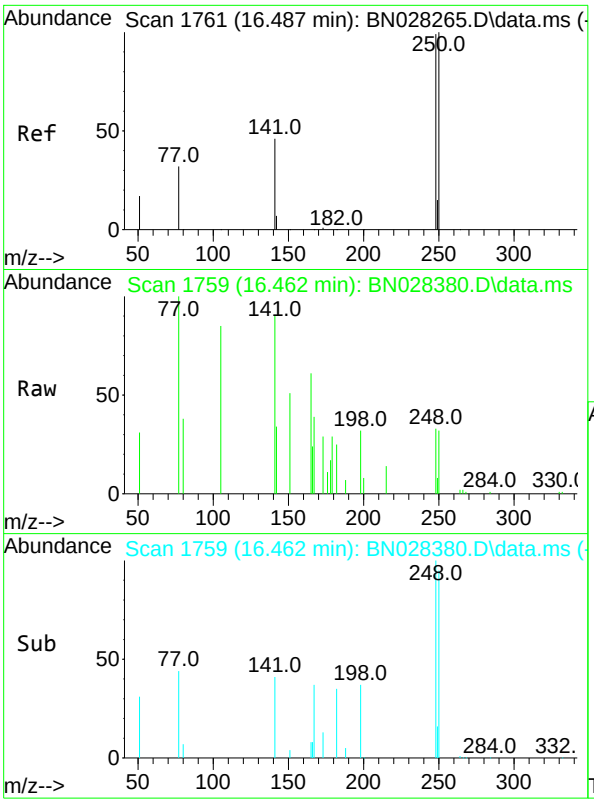

#21
4-Bromophenyl-phenylether
Concen: 0.545 ng
RT: 16.462 min Scan# 1
Delta R.T. -0.012 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:248 Resp: 310

Ion	Ratio	Lower	Upper
248	100		
250	96.1	80.5	120.7
141	271.9	38.9	58.3#

Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023



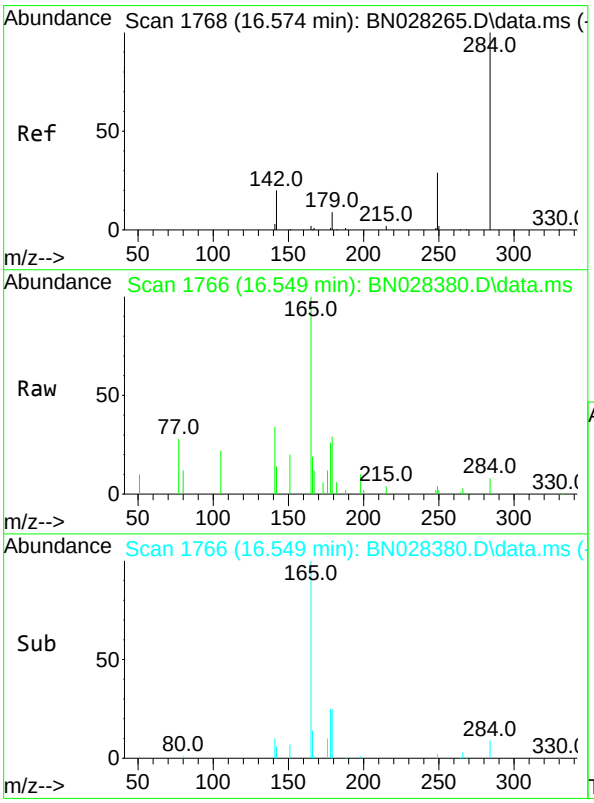

#22
Hexachlorobenzene
Concen: 0.499 ng
RT: 16.549 min Scan# 1766
Delta R.T. -0.012 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:284 Resp: 2927

Ion	Ratio	Lower	Upper
284	100		
142	107.0	32.1	48.1#
249	37.8	25.5	38.3



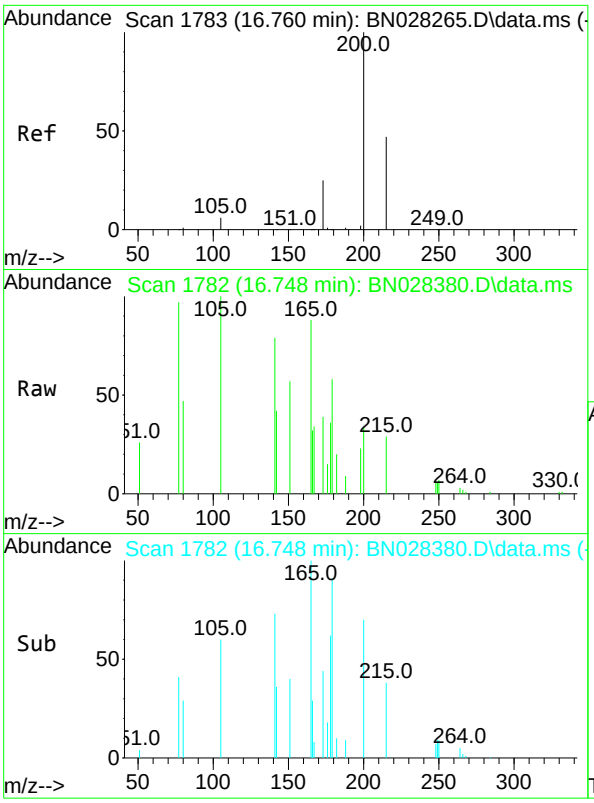

#23
Atrazine
Concen: 0.607 ng
RT: 16.748 min Scan# 1
Delta R.T. -0.012 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:200 Resp: 324

Ion	Ratio	Lower	Upper
200	100		
173	115.3	21.6	32.4#
215	85.1	39.0	58.6#



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

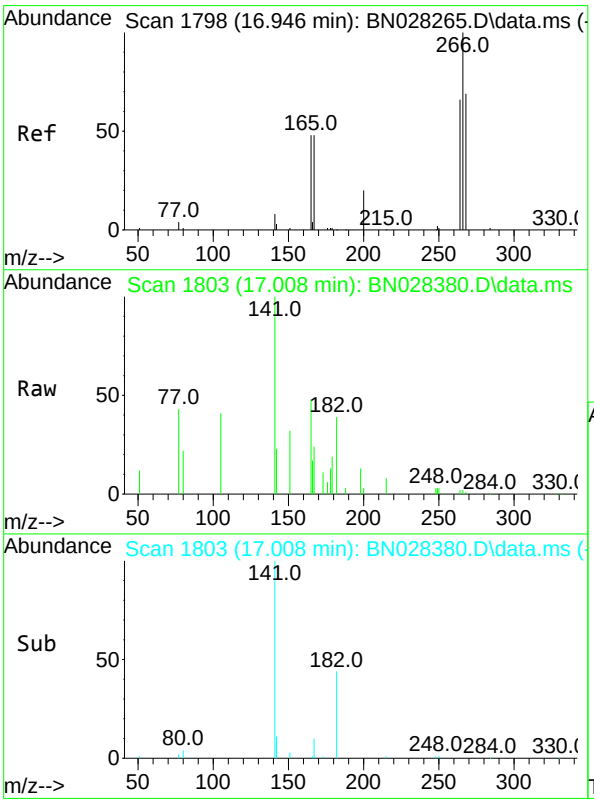

#24
Pentachlorophenol
Concen: 0.147 ng
RT: 17.008 min Scan# 1803
Delta R.T. -0.025 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:266 Resp: 395

Ion	Ratio	Lower	Upper
266	100		
264	0.0	51.5	77.3#
268	61.0	56.6	84.8



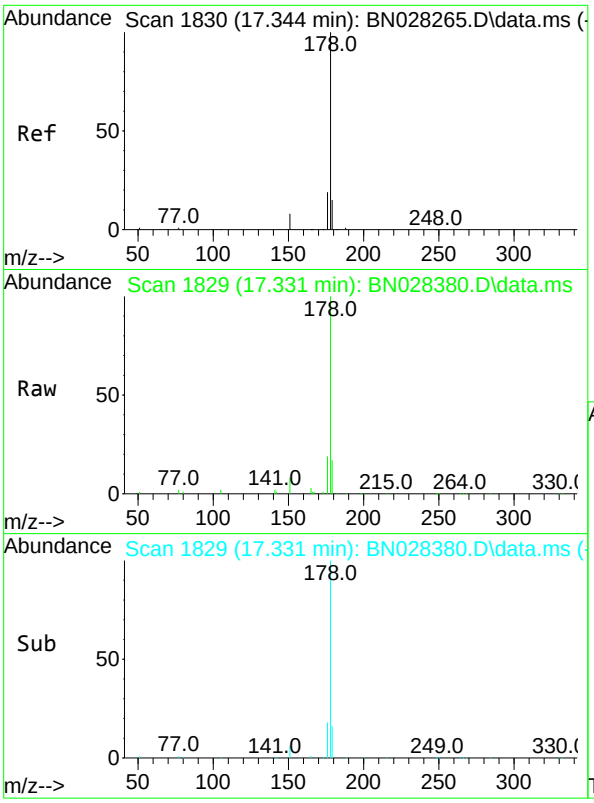

#25
Phenanthrene
Concen: 25.815 ng
RT: 17.331 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:178 Resp: 78181

Ion	Ratio	Lower	Upper
178	100		
176	19.1	15.3	22.9
179	16.1	12.5	18.7



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

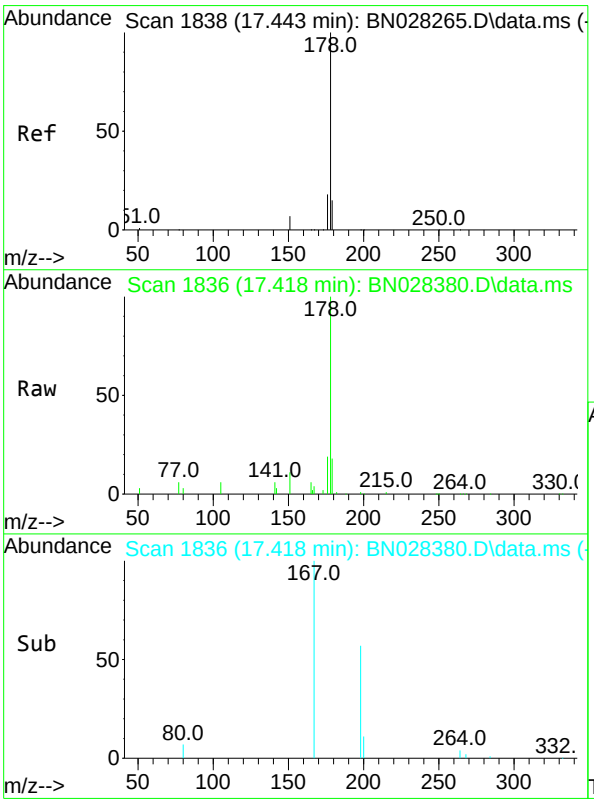

#26
Anthracene
Concen: 6.988 ng
RT: 17.418 min Scan# 1836
Delta R.T. -0.012 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:178 Resp: 202139

Ion	Ratio	Lower	Upper
178	100		
176	18.1	14.6	22.0
179	18.4	12.2	18.4#



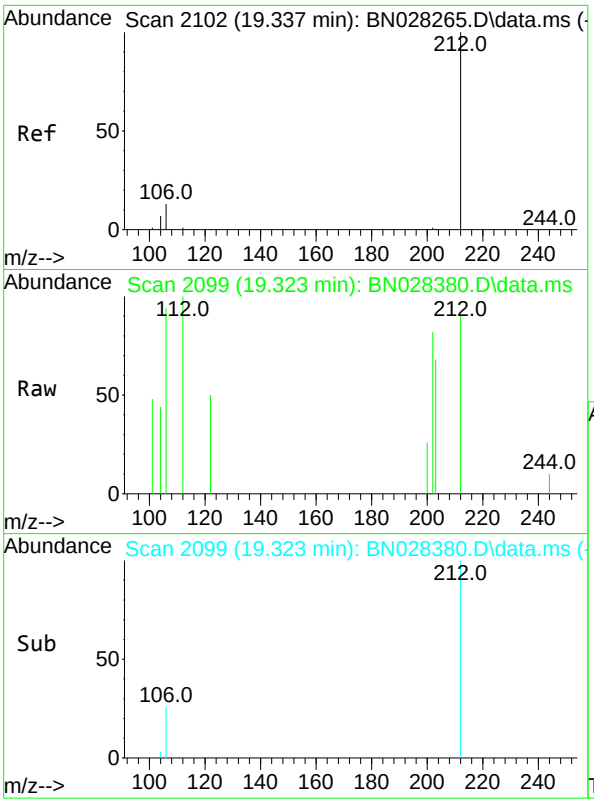

#27
Fluoranthene-d10
Concen: 0.167 ng
RT: 19.323 min Scan# 2
Delta R.T. -0.005 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:212 Resp: 494

Ion	Ratio	Lower	Upper
212	100		
106	66.2	11.5	17.3#
104	16.9	6.7	10.1#



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

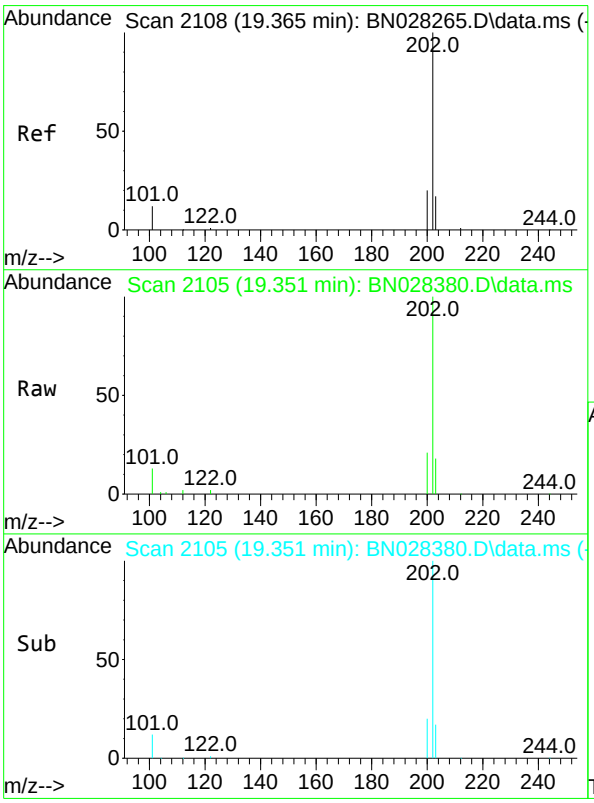

#28
Fluoranthene
Concen: 12.690 ng
RT: 19.351 min Scan# 2105
Delta R.T. -0.005 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:202 Resp: 482831

Ion	Ratio	Lower	Upper
202	100		
101	12.6	10.1	15.1
203	18.1	13.9	20.9



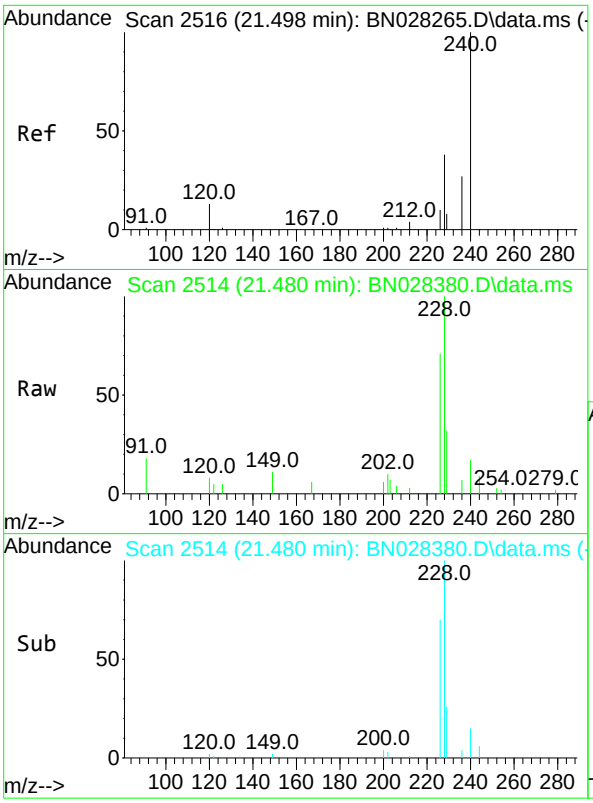

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.480 min Scan# 2
Delta R.T. -0.009 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:240 Resp: 1088

Ion	Ratio	Lower	Upper
240	100		
120	47.3	13.4	20.0#
236	40.8	22.7	34.1#



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

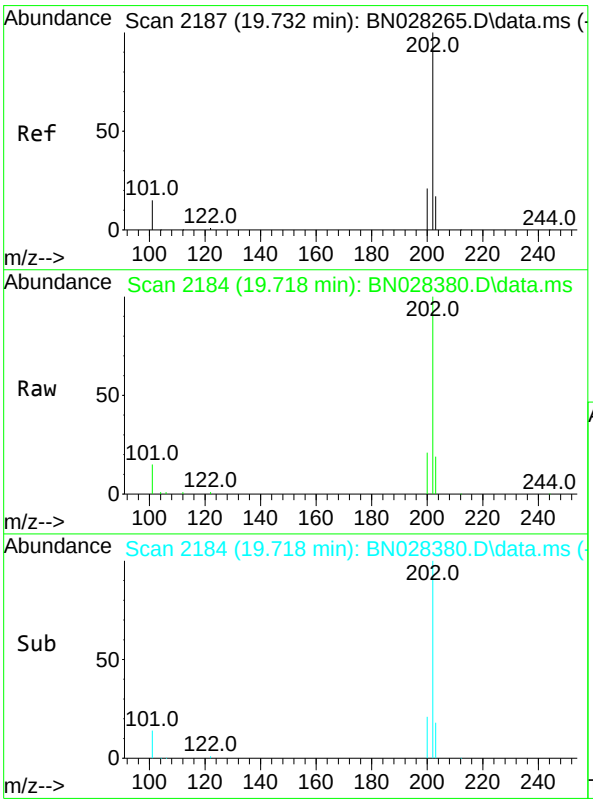

#30
Pyrene
Concen: 15.955 ng
RT: 19.718 min Scan# 2184
Delta R.T. -0.009 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:202 Resp: 594036

Ion	Ratio	Lower	Upper
202	100		
200	20.7	16.7	25.1
203	21.8	14.5	21.7#



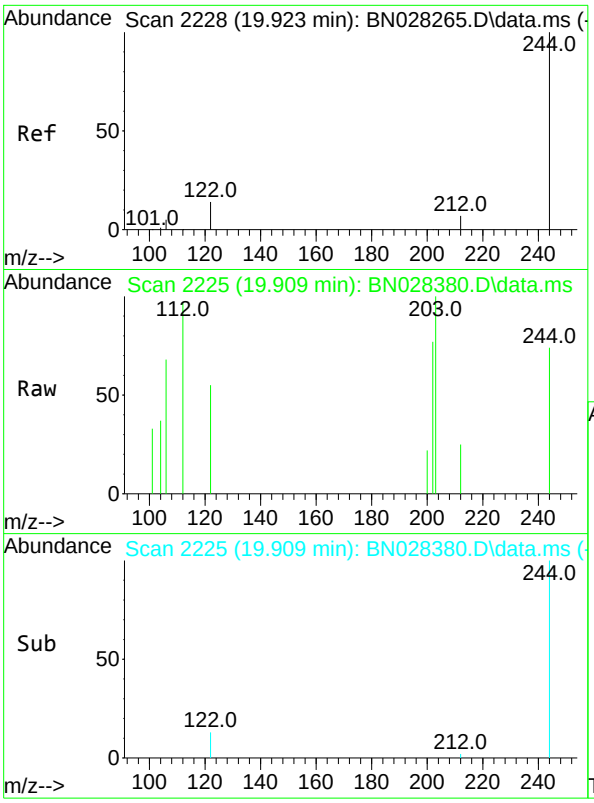

#31
Terphenyl-d14
Concen: 0.221 ng
RT: 19.909 min Scan# 2
Delta R.T. -0.009 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:244 Resp: 511

Ion	Ratio	Lower	Upper
244	100		
212	33.3	6.6	10.0#
122	74.7	11.7	17.5#



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

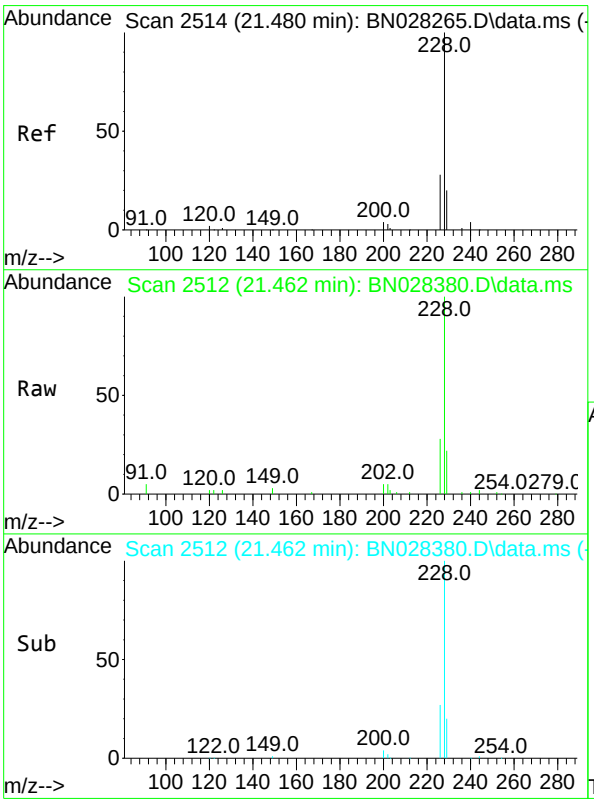

#32
Benzo(a)anthracene
Concen: 7.636 ng
RT: 21.462 min Scan# 2512
Delta R.T. -0.009 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:228 Resp: 295174

Ion	Ratio	Lower	Upper
228	100		
226	28.2	22.9	34.3
229	21.8	16.6	24.8



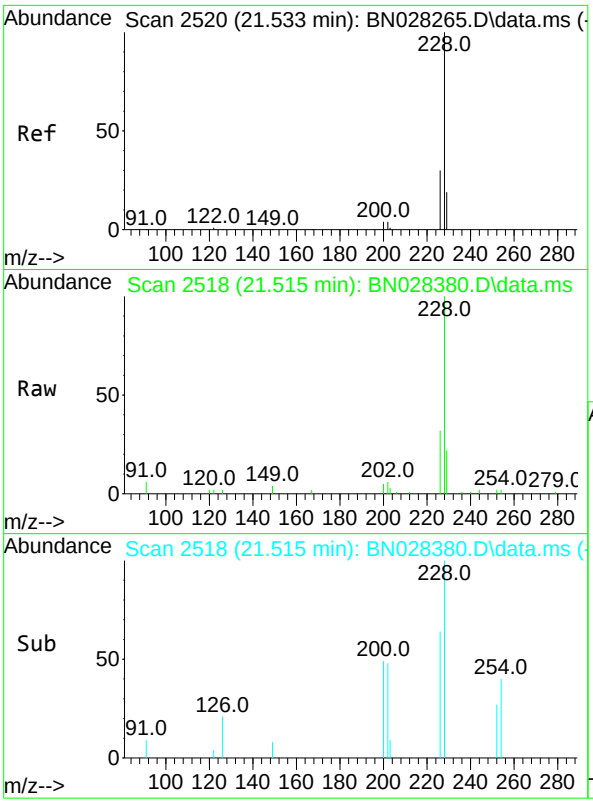

#33
Chrysene
Concen: 7.340 ng
RT: 21.515 min Scan# 2
Delta R.T. -0.009 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:228 Resp: 27156

Ion	Ratio	Lower	Upper
228	100		
226	32.3	25.2	37.8
229	22.4	16.6	25.0



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

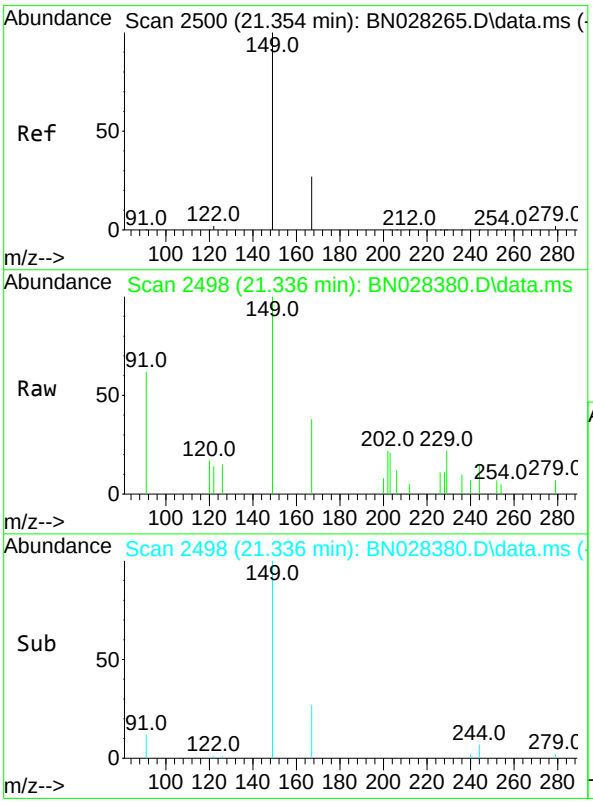

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.498 ng
RT: 21.336 min Scan# 2498
Delta R.T. -0.009 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:149 Resp: 14708

Ion	Ratio	Lower	Upper
149	100		
167	28.1	22.6	34.0
279	4.3	4.2	6.2



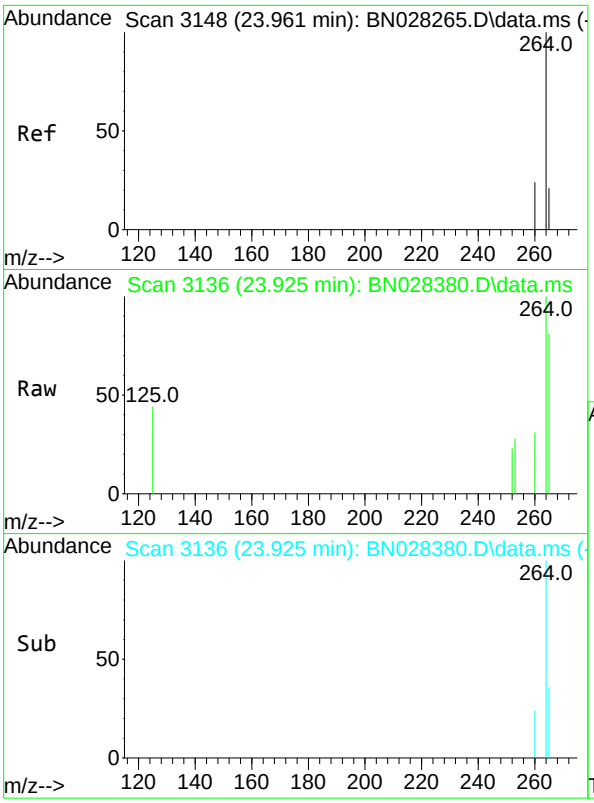

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.925 min Scan# 3
Delta R.T. -0.012 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:264 Resp: 1275

Ion	Ratio	Lower	Upper
264	100		
260	31.3	20.7	31.1#
265	81.2	38.3	57.5#

Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023



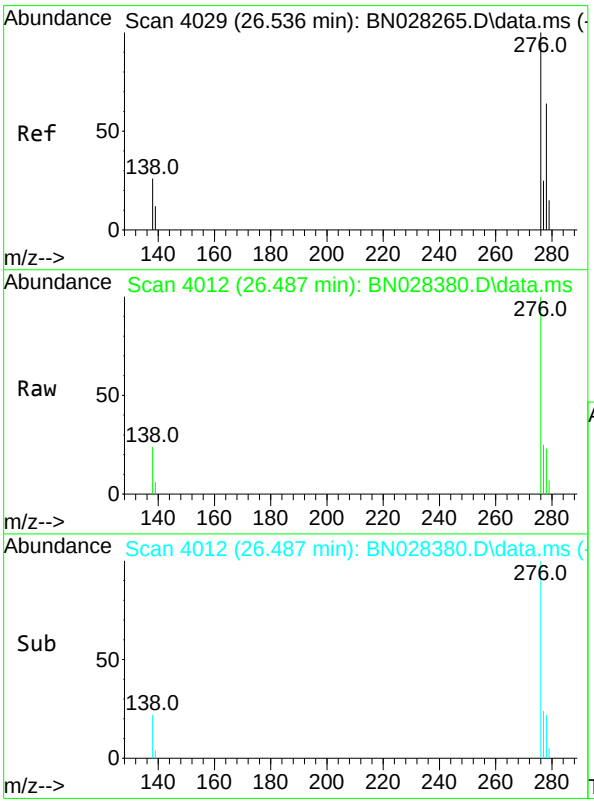

#36
Indeno(1,2,3-cd)pyrene
Concen: 4.230 ng
RT: 26.487 min Scan# 4012
Delta R.T. -0.017 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:276 Resp: 217483

Ion	Ratio	Lower	Upper
276	100		
138	23.4	21.3	31.9
277	24.3	20.0	30.0



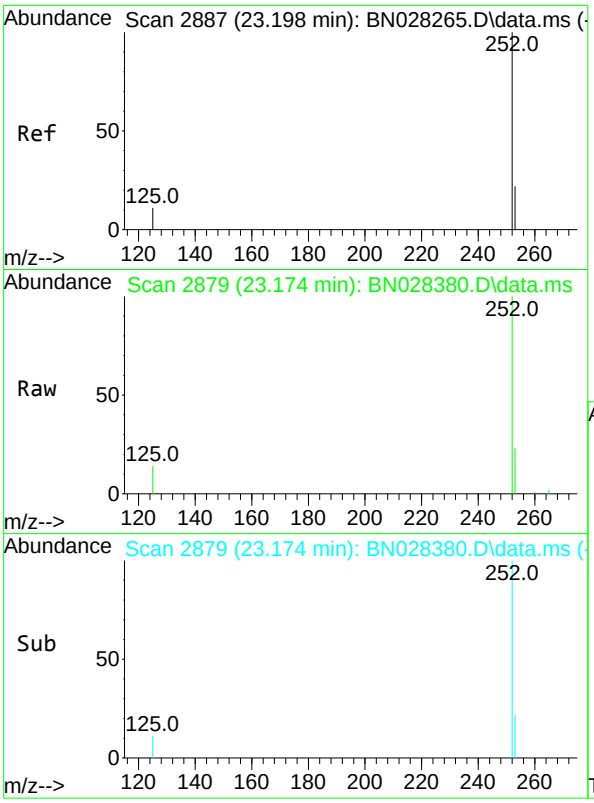

#37
Benzo(b)fluoranthene
Concen: 8.380 ng
RT: 23.174 min Scan# 2
Delta R.T. -0.003 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:252 Resp: 33406

Ion	Ratio	Lower	Upper
252	100		
253	23.2	21.8	32.8
125	13.6	15.6	23.4#



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

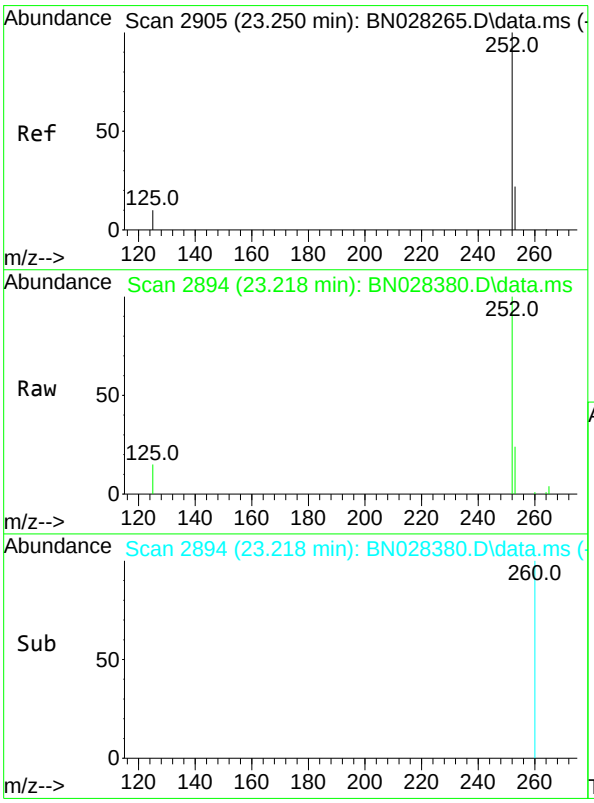

#38
Benzo(k)fluoranthene
Concen: 3.228 ng m
RT: 23.218 min Scan# 2894
Delta R.T. -0.009 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:252 Resp: 130906

Ion	Ratio	Lower	Upper
252	100		
253	24.4	22.0	33.0
125	14.8	15.3	22.9#



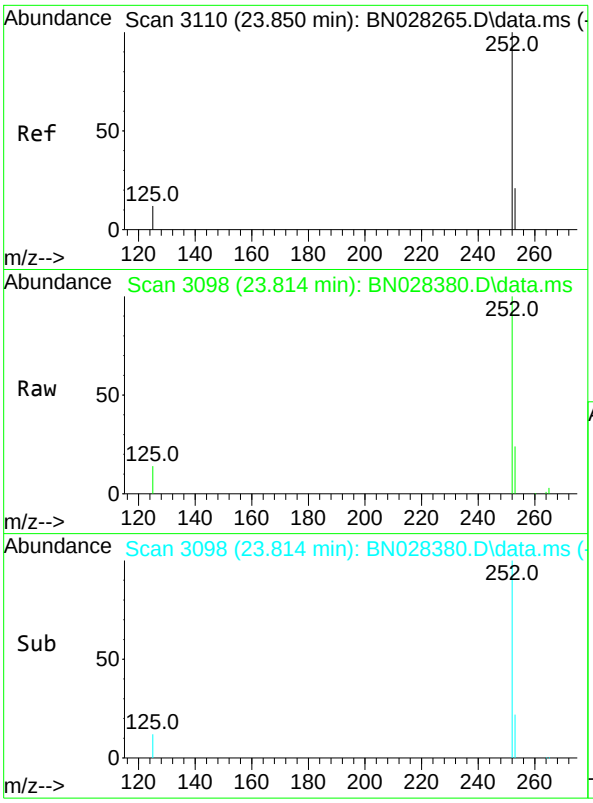

#39
Benzo(a)pyrene
Concen: 6.978 ng m
RT: 23.814 min Scan# 3
Delta R.T. -0.015 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:252 Resp: 27673

Ion	Ratio	Lower	Upper
252	100		
253	23.5	22.7	34.1
125	13.9	17.0	25.6



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023

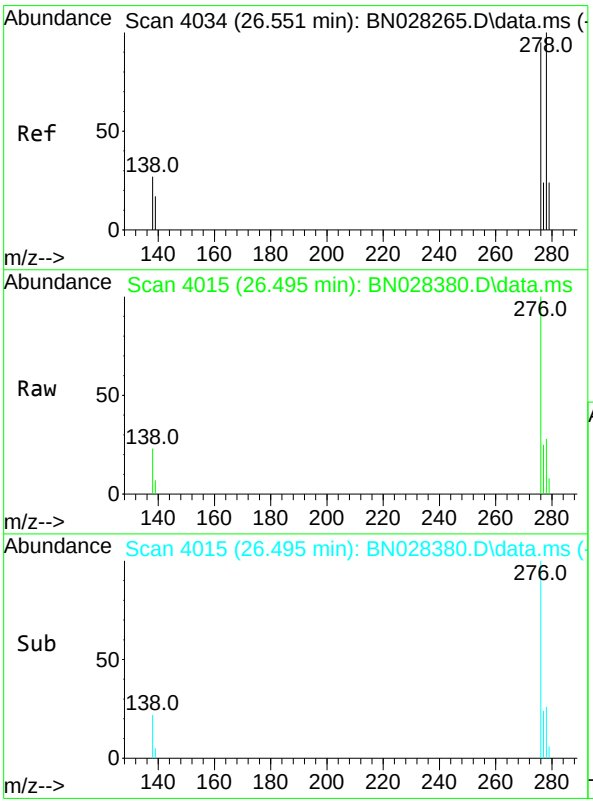

#40
Dibenzo(a,h)anthracene
Concen: 1.615 ng
RT: 26.495 min Scan# 4015
Delta R.T. -0.023 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:278 Resp: 67411

Ion	Ratio	Lower	Upper
278	100		
139	24.1	18.8	28.2
279	29.7	23.5	35.3



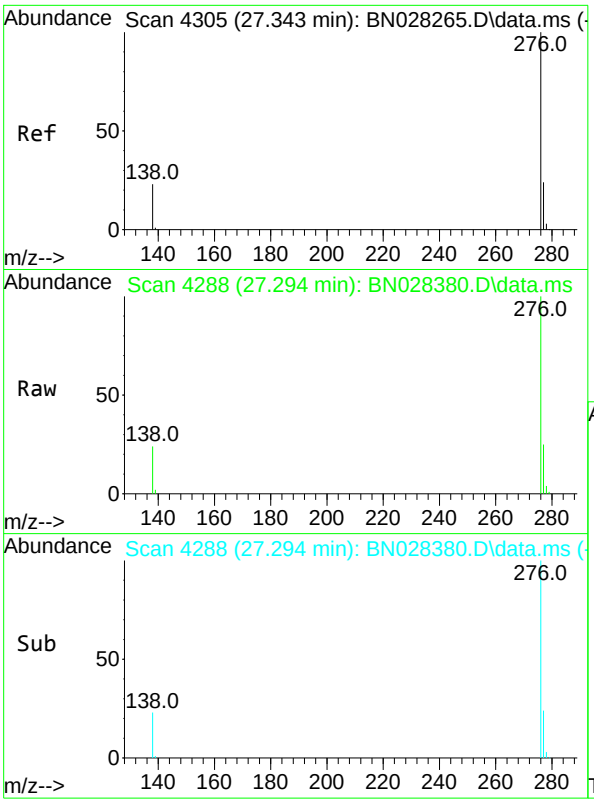

#41
Benzo(g,h,i)perylene
Concen: 6.112 ng
RT: 27.294 min Scan# 4
Delta R.T. -0.012 min
Lab File: BN028380.D
Acq: 24 Oct 2023 16:12

Tgt Ion:276 Resp: 26342

Ion	Ratio	Lower	Upper
276	100		
277	24.5	21.7	32.5
138	24.1	21.7	32.5



Instrument :
BNA_N
ClientSampleId :
0-2(0-10)MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :mohammad ahmed 10/25/2023